

Date: 2025-12-19

System Check_750MHz**DUT:D750V3-SN:1087**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.905$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.53, 10.34, 10.38); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.26 W/kg; SAR (10g) = 1.48 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 2.08 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 20.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

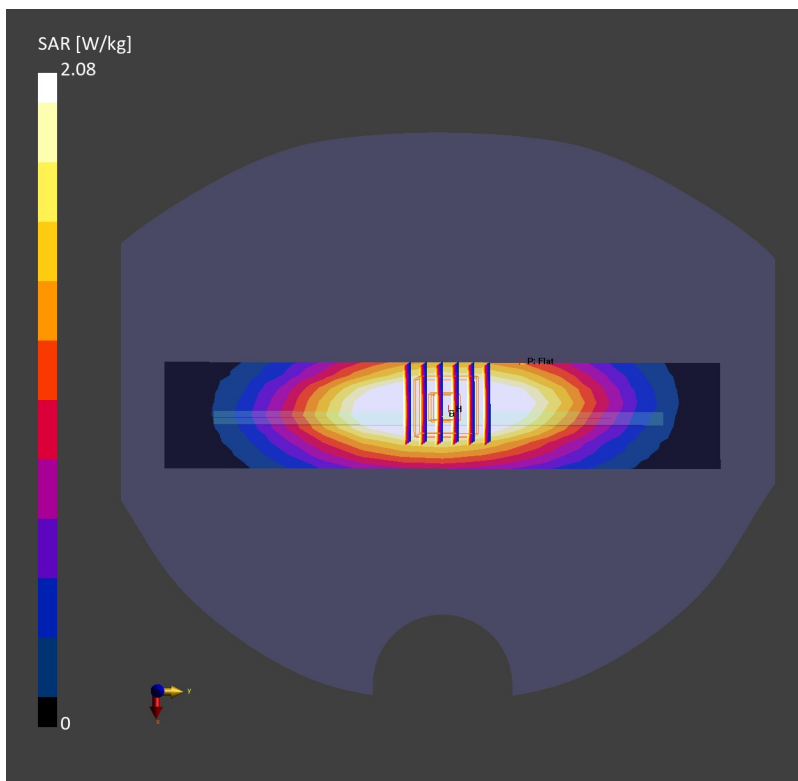

Date: 2026-01-02

System Check_750MHz**DUT:D750V3-SN:1087**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.53, 10.34, 10.38); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.33 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.01 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 21.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

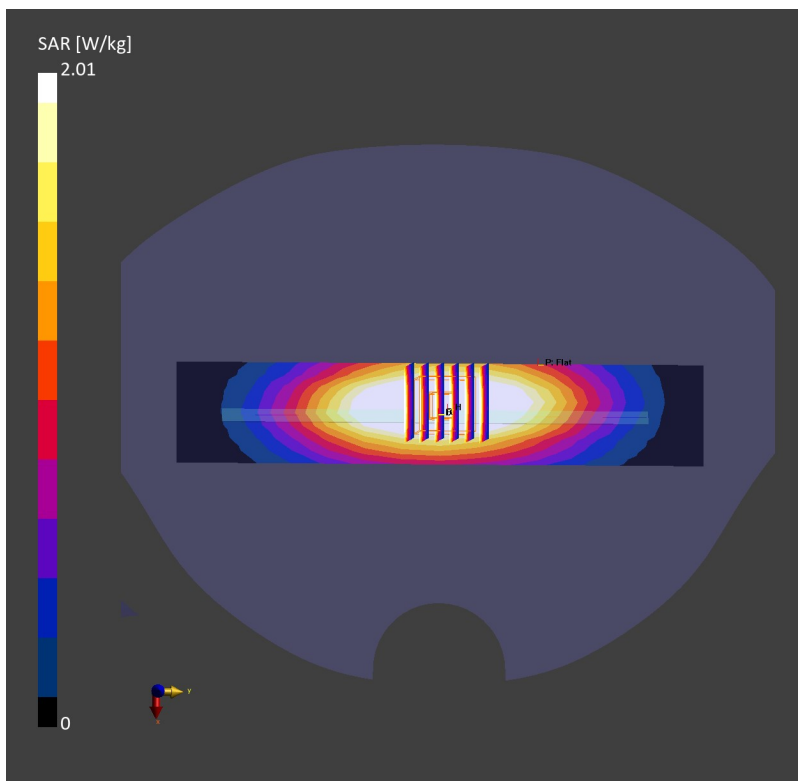

Date: 2025-12-20

System Check_835MHz**DUT:D835V2-SN:4d298**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.921$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.23, 10.04, 10.08); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.65 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.09 dB

SAR (1g) = 2.32 W/kg; SAR (10g) = 1.55 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

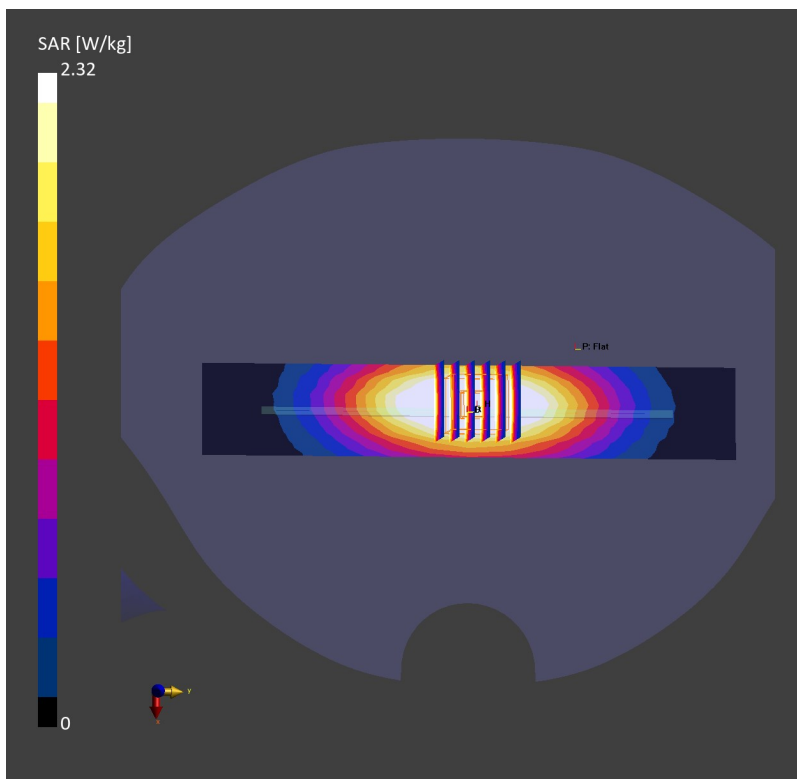

Date: 2026-01-03

System Check_835MHz**DUT:D835V2-SN:4d298**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.932$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.23, 10.04, 10.08); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.56 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.11 dB

SAR (1g) = 2.35 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 19.5 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

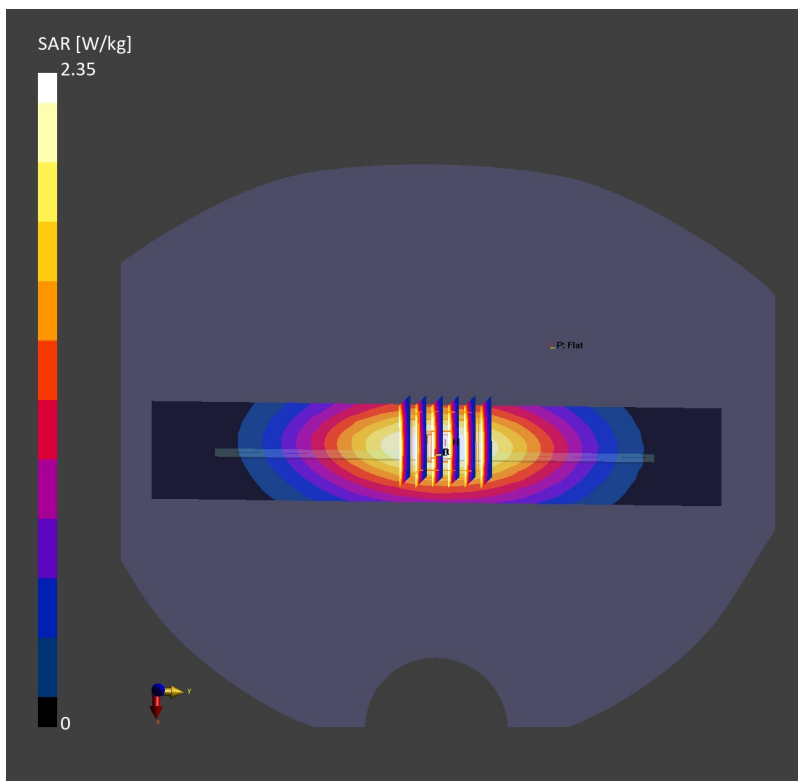

Date: 2025-12-22

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.61, 8.45, 8.49); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 9.45 W/kg; SAR (10g) = 4.89 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 9.28 W/kg; SAR (10g) = 4.86 W/kg

Smallest distance from peaks to all points 3 dB below = 10.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.4 %

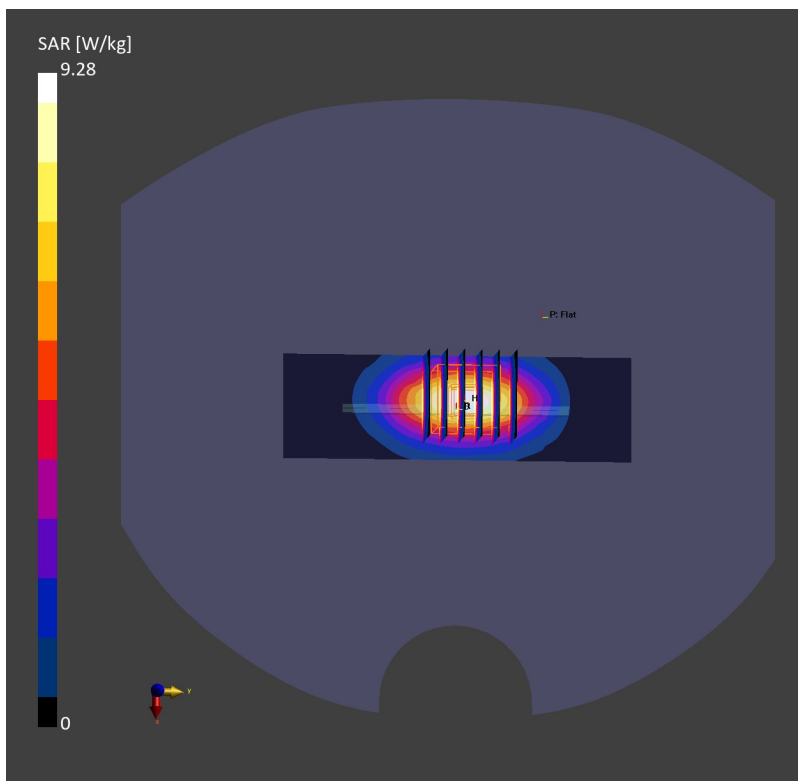

Date: 2026-01-05

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.61, 8.45, 8.49); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 9.27 W/kg; SAR (10g) = 4.73 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.16 dB

SAR (1g) = 9.16 W/kg; SAR (10g) = 4.78 W/kg

Smallest distance from peaks to all points 3 dB below = 11.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

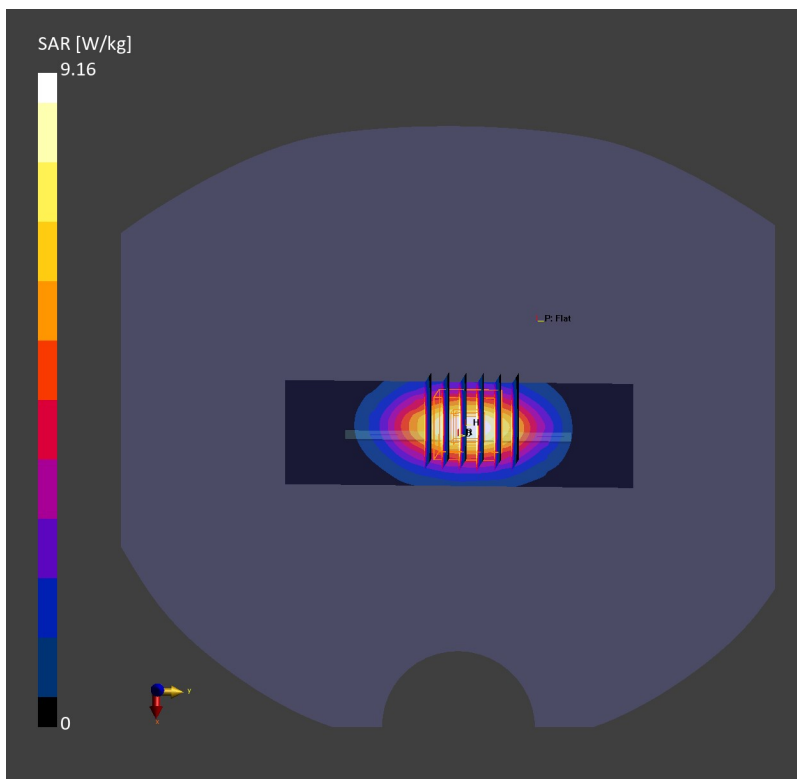

Date: 2026-01-02

System Check_1900MHz**DUT:D1900V2-SN:5d093**

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.33, 8.18, 8.21); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 9.71 W/kg; SAR (10g) = 5.13 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm

Power Drift = 0.09 dB

SAR (1g) = 9.47 W/kg; SAR (10g) = 4.96 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

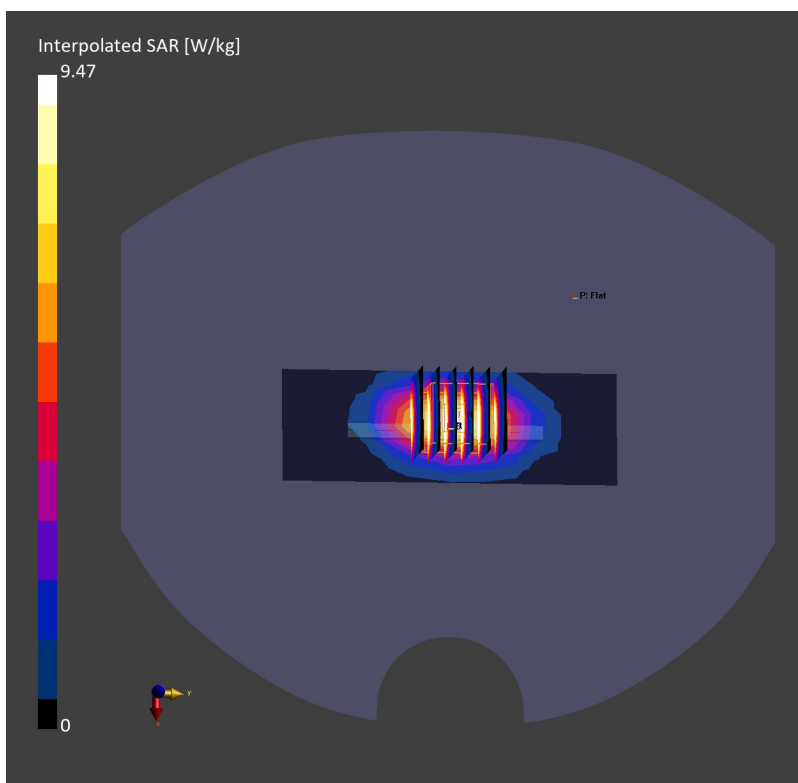

Date: 2026-01-07

System Check_1900MHz**DUT:D1900V2-SN:5d093**


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 38.4$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.33, 8.18, 8.21); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 9.97 W/kg; SAR (10g) = 5.23 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm
x 1.5 mm
Power Drift = -0.03 dB
SAR (1g) = 9.89 W/kg; SAR (10g) = 5.01 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 84.3 %

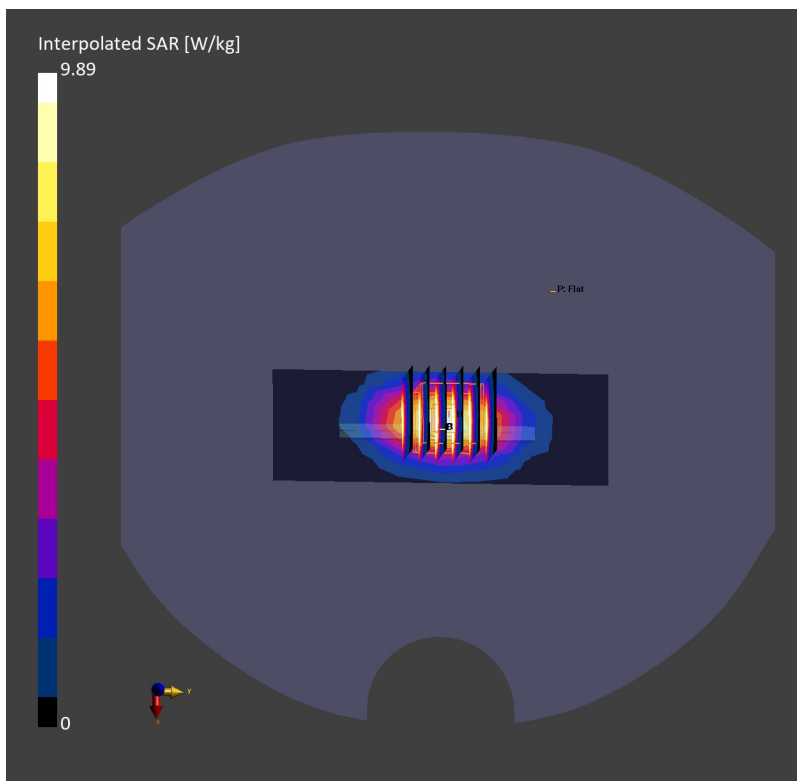

Date: 2025-12-24

System Check_2300MHz**DUT:D2300V2-SN:1055**

Communication System: CW; Frequency: 2300.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2300.0$ MHz; $\sigma = 1.69$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.24, 8.09, 8.13); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 12.3 W/kg; SAR (10g) = 6.24 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.13 dB

SAR (1g) = 11.9 W/kg; SAR (10g) = 6.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

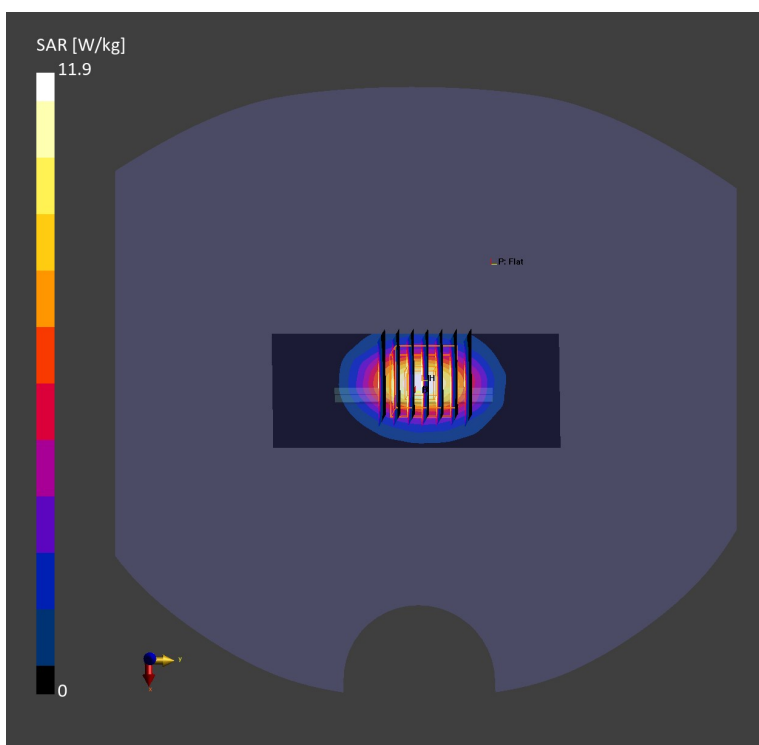

Date: 2026-01-06

System Check_2300MHz**DUT:D2300V2-SN:1055**

Communication System: CW; Frequency: 2300.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2300.0$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.24, 8.09, 8.13); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 12.5 W/kg; SAR (10g) = 6.63 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.13 dB

SAR (1g) = 12.6 W/kg; SAR (10g) = 5.97 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

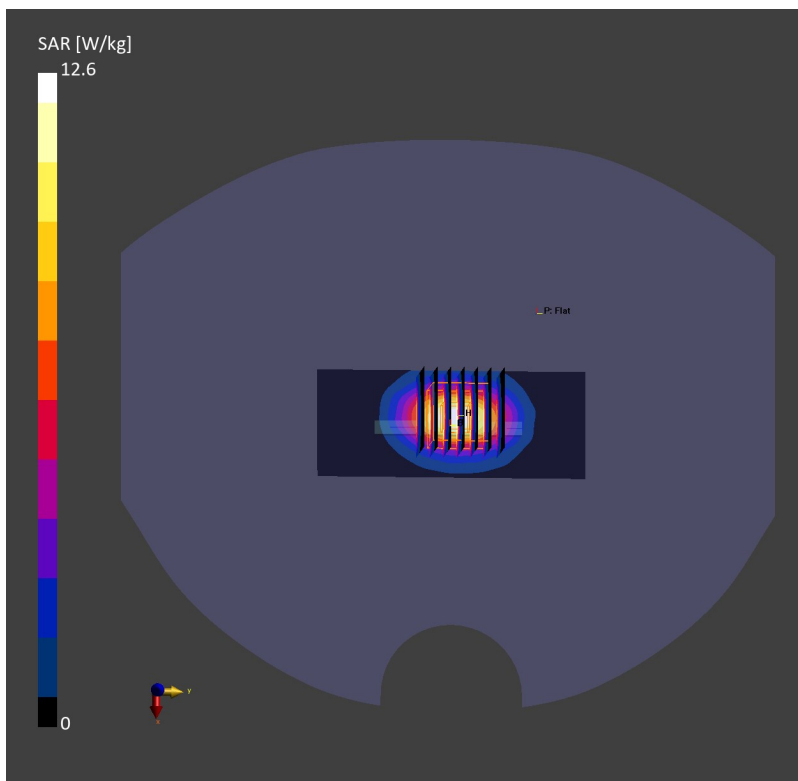

Date: 2025-12-25

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.1 W/kg; SAR (10g) = 6.28 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.13 dB

SAR (1g) = 13.9 W/kg; SAR (10g) = 6.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

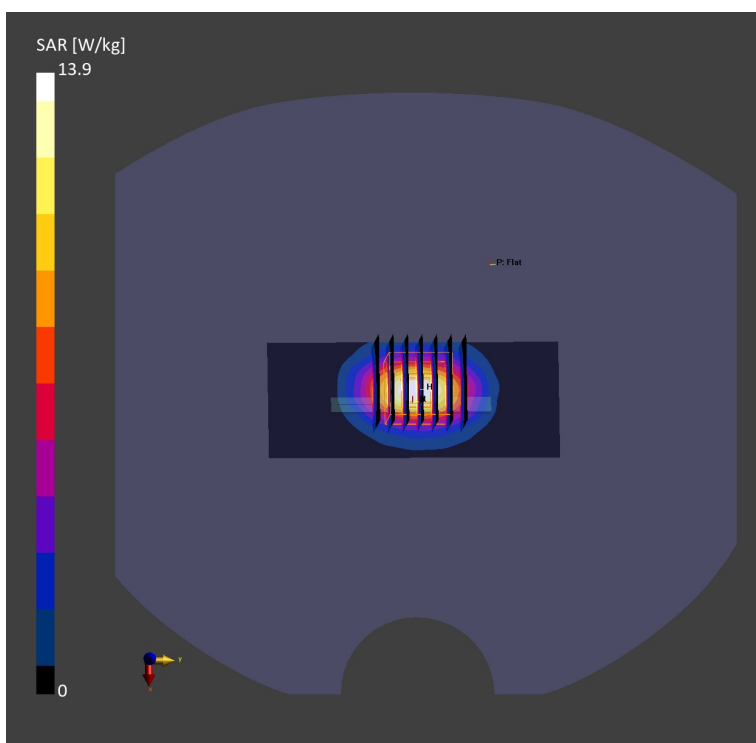

Date: 2026-01-03

System Check_2450MHz**DUT:D2450V2-SN:1095**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
 Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.78$ S/m; $\epsilon_r = 38.9$
 Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
 SAR (1g) = 12.9 W/kg; SAR (10g) = 6.08 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
 Power Drift = 0.03 dB
 SAR (1g) = 12.2 W/kg; SAR (10g) = 6.01 W/kg
 Smallest distance from peaks to all points 3 dB below = 8.9 mm
 Ratio of SAR at M2 to SAR at M1 = 79.9 %

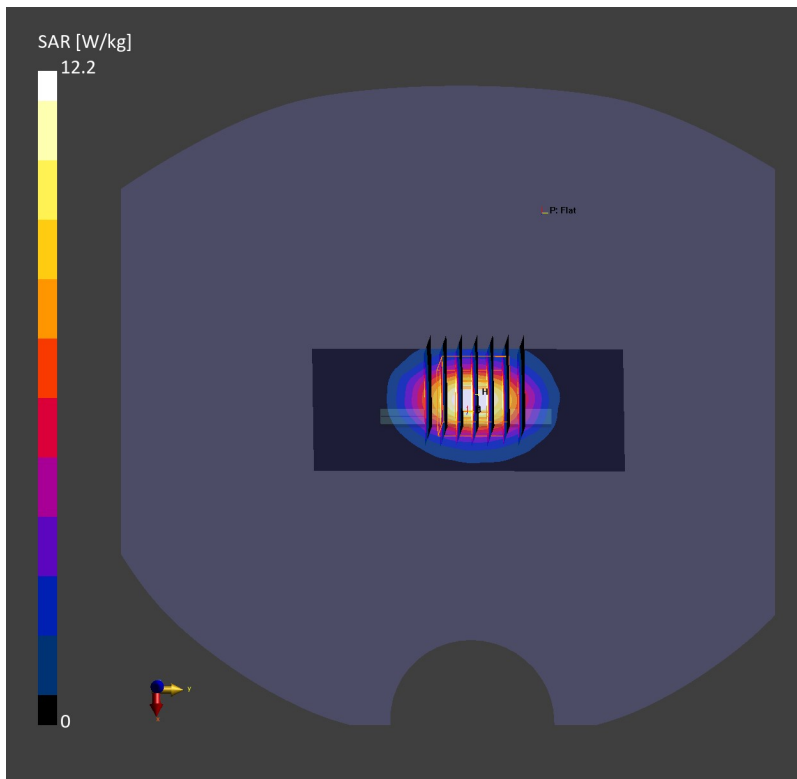

Date: 2025-12-26

System Check_2600MHz**DUT:D2600V2-SN:1112**

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.9, 7.75, 7.79); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.5 W/kg; SAR (10g) = 6.33 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.14 dB

SAR (1g) = 14.1 W/kg; SAR (10g) = 6.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

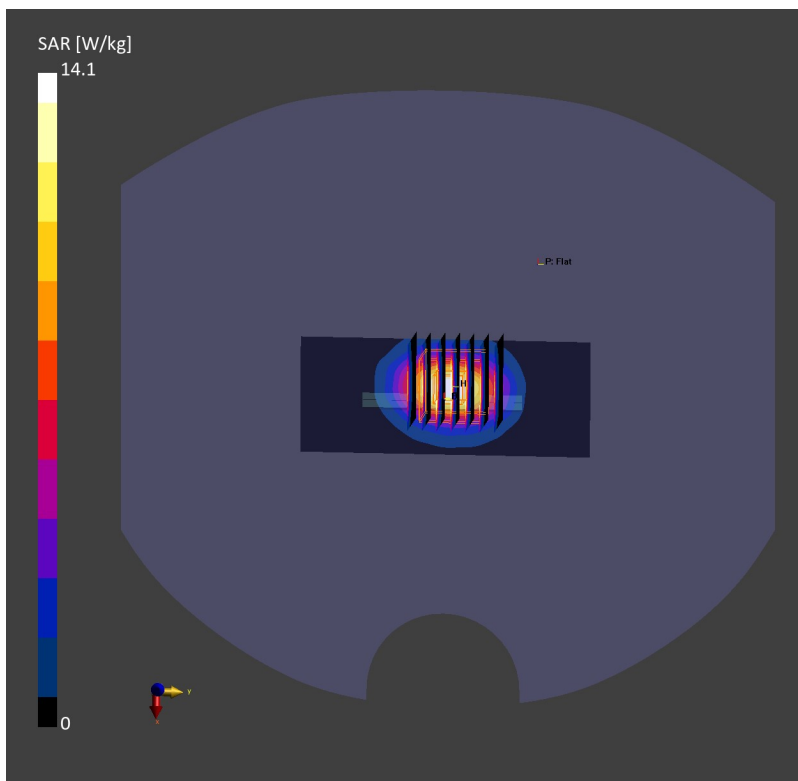

Date: 2026-01-05

System Check_2600MHz**DUT:D2600V2-SN:1112**

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.9, 7.75, 7.79); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.7 W/kg; SAR (10g) = 6.92 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

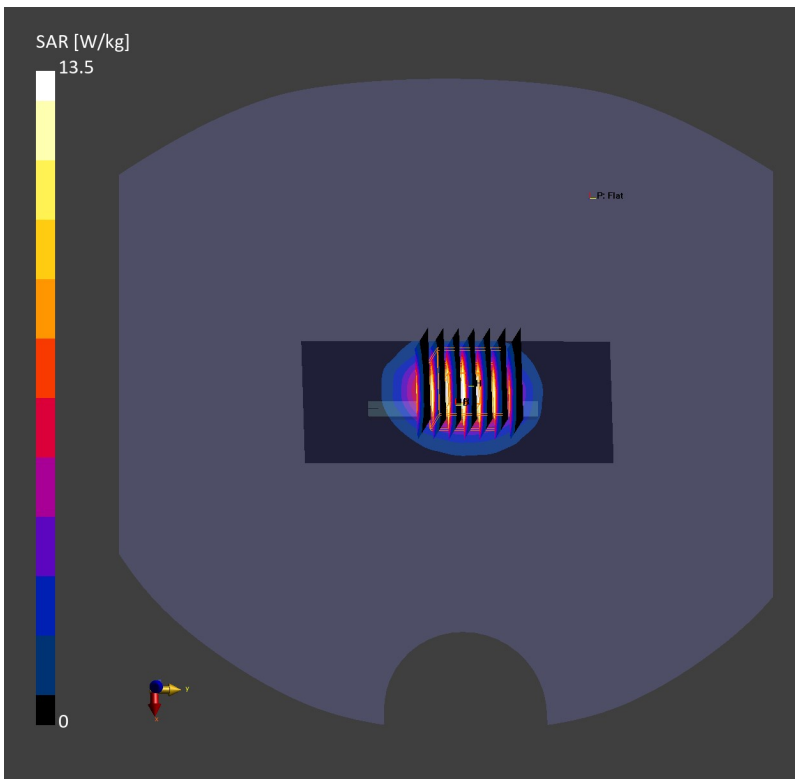

Date: 2026-01-11

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 36.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.99, 6.86, 6.89); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.95 W/kg; SAR (10g) = 2.44 W/kg;


Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.17 dB

SAR (1g) = 6.78 W/kg; SAR (10g) = 2.48 W/kg

Smallest distance from peaks to all points 3 dB below = 8.5 mm

Ratio of SAR at M2 to SAR at M1 = 78.9 %

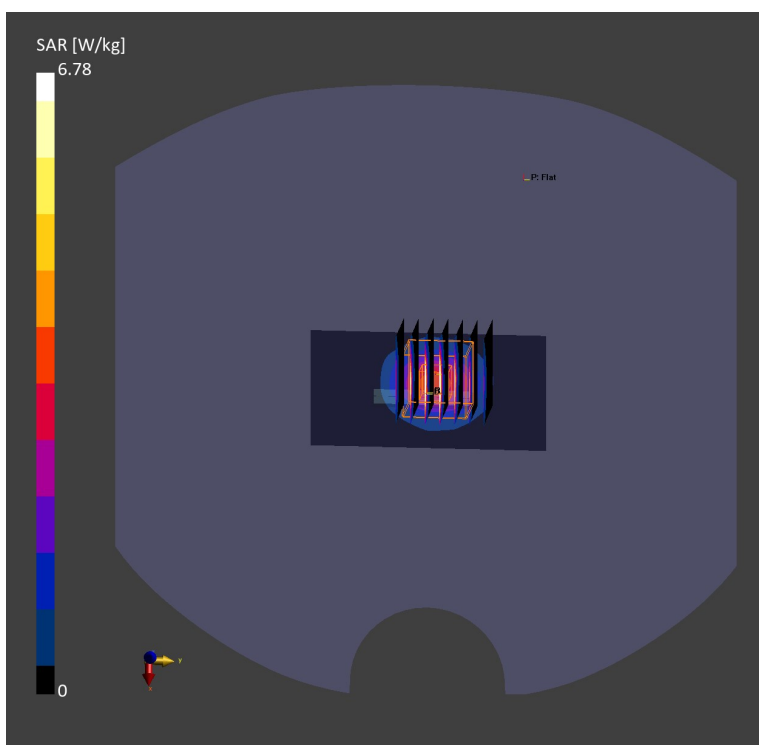

Date: 2026-01-07

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.99, 6.86, 6.89); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.99 W/kg; SAR (10g) = 2.56 W/kg;


Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 6.95 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 7.9 mm

Ratio of SAR at M2 to SAR at M1 = 78.8 %

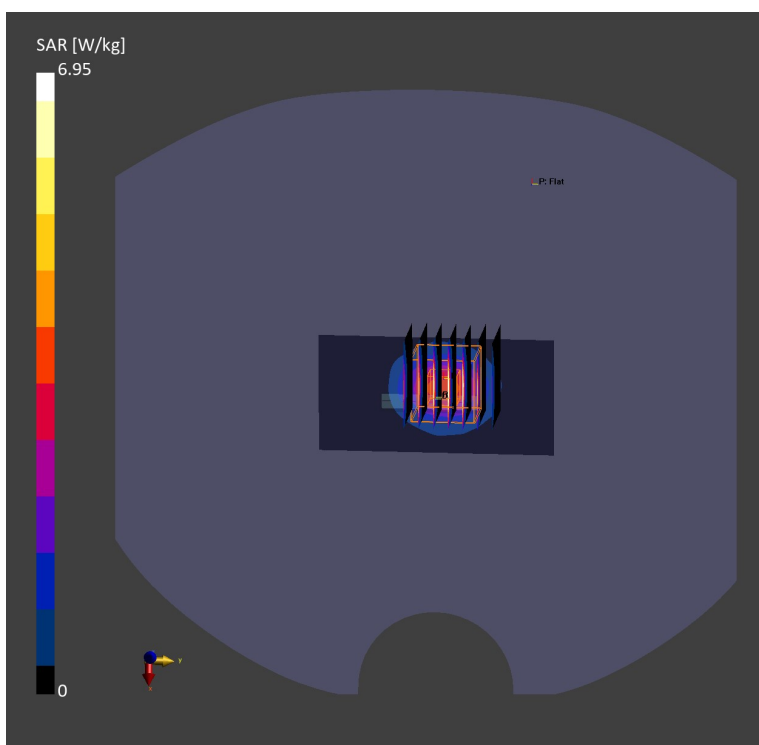

Date: 2026-01-13

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.85, 6.72, 6.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.58 W/kg; SAR (10g) = 2.26 W/kg;


Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.11 dB

SAR (1g) = 6.45 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

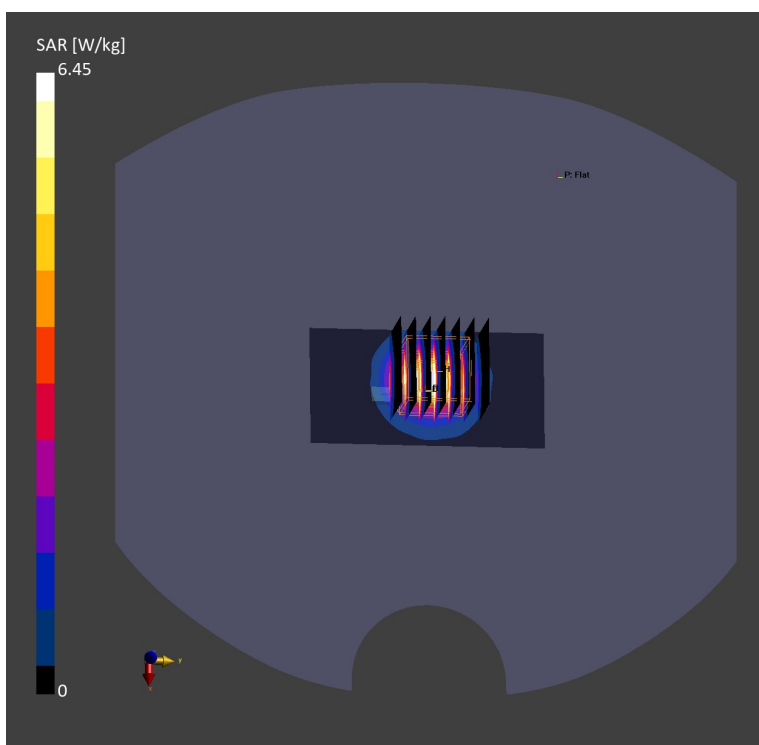

Date: 2026-01-04

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.14$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.85, 6.72, 6.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.02 W/kg; SAR (10g) = 2.46 W/kg;


Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.11 dB

SAR (1g) = 6.91 W/kg; SAR (10g) = 2.49 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 78.5 %

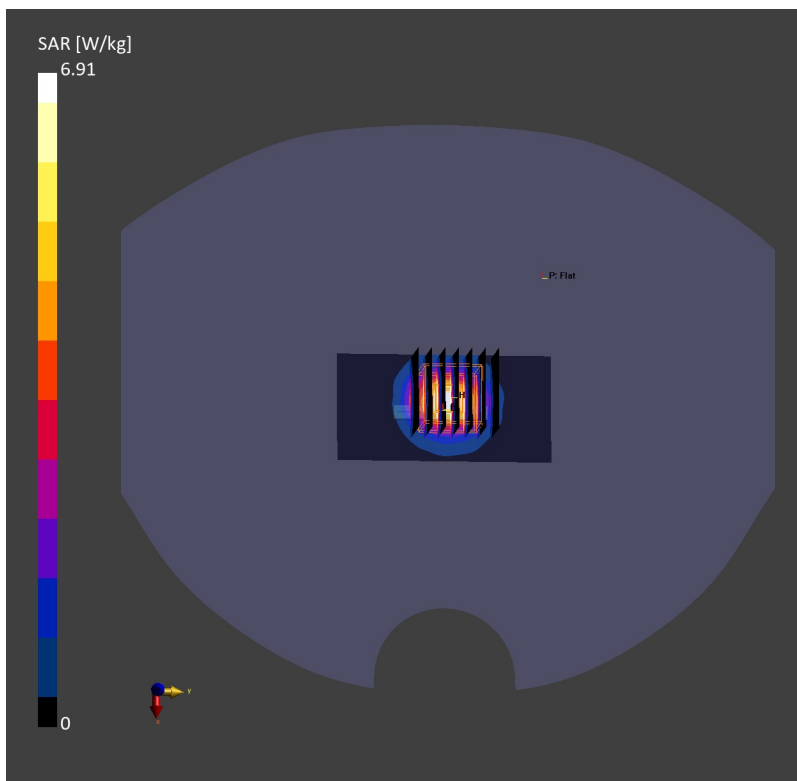

Date: 2026-01-14

System Check_3900MHz**DUT:D3900V2-SN:1022**

Communication System: CW; Frequency: 3900.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.26$ S/m; $\epsilon_r = 36.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.88, 6.76, 6.79); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.31 W/kg; SAR (10g) = 2.37 W/kg;


Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mmx 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 7.05 W/kg; SAR (10g) = 2.39 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

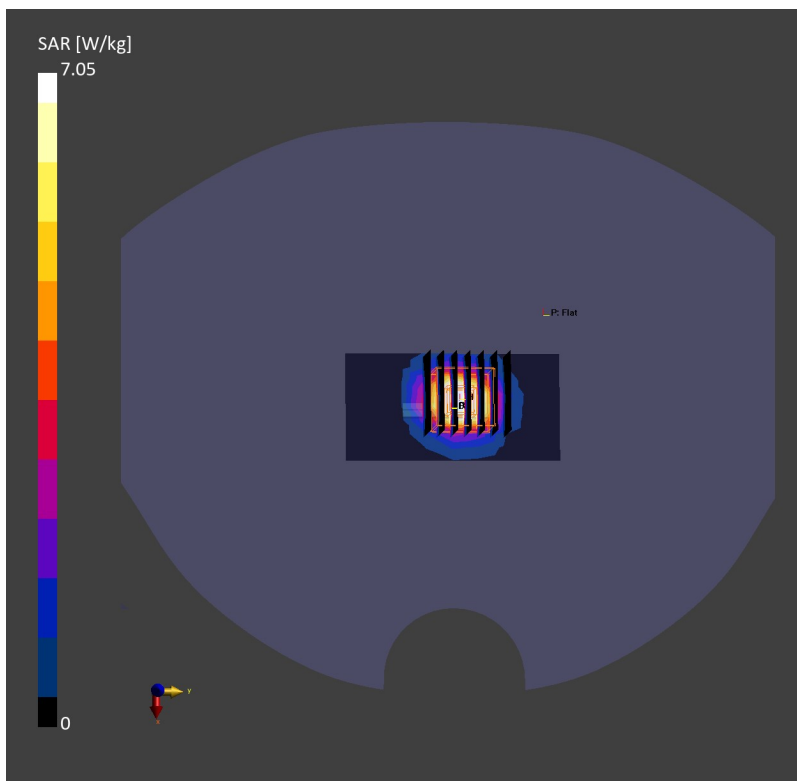

Date: 2025-12-20

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.0); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.99 W/kg; SAR (10g) = 2.38 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 7.99 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.7 mm

Ratio of SAR at M2 to SAR at M1 = 69.5 %

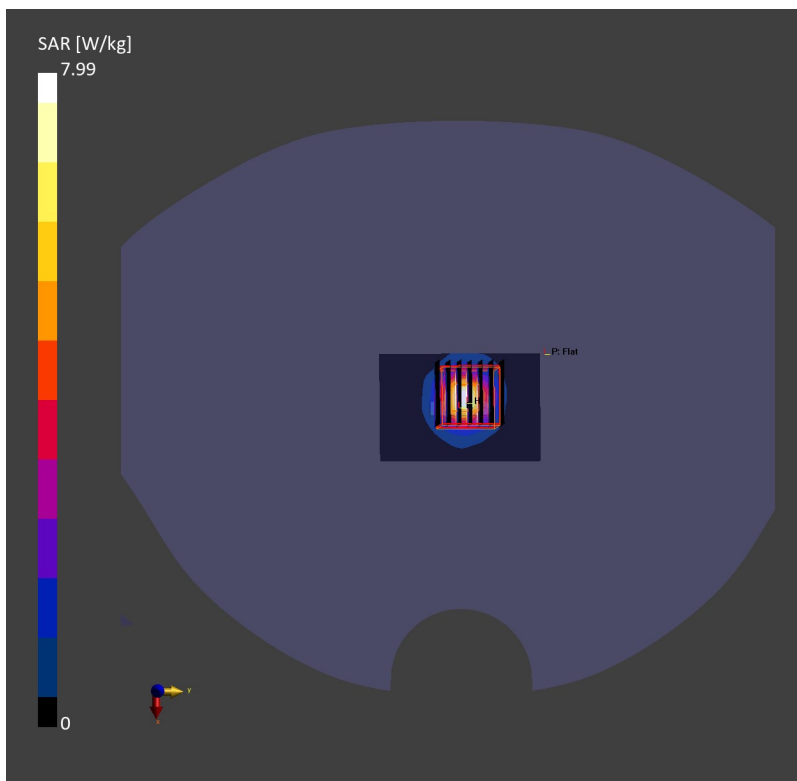

Date: 2026-01-07

System Check_5250MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.53$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.0); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.61 W/kg; SAR (10g) = 2.19 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.13 dB

SAR (1g) = 7.49 W/kg; SAR (10g) = 2.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.9 mm

Ratio of SAR at M2 to SAR at M1 = 68.8 %

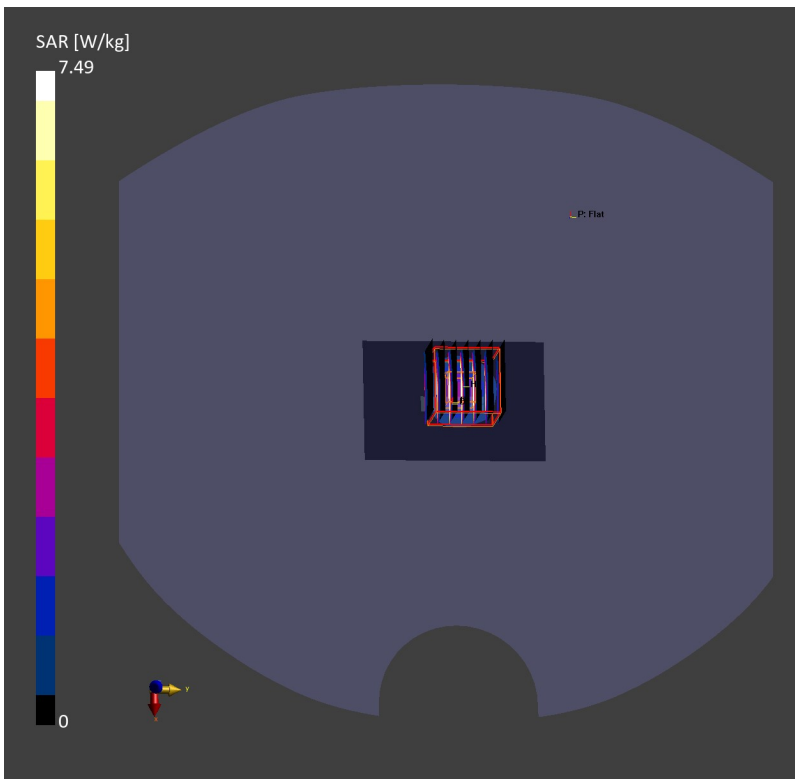

Date: 2025-12-22

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 8.21 W/kg; SAR (10g) = 2.28 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.11 W/kg; SAR (10g) = 2.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 69.7 %

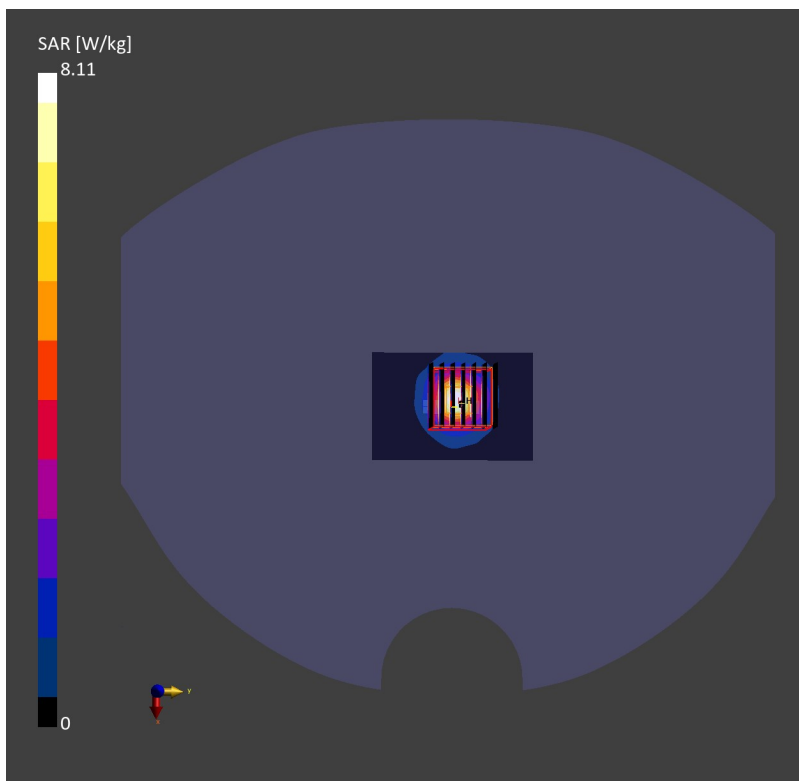

Date: 2026-01-09

System Check_5600MHz**DUT:D5GHzV2-SN:1113**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.88$ S/m; $\epsilon_r = 36.5$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.97 W/kg; SAR (10g) = 2.22 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.08 dB
SAR (1g) = 8.53 W/kg; SAR (10g) = 2.27 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 65.7 %

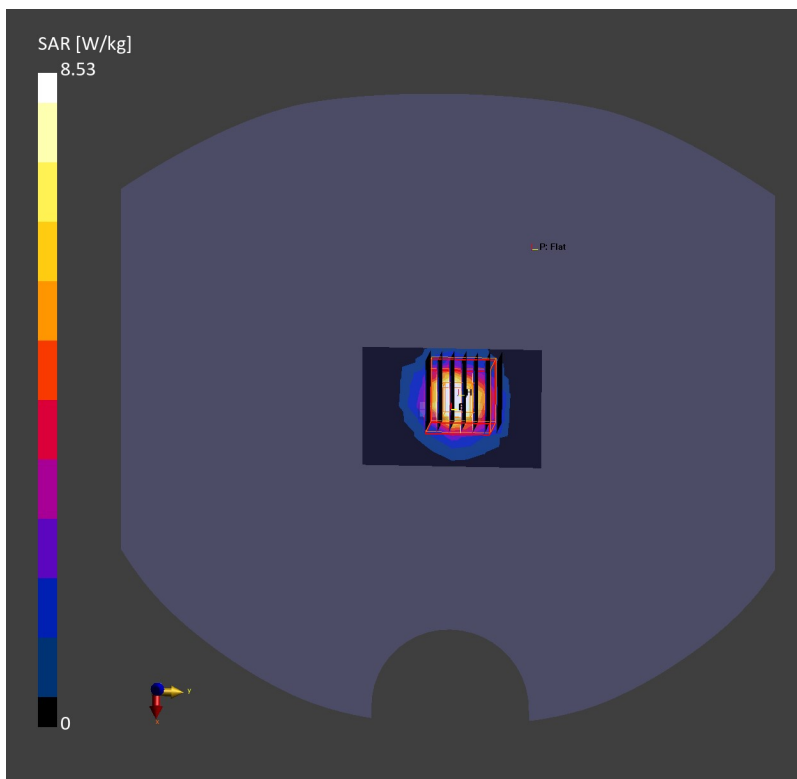

Date: 2025-12-23

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.07$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 8.05 W/kg; SAR (10g) = 2.43 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.07 dB

SAR (1g) = 8.22 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.5 %

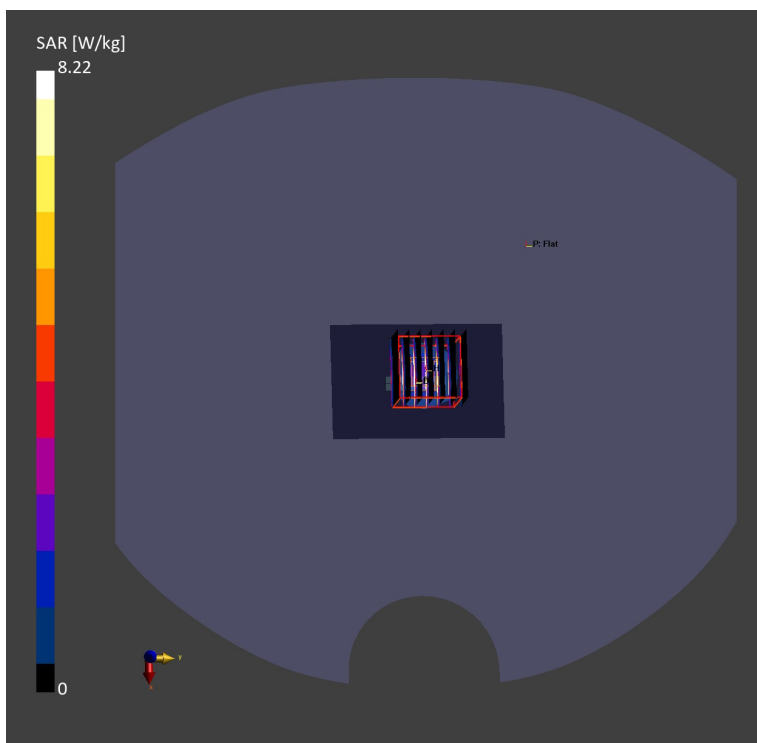

Date: 2026-01-08

System Check_5800MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 34.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.92 W/kg; SAR (10g) = 2.33 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 8.33 W/kg; SAR (10g) = 2.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 65.7 %

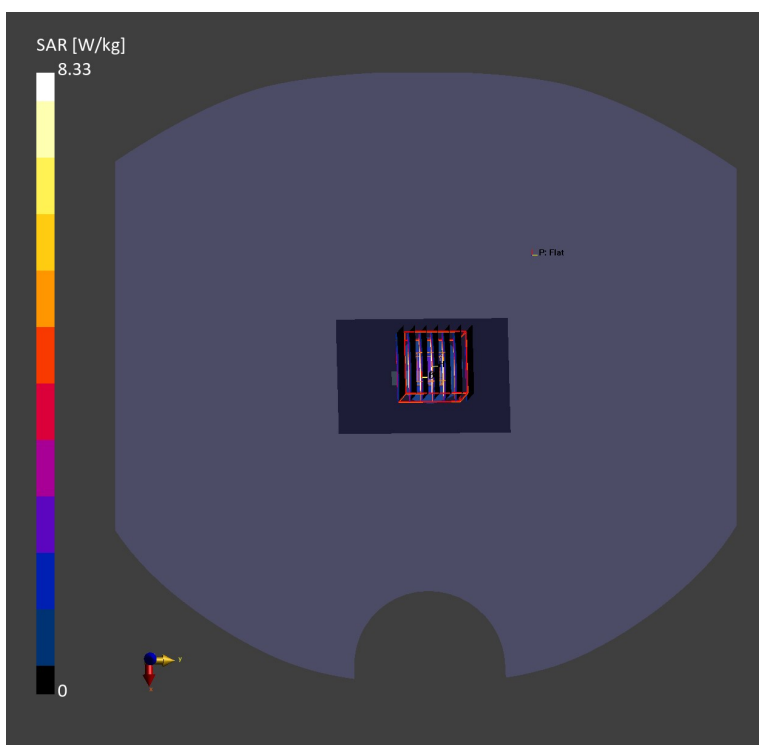

Date: 2026-03-10

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.85, 6.72, 6.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.68 W/kg; SAR (10g) = 2.27 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 6.37 W/kg; SAR (10g) = 2.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.1 %

