

Date: 2026/1/14

System Check_750MHz**DUT:D750V3-SN:1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.905$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.71, 9.32, 9.31); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025/11/28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 2.26 W/kg; SAR (10g) = 1.51 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.24 W/kg; SAR (10g) = 1.49 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

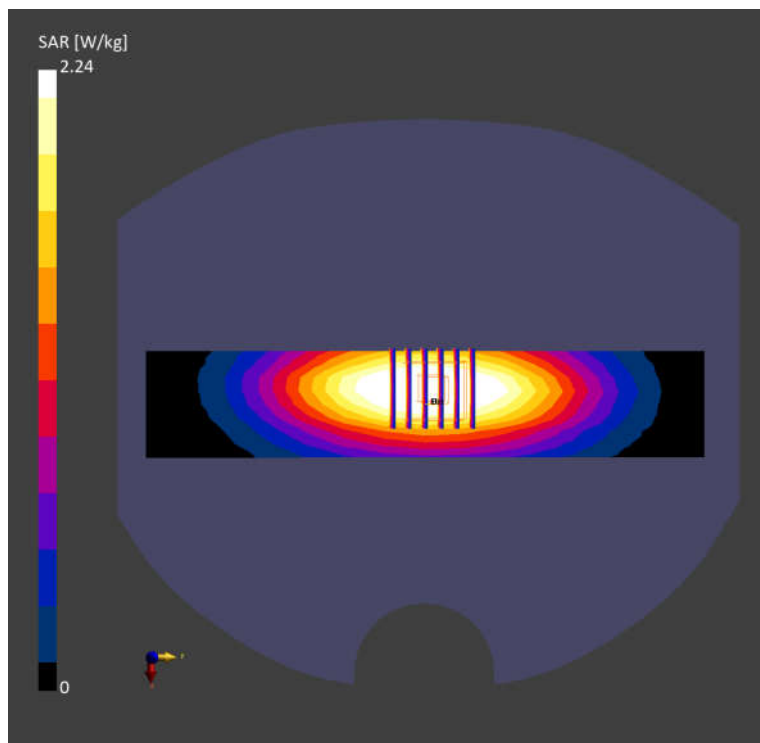

Date: 2026/1/29

System Check_1640MHz**DUT:D1640V2-SN:347**

Communication System: CW; Frequency: 1640.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1640.000$ MHz; $\sigma = 1.28$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.45, 8.29, 8.33); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025/11/28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (36.0 mm x 120.0 mm): Measurement Grid: 3.0 mm x 15.0 mm
SAR (1g) = 8.66 W/kg; SAR (10g) = 4.75 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 8.43 W/kg; SAR (10g) = 4.62 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

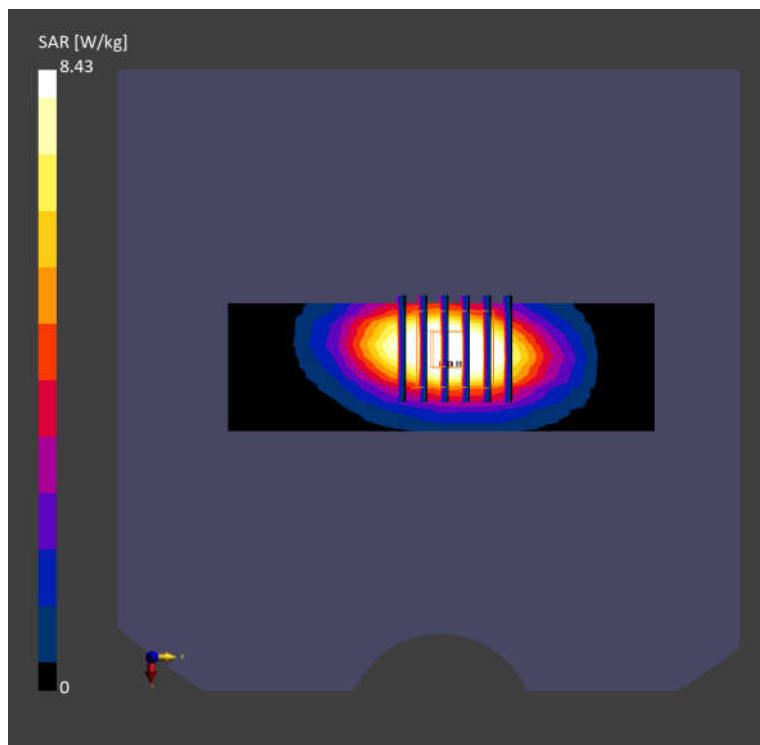

Date: 2026/1/16

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.31$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(8.14, 7.82, 7.81); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025/11/28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 9.27 W/kg; SAR (10g) = 5.00 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 9.18 W/kg; SAR (10g) = 4.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

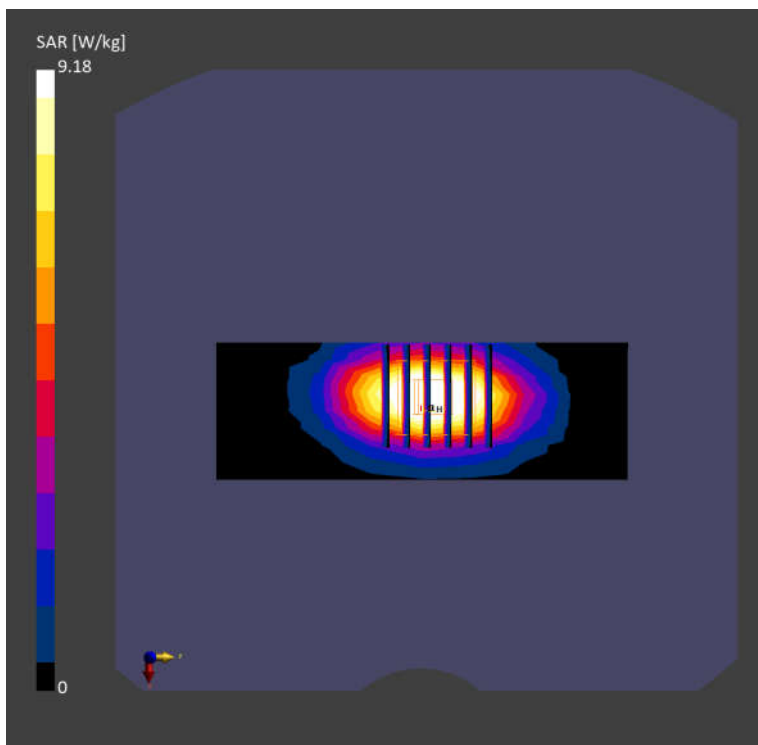

Date: 2026/1/18

System Check_1900MHz**DUT:D1900V2-SN:5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.9, 7.58, 7.57); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025/11/28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 11.2 W/kg; SAR (10g) = 5.82 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 10.2 W/kg; SAR (10g) = 5.42 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

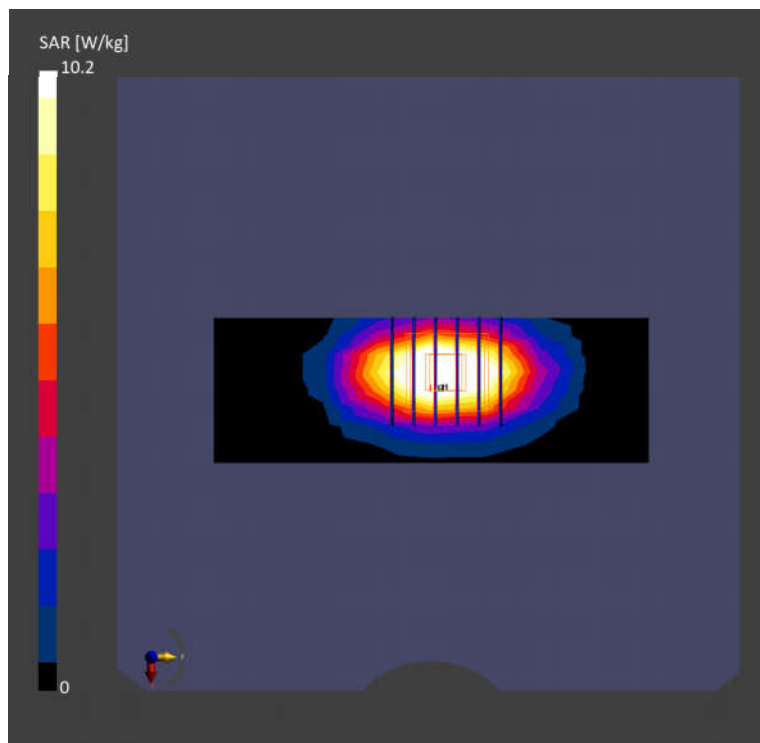

Date: 2026/1/20

System Check_2000MHz**DUT:D2000V2-SN:1071**

Communication System: CW; Frequency: 2000.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2000.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.75, 7.46, 7.45); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025/11/28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 10.1 W/kg; SAR (10g) = 5.20 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 10.1 W/kg; SAR (10g) = 5.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

