

WEGO

Intelligent Medical Consumables Management Cabinet



RoHS  **CE**

USER MANUAL

Product Introduction



This product is mainly used for storage and management of high-value consumables in warehouses of the operating room, the interventional room /DSA catheterization room, the endoscopy room / the gastroscopy center and other departments.

By using UHF RFID technology and long-distance batch identification, the refined management of high-value consumables in warehouses can be realized through one-thing one-code management mode.

Product Model



WEGOBX-01



WEGOBX-02




WEGOBX-03

Product Function

This product can be used in warehouses of the operating room , the interventional room / DSA catheter room, the endoscope room / the digestive gastroscopy center and other departments, for access, take, return,

inventory, query, multi-service early warning and other functions of high-value consumables, and can realize real-time record of personnel business operations.

Product Diagram

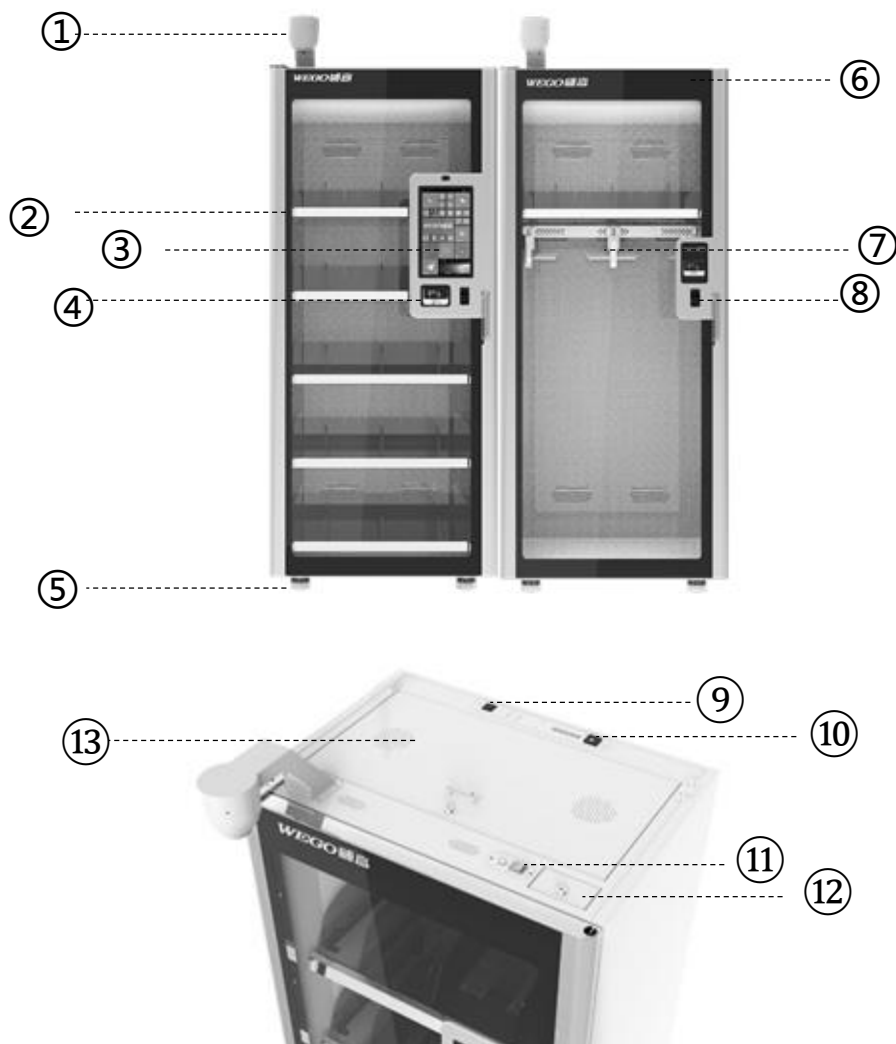

- ①Camera ②Laminate ③14"Operation screen ④Card swiping module
- ⑤Universal wheel ⑥LCD display screen ⑦Hanging piece hook
- ⑧Finger vein module ⑨Power cable interface ⑩Network interface
- ⑪Power switch ⑫Emergency zipper ⑬Central control cover plate

Matters need Attention

■ Open the door urgently

When it is found that the cabinet door cannot be opened normally, the emergency treatment plan is to pull the emergency zipper urgently, open the cabinet door, and take or return consumables.

■ Safe Operation

When troubleshooting, it is necessary to open the central control cover plate^⑬, make sure that the static electricity has been released or wear anti-static gloves before carrying out relevant operations.

■ Finger vein Entry

- Please do not press the finger vein module hard when registering, otherwise it will easily lead to unclear blood vessel scanning and poor quality of finger vein template.
- When registering, it needs to be verified at least 3 times, and the finger should be lifted and placed after each placement.
- When registering, do not press the glass surface with your finger, but place it in the module groove. It is recommended to use the index finger or middle finger.

FCC Statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Caution: Any changes or modifications to this device not explicitly approved by manufacturer could void your authority to operate this equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

RF Exposure Information

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with minimum distance 20cm between the radiator and your body.