

System Check: Head 750MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		CD750	CW, 0--	750.0, 100	10.64	0.906	41.9	22.8	21.4


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-14	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 160.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-14	2025-10-14
psSAR1g [W/kg]	0.818	0.823
psSAR10g [W/kg]	0.552	0.566
Power Drift [dB]	0.11	0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		85.1
Dist 3dB Peak [mm]		21.9

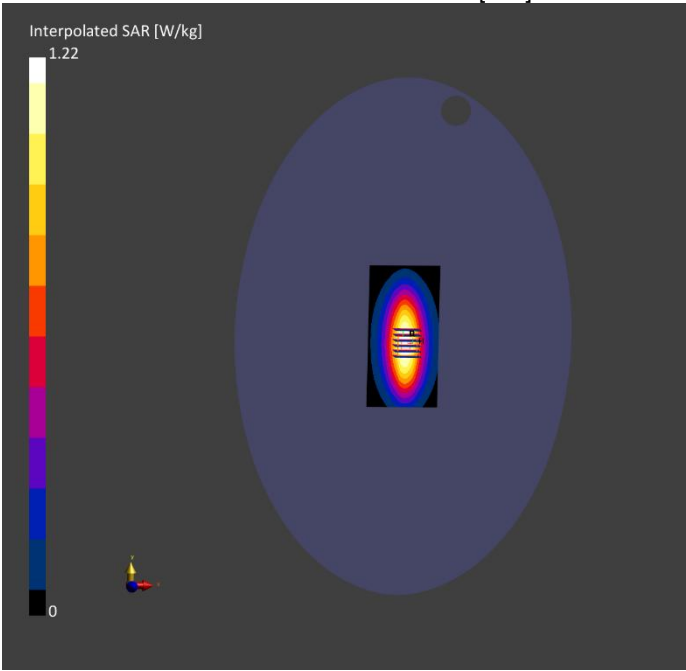

BL-SZ2591207-ASC

System Check: Head 750MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		CD750	CW, 0--	750.0, 100	10.64	0.897	41.8	22.2	21.9

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-15	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

Measurement Results

	Area Scan	Zoom Scan		Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 160.0	30.0 x 30.0 x 30.0	Date	2025-10-15	2025-10-15
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5	psSAR1g [W/kg]	0.862	0.878
Sensor Surface [mm]	3.0	1.4	psSAR10g [W/kg]	0.574	0.593
Graded Grid	Yes	Yes	Power Drift [dB]	-0.06	-0.03
Grading Ratio	1.5	1.5	Power Scaling	Disabled	Disabled
MAIA	N/A	N/A	Scaling Factor [dB]		
Surface Detection	All points	All points	TSL Correction	No correction	No correction
Scan Method	Measured	Measured	M2/M1 [%]		87.4
			Dist 3dB Peak [mm]		22.5

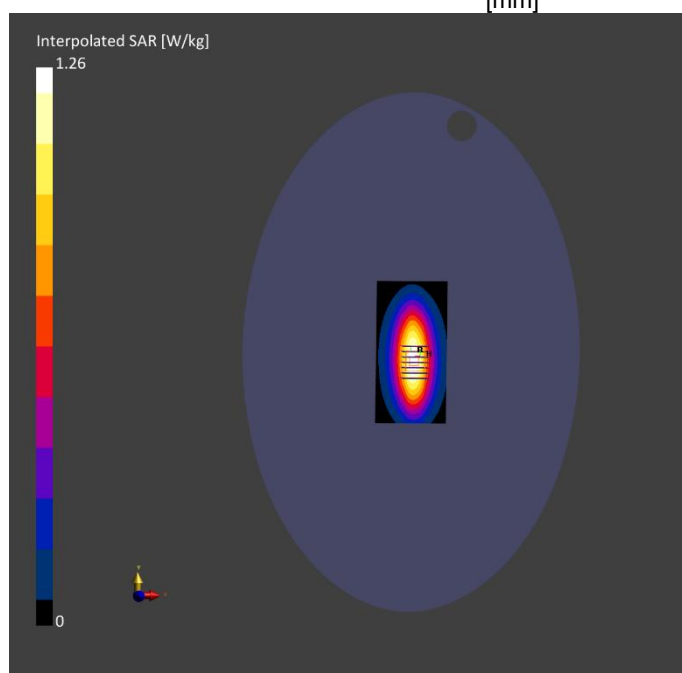

BL-SZ2591207-ASC

System Check: Head 750MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		CD750	CW, 0--	750.0, 100	10.64	0.898	41.7	22.5	21.7


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-16	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 160.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-16	2025-10-16
psSAR1g [W/kg]	0.833	0.862
psSAR10g [W/kg]	0.541	0.559
Power Drift [dB]	-0.09	-0.05
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		81.8
Dist 3dB Peak [mm]		21.3

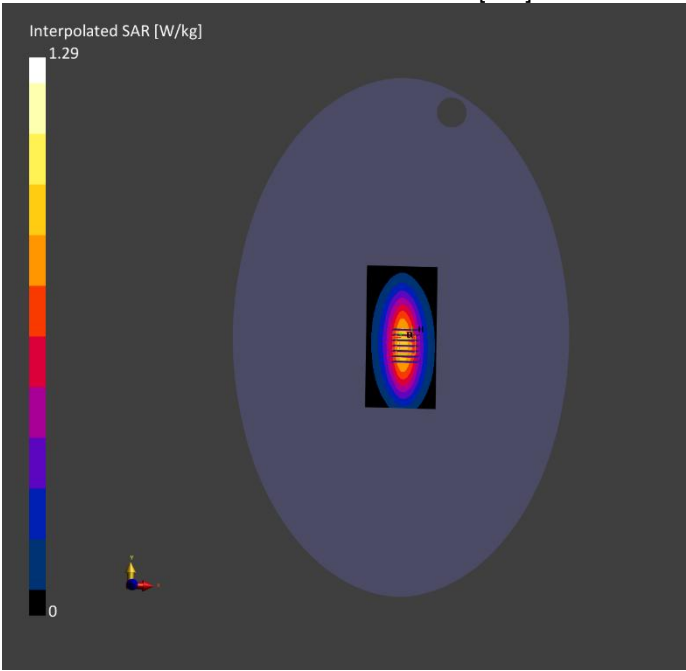

BL-SZ2591207-ASC

System Check: Head 835MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		CD835	CW, 0--	835.0, 50	10.25	0.895	41.7	22.3	21.5
Phantom	TSL, Measured Date			Probe, Calibration Date			DAE, Calibration Date		
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-17			EX3DV4 - SN7664, 2025-06-30			DAE4 Sn878, 2025-03-05		

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 160.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-17	2025-10-17
psSAR1g [W/kg]	0.932	0.941
psSAR10g [W/kg]	0.614	0.624
Power Drift [dB]	-0.11	0.09
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		79.5
Dist 3dB Peak [mm]		18.7

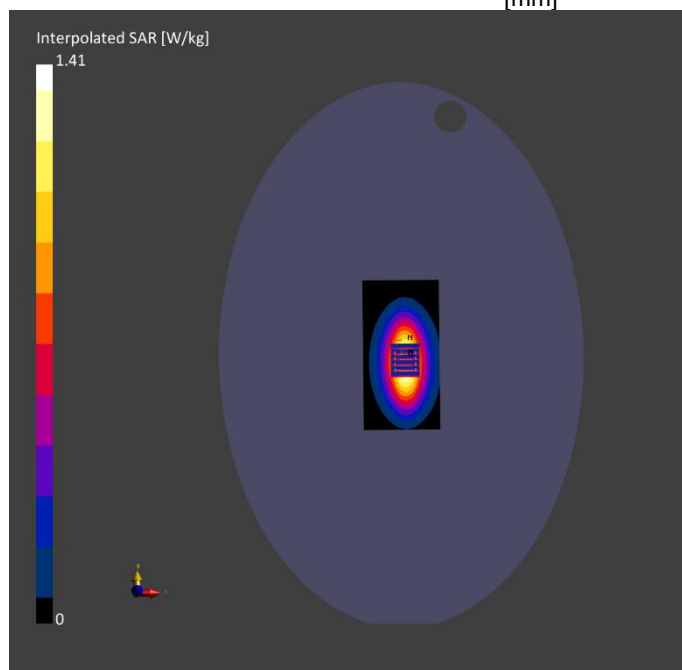

BL-SZ2591207-ASC

System Check: Head 835MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
----------------------	------------------------------	------	------------	---------------------------------	-------------------	------------------------	------------------	--------------------------	-------------------------

Flat, HSL Hardware Setup		CD835	CW, 0--	835.0, 50	10.25	0.891	42.1	22.4	21.8
--------------------------	--	-------	---------	-----------	-------	-------	------	------	------


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-18	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 160.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-18	2025-10-18
psSAR1g [W/kg]	0.949	0.957
psSAR10g [W/kg]	0.638	0.653
Power Drift [dB]	-0.04	0.17
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		77.5
Dist 3dB Peak [mm]		17.2

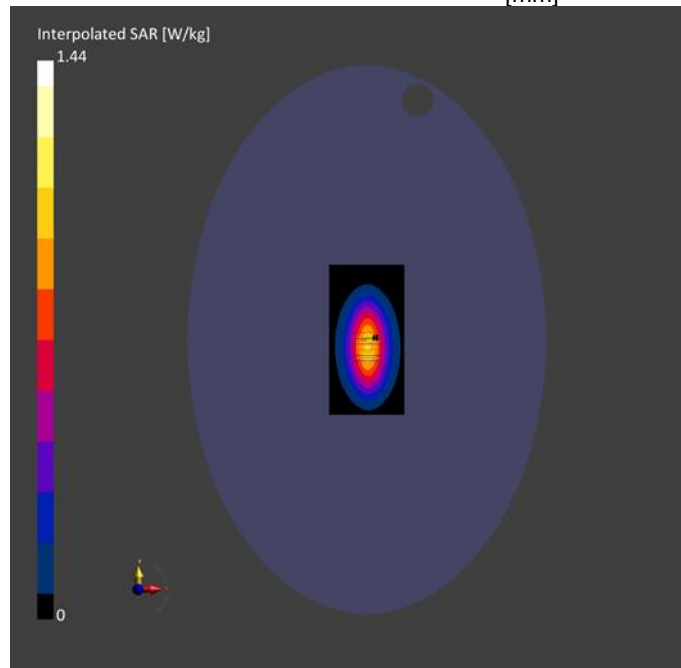

BL-SZ2591207-ASC

System Check: Head 1750MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		D1750	CW, 0--	1750.0, 50	8.72	1.38	40.1	22.6	21.3
Phantom	TSL, Measured Date			Probe, Calibration Date			DAE, Calibration Date		
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-19			EX3DV4 - SN7664, 2025-06-30			DAE4 Sn878, 2025-03-05		

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-19	2025-10-19
psSAR1g [W/kg]	3.51	3.59
psSAR10g [W/kg]	1.86	1.94
Power Drift [dB]	0.15	0.02
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		82.3
Dist 3dB Peak [mm]		12.7

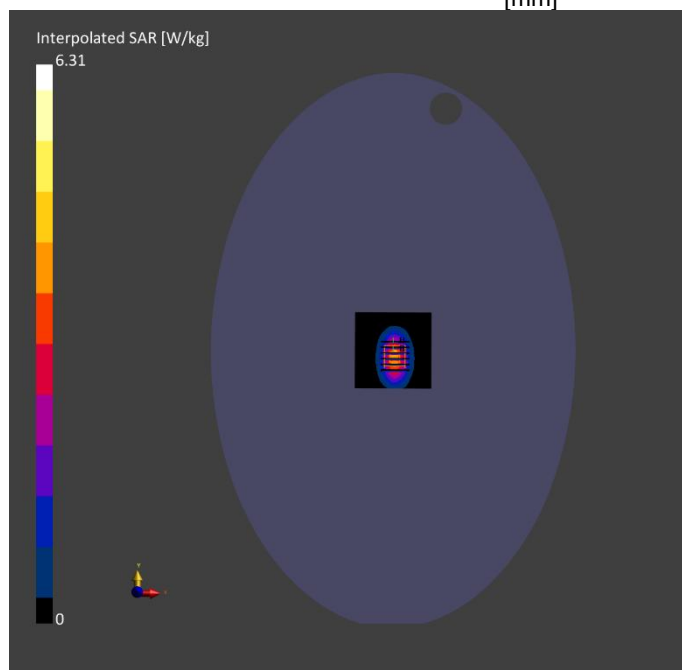

BL-SZ2591207-ASC

System Check: Head 1750MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		D1750	CW, 0--	1750.0, 50	8.72	1.38	40.1	22.8	21.8
Phantom	TSL, Measured Date			Probe, Calibration Date			DAE, Calibration Date		
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-20			EX3DV4 - SN7664, 2025-06-30			DAE4 Sn878, 2025-03-05		

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-20	2025-10-20
psSAR1g [W/kg]	3.56	3.77
psSAR10g [W/kg]	1.92	2.06
Power Drift [dB]	0.14	0.17
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		80.7
Dist 3dB Peak [mm]		11.9

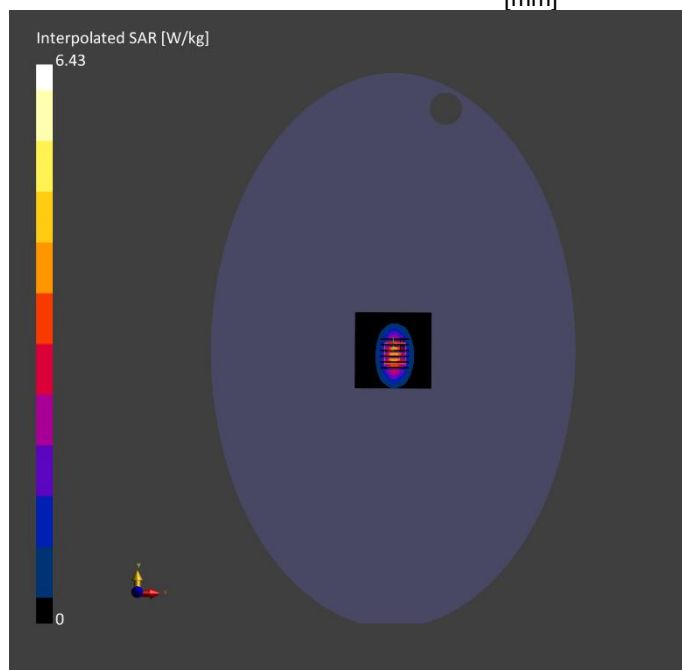

BL-SZ2591207-ASC

System Check: Head 1950MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		D1950	CW, 0--	1950.0, 50	8.35	1.42	39.1	22.1	21.6
Phantom	TSL, Measured Date			Probe, Calibration Date			DAE, Calibration Date		
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-21			EX3DV4 - SN7664, 2025-06-30			DAE4 Sn878, 2025-03-05		

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-21	2025-10-21
psSAR1g [W/kg]	4.26	4.31
psSAR10g [W/kg]	2.08	2.15
Power Drift [dB]	0.02	0.06
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		82.9
Dist 3dB Peak [mm]		10.4

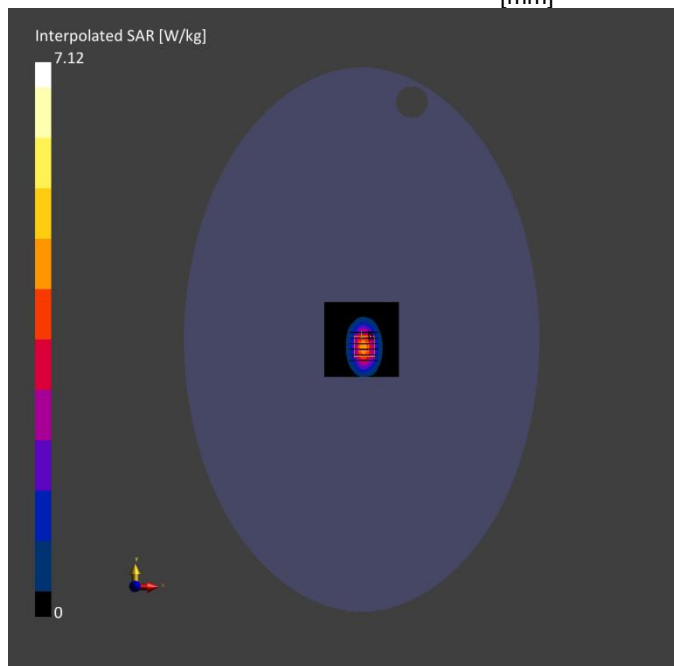

BL-SZ2591207-ASC

System Check: Head 1950MHz

Exposure Conditions


Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL Hardware Setup		D1950	CW, 0--	1950.0, 50	8.35	1.42	39.2	22.3	21.1
Phantom	TSL, Measured Date			Probe, Calibration Date			DAE, Calibration Date		
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-22			EX3DV4 - SN7664, 2025-06-30			DAE4 Sn878, 2025-03-05		

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-22	2025-10-22
psSAR1g [W/kg]	4.01	4.08
psSAR10g [W/kg]	2.17	2.23
Power Drift [dB]	0.11	0.15
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		77.4
Dist 3dB Peak [mm]		9.9

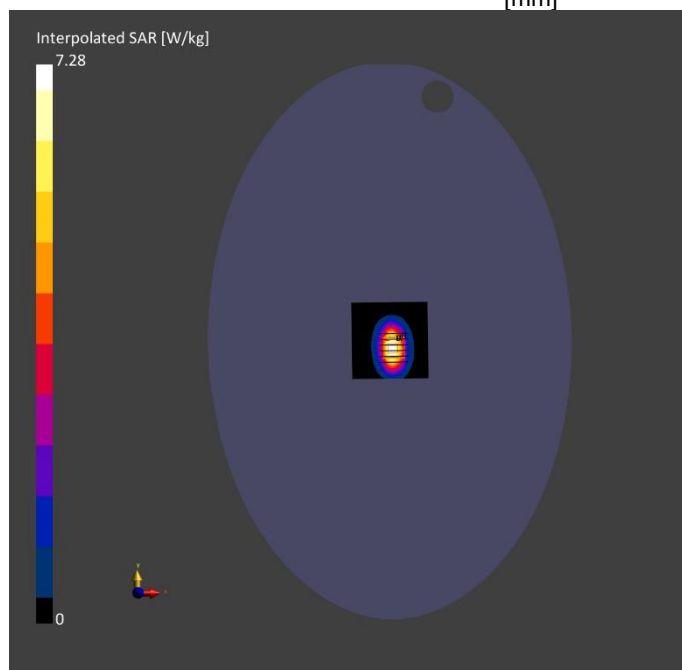

BL-SZ2591207-ASC

System Check: Head 2450MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		D2450	CW, 0--	2450.0, 50	7.80	1.80	39.4	22.7	21.4

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-23	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-23	2025-10-23
psSAR1g [W/kg]	5.25	5.38
psSAR10g [W/kg]	2.46	2.55
Power Drift [dB]	-0.13	0.09
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		78.1
Dist 3dB Peak [mm]		9.3

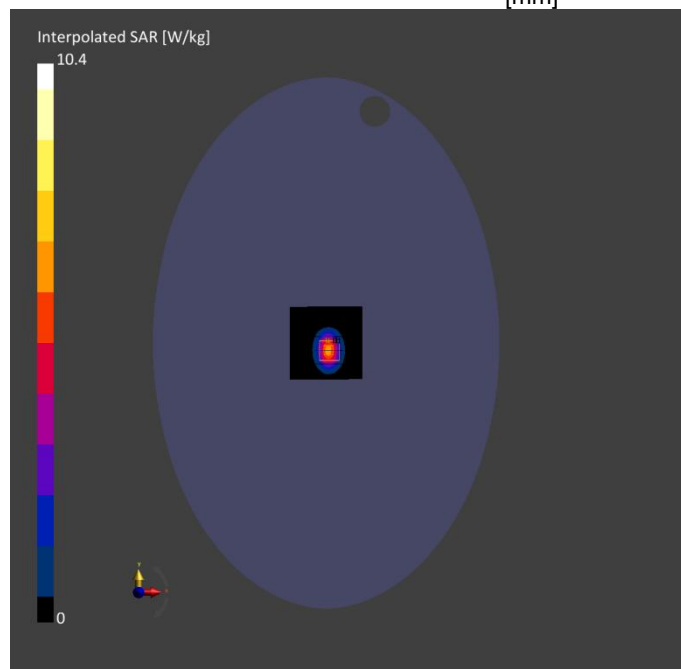

BL-SZ2591207-ASC

System Check: Head 2600MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		CD2600	CW, 0--	2600.0, 50	7.64	1.98	38.4	22.2	21.9

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-24	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-24	2025-10-24
psSAR1g [W/kg]	5.58	5.74
psSAR10g [W/kg]	2.51	2.63
Power Drift [dB]	-0.13	0.07
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		79.9
Dist 3dB Peak [mm]		9.8

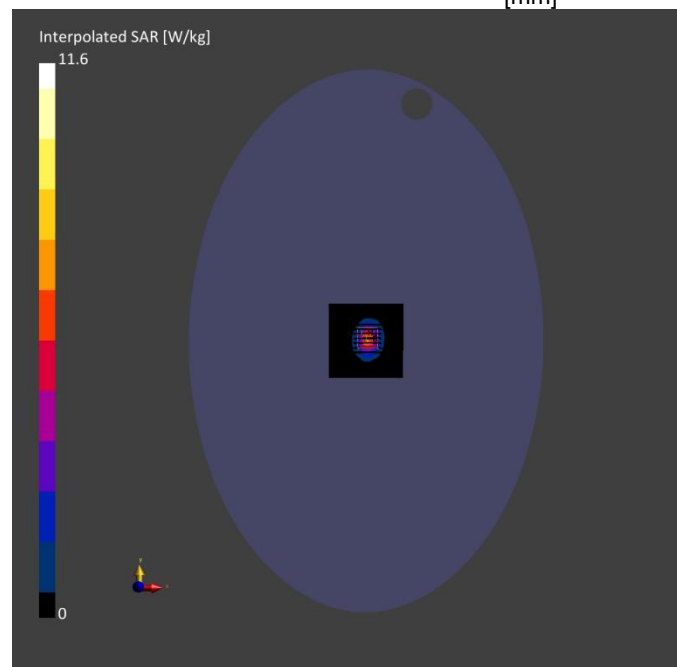

BL-SZ2591207-ASC

System Check: Head 2600MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		CD2600	CW, 0--	2600.0, 50	7.64	1.98	38.4	22.7	21.8

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-25	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-25	2025-10-25
psSAR1g [W/kg]	5.57	5.68
psSAR10g [W/kg]	2.34	2.48
Power Drift [dB]	0.18	0.13
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		80.7
Dist 3dB Peak [mm]		11.5

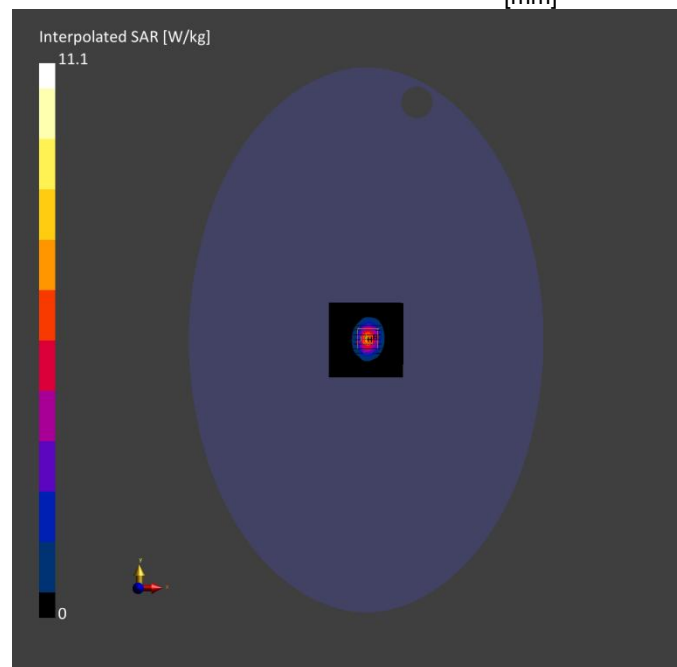

BL-SZ2591207-ASC

System Check: Head 2600MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		CD2600	CW, 0--	2600.0, 50	7.64	1.98	38.3	22.8	21.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-26	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-26	2025-10-26
psSAR1g [W/kg]	5.17	5.32
psSAR10g [W/kg]	2.41	2.46
Power Drift [dB]	0.06	0.08
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		79.2
Dist 3dB Peak [mm]		8.1

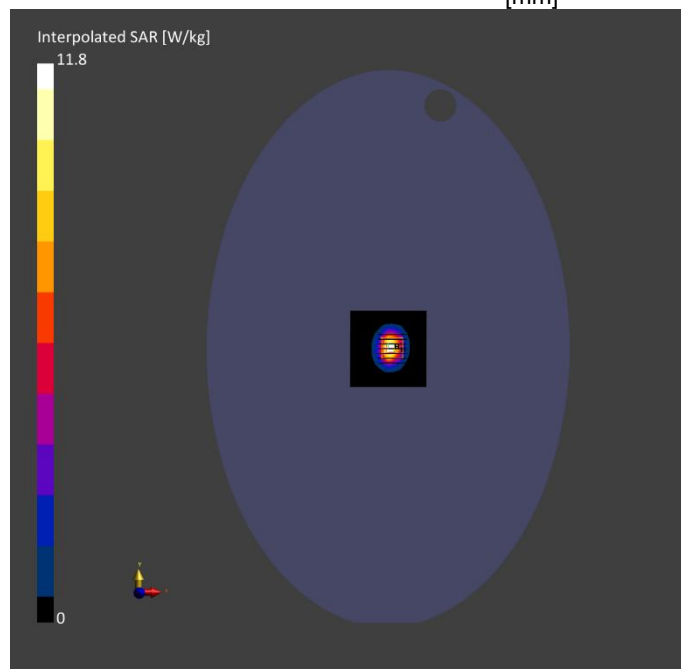

BL-SZ2591207-ASC

System Check: Head 3500MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		Custom Band	CW, 0--	3500.0, 3500000	7.02	2.87	38.5	22.6	21.3

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-27	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-27	2025-10-27
psSAR1g [W/kg]	6.84	6.93
psSAR10g [W/kg]	2.59	2.65
Power Drift [dB]	0.16	0.11
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		76.3
Dist 3dB Peak [mm]		10.2

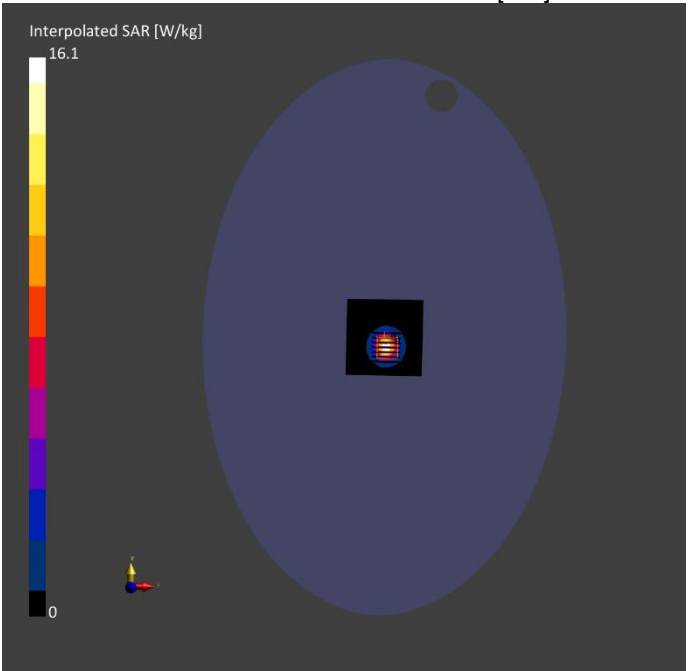

BL-SZ2591207-ASC

System Check: Head 3700MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity	Ambient Temperature [°C]	Liquid Temperature [°C]
Flat, HSL		Custom Band	CW, 0--	3700.0, 3700000	6.85	3.13	37.8	22.6	21.3

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2159	HBBL-600-10000 2025-10-27	EX3DV4 - SN7664, 2025-06-30	DAE4 Sn878, 2025-03-05

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	Yes	Yes
Grading Ratio	1.5	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-10-27	2025-10-27
psSAR1g [W/kg]	6.66	6.78
psSAR10g [W/kg]	2.35	2.42
Power Drift [dB]	-0.17	0.09
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction
M2/M1 [%]		75.8
Dist 3dB Peak [mm]		8.8

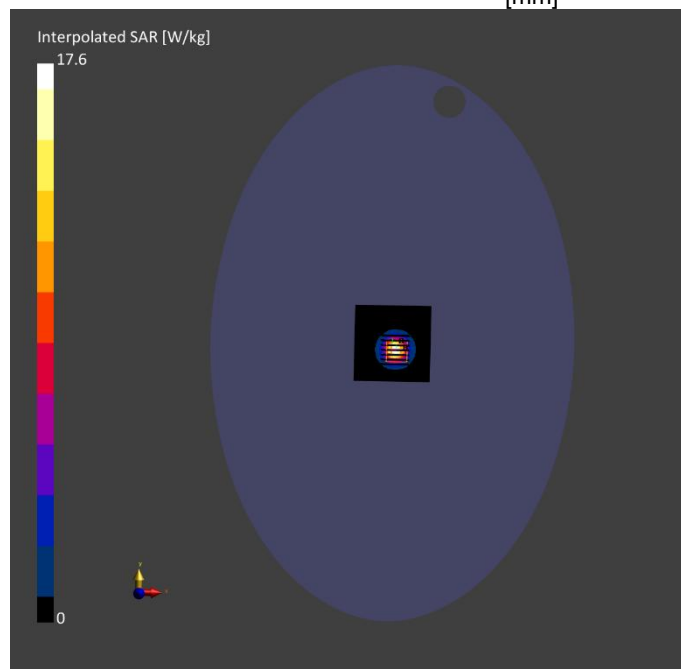

--BLANK BELOW--