



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: GFSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:15:40

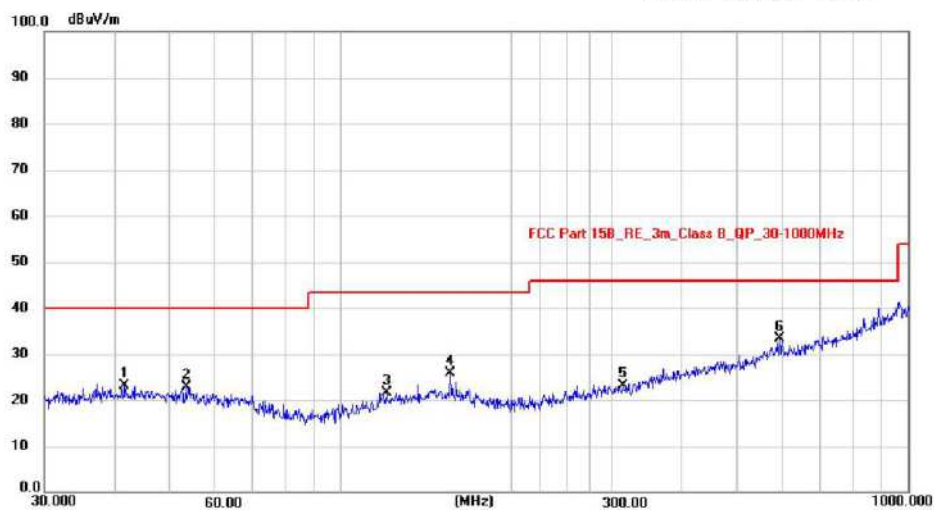

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 41.5670         | 8.72           | 14.50         | 23.22          | 40.00          | -16.78      | peak     | 100         | 78             | P   |        |
| 2   | 53.3180         | 9.18           | 13.81         | 22.99          | 40.00          | -17.01      | peak     | 100         | 206            | P   |        |
| 3   | 120.2766        | 9.15           | 12.57         | 21.72          | 43.50          | -21.78      | peak     | 100         | 249            | P   |        |
| 4   | 155.9101        | 11.60          | 14.26         | 25.86          | 43.50          | -17.64      | peak     | 100         | 357            | P   |        |
| 5   | 314.3763        | 7.70           | 15.31         | 23.01          | 46.00          | -22.99      | peak     | 100         | 314            | P   |        |
| 6 * | 593.0496        | 10.70          | 22.70         | 33.40          | 46.00          | -12.60      | peak     | 100         | 306            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: GFSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:19:00

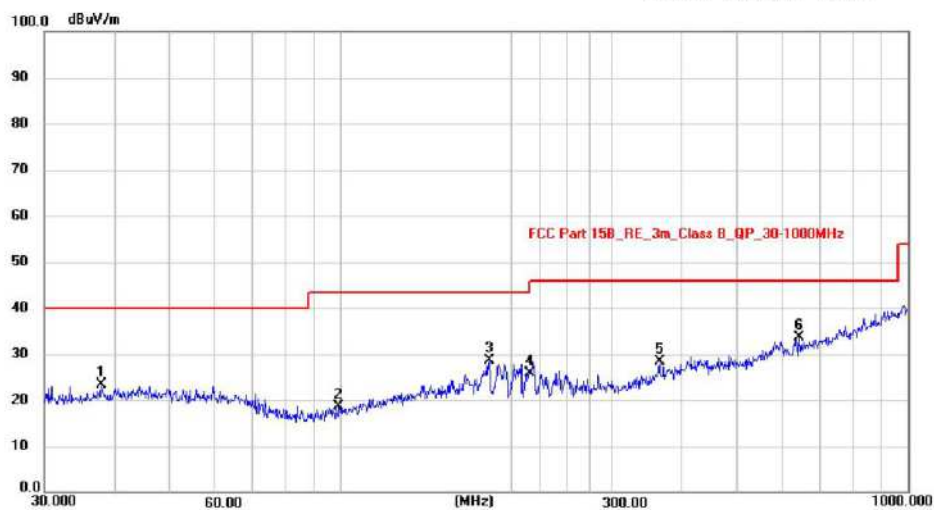

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 37.8121         | 9.06           | 14.25         | 23.31          | 40.00          | -16.69      | peak     | 200         | 106            | P   |        |
| 2   | 99.5279         | 8.00           | 10.56         | 18.56          | 43.50          | -24.94      | peak     | 200         | 196            | P   |        |
| 3   | 182.5592        | 16.51          | 12.24         | 28.75          | 43.50          | -14.75      | peak     | 200         | 128            | P   |        |
| 4   | 215.2676        | 14.26          | 11.72         | 25.98          | 43.50          | -17.52      | peak     | 200         | 254            | P   |        |
| 5   | 364.2595        | 11.75          | 16.72         | 28.47          | 46.00          | -17.53      | peak     | 200         | 299            | P   |        |
| 6 * | 642.8612        | 10.03          | 23.58         | 33.61          | 46.00          | -12.39      | peak     | 200         | 206            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:22:21

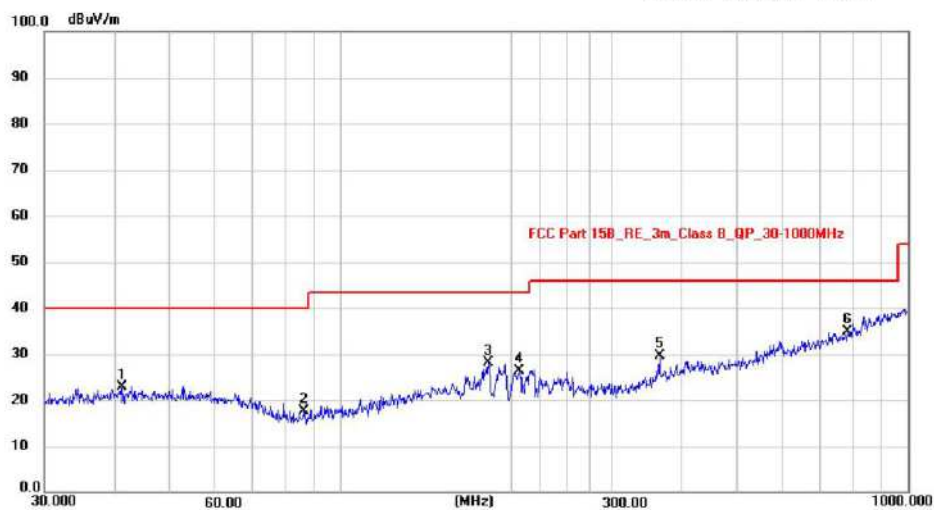

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 41.1320         | 8.27           | 14.52         | 22.79          | 40.00          | -17.21      | peak     | 200         | 329            | P   |        |
| 2   | 85.8983         | 8.02           | 9.62          | 17.64          | 40.00          | -22.36      | peak     | 200         | 346            | P   |        |
| 3   | 181.9202        | 15.84          | 12.27         | 28.11          | 43.50          | -15.39      | peak     | 200         | 225            | P   |        |
| 4   | 206.3975        | 15.07          | 11.39         | 26.46          | 43.50          | -17.04      | peak     | 200         | 298            | P   |        |
| 5   | 364.2595        | 12.82          | 16.72         | 29.54          | 46.00          | -16.46      | peak     | 200         | 108            | P   |        |
| 6 * | 782.3451        | 8.91           | 26.02         | 34.93          | 46.00          | -11.07      | peak     | 200         | 168            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:25:02

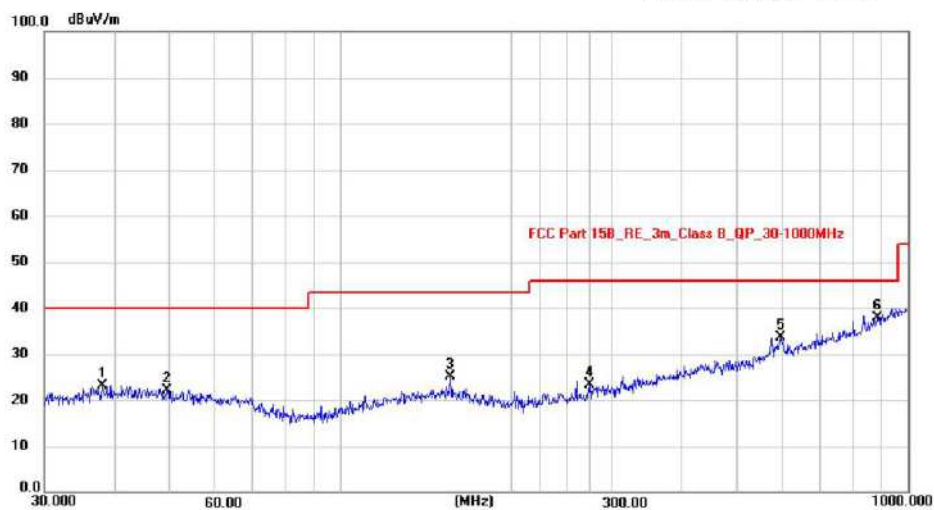

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 37.9450         | 8.88           | 14.27         | 23.15          | 40.00          | -16.85      | peak     | 100         | 157            | P   |        |
| 2   | 49.3594         | 7.87           | 14.17         | 22.04          | 40.00          | -17.96      | peak     | 100         | 214            | P   |        |
| 3   | 155.9101        | 10.94          | 14.26         | 25.20          | 43.50          | -18.30      | peak     | 100         | 236            | P   |        |
| 4   | 274.1938        | 9.10           | 14.28         | 23.38          | 46.00          | -22.62      | peak     | 100         | 255            | P   |        |
| 5   | 595.1326        | 10.97          | 22.75         | 33.72          | 46.00          | -12.28      | peak     | 100         | 325            | P   |        |
| 6 * | 881.4067        | 10.13          | 27.75         | 37.88          | 46.00          | -8.12       | peak     | 100         | 85             | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2441MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:28:17

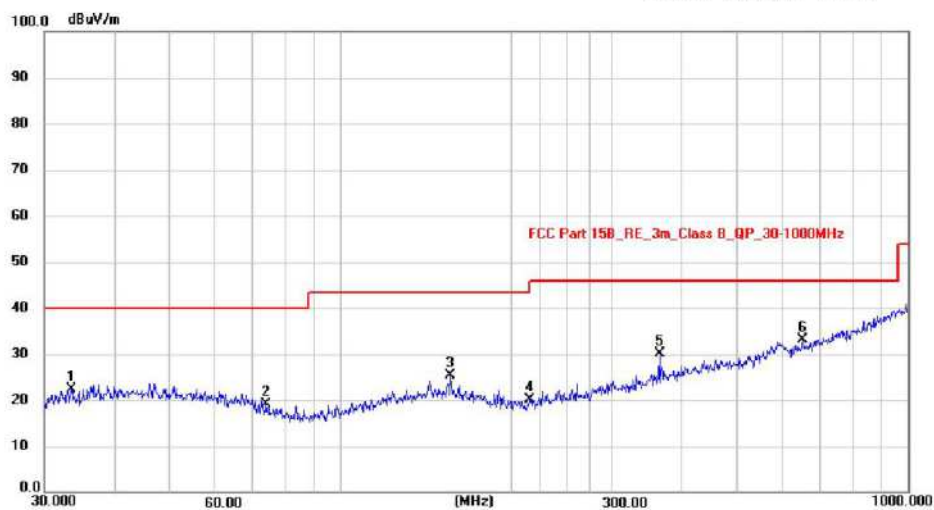

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 33.4450         | 8.92           | 13.57         | 22.49          | 40.00          | -17.51      | peak     | 100         | 279            | P   |        |
| 2   | 73.8756         | 7.95           | 11.06         | 19.01          | 40.00          | -20.99      | peak     | 100         | 169            | P   |        |
| 3   | 155.9101        | 11.22          | 14.26         | 25.48          | 43.50          | -18.02      | peak     | 100         | 304            | P   |        |
| 4   | 215.2676        | 8.51           | 11.72         | 20.23          | 43.50          | -23.27      | peak     | 100         | 216            | P   |        |
| 5   | 364.2595        | 13.30          | 16.72         | 30.02          | 46.00          | -15.98      | peak     | 100         | 84             | P   |        |
| 6 * | 651.9415        | 9.37           | 23.73         | 33.10          | 46.00          | -12.90      | peak     | 100         | 300            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2441MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:32:38



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 35.4992         | 9.45           | 13.91         | 23.36          | 40.00          | -16.64      | peak     | 200         | 168            | P   |        |
| 2   | 48.3316         | 9.27           | 14.21         | 23.48          | 40.00          | -16.52      | peak     | 200         | 89             | P   |        |
| 3   | 118.1860        | 8.81           | 12.38         | 21.19          | 43.50          | -22.31      | peak     | 200         | 137            | P   |        |
| 4 * | 194.4534        | 16.64          | 11.50         | 28.14          | 43.50          | -15.36      | peak     | 200         | 164            | P   |        |
| 5   | 219.0753        | 17.23          | 11.87         | 29.10          | 46.00          | -16.90      | peak     | 200         | 229            | P   |        |
| 6   | 468.8761        | 9.88           | 19.40         | 29.28          | 46.00          | -16.72      | peak     | 200         | 325            | P   |        |

Note: \*:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:36:56

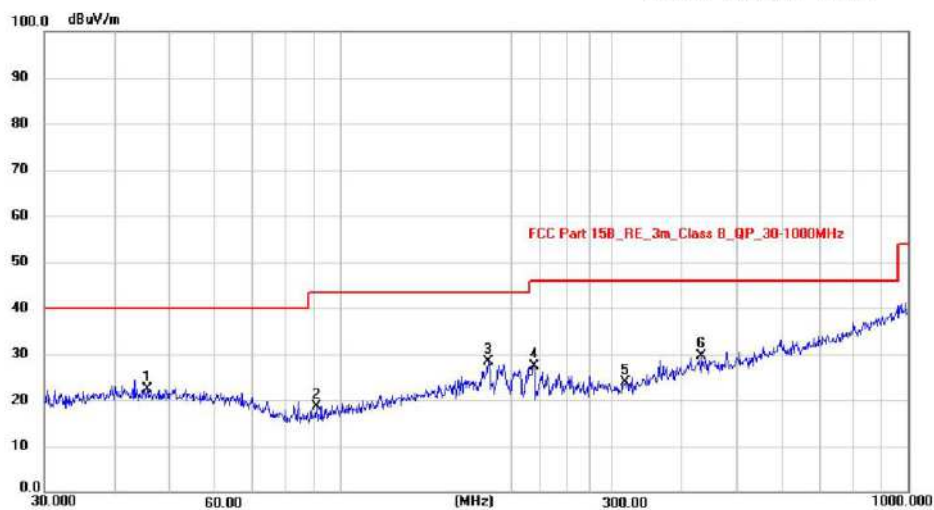

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 45.5347         | 8.17           | 14.33         | 22.50          | 40.00          | -17.50      | peak     | 200         | 116            | P   |        |
| 2   | 90.5374         | 8.82           | 9.77          | 18.59          | 43.50          | -24.91      | peak     | 200         | 225            | P   |        |
| 3 * | 181.9202        | 16.08          | 12.27         | 28.35          | 43.50          | -15.15      | peak     | 200         | 307            | P   |        |
| 4   | 219.0753        | 15.63          | 11.87         | 27.50          | 46.00          | -18.50      | peak     | 200         | 249            | P   |        |
| 5   | 316.5890        | 8.58           | 15.37         | 23.95          | 46.00          | -22.05      | peak     | 200         | 58             | P   |        |
| 6   | 432.5455        | 11.04          | 18.52         | 29.56          | 46.00          | -16.44      | peak     | 200         | 358            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:41:16

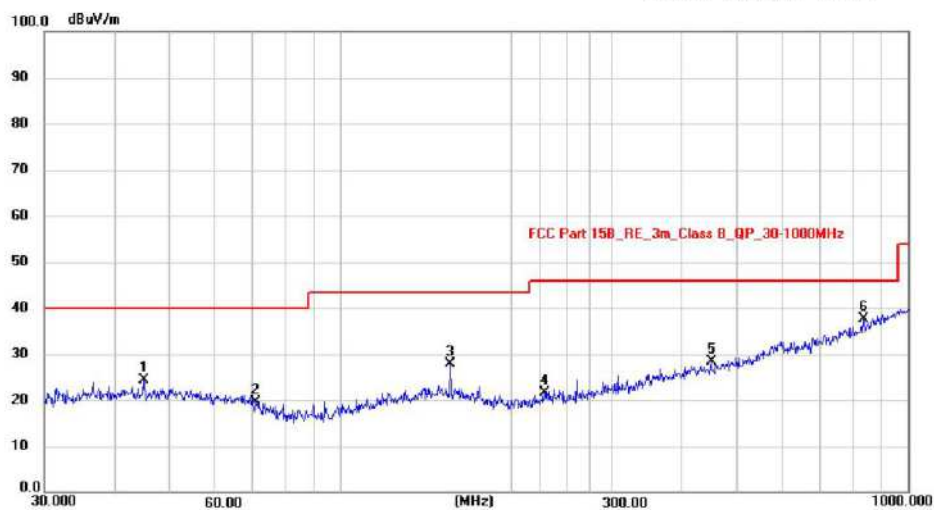

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 44.9006         | 10.14          | 14.36         | 24.50          | 40.00          | -15.50      | peak     | 100         | 258            | P   |        |
| 2   | 70.8315         | 7.88           | 11.87         | 19.75          | 40.00          | -20.25      | peak     | 100         | 311            | P   |        |
| 3   | 155.9101        | 13.56          | 14.26         | 27.82          | 43.50          | -15.68      | peak     | 100         | 268            | P   |        |
| 4   | 228.4902        | 9.30           | 12.43         | 21.73          | 46.00          | -24.27      | peak     | 100         | 169            | P   |        |
| 5   | 449.5557        | 9.33           | 18.93         | 28.26          | 46.00          | -17.74      | peak     | 100         | 55             | P   |        |
| 6 * | 833.3170        | 10.64          | 26.92         | 37.56          | 46.00          | -8.44       | peak     | 100         | 284            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:45:28

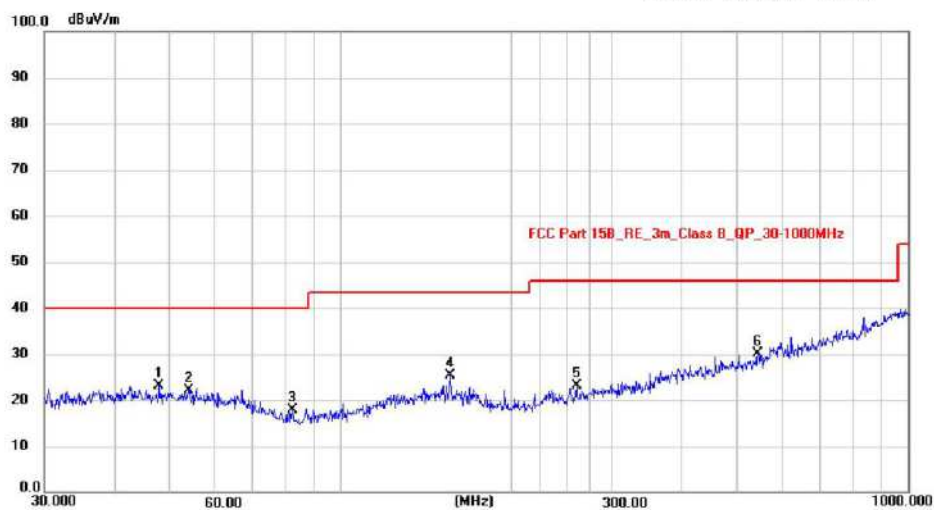

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 47.8260         | 8.98           | 14.24         | 23.22          | 40.00          | -16.78      | peak     | 100         | 148            | P   |        |
| 2   | 53.8817         | 8.37           | 13.74         | 22.11          | 40.00          | -17.89      | peak     | 100         | 251            | P   |        |
| 3   | 82.0704         | 8.26           | 9.51          | 17.77          | 40.00          | -22.23      | peak     | 100         | 121            | P   |        |
| 4   | 155.9101        | 11.13          | 14.26         | 25.39          | 43.50          | -18.11      | peak     | 100         | 357            | P   |        |
| 5   | 260.1444        | 9.44           | 13.61         | 23.05          | 46.00          | -22.95      | peak     | 100         | 65             | P   |        |
| 6 * | 543.2740        | 8.74           | 21.34         | 30.08          | 46.00          | -15.92      | peak     | 100         | 311            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:48:48

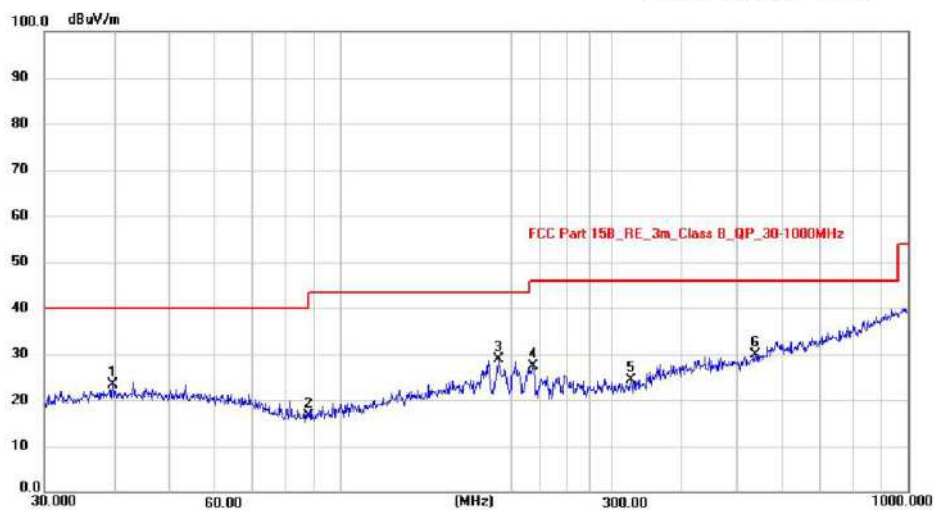

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 39.5756         | 8.90           | 14.51         | 23.41          | 40.00          | -16.59      | peak     | 200         | 255            | P   |        |
| 2   | 87.7245         | 6.98           | 9.66          | 16.64          | 40.00          | -23.36      | peak     | 200         | 202            | P   |        |
| 3 * | 189.7385        | 17.21          | 11.79         | 29.00          | 43.50          | -14.50      | peak     | 200         | 236            | P   |        |
| 4   | 218.3085        | 15.52          | 11.84         | 27.36          | 46.00          | -18.64      | peak     | 200         | 157            | P   |        |
| 5   | 324.4560        | 8.70           | 15.59         | 24.29          | 46.00          | -21.71      | peak     | 200         | 58             | P   |        |
| 6   | 537.5891        | 8.68           | 21.18         | 29.86          | 46.00          | -16.14      | peak     | 200         | 301            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2441MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:52:02



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 31.6201         | 8.10           | 13.27         | 21.37          | 40.00          | -18.63      | peak     | 200         | 354            | P   |        |
| 2   | 69.8450         | 8.63           | 12.10         | 20.73          | 40.00          | -19.27      | peak     | 200         | 248            | P   |        |
| 3   | 180.6488        | 14.97          | 12.36         | 27.33          | 43.50          | -16.17      | peak     | 200         | 157            | P   |        |
| 4   | 226.0994        | 13.02          | 12.29         | 25.31          | 46.00          | -20.69      | peak     | 200         | 169            | P   |        |
| 5   | 364.2595        | 12.17          | 16.72         | 28.89          | 46.00          | -17.11      | peak     | 200         | 249            | P   |        |
| 6 * | 642.8612        | 8.09           | 23.58         | 31.67          | 46.00          | -14.33      | peak     | 200         | 154            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2441MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:56:24

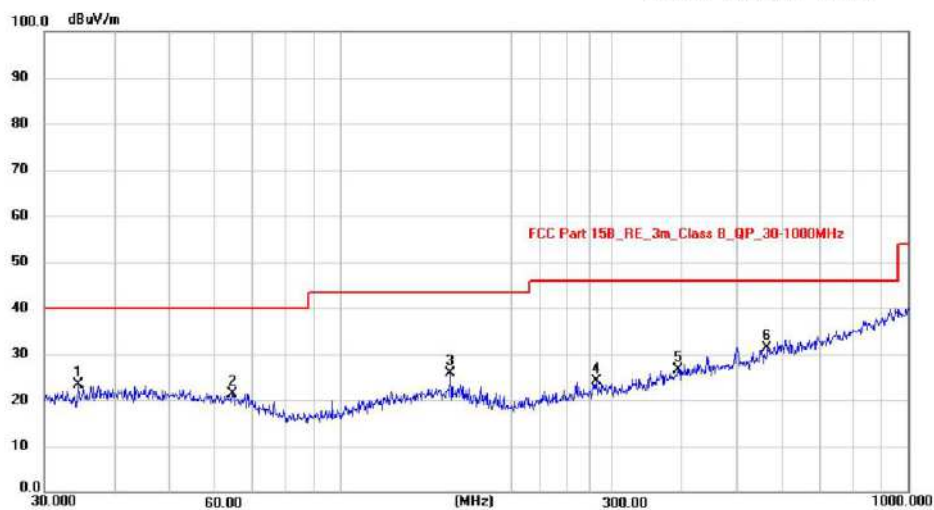

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 34.3964         | 9.64           | 13.73         | 23.37          | 40.00          | -16.63      | peak     | 100         | 148            | P   |        |
| 2   | 64.4330         | 8.68           | 12.66         | 21.34          | 40.00          | -18.66      | peak     | 100         | 206            | P   |        |
| 3   | 155.9101        | 11.74          | 14.26         | 26.00          | 43.50          | -17.50      | peak     | 100         | 355            | P   |        |
| 4   | 281.9945        | 9.51           | 14.58         | 24.09          | 46.00          | -21.91      | peak     | 100         | 21             | P   |        |
| 5   | 393.4723        | 9.06           | 17.54         | 26.60          | 46.00          | -19.40      | peak     | 100         | 241            | P   |        |
| 6 * | 564.6386        | 9.44           | 21.92         | 31.36          | 46.00          | -14.64      | peak     | 100         | 350            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 13:59:36

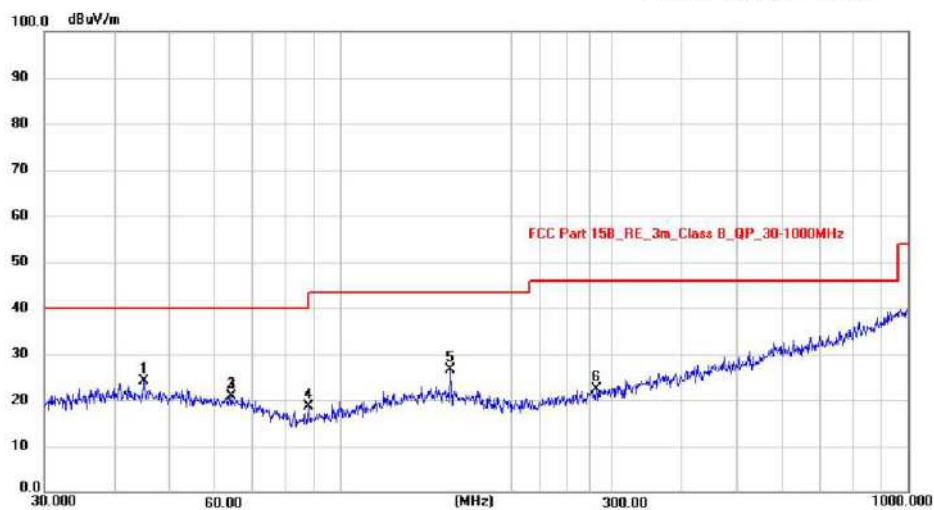

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 44.9006         | 9.86           | 14.36         | 24.22          | 40.00          | -15.78      | peak     | 100         | 148            | P   |        |
| 2   | 64.2074         | 8.12           | 12.68         | 20.80          | 40.00          | -19.20      | peak     | 100         | 255            | P   |        |
| 3   | 64.2074         | 8.12           | 12.68         | 20.80          | 40.00          | -19.20      | peak     | 100         | 308            | P   |        |
| 4   | 87.7245         | 8.92           | 9.66          | 18.58          | 40.00          | -21.42      | peak     | 100         | 96             | P   |        |
| 5   | 155.9101        | 12.33          | 14.26         | 26.59          | 43.50          | -16.91      | peak     | 100         | 217            | P   |        |
| 6   | 281.9945        | 7.88           | 14.58         | 22.46          | 46.00          | -23.54      | peak     | 100         | 195            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/14 14:05:58

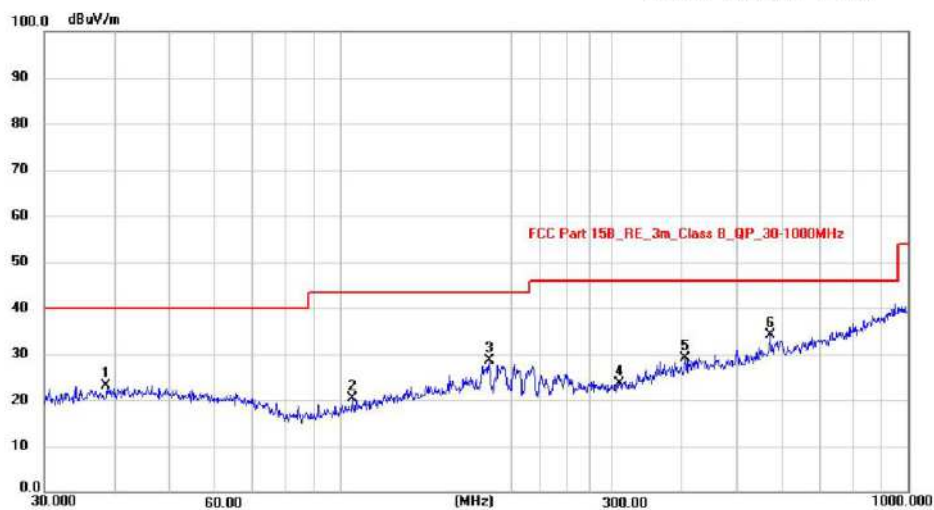

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 38.6160         | 8.68           | 14.37         | 23.05          | 40.00          | -16.95      | peak     | 200         | 144            | P   |        |
| 2   | 104.5360        | 9.25           | 11.04         | 20.29          | 43.50          | -23.21      | peak     | 200         | 65             | P   |        |
| 3   | 182.5592        | 16.34          | 12.24         | 28.58          | 43.50          | -14.92      | peak     | 200         | 124            | P   |        |
| 4   | 309.9977        | 8.56           | 15.18         | 23.74          | 46.00          | -22.26      | peak     | 200         | 305            | P   |        |
| 5   | 404.6664        | 11.33          | 17.84         | 29.17          | 46.00          | -16.83      | peak     | 200         | 228            | P   |        |
| 6 * | 572.6144        | 11.96          | 22.14         | 34.10          | 46.00          | -11.90      | peak     | 200         | 157            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit

1GHz - 18GHz



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber      Polarization: **Vertical**      Temperature: 26 °C  
EUT: ITE Hearing Aids      Distance: 3m      Humidity: 54 %RH  
M/N: Sara 1      Test Engineer: Felix Pang  
Test Mode: GFSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Radiated Emission Measurement

Test Date: 2024/10/16 13:04:34



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 5035.375        | 49.90          | -13.47        | 36.43          | 74.00          | -37.57      | peak     | 150         | 201            | P   |        |
| 2 * | 7154.000        | 45.63          | -7.91         | 37.72          | 74.00          | -36.28      | peak     | 150         | 134            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: GFSK 2402MHz           |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:08:04



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 4803.750        | 49.71          | -13.25        | 36.46          | 74.00          | -37.54      | peak     | 150         | 204            | P   |        |
| 2 * | 8091.125        | 44.73          | -7.08         | 37.65          | 74.00          | -36.35      | peak     | 150         | 185            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: GFSK 2441MHz           |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:12:48



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 6603.625        | 47.06          | -9.16         | 37.90          | 74.00          | -36.10      | peak     | 150         | 325            | P   |        |
| 2   | 8108.125        | 44.96          | -7.06         | 37.90          | 74.00          | -36.10      | peak     | 150         | 146            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: GFSK 2441MHz           |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:17:12



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 6695.000        | 46.70          | -8.90         | 37.80          | 74.00          | -36.20      | peak     | 150         | 257            | P   |        |
| 2 * | 8335.500        | 44.70          | -6.84         | 37.86          | 74.00          | -36.14      | peak     | 150         | 158            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: GFSK 2480MHz           |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:21:53



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 6612.125        | 47.15          | -9.14         | 38.01          | 74.00          | -35.99      | peak     | 150         | 354            | P   |        |
| 2   | 8273.875        | 44.38          | -6.90         | 37.48          | 74.00          | -36.52      | peak     | 150         | 214            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: GFSK 2480MHz           |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:25:31



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 7064.750        | 46.00          | -7.98         | 38.02          | 74.00          | -35.98      | peak     | 150         | 254            | P   |        |
| 2   | 7995.500        | 44.85          | -7.16         | 37.69          | 74.00          | -36.31      | peak     | 150         | 127            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:28:56



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 4869.625        | 49.01          | -13.02        | 35.99          | 74.00          | -38.01      | peak     | 150         | 325            | P   |        |
| 2 * | 7253.875        | 46.10          | -7.82         | 38.28          | 74.00          | -35.72      | peak     | 150         | 147            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: Pi/4DQPSK 2402MHz      |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:33:28



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 5768.500        | 47.88          | -11.49        | 36.39          | 74.00          | -37.61      | peak     | 150         | 235            | P   |        |
| 2 * | 7319.750        | 45.48          | -7.76         | 37.72          | 74.00          | -36.28      | peak     | 150         | 168            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: Pi/4DQPSK 2441MHz      |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:36:05



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 7066.875        | 45.57          | -7.98         | 37.59          | 74.00          | -36.41      | peak     | 150         | 324            | P   |        |
| 2   | 8361.000        | 44.20          | -6.82         | 37.38          | 74.00          | -36.62      | peak     | 150         | 154            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: Pi/4DQPSK 2441MHz      |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:39:35



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 5917.250        | 47.40          | -11.00        | 36.40          | 74.00          | -37.60      | peak     | 150         | 45             | P   |        |
| 2 * | 6852.250        | 46.55          | -8.46         | 38.09          | 74.00          | -35.91      | peak     | 150         | 168            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:43:17



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 6435.750        | 46.95          | -9.64         | 37.31          | 74.00          | -36.69      | peak     | 150         | 328            | P   |        |
| 2 * | 8027.375        | 45.24          | -7.13         | 38.11          | 74.00          | -35.89      | peak     | 150         | 124            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: Pi/4DQPSK 2480MHz      |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:47:41



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 6612.125        | 46.53          | -9.14         | 37.39          | 74.00          | -36.61      | peak     | 150         | 89             | P   |        |
| 2 * | 8263.250        | 44.51          | -6.90         | 37.61          | 74.00          | -36.39      | peak     | 150         | 157            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: 8DPSK 2402MHz          |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:51:24



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 5269.125        | 49.66          | -12.83        | 36.83          | 74.00          | -37.17      | peak     | 150         | 345            | P   |        |
| 2 * | 7003.125        | 46.32          | -8.04         | 38.28          | 74.00          | -35.72      | peak     | 150         | 128            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: 8DPSK 2402MHz          |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:54:55



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 7015.875        | 45.96          | -8.03         | 37.93          | 74.00          | -36.07      | peak     | 150         | 78             | P   |        |
| 2   | 8363.125        | 44.54          | -6.81         | 37.73          | 74.00          | -36.27      | peak     | 150         | 63             | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2441MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 13:59:01



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 4880.250        | 50.36          | -12.98        | 37.38          | 74.00          | -36.62      | peak     | 150         | 351            | P   |        |
| 2 * | 7030.750        | 46.36          | -8.02         | 38.34          | 74.00          | -35.66      | peak     | 150         | 153            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: 8DPSK 2441MHz          |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 14:04:26



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 5910.875        | 46.81          | -11.11        | 35.70          | 74.00          | -38.30      | peak     | 150         | 78             | P   |        |
| 2 * | 7334.625        | 45.49          | -7.75         | 37.74          | 74.00          | -36.26      | peak     | 150         | 146            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Vertical**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 14:09:15



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 7039.250        | 46.22          | -8.01         | 38.21          | 74.00          | -35.79      | peak     | 150         | 98             | P   |        |
| 2 * | 7970.000        | 46.30          | -7.18         | 39.12          | 74.00          | -34.88      | peak     | 150         | 187            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber      Polarization: **Horizontal**      Temperature: 26 °C  
 EUT: ITE Hearing Aids      Distance: 3m      Humidity: 54 %RH  
 M/N: Sara 1      Test Engineer: Felix Pang  
 Test Mode: 8DPSK 2480MHz  
 Test Voltage: DC 3.7V  
 Note:

Radiated Emission Measurement

Test Date: 2024/10/16 14:14:37



| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 8269.625        | 44.69          | -6.90         | 37.79          | 74.00          | -36.21      | peak     | 150         | 45             | P   |        |
| 2 * | 7239.000        | 45.86          | -7.84         | 38.02          | 74.00          | -35.98      | peak     | 150         | 258            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit

## Appendix A.8: Test Results of Radiated Emissions in Restricted Bands




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber      Polarization: **Horizontal**      Temperature: 26 °C  
EUT: ITE Hearing Aids      Distance: 3m      Humidity: 54 %RH  
M/N: Sara 1      Test Engineer: Felix Pang  
Test Mode: GFSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

### Radiated Emission Measurement

Test Date: 2024/10/16 15:22:04

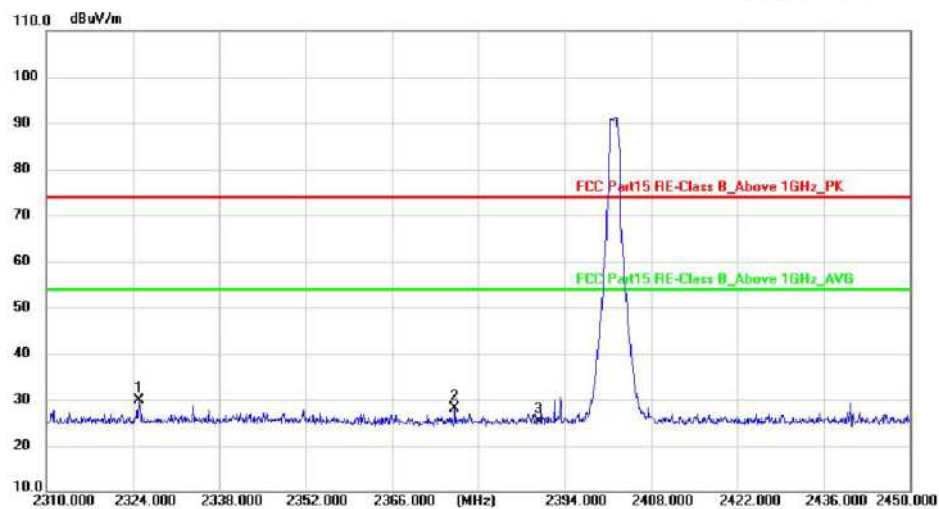

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2325.050        | 56.29          | -26.32        | 29.97          | 74.00          | -44.03      | peak     | 150         | 324            | P   |        |
| 2   | 2376.290        | 54.40          | -26.15        | 28.25          | 74.00          | -45.75      | peak     | 150         | 257            | P   |        |
| 3   | 2390.000        | 51.58          | -26.12        | 25.46          | 74.00          | -48.54      | peak     | 150         | 158            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: GFSK 2402MHz           |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:27:40

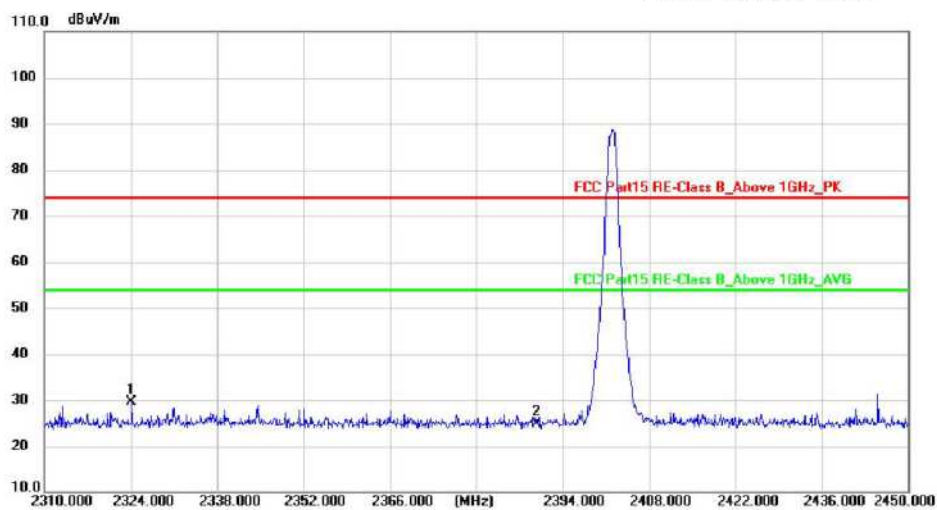

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2324.140        | 55.86          | -26.32        | 29.54          | 74.00          | -44.46      | peak     | 150         | 78             | P   |        |
| 2   | 2390.000        | 50.95          | -26.12        | 24.83          | 74.00          | -49.17      | peak     | 150         | 125            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: GFSK 2480MHz           |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:34:54

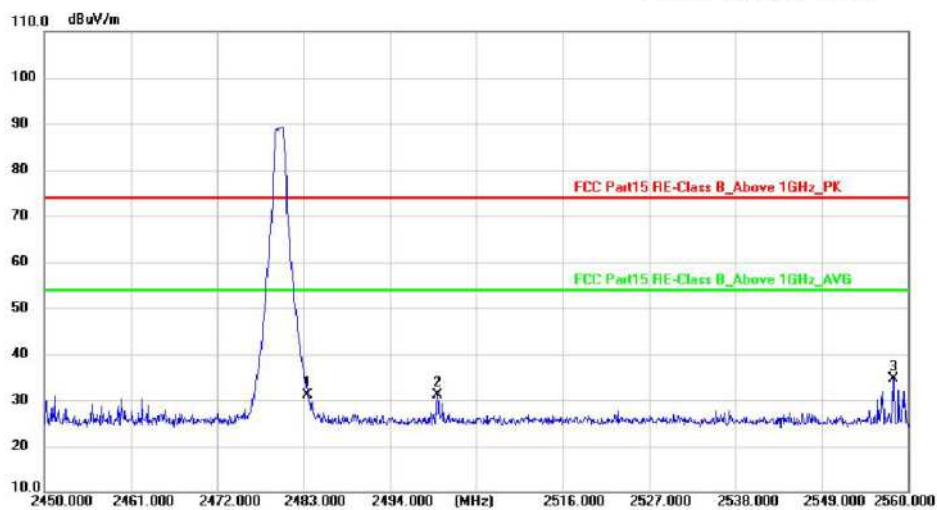

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 2483.500        | 56.85          | -25.84        | 31.01          | 74.00          | -42.99      | peak     | 150         | 254            | P   |        |
| 2   | 2500.133        | 56.95          | -25.78        | 31.17          | 74.00          | -42.83      | peak     | 150         | 156            | P   |        |
| 3 * | 2558.144        | 60.26          | -25.60        | 34.66          | 74.00          | -39.34      | peak     | 150         | 78             | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                                 |                    |
|-----------------------------------|---------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Horizontal</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                    | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang       |                    |
| Test Mode: GFSK 2480MHz           |                                 |                    |
| Test Voltage: DC 3.7V             |                                 |                    |
| Note:                             |                                 |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:38:05

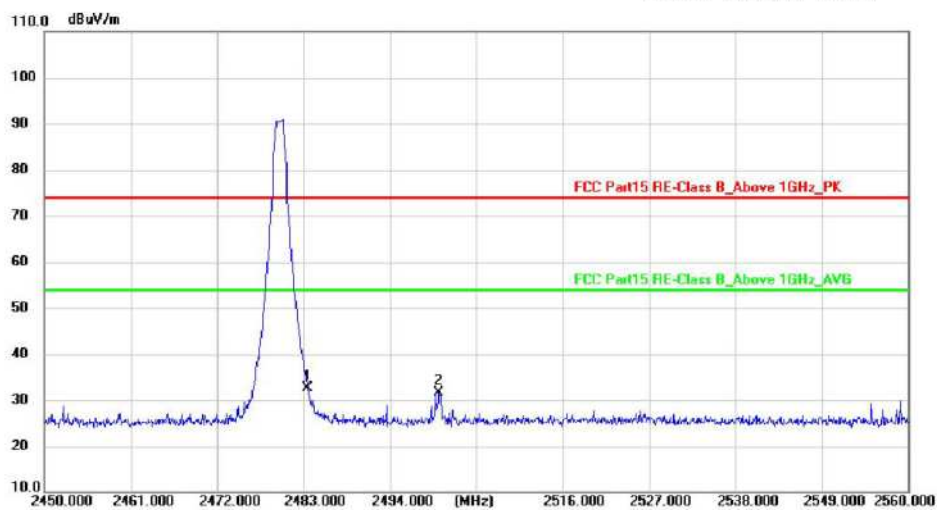

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2483.500        | 58.56          | -25.84        | 32.72          | 74.00          | -41.28      | peak     | 150         | 78             | P   |        |
| 2   | 2500.298        | 57.51          | -25.78        | 31.73          | 74.00          | -42.27      | peak     | 150         | 125            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:43:30

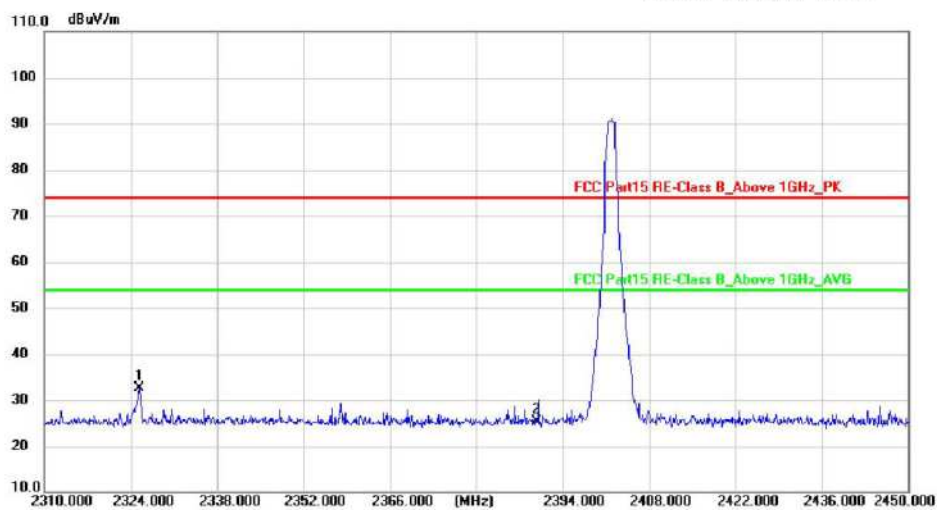

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2325.435        | 58.94          | -26.32        | 32.62          | 74.00          | -41.38      | peak     | 150         | 127            | P   |        |
| 2   | 2390.000        | 51.58          | -26.12        | 25.46          | 74.00          | -48.54      | peak     | 150         | 157            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber      Polarization: **Vertical**      Temperature: 26 °C  
 EUT: ITE Hearing Aids      Distance: 3m      Humidity: 54 %RH  
 M/N: Sara 1      Test Engineer: Felix Pang  
 Test Mode: Pi/4DQPSK 2402MHz  
 Test Voltage: DC 3.7V  
 Note:

Radiated Emission Measurement

Test Date: 2024/10/16 15:47:48

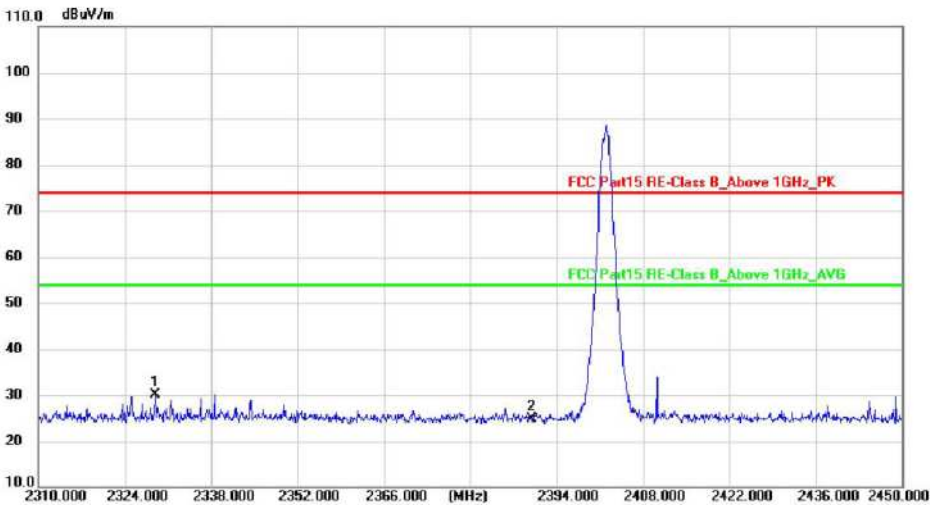

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2328.935        | 56.39          | -26.31        | 30.08          | 74.00          | -43.92      | peak     | 150         | 75             | P   |        |
| 2   | 2390.000        | 51.06          | -26.12        | 24.94          | 74.00          | -49.06      | peak     | 150         | 145            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
 1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
 Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber      Polarization: **Vertical**      Temperature: 26 °C  
 EUT: ITE Hearing Aids      Distance: 3m      Humidity: 54 %RH  
 M/N: Sara 1      Test Engineer: Felix Pang  
 Test Mode: Pi/4DQPSK 2480MHz  
 Test Voltage: DC 3.7V  
 Note:

Radiated Emission Measurement

Test Date: 2024/10/16 15:49:56

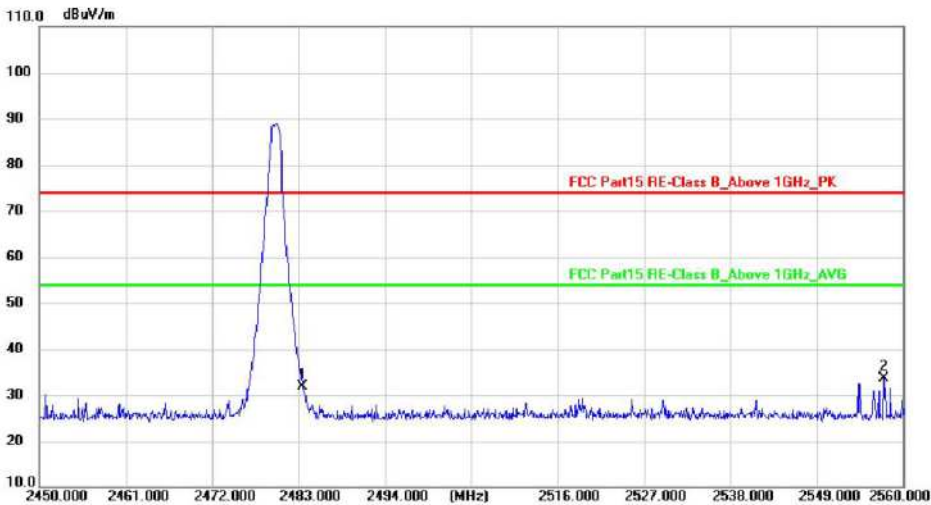

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 2483.500        | 57.70          | -25.84        | 31.86          | 74.00          | -42.14      | peak     | 150         | 325            | P   |        |
| 2 * | 2557.608        | 59.34          | -25.60        | 33.74          | 74.00          | -40.26      | peak     | 150         | 127            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: Pi/4DQPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:53:40

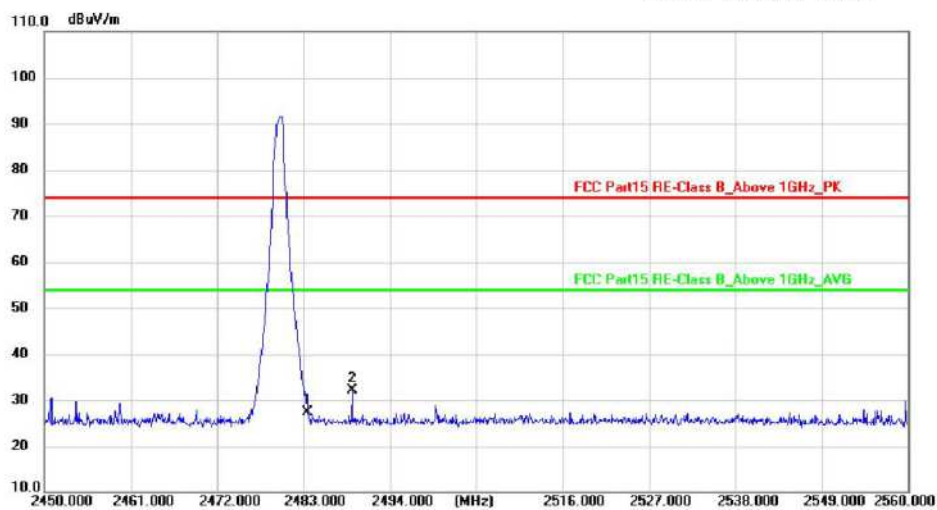

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 2483.500        | 53.16          | -25.84        | 27.32          | 74.00          | -46.68      | peak     | 150         | 124            | P   |        |
| 2 * | 2489.229        | 58.04          | -25.81        | 32.23          | 74.00          | -41.77      | peak     | 150         | 257            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2402MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 15:58:44

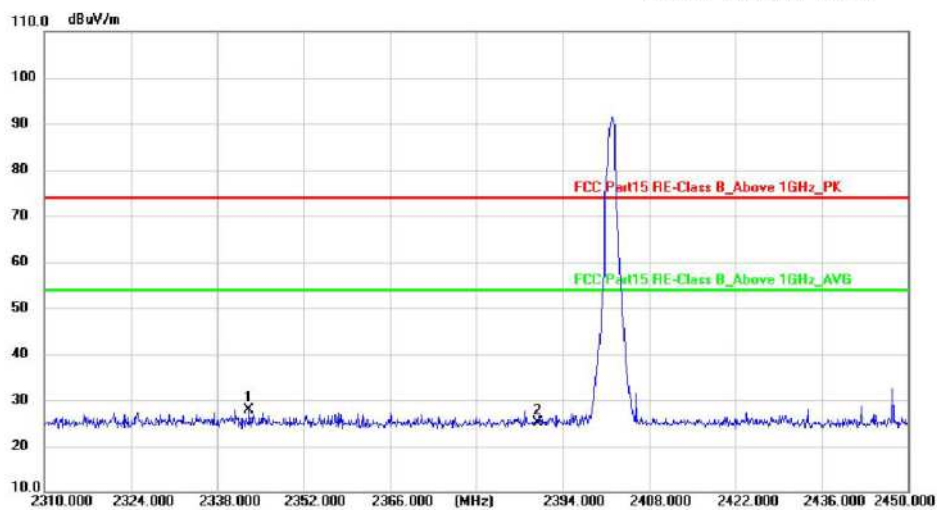

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2343.285        | 54.08          | -26.25        | 27.83          | 74.00          | -46.17      | peak     | 150         | 325            | P   |        |
| 2   | 2390.000        | 51.30          | -26.12        | 25.18          | 74.00          | -48.82      | peak     | 150         | 157            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: 8DPSK 2402MHz          |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 16:02:52

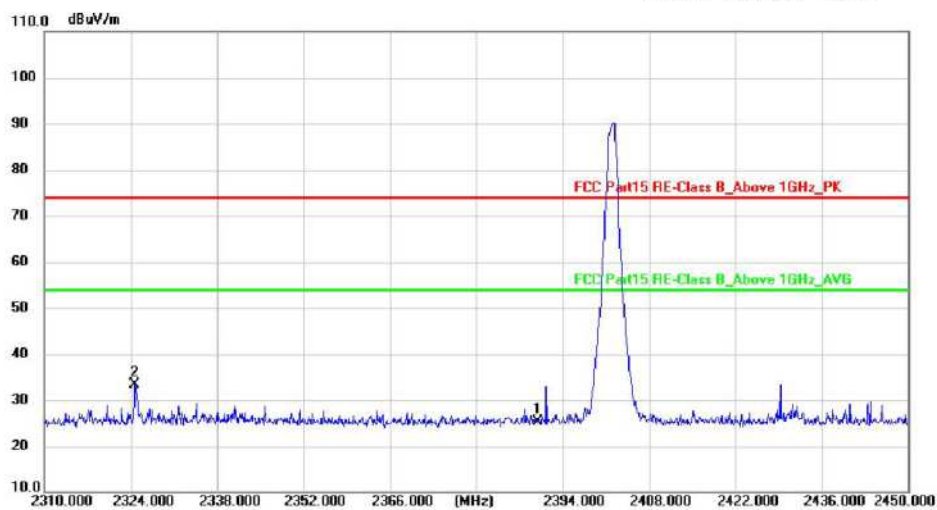

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 2390.000        | 51.42          | -26.12        | 25.30          | 74.00          | -48.70      | peak     | 150         | 257            | P   |        |
| 2 * | 2324.770        | 59.69          | -26.32        | 33.37          | 74.00          | -40.63      | peak     | 150         | 214            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

|                                   |                               |                    |
|-----------------------------------|-------------------------------|--------------------|
| Test Site: PSI EMC Lab-3m Chamber | Polarization: <b>Vertical</b> | Temperature: 26 °C |
| EUT: ITE Hearing Aids             | Distance: 3m                  | Humidity: 54 %RH   |
| M/N: Sara 1                       | Test Engineer: Felix Pang     |                    |
| Test Mode: 8DPSK 2480MHz          |                               |                    |
| Test Voltage: DC 3.7V             |                               |                    |
| Note:                             |                               |                    |

#### Radiated Emission Measurement

Test Date: 2024/10/16 16:05:56

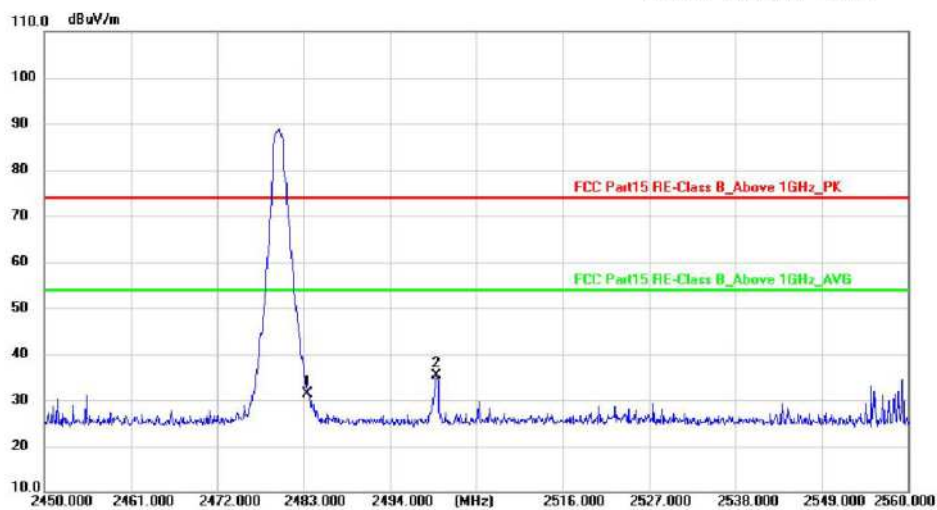

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1   | 2483.500        | 57.26          | -25.84        | 31.42          | 74.00          | -42.58      | peak     | 150         | 324            | P   |        |
| 2 * | 2499.954        | 61.07          | -25.78        | 35.29          | 74.00          | -38.71      | peak     | 150         | 127            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit



Shenzhen PSI Testing Co., Ltd.  
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,  
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber  
EUT: ITE Hearing Aids  
M/N: Sara 1  
Test Mode: 8DPSK 2480MHz  
Test Voltage: DC 3.7V  
Note:

Polarization: **Horizontal**  
Distance: 3m  
Test Engineer: Felix Pang

Temperature: 26 °C  
Humidity: 54 %RH

#### Radiated Emission Measurement

Test Date: 2024/10/16 16:09:41

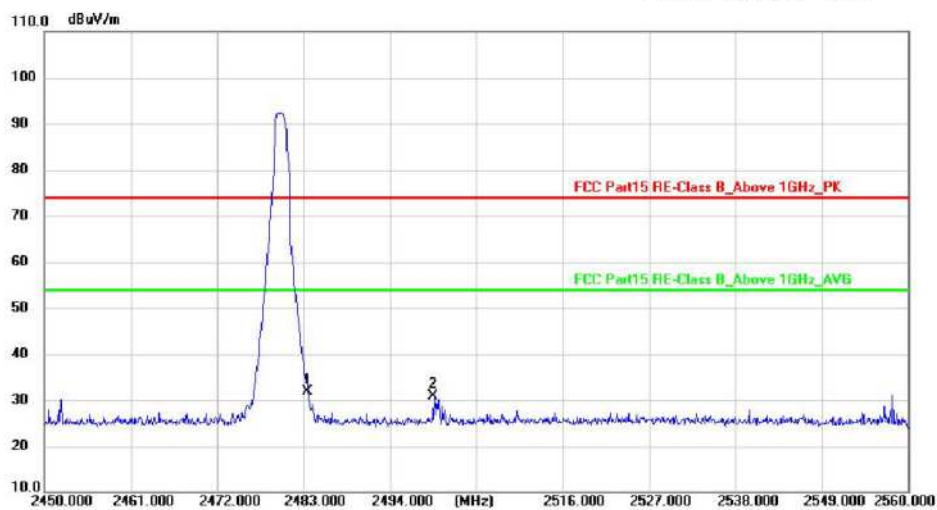

| No. | Frequency (MHz) | Reading (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Detector | Height (cm) | Azimuth (deg.) | P/F | Remark |
|-----|-----------------|----------------|---------------|----------------|----------------|-------------|----------|-------------|----------------|-----|--------|
| 1 * | 2483.500        | 57.80          | -25.84        | 31.96          | 74.00          | -42.04      | peak     | 150         | 124            | P   |        |
| 2   | 2499.706        | 56.71          | -25.78        | 30.93          | 74.00          | -43.07      | peak     | 150         | 185            | P   |        |

Note: \*:Maximum data    x:Over limit    !:over margin    Level = Reading + Factor    Margin = Level - Limit