

System Performance Check-900MHz

Communication System: UID 0, CW (0); Communication System Band: D900 (900.0 MHz);

Frequency: 900 MHz;

Medium parameters used: $f = 900$ MHz; $\sigma = 0.937$ S/m; $\epsilon_r = 42.062$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN7383; ConvF(10.05, 10.05, 10.05); Calibrated: 2023/6/5;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection), $z = -19.0, 31.0$
- Electronics: DAE3 Sn427; Calibrated: 2023/5/17
- Phantom: SAM; Type: QD000P40CD; Serial: 1805
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Configuration/Body/Area Scan (5x12x1): Measurement grid: $dx=15$ mm, $dy=15$ mm

Maximum value of SAR (measured) = 3.66 W/kg

Configuration/Body/Zoom Scan (5x5x5mm, graded), dist=1.4mm (5x6x5)/Cube 0:


Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm

Reference Value = 56.43 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 4.48 W/kg

SAR(1 g) = 2.65 W/kg; SAR(10 g) = 1.72 W/kg

Maximum value of SAR (measured) = 3.68 W/kg

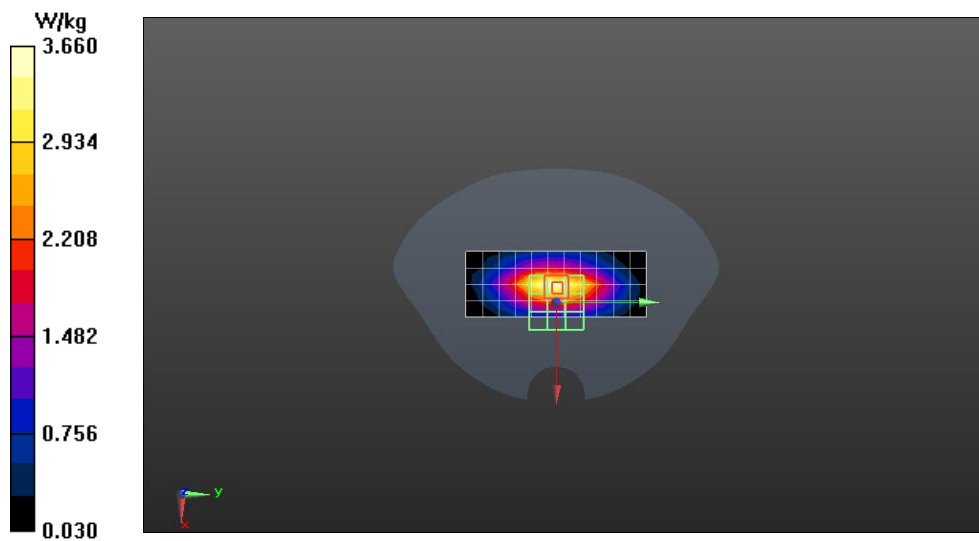

System Performance Check-2450MHz

Communication System: UID 0, CW (0); Communication System Band: D2450 (2450.0 MHz);

Frequency: 2450 MHz;

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.829$ S/m; $\epsilon_r = 39.919$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN7383; ConvF(7.85, 7.85, 7.85); Calibrated: 2023/6/5;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection), $z = 1.0, 31.0$
- Electronics: DAE3 Sn427; Calibrated: 2023/5/17
- Phantom: SAM; Type: QD000P40CD; Serial: 1805
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Configuration/Body/Area Scan (7x9x1): Measurement grid: $dx=12$ mm, $dy=12$ mm

Maximum value of SAR (measured) = 21.8 W/kg

Configuration/Body/Zoom Scan (7x7x4)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 114.6 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.2 W/kg

SAR(1 g) = 12.7 W/kg; SAR(10 g) = 5.94 W/kg

Maximum value of SAR (measured) = 21.6 W/kg

