

Appendix A

System Validation Plots

Table of Contents

1. D2450V2-SN: 904 Validation Plot 3

2. D5GV2-SN: 1148 Validation Plot..... 4

1. D2450V2-SN: 904 Validation Plot

Date: 03.08.2026

Test Laboratory: Guangdong Dongdian Testing Service Co., Ltd.

2450

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN:904


Communication System: UID 0, CW (0); Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Communication System PAR: 0 dB; PMF: 1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.78$ S/m; $\epsilon_r = 38.493$; $\rho = 1000$ kg/m³
Phantom section: Flat Section
Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2011)

DASY Configuration:

- Probe: EX3DV4 - SN3906; ConvF(7.91, 7.91, 7.91) @ 2450 MHz; Calibrated: 22.06.2026
- Sensor-Surface: 3mm (Mechanical Surface Detection), Sensor-Surface: 4mm (Mechanical Surface Detection), $z = 1.0, 31.0$
- Electronics: DAE4 Sn1366; Calibrated: 22.06.2026
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1197
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Configuration/tilt/Area Scan (6x11x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
Maximum value of SAR (measured) = 5.85 W/kg

Configuration/tilt/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 52.77 V/m; Power Drift = 0.15 dB
Peak SAR (extrapolated) = 9.86 W/kg
SAR(1 g) = 5.04 W/kg; SAR(10 g) = 2.47 W/kg
Smallest distance from peaks to all points 3 dB below = 10.4 mm
Ratio of SAR at M2 to SAR at M1 = 53.2%
Maximum value of SAR (measured) = 5.76 W/kg

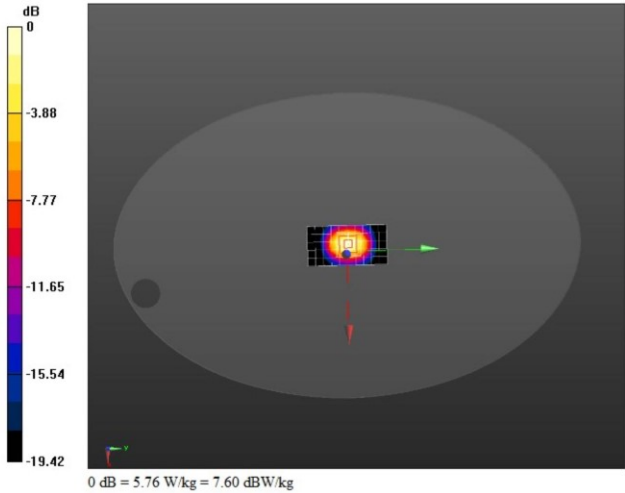

2. D5GV2-SN: 1148 Validation Plot

Date: 04.08.2026

Test Laboratory: Guangdong Dongdian Testing Service Co., Ltd.

5G

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1148

Communication System: UID 0, CW (0); Communication System Band: D5GHz (5000.0 - 6000.0 MHz); Frequency: 5800 MHz; Communication System PAR: 0 dB; PMF: 1

Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.1 \text{ S/m}$; $\epsilon_r = 35.166$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2011)

DASY Configuration:

- Probe: EX3DV4 - SN3906; ConvF(4.97, 4.97, 4.97) @ 5800 MHz; Calibrated: 22.06.2026
- Sensor-Surface: 3mm (Mechanical Surface Detection), Sensor-Surface: 1.4mm (Mechanical Surface Detection), $z = 1.0, 25.0$
- Electronics: DAE4 Sn1366; Calibrated: 22.06.2026
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1197
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Configuration/5800/Area Scan (6x11x1): Measurement grid: $dx=10\text{mm}$, $dy=10\text{mm}$

Maximum value of SAR (measured) = 9.10 W/kg

Configuration/5800/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=1.4\text{mm}$

Reference Value = 39.06 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 34.5 W/kg

SAR(1 g) = 7.66 W/kg; SAR(10 g) = 2.23 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 61.2%

Maximum value of SAR (measured) = 19.7 W/kg

