


Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2402MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

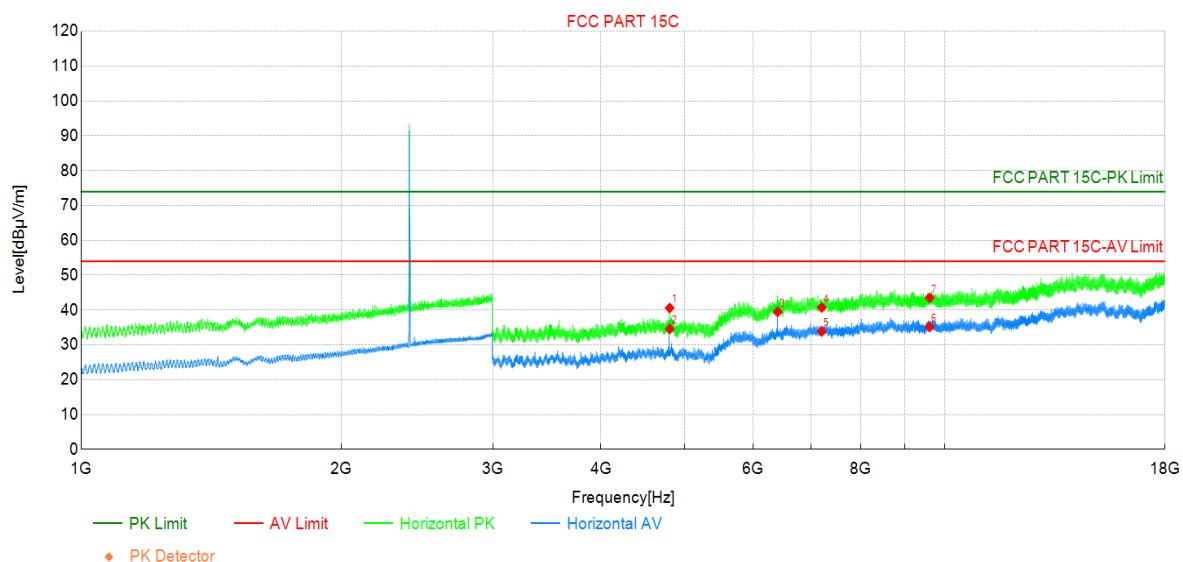

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	46.63	40.60	-6.03	74.00	33.40	PK	Horizo	PASS
2	4804.00	40.59	34.56	-6.03	54.00	19.44	AV	Horizo	PASS
3	6405.75	38.05	39.48	1.43	54.00	14.52	AV	Horizo	PASS
4	7206.00	37.77	40.74	2.97	74.00	33.26	PK	Horizo	PASS
5	7206.00	30.89	33.86	2.97	54.00	20.14	AV	Horizo	PASS
6	9608.00	29.22	35.16	5.94	54.00	18.84	AV	Horizo	PASS
7	9608.00	37.56	43.50	5.94	74.00	30.50	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2402MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

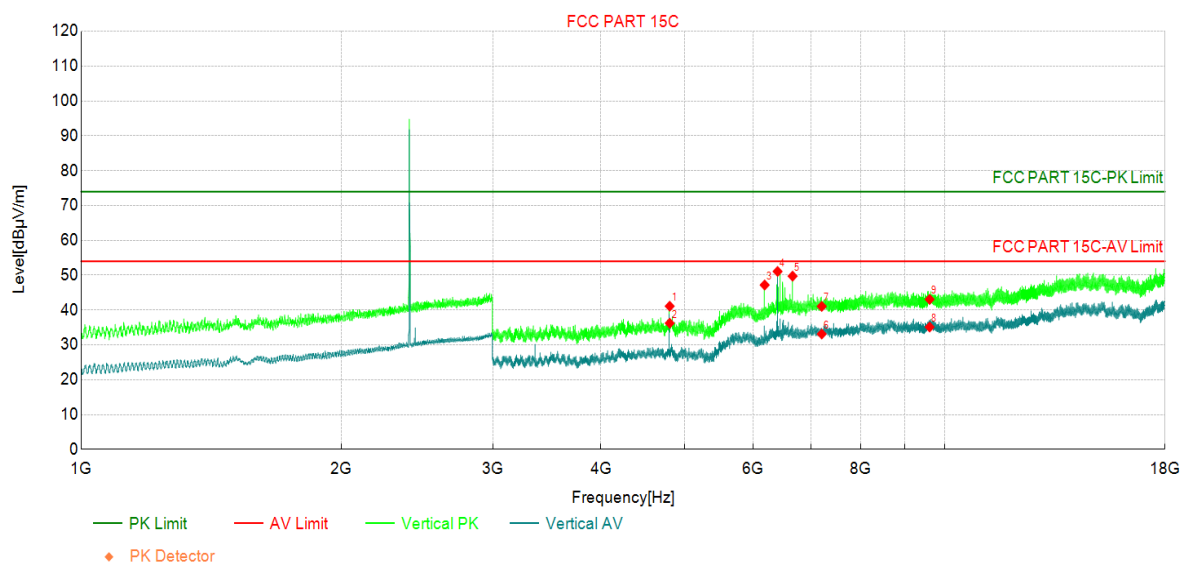

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	47.13	41.10	-6.03	74.00	32.90	PK	Vertic	PASS
2	4804.00	42.26	36.23	-6.03	54.00	17.77	AV	Vertic	PASS
3	6189.00	47.76	47.18	-0.58	74.00	26.82	PK	Vertic	PASS
4	6405.38	49.64	51.07	1.43	74.00	22.93	PK	Vertic	PASS
5	6667.13	48.01	49.73	1.72	74.00	24.27	PK	Vertic	PASS
6	7206.00	30.14	33.11	2.97	54.00	20.89	AV	Vertic	PASS
7	7206.00	38.08	41.05	2.97	74.00	32.95	PK	Vertic	PASS
8	9608.00	29.17	35.11	5.94	54.00	18.89	AV	Vertic	PASS
9	9608.00	37.12	43.06	5.94	74.00	30.94	PK	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2440MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

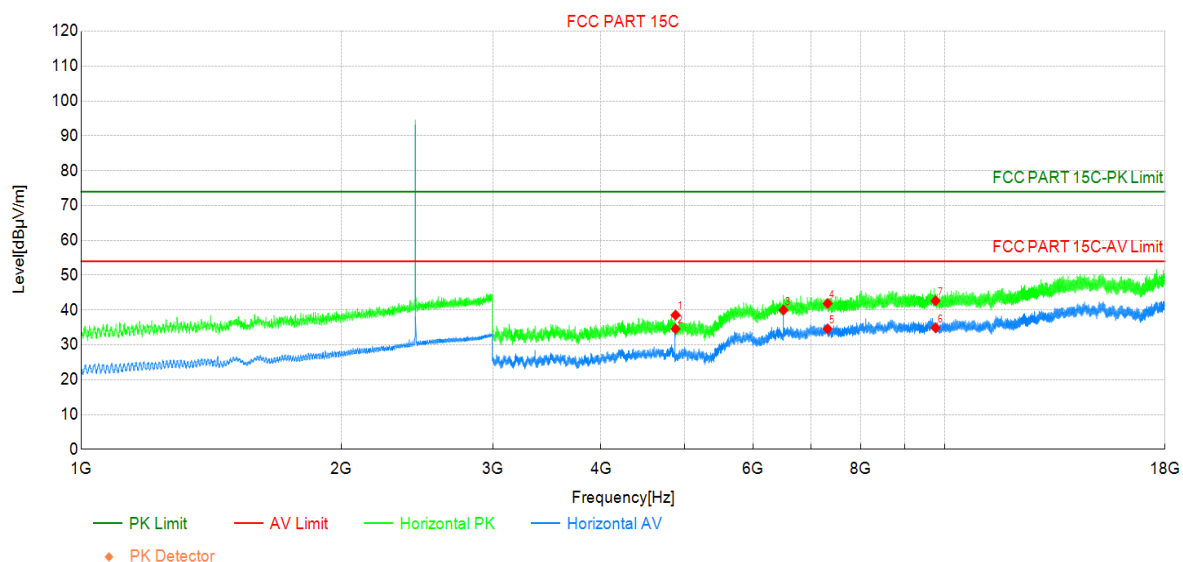

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	44.63	38.55	-6.08	74.00	35.45	PK	Horizo	PASS
2	4880.00	40.67	34.59	-6.08	54.00	19.41	AV	Horizo	PASS
3	6507.00	38.29	39.98	1.69	54.00	14.02	AV	Horizo	PASS
4	7320.00	39.07	41.87	2.80	74.00	32.13	PK	Horizo	PASS
5	7320.00	31.78	34.58	2.80	54.00	19.42	AV	Horizo	PASS
6	9760.00	28.77	34.90	6.13	54.00	19.10	AV	Horizo	PASS
7	9760.00	36.51	42.64	6.13	74.00	31.36	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2440MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C ; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

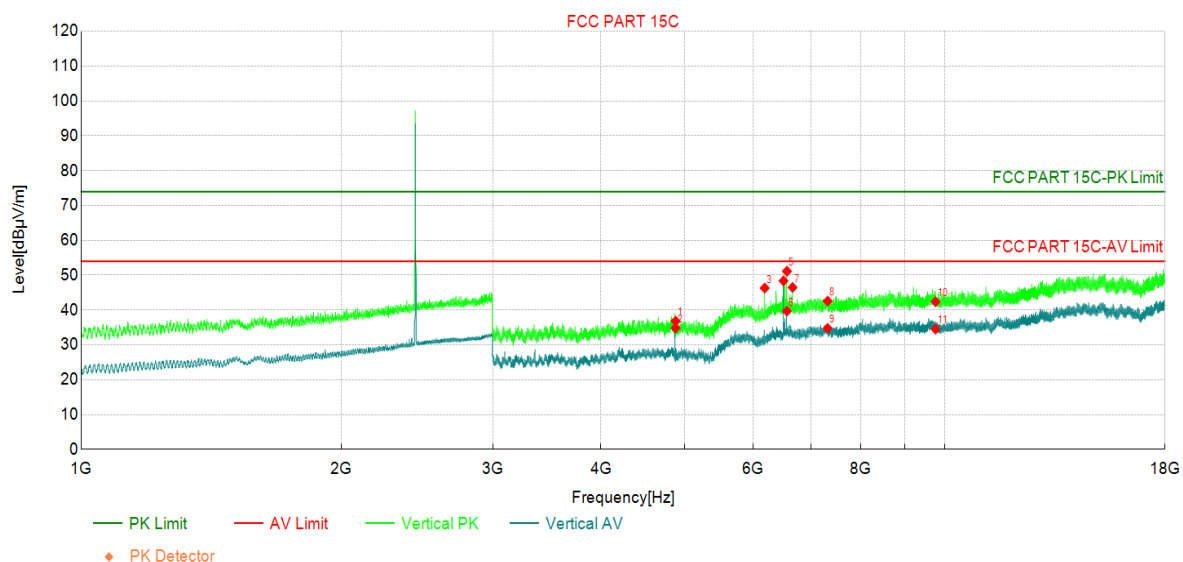

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	42.89	36.81	-6.08	74.00	37.19	PK	Vertic	PASS
2	4880.00	40.90	34.82	-6.08	54.00	19.18	AV	Vertic	PASS
3	6189.38	46.88	46.30	-0.58	74.00	27.70	PK	Vertic	PASS
4	6507.00	46.69	48.38	1.69	54.00	5.62	AV	Vertic	PASS
5	6566.25	49.09	51.14	2.05	74.00	22.86	PK	Vertic	PASS
6	6566.63	37.63	39.68	2.05	54.00	14.32	AV	Vertic	PASS
7	6666.38	44.76	46.49	1.73	74.00	27.51	PK	Vertic	PASS
8	7320.00	39.77	42.57	2.80	74.00	31.43	PK	Vertic	PASS
9	7320.00	31.96	34.76	2.80	54.00	19.24	AV	Vertic	PASS
10	9760.00	36.25	42.38	6.13	74.00	31.62	PK	Vertic	PASS
11	9760.00	28.40	34.53	6.13	54.00	19.47	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2480MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C ; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

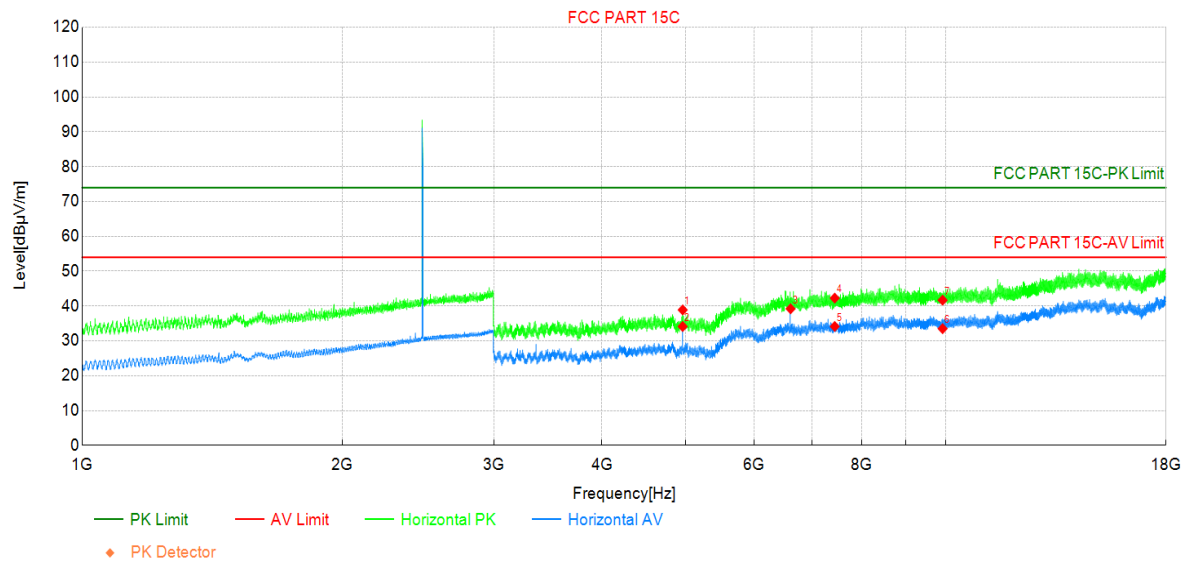

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	44.15	38.88	-5.27	74.00	35.12	PK	Horizo	PASS
2	4960.00	39.39	34.12	-5.27	54.00	19.88	AV	Horizo	PASS
3	6613.50	37.04	39.20	2.16	54.00	14.80	AV	Horizo	PASS
4	7440.00	39.72	42.28	2.56	74.00	31.72	PK	Horizo	PASS
5	7440.00	31.57	34.13	2.56	54.00	19.87	AV	Horizo	PASS
6	9920.00	27.89	33.51	5.62	54.00	20.49	AV	Horizo	PASS
7	9920.00	36.06	41.68	5.62	74.00	32.32	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2480MHz by LE2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C ; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

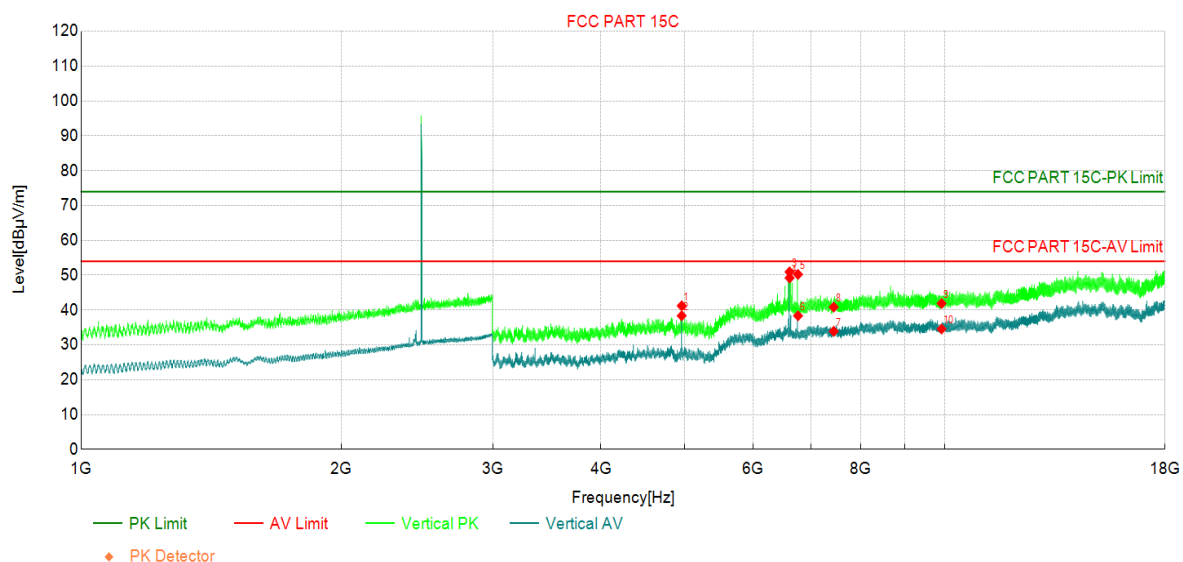

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	46.48	41.21	-5.27	74.00	32.79	PK	Vertic	PASS
2	4960.00	43.62	38.35	-5.27	54.00	15.65	AV	Vertic	PASS
3	6613.50	48.79	50.95	2.16	74.00	23.05	PK	Vertic	PASS
4	6613.88	47.05	49.20	2.15	54.00	4.80	AV	Vertic	PASS
5	6764.25	48.37	50.23	1.86	74.00	23.77	PK	Vertic	PASS
6	6764.63	36.49	38.35	1.86	54.00	15.65	AV	Vertic	PASS
7	7440.00	31.34	33.90	2.56	54.00	20.10	AV	Vertic	PASS
8	7440.00	38.28	40.84	2.56	74.00	33.16	PK	Vertic	PASS
9	9920.00	36.26	41.88	5.62	74.00	32.12	PK	Vertic	PASS
10	9920.00	28.94	34.56	5.62	54.00	19.44	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2402MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

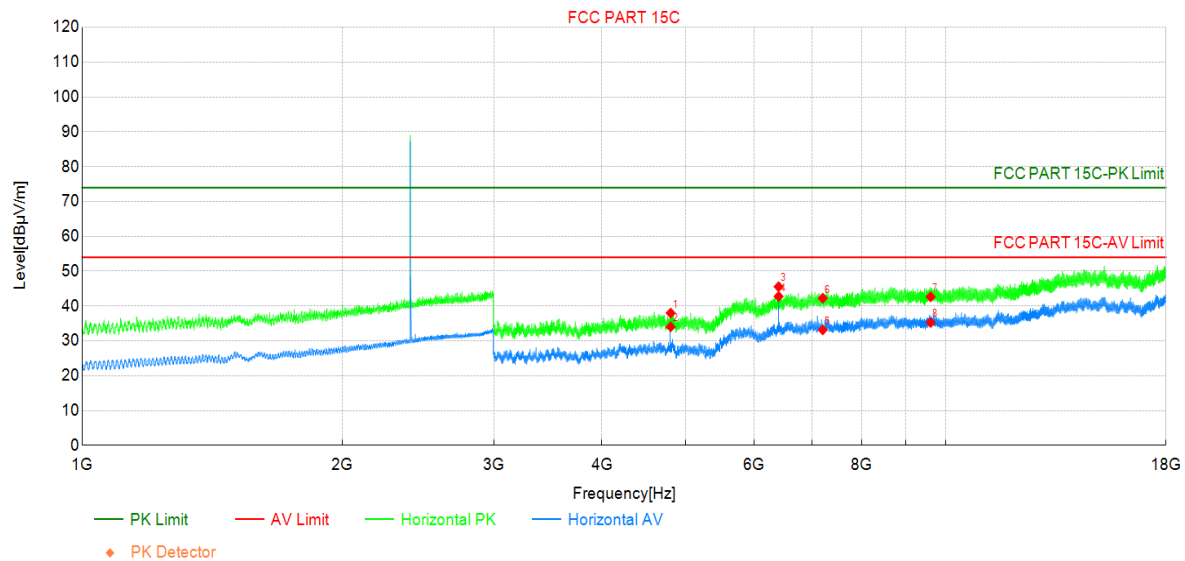

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	44.00	37.97	-6.03	74.00	36.03	PK	Horizo	PASS
2	4804.00	40.06	34.03	-6.03	54.00	19.97	AV	Horizo	PASS
3	6405.38	44.12	45.55	1.43	74.00	28.45	PK	Horizo	PASS
4	6405.75	41.31	42.74	1.43	54.00	11.26	AV	Horizo	PASS
5	7206.00	30.17	33.14	2.97	54.00	20.86	AV	Horizo	PASS
6	7206.00	39.28	42.25	2.97	74.00	31.75	PK	Horizo	PASS
7	9608.00	36.70	42.64	5.94	74.00	31.36	PK	Horizo	PASS
8	9608.00	29.32	35.26	5.94	54.00	18.74	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2402MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

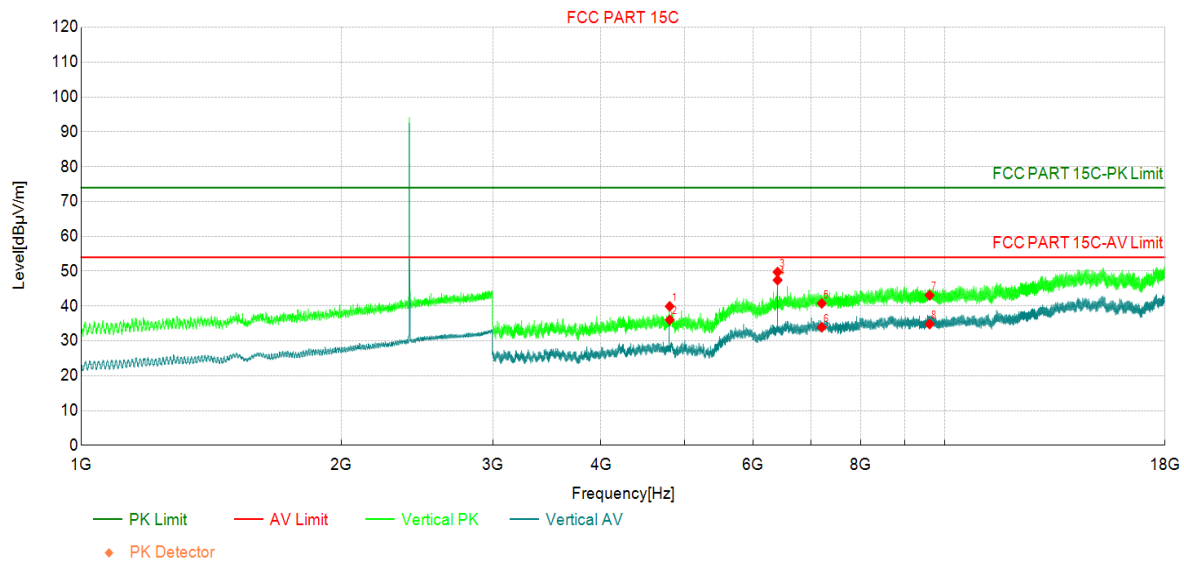

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	45.93	39.90	-6.03	74.00	34.10	PK	Vertic	PASS
2	4804.00	42.05	36.02	-6.03	54.00	17.98	AV	Vertic	PASS
3	6405.38	48.31	49.74	1.43	74.00	24.26	PK	Vertic	PASS
4	6405.75	46.01	47.44	1.43	54.00	6.56	AV	Vertic	PASS
5	7206.00	37.78	40.75	2.97	74.00	33.25	PK	Vertic	PASS
6	7206.00	30.95	33.92	2.97	54.00	20.08	AV	Vertic	PASS
7	9608.00	37.13	43.07	5.94	74.00	30.93	PK	Vertic	PASS
8	9608.00	28.87	34.81	5.94	54.00	19.19	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2440MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Enginee	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

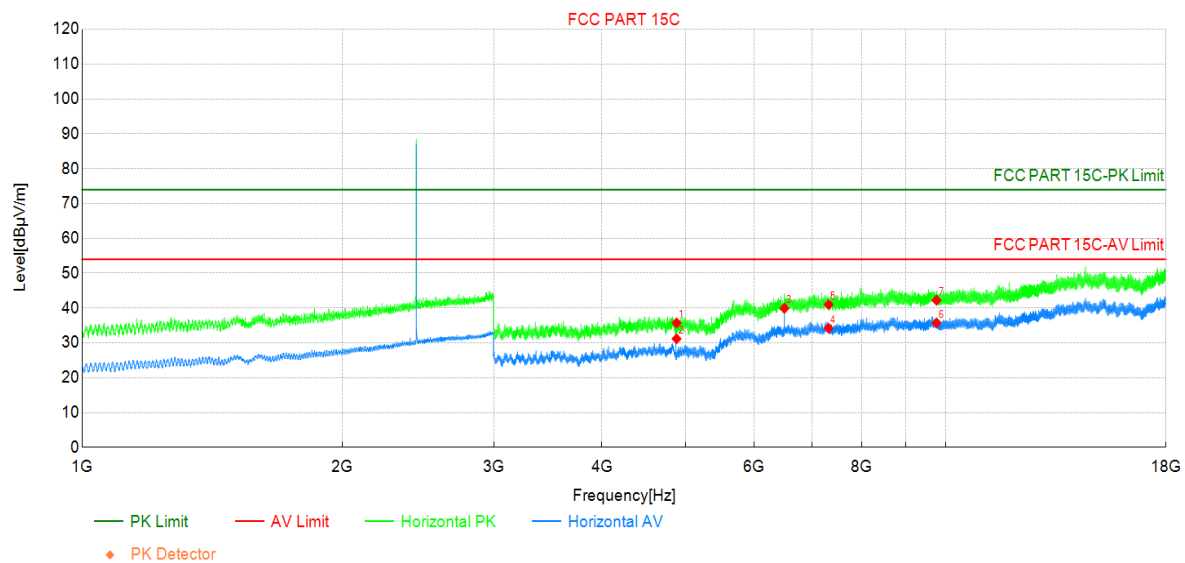

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	41.82	35.74	-6.08	74.00	38.26	PK	Horizo	PASS
2	4880.00	37.25	31.17	-6.08	54.00	22.83	AV	Horizo	PASS
3	6507.00	38.24	39.93	1.69	54.00	14.07	AV	Horizo	PASS
4	7320.00	31.41	34.21	2.80	54.00	19.79	AV	Horizo	PASS
5	7320.00	38.20	41.00	2.80	74.00	33.00	PK	Horizo	PASS
6	9760.00	29.59	35.72	6.13	54.00	18.28	AV	Horizo	PASS
7	9760.00	36.10	42.23	6.13	74.00	31.77	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2440MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

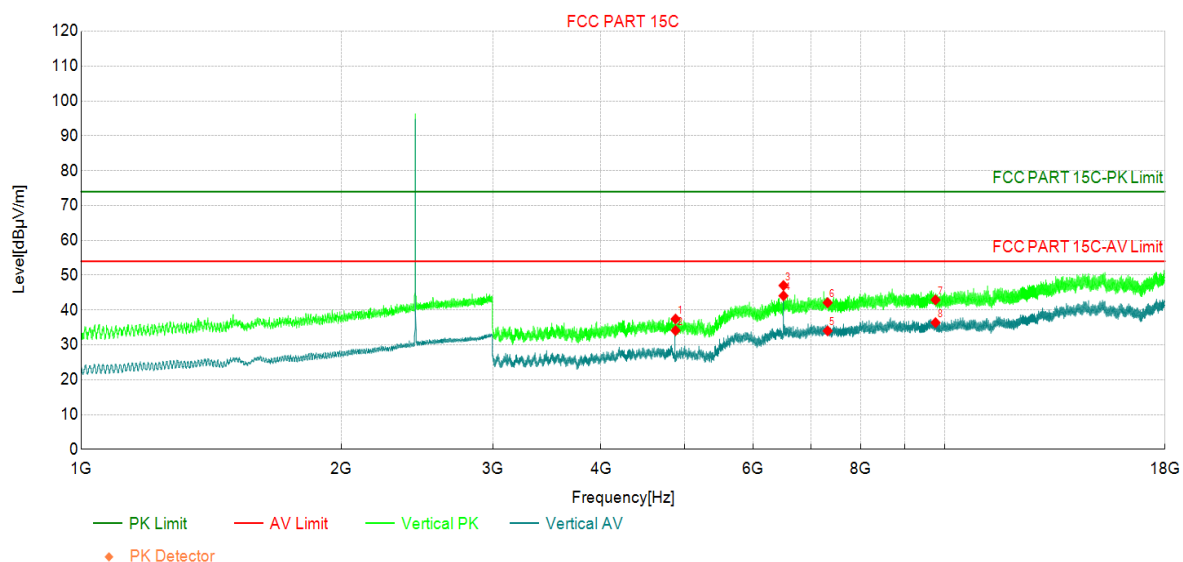

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	43.50	37.42	-6.08	74.00	36.58	PK	Vertic	PASS
2	4880.00	40.20	34.12	-6.08	54.00	19.88	AV	Vertic	PASS
3	6506.63	45.34	47.03	1.69	74.00	26.97	PK	Vertic	PASS
4	6507.00	42.39	44.08	1.69	54.00	9.92	AV	Vertic	PASS
5	7320.00	31.21	34.01	2.80	54.00	19.99	AV	Vertic	PASS
6	7320.00	39.32	42.12	2.80	74.00	31.88	PK	Vertic	PASS
7	9760.00	36.78	42.91	6.13	74.00	31.09	PK	Vertic	PASS
8	9760.00	30.25	36.38	6.13	54.00	17.62	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2480MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

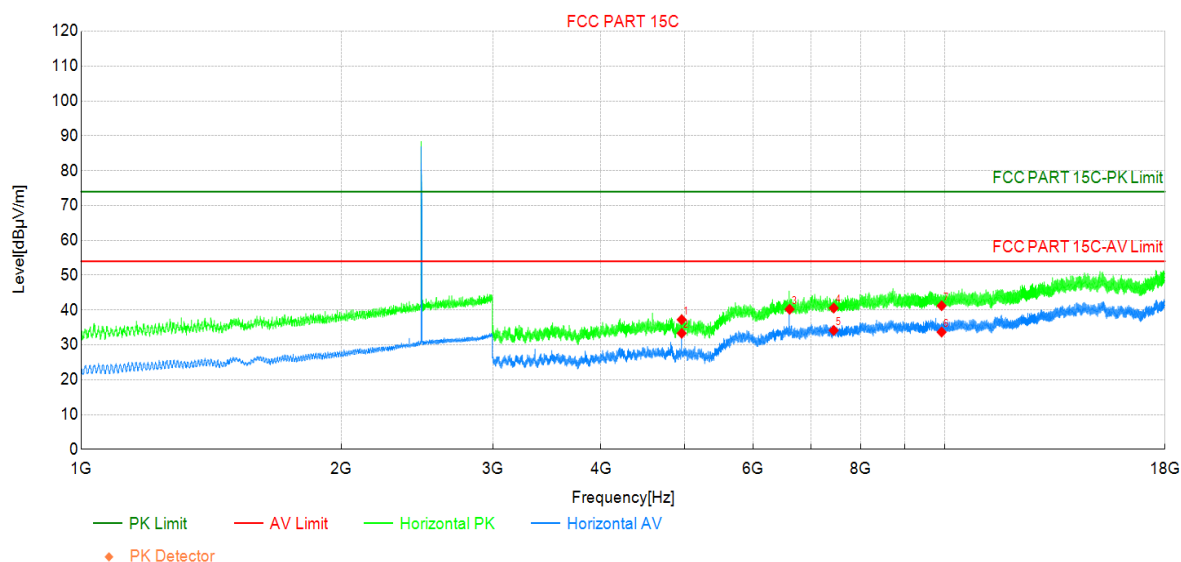

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	42.50	37.23	-5.27	74.00	36.77	PK	Horizo	PASS
2	4960.00	38.59	33.32	-5.27	54.00	20.68	AV	Horizo	PASS
3	6613.88	38.06	40.21	2.15	54.00	13.79	AV	Horizo	PASS
4	7440.00	38.00	40.56	2.56	74.00	33.44	PK	Horizo	PASS
5	7440.00	31.59	34.15	2.56	54.00	19.85	AV	Horizo	PASS
6	9920.00	28.05	33.67	5.62	54.00	20.33	AV	Horizo	PASS
7	9920.00	35.61	41.23	5.62	74.00	32.77	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2480MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

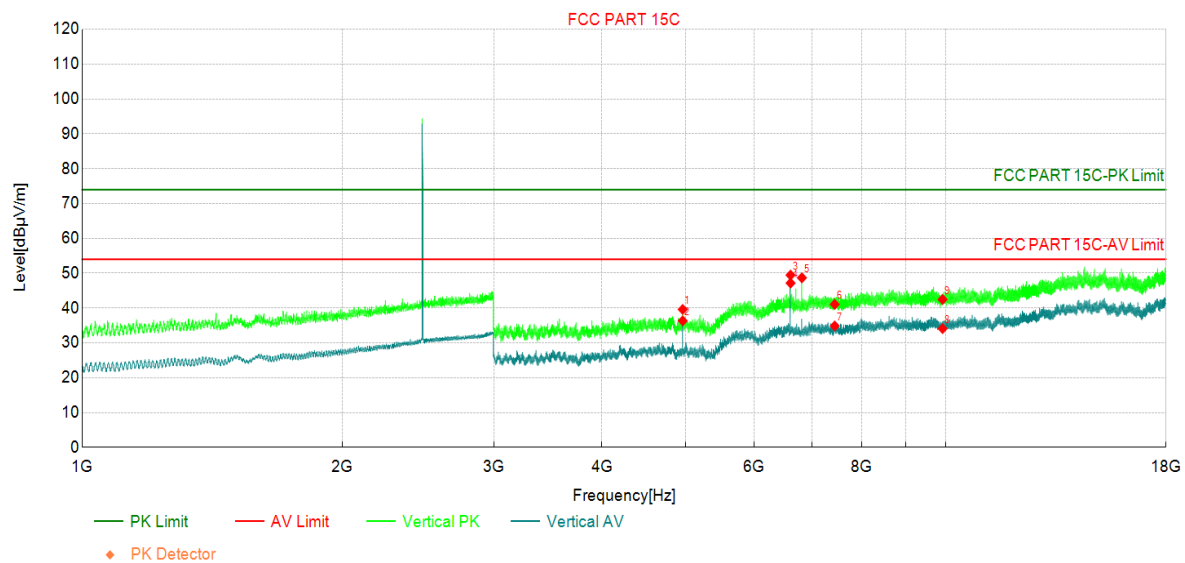

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	44.86	39.59	-5.27	74.00	34.41	PK	Vertic	PASS
2	4960.00	41.60	36.33	-5.27	54.00	17.67	AV	Vertic	PASS
3	6613.13	47.30	49.45	2.15	74.00	24.55	PK	Vertic	PASS
4	6613.50	44.99	47.15	2.16	54.00	6.85	AV	Vertic	PASS
5	6816.38	46.61	48.68	2.07	74.00	25.32	PK	Vertic	PASS
6	7440.00	38.49	41.05	2.56	74.00	32.95	PK	Vertic	PASS
7	7440.00	32.29	34.85	2.56	54.00	19.15	AV	Vertic	PASS
8	9920.00	28.47	34.09	5.62	54.00	19.91	AV	Vertic	PASS
9	9920.00	36.85	42.47	5.62	74.00	31.53	PK	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2402MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

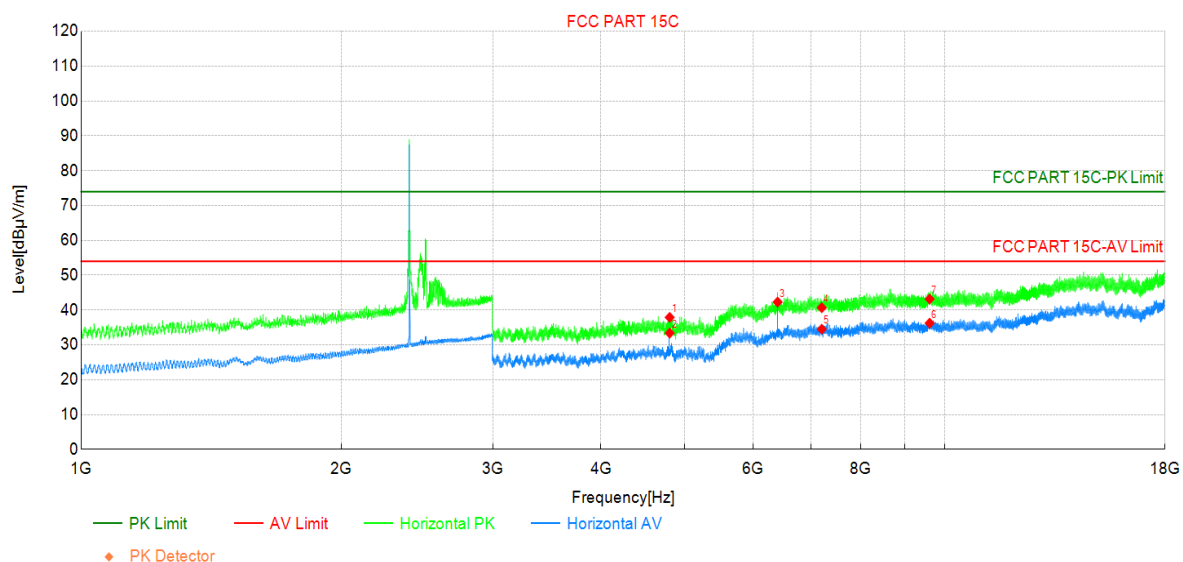

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	43.92	37.89	-6.03	74.00	36.11	PK	Horizo	PASS
2	4804.00	39.41	33.38	-6.03	54.00	20.62	AV	Horizo	PASS
3	6405.75	40.84	42.27	1.43	54.00	11.73	AV	Horizo	PASS
4	7206.00	37.71	40.68	2.97	74.00	33.32	PK	Horizo	PASS
5	7206.00	31.52	34.49	2.97	54.00	19.51	AV	Horizo	PASS
6	9608.00	30.29	36.23	5.94	54.00	17.77	AV	Horizo	PASS
7	9608.00	37.21	43.15	5.94	74.00	30.85	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2402MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

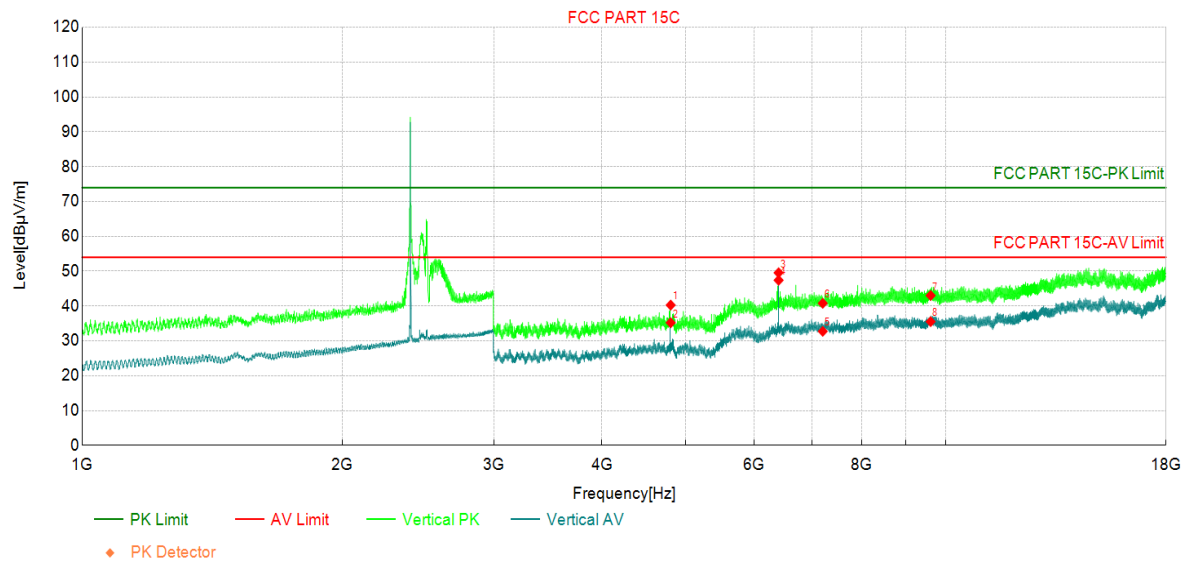

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	46.30	40.27	-6.03	74.00	33.73	PK	Vertic	PASS
2	4804.00	41.23	35.20	-6.03	54.00	18.80	AV	Vertic	PASS
3	6405.38	48.11	49.54	1.43	74.00	24.46	PK	Vertic	PASS
4	6405.75	45.97	47.40	1.43	54.00	6.60	AV	Vertic	PASS
5	7206.00	29.77	32.74	2.97	54.00	21.26	AV	Vertic	PASS
6	7206.00	37.81	40.78	2.97	74.00	33.22	PK	Vertic	PASS
7	9608.00	37.07	43.01	5.94	74.00	30.99	PK	Vertic	PASS
8	9608.00	29.58	35.52	5.94	54.00	18.48	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2440MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

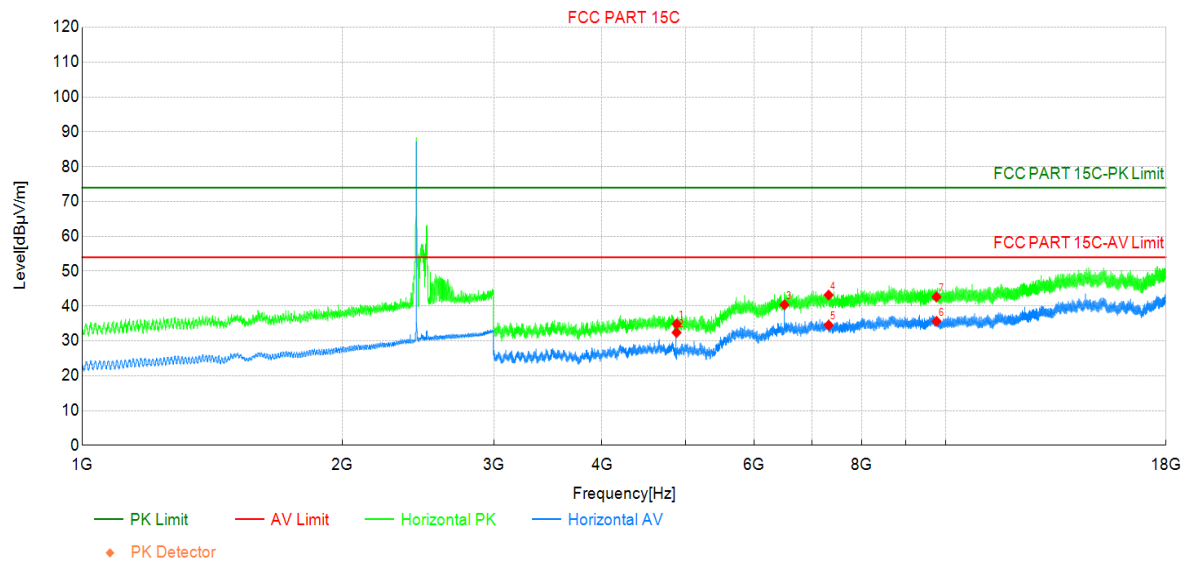

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	40.94	34.86	-6.08	74.00	39.14	PK	Horizo	PASS
2	4880.00	38.47	32.39	-6.08	54.00	21.61	AV	Horizo	PASS
3	6507.00	38.65	40.34	1.69	54.00	13.66	AV	Horizo	PASS
4	7320.00	40.35	43.15	2.80	74.00	30.85	PK	Horizo	PASS
5	7320.00	31.71	34.51	2.80	54.00	19.49	AV	Horizo	PASS
6	9760.00	29.50	35.63	6.13	54.00	18.37	AV	Horizo	PASS
7	9760.00	36.48	42.61	6.13	74.00	31.39	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2440MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

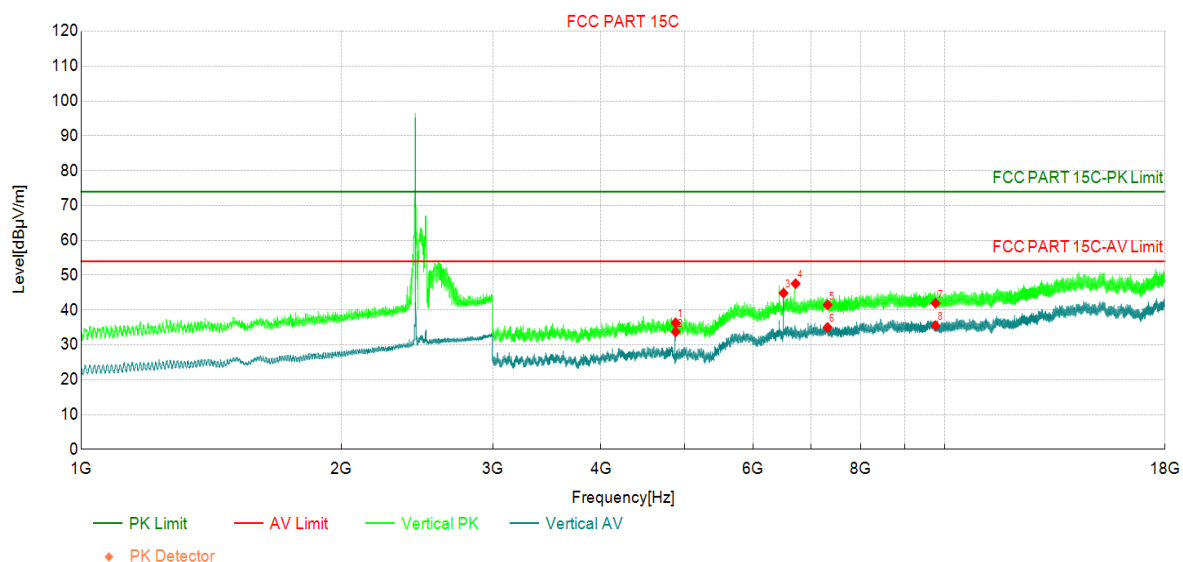

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	42.39	36.31	-6.08	74.00	37.69	PK	Vertic	PASS
2	4880.00	39.80	33.72	-6.08	54.00	20.28	AV	Vertic	PASS
3	6507.00	43.16	44.85	1.69	54.00	9.15	AV	Vertic	PASS
4	6720.75	45.99	47.58	1.59	74.00	26.42	PK	Vertic	PASS
5	7320.00	38.70	41.50	2.80	74.00	32.50	PK	Vertic	PASS
6	7320.00	32.21	35.01	2.80	54.00	18.99	AV	Vertic	PASS
7	9760.00	35.81	41.94	6.13	74.00	32.06	PK	Vertic	PASS
8	9760.00	29.40	35.53	6.13	54.00	18.47	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2480MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

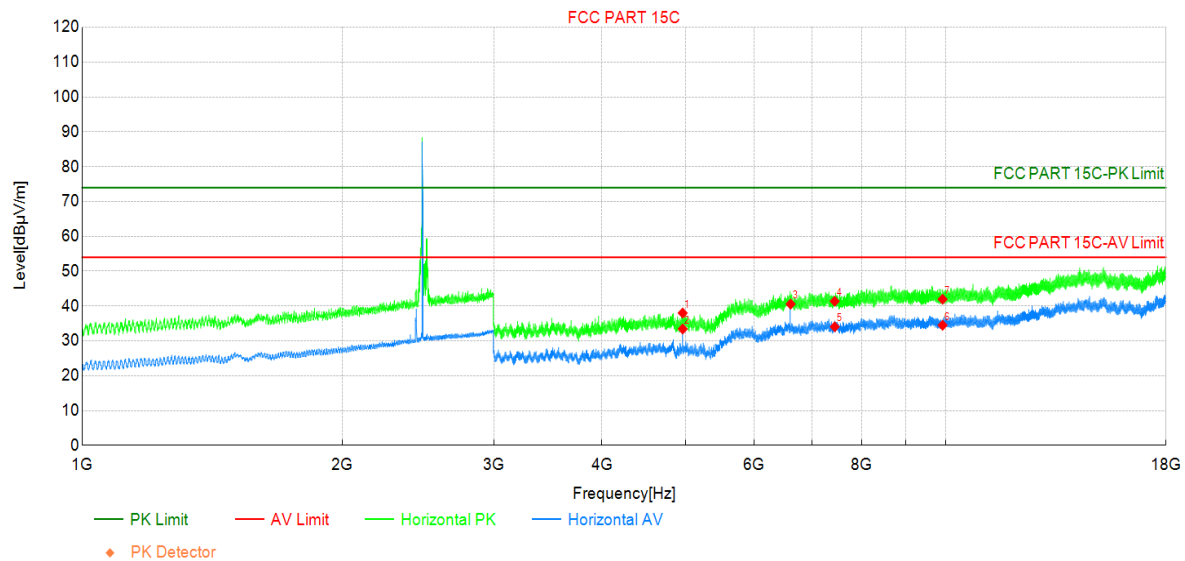

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	43.26	37.99	-5.27	74.00	36.01	PK	Horizo	PASS
2	4960.00	38.68	33.41	-5.27	54.00	20.59	AV	Horizo	PASS
3	6613.88	38.42	40.57	2.15	54.00	13.43	AV	Horizo	PASS
4	7440.00	38.81	41.37	2.56	74.00	32.63	PK	Horizo	PASS
5	7440.00	31.48	34.04	2.56	54.00	19.96	AV	Horizo	PASS
6	9920.00	28.86	34.48	5.62	54.00	19.52	AV	Horizo	PASS
7	9920.00	36.33	41.95	5.62	74.00	32.05	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2480MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

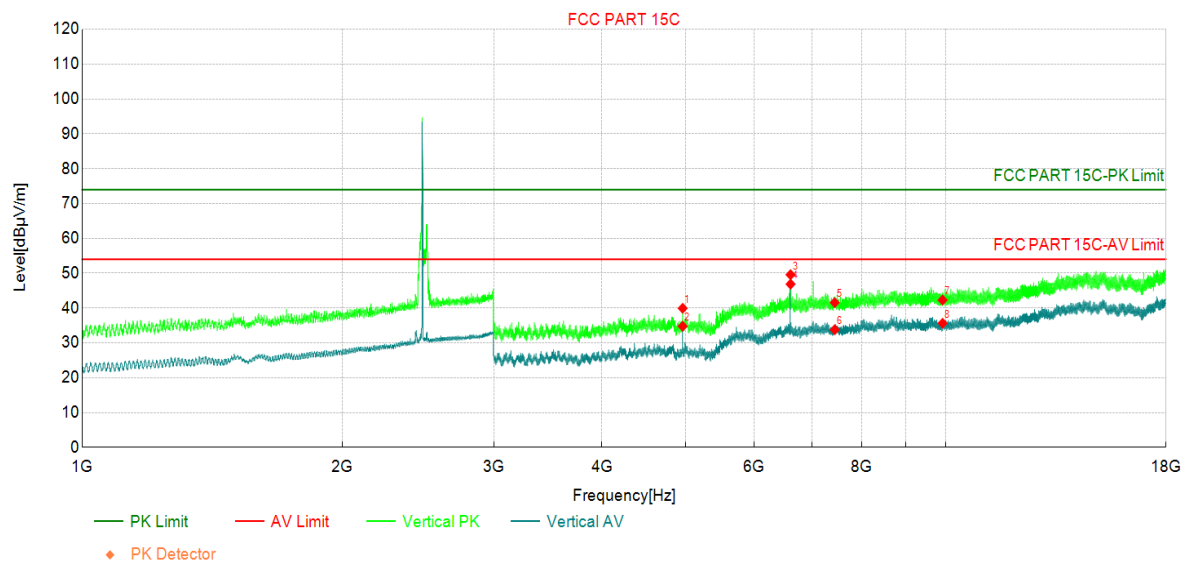

Suspected Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	45.19	39.92	-5.27	74.00	34.08	PK	Vertic	PASS
2	4960.00	40.05	34.78	-5.27	54.00	19.22	AV	Vertic	PASS
3	6613.13	47.42	49.57	2.15	74.00	24.43	PK	Vertic	PASS
4	6613.50	44.70	46.86	2.16	54.00	7.14	AV	Vertic	PASS
5	7440.00	38.99	41.55	2.56	74.00	32.45	PK	Vertic	PASS
6	7440.00	31.22	33.78	2.56	54.00	20.22	AV	Vertic	PASS
7	9920.00	36.66	42.28	5.62	74.00	31.72	PK	Vertic	PASS
8	9920.00	30.01	35.63	5.62	54.00	18.37	AV	Vertic	PASS


Right Ear

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2402MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer:	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

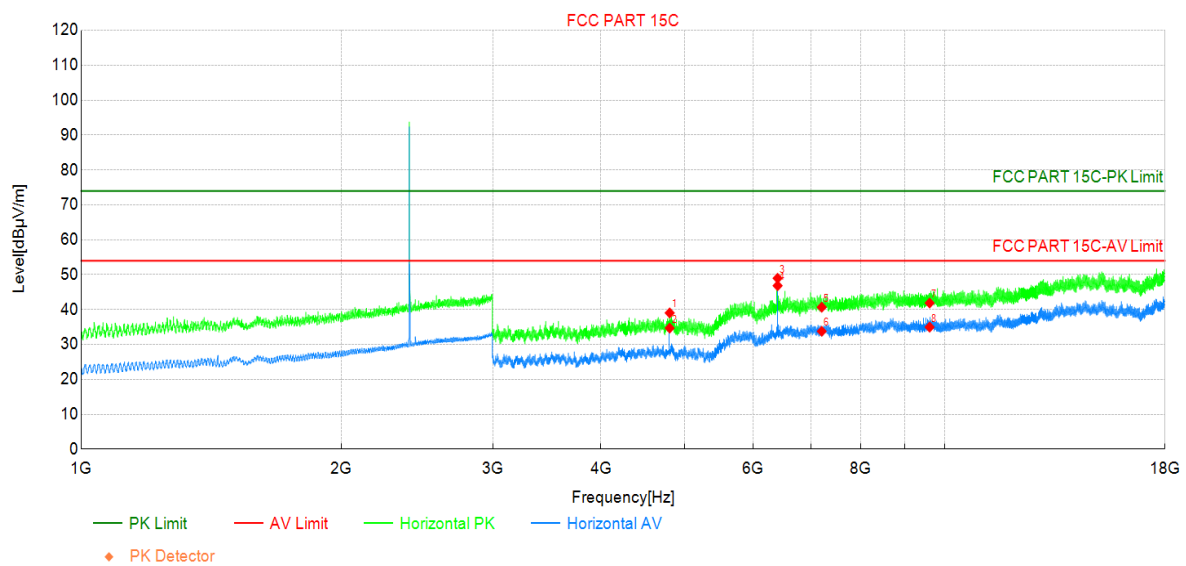

Suspected Data List


NO	Frequency [MHz]	Reading [dBµV]	Level [dBµV/m]	Factor [dB/m]	Limit [dBµV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	45.07	39.04	-6.03	74.00	34.96	PK	Horizo	PASS
2	4804.00	40.71	34.68	-6.03	54.00	19.32	AV	Horizo	PASS
3	6405.38	47.53	48.96	1.43	74.00	25.04	PK	Horizo	PASS
4	6405.75	45.40	46.83	1.43	54.00	7.17	AV	Horizo	PASS
5	7206.00	37.71	40.68	2.97	74.00	33.32	PK	Horizo	PASS
6	7206.00	30.81	33.78	2.97	54.00	20.22	AV	Horizo	PASS
7	9608.00	35.92	41.86	5.94	74.00	32.14	PK	Horizo	PASS
8	9608.00	29.02	34.96	5.94	54.00	19.04	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2402MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

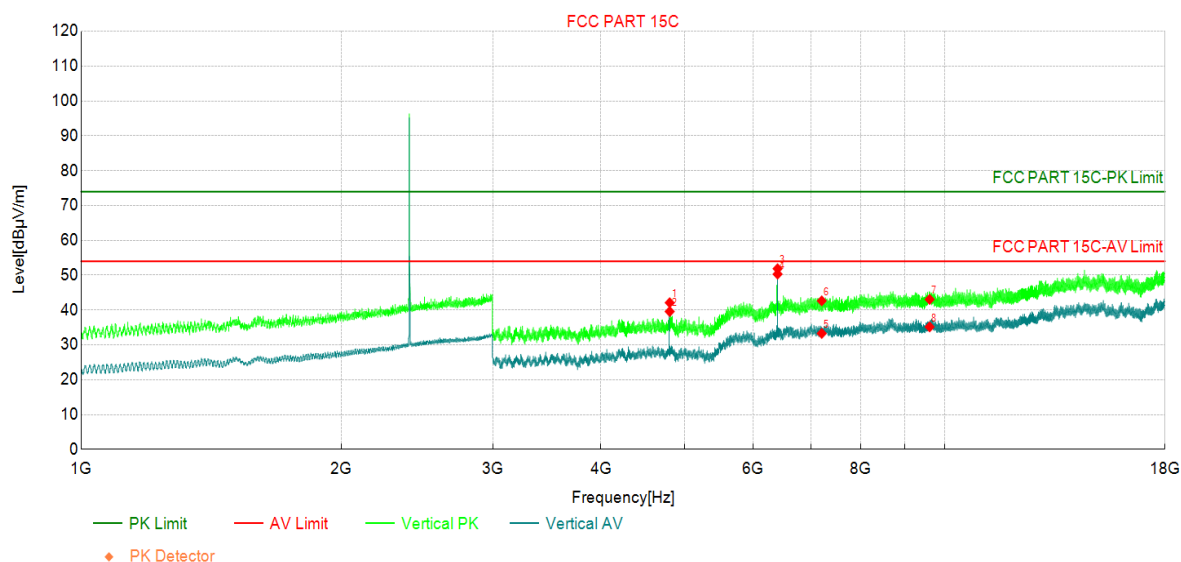

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	48.13	42.10	-6.03	74.00	31.90	PK	Vertic	PASS
2	4804.00	45.60	39.57	-6.03	54.00	14.43	AV	Vertic	PASS
3	6405.38	50.42	51.85	1.43	74.00	22.15	PK	Vertic	PASS
4	6405.75	48.87	50.30	1.43	54.00	3.70	AV	Vertic	PASS
5	7206.00	30.32	33.29	2.97	54.00	20.71	AV	Vertic	PASS
6	7206.00	39.66	42.63	2.97	74.00	31.37	PK	Vertic	PASS
7	9608.00	37.10	43.04	5.94	74.00	30.96	PK	Vertic	PASS
8	9608.00	29.22	35.16	5.94	54.00	18.84	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2440MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

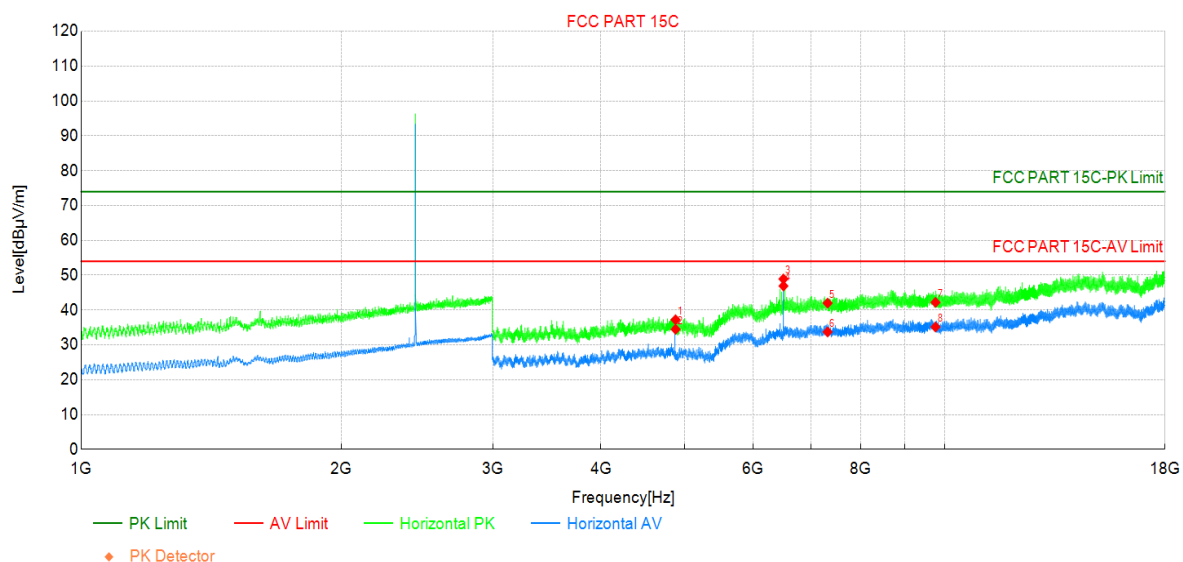

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	43.28	37.20	-6.08	74.00	36.80	PK	Horizo	PASS
2	4880.00	40.55	34.47	-6.08	54.00	19.53	AV	Horizo	PASS
3	6506.63	47.22	48.91	1.69	74.00	25.09	PK	Horizo	PASS
4	6507.00	45.20	46.89	1.69	54.00	7.11	AV	Horizo	PASS
5	7320.00	39.19	41.99	2.80	74.00	32.01	PK	Horizo	PASS
6	7320.00	30.91	33.71	2.80	54.00	20.29	AV	Horizo	PASS
7	9760.00	36.06	42.19	6.13	74.00	31.81	PK	Horizo	PASS
8	9760.00	29.01	35.14	6.13	54.00	18.86	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2440MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

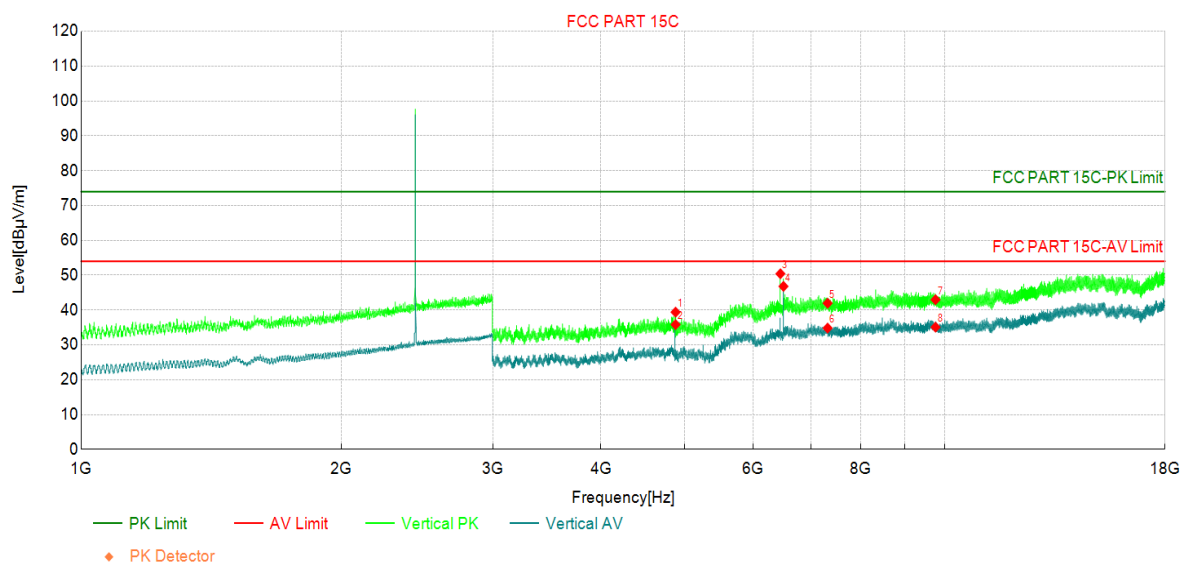

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	45.47	39.39	-6.08	74.00	34.61	PK	Vertic	PASS
2	4880.00	41.89	35.81	-6.08	54.00	18.19	AV	Vertic	PASS
3	6453.75	48.87	50.41	1.54	74.00	23.59	PK	Vertic	PASS
4	6507.00	45.10	46.79	1.69	54.00	7.21	AV	Vertic	PASS
5	7320.00	39.15	41.95	2.80	74.00	32.05	PK	Vertic	PASS
6	7320.00	32.01	34.81	2.80	54.00	19.19	AV	Vertic	PASS
7	9760.00	36.83	42.96	6.13	74.00	31.04	PK	Vertic	PASS
8	9760.00	28.96	35.09	6.13	54.00	18.91	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2480MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

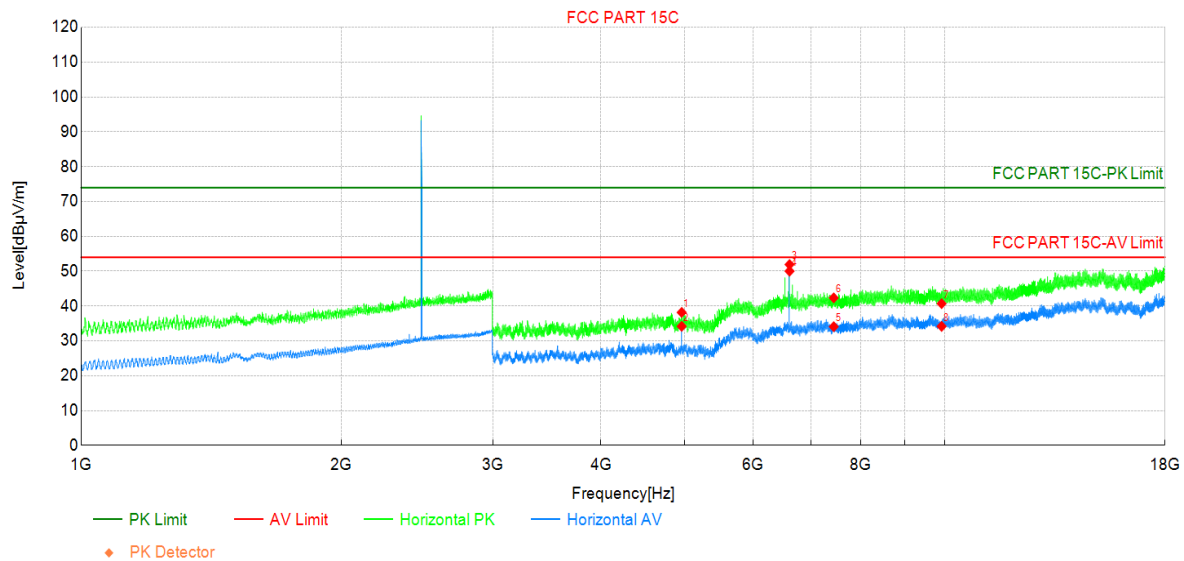

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	43.44	38.17	-5.27	74.00	35.83	PK	Horizo	PASS
2	4960.00	39.44	34.17	-5.27	54.00	19.83	AV	Horizo	PASS
3	6613.13	49.76	51.91	2.15	74.00	22.09	PK	Horizo	PASS
4	6613.50	47.85	50.01	2.16	54.00	3.99	AV	Horizo	PASS
5	7440.00	31.51	34.07	2.56	54.00	19.93	AV	Horizo	PASS
6	7440.00	39.78	42.34	2.56	74.00	31.66	PK	Horizo	PASS
7	9920.00	35.07	40.69	5.62	74.00	33.31	PK	Horizo	PASS
8	9920.00	28.55	34.17	5.62	54.00	19.83	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_1M:Transmit at 2480MHz by LE 1M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

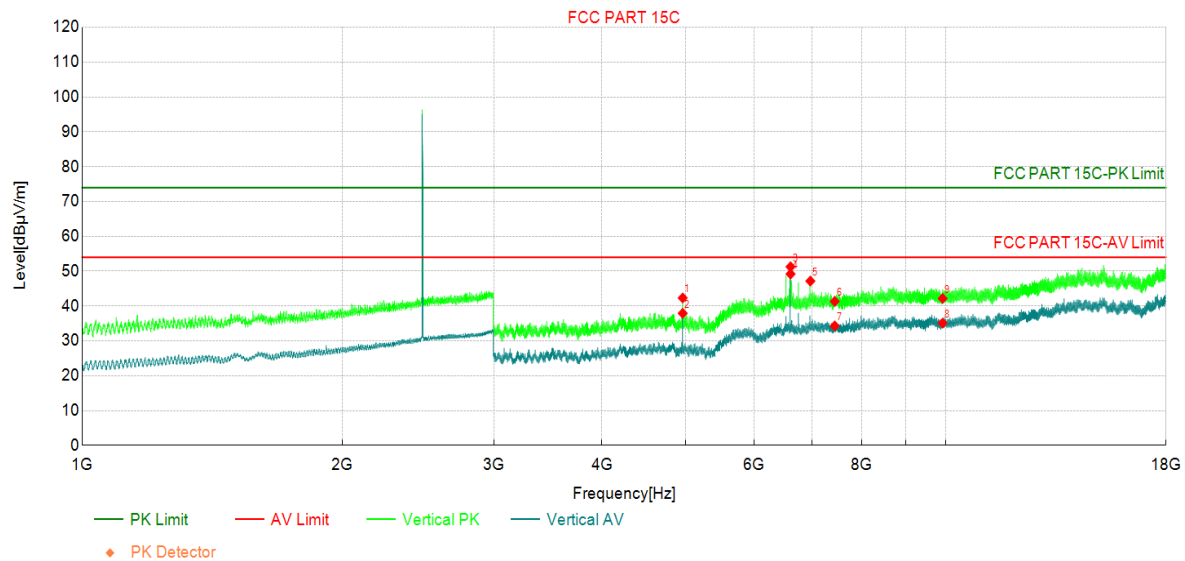

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	47.59	42.32	-5.27	74.00	31.68	PK	Vertic	PASS
2	4960.00	43.18	37.91	-5.27	54.00	16.09	AV	Vertic	PASS
3	6613.13	49.11	51.26	2.15	74.00	22.74	PK	Vertic	PASS
4	6613.50	47.03	49.19	2.16	54.00	4.81	AV	Vertic	PASS
5	6972.00	44.79	47.17	2.38	74.00	26.83	PK	Vertic	PASS
6	7440.00	38.77	41.33	2.56	74.00	32.67	PK	Vertic	PASS
7	7440.00	31.71	34.27	2.56	54.00	19.73	AV	Vertic	PASS
8	9920.00	29.47	35.09	5.62	54.00	18.91	AV	Vertic	PASS
9	9920.00	36.54	42.16	5.62	74.00	31.84	PK	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2402MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

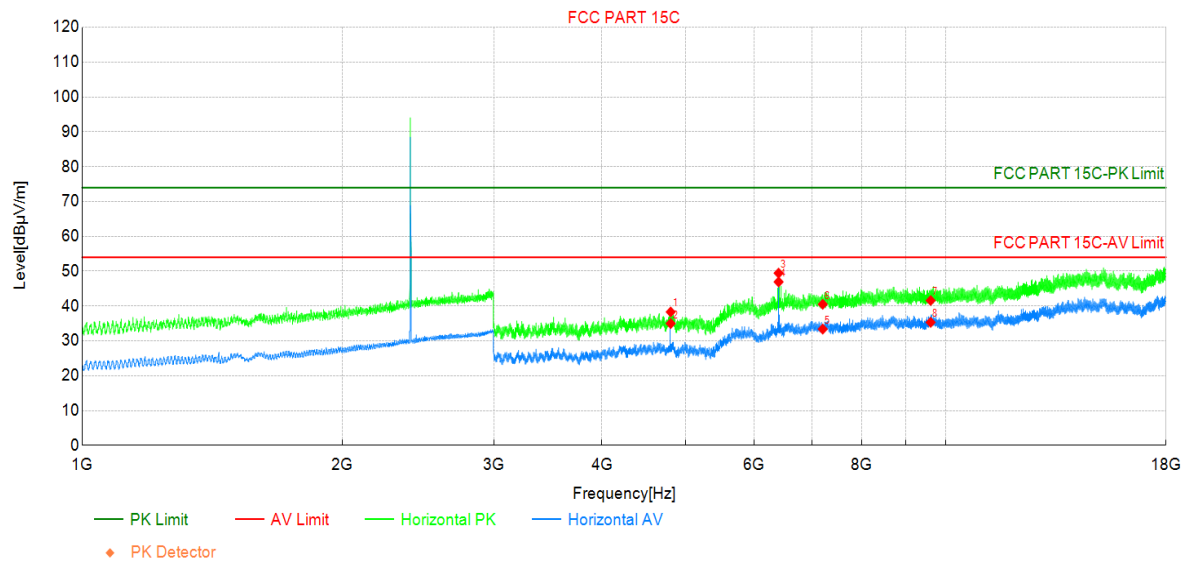

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	44.33	38.30	-6.03	74.00	35.70	PK	Horizo	PASS
2	4804.00	41.01	34.98	-6.03	54.00	19.02	AV	Horizo	PASS
3	6405.38	48.01	49.44	1.43	74.00	24.56	PK	Horizo	PASS
4	6405.75	45.50	46.93	1.43	54.00	7.07	AV	Horizo	PASS
5	7206.00	30.41	33.38	2.97	54.00	20.62	AV	Horizo	PASS
6	7206.00	37.53	40.50	2.97	74.00	33.50	PK	Horizo	PASS
7	9608.00	35.65	41.59	5.94	74.00	32.41	PK	Horizo	PASS
8	9608.00	29.37	35.31	5.94	54.00	18.69	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2402MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

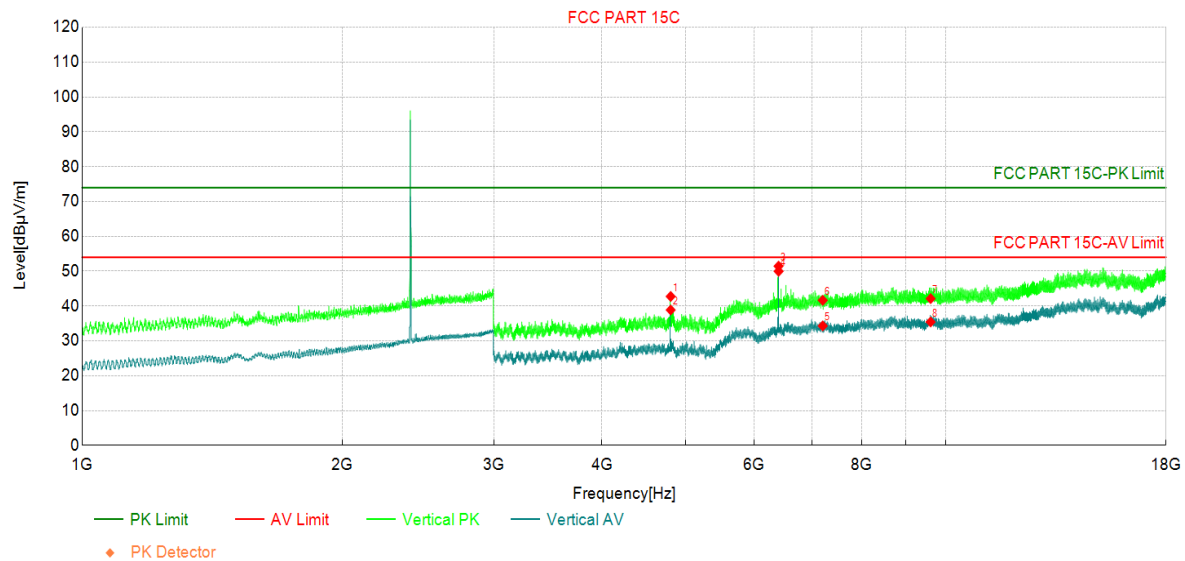

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	48.77	42.74	-6.03	74.00	31.26	PK	Vertic	PASS
2	4804.00	44.90	38.87	-6.03	54.00	15.13	AV	Vertic	PASS
3	6404.63	50.03	51.45	1.42	74.00	22.55	PK	Vertic	PASS
4	6405.75	48.55	49.98	1.43	54.00	4.02	AV	Vertic	PASS
5	7206.00	31.32	34.29	2.97	54.00	19.71	AV	Vertic	PASS
6	7206.00	38.67	41.64	2.97	74.00	32.36	PK	Vertic	PASS
7	9608.00	36.18	42.12	5.94	74.00	31.88	PK	Vertic	PASS
8	9608.00	29.48	35.42	5.94	54.00	18.58	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2440MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

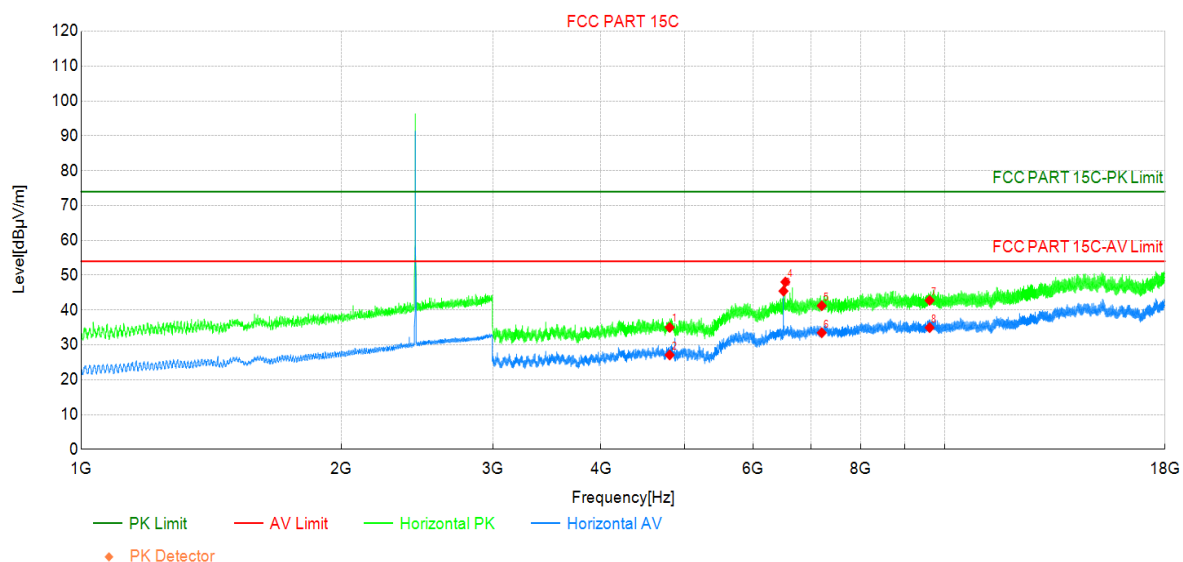

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	41.03	35.00	-6.03	74.00	39.00	PK	Horizo	PASS
2	4804.00	33.12	27.09	-6.03	54.00	26.91	AV	Horizo	PASS
3	6507.00	43.75	45.44	1.69	54.00	8.56	AV	Horizo	PASS
4	6539.63	46.16	48.05	1.89	74.00	25.95	PK	Horizo	PASS
5	7206.00	38.27	41.24	2.97	74.00	32.76	PK	Horizo	PASS
6	7206.00	30.50	33.47	2.97	54.00	20.53	AV	Horizo	PASS
7	9608.00	36.80	42.74	5.94	74.00	31.26	PK	Horizo	PASS
8	9608.00	28.99	34.93	5.94	54.00	19.07	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2440MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

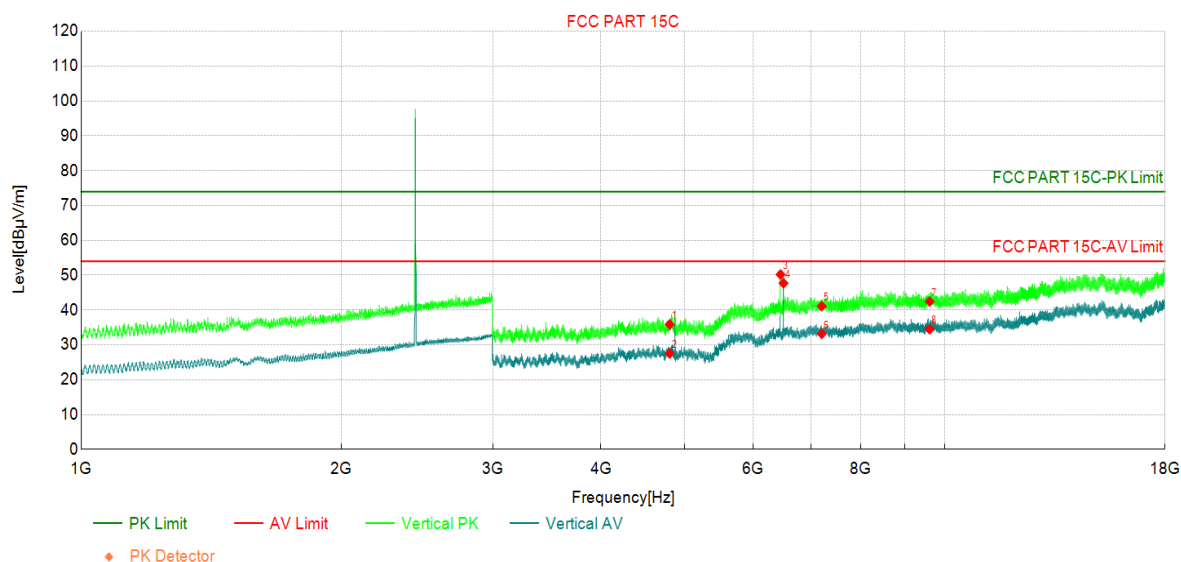

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	41.90	35.87	-6.03	74.00	38.13	PK	Vertic	PASS
2	4804.00	33.56	27.53	-6.03	54.00	26.47	AV	Vertic	PASS
3	6456.38	48.65	50.19	1.54	74.00	23.81	PK	Vertic	PASS
4	6507.00	46.01	47.70	1.69	54.00	6.30	AV	Vertic	PASS
5	7206.00	38.12	41.09	2.97	74.00	32.91	PK	Vertic	PASS
6	7206.00	30.20	33.17	2.97	54.00	20.83	AV	Vertic	PASS
7	9608.00	36.49	42.43	5.94	74.00	31.57	PK	Vertic	PASS
8	9608.00	28.56	34.50	5.94	54.00	19.50	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2480MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

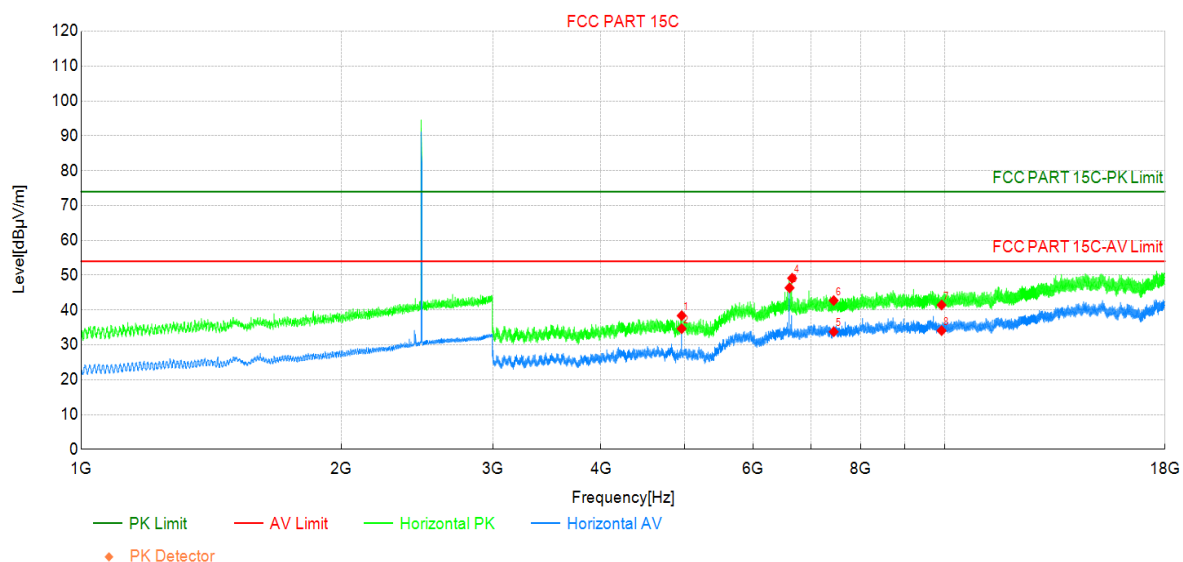

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	43.66	38.39	-5.27	74.00	35.61	PK	Horizo	PASS
2	4960.00	39.92	34.65	-5.27	54.00	19.35	AV	Horizo	PASS
3	6613.50	44.20	46.36	2.16	54.00	7.64	AV	Horizo	PASS
4	6658.88	47.34	49.13	1.79	74.00	24.87	PK	Horizo	PASS
5	7440.00	31.20	33.76	2.56	54.00	20.24	AV	Horizo	PASS
6	7440.00	40.15	42.71	2.56	74.00	31.29	PK	Horizo	PASS
7	9920.00	35.82	41.44	5.62	74.00	32.56	PK	Horizo	PASS
8	9920.00	28.47	34.09	5.62	54.00	19.91	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_2M:Transmit at 2480MHz by LE 2M	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

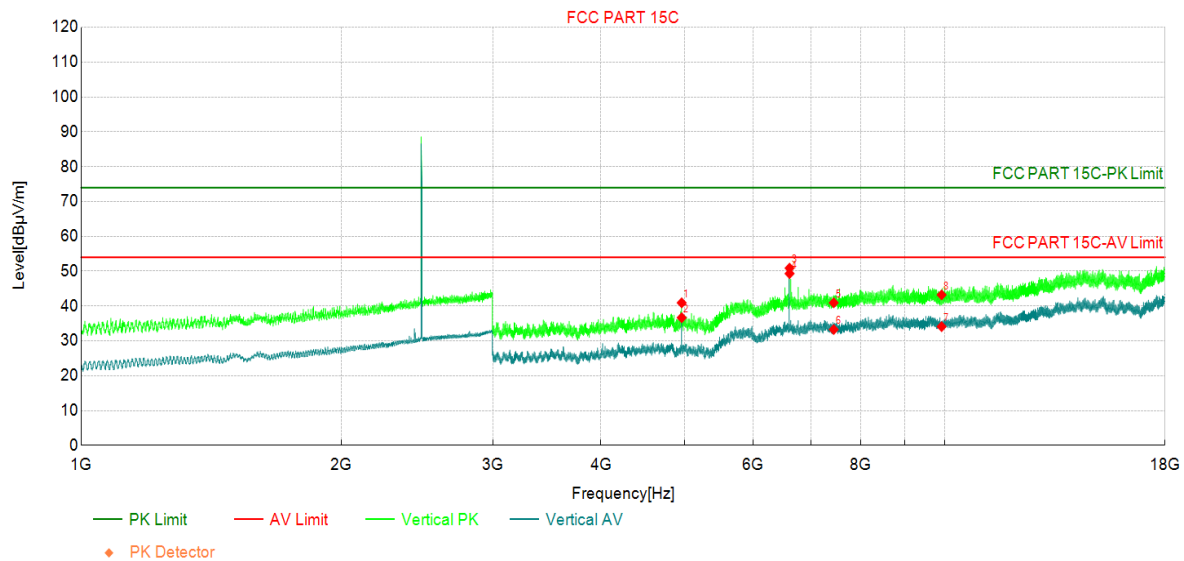

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	46.19	40.92	-5.27	74.00	33.08	PK	Vertic	PASS
2	4960.00	41.92	36.65	-5.27	54.00	17.35	AV	Vertic	PASS
3	6613.13	48.73	50.88	2.15	74.00	23.12	PK	Vertic	PASS
4	6613.50	47.15	49.31	2.16	54.00	4.69	AV	Vertic	PASS
5	7440.00	38.37	40.93	2.56	74.00	33.07	PK	Vertic	PASS
6	7440.00	30.70	33.26	2.56	54.00	20.74	AV	Vertic	PASS
7	9920.00	28.46	34.08	5.62	54.00	19.92	AV	Vertic	PASS
8	9920.00	37.58	43.20	5.62	74.00	30.80	PK	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2402MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

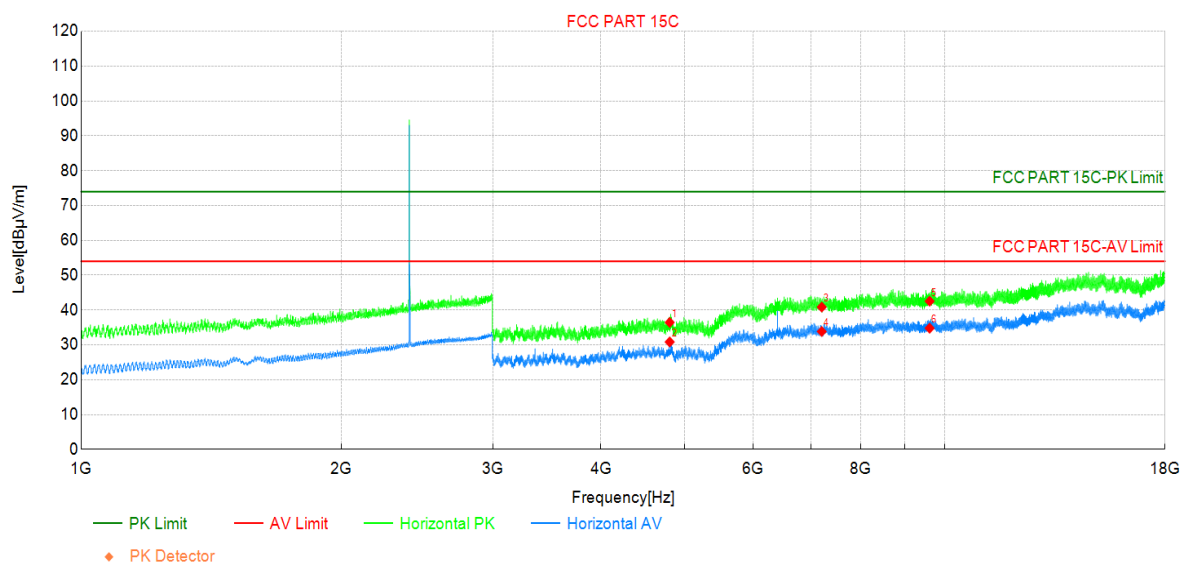

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	42.48	36.45	-6.03	74.00	37.55	PK	Horizo	PASS
2	4804.00	36.87	30.84	-6.03	54.00	23.16	AV	Horizo	PASS
3	7206.00	37.88	40.85	2.97	74.00	33.15	PK	Horizo	PASS
4	7206.00	30.86	33.83	2.97	54.00	20.17	AV	Horizo	PASS
5	9608.00	36.59	42.53	5.94	74.00	31.47	PK	Horizo	PASS
6	9608.00	28.84	34.78	5.94	54.00	19.22	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2402MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

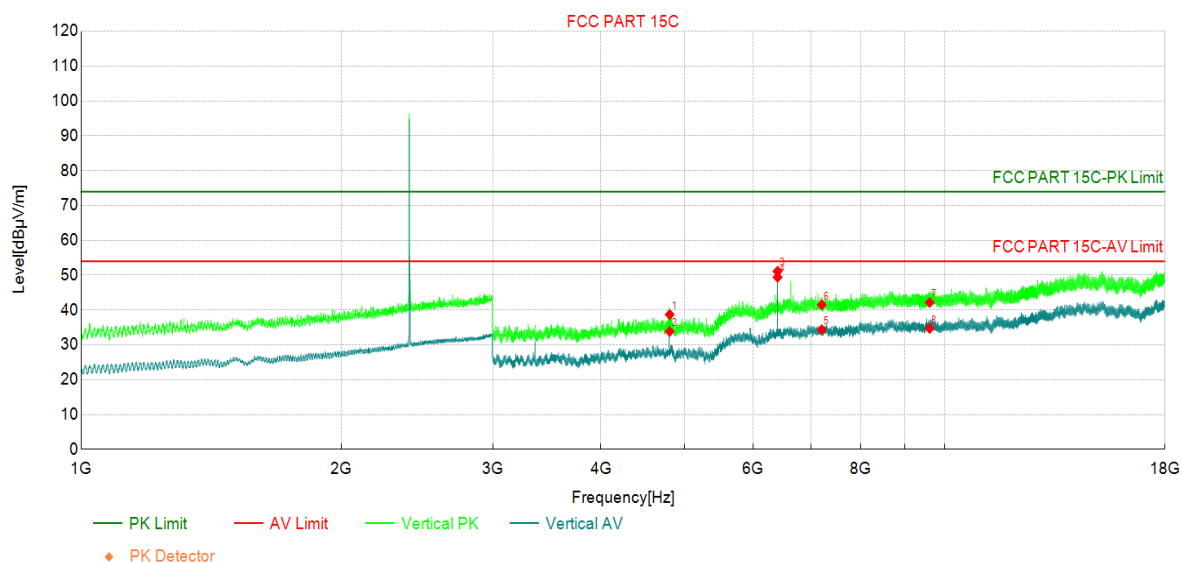

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	44.74	38.71	-6.03	74.00	35.29	PK	Vertic	PASS
2	4804.00	39.87	33.84	-6.03	54.00	20.16	AV	Vertic	PASS
3	6405.00	49.70	51.12	1.42	74.00	22.88	PK	Vertic	PASS
4	6405.75	47.98	49.41	1.43	54.00	4.59	AV	Vertic	PASS
5	7206.00	31.35	34.32	2.97	54.00	19.68	AV	Vertic	PASS
6	7206.00	38.54	41.51	2.97	74.00	32.49	PK	Vertic	PASS
7	9608.00	36.21	42.15	5.94	74.00	31.85	PK	Vertic	PASS
8	9608.00	28.78	34.72	5.94	54.00	19.28	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2440MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Enginee	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

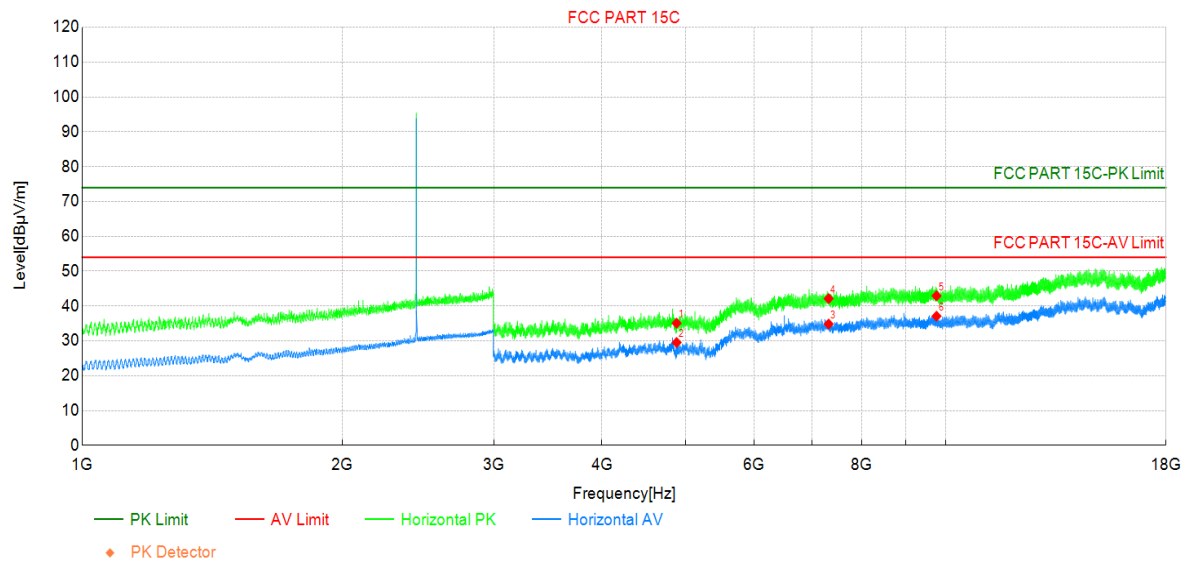

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	41.15	35.07	-6.08	74.00	38.93	PK	Horizo	PASS
2	4880.00	35.62	29.54	-6.08	54.00	24.46	AV	Horizo	PASS
3	7320.00	32.03	34.83	2.80	54.00	19.17	AV	Horizo	PASS
4	7320.00	39.33	42.13	2.80	74.00	31.87	PK	Horizo	PASS
5	9760.00	36.79	42.92	6.13	74.00	31.08	PK	Horizo	PASS
6	9760.00	30.95	37.08	6.13	54.00	16.92	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2440MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

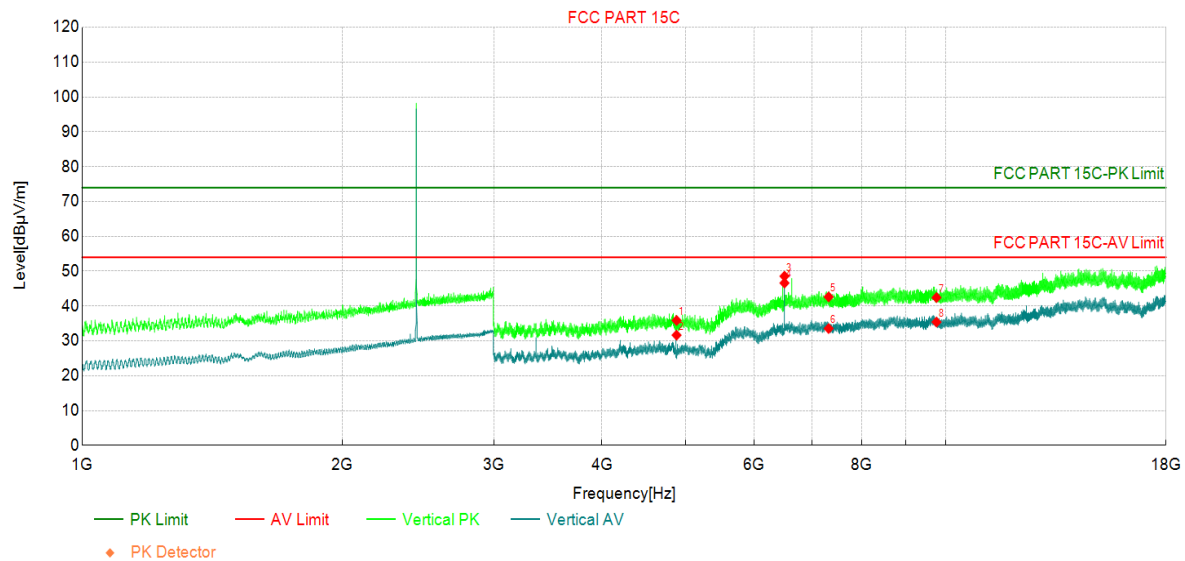

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	41.95	35.87	-6.08	74.00	38.13	PK	Vertic	PASS
2	4880.00	37.72	31.64	-6.08	54.00	22.36	AV	Vertic	PASS
3	6506.63	46.87	48.56	1.69	74.00	25.44	PK	Vertic	PASS
4	6507.00	44.90	46.59	1.69	54.00	7.41	AV	Vertic	PASS
5	7320.00	39.82	42.62	2.80	74.00	31.38	PK	Vertic	PASS
6	7320.00	30.75	33.55	2.80	54.00	20.45	AV	Vertic	PASS
7	9760.00	36.29	42.42	6.13	74.00	31.58	PK	Vertic	PASS
8	9760.00	29.27	35.40	6.13	54.00	18.60	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2480MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

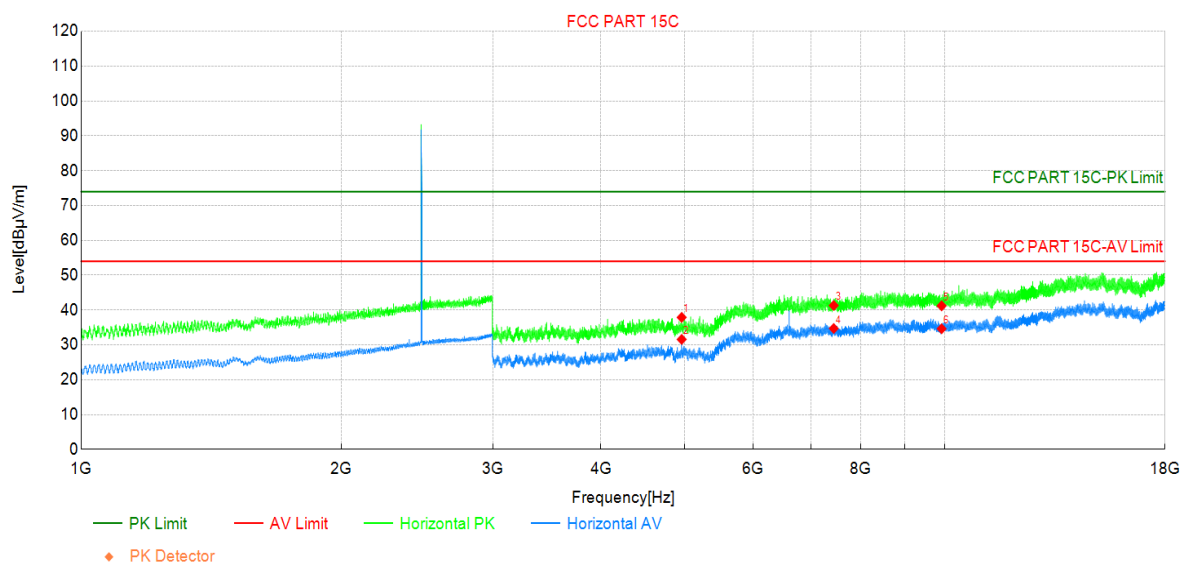

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	43.15	37.88	-5.27	74.00	36.12	PK	Horizo	PASS
2	4960.00	36.84	31.57	-5.27	54.00	22.43	AV	Horizo	PASS
3	7440.00	38.74	41.30	2.56	74.00	32.70	PK	Horizo	PASS
4	7440.00	32.14	34.70	2.56	54.00	19.30	AV	Horizo	PASS
5	9920.00	35.58	41.20	5.62	74.00	32.80	PK	Horizo	PASS
6	9920.00	29.00	34.62	5.62	54.00	19.38	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_125K:Transmit at 2480MHz by 125K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

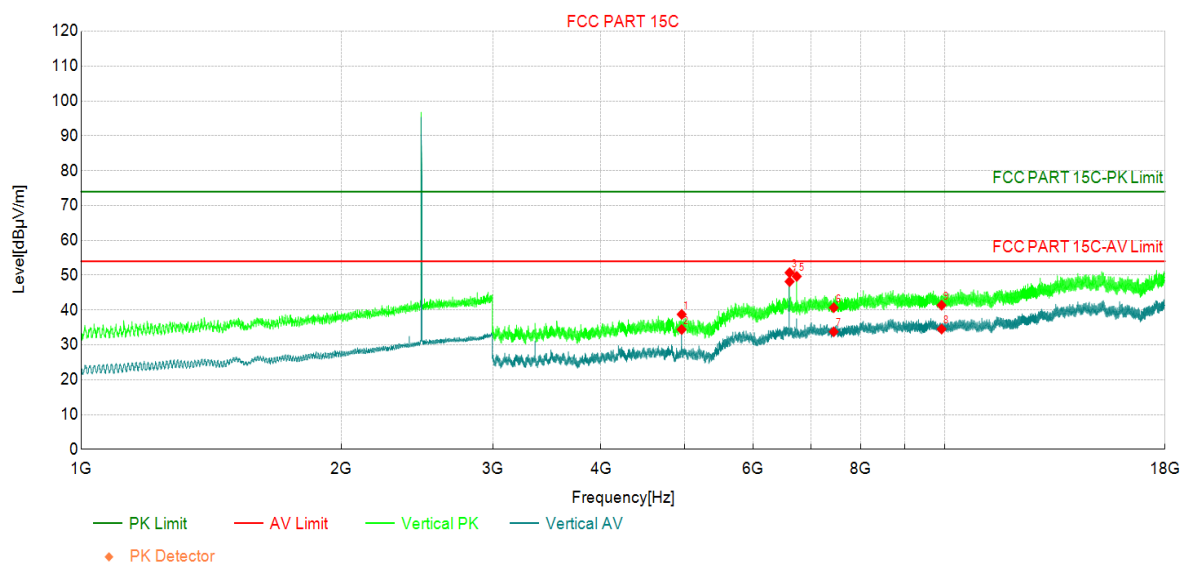

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	44.02	38.75	-5.27	74.00	35.25	PK	Vertic	PASS
2	4960.00	39.68	34.41	-5.27	54.00	19.59	AV	Vertic	PASS
3	6613.50	48.56	50.72	2.16	74.00	23.28	PK	Vertic	PASS
4	6613.50	46.01	48.17	2.16	54.00	5.83	AV	Vertic	PASS
5	6741.75	47.93	49.64	1.71	74.00	24.36	PK	Vertic	PASS
6	7440.00	38.11	40.67	2.56	74.00	33.33	PK	Vertic	PASS
7	7440.00	31.20	33.76	2.56	54.00	20.24	AV	Vertic	PASS
8	9920.00	28.90	34.52	5.62	54.00	19.48	AV	Vertic	PASS
9	9920.00	35.76	41.38	5.62	74.00	32.62	PK	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2402MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

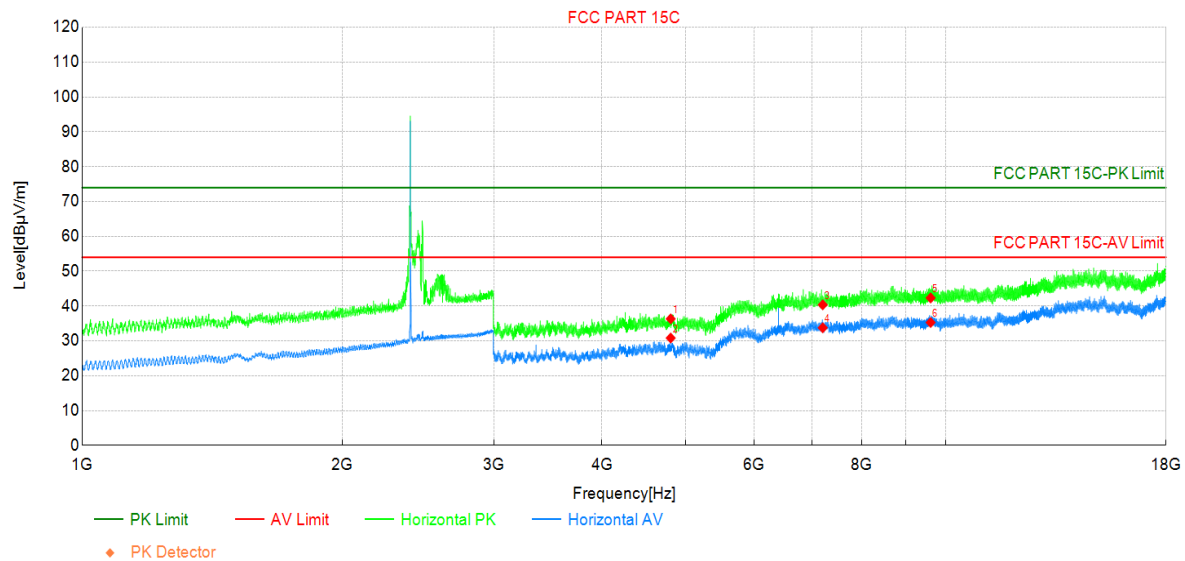

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	42.35	36.32	-6.03	74.00	37.68	PK	Horizo	PASS
2	4804.00	36.84	30.81	-6.03	54.00	23.19	AV	Horizo	PASS
3	7206.00	37.37	40.34	2.97	74.00	33.66	PK	Horizo	PASS
4	7206.00	30.79	33.76	2.97	54.00	20.24	AV	Horizo	PASS
5	9608.00	36.38	42.32	5.94	74.00	31.68	PK	Horizo	PASS
6	9608.00	29.33	35.27	5.94	54.00	18.73	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2402MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

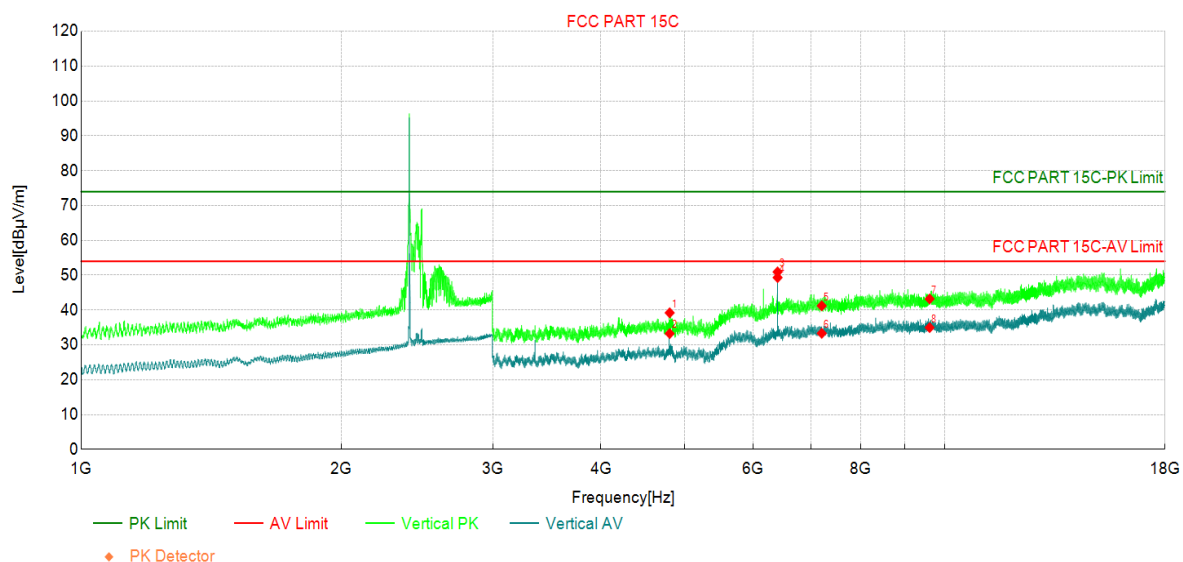

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	45.22	39.19	-6.03	74.00	34.81	PK	Vertic	PASS
2	4804.00	39.27	33.24	-6.03	54.00	20.76	AV	Vertic	PASS
3	6405.00	49.52	50.94	1.42	74.00	23.06	PK	Vertic	PASS
4	6405.75	47.88	49.31	1.43	54.00	4.69	AV	Vertic	PASS
5	7206.00	38.24	41.21	2.97	74.00	32.79	PK	Vertic	PASS
6	7206.00	30.35	33.32	2.97	54.00	20.68	AV	Vertic	PASS
7	9608.00	37.24	43.18	5.94	74.00	30.82	PK	Vertic	PASS
8	9608.00	29.01	34.95	5.94	54.00	19.05	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2440MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

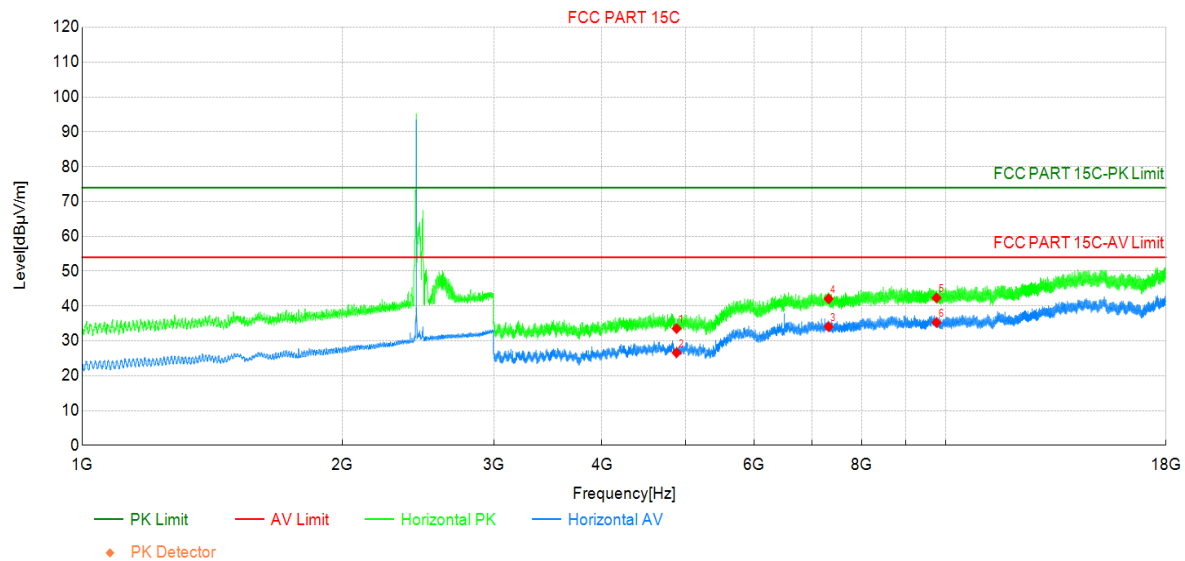

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	39.61	33.53	-6.08	74.00	40.47	PK	Horizo	PASS
2	4880.00	32.68	26.60	-6.08	54.00	27.40	AV	Horizo	PASS
3	7320.00	31.28	34.08	2.80	54.00	19.92	AV	Horizo	PASS
4	7320.00	39.26	42.06	2.80	74.00	31.94	PK	Horizo	PASS
5	9760.00	36.20	42.33	6.13	74.00	31.67	PK	Horizo	PASS
6	9760.00	29.14	35.27	6.13	54.00	18.73	AV	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2440MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

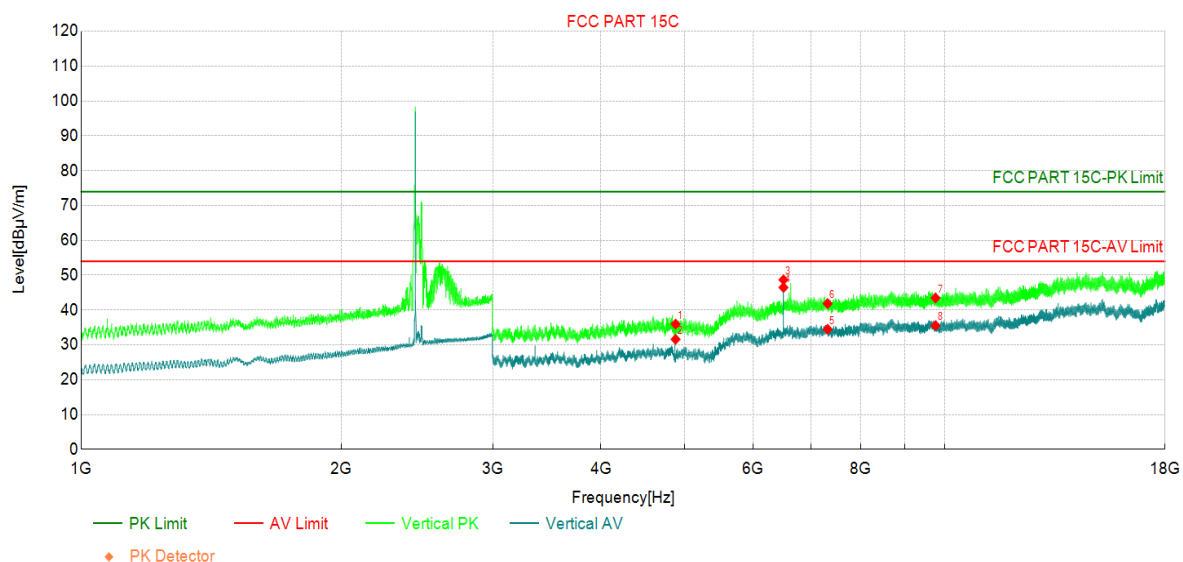

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4880.00	42.04	35.96	-6.08	74.00	38.04	PK	Vertic	PASS
2	4880.00	37.68	31.60	-6.08	54.00	22.40	AV	Vertic	PASS
3	6506.63	46.99	48.68	1.69	74.00	25.32	PK	Vertic	PASS
4	6507.00	44.78	46.47	1.69	54.00	7.53	AV	Vertic	PASS
5	7320.00	31.68	34.48	2.80	54.00	19.52	AV	Vertic	PASS
6	7320.00	39.05	41.85	2.80	74.00	32.15	PK	Vertic	PASS
7	9760.00	37.34	43.47	6.13	74.00	30.53	PK	Vertic	PASS
8	9760.00	29.40	35.53	6.13	54.00	18.47	AV	Vertic	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2480MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

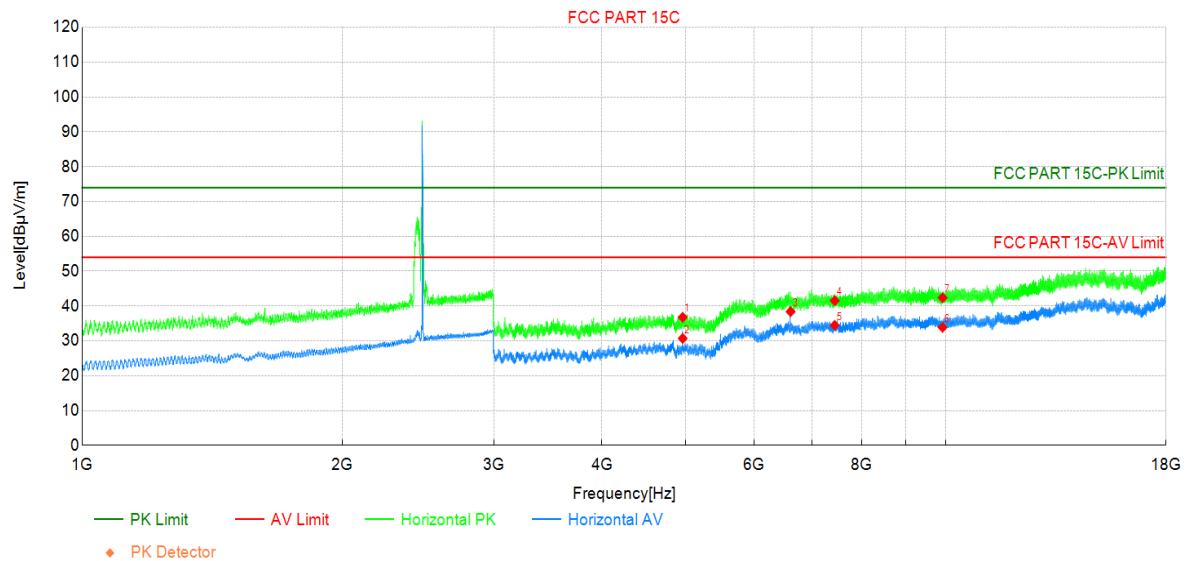

Suspected Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	42.03	36.76	-5.27	74.00	37.24	PK	Horizo	PASS
2	4960.00	35.97	30.70	-5.27	54.00	23.30	AV	Horizo	PASS
3	6613.88	36.25	38.40	2.15	54.00	15.60	AV	Horizo	PASS
4	7440.00	38.98	41.54	2.56	74.00	32.46	PK	Horizo	PASS
5	7440.00	31.89	34.45	2.56	54.00	19.55	AV	Horizo	PASS
6	9920.00	28.24	33.86	5.62	54.00	20.14	AV	Horizo	PASS
7	9920.00	36.75	42.37	5.62	74.00	31.63	PK	Horizo	PASS

Test Report

Project Information

Profile:	25B0571R	EUT:	Hearing aids
Mode:	BLE_500K:Transmit at 2480MHz by 500K	Voltage:	120 Vac / 60 Hz
Environment:	Temp: 25°C; Humi:60%	Engineer	Reyn Chen
Test Standard:	FCC PART 15C		

Test Graph

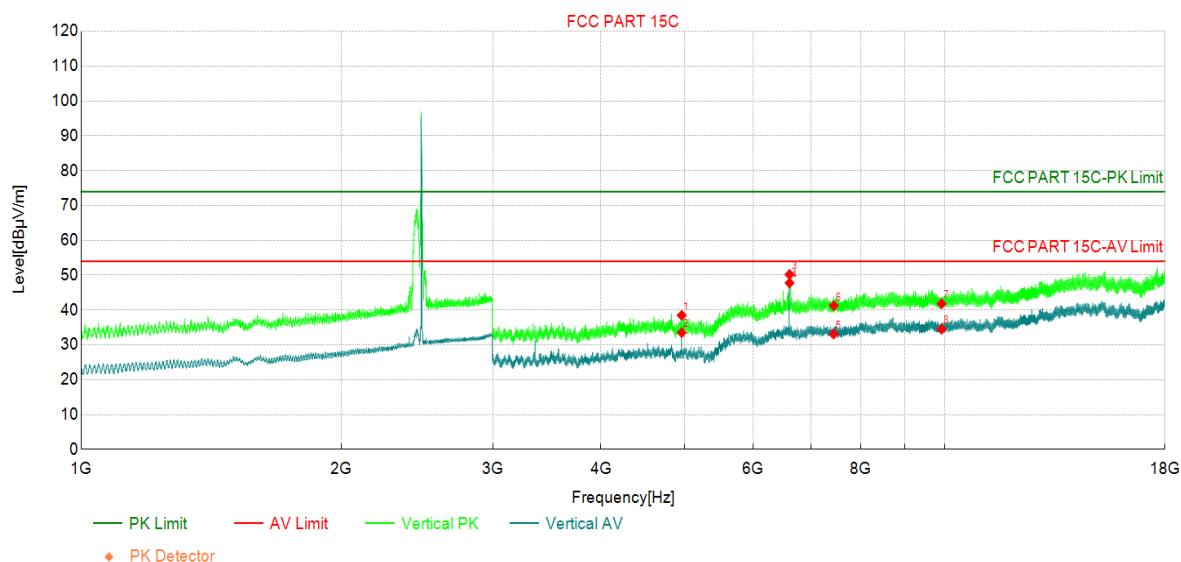

Suspected Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4960.00	43.74	38.47	-5.27	74.00	35.53	PK	Vertic	PASS
2	4960.00	38.80	33.53	-5.27	54.00	20.47	AV	Vertic	PASS
3	6613.13	48.05	50.20	2.15	74.00	23.80	PK	Vertic	PASS
4	6613.50	45.61	47.77	2.16	54.00	6.23	AV	Vertic	PASS
5	7440.00	30.56	33.12	2.56	54.00	20.88	AV	Vertic	PASS
6	7440.00	38.70	41.26	2.56	74.00	32.74	PK	Vertic	PASS
7	9920.00	36.19	41.81	5.62	74.00	32.19	PK	Vertic	PASS
8	9920.00	28.89	34.51	5.62	54.00	19.49	AV	Vertic	PASS

Note:

1. Level=Reading+Factor .


2. Margin=Limit-Level.

3. The test frequency range, 9kHz~30MHz, worst case are at least 20dB below the limits, therefore no data appear in the report.

4. The test frequency range, 18GHz~26GHz test result on peak is lower than average limit, all is the noise base, therefore no data appear in the report.

The worst case of Radiated Emission below 1GHz :

Limit: FCC_Part15.109_RE(3m)_ClassB	Margin: 0
Probe: CBL6112B_2931(30-1000MHz)	Polarity: Horizontal
EUT: Hearing aids	Power: 120Vac / 60Hz
Note: BLE_1M Transmit at 2402MHz by DH5	

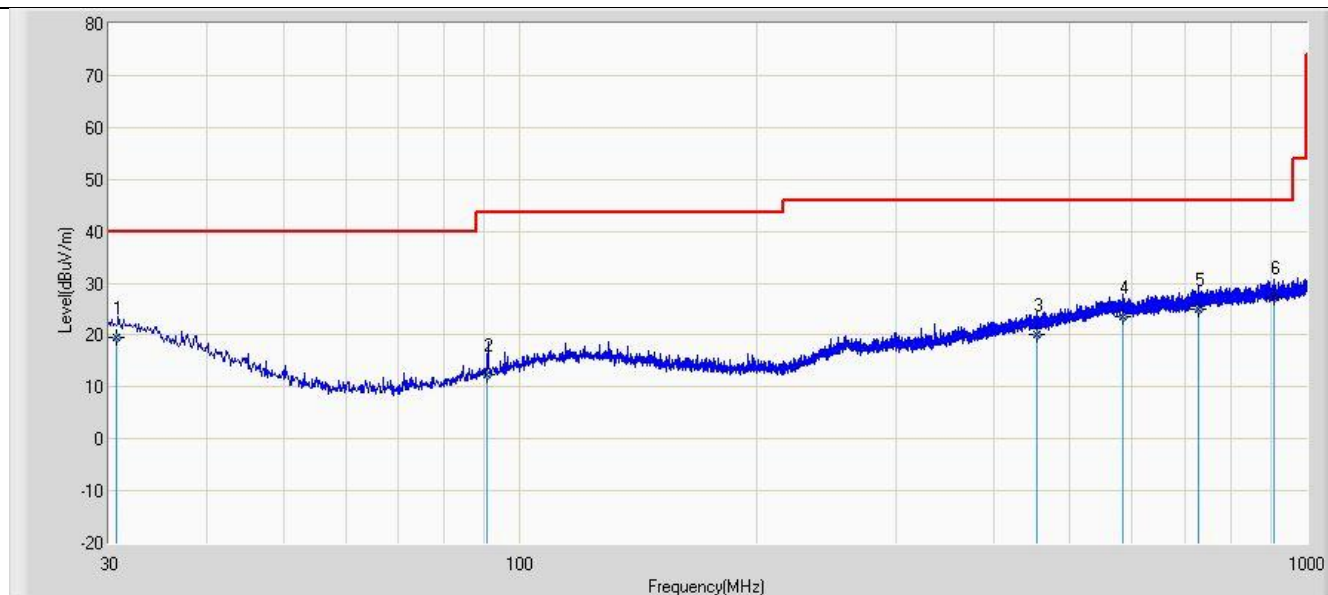


No	Mark	Frequency (MHz)	Measure Level (dBuV/m)	Reading Level (dBuV)	Over Limit (dB)	Limit (dBuV/m)	Probe (dB/m)	Cable (dB)	Amp (dB)	Ant Pos (cm)	Table Pos (deg)	Type
1		30.600	19.409	-5.400	-20.591	40.000	18.456	6.353	0.000	101	218	QP
2		90.600	12.448	-3.500	-31.052	43.500	9.255	6.694	0.000	300	63	QP
3		453.200	19.998	-4.600	-26.002	46.000	16.689	7.909	0.000	133	170	QP
4		584.630	23.610	-3.500	-22.390	46.000	18.868	8.242	0.000	100	89	QP
5		729.630	25.114	-3.200	-20.886	46.000	19.738	8.576	0.000	150	255	QP
6	*	908.630	27.194	-2.600	-18.806	46.000	20.846	8.948	0.000	185	249	QP

Note:

1. " * ", means this data is the worst emission level.
2. Measurement Level = Reading Level + Factor(Probe+Cable-Amp).


Limit: FCC_Part15.109_RE(3m)_ClassB	Margin: 0
Probe: CBL6112B_2931(30-1000MHz)	Polarity: Vertical
EUT: Hearing aids	Power: 120Vac / 60Hz
Note: BLE_1M Transmit at 2402MHz by DH5	

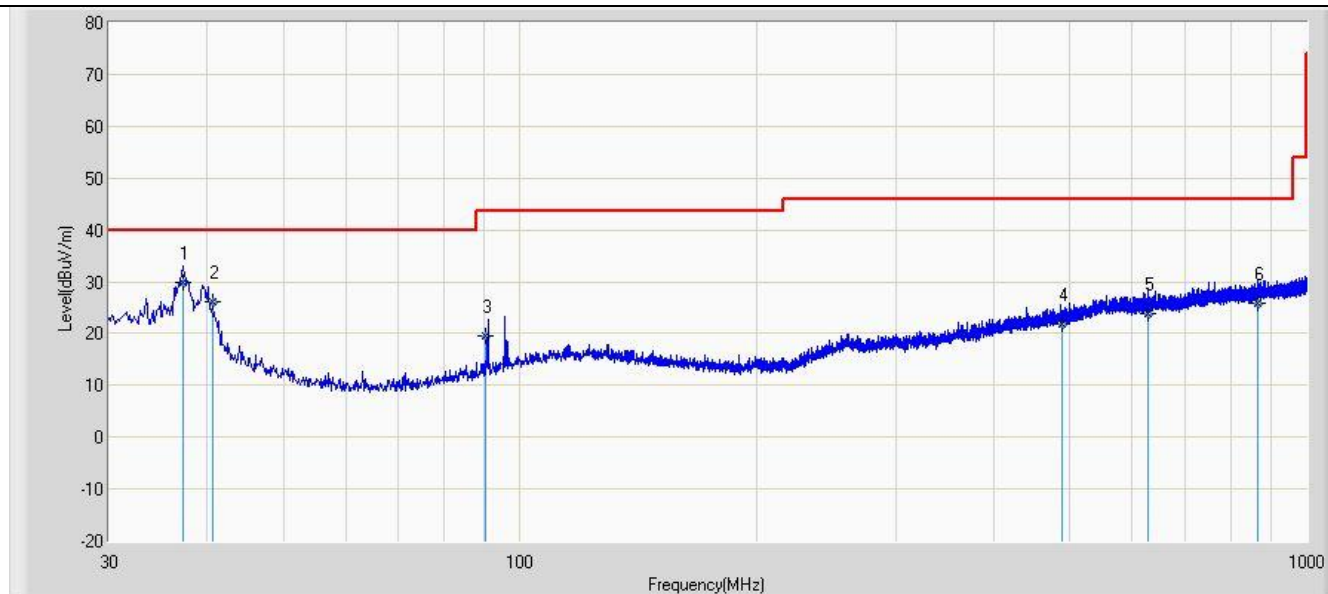

No	Mark	Frequency (MHz)	Measure Level (dBuV/m)	Reading Level (dBuV)	Over Limit (dB)	Limit (dBuV/m)	Probe (dB/m)	Cable (dB)	Amp (dB)	Ant Pos (cm)	Table Pos (deg)	Type
1	*	37.260	29.984	8.500	-10.016	40.000	15.098	6.386	0.000	122	131	QP
2		40.630	26.098	6.500	-13.902	40.000	13.195	6.404	0.000	258	82	QP
3		90.460	19.423	3.500	-24.077	43.500	9.230	6.693	0.000	260	16	QP
4		487.630	21.930	-3.500	-24.070	46.000	17.432	7.998	0.000	100	122	QP
5		627.630	23.933	-3.500	-22.067	46.000	19.089	8.343	0.000	226	124	QP
6		867.630	25.887	-3.500	-20.113	46.000	20.522	8.865	0.000	104	300	QP

Note:


1. " * ", means this data is the worst emission level.
2. Measurement Level = Reading Level + Factor(Probe+Cable-Amp).

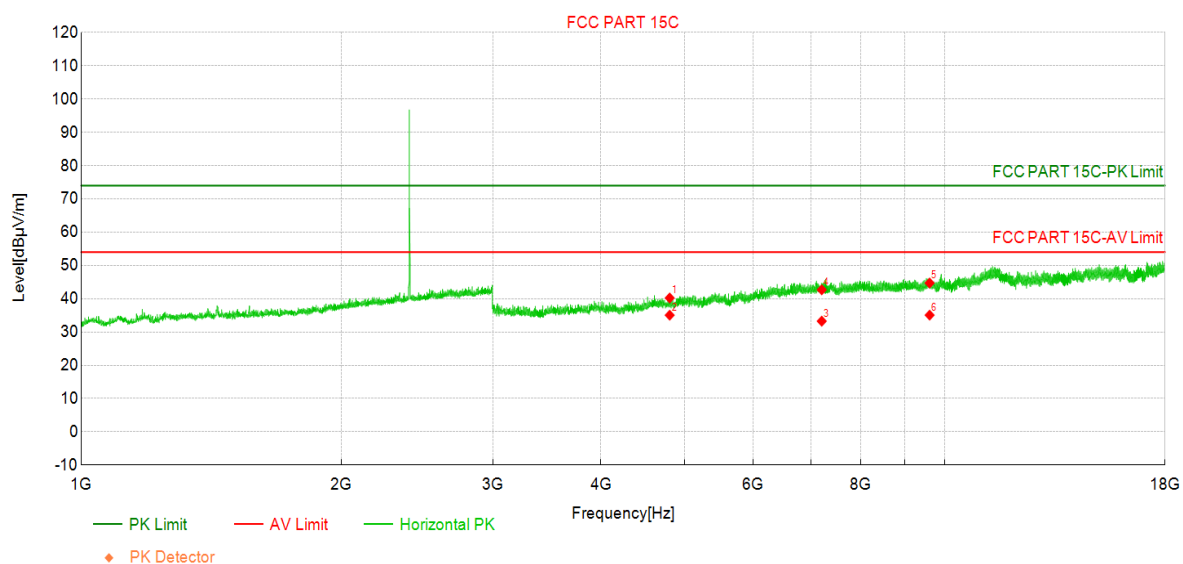Worst-case mode data check.**Left Ear****Transmit at 2402MHz by LE_1Mbps***Test Graph***Data List**

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	48.7	40.23	-8.480	74.00	33.77	PK	Horizo	PASS
2	4804.00	43.5	35.06	-8.480	54.00	18.94	AV	Horizo	PASS
3	7206.00	34.9	33.26	-1.620	54.00	20.74	AV	Horizo	PASS
4	7206.00	44.3	42.68	-1.620	74.00	31.32	PK	Horizo	PASS
5	9608.00	43.3	44.72	1.380	74.00	29.28	PK	Horizo	PASS
6	9608.00	33.7	35.07	1.380	54.00	18.93	AV	Horizo	PASS

Transmit at 2402MHz by LE_1Mbps


Test Graph

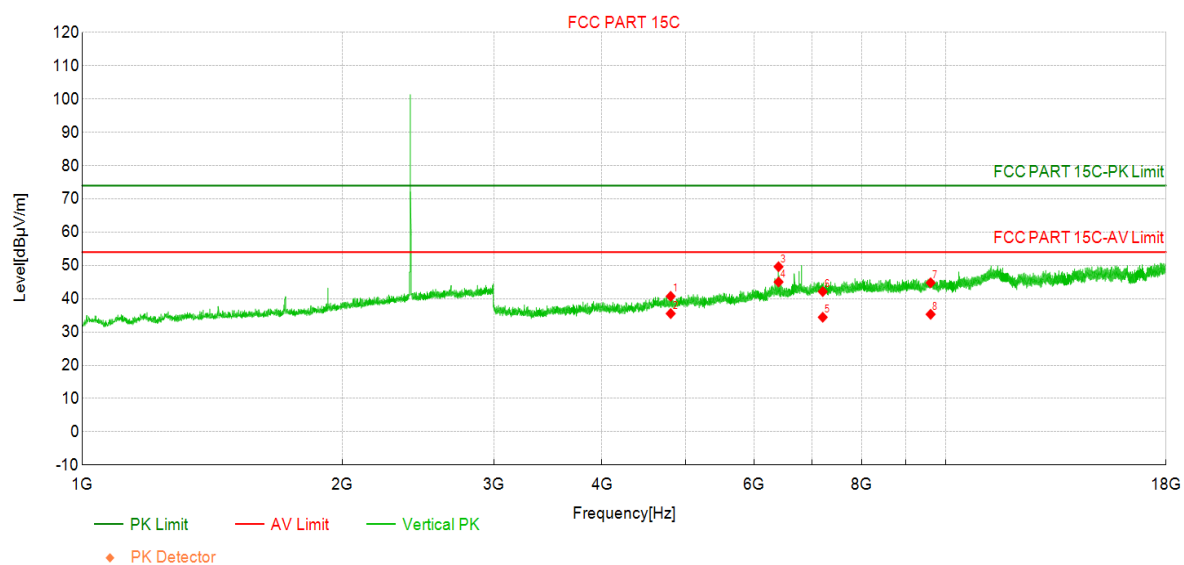

Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	49.2	40.73	-8.480	74.00	33.27	PK	Vertic	PASS
2	4804.00	44.0	35.53	-8.480	54.00	18.47	AV	Vertic	PASS
3	6405.00	52.3	49.62	-2.630	74.00	24.38	PK	Vertic	PASS
4	6405.75	47.7	45.04	-2.640	54.00	8.96	AV	Vertic	PASS
5	7206.00	36.0	34.42	-1.620	54.00	19.58	AV	Vertic	PASS
6	7206.00	43.8	42.15	-1.620	74.00	31.85	PK	Vertic	PASS
7	9608.00	43.4	44.79	1.380	74.00	29.21	PK	Vertic	PASS
8	9608.00	33.9	35.31	1.380	54.00	18.69	AV	Vertic	PASS

Transmit at 2402MHz by LE_1Mbps

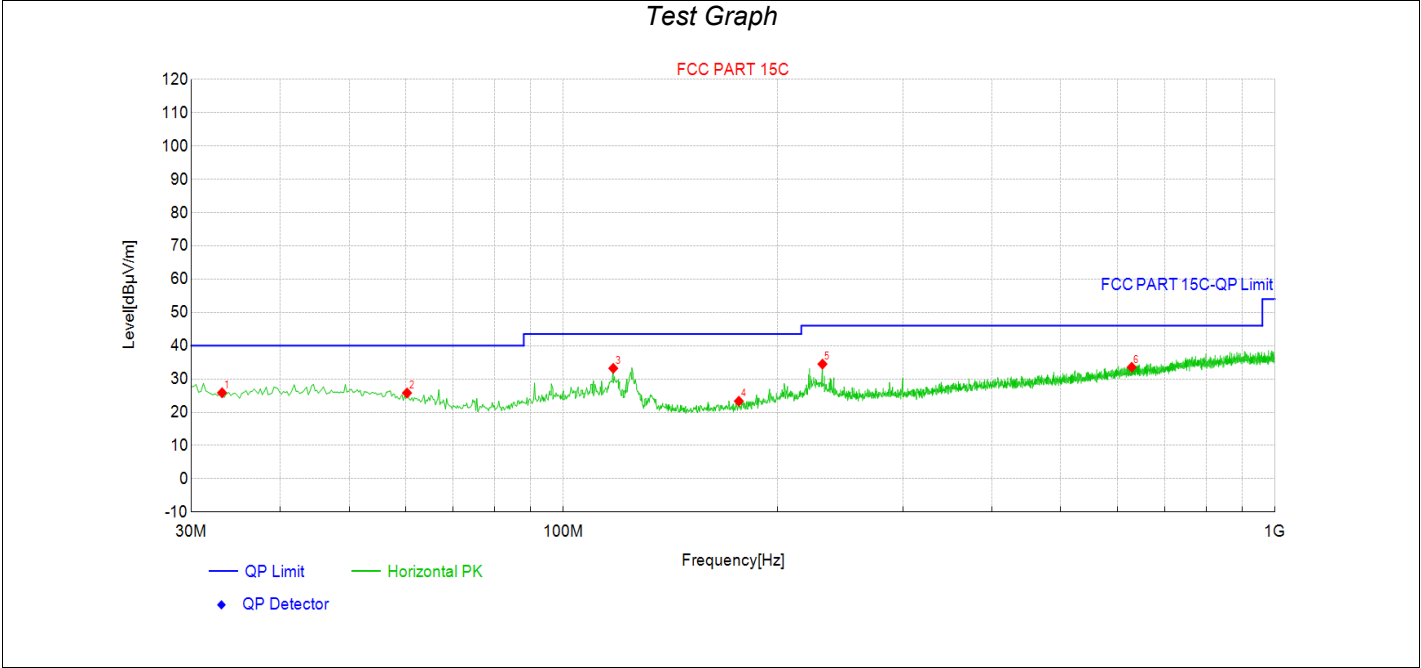


Data List

NO	Freque ncy [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdi ct
1	33.15	12.9	25.85	13.000	40.00	14.15	PK	Horizo	PASS
2	60.31	13.1	25.79	12.720	40.00	14.21	PK	Horizo	PASS
3	117.54	22.0	33.21	11.190	43.50	10.29	PK	Horizo	PASS
4	176.47	13.0	23.32	10.320	43.50	20.18	PK	Horizo	PASS
5	231.28	21.8	34.48	12.680	46.00	11.52	PK	Horizo	PASS
6	628.98	13.6	33.53	19.900	46.00	12.47	PK	Horizo	PASS


Transmit at 2402MHz by LE_1Mbps

Test Graph

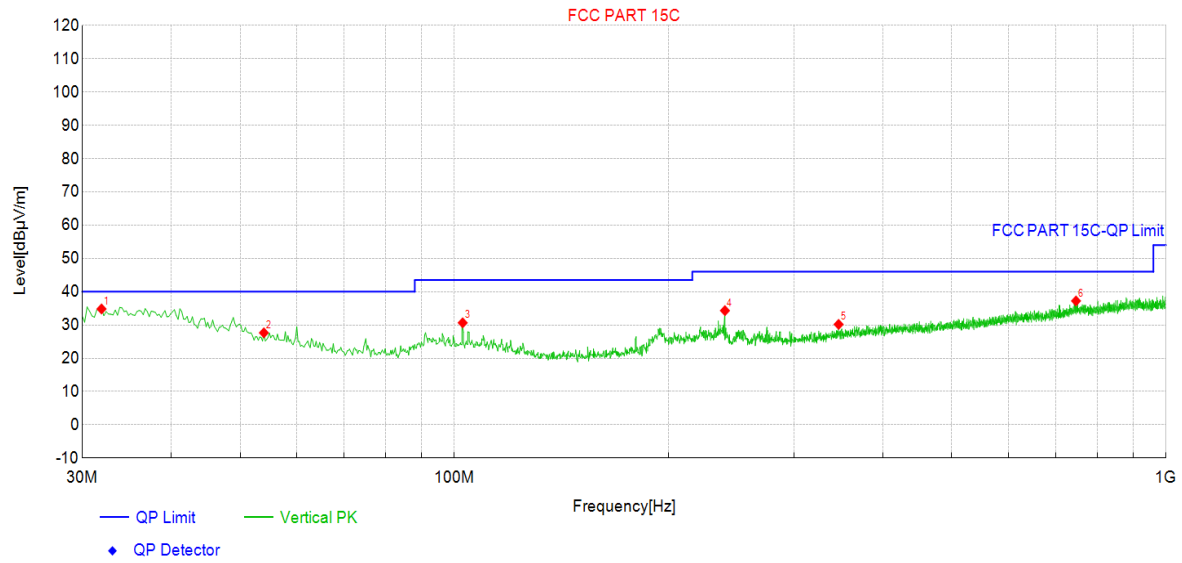

Data List


NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	31.94	21.9	34.82	12.970	40.00	5.18	PK	Vertic	PASS
2	54.01	13.6	27.65	14.100	40.00	12.35	PK	Vertic	PASS
3	102.75	18.2	30.66	12.460	43.50	12.84	PK	Vertic	PASS
4	240.01	21.4	34.32	12.930	46.00	11.68	PK	Vertic	PASS
5	346.71	14.9	30.18	15.320	46.00	15.82	PK	Vertic	PASS
6	747.32	15.8	37.23	21.430	46.00	8.77	PK	Vertic	PASS

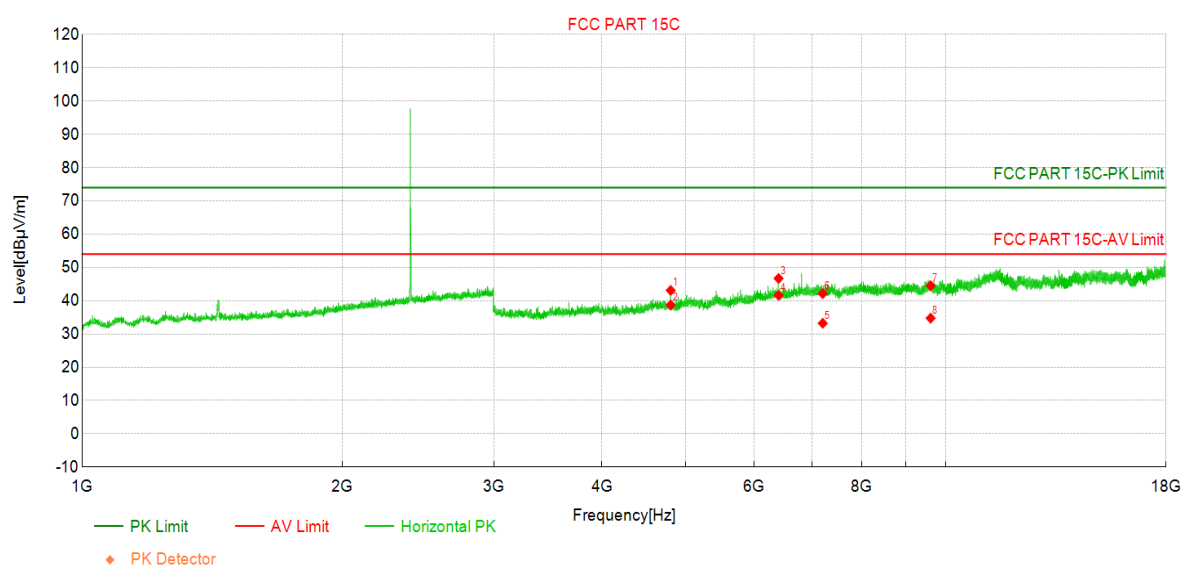Right Ear**Transmit at 2402MHz by LE_1Mbps****Test Graph****Data List**

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	51.6	43.12	-8.480	74.00	30.88	PK	Horizo	PASS
2	4804.00	47.2	38.73	-8.480	54.00	15.27	AV	Horizo	PASS
3	6405.00	49.3	46.69	-2.630	74.00	27.31	PK	Horizo	PASS
4	6405.75	44.3	41.62	-2.640	54.00	12.38	AV	Horizo	PASS
5	7206.00	34.9	33.23	-1.620	54.00	20.77	AV	Horizo	PASS
6	7206.00	43.7	42.12	-1.620	74.00	31.88	PK	Horizo	PASS
7	9608.00	43.1	44.51	1.380	74.00	29.49	PK	Horizo	PASS
8	9608.00	33.4	34.75	1.380	54.00	19.25	AV	Horizo	PASS

Transmit at 2402MHz by LE_1Mbps

Test Graph

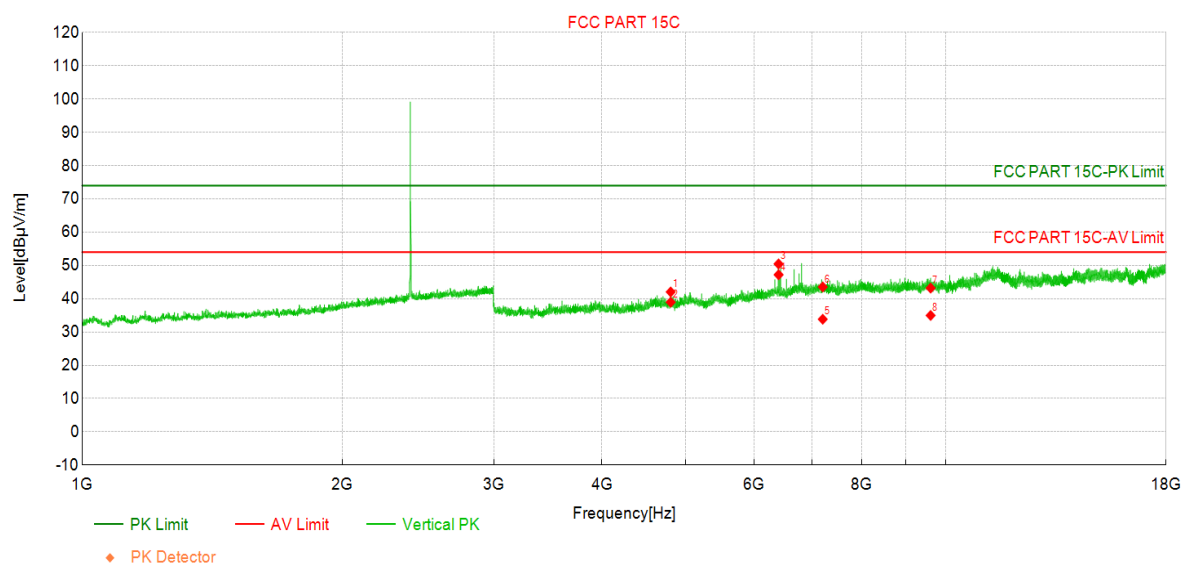


Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	4804.00	50.5	42.04	-8.480	74.00	31.96	PK	Vertic	PASS
2	4804.00	47.4	38.96	-8.480	54.00	15.04	AV	Vertic	PASS
3	6405.00	53.1	50.46	-2.630	74.00	23.54	PK	Vertic	PASS
4	6405.75	49.9	47.21	-2.640	54.00	6.79	AV	Vertic	PASS
5	7206.00	35.5	33.83	-1.620	54.00	20.17	AV	Vertic	PASS
6	7206.00	45.2	43.54	-1.620	74.00	30.46	PK	Vertic	PASS
7	9608.00	41.8	43.20	1.380	74.00	30.80	PK	Vertic	PASS
8	9608.00	33.6	34.97	1.380	54.00	19.03	AV	Vertic	PASS

Transmit at 2402MHz by LE_1Mbps

Test Graph

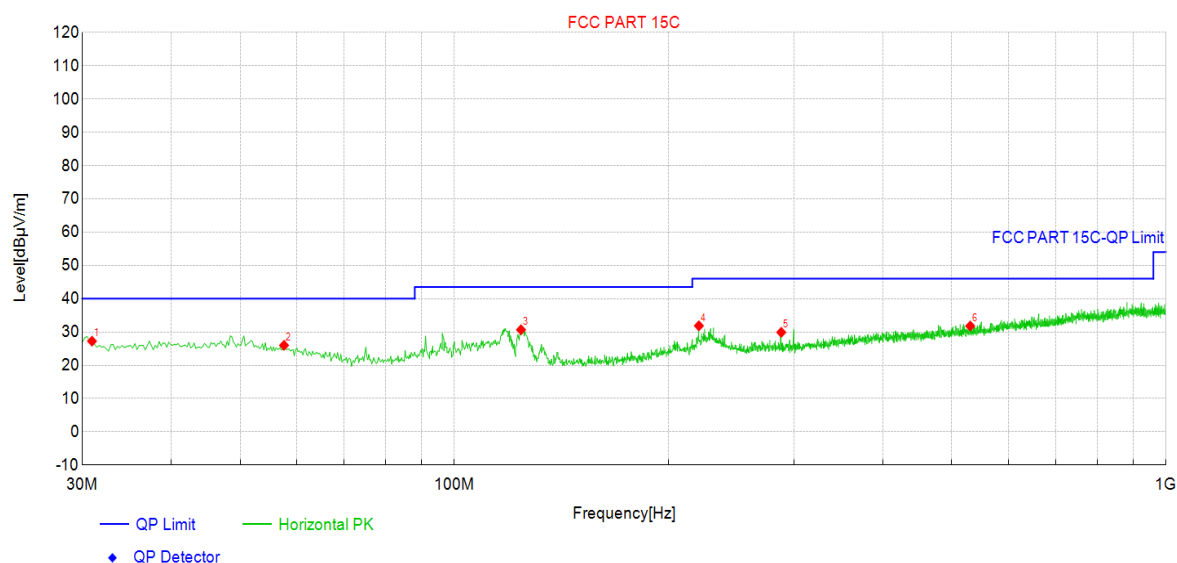


Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	30.97	14.3	27.23	12.940	40.00	12.77	PK	Horizo	PASS
2	57.65	12.7	25.99	13.310	40.00	14.01	PK	Horizo	PASS
3	124.09	20.3	30.66	10.330	43.50	12.84	PK	Horizo	PASS
4	220.61	19.5	31.86	12.360	46.00	14.14	PK	Horizo	PASS
5	288.02	16.1	29.89	13.800	46.00	16.11	PK	Horizo	PASS
6	530.76	13.7	31.79	18.080	46.00	14.21	PK	Horizo	PASS

Transmit at 2402MHz by LE_1Mbps

Test Graph

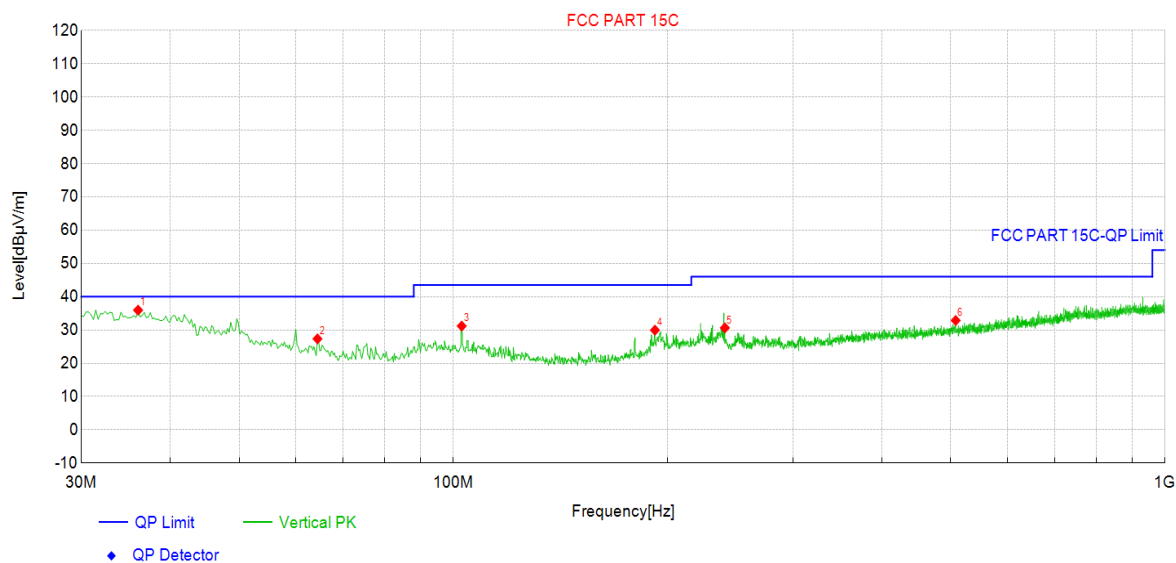

Data List

NO	Frequency [MHz]	Reading [dBμV]	Level [dBμV/m]	Factor [dB/m]	Limit [dBμV/m]	Margin [dB]	Det	Pol	Verdict
1	36.06	22.7	35.96	13.230	40.00	4.04	PK	Vertic	PASS
2	64.44	15.8	27.34	11.590	40.00	12.66	PK	Vertic	PASS
3	102.75	18.7	31.18	12.460	43.50	12.32	PK	Vertic	PASS
4	191.99	18.7	29.95	11.270	43.50	13.55	PK	Vertic	PASS
5	240.73	17.7	30.63	12.950	46.00	15.37	PK	Vertic	PASS
6	507.97	15.1	32.88	17.760	46.00	13.12	PK	Vertic	PASS

Note:

1. Level=Reading+Factor .


2. Margin=Limit-Level.

3. The test frequency range, 9kHz~30MHz, worst case are at least 20dB below the limits, therefore no data appear in the report.

4. The test frequency range, 18GHz~26GHz test result on peak is lower than average limit, all is the noise base, therefore no data appear in the report.

AC Power Line Conducted Emission

Limit: FCC_Part 15.107_CE_AC Power_Class B	Margin: 0
Probe: ENV216_101189(0.009-30MHz)	Polarity: Line
EUT: Hearing aids	Power: 120Vac / 60Hz
Note: BLE_1M Transmit at 2402MHz by DH5	

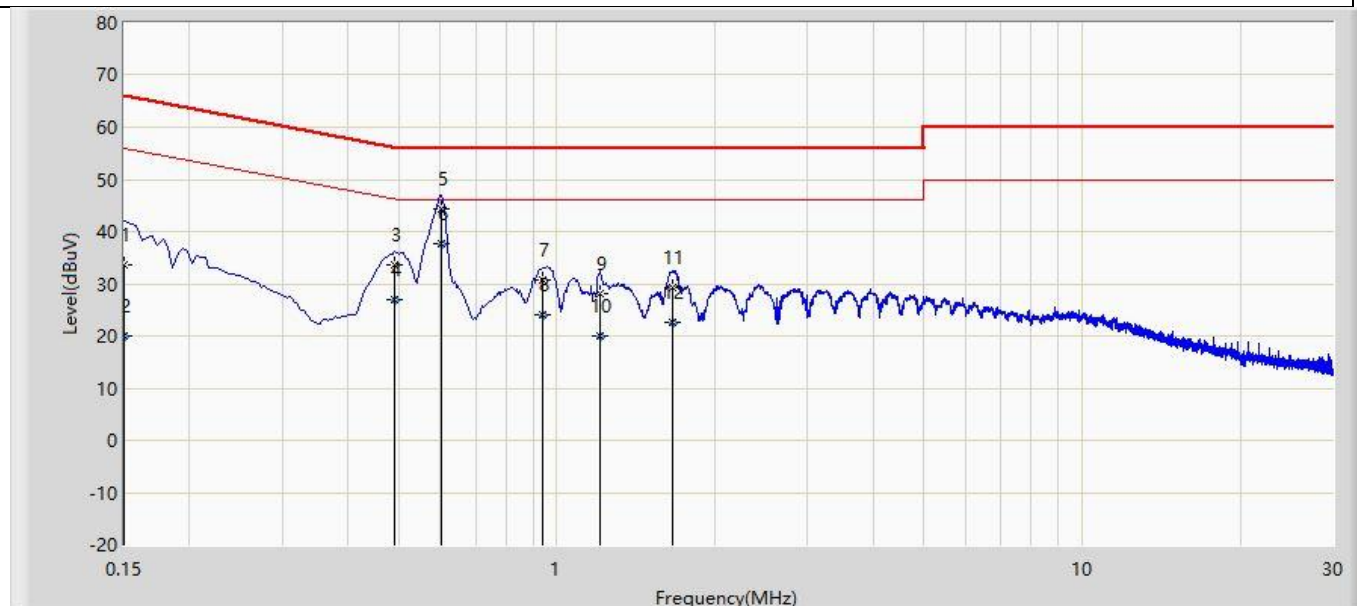


No	Mark	Frequency (MHz)	Measure Level (dBuV)	Reading Level (dBuV)	Over Limit (dB)	Limit (dBuV)	Probe (dB)	Cable (dB)	Amp (dB)	Type
1		0.150	33.714	24.089	-32.286	66.000	9.565	0.060	0.000	QP
2		0.150	20.142	10.517	-35.858	56.000	9.565	0.060	0.000	AV
3		0.490	33.593	23.957	-22.575	56.168	9.560	0.076	0.000	QP
4		0.490	26.844	17.209	-19.324	46.168	9.560	0.076	0.000	AV
5		0.602	44.351	34.709	-11.649	56.000	9.560	0.081	0.000	QP
6	*	0.602	37.550	27.909	-8.450	46.000	9.560	0.081	0.000	AV
7		0.938	30.836	21.170	-25.164	56.000	9.568	0.097	0.000	QP
8		0.938	24.050	14.385	-21.950	46.000	9.568	0.097	0.000	AV
9		1.210	28.072	18.396	-27.928	56.000	9.570	0.106	0.000	QP
10		1.210	19.936	10.260	-26.064	46.000	9.570	0.106	0.000	AV
11		1.662	29.298	19.611	-26.702	56.000	9.570	0.117	0.000	QP
12		1.662	22.475	12.788	-23.525	46.000	9.570	0.117	0.000	AV

Note:

1. " * ", means this data is the worst emission level.
2. Measurement Level = Reading Level + Factor(Probe+Cable-Amp).

Limit: FCC_Part 15.107_CE_AC Power_Class B	Margin: 0
Probe: ENV216_101189(0.009-30MHz)	Polarity: Neutral
EUT: Hearing aids	Power: 120Vac / 60Hz
Note: BLE_1M Transmit at 2402MHz by DH5	

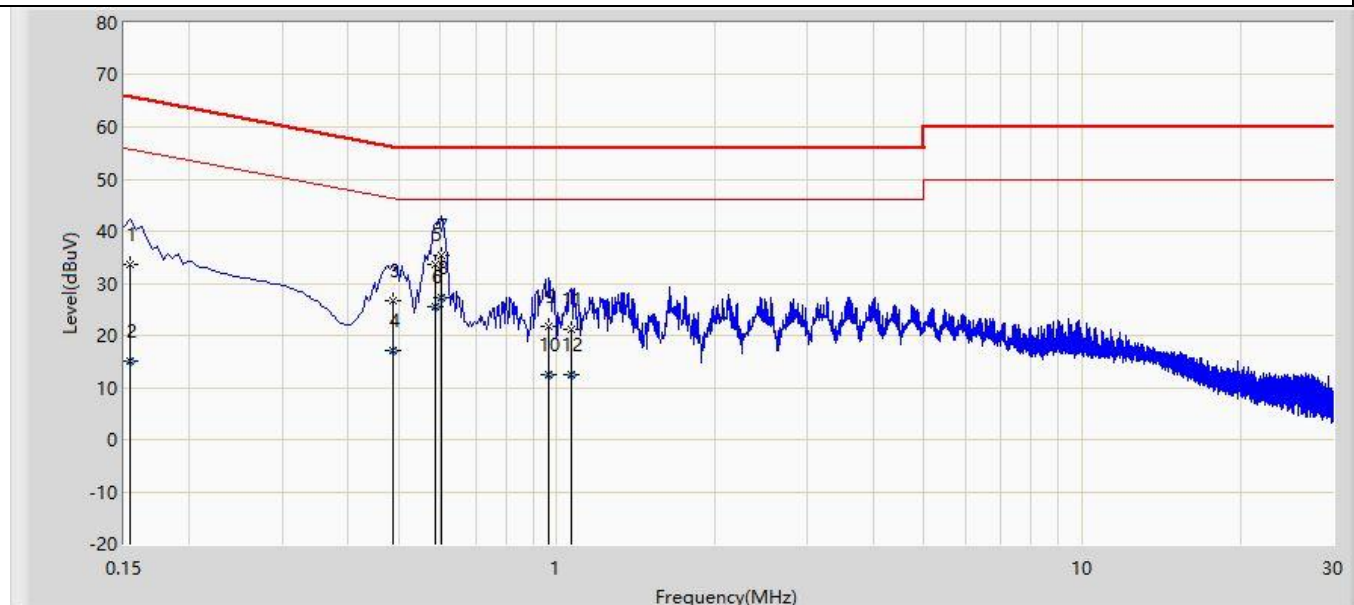

No	Mark	Frequency (MHz)	Measure Level (dBuV)	Reading Level (dBuV)	Over Limit (dB)	Limit (dBuV)	Probe (dB)	Cable (dB)	Amp (dB)	Type
1		0.154	33.625	23.995	-32.156	65.781	9.570	0.060	0.000	QP
2		0.154	15.119	5.489	-40.662	55.781	9.570	0.060	0.000	AV
3		0.486	26.714	17.068	-29.522	56.236	9.570	0.076	0.000	QP
4		0.486	17.184	7.539	-29.051	46.236	9.570	0.076	0.000	AV
5		0.586	33.673	24.022	-22.327	56.000	9.570	0.081	0.000	QP
6		0.586	25.433	15.783	-20.567	46.000	9.570	0.081	0.000	AV
7		0.602	35.245	25.594	-20.755	56.000	9.570	0.081	0.000	QP
8	*	0.602	27.111	17.460	-18.889	46.000	9.570	0.081	0.000	AV
9		0.966	21.602	11.934	-34.398	56.000	9.570	0.098	0.000	QP
10		0.966	12.387	2.718	-33.613	46.000	9.570	0.098	0.000	AV
11		1.066	21.144	11.473	-34.856	56.000	9.570	0.102	0.000	QP
12		1.066	12.358	2.687	-33.642	46.000	9.570	0.102	0.000	AV

Note:

1. " * ", means this data is the worst emission level.
2. Measurement Level = Reading Level + Factor(Probe+Cable-Amp).

The End