


Calibrated impedance: $47.44\Omega - 4.21j\Omega$; Measurement impedance: $48.59\Omega - 6.81j\Omega$ (within 5Ω)

Calibrated impedance: $47.44\Omega - 4.21j\Omega$; Measurement impedance: $48.59\Omega - 6.81j\Omega$ (within 5Ω)



Trc1 S11 Smith Ref 1 U

5.800000 GHz	48.591	Ω
	-j6.805	Ω
	4.032	pF

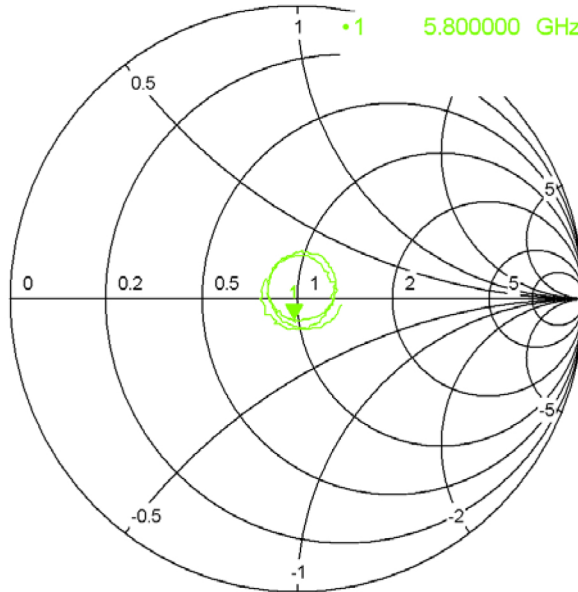

Ch1 Center 5.8 GHz

Pwr -10 dBm

Span 200 MHz


Date: 24.MAY.2024 11:15:47

Calibrated return loss: -26.14dB; Measurement return loss: -22.57dB(within 20%)



Trc1 S11 dB Mag 10 dB / Ref -20 dB

•1 5.800000 GHz -22.574 dB

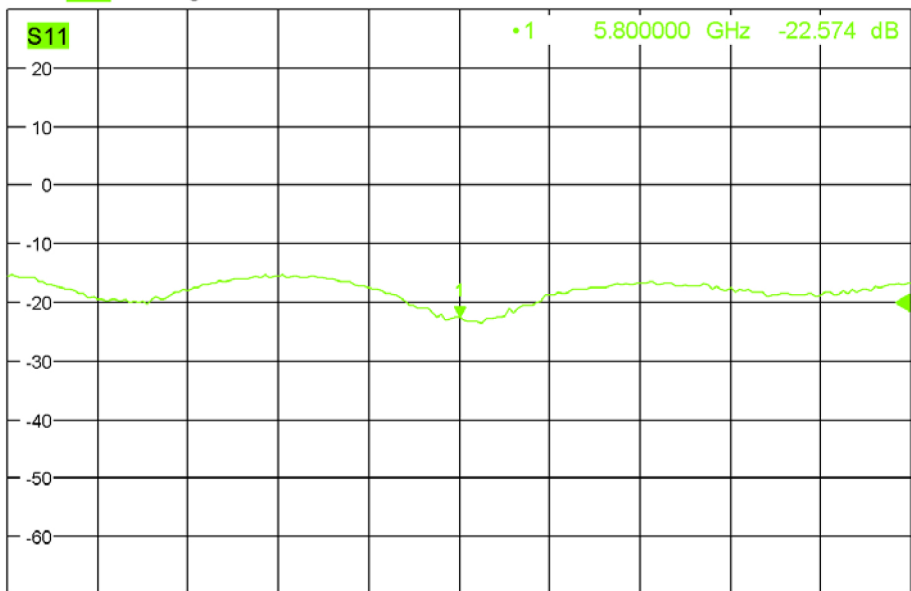

Ch1 Center 5.8 GHz

Pwr -10 dBm

Span 200 MHz

Date: 24.MAY.2024 11:14:59