



Impedance Plot for SN 29/15 DIP 2G450-393
2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $50.0\Omega + 5.0j\Omega$ (within 5Ω)

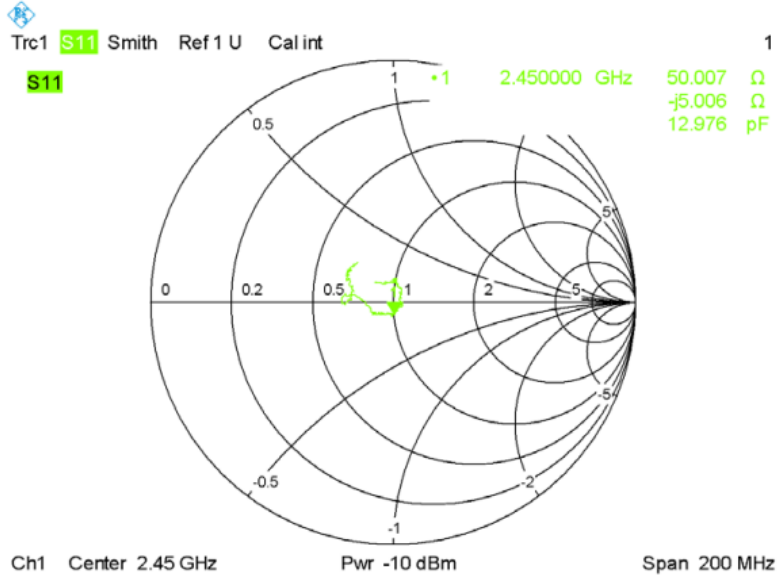

Date: 21.FEB.2024 19:04:50

Calibrated return loss: -27.80dB; Measurement return loss: -26.75dB (within 20%)

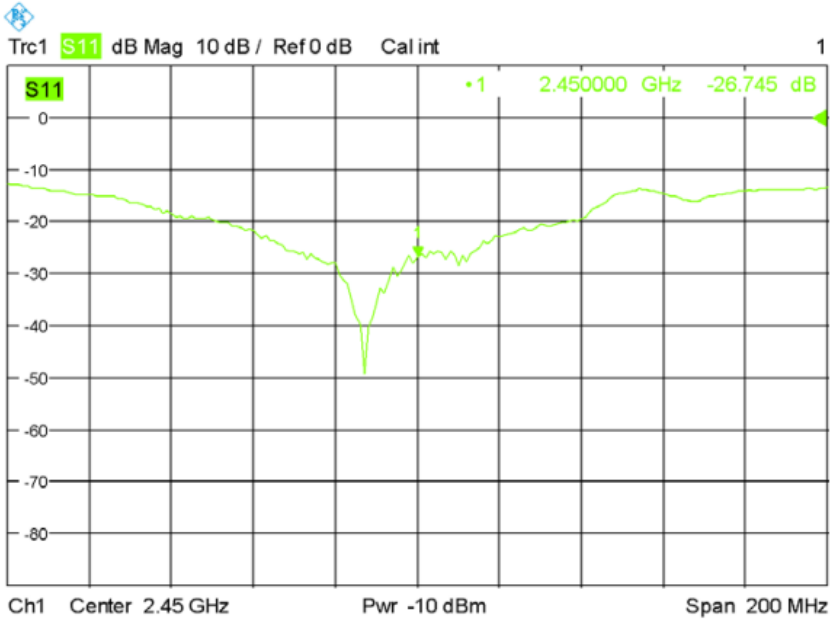

Date: 26.FEB.2024 19:28:46

5200 Head

S11

Span 200 MHz

Calibrated return loss: -20.52dB; Measurement return loss: -21.29dB(within 20%)



S11

Span 200 MHz

Date: 24.MAY.2024 11:08:53