

Technical documentation	Doc-id IZDOSE-PR-OTH-037	Pages 1(10)
Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6		Revision 05

DOSE

Labelling and Packaging Specification

Author, date 2023-03-02	Signature 	Clarification of signature Emma Widehäll
Approved, date 2023-03-02	Signature 	Clarification of signature Dean Minnock

Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	Doc-id IZDOSE-PR-OTH-037	Pages 2(10)
--	------------------------------------	-----------------------

CONTENTS

1	Introduction	3
1.1	Scope.....	3
1.2	Revision history.....	3
1.3	Definitions.....	3
1.4	References	3
2	Unique Label Identifier	4
3	Markings on the outside of the device – Device label	4
3.1	Elements on Device label	4
3.2	Device label size and layout	5
3.3	Label position	5
4	Information on the Packaging	6
4.1	Translations.....	6
4.2	Elements on Packaging label.....	6
4.3	Packaging label size and layout.....	8
5	Packaging details	10

Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	Doc-id IZDOSE-PR-OTH-037	Pages 3(10)
--	------------------------------------	-----------------------

1 Introduction

1.1 Scope

This report describes the labelling and packaging, for DOSE.

1.2 Revision history

<i>Version</i>	<i>Approved by</i>	<i>Approval date</i>	<i>Description</i>
01			First version
02			References corrected. Symbol for consulting IFU changed from the version in ISO 15223-1 to “the blue man”.
03	Dean Minnock	2022-12-23	Added FCC ID number
04	Dean Minnock	2023-01-10	Legal manufacturer address updated on labels. Label position added (chapter 3.3)
05	Dean Minnock	2023-02-23	Updated layout for LBL02 (v05) with separate sticker. Details added on printing and label content.
06		2023-03-02	Figures are updated with the V6 of the packaging label. Figure 3 is updated to include the printed label.

1.3 Definitions

<i>Term</i>	<i>Definition</i>

1.4 References

- [1] IZDOSE-LBL01 Device label
- [2] IZDOSE-LBL02 Packaging label
- [3] IZDOSE-PR-OTH-047 Packaging with print

2 Unique Label Identifier

The label issue shall be present on the label according to ISO 20417; paragraph 6.1.4 d). The unique label identifier is a combination of the identification number for the device – IZDOSE – the label identifier – LBLXX – and the version code – XX, starting at 01.

For DOSE there are two different labels, the device label and the packaging label. Below are the different unique label identifiers for DOSE labels presented. XX represents the version.

Table 1: Overview of Unique label identifiers for DOSE labels.

Label type	Unique label identifier
Device label	IZDOSE-LBL01-XX
Packaging label	IZDOSE-LBL02-XX

3 Markings on the outside of the device – Device label

3.1 Elements on Device label

The elements to be used on the outside of the device, i.e. on the device label, are presented in Table 2 below.

Table 2 Elements to include on the outside of the device.

Element	ISO 15223-1	Requirement	Comment
	5.1.1	IEC 60601-1, Clause 7.2.2	Manufacturer info (name, trademark, and address)
	5.1.6	IEC 60601-1, Clause 7.2.2	Type Reference or Model Version
	-	IEC 60601-1, Clause 7.2.2	Serial number. May be removed if lot or batch identifier is used.
	-	IEC 60601-1, Clause 7.2.2	The date of manufacture
	-	IEC 60601-1, Clause 7.2.3	Indicates the need for the user to consult the instructions for use. To be accompanied with URL for e-IFU.
		IEC 60601-1, Clause 7.2.6, 7.2.7	The RATED supply voltage, the nature of supply
FCC ID	-	47 CFR on FCC	Legal requirement in the US market

Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	Doc-id IZDOSE-PR-OTH-037	Pages 5(10)
--	------------------------------------	----------------

<i>Element</i>	<i>ISO 15223-1</i>	<i>Requirement</i>	<i>Comment</i>
	-	ISO 20417, Clause 6.5.2	WEEE, safe disposal information
GTIN	-		Global trade item number
	-		BLE ID
	-		Legal requirement on the EU market
IP 22	-	IEC 60601-1, Clause 7.2.9	IP classification

3.2 Device label size and layout

The measurements of the device label [1] is 48,3 mm wide and 8,5 mm high.

The device label, IZDOSE-LBL01 has a layout according to Figure 1.

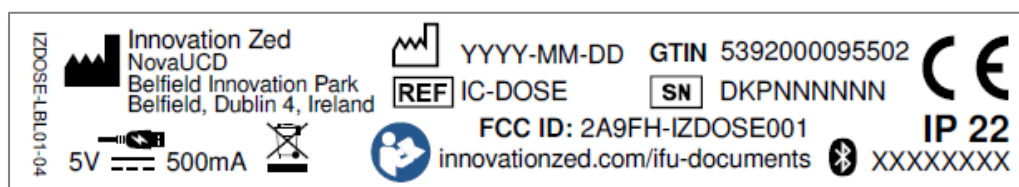


Figure 1: Label IZDOSE-LBL01-04

Some of the elements on the label are different depending on when the device is produced and specific device characteristics. These unique items are highlighted with yellow in Figure 2.

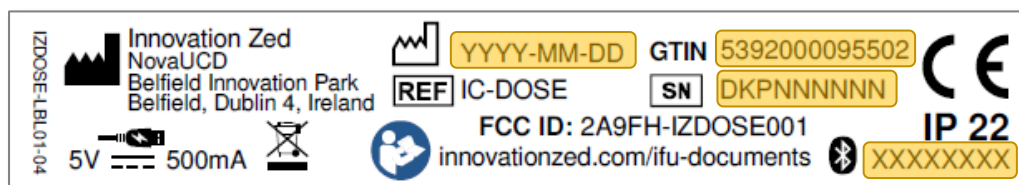


Figure 2: Unique items, based on manufacturing date and device characteristics.

3.3 Label position

The label is a sticker, fastened directly to the Dose device, with position and orientation according to Figure 3.

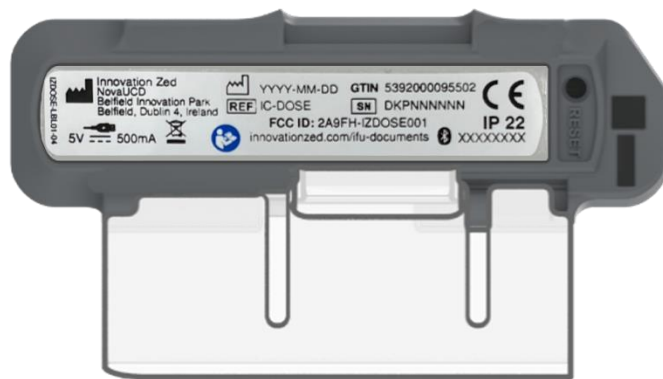


Figure 3: Position of the label on the device.

4 Information on the Packaging

The information elements to be established are presented below. In Section 4.3, an example of how the information may be incorporated in the label is shown.

4.1 Translations

Today there are no requirements on translations for the Dose device labels. However, if the device in the future becomes a Medical Device on the European market, all text strings on the label will require translations to local languages (according to GSPR 23.2b).


4.2 Elements on Packaging label

The elements to be used on the label are presented in Table 3 below.

Table 3 Elements to include on the label.

Element	ISO 15223-1	Requirement	Comment
	5.1.1	ISO 20417, Clause 6.5.1	Manufacturer info (name and address)
	5.1.3	ISO 20417, Clause 6.5.1	Indicates the date when the device was manufactured
	5.1.5	ISO 20417, Clause 6.5.1	Indicates the manufacturer's batch code so that the batch or lot can be identified
	5.1.6	ISO 20417, Clause 6.5.1	Indicates the manufacturer's Catalogue number so that the device can be identified
	5.1.7	ISO 20417, Clause 6.5.1	Indicates the manufacturer's serial number so that a specific device can be identified

Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	Doc-id IZDOSE-PR-OTH-037	Pages 7(10)
--	------------------------------------	-----------------------

<i>Element</i>	<i>ISO 15223-1</i>	<i>Requirement</i>	<i>Comment</i>
	5.2.8	IZDOSE-RMF-010	If the packaging is damaged, the manufacturer cannot ensure the full function of the device.
	5.3.2	ISO 20417, Clause 6.5.3	Indicates a device that needs protection from sunlight
	5.3.4	ISO 20417, Clause 6.5.3	Indicates a device that needs to be protected from moisture
	5.3.7	ISO 20417, Clause 6.5.3	Indicates the temperature limits to which the device can be safely exposed
	5.3.8	ISO 20417, Clause 6.5.3	Indicates the range of humidity to which the device can be safely exposed
	-	ISO 20417, Clause 6.1.5	Indicates the need for the user to consult the instructions for use. To be accompanied with URL for e-IFU.
	-	ISO 20417, Clause 6.5.2	WEEE, safe disposal information
Unique Device Identifier (UDI)	-	ISO 20417, Clause 6.5.1	Identifies the UDI carrier, including the AIDC and human readable information.
Necessary contraindications	-	ISO 20417, Clause 6.5.2	
Details necessary to identify the medical device and its use. (statement of intended use)	-	ISO 20417, Clause 6.1.3	
Commercial product name/ Name or trade name of the device	-	ISO 20417, Clause 6.1.3 and 6.5.1	
	-		Legal requirement on the EU market

Document name IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	Doc-id IZDOSE-PR-OTH-037	Pages 8(10)
--	------------------------------------	-----------------------

4.3 Packaging label size and layout

Some items on the label will be specific for each device (e.g. manufacturing date), and to handle this within production, the packaging label is created in two steps. One step is to print the consistent information on the packaging using the layout file Packaging with Print [3] and the second step is to print the device specific information on a small sticker using the layout file Packaging Label [2], and this sticker will be added to the package afterwards, see Figure 4. For a correct placement of the sticker, a grey area is printed in the first step, which the sticker should be added on top of, covering it entirely, see Figure 5.

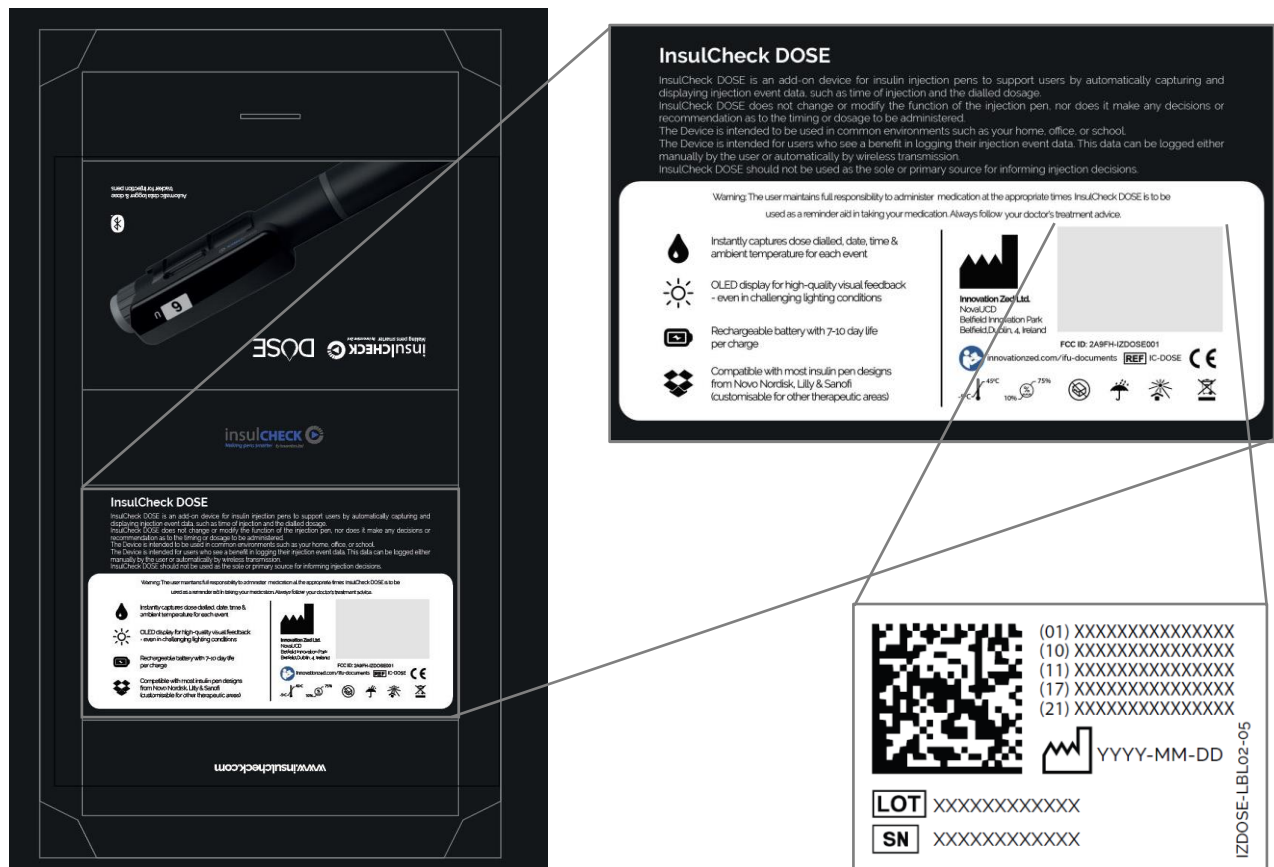


Figure 4: The packaging print with the packaging label integrated. Some information is printed on a separate sticker.

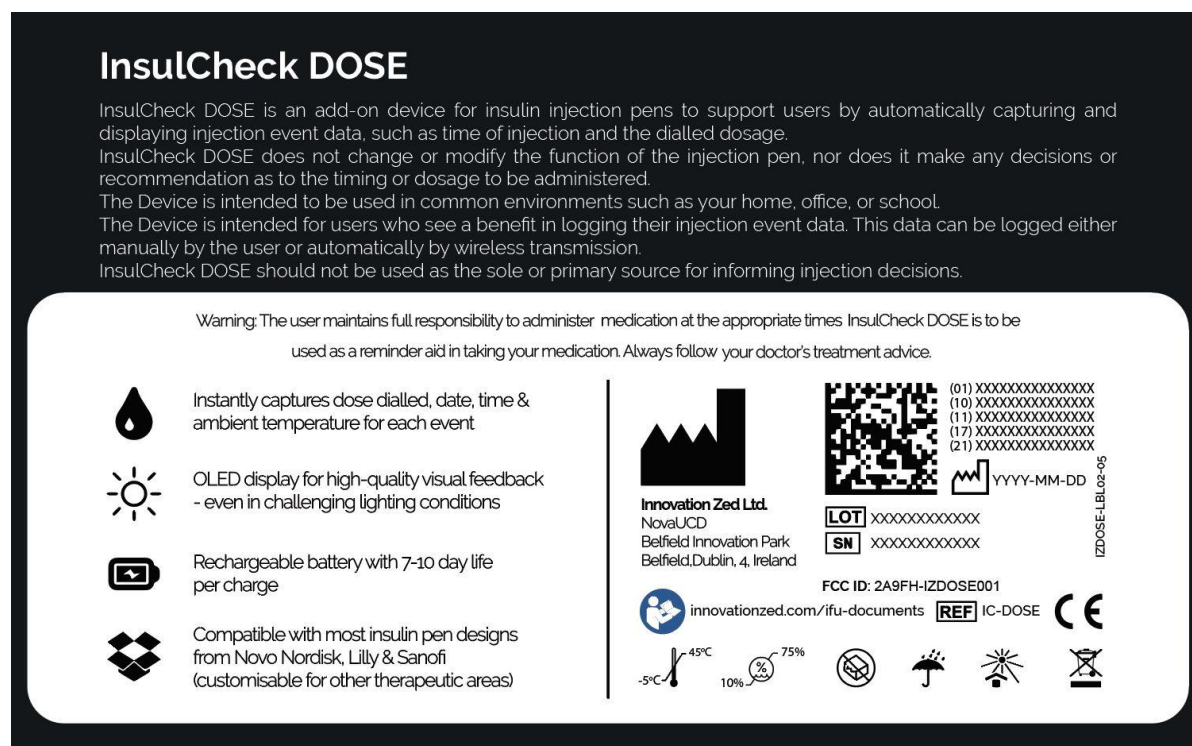


Figure 5: The packaging print after the sticker is added on top of the grey area

The separate sticker, IZDOSE-LBL02, contains the fields with date and device specific information. This date and device specific information is explained in Figure 6.

The size of IZDOSE-LBL02 is 46x30 mm, and it is positioned on the packaging according to Figure 4.

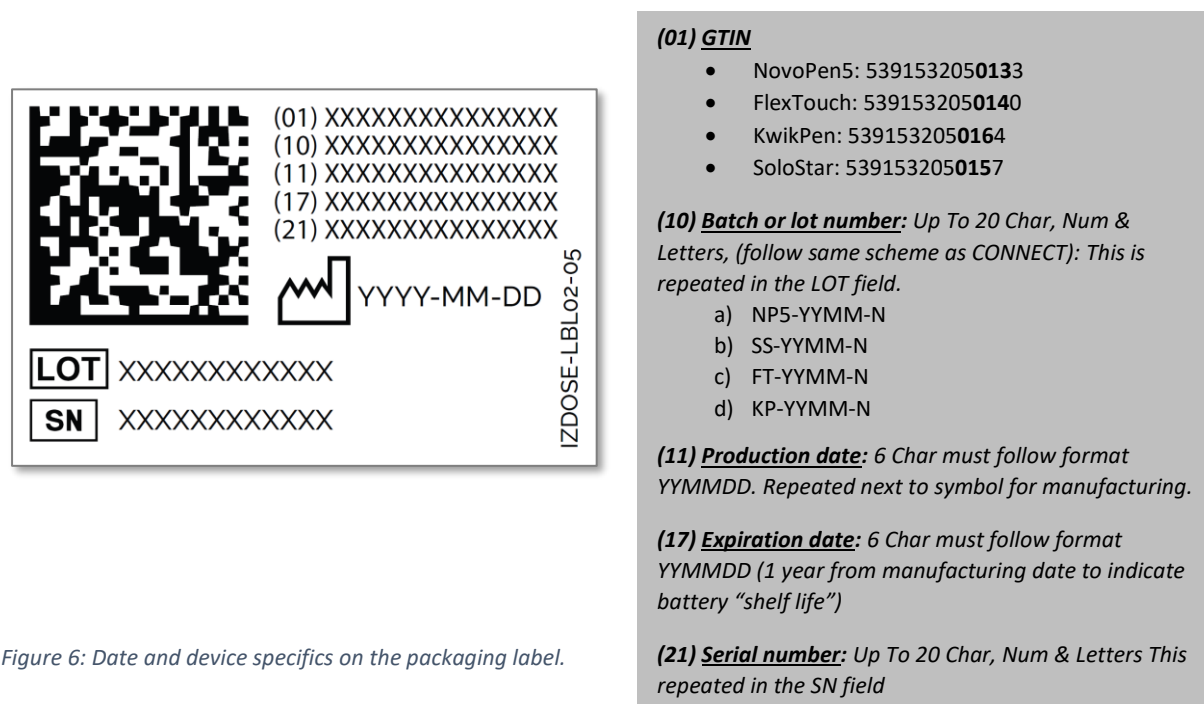


Figure 6: Date and device specifics on the packaging label.

Document name	Doc-id	Pages
IZDOSE-PR-OTH-037 Labelling and Packaging Specification v6	IZDOSE-PR-OTH-037	10(10)

5 Packaging details

The packaging for DOSE is a printed cardboard box according to Packaging with print [3]. This file also specifies dimensions of the packaging.

The Packaging label is included in the box print as described in Section 4.