RADIO REPORT

FCC 47 CFR Part 15C

Digital transmission systems operating within the 2400.0 MHz - 2483.5 MHz band

Report Reference No	G0M-2112-1231-TFC247WF-V02
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	DAkkS - Registration number : D-PL-12092-01-04 (FCC) FCC Filed Test Laboratory, Reg.-No.: 96970
Applicant	eResearchTechnology GmbH
Address	Sieboldstrasse 3 97230 Estenfeld Germany
Test Specification	47 CFR Part 15C
Non-Standard Test Method	None
Equipment under Test (EUT):	
Product Description	Spirometer System
Model(s)	SpiroSphere
Additional Model(s)	None
Brand Name(s)	None
Hardware Version(s)	N7 (12.07.06)
Software Version(s)	SpiroSpherePackage V4.6.5 Jet_Lib + TestAPP 1.0.0
FCC ID	2AAUFSPS003
Test Result	**PASSED**

Possible test case verdicts:		
Required by standard but not tested	N/T	
Not required by standard	N/R	
Not applicable to EUT	N/A	
Test object does meet the requirement	P(PASS)	
Test object does not meet the requirement	F(FAIL)	
Testing:		
Test Lab Temperature	20 °C - 30 °C	
Test Lab Humidity	25 % - 55 %	
Date of receipt of test item	2022-02-03	
Report:		
Compiled by	Odai Qawasmeh	
Tested by (+ signature) (Responsible for Test)	Radwan Jaafar	.....
Approved by (+ signature) (Test Lab Engineer)	Wilfried Treffke	W. Treff .....
Date of Issue	2022-09-27	
Total number of pages	33	
General Remarks:		
The test results presented in this report relate only to the object tested. **The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.** This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.		
Additional Comments:		

VERSION HISTORY

Version History			
Version	Issue Date	Remarks	Revised By
01	2022-05-16	Initial Release	
02	2022-09-27	Replaced document: G0M-2112-1231-TFC247WF-V01 Replaced by: G0M-2112-1231-TFC247WF-V02 Reason: - Reference Module test report is added to the clause Test modes. - HW and SW Version changed - Delete ISED (Canada) relevant tests and information. This report version (V02) shall be applicable for FCC (USA) certification only.	R. Jaafar

ABBREVIATIONS AND ACRONYMS

Acronyms	
Acronym	Description
BPSK	Binary Phase Shift Keying
DSSS	Direct Sequence Spread Spectrum
EUT	Equipment Under Test
FCC	Federal Communications Commission
HT	High Throughput
IEEE 802.11	MAC and PHY Layer for WiFi
ISED	Innovation, Science and Economic Development Canada
OFDM	Orthogonal Frequency Division Multiplexing
QAM	Quadrature Amplitude Modulation
QPSK	Quadrature Phase Shift Keying
RBW	Resolution bandwidth
RMS	Root mean square
VBW	Video bandwidth
V_{NOM}	Nominal supply voltage

REPORT INDEX

1 Equipment (Test Item) Under Test 6
1.1 Photos – Equipment External 7
1.2 Photos – Equipment Internal 9
1.3 Support Equipment 12
1.4 Test Modes 13
1.5 Test Frequencies 14
1.6 Sample emission level calculation 15
2 Result Summary 16
3 Test Conditions and Results 17
3.1 Test Conditions and Results - AC powerline conducted emissions 17
3.2 Test Conditions and Results - Transmitter radiated emissions 21

ANNEX A Transmitter spurious emissions 27

1 Equipment (Test Item) Under Test

Description	Spirometer System	
Model	SpiroSphere	
Additional Model(s)	None	
Brand Name(s)	None	
Serial Number(s)	SN: 10010003 Test Sample ID 38262	
Hardware Version(s)	N7 (12.07.06)	
Software Version(s)	SpiroSpherePackage V4.6.5 Jet_Lib + TestAPP 1.0.0	
FCC ID	2AAUFSPS003	
Equipment type	End Product	
Radio type	Transceiver	
Assigned frequency bands	2400.0 MHz - 2483.5 MHz	
Radio technology	IEEE 802.11 b/g/n (HT20 + HT40)	
Modulation	BPSK, QPSK, 16-QAM, 64-QAM	
Number of antenna ports	2	
Radio Module	Type	WiFi/Bluetooth module
	Model	WL18 MODGB
	Manufacturer	Texas Instruments
	HW Version	Rev. N
	SW Version	F-Rev 8.8.0.0.13 P-Rev 8.2.0.0.195
	FCC-ID	Z64-WL18SBMOD
Antenna (1 & 2)	Type	Integrated antenna
	Model	ANT016008LCD2442MA1
	Manufacturer	TDK
	Gain	2.4 dBi
Supply Voltage	V_{NOM}	120 VAC
Operating Temperature	T_{NOM}	25 °C
AC/DC-Adaptor	Model	GTM91099-3009-4.0-T2
	Vendor	GlobTek
	Input	100 to 240VAC /50/60Hz
	Output	5 VDC
Manufacturer	eResearchTechnology GmbH Sieboldstrasse 3 97230 Estenfeld Germany	

1.1 Photos – Equipment External

EUT Top View

EUT Bottom View

EUT Ports

EUT Side View (left)

EUT Side View (right)

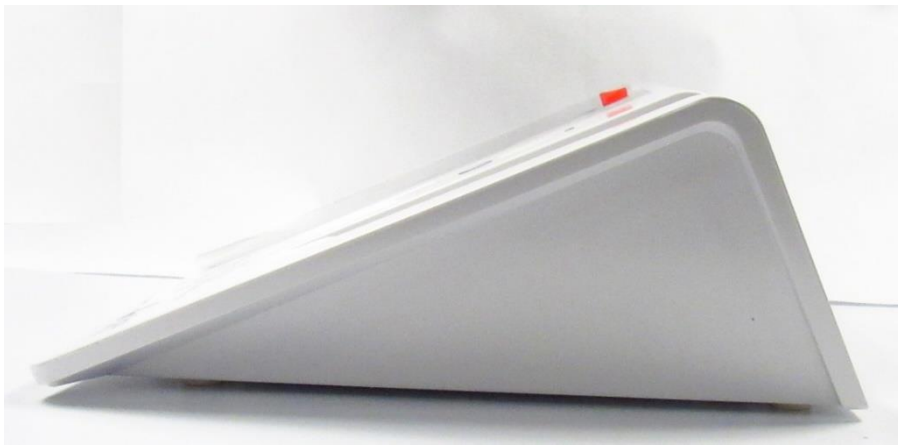

1.2 Photos – Equipment Internal

EUT PCB FINGERPRINT SWITCH

EUT PCB MAINBOARD
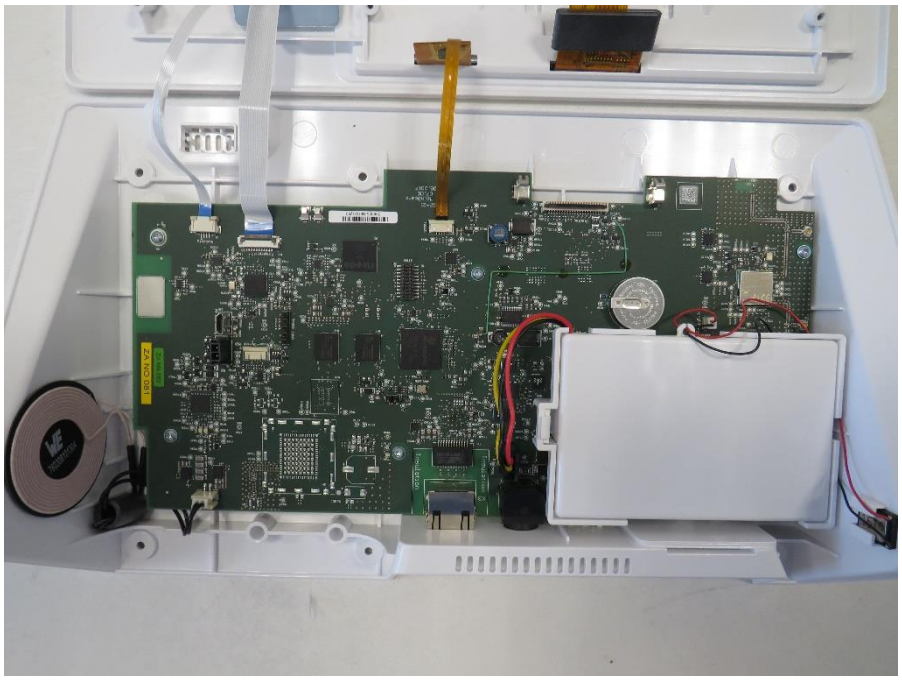

EUT PCB MAINBOARD FOCUS 1
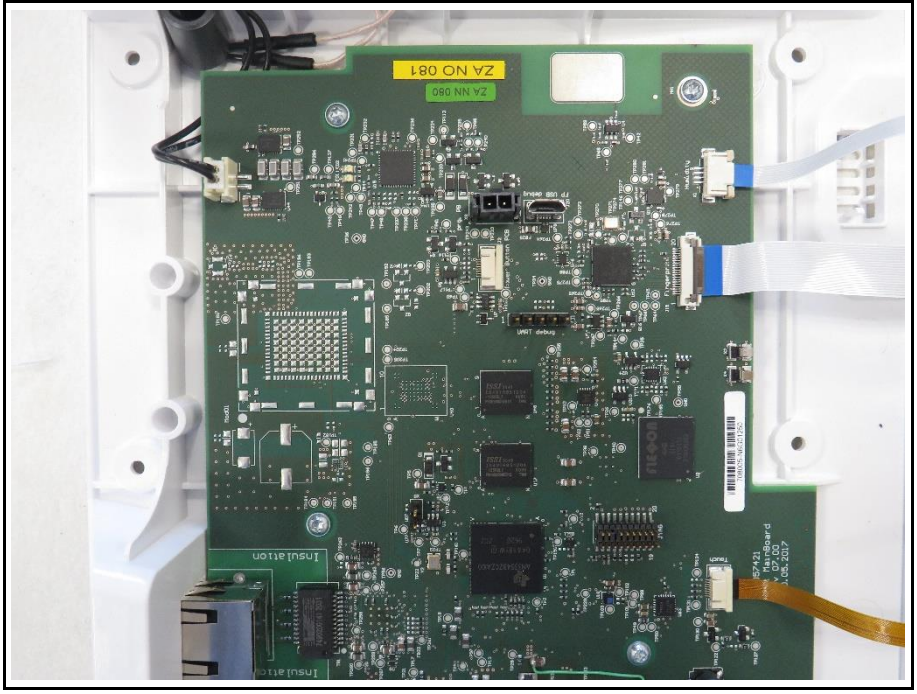

EUT PCB MAINBOARD FOCUS 2

EUT WITH OPEN COVER

EUT WITH OPEN COVER FOCUS

1.3 Support Equipment

Product Type	Device	Manufacturer	Model	Comment
AE	Medical ITE Power Supply	GlobTek	GTM91099-3009-4.0-T2	Medical Grad Wall-plug
CBL	WiFi-BT Stecker	-	-	USB to WiFi-BT connecter
SFT	Laptop	Dell	DELT0671	With control SW: HTCI tester for BT and RTTT for WiFi
Description:				
AE	Auxiliary Equipment			
SIM	Simulator			
CBL	Connecting Cable			
SFT	Software			
Comment:				

1.4 Test Modes

Mode	Description
OFDM (IEEE 802.11n)	Mode = Transmit Modulation = BPSK Spreading = OFDM Channel = 6 (2437 MHz) Bandwidth = 20 MHz Duty cycle = 100% Power setting = 19 dBm Data rate = MCS12
Comment: The above settings were found as worst case by evaluation of the original radio module test report FR741320C issued by Sporton International Inc. on Feb. 07, 2018. Determination of worst case is based on peak conducted output power from the original test report.	

1.5 Test Frequencies

Designator	Mode	Channel	Frequency [MHz]
F1	Tx	1	2412
F2	Tx	6	2437
F3	Tx	11	2462

1.6 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dBµV. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

Reading on Analyzer (dBµV) + A.F. (dB/m) = Net field strength (dBµV/m)

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dBµV/m). The FCC limits are given in units of µV/m. The following formula is used to convert the units of µV/m to dBµV/m:

Limit (dBµV/m) = 20*log (µV/m)

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

Reading + AF	= Net Reading	:	Net reading - FCC limit	= Margin
+21.5 dBµV + 26 dB/m	= 47.5 dBµV/m	:	47.5 dBµV/m - 57.0 dBµV/m	= -9.5 dB

2 Result Summary

FCC 47 CFR Part 15C				
Product Standard Reference	**Requirement**	**Reference Method**	**Result**	**Remarks**
FCC § 15.247(a)(2)	6 dB Bandwidth	ANSI C63.10-2013	N/T	Note 1
FCC § 15.247(b)	Maximum peak conducted power	ANSI C63.10-2013	N/T	Note 1
FCC § 15.247(e)	Power spectral density	ANSI C63.10-2013	N/T	Note 1
FCC § 15.207	AC power line conducted emissions	ANSI C63.10-2013	PASS	Note 1
FCC § 15.247(d)	Band edge compliance	ANSI C63.10-2013	N/T	Note 1
FCC § 15.247(d)	Conducted spurious emissions	ANSI C63.10-2013	N/T	Note 1
FCC § 15.247(d) FCC § 15.209	Transmitter radiated spurious emissions	ANSI C63.10-2013	PASS	Note 1
Note 1: Due to the integration of a pre-certified module, only partial and spot check tests were performed with reference to the original test report FR741320C issued by Sporton International Inc. on Feb. 07, 2018.				
Comment: The Decision Rule is applied on the basis of ETSI TR 102 273 and ETSI TR 100 028. These standards provide guidance on how to calculate and apply measurement uncertainty whilst providing maximum uncertainties allowance. In all cases due consideration will be given to ILAC-G8:09/2019. Where a result is considered conditional in respect of its proximity to the limit line, the customer would be made aware of situation so that they can make an informed decision on how to proceed.				

Possible Test Case Verdicts	
PASS	Test object does meet the requirements
FAIL	Test object does not meet the requirements
N/T	Required by standard but not tested
N/R	Not required by standard for the test object

3 Test Conditions and Results

3.1 Test Conditions and Results - AC powerline conducted emissions

3.1.1 Information

Test Information	
Reference	FCC § 15.207
Measurement Method	ANSI C63.10 6.2
Measurement Uncertainty	± 3.82 dB
Operator	Odai Qawasmeh
Date	2022-03-18

3.1.2 Limits

Limits		
Frequency [MHz]	Quasi-Peak [dBµV]	Average [dBµV]
0.15 - 0.5	66 - 56*	56 - 46*
0.5 - 5	56	46
5 - 30	60	50
* Limit decreases linearly with the logarithm of the frequency		

3.1.3 Setup

Test Setup

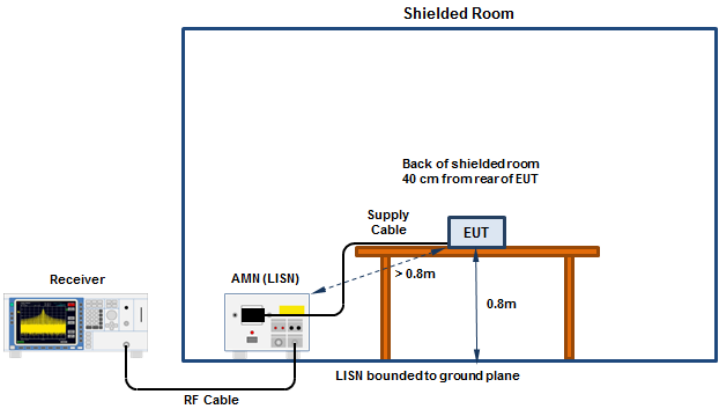

3.1.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2020.1.8

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
EMI Test Receiver	R&S	ESR7	EF00943	2021-08	2022-08
Pulse Limiter	R&S	ESH3-Z2	EF01222	2021-07	2022-07
LISN	Schwarzbeck	NSLK 8127 RC	EF01592	2021-07	2022-07

3.15 Setup Photos

Setup for measurement 150 kHz – 30 MHz

Setup for measurement 150 kHz – 30 MHz

Conducted emissions at the mains power port according to 47 CFR § 15.207

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Qawasmeh
Test Date:	2022-03-18
Operating Conditions:	ambient temperature: 20 °Celsius power input:
LISN:	Schwarzbeck NSLK 8127 RC L
Operational Mode:	IEEE 802.11, HT20, MCS12, 2437 Mhz
EUT Configuration:	
Applied to Port:	AC/DC Adapter to EUT (120V/60Hz to 5 VDC)
Note 1:	

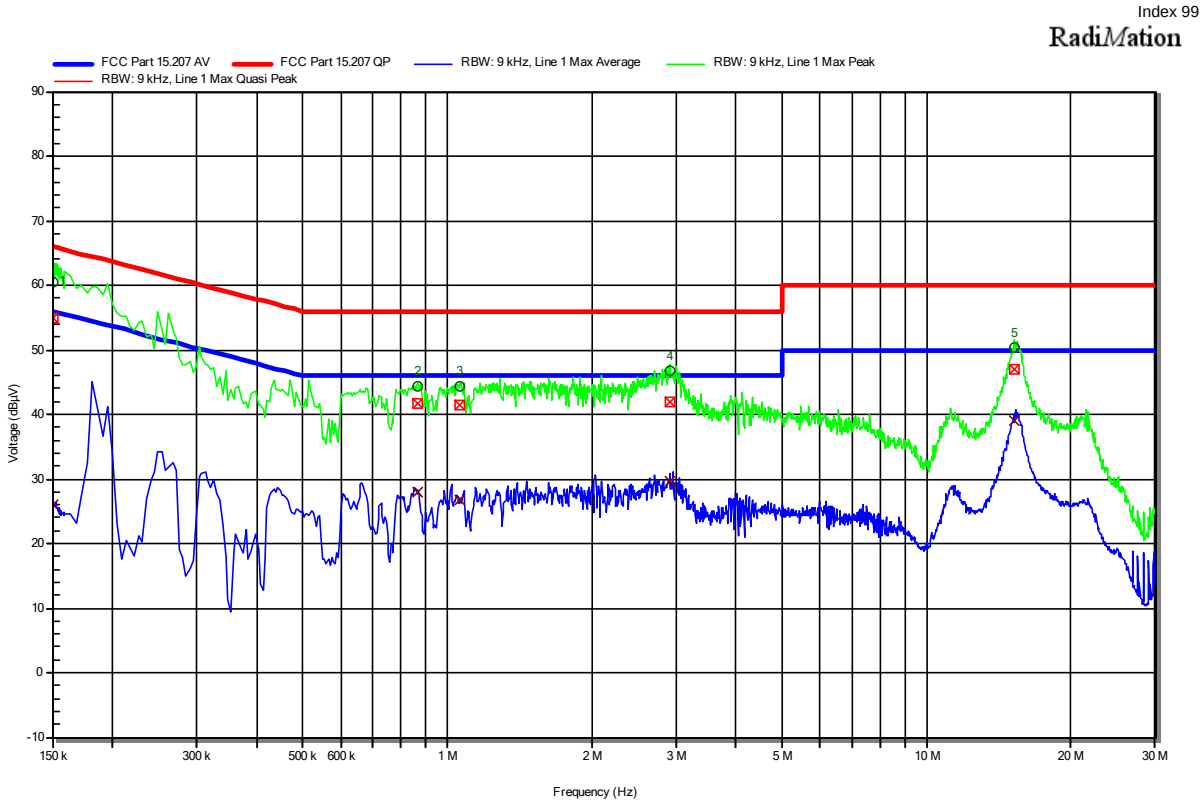

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	LISN
1	150 kHz	54.84 dBµV	66 dBµV	-11.16 dB	Pass	Line 1
2	865.5 kHz	41.57 dBµV	56 dBµV	-14.43 dB	Pass	Line 1
3	1.063 MHz	41.48 dBµV	56 dBµV	-14.52 dB	Pass	Line 1
4	2.918 MHz	41.93 dBµV	56 dBµV	-14.07 dB	Pass	Line 1
5	15.284 MHz	47.08 dBµV	60 dBµV	-12.92 dB	Pass	Line 1

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	LISN
1	150 kHz	25.92 dBµV	56 dBµV	-30.08 dB	Pass	Line 1
2	865.5 kHz	27.96 dBµV	46 dBµV	-18.04 dB	Pass	Line 1
3	1.063 MHz	26.67 dBµV	46 dBµV	-19.33 dB	Pass	Line 1
4	2.918 MHz	29.53 dBµV	46 dBµV	-16.47 dB	Pass	Line 1
5	15.284 MHz	39.07 dBµV	50 dBµV	-10.93 dB	Pass	Line 1

Conducted emissions at the mains power port according to 47 CFR § 15.207

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Qawasmeh
Test Date:	2022-03-18
Operating Conditions:	ambient temperature: 20 °Celsius power input:
LISN:	Schwarzbeck NSLK 8127 RC N
Operational Mode:	IEEE 802.11, HT20, MCS12, 2437 Mhz
EUT Configuration:	
Applied to Port:	AC/DC Adapter to EUT (120V/60Hz to 5 VDC)
Note 1:	

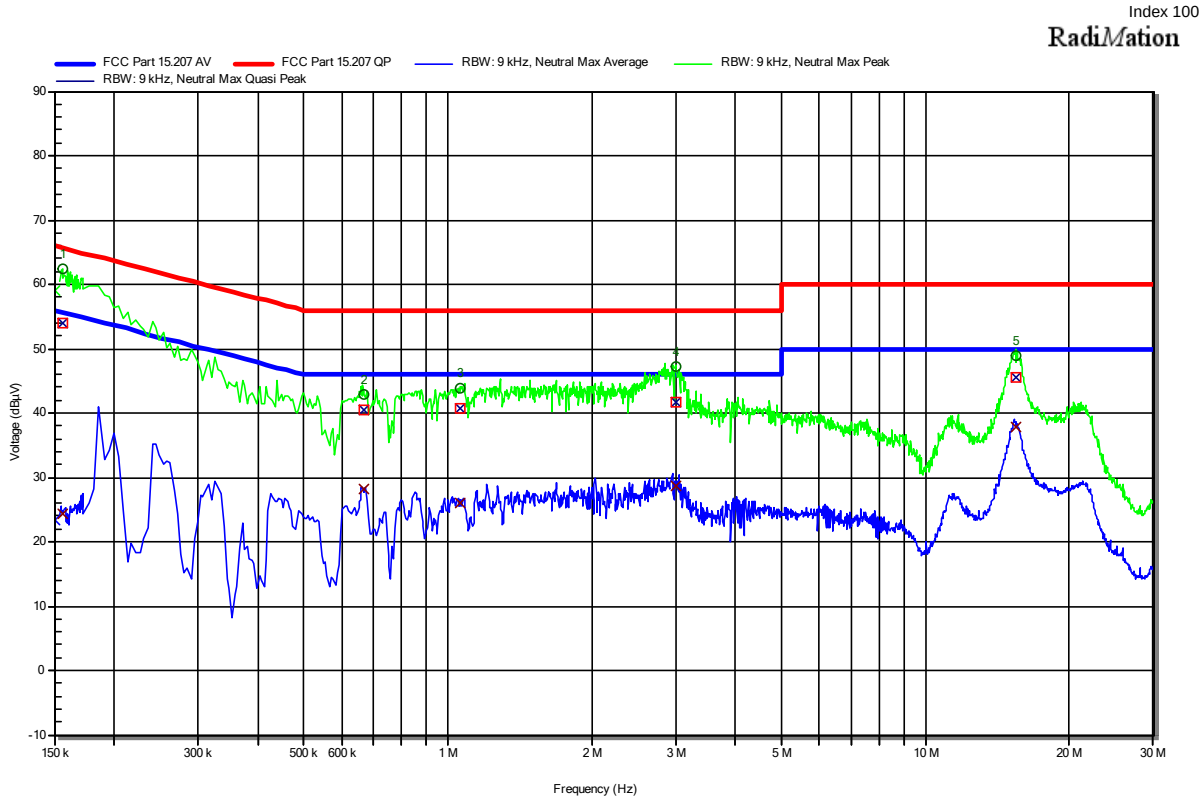

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	LISN
1	155.85 kHz	54.09 dBµV	65.68 dBµV	-11.6 dB	Pass	Neutral
2	665.25 kHz	40.39 dBµV	56 dBµV	-15.61 dB	Pass	Neutral
3	1.063 MHz	40.69 dBµV	56 dBµV	-15.31 dB	Pass	Neutral
4	2.999 MHz	41.73 dBµV	56 dBµV	-14.27 dB	Pass	Neutral
5	15.446 MHz	45.58 dBµV	60 dBµV	-14.42 dB	Pass	Neutral

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	LISN
1	155.85 kHz	24.39 dBµV	55.68 dBµV	-31.29 dB	Pass	Neutral
2	665.25 kHz	28.08 dBµV	46 dBµV	-17.92 dB	Pass	Neutral
3	1.063 MHz	26.11 dBµV	46 dBµV	-19.89 dB	Pass	Neutral
4	2.999 MHz	28.73 dBµV	46 dBµV	-17.27 dB	Pass	Neutral
5	15.446 MHz	37.93 dBµV	50 dBµV	-12.07 dB	Pass	Neutral

3.2 Test Conditions and Results - Transmitter radiated emissions

3.2.1 Information

Test Information	
Reference	FCC § 15.247(d); FCC § 15.209
Measurement Uncertainty	± 5.95 dB
Measurement Method	ANSI C63.10 6.4, 6.5, 6.6, 11.12
Operator	Odai Qawasmeh
Date	2022-02-28

3.2.2 Limits

Limits			
Frequency range [MHz]	Detector	Field strength [µV/m]	Measurement distance [m]
0.009 - 0.09	Average	2400/F[kHz]	300
0.09 - 0.110	Quasi-Peak	2400/F[kHz]	300
0.110 - 0.490	Average	2400/F[kHz]	300
0.490 - 1.705	Quasi-Peak	24000/F[kHz]	30
1.705 - 30.0	Quasi-Peak	30	30
30 - 88	Quasi-Peak	100	3
88 - 216	Quasi-Peak	150	3
216 - 960	Quasi-Peak	200	3
960 - 1000	Quasi-Peak	500	3
>1000	Average	500	3

3.2.3 Setup

Test Setup 30 MHz - 1000 MHz

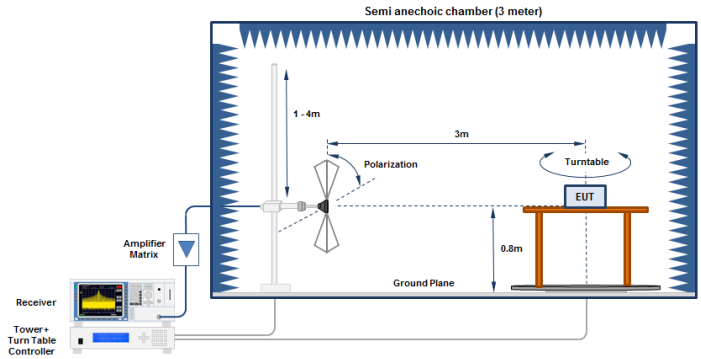

Test Setup > 1 GHz

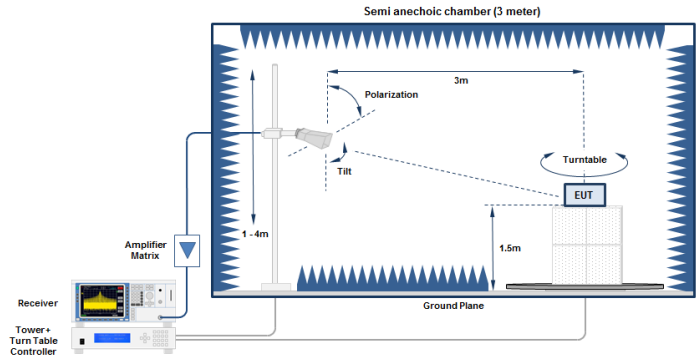

3.2.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2020.1.8

Test Equipment 30 MHz - 1000 MHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00910	-	-
MXE EMI Receiver	Keysight Technologies	N9038A-526/WXP	EF01070	2021-07	2022-07
Biconical antenna	R&S	HK116	EF00030	2021-05	2024-05
LPD antenna	R&S	HL223	EF00187	2019-05	2022-05

Test Equipment > 1 GHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic chamber	Frankonia	AC2	EF00196	-	-
Spectrum analyzer	R&S	FSU43	EF01631	2021-07	2022-07
Antenna	Schwarzbeck	BBHA 9120B	EF01678	2021-03	2022-03
Antenna	Schwarzbeck	HWRD 650	EF01679	2021-03	2022-03
40GHz High Gain Antenna	Amplifier Research	AT4560	EF00302	2021-06	2023-06

3.2.5 Procedure

Test Procedure 30 MHz - 1000 MHz
1. EUT is placed on a non conducting support at the center of a turn table 0.8 m above the ground 2. EUT set to test mode 3. The receiver is set to peak detection with max hold 4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m 5. All significant emissions are measured again using the corresponding final detector

Test Procedure > 1 GHz
1. EUT is placed on a non conducting support at the center of a turn table 1.5 m above the ground 2. EUT set to test mode 3. The receiver is set to peak detection with max hold 4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m 5. All significant emissions are measured again using the corresponding final detector

3.2.6 Results

Test Results - HT20						
Channel [MHz]	Emission [MHz]	Level [dBµV/m]	Det.	Pol.	Limit [dBµV/m]	Margin [dB]
2412	2322.3	58.49	pk	ver	74.00	-15.51
2412	2322.3	45.09	avg	ver	54.00	-08.91
2437	37.9875	35.00	qpk	ver	40.00	-05.05
2437	74.9055	31.90	qpk	ver	40.00	-08.07
2437	120.0251	29.80	qpk	ver	43.50	-13.73
2437	169.4595	30.50	qpk	ver	43.50	-13.03
2437	249.66	37.00	qpk	hor	46.00	-08.97
2437	259.96	27.50	qpk	hor	46.00	-18.52
2437	324.86	33.50	qpk	hor	46.00	-12.54
2437	408.06	30.20	qpk	hor	46.00	-15.85
2437	992.3	42.30	pk	ver	54.00	-11.74
2437	2727	49.23	pk	ver	74.00	-24.77
2437	2727	36.35	avg	ver	54.00	-17.65
2437	4879	46.18	pk	ver	74.00	-27.82
2437	4879	34.35	avg	ver	54.00	-19.65
2462	2492.8	59.72	pk	hor	74.00	-14.28
2462	2492.8	45.44	avg	hor	54.00	-08.56

3.2.7 Setup Photos

Setup for measurements below 1 GHz
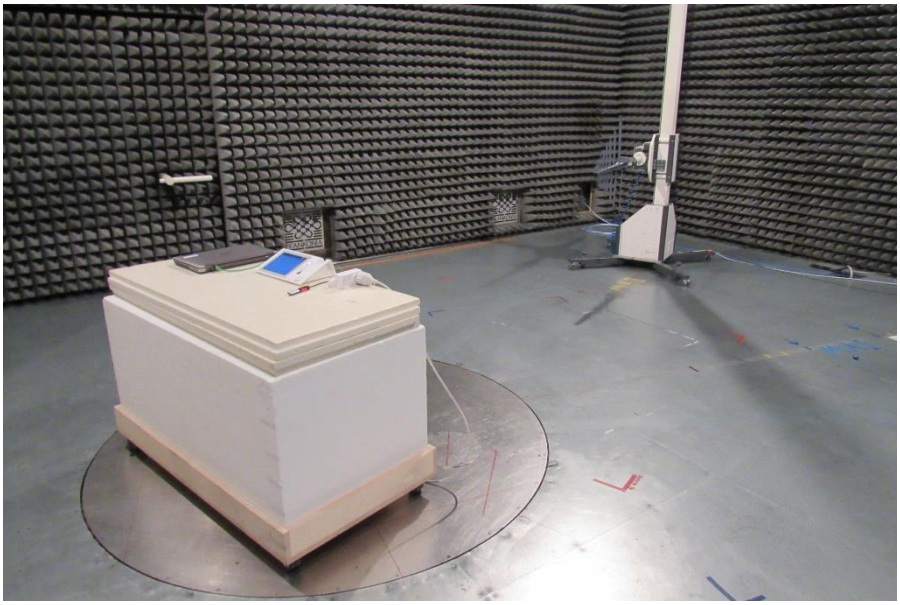

Setup for measurements below 1 GHz
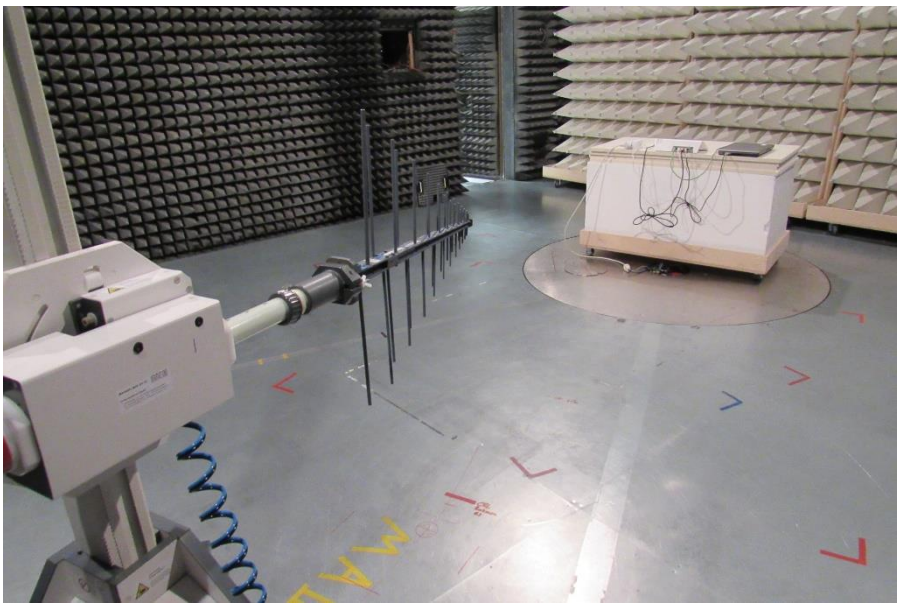

EUT Setup
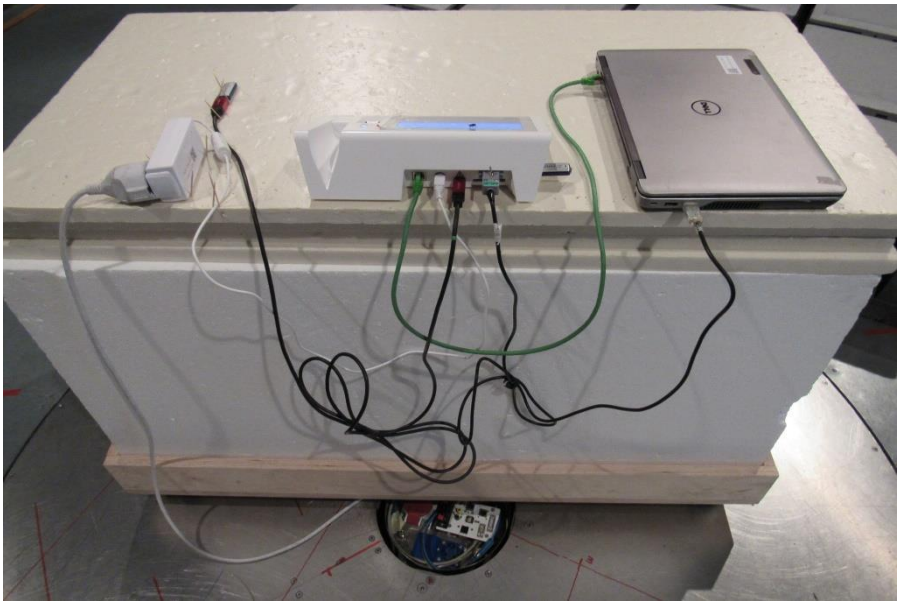

Setup for measurements above 1 GHz
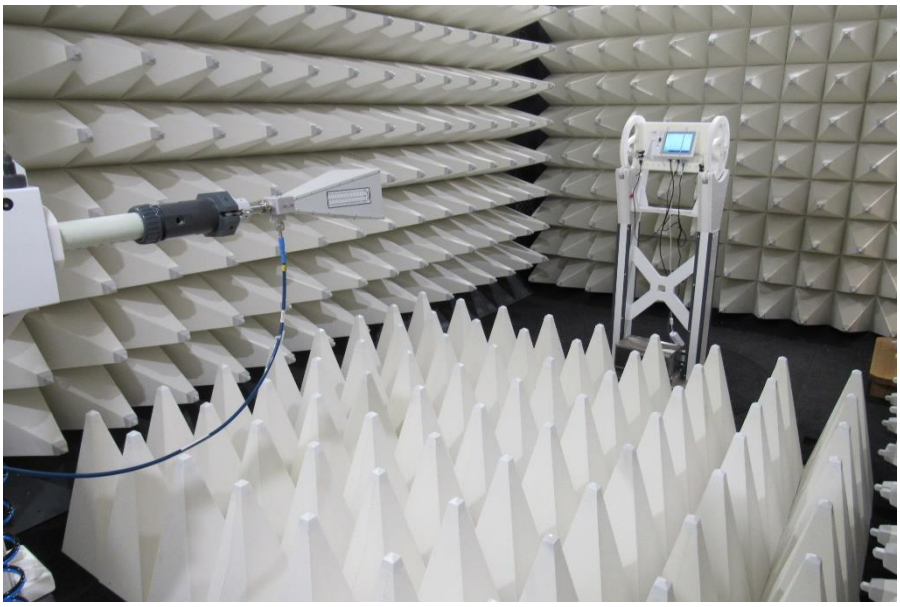

EUT Setup
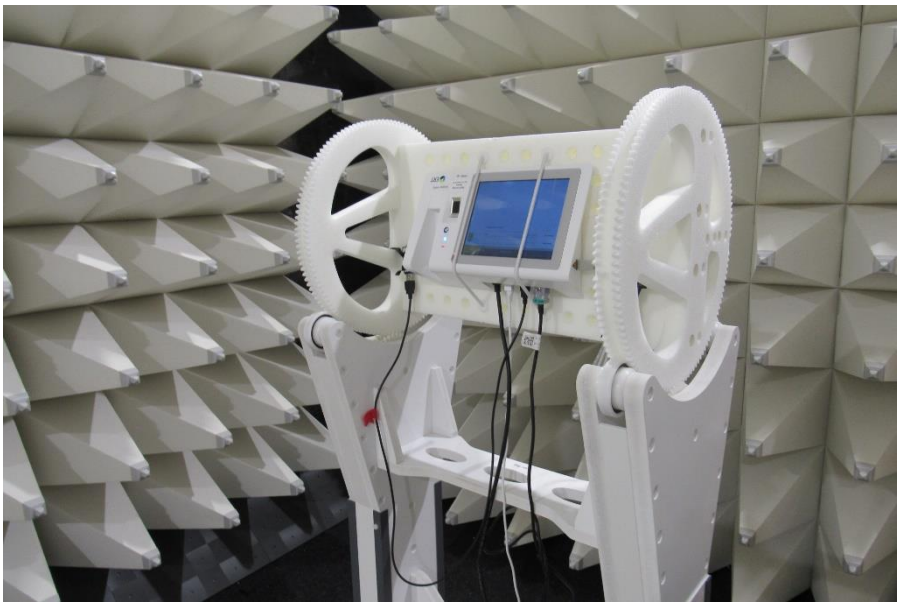

ANNEX A Transmitter spurious emissions

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Qawasmeh
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Rohde & Schwarz HK 116
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2437 Mhz
Test Date:	2022-03-04
Note:	

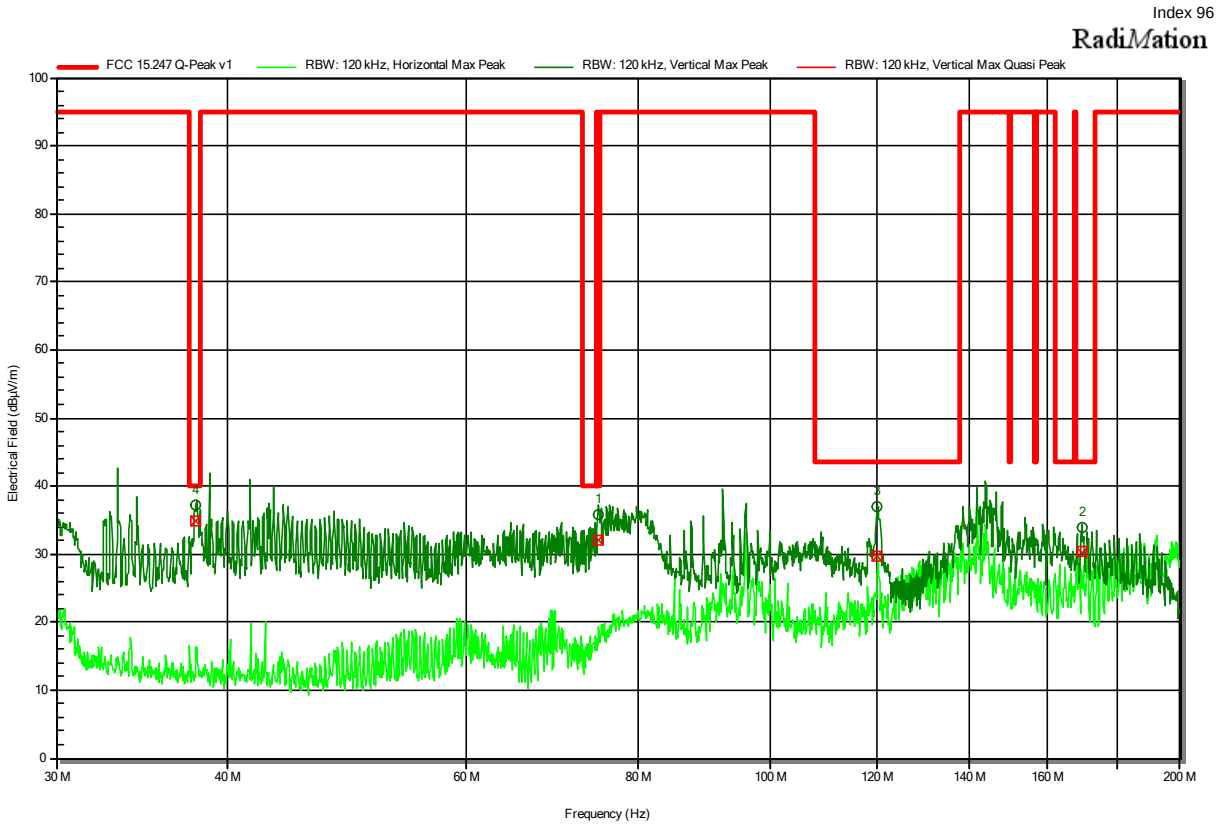

Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	Polarization
37.9875 MHz	35 dBµV/m	40 dBµV/m	-5.05 dB	Pass	Vertical
74.9055 MHz	31.9 dBµV/m	40 dBµV/m	-8.07 dB	Pass	Vertical
120.0251 MHz	29.8 dBµV/m	43.5 dBµV/m	-13.73 dB	Pass	Vertical
169.4595 MHz	30.5 dBµV/m	43.5 dBµV/m	-13.03 dB	Pass	Vertical

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Qawasmeh
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Rohde & Schwarz HL 223
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2437 Mhz
Test Date:	2022-03-02
Note:	

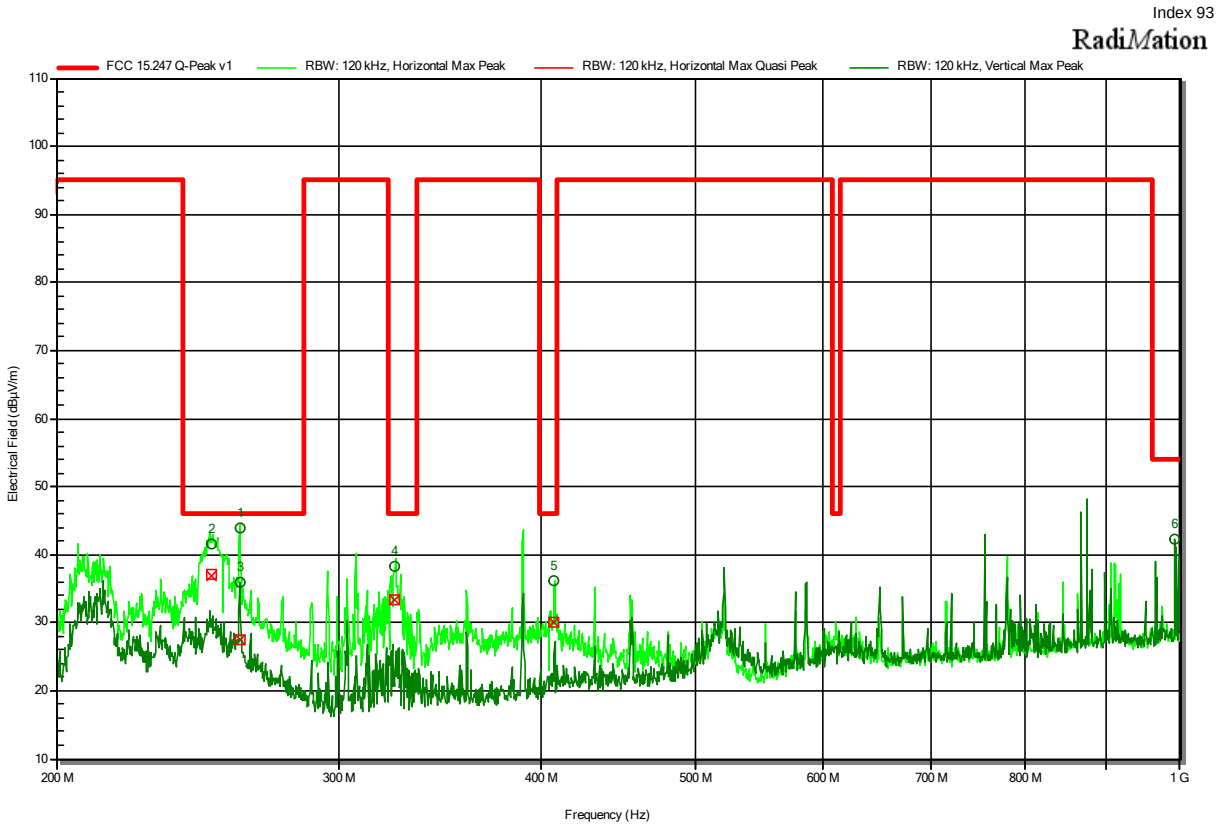

Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Polarization
260.02 MHz	35.9 dBµV/m	46 dBµV/m	-10.13 dB	Pass	Vertical
992.3 MHz	42.3 dBµV/m	54 dBµV/m	-11.74 dB	Pass	Vertical

Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	Polarization
249.66 MHz	37 dBµV/m	46 dBµV/m	-8.97 dB	Pass	Horizontal
259.96 MHz	27.5 dBµV/m	46 dBµV/m	-18.52 dB	Pass	Horizontal
324.86 MHz	33.5 dBµV/m	46 dBµV/m	-12.54 dB	Pass	Horizontal
408.06 MHz	30.2 dBµV/m	46 dBµV/m	-15.85 dB	Pass	Horizontal

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	R. Jaafar
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 24 °Celsius, Vnom:
Antenna:	Schwarzbeck BBHA 9120B
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2437 Mhz
Test Date:	2022-03-18
Note:	

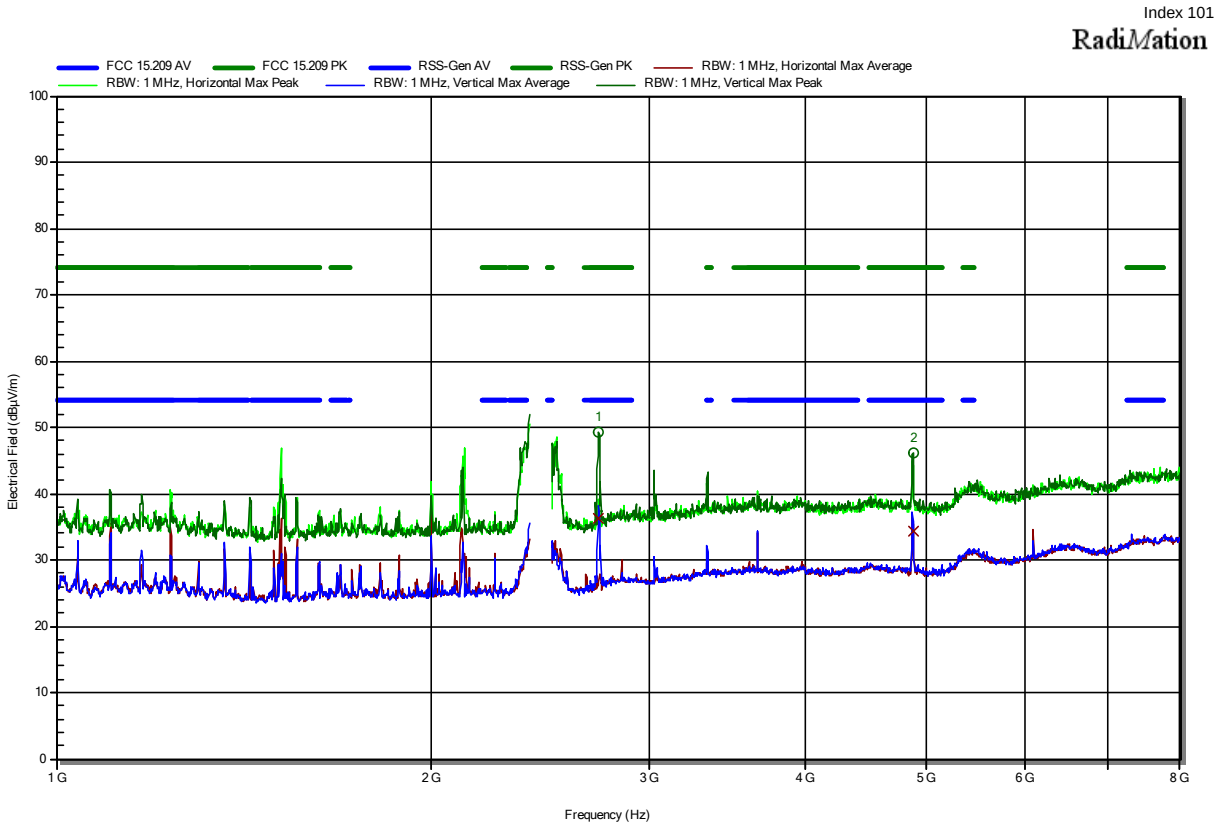

Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Polarization
2.727 GHz	49.23 dBµV/m	74 dBµV/m	-24.77 dB	Pass	Vertical
4.879 GHz	46.18 dBµV/m	74 dBµV/m	-27.82 dB	Pass	Vertical

Frequency	Average	Average Limit	Average Difference	Average Status	Polarization
2.727 GHz	36.35 dBµV/m	54 dBµV/m	-17.65 dB	Pass	Vertical
4.879 GHz	34.35 dBµV/m	54 dBµV/m	-19.65 dB	Pass	Vertical

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	R. Jaafar
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Schwarzbeck BBHA 9120B
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2412 Mhz
Test Date:	2022-02-28
Note:	lower bandedge

Index 85

RadiMation

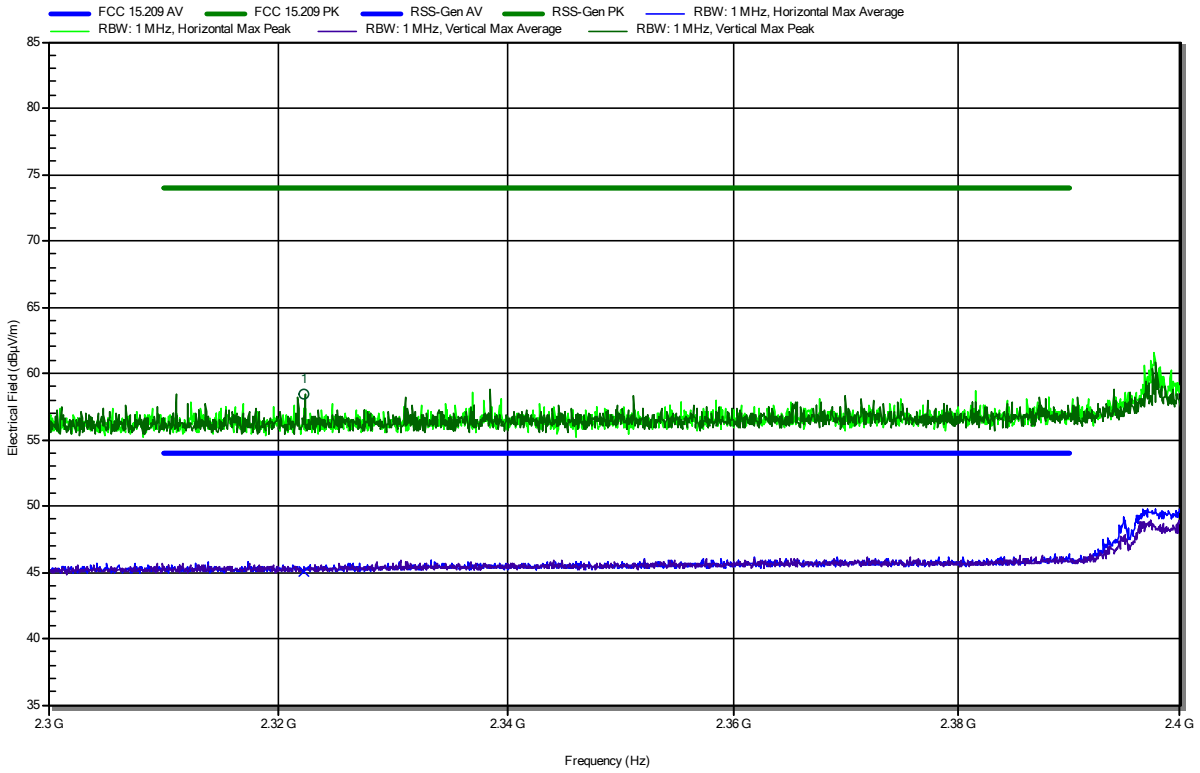

Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Polarization
2.3223 GHz	58.49 dBµV/m	74 dBµV/m	-15.51 dB	Pass	Vertical

Frequency	Average	Average Limit	Average Difference	Average Status	Polarization
2.3223 GHz	45.09 dBµV/m	54 dBµV/m	-8.91 dB	Pass	Vertical

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	R. Jaafar
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Schwarzbeck BBHA 9120B
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2462 Mhz
Test Date:	2022-02-28
Note:	upper bandedge

Index 84

RadiMation

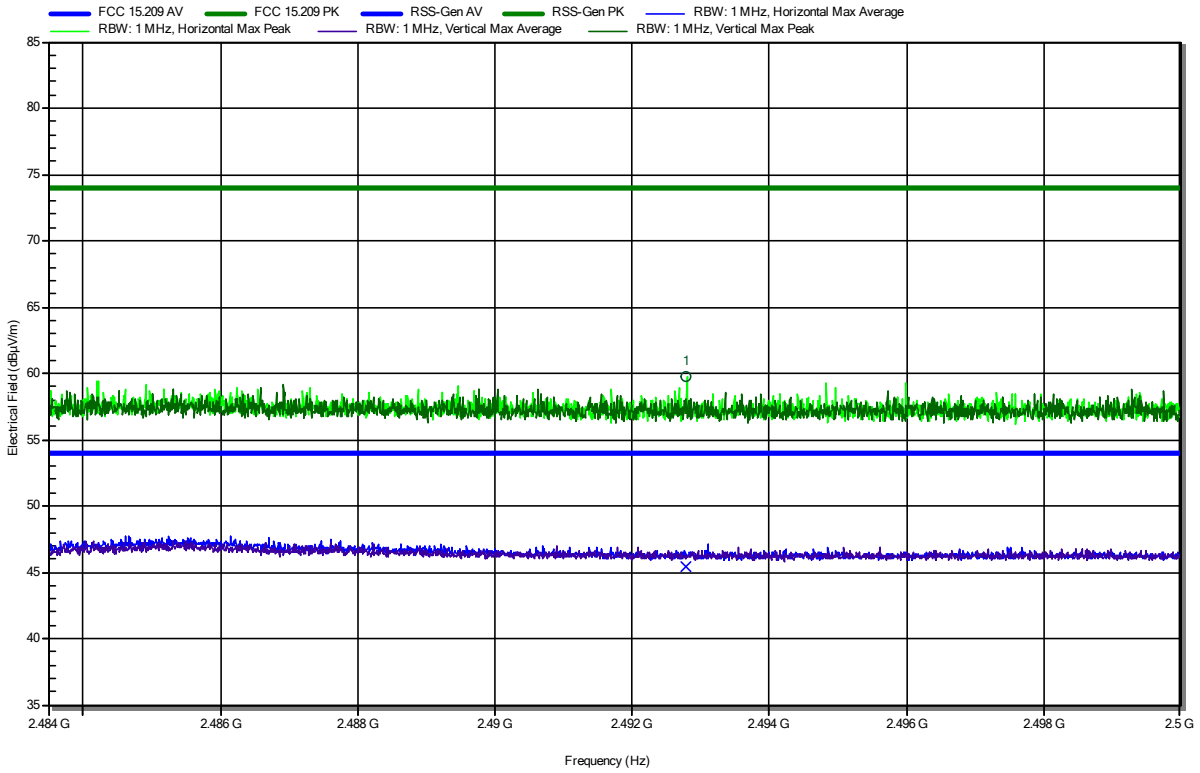

Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Polarization
2.4928 GHz	59.72 dBµV/m	74 dBµV/m	-14.28 dB	Pass	Horizontal

Frequency	Average	Average Limit	Average Difference	Average Status	Polarization
2.4928 GHz	45.44 dBµV/m	54 dBµV/m	-8.56 dB	Pass	Horizontal

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	R. Jaafar
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Schwarzbeck HWRD 650
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2437 Mhz
Test Date:	2022-02-28
Note:	

Index 87

RadiMation

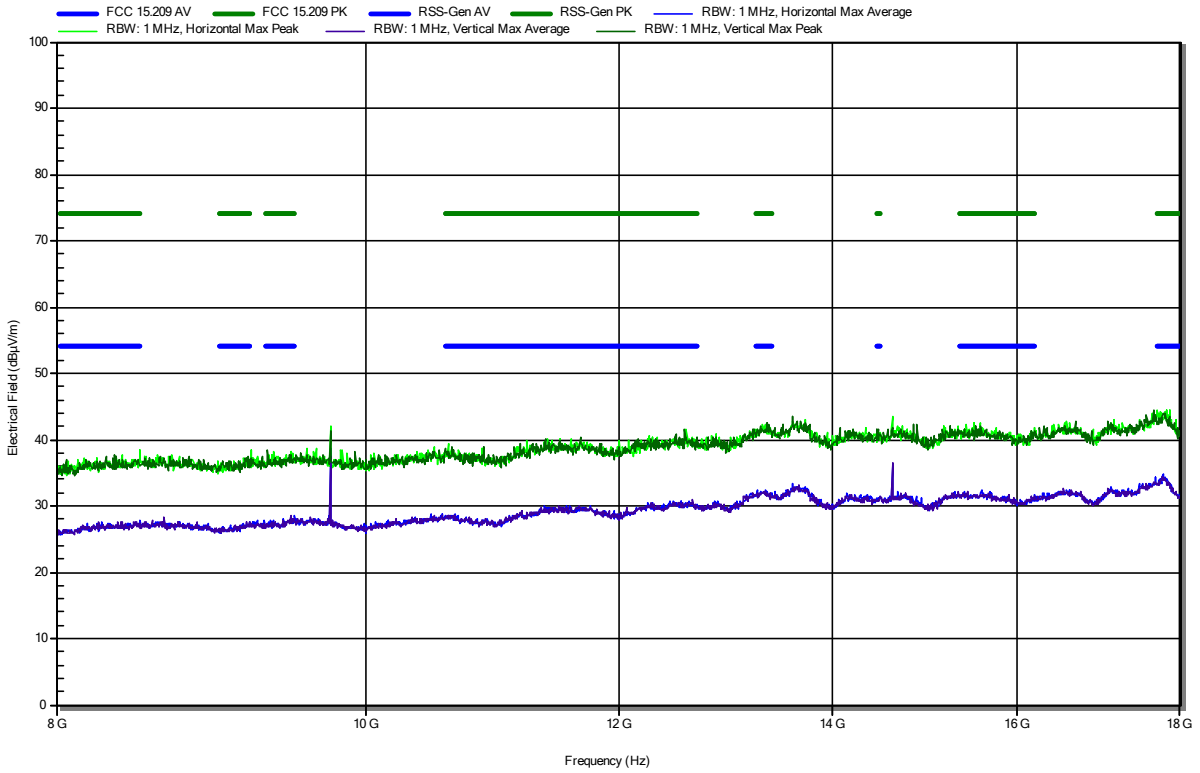

Radiated Spurious Emissions according to FCC 15.247

Project Number:	G0M-2112-1231
Applicant:	eResearchTechnology GmbH
Model Description:	Spirometer System
Model:	SpiroSphere
Test Sample ID:	38262
Test Site:	Eurofins Product Service GmbH
Operator:	R. Jaafar
Measurement software:	RadiMation, version 2020.1.8
Test Conditions:	Tnom: 23.5 °Celsius, Vnom:
Antenna:	Amplifier Research AT4560
Measurement distance:	3 m
Mode:	Tx; IEEE 802.11, HT20, MCS12, 2437 Mhz
Test Date:	2022-02-28
Note:	

Index 90

RadiMation

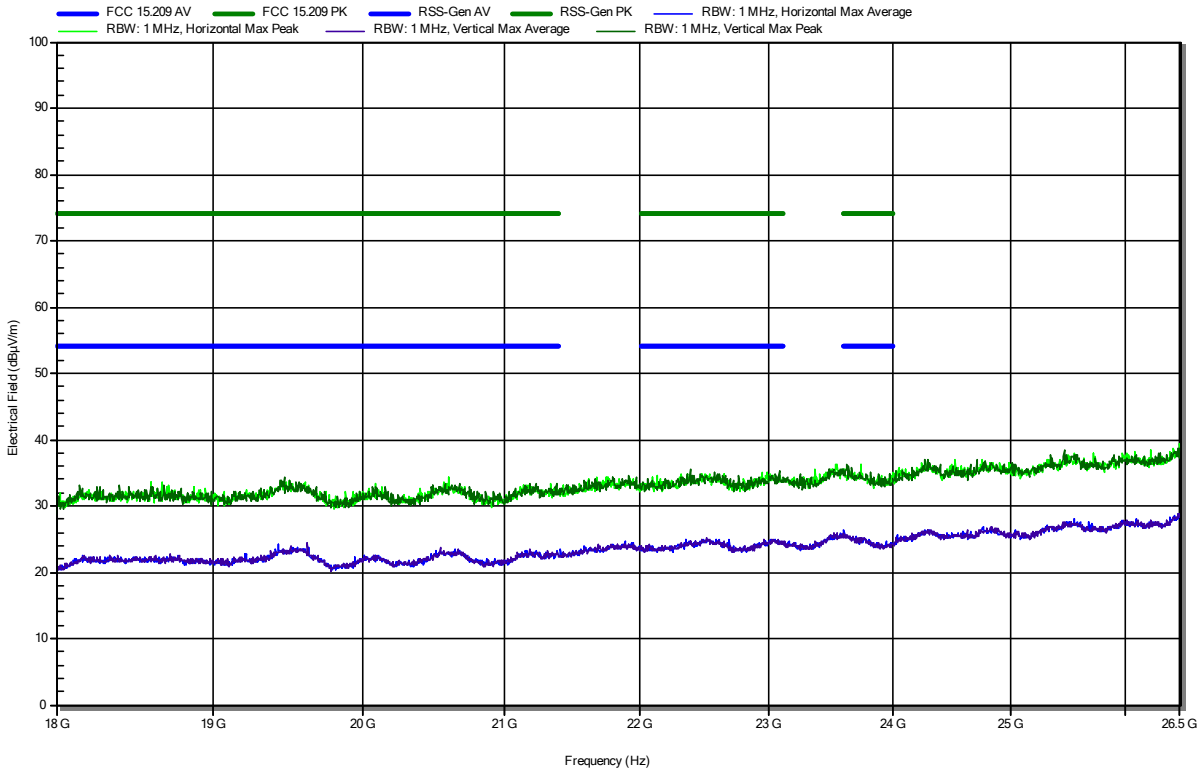

= = = END OF TEST REPORT = = =