

Date: September 25, 2014

Equipment Authorization Branch
Federal Communications Commission
7435 Oakland Mills Road.
Columbia , MD 21046

Re Filing for FCC ID : 2AB2MPECGT-III
Subject: SAR testing

Ladies and Gentlemen:

To not exceed the limits for exposure to radio frequency electromagnetic fields the PocketECG III during normal operation shall be carried out using dedicated pouch provided by Medicalgorithmics S.A. or equivalent holster. Body-worn SAR testing of PocketECG III has been carried out at a separation distance of 10 mm. Dedicated pouch is constructed to provide 10 mm separation between PocketECG III and patient's body. The spacer is permanently built in to the pouch and made of polymeric material.

Please see enclosed photos from 1 to 5 that shows pouch intended use and 10 mm spacer location.



Fig. 1 PocketECG III pouch normal operation



Fig. 2 Front view of PocketECG III pouch

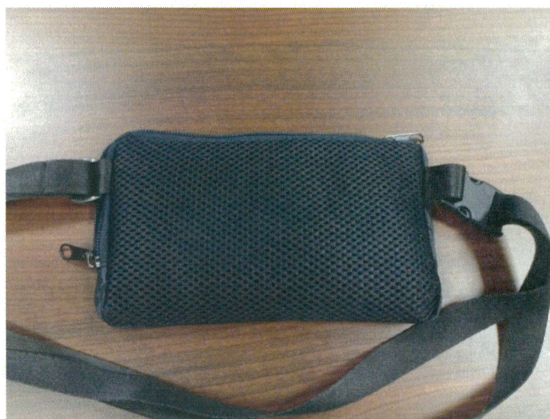


Fig. 3 Rear view of PocketECG III pouch

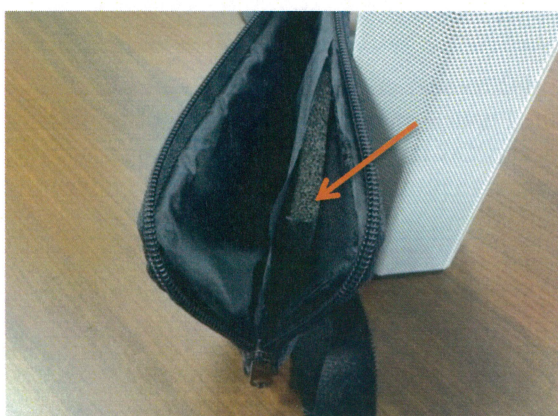


Fig. 4 Internal view of 10 mm spacer location



Fig. 5 Internal view of 10 mm spacer location

Respectfully,

Signature
Przemyslaw Tadla
Strategy Director
Medicalgorithmics S.A.
Al. Jerozolimskie 81, 02-001 Warsaw
POLAND