

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  | 68.70    | 39.5 ±1 %.  | 39.51    | 3.6 ±1 %.  | 3.61     |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         | 38.6     | 1.40 $\pm$ 10 %               | 1.34     |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.




## SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.42.9.23.BES.A

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Head Liquid Values: $\epsilon_s'$ : 38.4 $\sigma$ : 1.36 |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 1900 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             |              | 20.1              |              |
| 1900             | 39.7             | 39.84 (3.98) | 20.5              | 20.20 (2.02) |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             |              | 23.3              |              |
| 2450             | 52.4             |              | 24                |              |
| 2600             | 55.3             |              | 24.6              |              |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

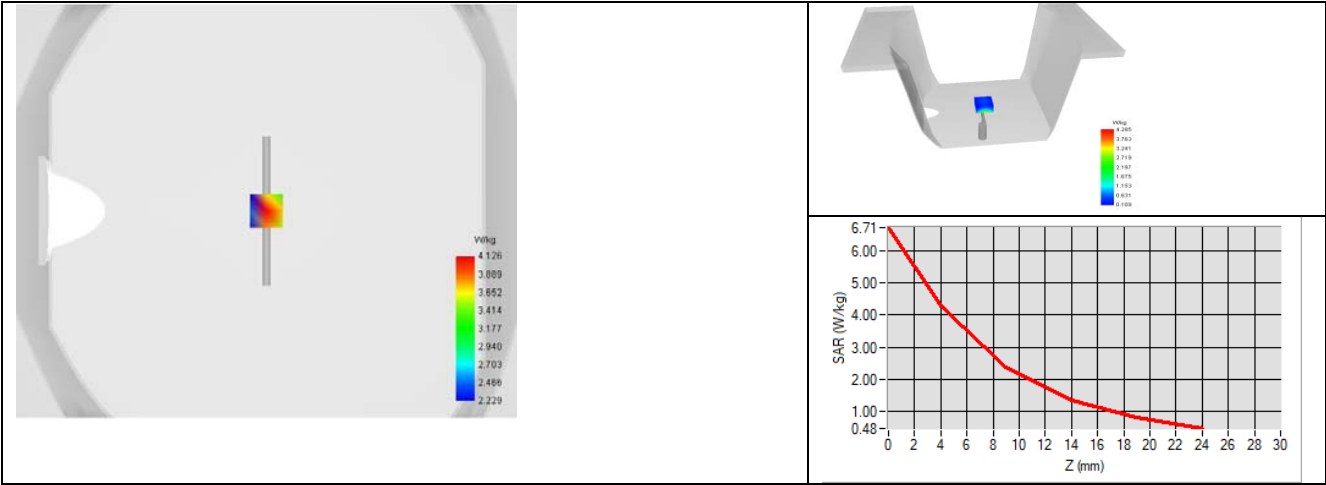


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         | 55.3     | 1.52 $\pm$ 10 %               | 1.49     |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

#### 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}'$ : 55.3 sigma : 1.49 |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 1900 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 1900             | 43.33 (4.33)     | 21.59 (2.16)      |

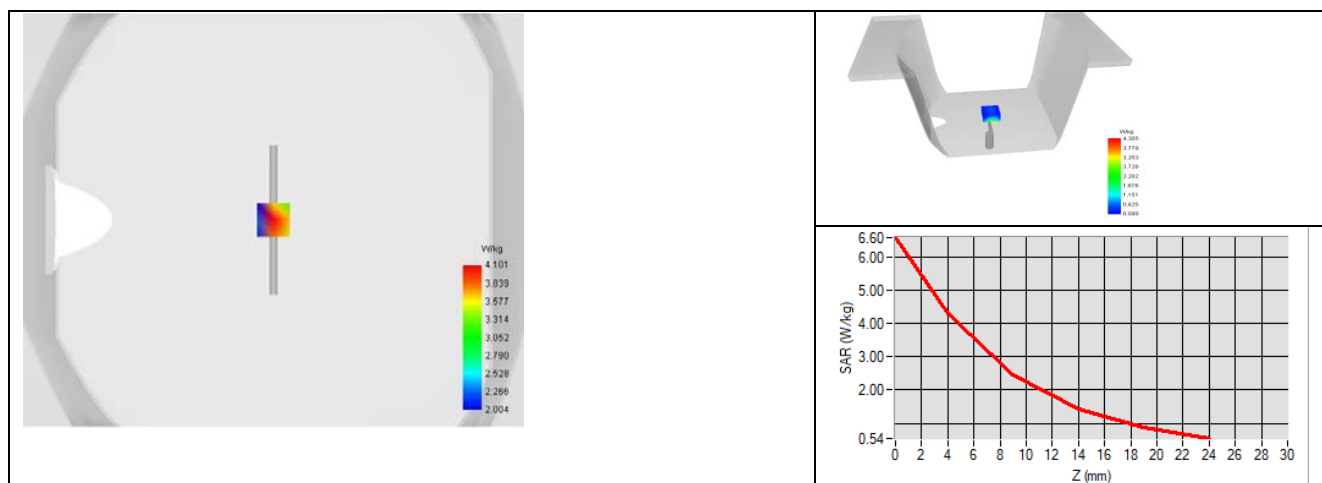

## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2026                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |