

Date: 2025/10/31

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(8.14, 7.82, 7.81); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 9.27 W/kg; SAR (10g) = 5.00 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 9.18 W/kg; SAR (10g) = 4.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

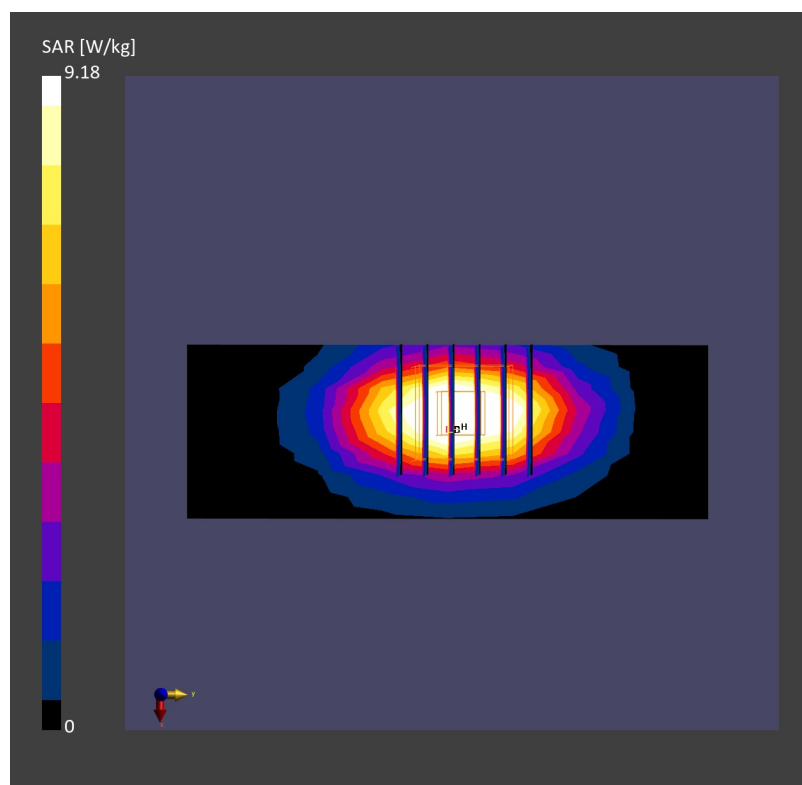

Date: 2025/10/31

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.9, 7.58, 7.57); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 11.2 W/kg; SAR (10g) = 5.82 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 10.7 W/kg; SAR (10g) = 5.56 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

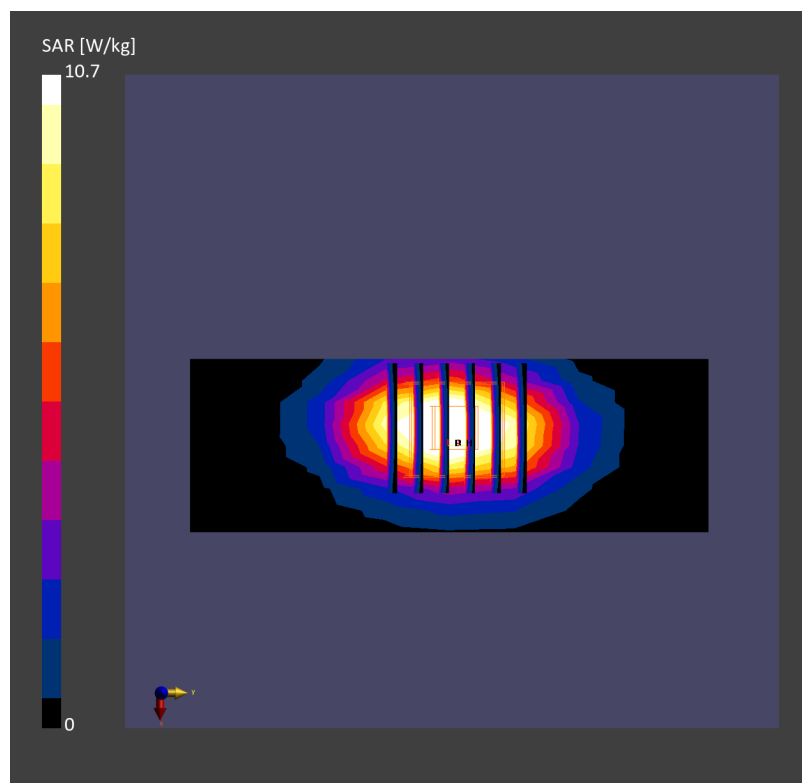

Date: 2025/10/31

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 12.6 W/kg; SAR (10g) = 6.04 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 12.7 W/kg; SAR (10g) = 5.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 83.0 %

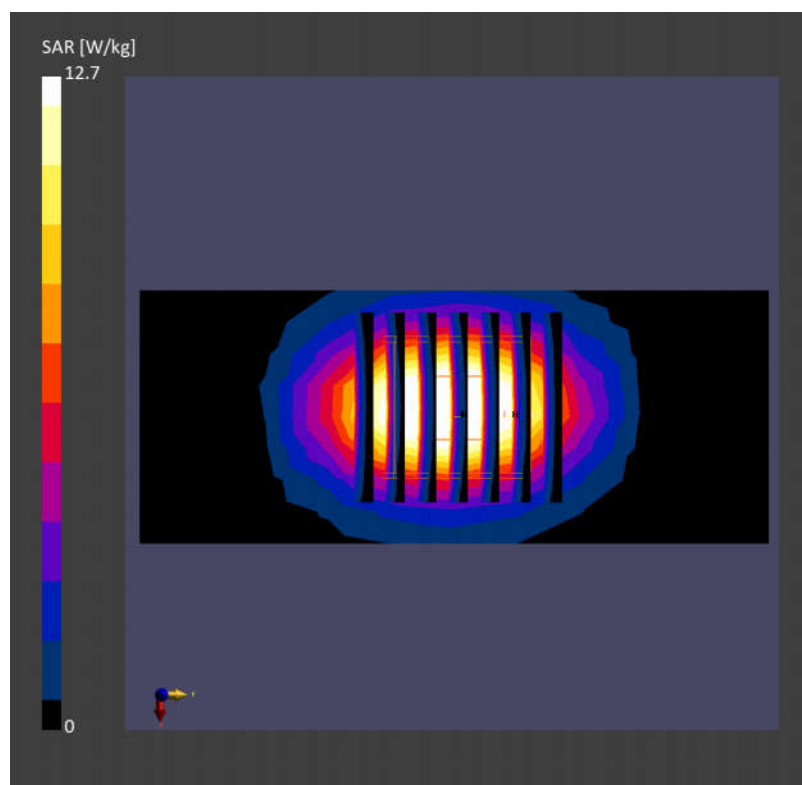

Date: 2025/10/31

System Check_2600MHz**DUT:D2600V2-SN:1070**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.13, 6.85, 6.84); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.08 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.2 W/kg; SAR (10g) = 5.96 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

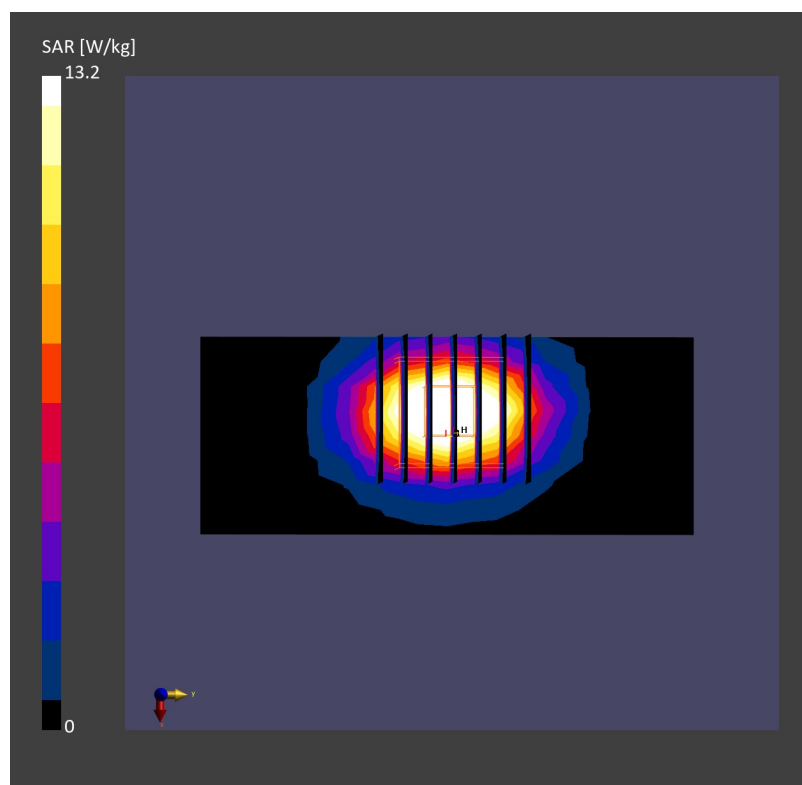

Date: 2025/10/31

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.82$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.78, 6.51, 6.5); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.85 W/kg; SAR (10g) = 2.66 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 6.81 W/kg; SAR (10g) = 2.64 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.4 %

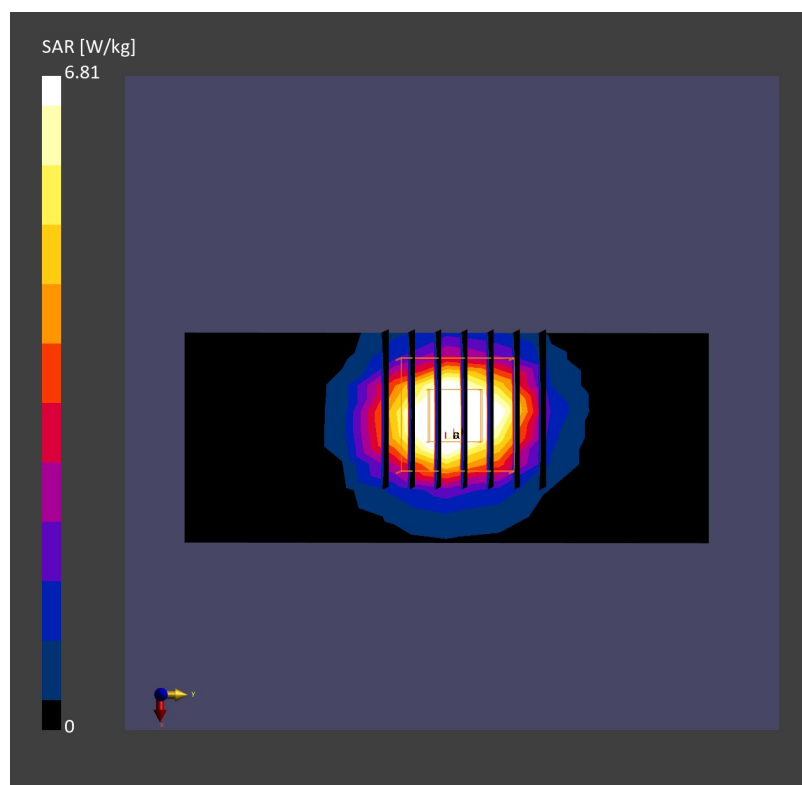

Date: 2025/10/31

System Check_5600MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.00$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.37 W/kg; SAR (10g) = 2.13 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 7.86 W/kg; SAR (10g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.2 %

