



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

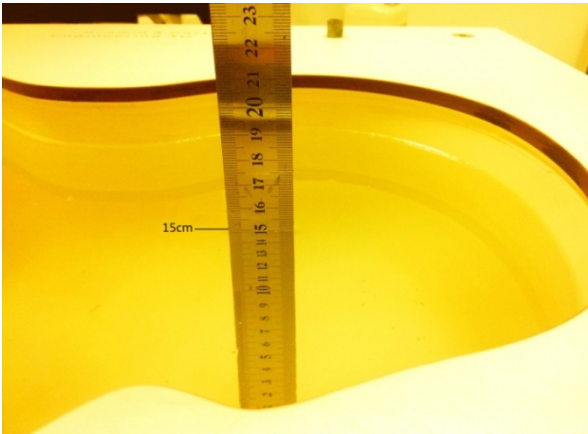
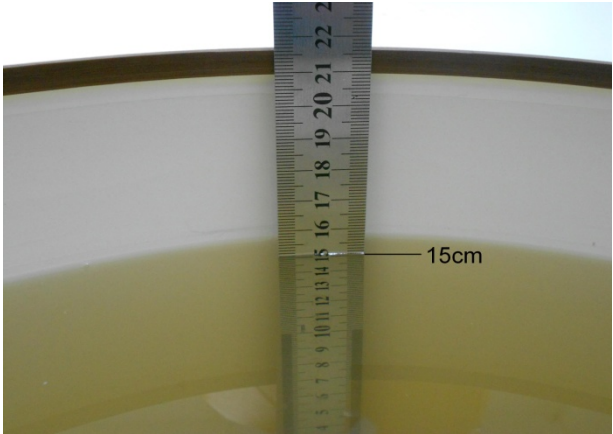
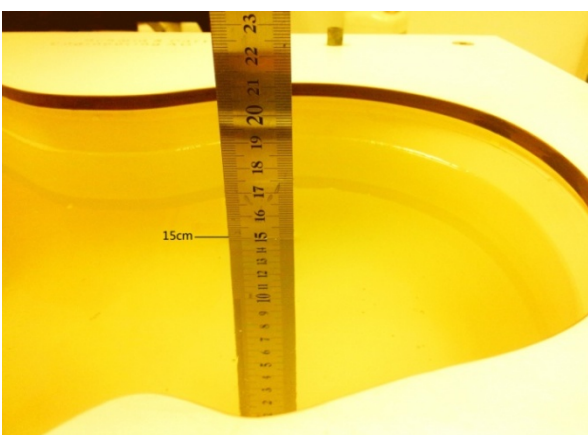
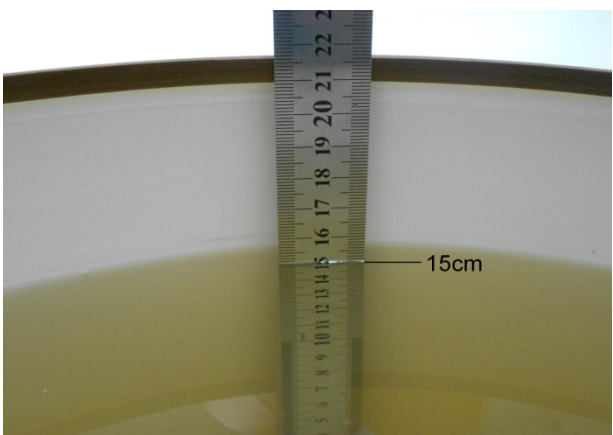
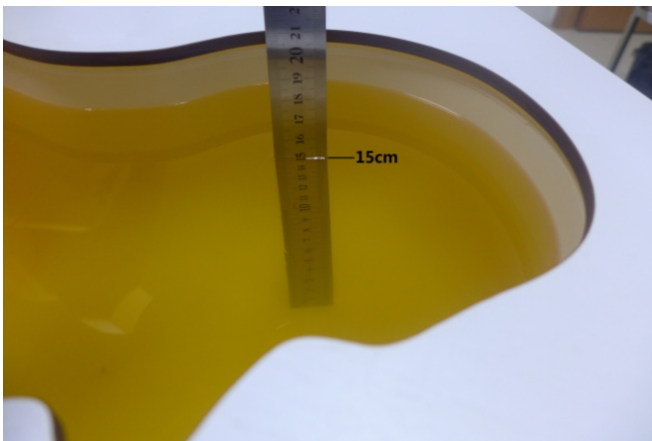
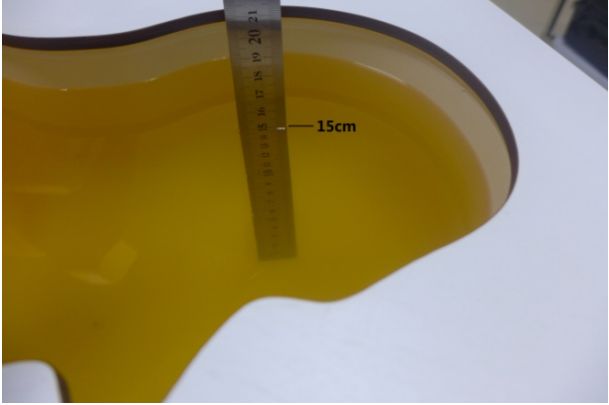
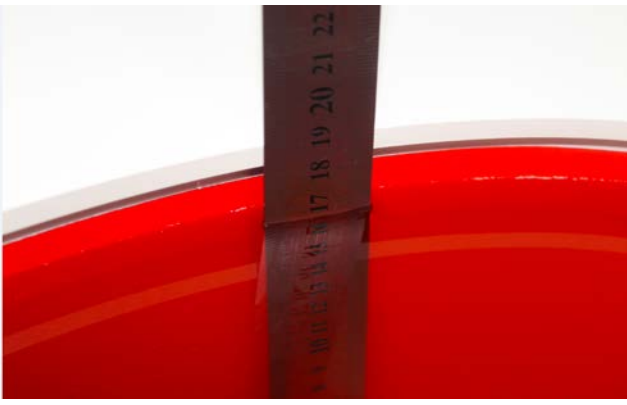
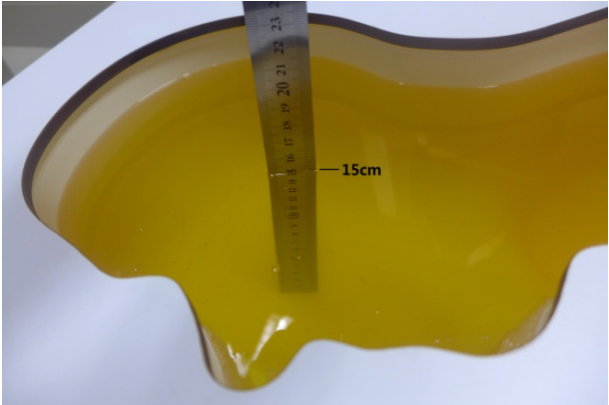
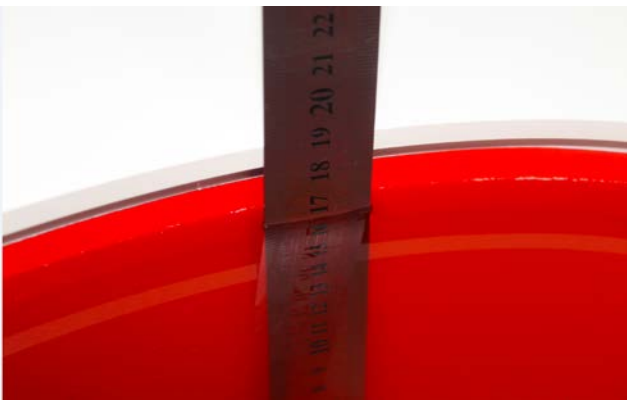
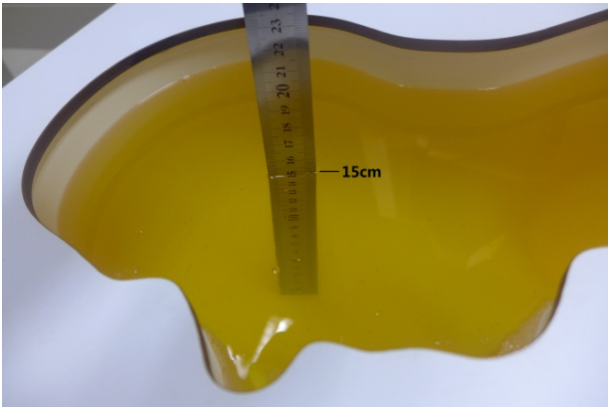
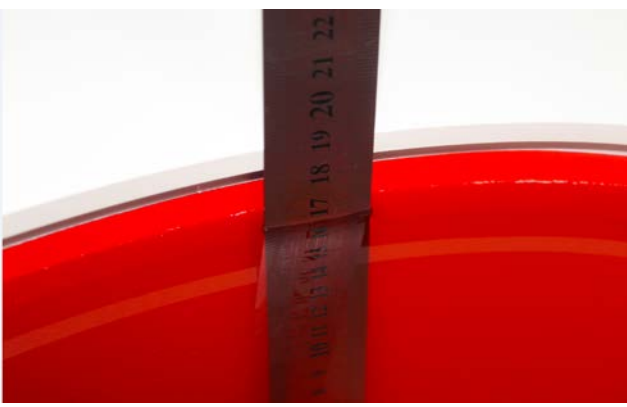
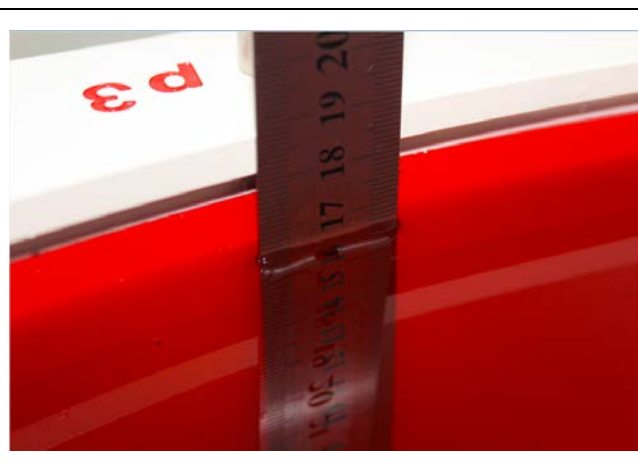
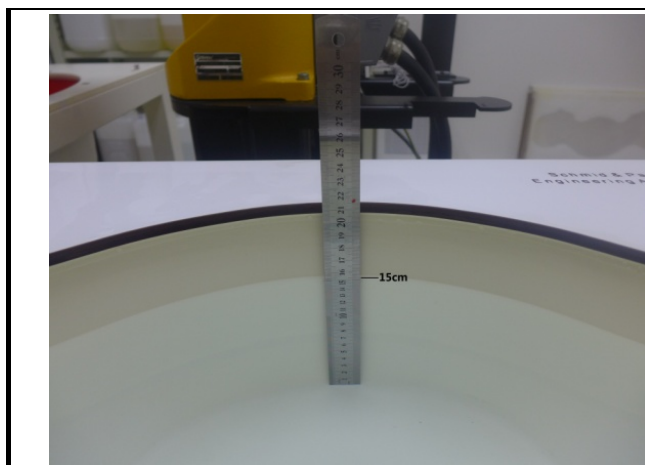
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	
Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
	

Photo 7: Tissue Simulant Liquid for Head 1900	Photo 8: Tissue Simulant Liquid for Body 1900
	
Photo 9: Tissue Simulant Liquid for Head 2450	Photo 10: Tissue Simulant Liquid for Body 2450
	
Photo 11: Tissue Simulant Liquid for Head 2600	Photo 12: Tissue Simulant Liquid for Body 2600
	
Photo 13: Tissue Simulant Liquid for Head 5G	Photo 14: Tissue Simulant Liquid for Body 5G



3. Photographs of EUT test position

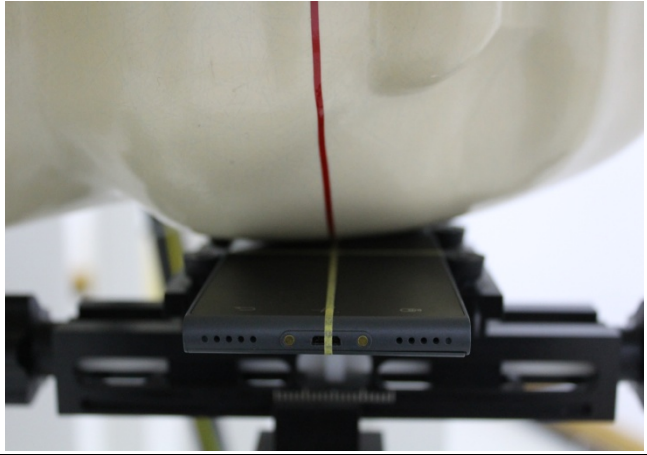
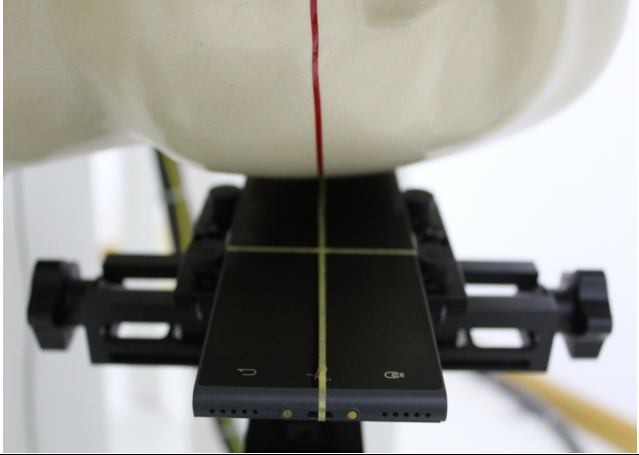
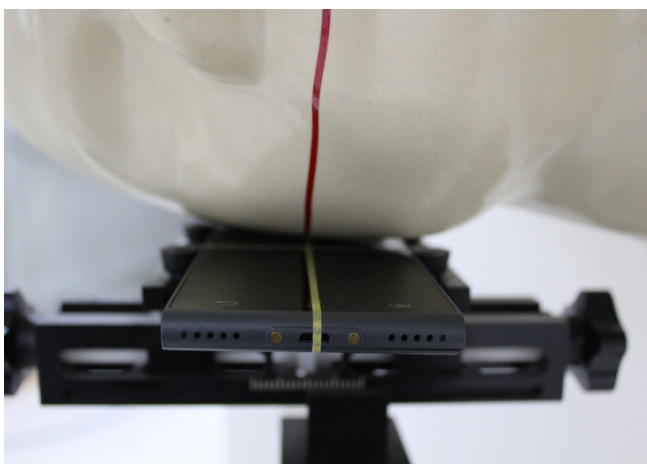
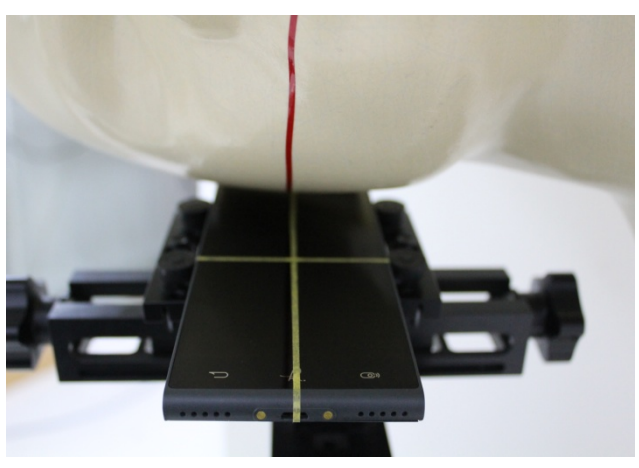
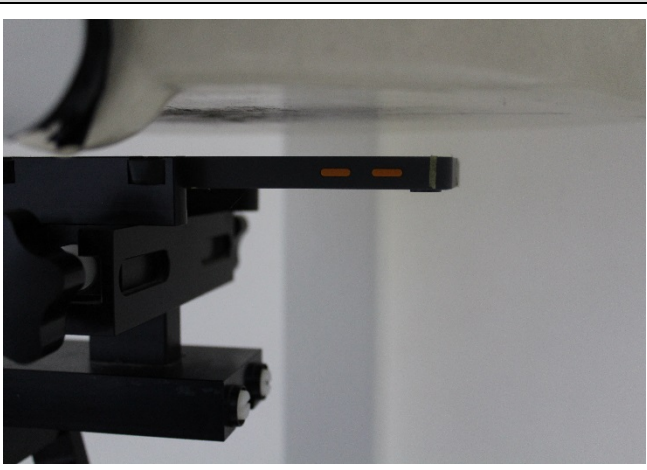
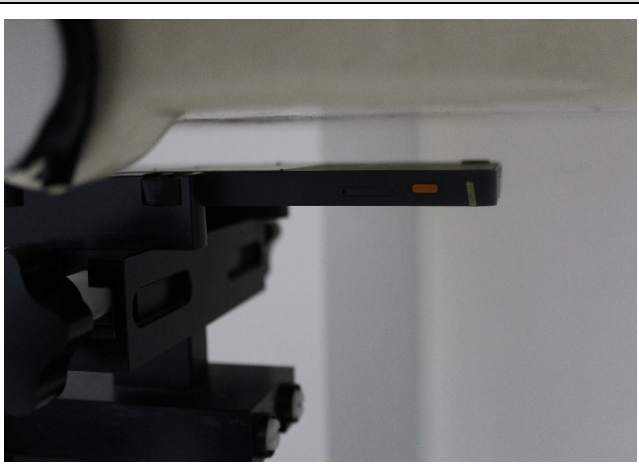
Photo 15: Left touch cheek	Photo 16: Left tilted 15 degree
	
Photo 17: Right touch cheek	Photo 18: Right tilted 15 degree
	
Photo 19: Front side 15mm	Photo 20: Back side 15mm
	

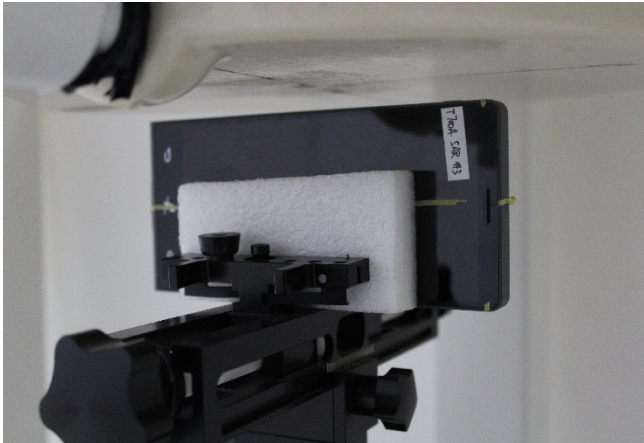
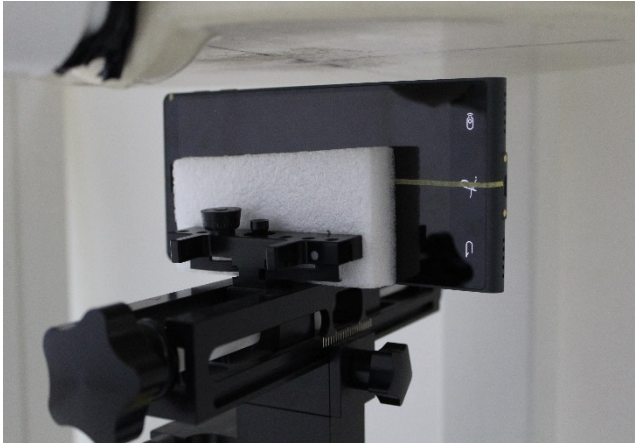
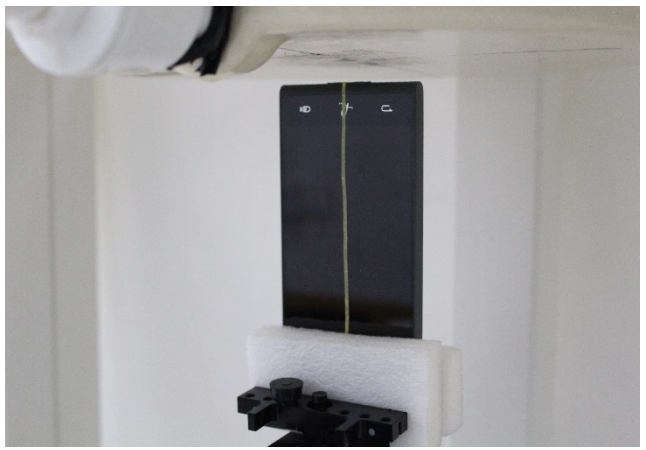
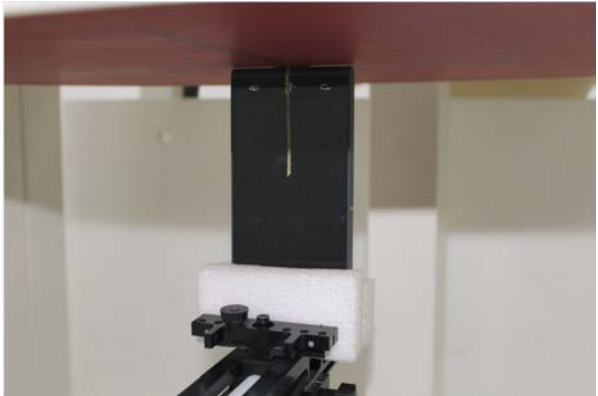
Photo 21: Front side 10mm 	Photo 22: Back side 10mm 
Photo 23: Front side 0mm 	Photo 24: Back side 0mm 
Photo 25: Left side 10mm 	Photo 26: Right side 10mm 

Photo 27: Top side 10mm	Photo 28: Bottom side 10mm
	
Photo 29: Bottom side 0mm	
	

4. EUT Constructional Details

