



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

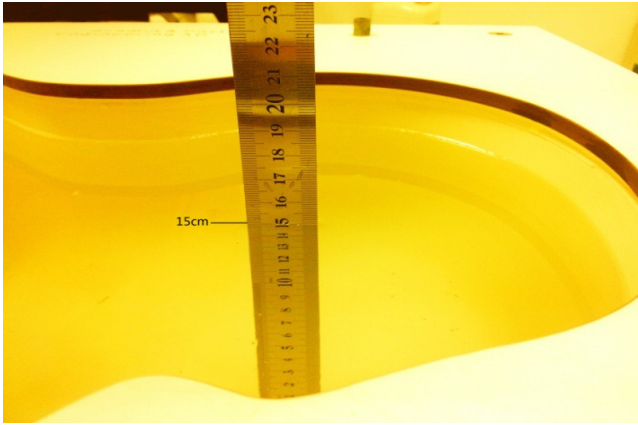
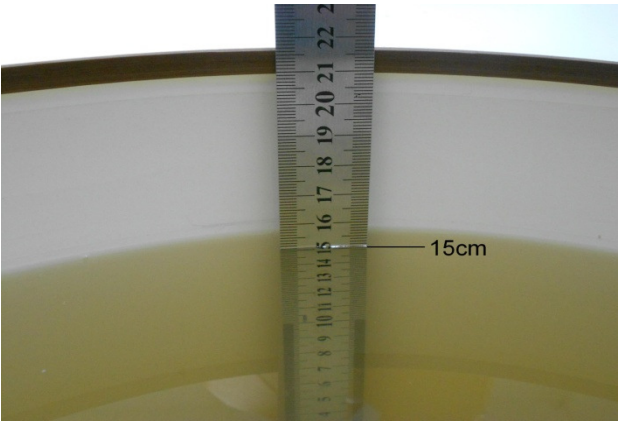
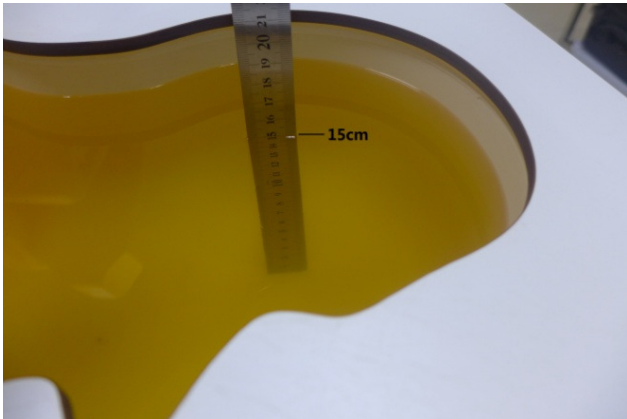
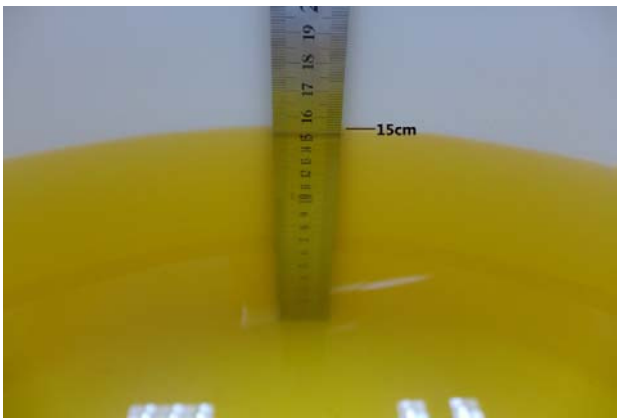
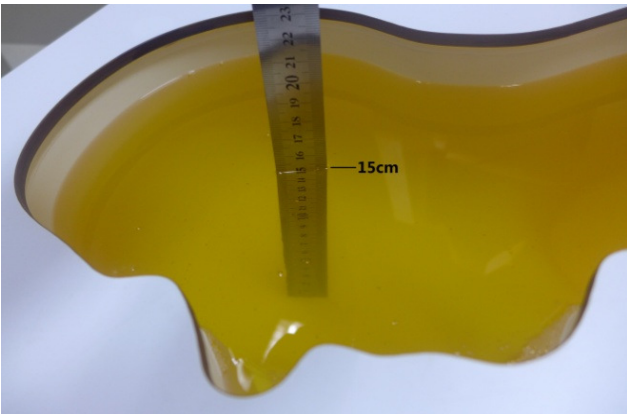
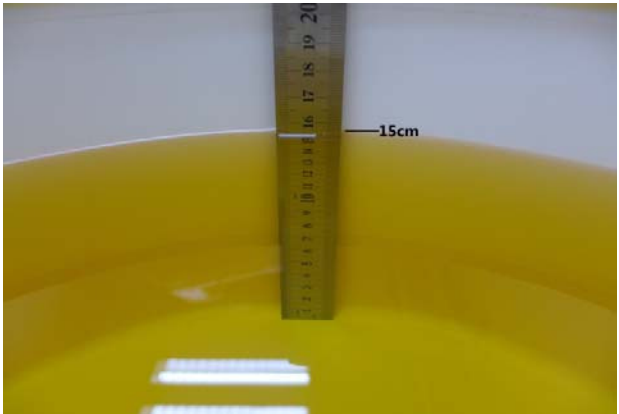
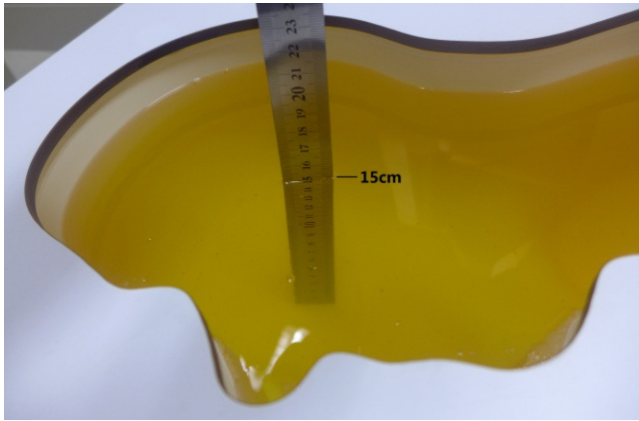
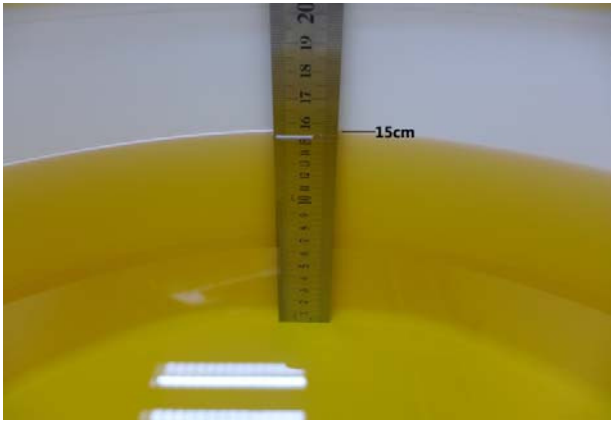
Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Body 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Body 2450
	

Photo 7: Tissue Simulant Liquid for Head 2600	Photo 8: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position












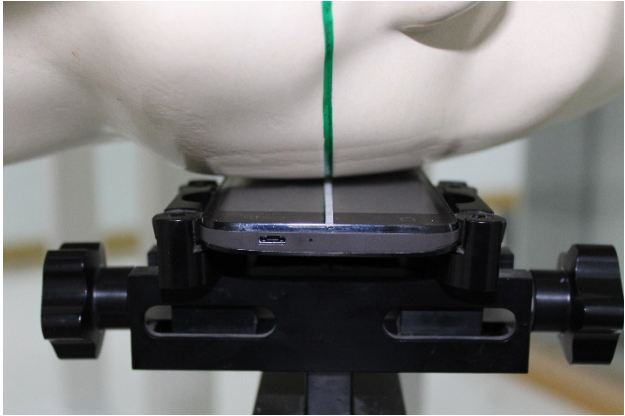
Photo 9: Left touch cheek	Photo 10: Left tilted 15 degree
	
Photo 11: Right touch cheek	Photo 12: Right tilted 15 degree
	
Photo 13: Front side 15mm	Photo 14: Back side 15mm
	

Photo 15: Front side 10mm 	Photo 16: Back side 10mm 
Photo 17: Left side 10mm 	Photo 18: Right side 10mm 
Photo 19: Bottom side 10mm 	Photo 20: Top side 10mm 

4. EUT Constructional Details

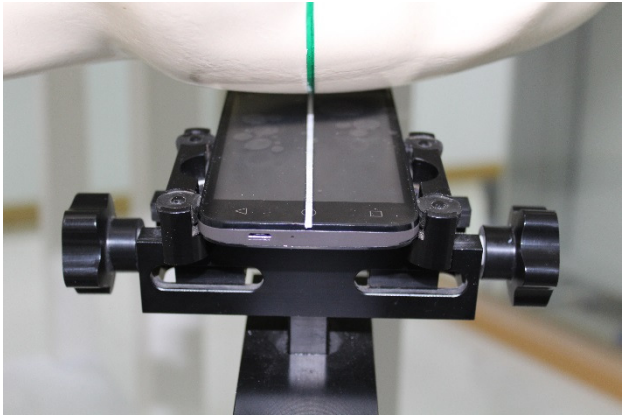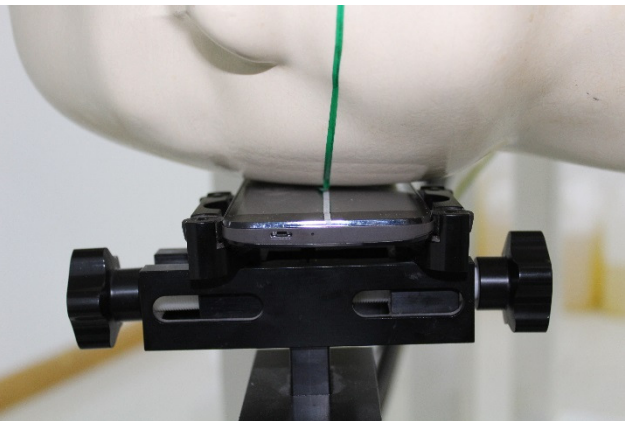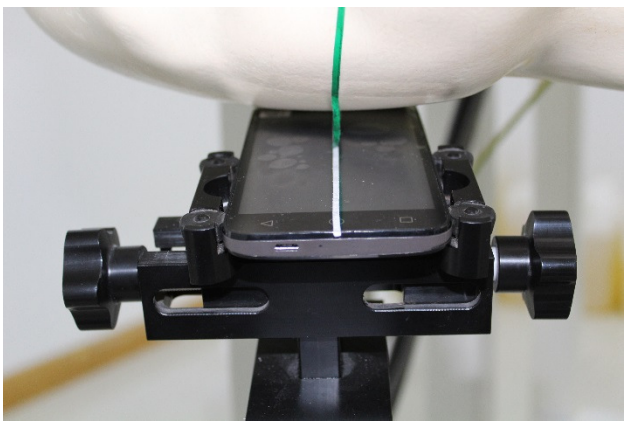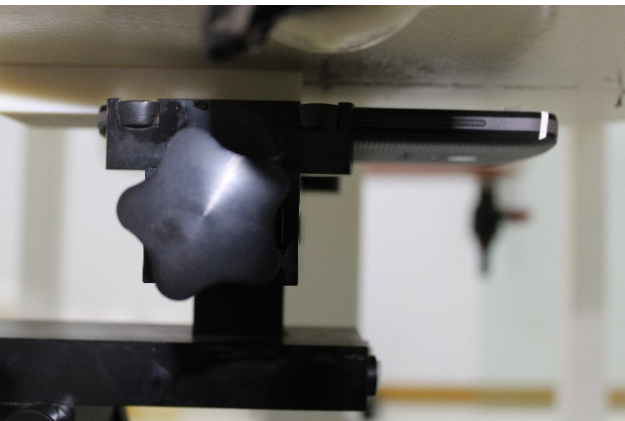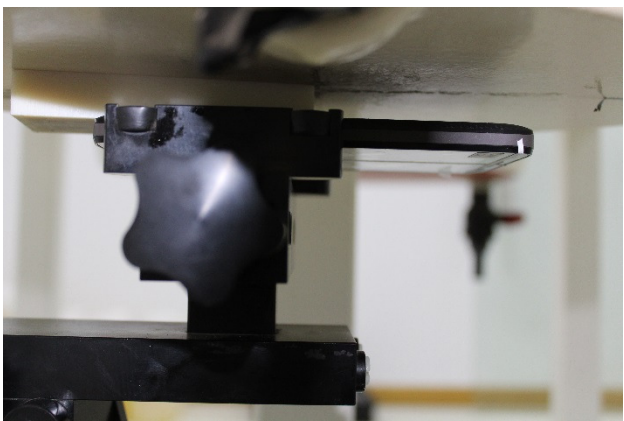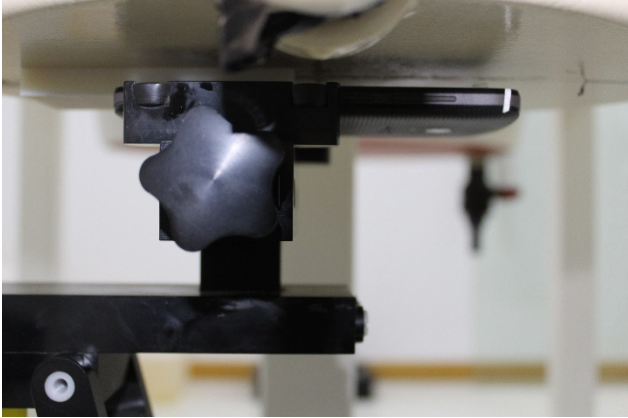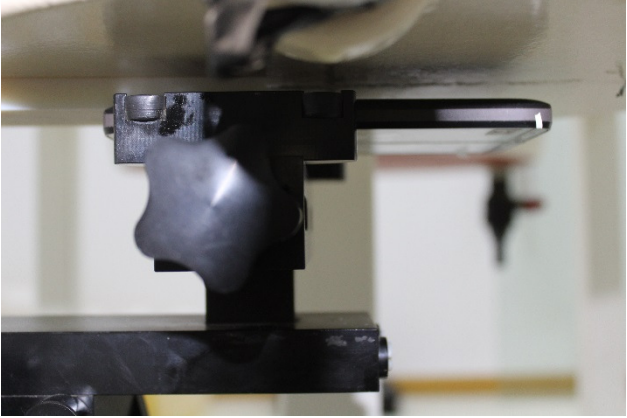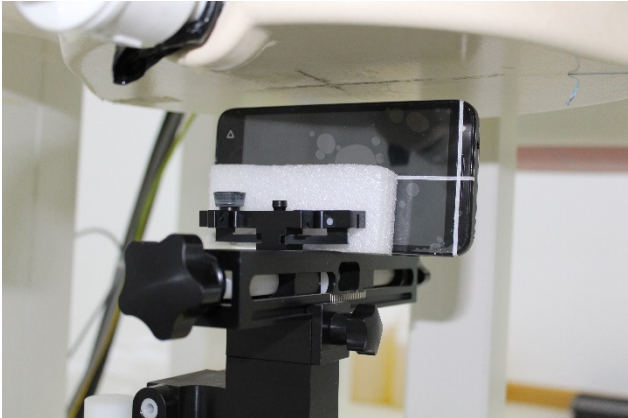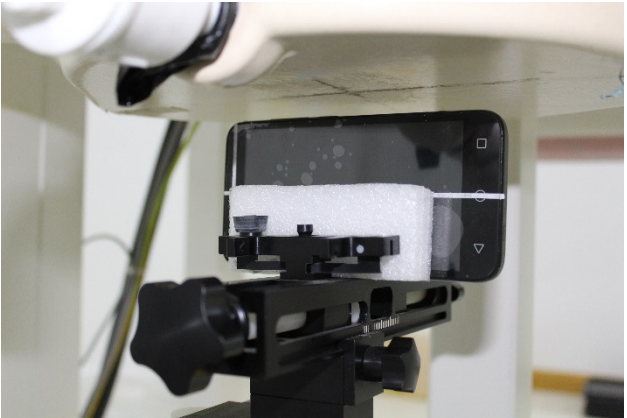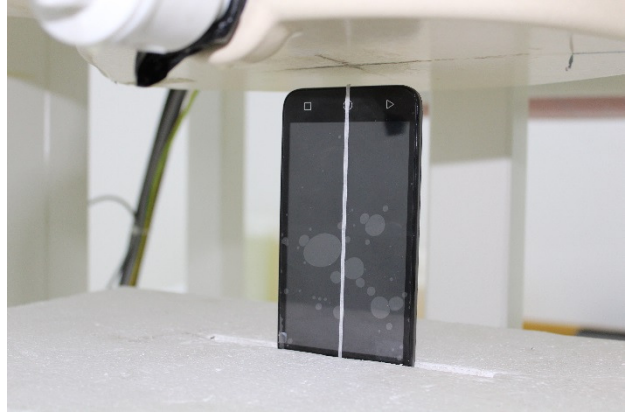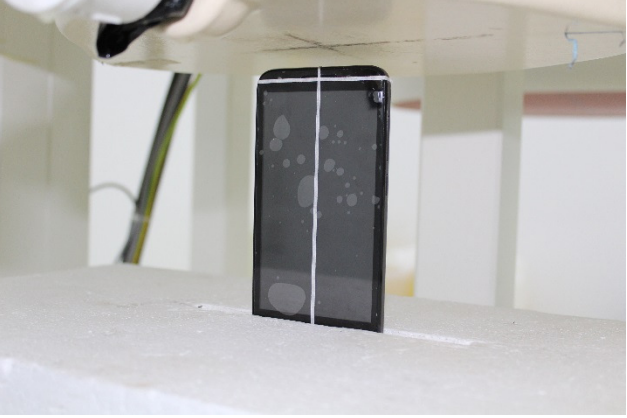