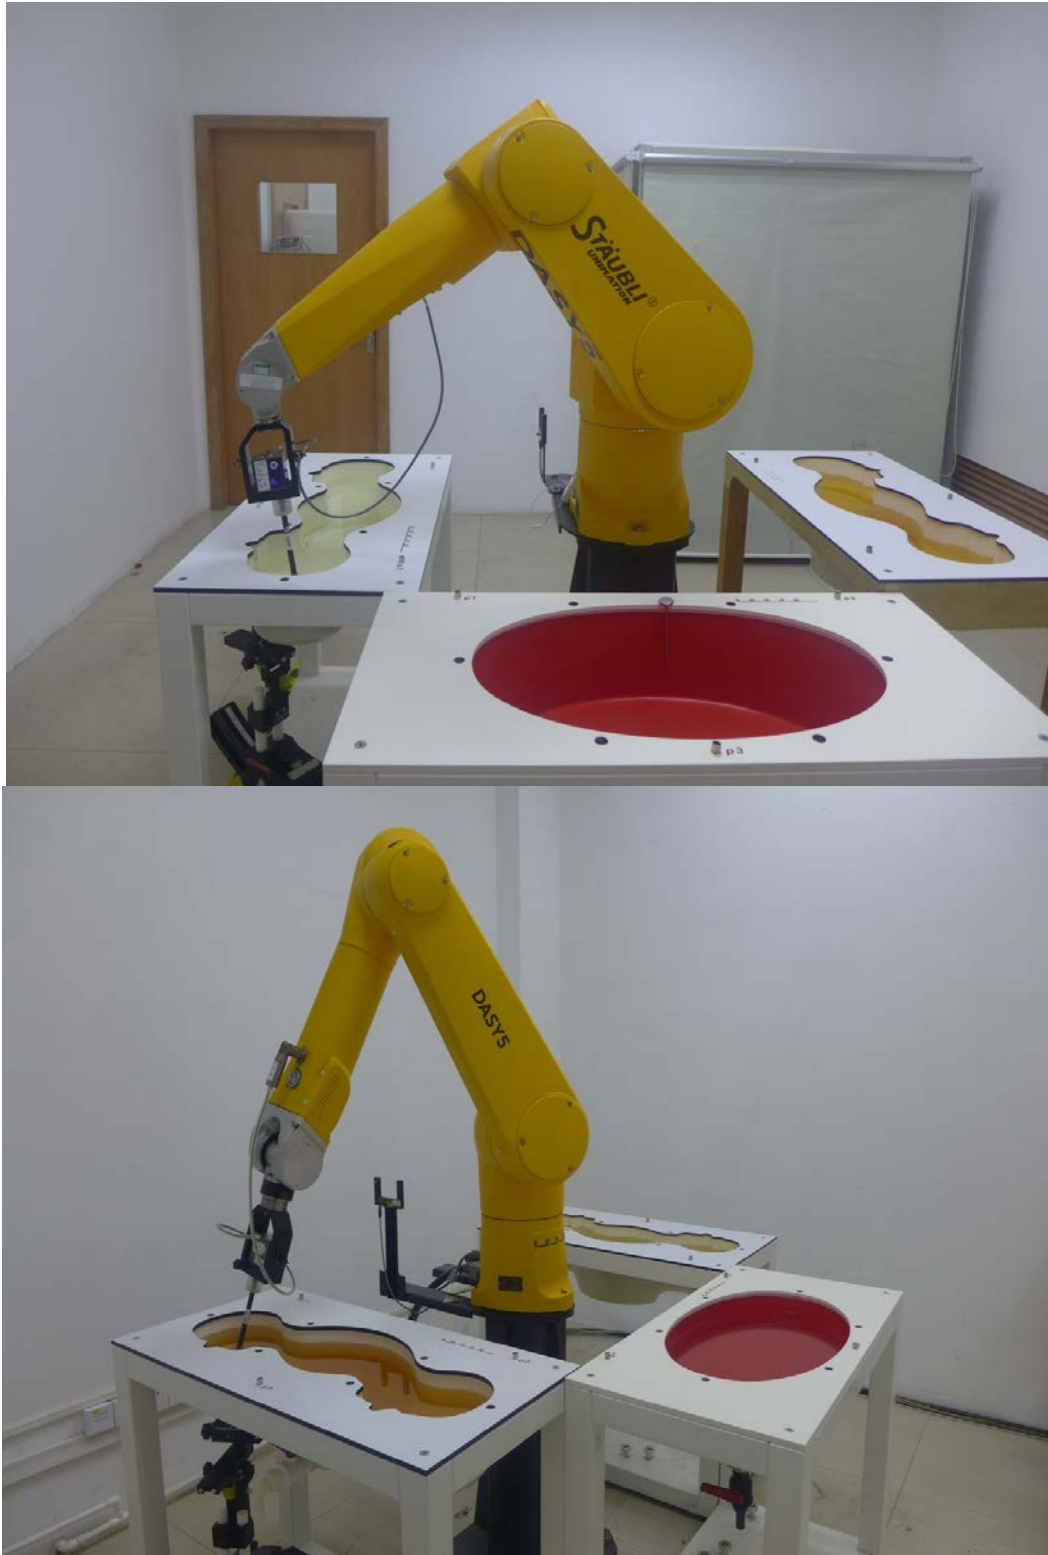


Appendix D

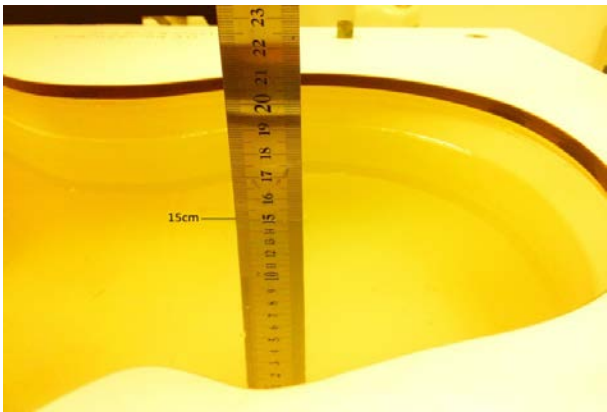
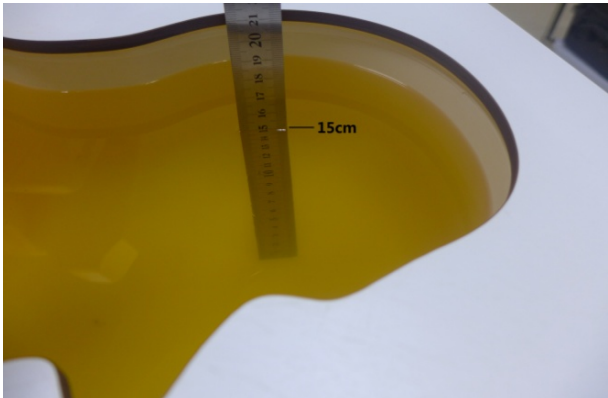
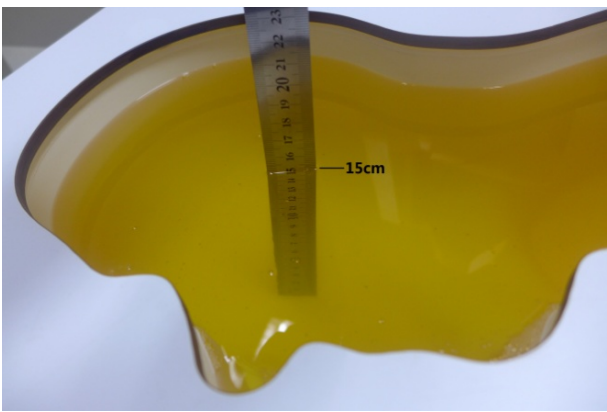
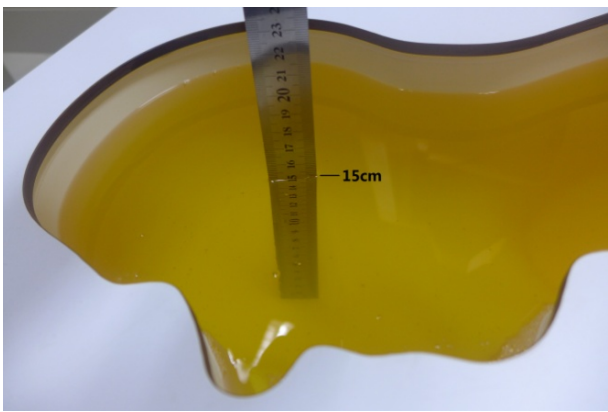
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1900
	
Photo 3: Tissue Simulant Liquid for Head 2450	Photo 4: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

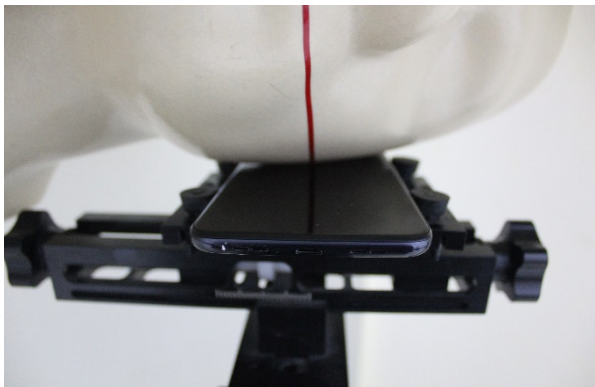
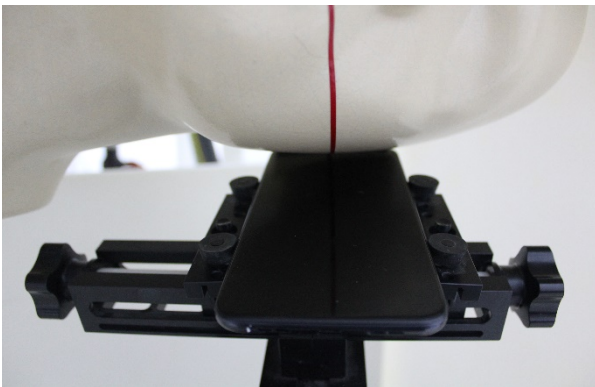
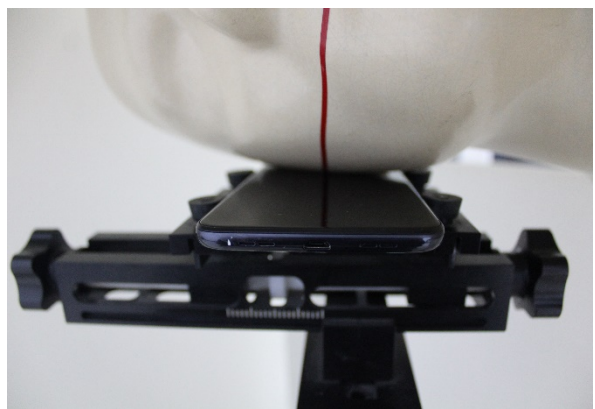
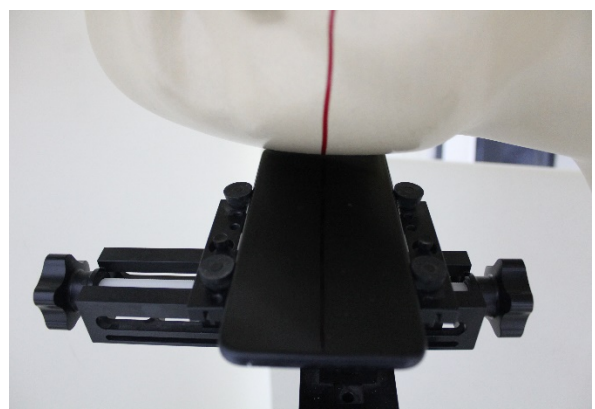
Photo 5: Left touch cheek	Photo 6: Left tilted 15 degree
	
Photo 7: Right touch cheek	Photo 8: Right tilted 15 degree
	

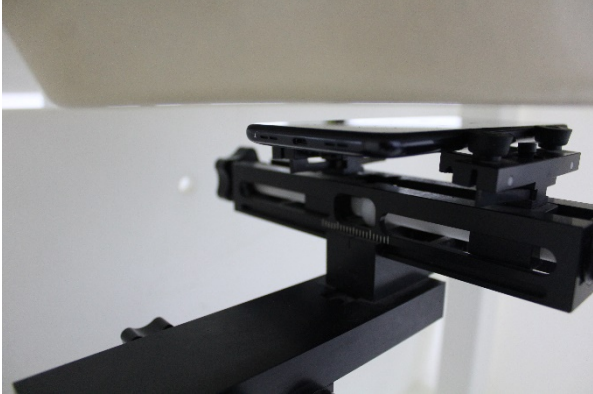
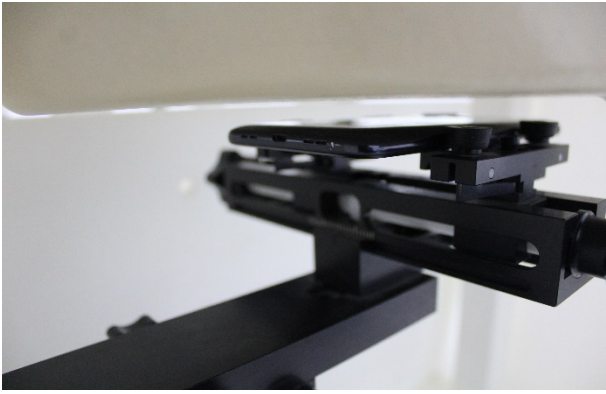
Photo 9: Front side 10mm	Photo 10: Back side 10mm
	
Photo 11: Left side 10mm	Photo 12: Right side 10mm
	
Photo 13: Top side 10mm	Photo 14: Bottom side 10mm
	

Photo 15: Bottom side 0mm	NA
	NA

4. EUT Constructional Details

Photo 16: Front View	Photo 17: Back View
	
Photo 18: Accessory	NA
	NA