

Date: 2025-09-07

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.912$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.66, 8.53, 8.82); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.28 W/kg; SAR (10g) = 1.61 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 21.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

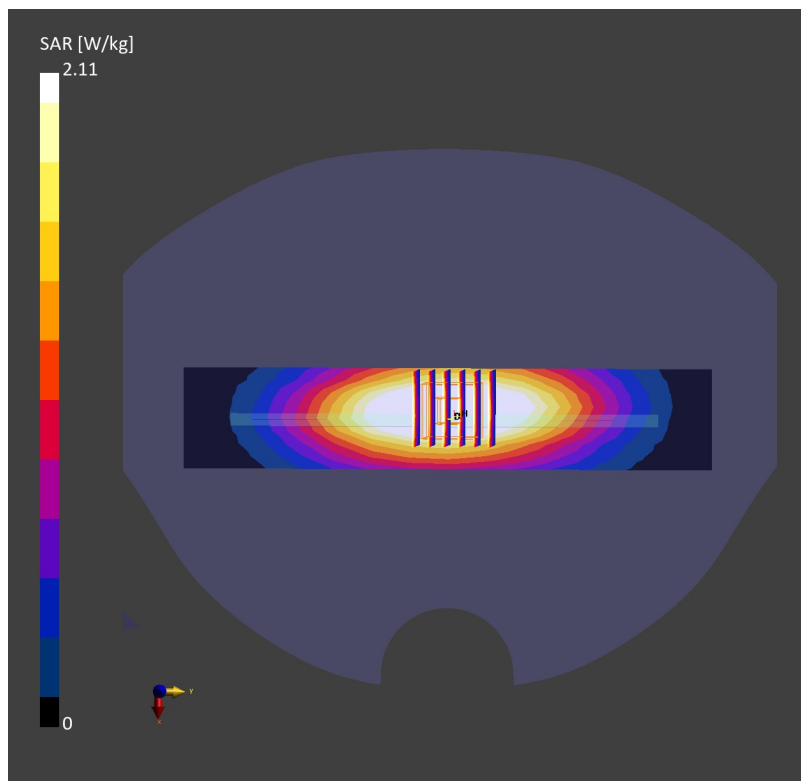

Date: 2025-09-09

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.933$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.55, 8.42, 8.7); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.46 W/kg; SAR (10g) = 1.74 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.08 dB

SAR (1g) = 2.32 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 17.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

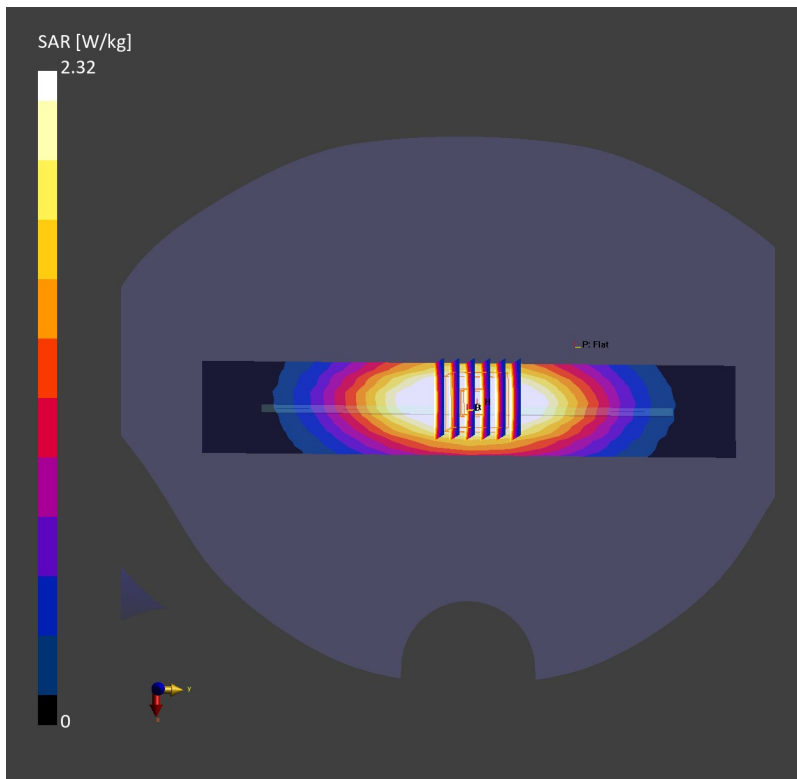

Date: 2025-09-10

System Check_1750MHz**DUT:D1750V2-SN:1137**


Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.9$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.34, 7.23, 7.47); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 9.33 W/kg; SAR (10g) = 4.89 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.04 dB
SAR (1g) = 9.16 W/kg; SAR (10g) = 4.79 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 84.8 %

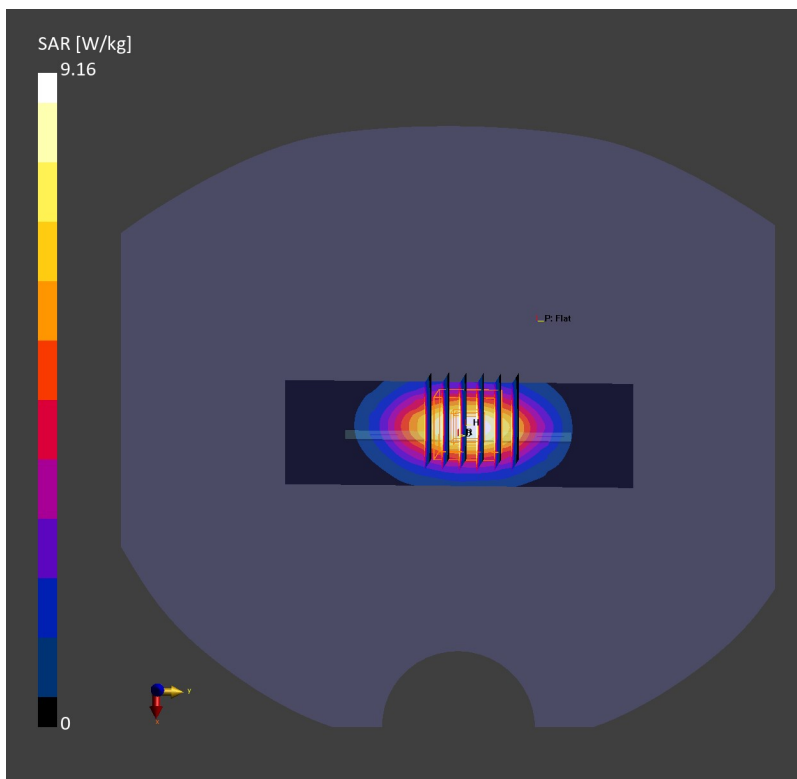

Date: 2025-09-08

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.15, 7.04, 7.28); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 10.8 W/kg; SAR (10g) = 5.28 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.15 dB

SAR (1g) = 10.2 W/kg; SAR (10g) = 5.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

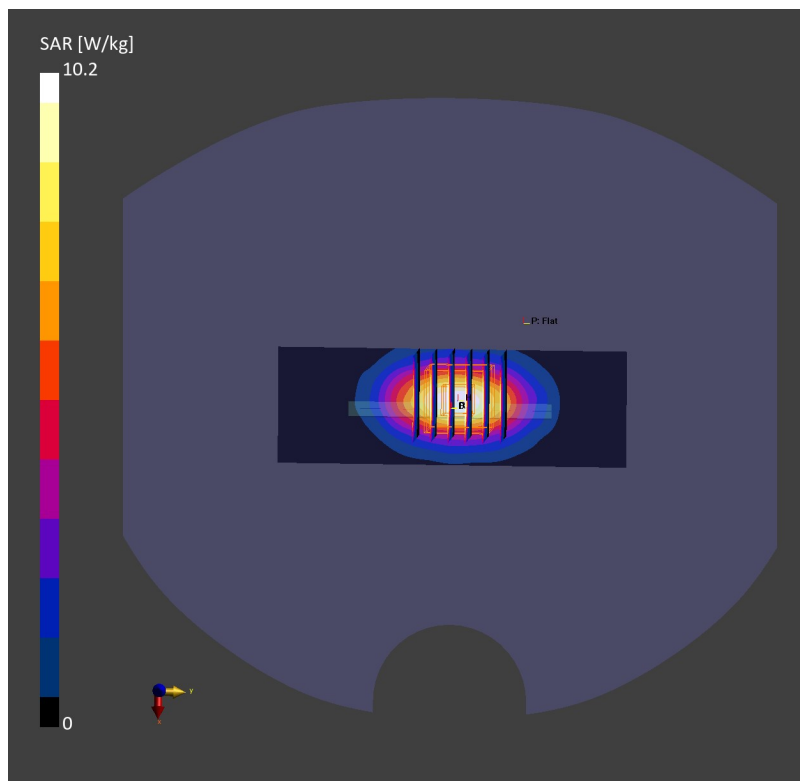

Date: 2025-09-13

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.78$ S/m; $\epsilon_r = 37.9$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.56, 6.78); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.8 W/kg; SAR (10g) = 6.36 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.08 dB
SAR (1g) = 13.3 W/kg; SAR (10g) = 6.25 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 82.3 %

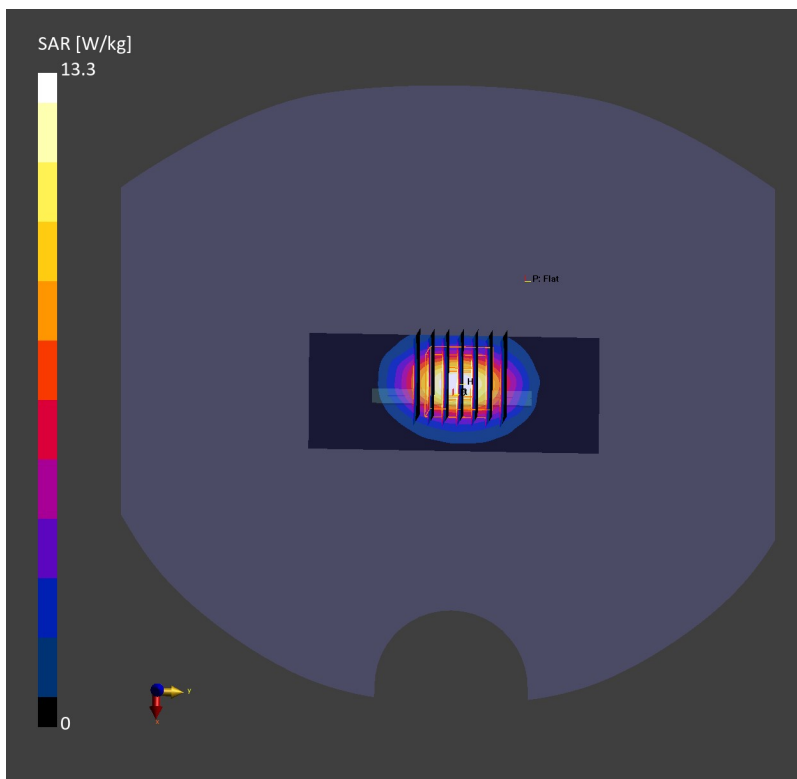

Date: 2025-09-14

System Check_2600MHz**DUT:D2600V2-SN:1070**


Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 2.05$ S/m; $\epsilon_r = 38.1$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.52, 6.42, 6.64); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 14.3 W/kg; SAR (10g) = 6.29 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 13.8 W/kg; SAR (10g) = 6.17 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.0 %

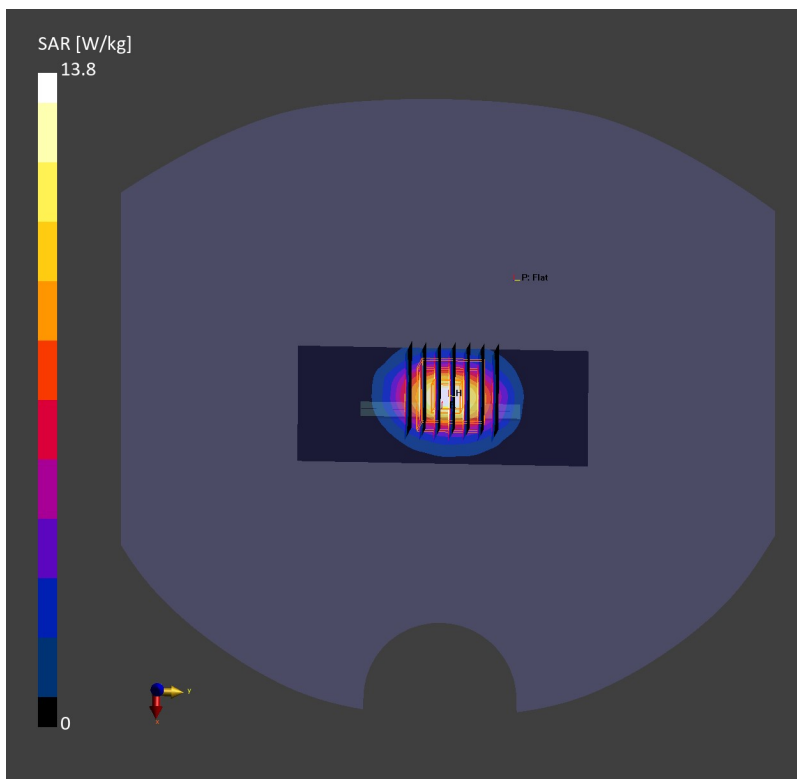

Date: 2025-09-15

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.58$ S/m; $\epsilon_r = 36.0$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(5.44, 5.36, 5.54); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.93 W/kg; SAR (10g) = 2.21 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 7.81 W/kg; SAR (10g) = 2.19 W/kg
Smallest distance from peaks to all points 3 dB below = 6.8 mm
Ratio of SAR at M2 to SAR at M1 = 65.4 %

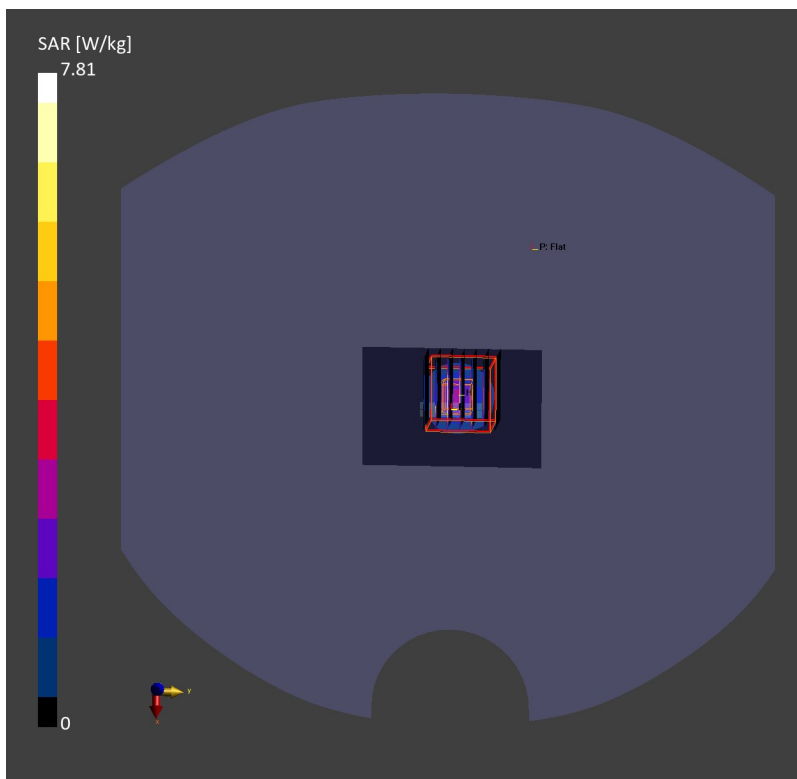

Date: 2025-09-18

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.93$ S/m; $\epsilon_r = 35.5$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.89, 4.82, 4.98); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.47 W/kg; SAR (10g) = 2.39 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.05 dB
SAR (1g) = 8.53 W/kg; SAR (10g) = 2.42 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 62.1 %

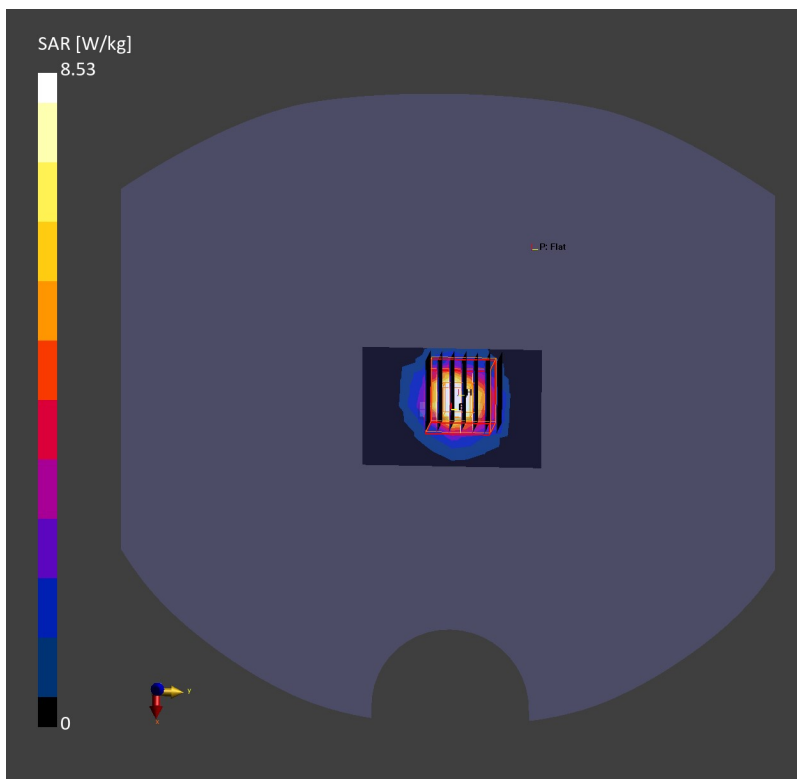

Date: 2025-09-17

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.14$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.86, 4.78, 4.94); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2024-12-17
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.94 W/kg; SAR (10g) = 2.25 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 8.04 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.1 %

