

SPEC NO.	eLB1392-074
REV	2.0
PAGE	1 OF 4

Melanie Webster
29 January 2021

Common labels/moulded in artwork




BRAND
ResMed branding
chrome or colour foiled
on front of product




“BF APPLIED PART”
Body Fibrillation Icon
Moulded into plastic case
using an insert
on rear of device,
adjacent to the device outlet



“R390-411 Label - MR Unsafe”
White pre-printed label stuck next to
power connector on rear of assembly

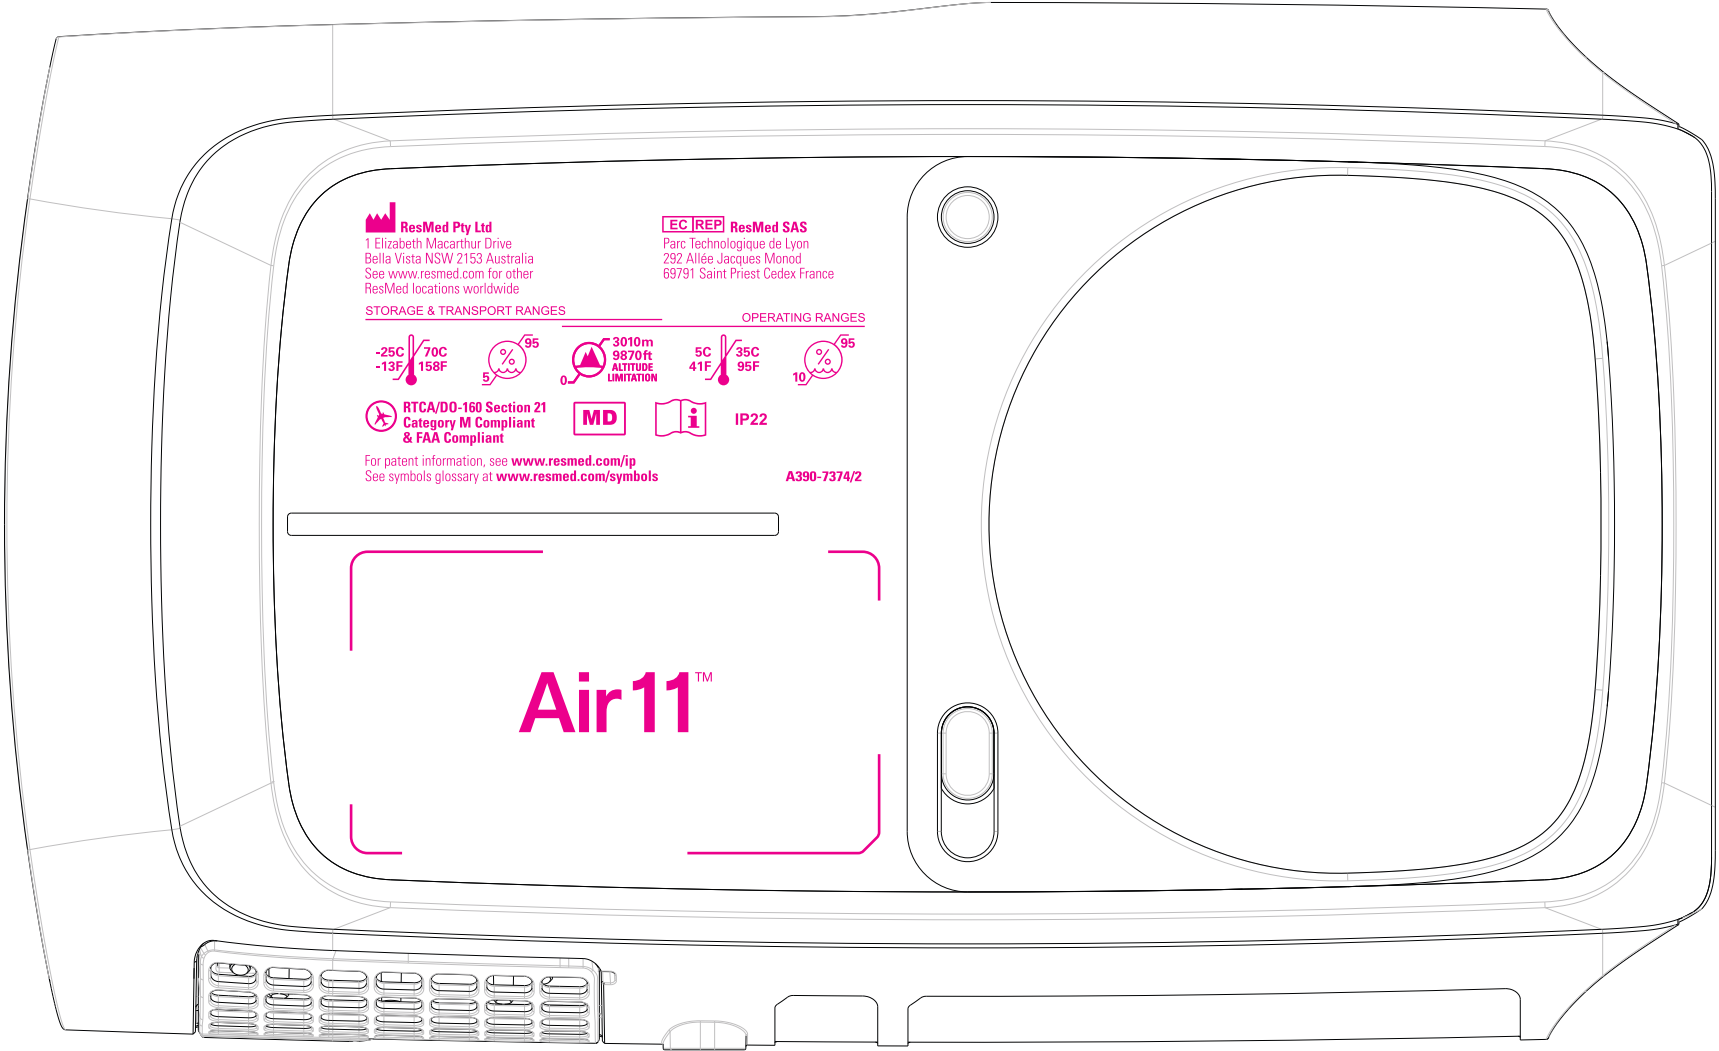

A390-7374 Bottom Case Assembly
Laser-Etched on bottom of chassis

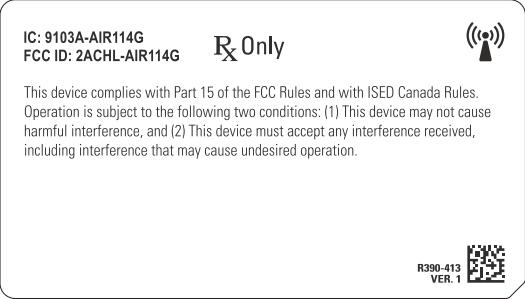

“R390-413 Label - FCC & IC NIR”
White pre-printed label
stuck on bottom of assembly

SPEC NO.	eLB1392-074
REV	2.0
PAGE	2 OF 4

Melanie Webster
29 January 2021

Product Specific Labels for FCC




39000 AirSense 11 AutoSet USA CO
(Base Code: 39420)

R390-7396



39002 AirSense 11 CPAP USA CO
(Base Code: 39421)

R390-7397

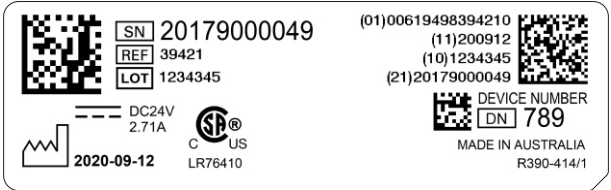

39004 AirSense 11 Elite USA CO
(Base Code: 39422)

R390-7398



PRODUCT NAME PLAQUES
Foiled product variant badges
“permanently” attached to front of product

SERIAL NUMBER LABELS
Thermally printed labels
attached to rear of product



39001 AirSense 11 AutoSet USA TRI
(Base Code: 39420)

R390-7396



39003 AirSense 11 CPAP USA TRI
(Base Code: 39421)

R390-7397



39005 AirSense 11 Elite USA TRI
(Base Code: 39422)

R390-7398



NOTE:
- The device ID is the base code, which can be packaged in different boxes of accessories
- CO means it is packed with a humidifier.
- TRI means it is packed with a humidifier and heated tube.

29 January 2021

A close-up of the AirSense 11 AUTASET CPAP mask, showing the front panel with the brand name and model.A close-up image of the AirSense 11 CPAP device, showing the mask and the device's interface. The device is black and white, with the text "AirSense 11" and "CPAP" visible on the front.A close-up image of the AirSense 11 ELITE CPAP mask, showing the front panel with the brand name and model.



SN	20179000049
REF	39423
LOT	234345




DC24V
2.71A


C US
LR76410

(01)00619498394234
 (11)200912
 (10)1234345
 (21)20179000049


 DEVICE NUMBER
DN 789

MADE IN AUSTRALIA
 R390-414/1

2020-09-12

Barcode: 20179000049

SN: 39424

REF: 1234345

LOT: 1234345

(01)00619498394241

(11)200912

(10)1234345

(21)20179000049

DC2V 2.71A

DATE: 2020-09-12

CE MARKING: C US

LR76410

DEVICE NUMBER: DN 789

MADE IN AUSTRALIA

R390-414/1

A close-up of the AirSense 11 AUTASET CPAP device, showing the mask and the device's interface. The device is white with a black mask. The text "AirSense 11" and "AUTASET" is visible on the device.A close-up of the AirSense 11 CPAP device, showing the mask and the device's interface. The device is white and black, with the text "AirSense 11" and "CPAP" visible.A close-up image of the AirSense 11 ELITE CPAP mask, showing the front panel with the brand name and model.

Bottom section of the label. On the left is a barcode. To its right is a table with three rows: 'SN' with value '20179000049', 'REF' with value '39423', and 'LOT' with value '1234345'. To the right of this table is the text '(01)00619498394234', '(11)200912', '(10)1234345', and '(21)20179000049'. Further right is another barcode. Below the barcode on the right is the text 'DEVICE NUMBER' and 'DN 789'. At the bottom right is the text 'MADE IN AUSTRALIA' and 'R390-414/1'. In the bottom left corner is a triangle symbol with a wavy line inside, followed by the date '2020-09-12'. In the bottom center is the 'SP' logo with 'C' and 'US' on either side, and 'LR76410' below it.



SN	20179000049
REF	39424
LOT	1234345

(01)00619498394241
(11)200912
(10)1234345
(21)20179000049



DC24V
2.71A



2020-09-12


 C⁺ US
 LR76410

DEVICE NUMBER
DN 789

MADE IN AUSTRALIA
R390-414/1

Thermally printed labels
attached to rear of product

- The device ID is the base code, which can be packaged in different boxes of accessories
- CO means it is packed with a humidifier.
- TRI means it is packed with a humidifier and heated tube.

SPEC NO.	eLB1392-074
REV	2.0
PAGE	4 OF 4

Melanie Webster
29 January 2021



FRONT VIEW



SIDE VIEW



REAR VIEW



BOTTOM VIEW