Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

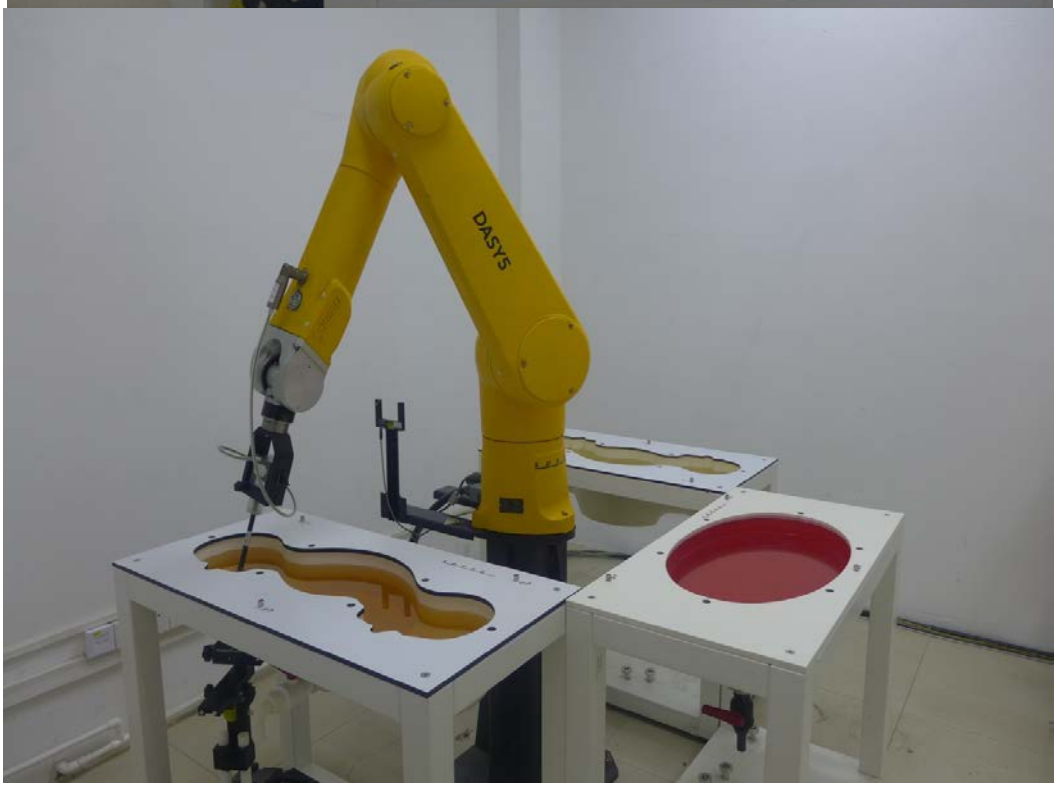

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
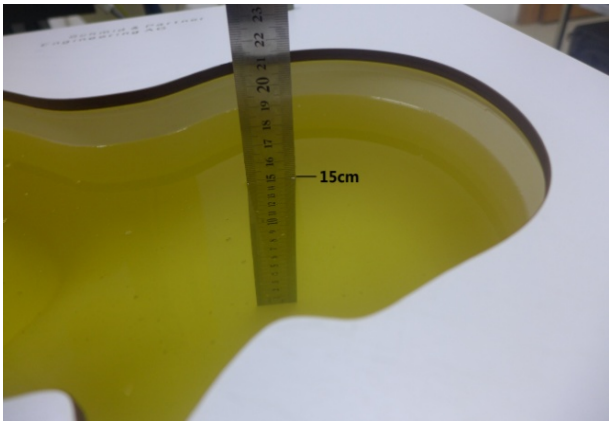	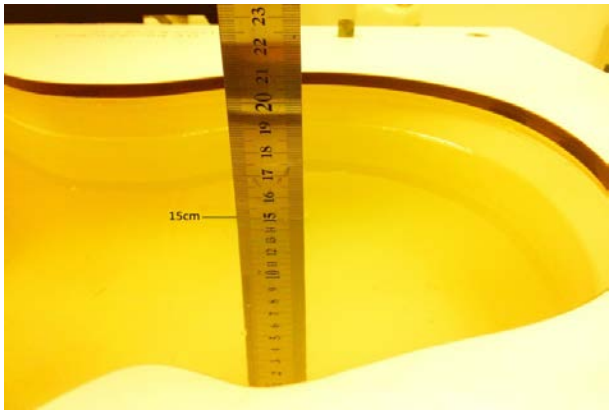
Photo 3: Tissue Simulant Liquid for Head 1750	**Photo 4: Tissue Simulant Liquid for Head 1900**
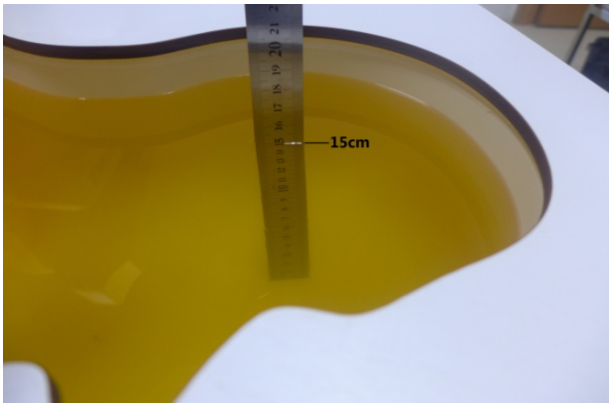	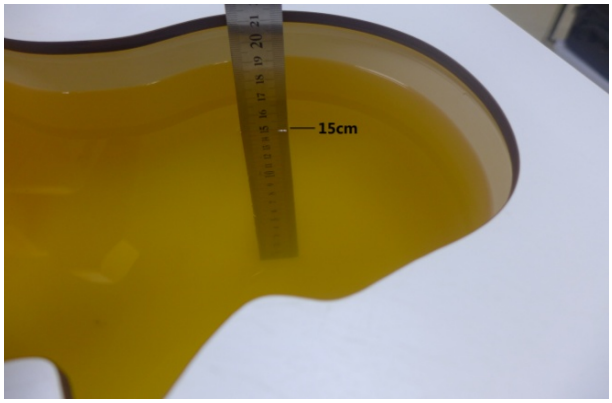
Photo 5: Tissue Simulant Liquid for Head 2450	**Photo 6: Tissue Simulant Liquid for Head 2600**
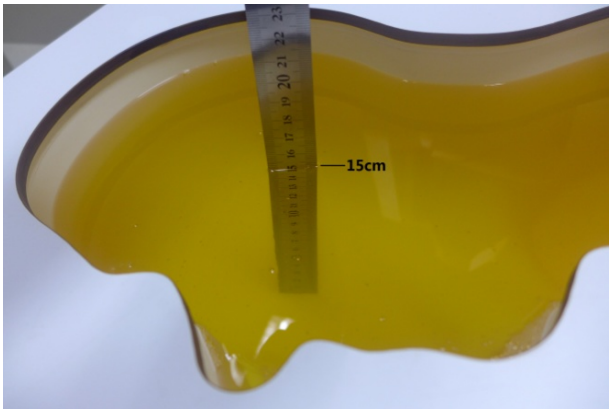	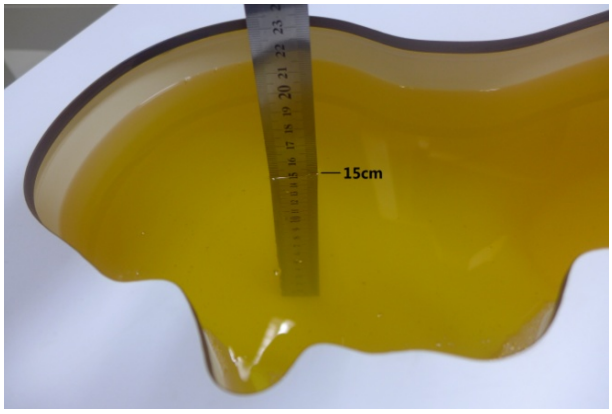

Photo 7: Tissue Simulant Liquid for Head 5G	NA
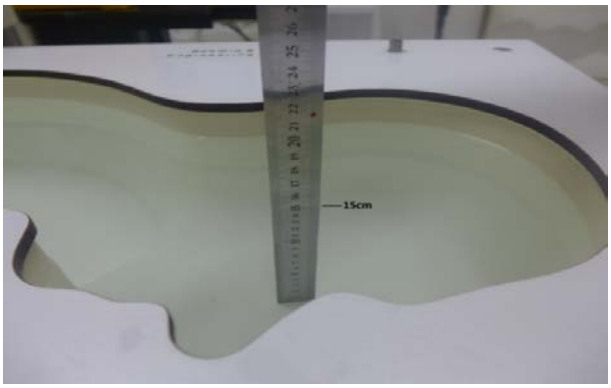	NA

3. Photographs of EUT test position

Photo 8: Left touch cheek	Photo 9: Left tilted 15 degree
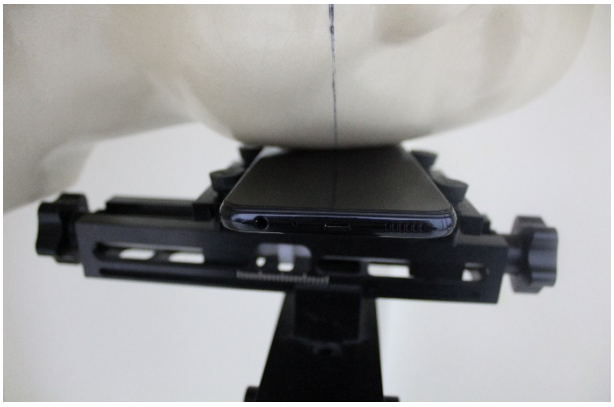	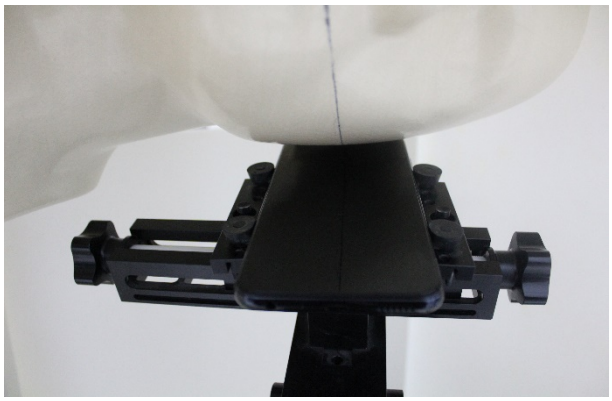
Photo 10: Right touch cheek	**Photo 11: Right tilted 15 degree**
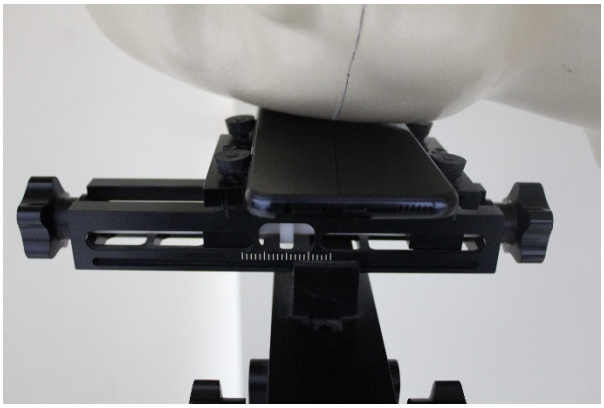	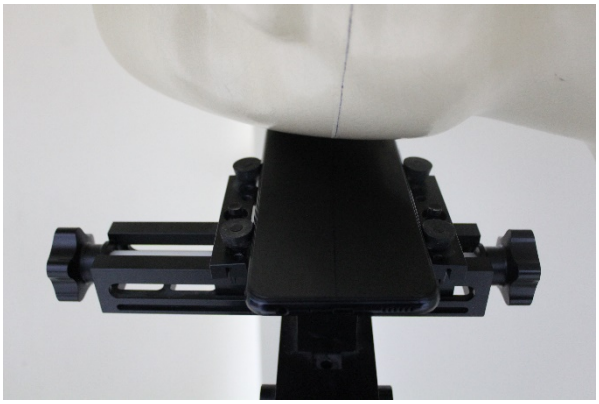
Photo 12: Front side 15mm	**Photo 13: Back side 15mm**
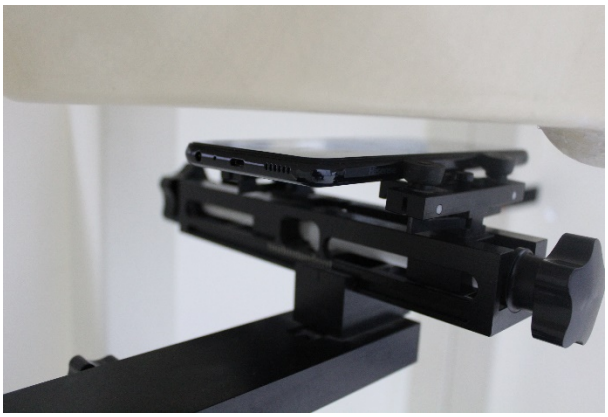	

Photo 14: Front side 10mm	Photo 15: Back side 10mm
Photo 16: Left side 10mm	**Photo 17: Right side 10mm**
Photo 18: Top side 10mm	**Photo 19: Bottom side 10mm**
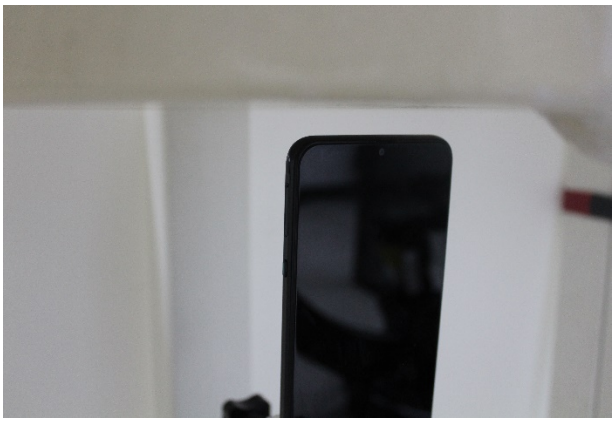	

Photo 20: Front side 0mm	Photo 21: Back side 0mm
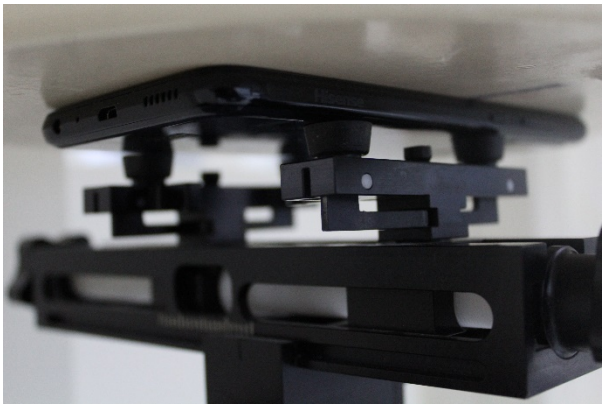	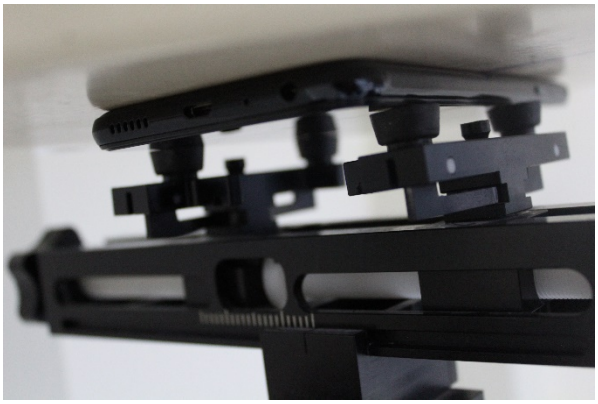
Photo 22: Right side 0mm	**Photo 23: Top side 0mm**
	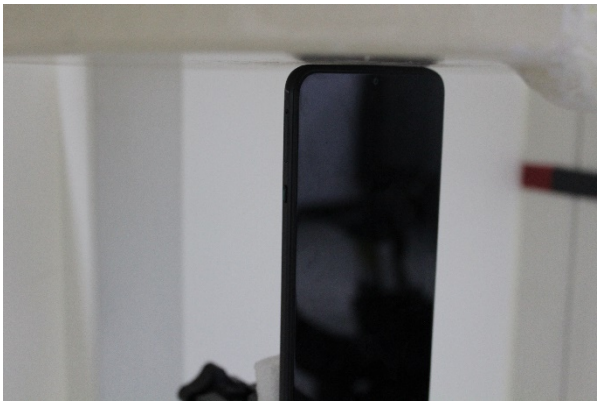
Photo 24: Bottom side 0mm	**NA**
	NA

Photo 25: Left touch cheek with back cover	Photo 26: Left tilted 15 degree with back cover
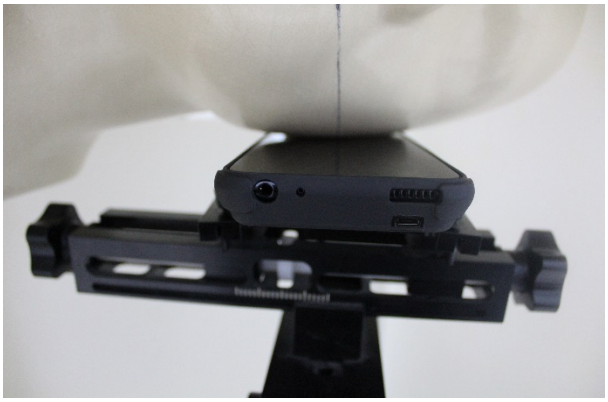	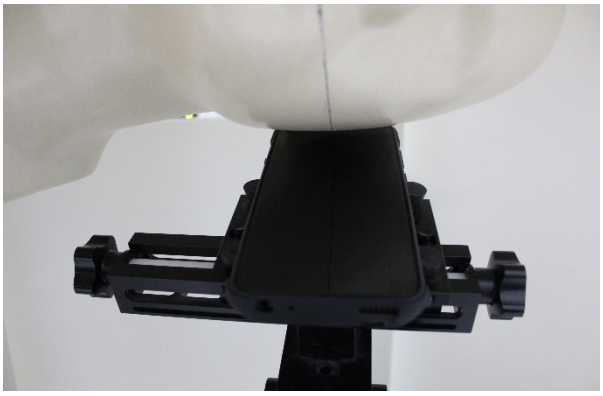
Photo 27: Right touch cheek with back cover	**Photo 28: Right tilted 15 degree with back cover**
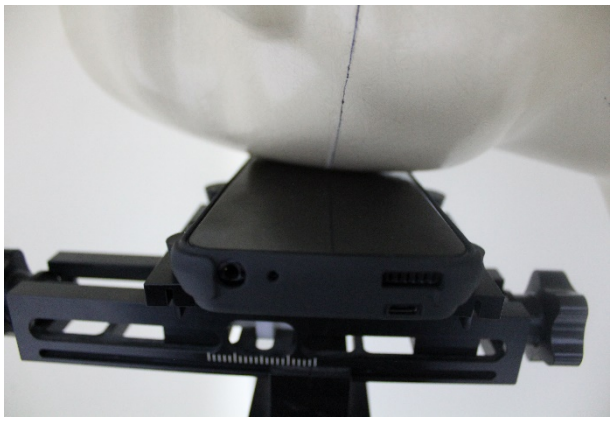	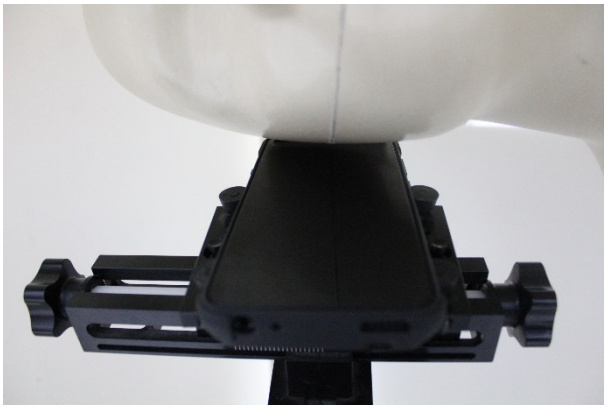
Photo 29: Front side 15mm with back cover	**Photo 30: Back side 15mm with back cover**
	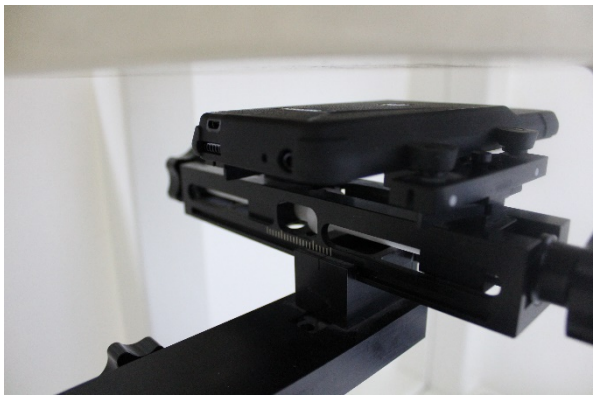

Photo 31: Front side 10mm with back cover	Photo 32: Back side 10mm with back cover
Photo 33: Left side 10mm with back cover	**Photo 34: Right side 10mm with back cover**
Photo 35: Top side 10mm with back cover	**Photo 36: Bottom side 10mm with back cover**
	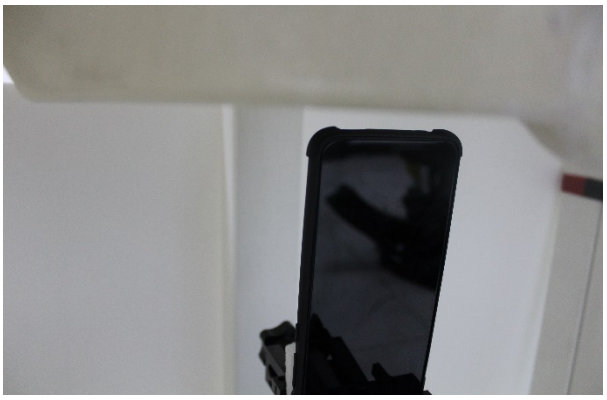

Photo 37: Top side 0mm with back cover	Photo 38: Bottom side 0mm with back cover

4. EUT Constructional Details

Photo 39: Front View	Photo 40: Back View
Photo 41: Accessory	