

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid (Body)

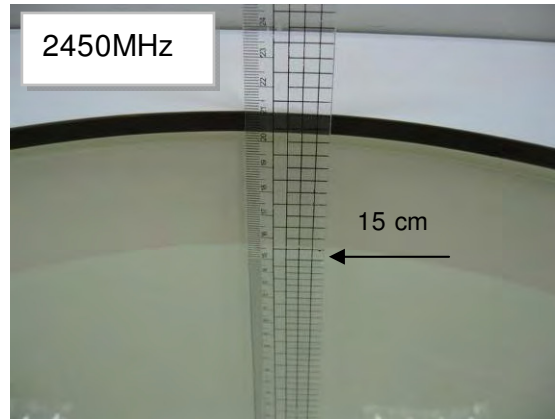


Fig.2

Extremity exposure - distance between flat phantom and backside of device is 0 mm



Fig.3 EUT Back side to flat phantom

12. Photographs of the EUT



Fig.4 Front view of EUT



Fig.5 Back view of EUT

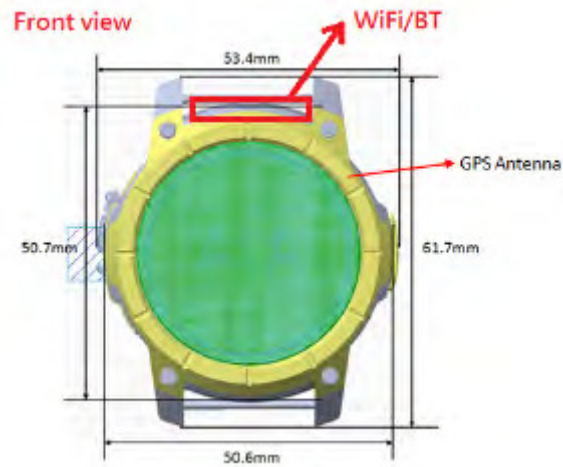


Fig.6 Antenna position of EUT (front view)

- End of Report -