

### Head TSL parameters at 5300 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.9         | 4.76 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.7 ±6%     | 4.60 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5300 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.06 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 80.6 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.33 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 23.3 W/kg ±19.5% (k = 2) |

### Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.6         | 4.96 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.3 ±6%     | 4.82 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5500 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.56 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 85.6 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.45 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.5 W/kg ±19.5% (k = 2) |

### Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.5         | 5.07 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.1 ±6%     | 4.94 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5600 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.33 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 83.3 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.41 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.1 W/kg ±19.5% (k = 2) |

### Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.3         | 5.27 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 34.9 ±6%     | 5.15 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5800 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 7.90 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 79.0 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.27 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 22.7 W/kg ±19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 5200 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 53.3 $\Omega$ – 4.8 j $\Omega$ |
| Return Loss | -25.0 dB                       |

**Antenna Parameters with Head TSL at 5300 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 48.4 $\Omega$ + 2.0 j $\Omega$ |
| Return Loss | -31.6 dB                       |

**Antenna Parameters with Head TSL at 5500 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 47.6 $\Omega$ – 2.2 j $\Omega$ |
| Return Loss | -29.5 dB                       |

**Antenna Parameters with Head TSL at 5600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 55.9 $\Omega$ + 0.5 j $\Omega$ |
| Return Loss | -25.1 dB                       |

**Antenna Parameters with Head TSL at 5800 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 50.5 $\Omega$ + 4.2 j $\Omega$ |
| Return Loss | -27.5 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.207 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1412 | 5200            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5200, 0                         | 5.68              | 4.51                   | 35.9             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-17    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-17          |
| psSAR1g [W/Kg]      | 7.60                |
| psSAR10g [W/Kg]     | 2.20                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

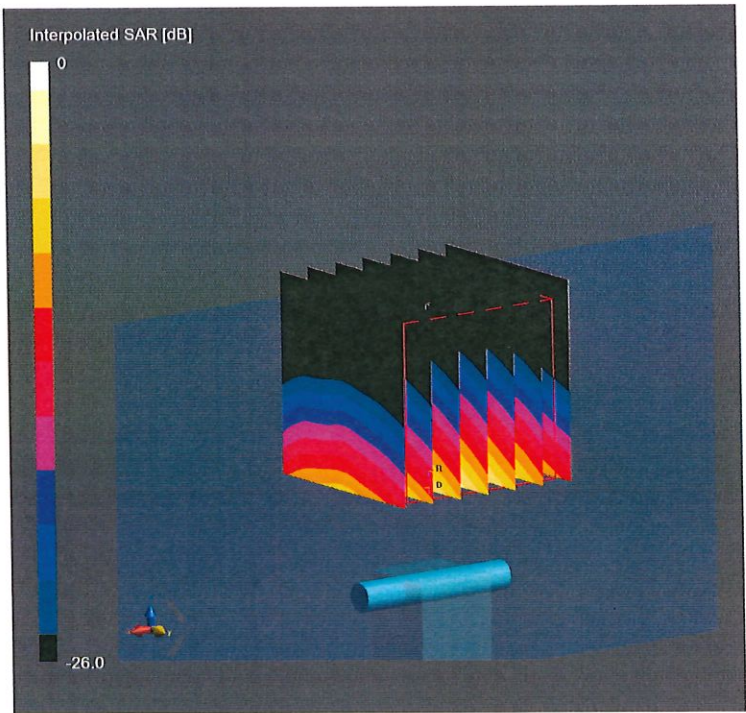

0 dB = 30.4 W/Kg

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1412 | 5300            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5300, 0                         | 5.45              | 4.60                   | 35.7             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-17    | EX3DV4 - SN7349, 2024-06-03 | DAE4lp Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-17          |
| psSAR1g [W/Kg]      | 8.06                |
| psSAR10g [W/Kg]     | 2.33                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

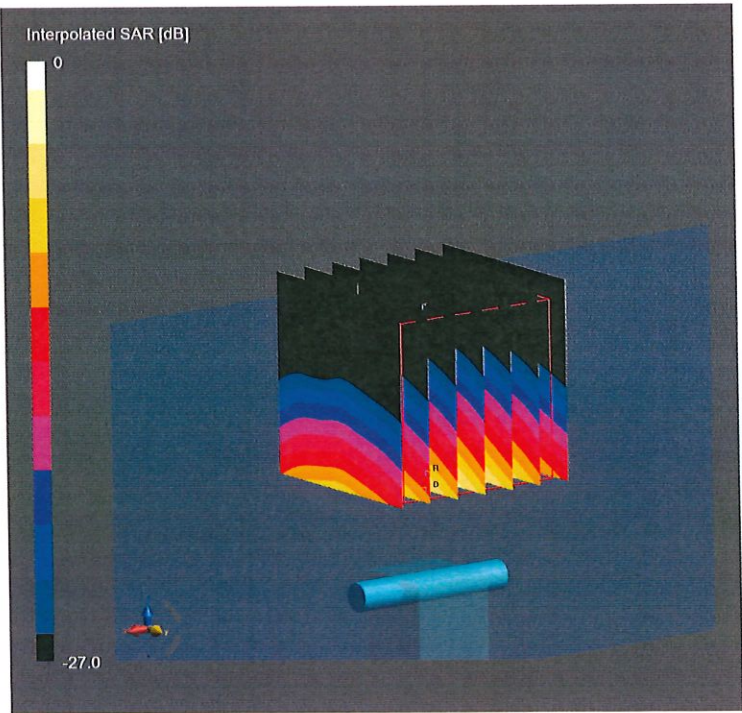

0 dB = 33.1 W/Kg

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1412 | 5500            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5500, 0                         | 5.07              | 4.82                   | 35.3             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-17    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-17          |
| psSAR1g [W/Kg]      | 8.56                |
| psSAR10g [W/Kg]     | 2.45                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

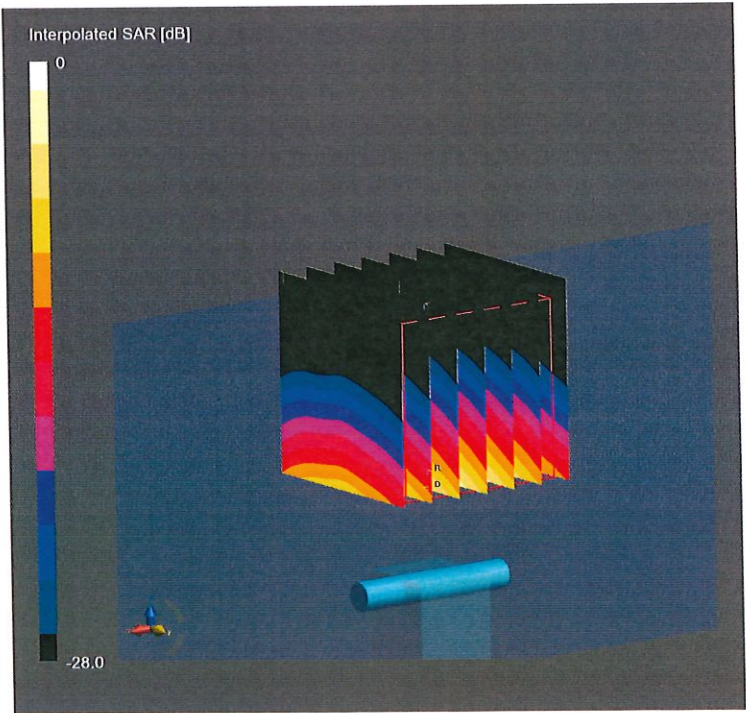

0 dB = 36.7 W/Kg

## System Performance Check Report

## Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1412 | 5600            | HSL | 20          |

## Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5600, 0                         | 5.03              | 4.94                   | 35.1             |

## Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-17    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

## Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

## Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-17          |
| psSAR1g [W/Kg]      | 8.33                |
| psSAR10g [W/Kg]     | 2.41                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

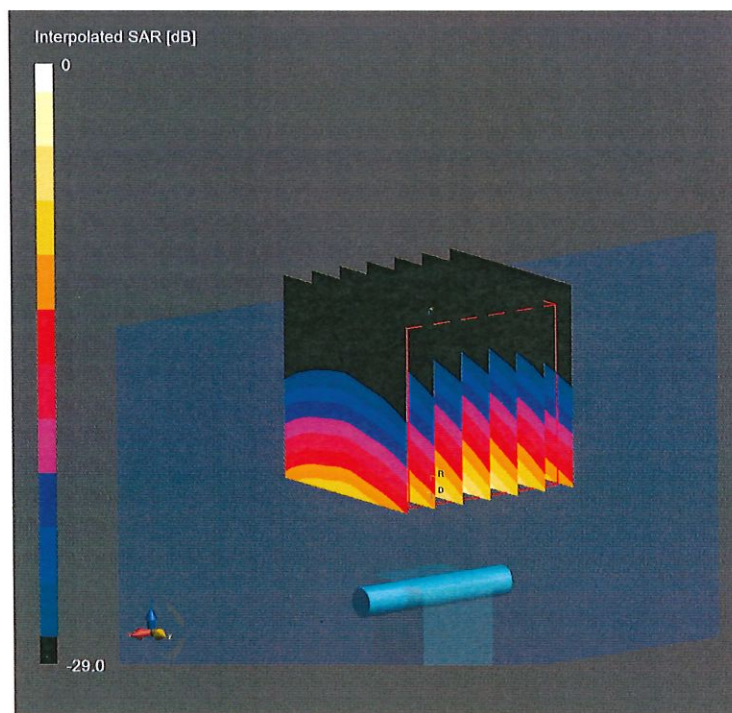

System Performance Check Report


|                  |                 |     |             |
|------------------|-----------------|-----|-------------|
| Summary          |                 |     |             |
| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
| D5GHzV2 – SN1412 | 5800            | HSL | 20          |

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Exposure Conditions  |                    |      |            |                                 |                   |                        |                  |
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat                 | 10                 |      | CW, 0--    | 5800, 0                         | 5.08              | 5.15                   | 34.9             |

|                 |                    |                             |                           |
|-----------------|--------------------|-----------------------------|---------------------------|
| Hardware Setup  |                    |                             |                           |
| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
| MFP V8.0 Center | HSL, 2024-10-17    | EX3DV4 – SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

|                     |                 |
|---------------------|-----------------|
| Scans Setup         |                 |
|                     | Zoom Scan       |
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |



|                     |                     |
|---------------------|---------------------|
| Measurement Results |                     |
|                     | Zoom Scan           |
| Date                | 2024-10-17          |
| psSAR1g [W/Kg]      | 7.90                |
| psSAR10g [W/Kg]     | 2.27                |
| Power Drift [dB]    | -0.01               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

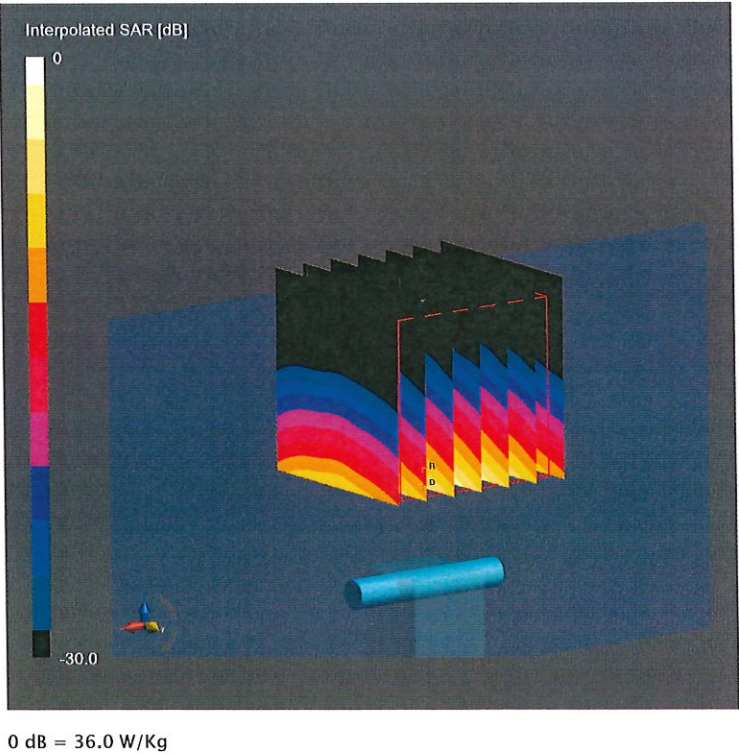

Impedance Measurement Plot for Head TSL

S11 Smith (R+jX) Scale 1.00

|    |              |                 |                   |
|----|--------------|-----------------|-------------------|
| >1 | 5.200000 GHz | 53.331 $\Omega$ | -4.787 j $\Omega$ |
| >2 | 5.300000 GHz | 48.405 $\Omega$ | 2.049 j $\Omega$  |
| >3 | 5.500000 GHz | 47.552 $\Omega$ | -2.187 j $\Omega$ |
| >4 | 5.600000 GHz | 55.889 $\Omega$ | 0.477 j $\Omega$  |
| >5 | 5.800000 GHz | 50.472 $\Omega$ | 4.191 j $\Omega$  |

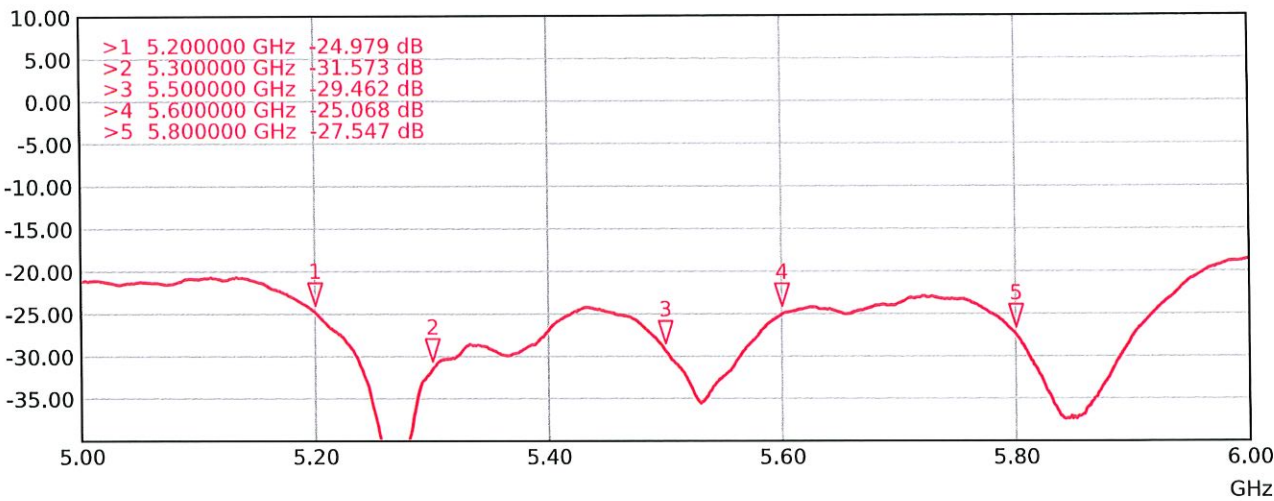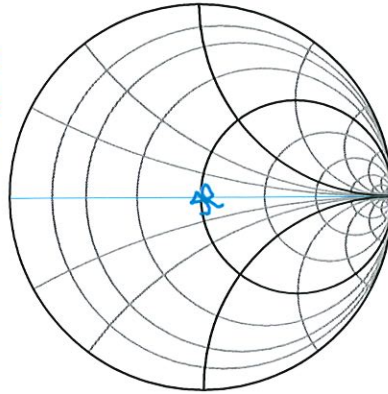



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **WSCT**  
Shenzhen

Certificate No: **DAE4ip-1872\_Oct24**

## CALIBRATION CERTIFICATE

Object **DAE4ip - SD 000 D14 AG - SN: 1872**

Calibration procedure(s) **QA CAL-06.v30**  
**Calibration procedure for the data acquisition electronics (DAE)**


Calibration date: **October 18, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards             | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 0810278        | 27-Aug-24 (No:40547)       | Aug-25                 |
| Secondary Standards           | ID #               | Check Date (in house)      | Scheduled Check        |
| Auto DAE Calibration Unit     | SE UWS 053 AA 1001 | 23-Jan-24 (in house check) | In house check: Jan-25 |
| Calibrator Box V2.1           | SE UMS 006 AA 1002 | 23-Jan-24 (in house check) | In house check: Jan-25 |

|                |                        |                                   |                                                                                                    |
|----------------|------------------------|-----------------------------------|----------------------------------------------------------------------------------------------------|
| Calibrated by: | Name<br>Adrian Gehring | Function<br>Laboratory Technician | Signature<br> |
| Approved by:   | Sven Kühn              | Technical Manager                 |               |

Issued: October 18, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

## Glossary

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 405.516 $\pm$ 0.02% (k=2) | 405.743 $\pm$ 0.02% (k=2) | 405.517 $\pm$ 0.02% (k=2) |
| Low Range           | 3.97808 $\pm$ 1.50% (k=2) | 3.99468 $\pm$ 1.50% (k=2) | 3.97864 $\pm$ 1.50% (k=2) |

## Connector Angle

|                                           |                   |
|-------------------------------------------|-------------------|
| Connector Angle to be used in DASY system | 206.5 ° $\pm$ 1 ° |
|-------------------------------------------|-------------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range        | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 199998.14                 | 1.11                         | 0.00      |
| Channel X + Input | 20003.88                  | 1.08                         | 0.01      |
| Channel X - Input | -20001.65                 | 0.61                         | -0.00     |
| Channel Y + Input | 199999.84                 | 2.82                         | 0.00      |
| Channel Y + Input | 20001.02                  | -1.73                        | -0.01     |
| Channel Y - Input | -20002.12                 | 0.19                         | -0.00     |
| Channel Z + Input | 199995.41                 | -1.01                        | -0.00     |
| Channel Z + Input | 20001.78                  | -0.94                        | -0.00     |
| Channel Z - Input | -20002.55                 | -0.24                        | 0.00      |

| Low Range         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 2001.17                   | -0.31                        | -0.02     |
| Channel X + Input | 202.08                    | 0.64                         | 0.32      |
| Channel X - Input | -197.21                   | 0.83                         | -0.42     |
| Channel Y + Input | 2001.25                   | 0.08                         | 0.00      |
| Channel Y + Input | 201.01                    | -0.31                        | -0.16     |
| Channel Y - Input | -198.91                   | -0.55                        | 0.28      |
| Channel Z + Input | 2001.51                   | 0.45                         | 0.02      |
| Channel Z + Input | 200.43                    | -0.89                        | -0.44     |
| Channel Z - Input | -199.69                   | -1.39                        | 0.70      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | 19.34                                        | 18.17                                       |
|           | - 200                          | -17.47                                       | -18.30                                      |
| Channel Y | 200                            | 6.89                                         | 6.47                                        |
|           | - 200                          | -6.94                                        | -7.73                                       |
| Channel Z | 200                            | 10.21                                        | 9.75                                        |
|           | - 200                          | -12.83                                       | -12.52                                      |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | 0.42                        | -2.57                       |
| Channel Y | 200                | 5.19                        | -                           | 2.08                        |
| Channel Z | 200                | 8.69                        | 2.55                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15797            | 17374           |
| Channel Y | 16064            | 13550           |
| Channel Z | 15971            | 14566           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.67               | 0.01                   | 1.30                   | 0.27                      |
| Channel Y | -0.40              | -1.22                  | 0.56                   | 0.36                      |
| Channel Z | -0.58              | -1.57                  | 0.50                   | 0.51                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |

Client : **WSCT**

Certificate No: **24J02Z000415**

## CALIBRATION CERTIFICATE

Object **DAE4 - SN: 1495**

Calibration Procedure(s) **FF-Z11-002-01**  
**Calibration Procedure for the Data Acquisition Electronics (DAEx)**


Calibration date: **July 24, 2024**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards      | ID #    | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|------------------------|---------|------------------------------------------|-----------------------|
| Process Calibrator 753 | 1971018 | 11-Jun-24 (CTTL, No.24J02X005147)        | Jun-25                |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Yu Zongying | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: August 01, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

### Glossary:

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

### Methods Applied and Interpretation of Parameters:

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 404.380 $\pm$ 0.15% (k=2) | 404.618 $\pm$ 0.15% (k=2) | 404.873 $\pm$ 0.15% (k=2) |
| Low Range           | 3.96611 $\pm$ 0.7% (k=2)  | 3.97363 $\pm$ 0.7% (k=2)  | 3.99493 $\pm$ 0.7% (k=2)  |

## Connector Angle

|                                           |                |
|-------------------------------------------|----------------|
| Connector Angle to be used in DASY system | 109° $\pm$ 1 ° |
|-------------------------------------------|----------------|

Client

**WSCT**

**Certificate No: 24J02Z000487**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN : 7391**

Calibration Procedure(s) **FF-Z11-004-02**  
**Calibration Procedures for Dosimetric E-field Probes**

Calibration date: **August 29, 2024**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards        | ID #               | Cal Date(Calibrated by, Certificate No.)  | Scheduled Calibration |
|--------------------------|--------------------|-------------------------------------------|-----------------------|
| Power Meter NRP2         | 106277             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Power sensor NRP8S       | 104291             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Power sensor NRP8S       | 104292             | 19-Oct-23(CTTL, No.J23X11026)             | Oct-24                |
| Reference 10dBAttenuator | 18N50W-10dB        | 19-Jan-23(CTTL, No.J23X00212)             | Jan-25                |
| Reference 20dBAttenuator | 18N50W-20dB        | 19-Jan-23(CTTL, No.J23X00211)             | Jan-25                |
| Reference Probe EX3DV4   | SN 7307            | 28-May-24(SPEAG, No.EX-7307_May24)        | May-25                |
| DAE4                     | SN 771             | 19-Jan-24(SPEAG, No.DAE4-771_Jan24)       | Jan-25                |
| Secondary Standards      | ID #               | Cal Date(Calibrated by, Certificate No.)  | Scheduled Calibration |
| SignalGenerator MG3700A  | 6201052605         | 12-Jun-24(CTTL, No.24J02X005419)          | Jun-25                |
| SignalGenerator APSIN26G | 181-33A6D0700-1959 | 26-Mar-24(CTTL, No.24J02X002468)          | Mar-25                |
| Network Analyzer E5071C  | MY46110673         | 25-Dec-23(CTTL, No.J23X13425)             | Dec-24                |
| Reference 10dBAttenuator | BT0520             | 11-May-23(CTTL, No.J23X04061)             | May-25                |
| Reference 20dBAttenuator | BT0267             | 11-May-23(CTTL, No.J23X04062)             | May-25                |
| OCP DAK-12               | SN 1174            | 25-Oct-23(SPEAG, No.OCP-DAK12-1174_Oct23) | Oct-24                |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Yu Zongying | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: September 07, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>**Glossary:**

|                       |                                                                                                                                             |
|-----------------------|---------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                   | tissue simulating liquid                                                                                                                    |
| NORM <sub>x,y,z</sub> | sensitivity in free space                                                                                                                   |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                  |
| DCP                   | diode compression point                                                                                                                     |
| CF                    | crest factor (1/duty_cycle) of the RF signal                                                                                                |
| A,B,C,D               | modulation dependent linearization parameters                                                                                               |
| Polarization $\Phi$   | $\Phi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i<br>$\theta=0$ is normal to probe axis |

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta=0$  ( $f \leq 900\text{MHz}$  in TEM-cell;  $f > 1800\text{MHz}$ : waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800\text{MHz}$ ) and inside waveguide using analytical field distributions based on power measurements for  $f > 800\text{MHz}$ . The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50\text{MHz}$  to  $\pm 100\text{MHz}$ .
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 7391

### Basic Calibration Parameters

|                                      | Sensor X | Sensor Y | Sensor Z | Unc ( $k=2$ ) |
|--------------------------------------|----------|----------|----------|---------------|
| Norm( $\mu V/(V/m)^2$ ) <sup>A</sup> | 0.35     | 0.32     | 0.34     | $\pm 10.0\%$  |
| DCP(mV) <sup>B</sup>                 | 101.8    | 106.3    | 99.8     |               |

### Calibration Results for Modulation Response

| UID       | Communication System Name   |   | A<br>dB | B<br>dB $\sqrt{\mu V}$ | C      | D<br>dB | VR<br>mV | Max<br>Dev. | Max<br>Unc <sup>E</sup><br>( $k=2$ ) |
|-----------|-----------------------------|---|---------|------------------------|--------|---------|----------|-------------|--------------------------------------|
| 0         | CW                          | X | 0.0     | 0.0                    | 1.0    | 0.00    | 146.3    | $\pm 2.7\%$ | $\pm 4.7\%$                          |
|           |                             | Y | 0.0     | 0.0                    | 1.0    |         | 141.5    |             |                                      |
|           |                             | Z | 0.0     | 0.0                    | 1.0    |         | 143.2    |             |                                      |
| 10352-AAA | Pulse Waveform (200Hz, 10%) | X | 1.32    | 60.00                  | 4.99   | 10.00   | 60       | $\pm 5.2\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 1.47    | 60.85                  | 6.63   |         | 60       |             |                                      |
|           |                             | Z | 1.31    | 60.00                  | 5.20   |         | 60       |             |                                      |
| 10353-AAA | Pulse Waveform (200Hz, 20%) | X | 36.00   | 72.00                  | 7.00   | 6.99    | 80       | $\pm 4.2\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 0.82    | 60.00                  | 4.99   |         | 80       |             |                                      |
|           |                             | Z | 14.00   | 70.00                  | 7.00   |         | 80       |             |                                      |
| 10354-AAA | Pulse Waveform (200Hz, 40%) | X | 0.00    | 69.19                  | 37.94  | 3.98    | 95       | $\pm 4.6\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 0.05    | 60.00                  | 100.00 |         | 95       |             |                                      |
|           |                             | Z | 0.00    | 69.91                  | 38.60  |         | 95       |             |                                      |
| 10355-AAA | Pulse Waveform (200Hz, 60%) | X | 0.00    | 92.27                  | 100.00 | 2.22    | 120      | $\pm 5.5\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 0.02    | 60.00                  | 100.00 |         | 120      |             |                                      |
|           |                             | Z | 0.00    | 90.64                  | 99.97  |         | 120      |             |                                      |
| 10387-AAA | QPSK Waveform, 1 MHz        | X | 20.00   | 126.25                 | 38.29  | 1.00    | 150      | $\pm 3.6\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 20.00   | 123.70                 | 37.08  |         | 150      |             |                                      |
|           |                             | Z | 20.00   | 132.56                 | 41.66  |         | 150      |             |                                      |
| 10388-AAA | QPSK Waveform, 10 MHz       | X | 20.00   | 118.30                 | 36.15  | 0.00    | 150      | $\pm 3.3\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 20.00   | 116.69                 | 35.33  |         | 150      |             |                                      |
|           |                             | Z | 20.00   | 121.31                 | 37.90  |         | 150      |             |                                      |
| 10396-AAA | 64-QAM Waveform, 100 kHz    | X | 10.12   | 112.49                 | 39.41  | 3.01    | 150      | $\pm 2.2\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 6.92    | 101.30                 | 35.39  |         | 150      |             |                                      |
|           |                             | Z | 20.00   | 130.56                 | 45.18  |         | 150      |             |                                      |
| 10414-AAA | WLAN CCDF, 64-QAM, 40MHz    | X | 5.24    | 69.75                  | 18.68  | 0.00    | 150      | $\pm 3.7\%$ | $\pm 9.6\%$                          |
|           |                             | Y | 5.14    | 69.21                  | 18.25  |         | 150      |             |                                      |
|           |                             | Z | 5.28    | 70.02                  | 18.92  |         | 150      |             |                                      |

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the  $E^2$ -field uncertainty inside TSL (see Page 5).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 7391

### Sensor Model Parameters

|   | C1<br>fF | C2<br>fF | $\alpha$<br>V <sup>-1</sup> | T1<br>ms.V <sup>-2</sup> | T2<br>ms.V <sup>-1</sup> | T3<br>ms | T4<br>V <sup>-2</sup> | T5<br>V <sup>-1</sup> | T6   |
|---|----------|----------|-----------------------------|--------------------------|--------------------------|----------|-----------------------|-----------------------|------|
| X | 31.12    | 230.42   | 36.27                       | 4.26                     | 0.00                     | 4.90     | 0.00                  | 0.17                  | 1.02 |
| Y | 30.26    | 220.54   | 35.20                       | 5.72                     | 0.00                     | 5.03     | 0.25                  | 0.13                  | 1.02 |
| Z | 30.51    | 224.99   | 36.20                       | 5.41                     | 0.00                     | 4.93     | 0.28                  | 0.15                  | 1.02 |

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | 118.6      |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disable    |
| Probe Overall Length                          | 337mm      |
| Probe Body Diameter                           | 10mm       |
| Tip Length                                    | 9mm        |
| Tip Diameter                                  | 2.5mm      |
| Probe Tip to Sensor X Calibration Point       | 1mm        |
| Probe Tip to Sensor Y Calibration Point       | 1mm        |
| Probe Tip to Sensor Z Calibration Point       | 1mm        |
| Recommended Measurement Distance from Surface | 1.4mm      |