Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 700-3000MHz	N/A

3. Photographs of EUT test position

Photo 2: Left touch cheek	Photo 3: Left tilted 15 degree
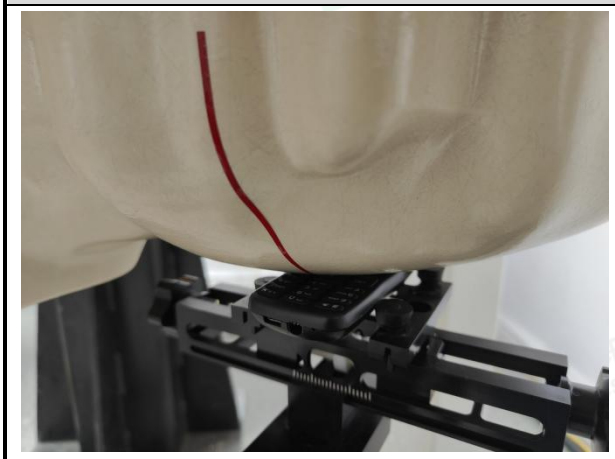	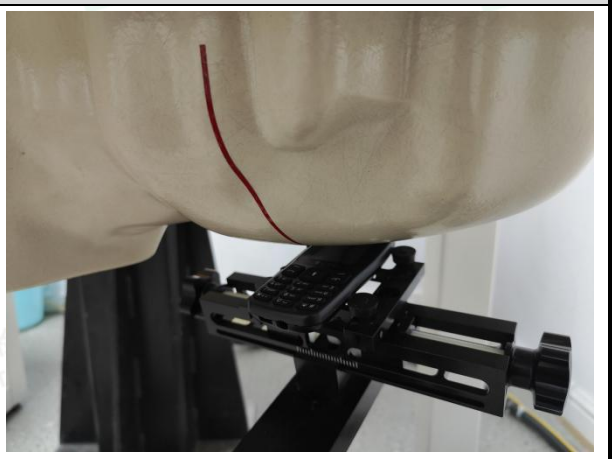
Photo 4: Right touch cheek	**Photo 5: Right tilted 15 degree**
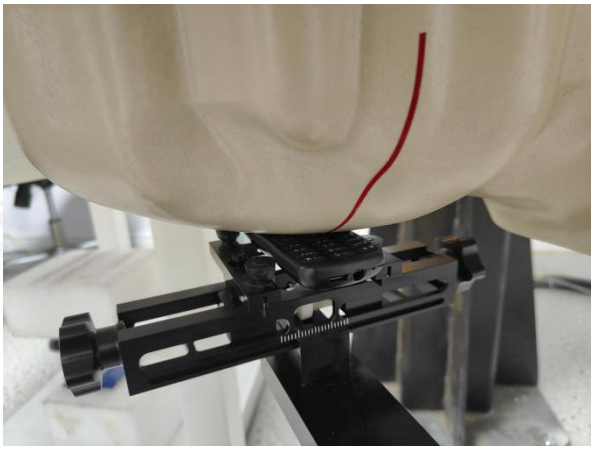	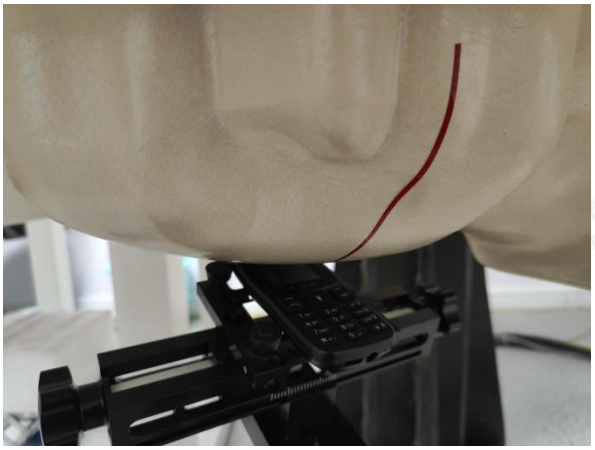

Photo 6: Front side 5mm	Photo 7: Back side 5mm
Photo 8: Left side 5mm	**Photo 9: Right side 5mm**
Photo 16 :Bottom side 5mm	

4. EUT Constructional Details

Photo 10: Front View	Photo 11: Back View
Photo 12: Front View	**Photo 13: Back View**