

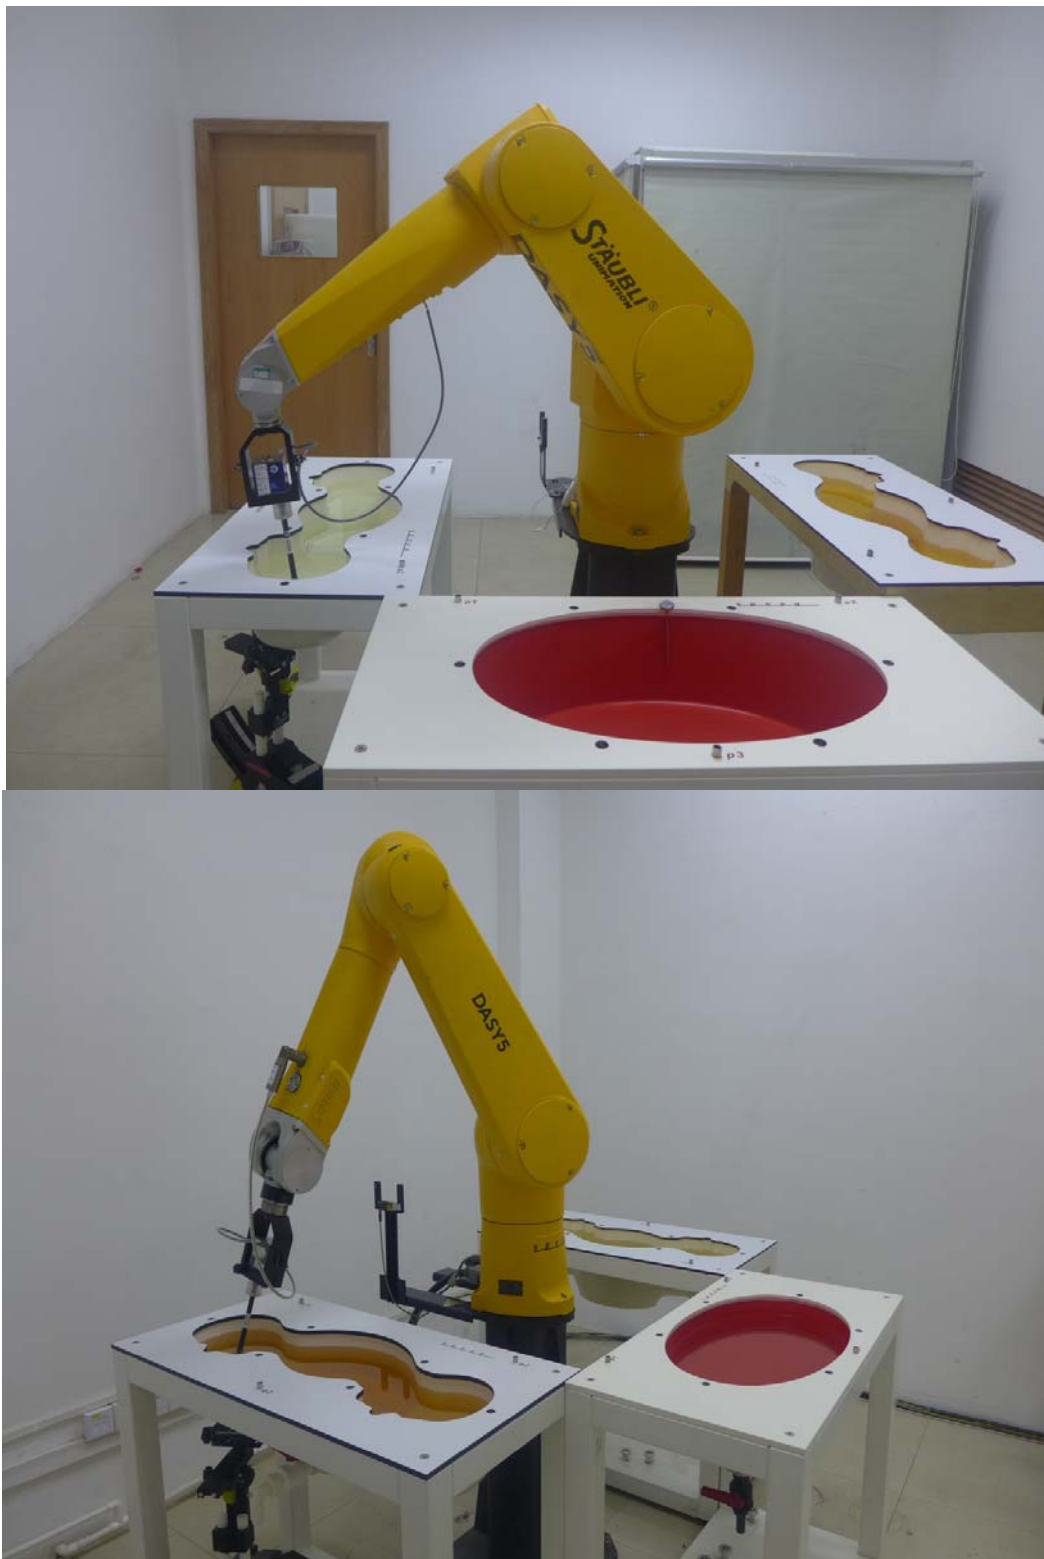


Appendix D

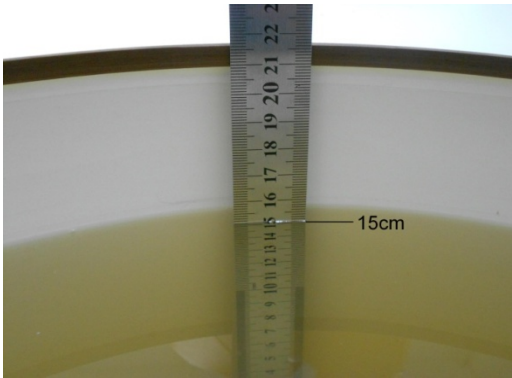
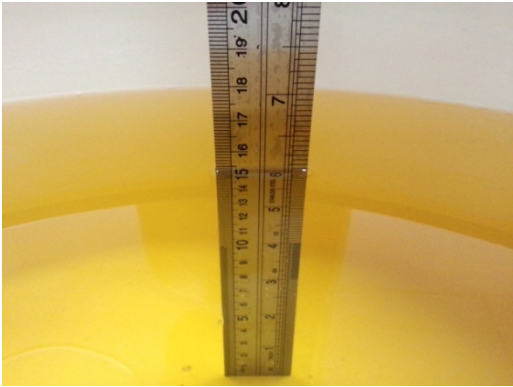
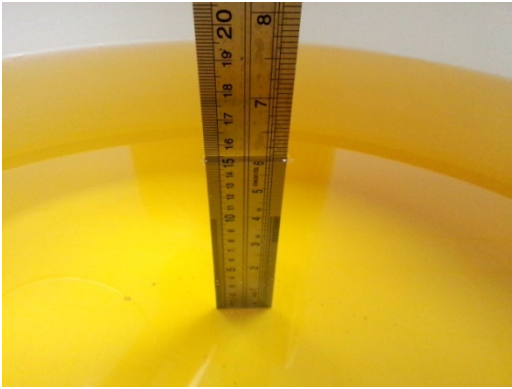
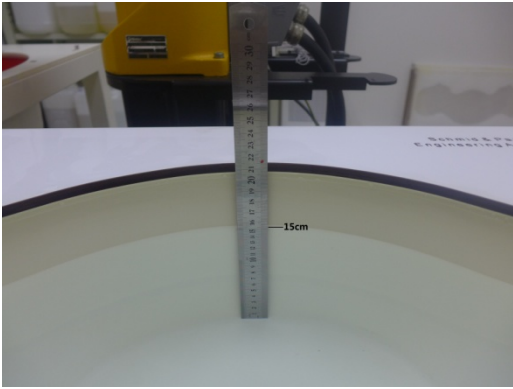
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1750
	
Photo 3: Tissue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Head 2450
	
Photo 5: Tissue Simulant Liquid for Head 2600	Photo 6: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position

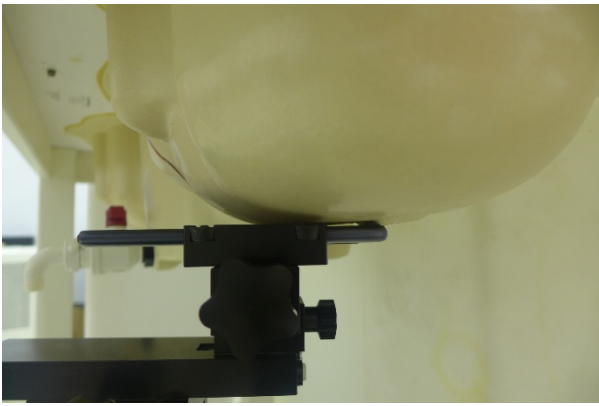
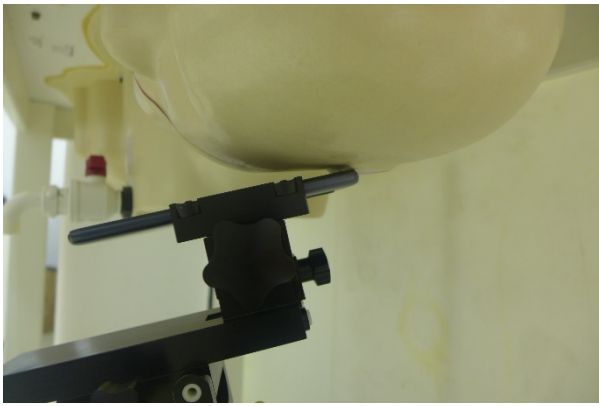
Photo 7: Left touch cheek	Photo 8: Left tilted 15 degree
	
Photo 9: Right touch cheek	Photo 10: Right tilted 15 degree
	
Photo 11: Front side 10mm	Photo 12: Back side 10mm
	

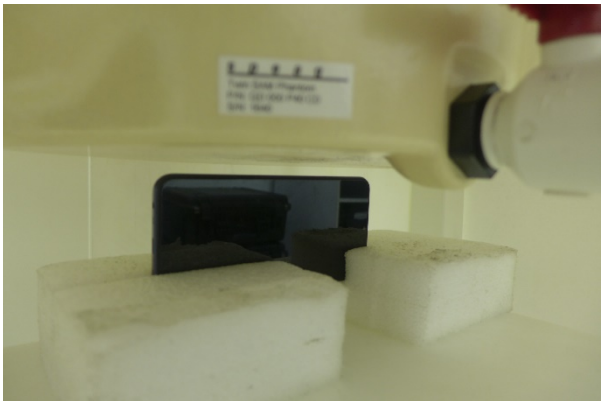
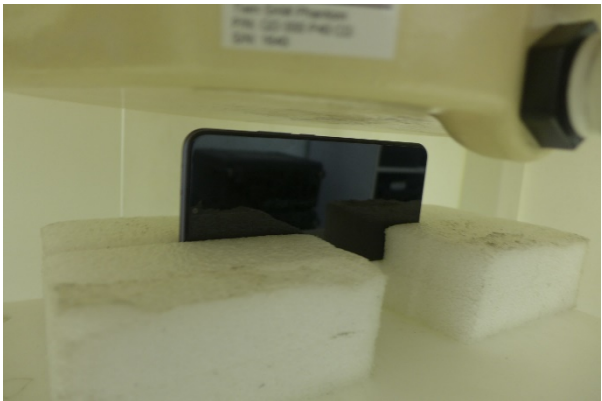
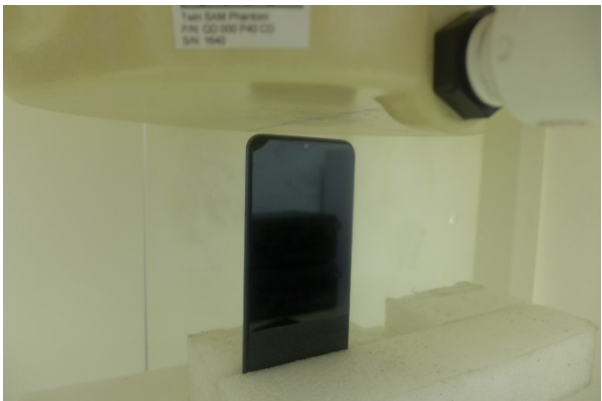
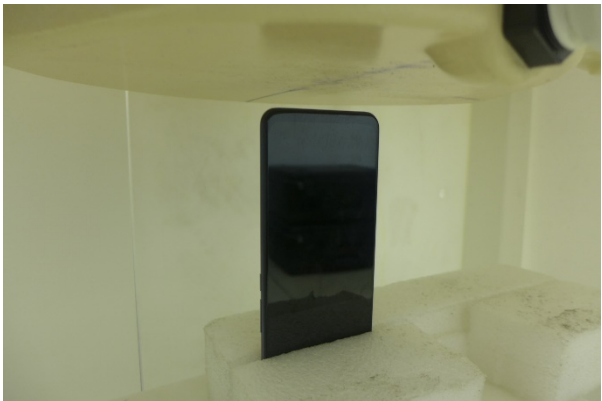
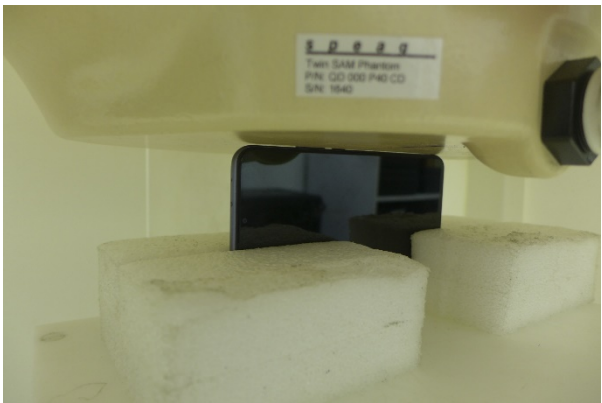
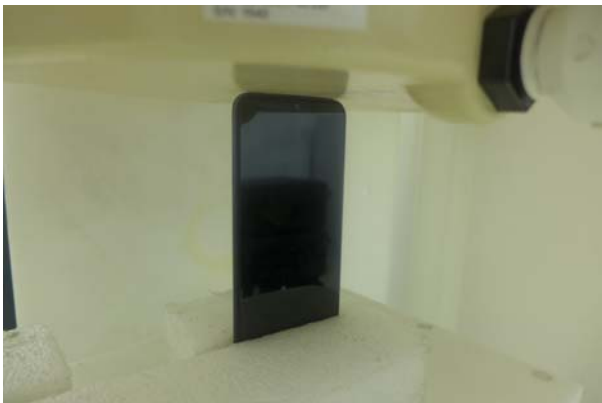
Photo 13: Left side 10mm	Photo 14: Right side 10mm
	
Photo 15: Top side 10mm	Photo 16: Bottom side 10mm
	
Photo 17: Back side 15mm	Photo 18: Bottom side 15mm
	

Photo 19: Front side 0mm	Photo 20: Back side 0mm
	
Photo 21: Right side 0mm	Photo 22: Top side 0mm
	

4. EUT Constructional Details

Photo 23: Front View	Photo 24: Back View
	