

Date: 2025/9/17

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.53, 10.34, 10.38); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.51 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.24 W/kg; SAR (10g) = 1.45 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

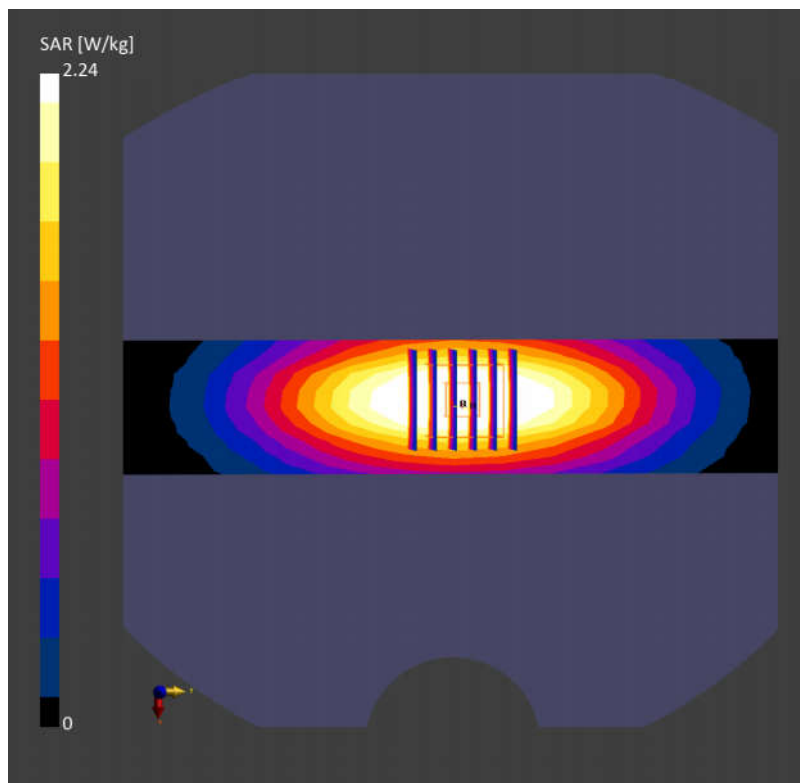

Date: 2025/9/17

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.23, 10.04, 10.08); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.73 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.50 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

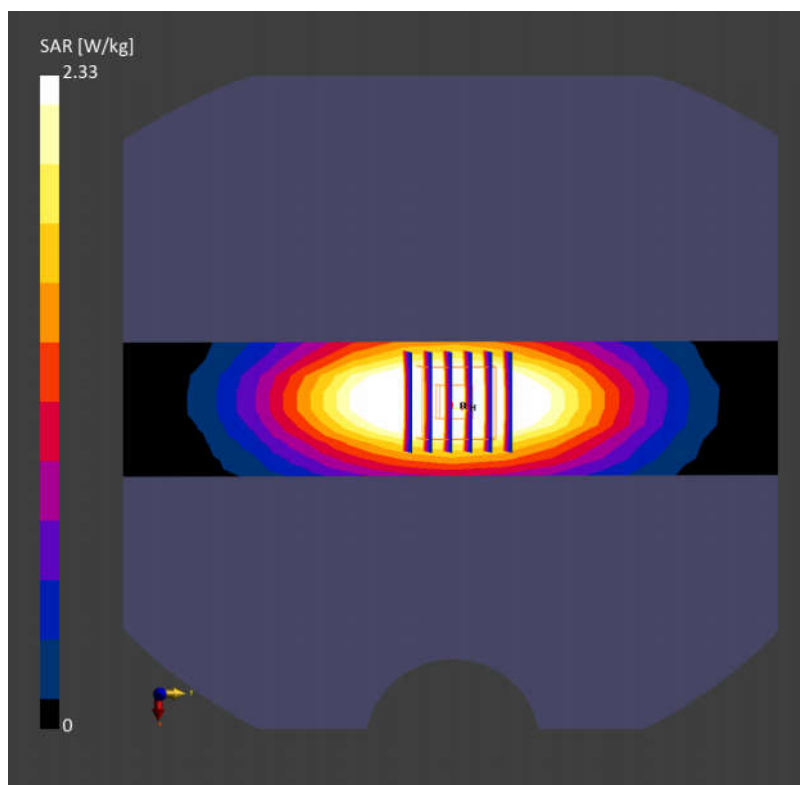

Date: 2025/9/17

System Check_1750MHz**DUT:D1750V2-SN:1137**

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.61, 8.45, 8.49); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 9.92 W/kg; SAR (10g) = 5.37 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 9.64 W/kg; SAR (10g) = 5.14 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

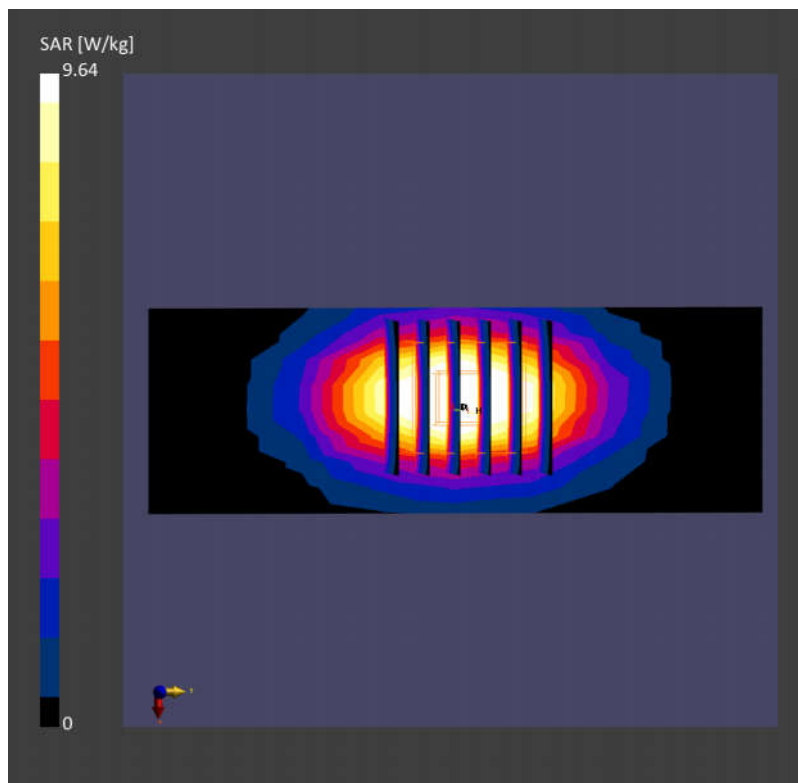

Date: 2025/9/17

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.33, 8.18, 8.21); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 11.1 W/kg; SAR (10g) = 5.80 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

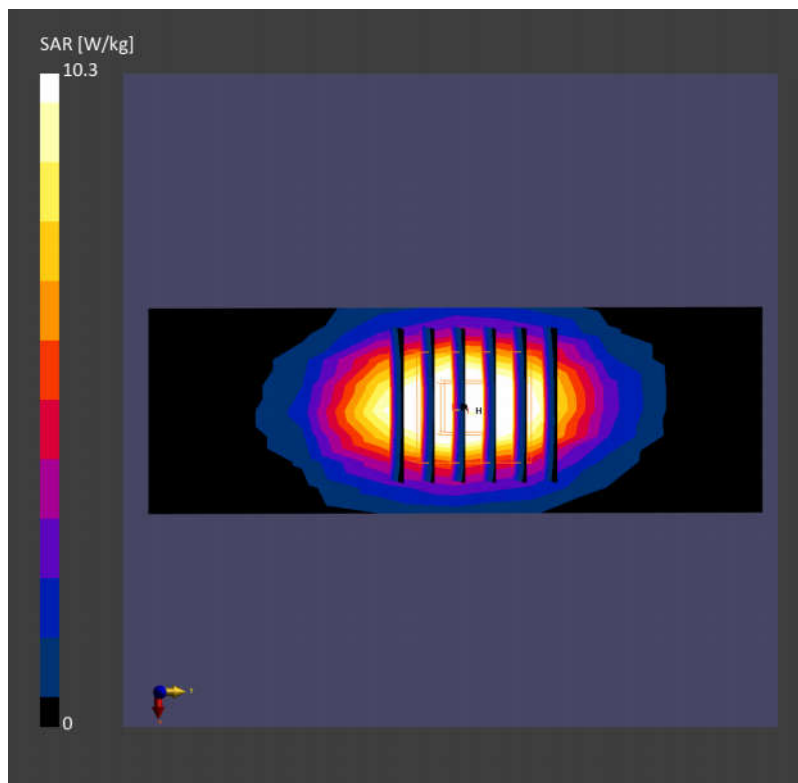

Date: 2025/9/17

System Check_2450MHz**DUT:D2450V2-SN:924**

Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.9 W/kg; SAR (10g) = 6.95 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 13.3 W/kg; SAR (10g) = 6.53 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

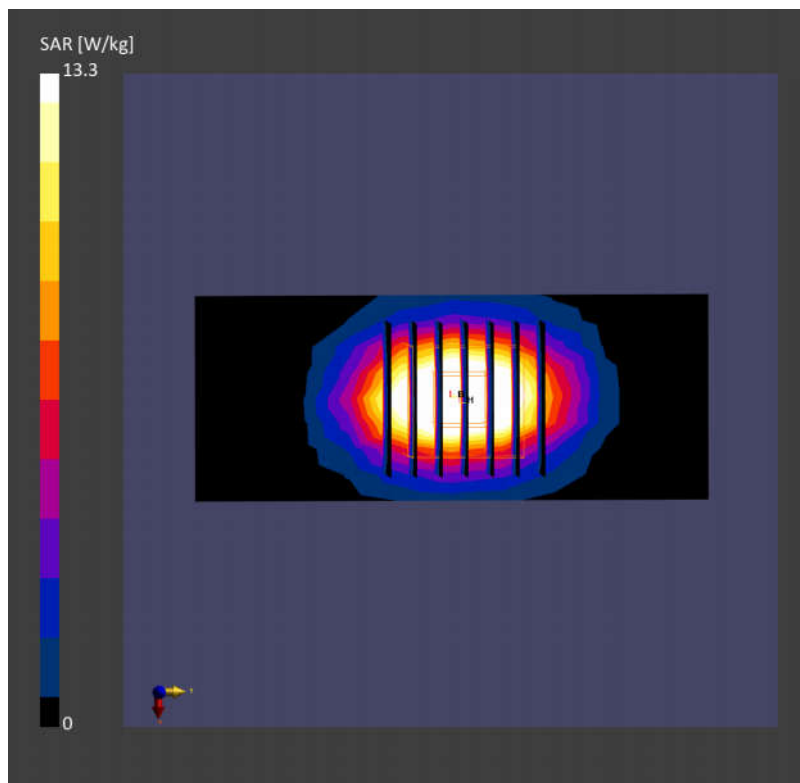

Date: 2025/9/17

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.99, 6.86, 6.89); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 6.42 W/kg; SAR (10g) = 2.51 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 6.52 W/kg; SAR (10g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.9 %

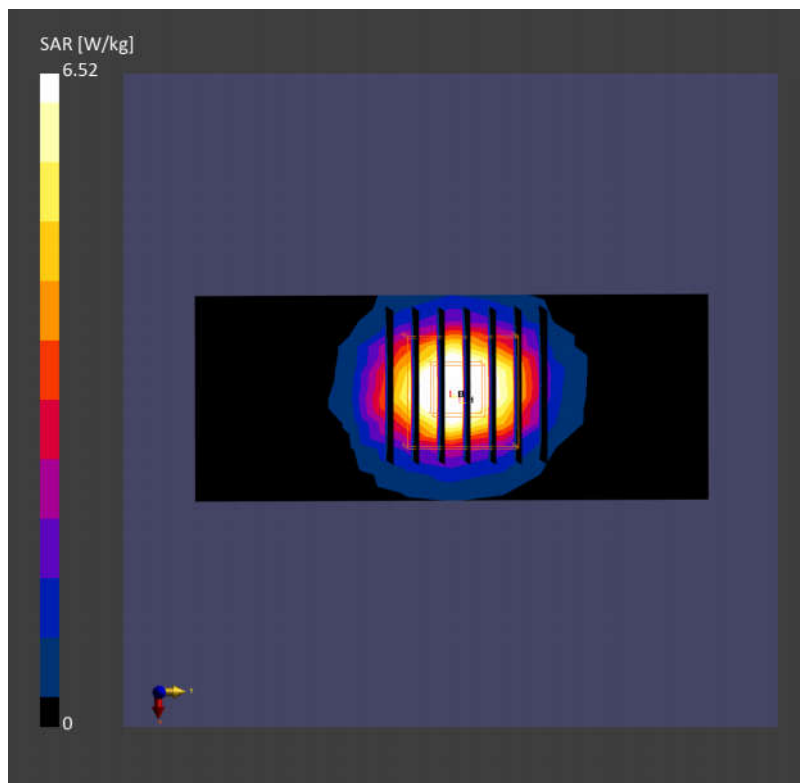

Date: 2025/9/17

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.85, 6.72, 6.76); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.64 W/kg; SAR (10g) = 2.86 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 7.07 W/kg; SAR (10g) = 2.53 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

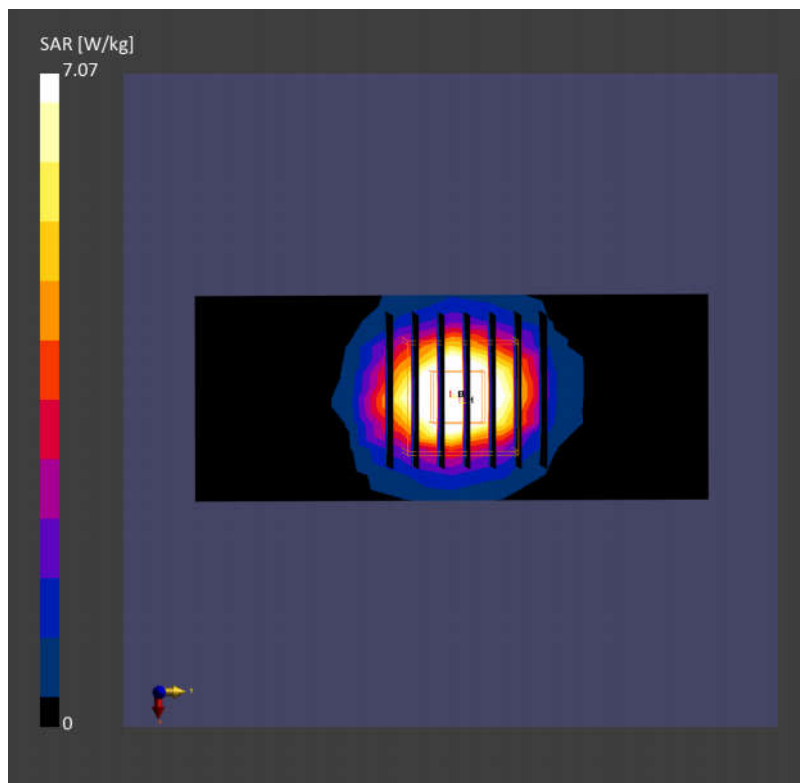

Date: 2025/9/17

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: Head Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.59$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.0); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2025/4/16
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.36 W/kg; SAR (10g) = 2.13 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.87 W/kg; SAR (10g) = 2.20 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 63.7 %

