11G_LCH_Graphs	
Pref/11G/LCH	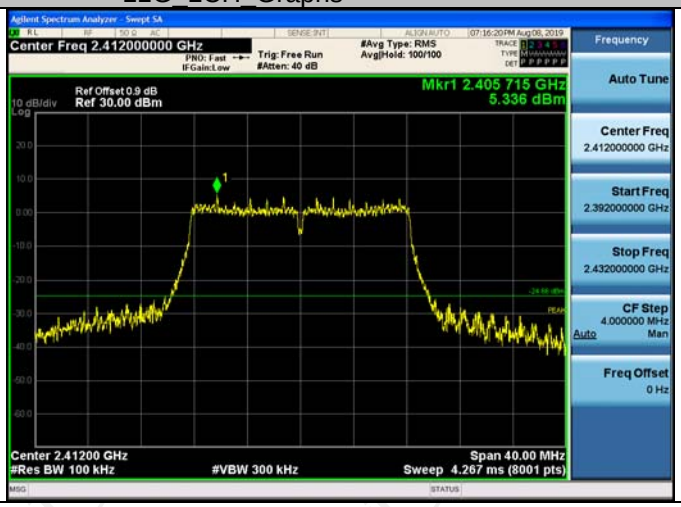

Puw/11G/LCH		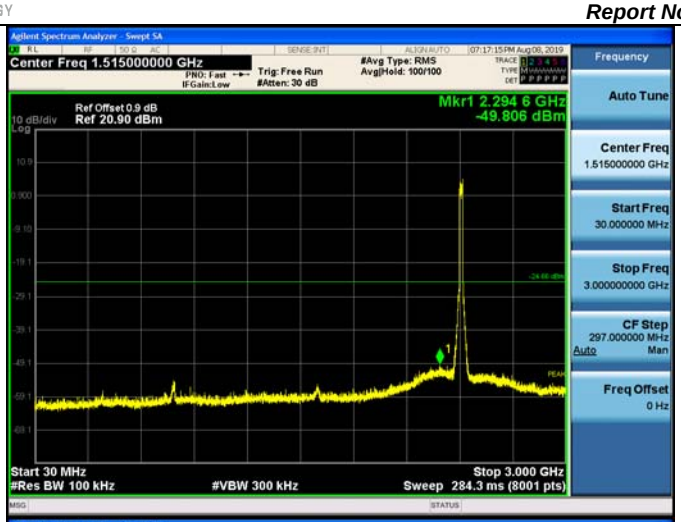 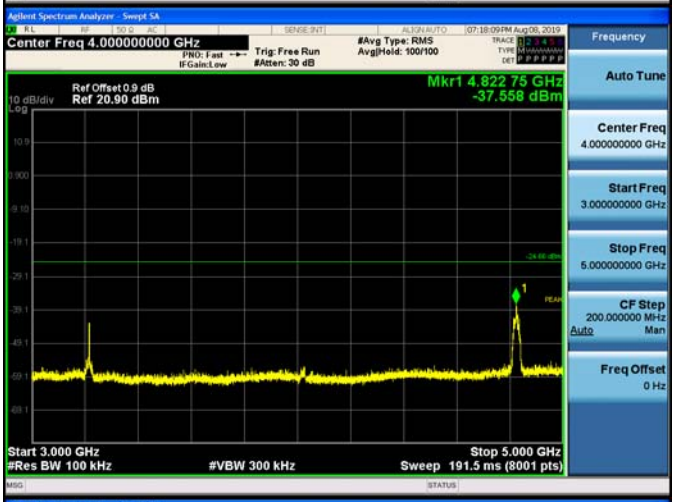 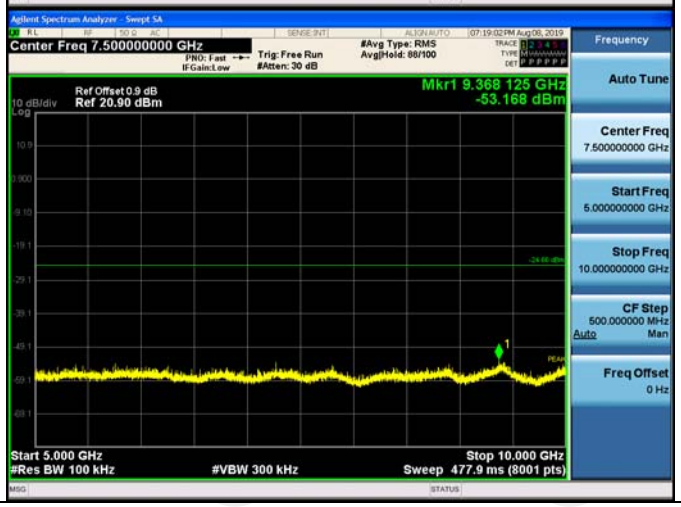	

11G_MCH_Graphs	
Pref/11G/MCH	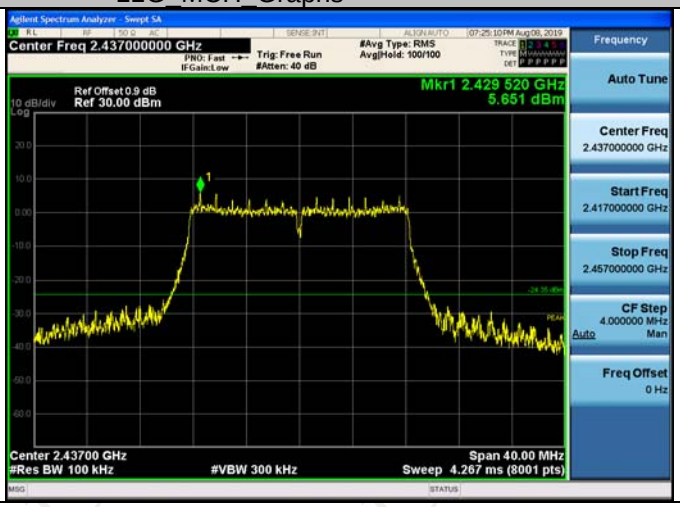

Puw/11G/MCH		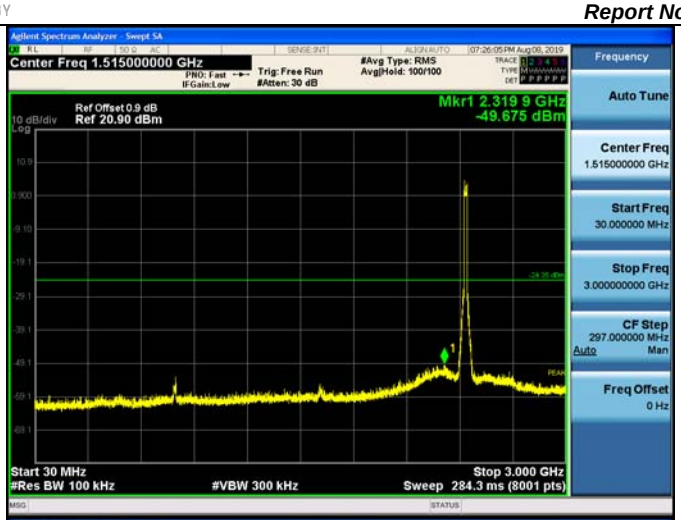 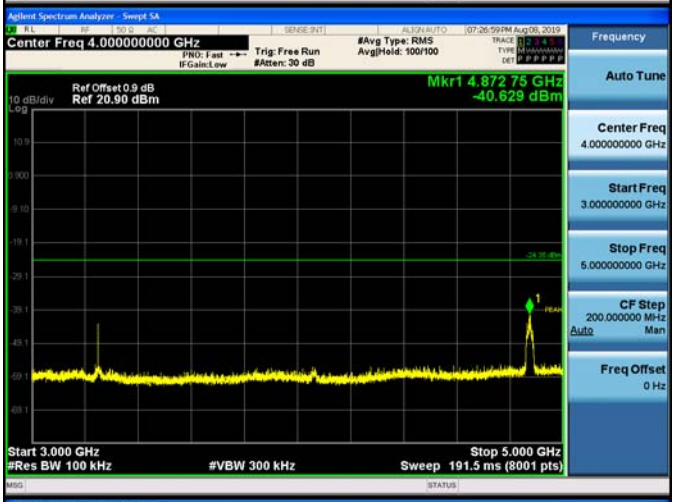 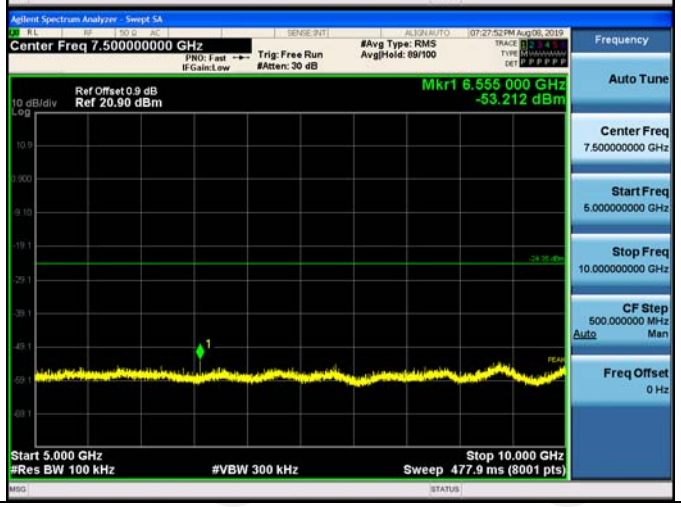	

11G_HCH_Graphs	
Pref/11G/HCH	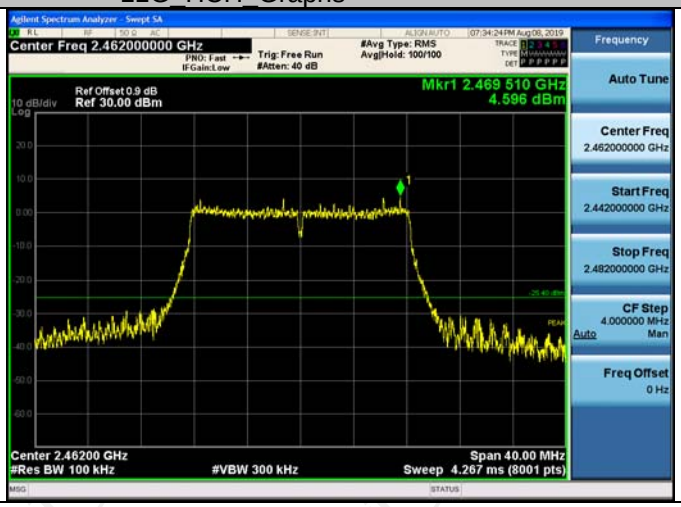

Puw/11G/HCH		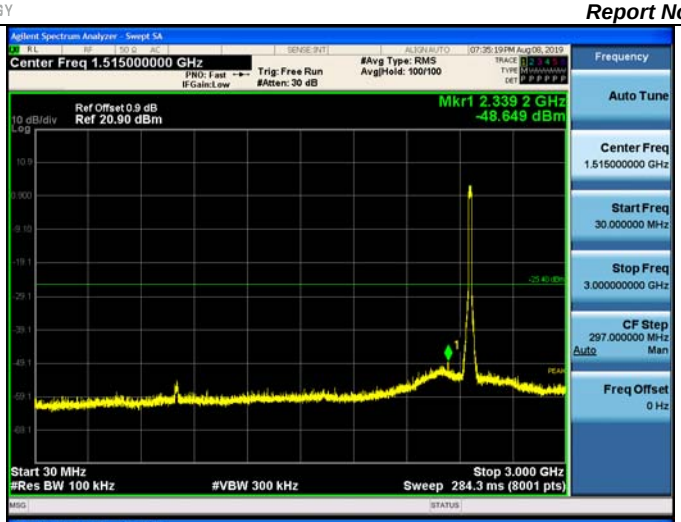 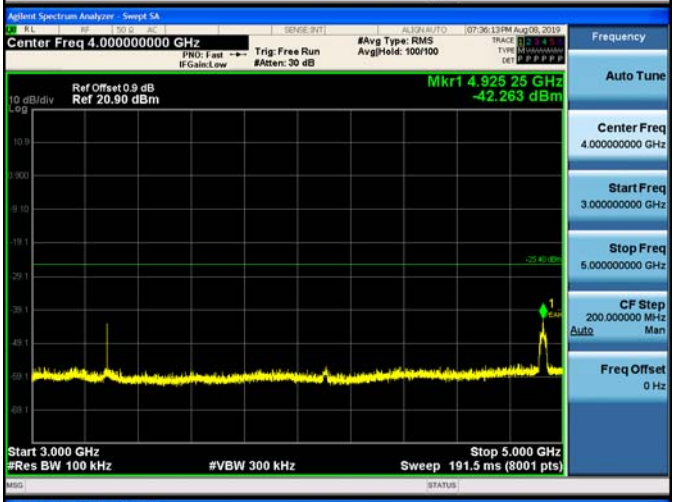 	

11N20SISO_LCH_Graphs	
Pref/11N20SISO/LCH	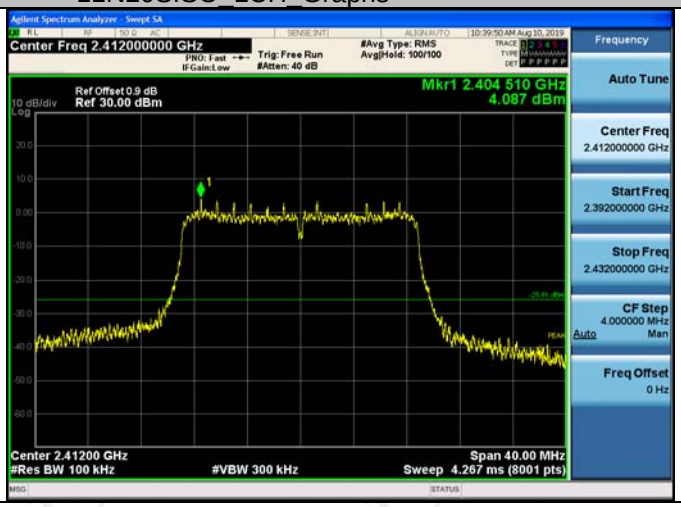

/11N20SISO/LCH		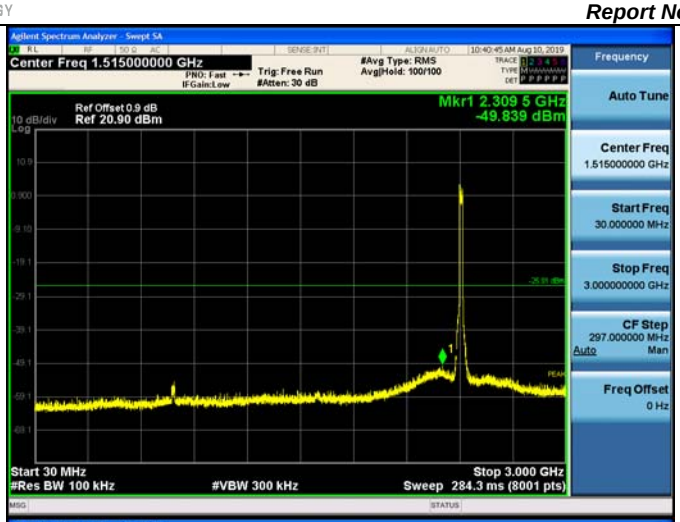 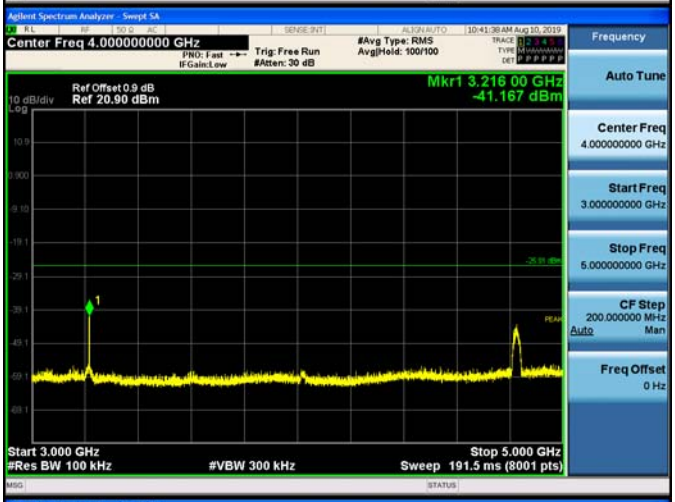 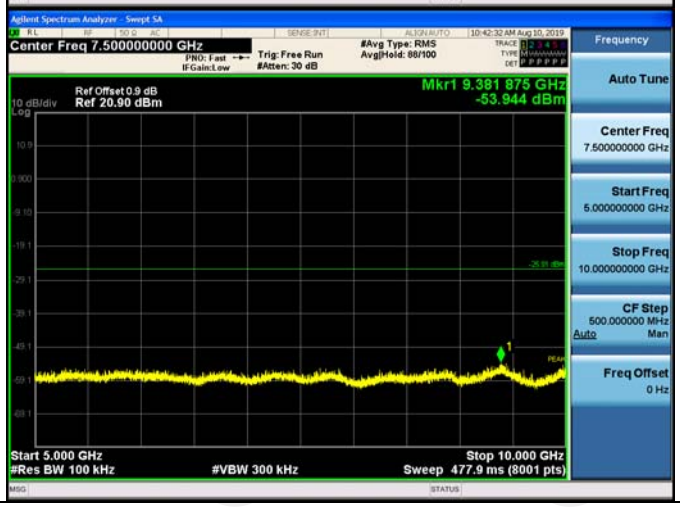	

11N20SISO_MCH_Graphs	
Pref/11N20SISO/MCH	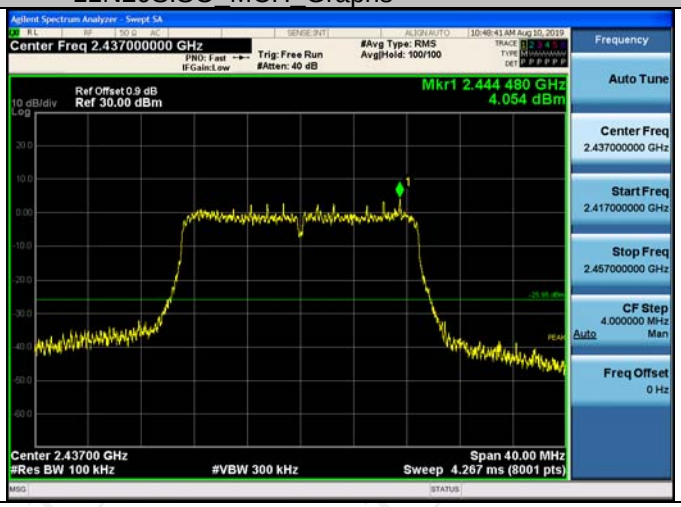

Puw/11N20SISO/MCH		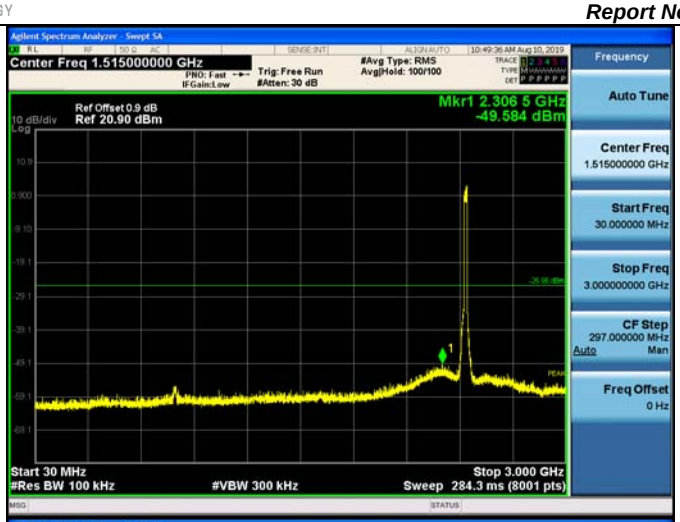 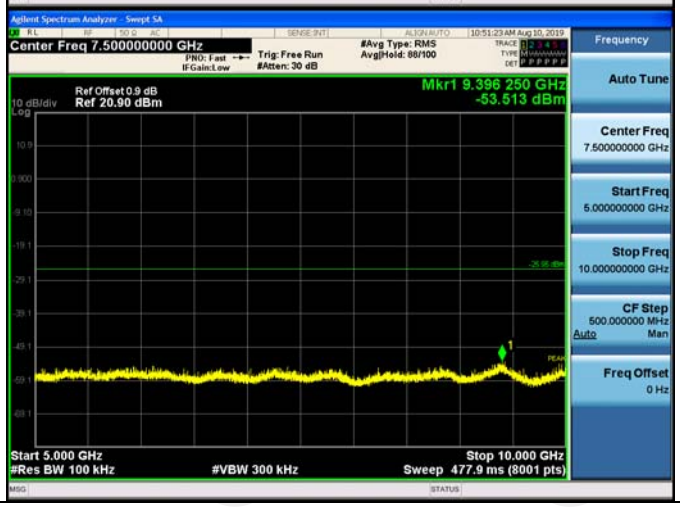	

11N20SISO_HCH_Graphs	
Pref/11N20SISO/HCH	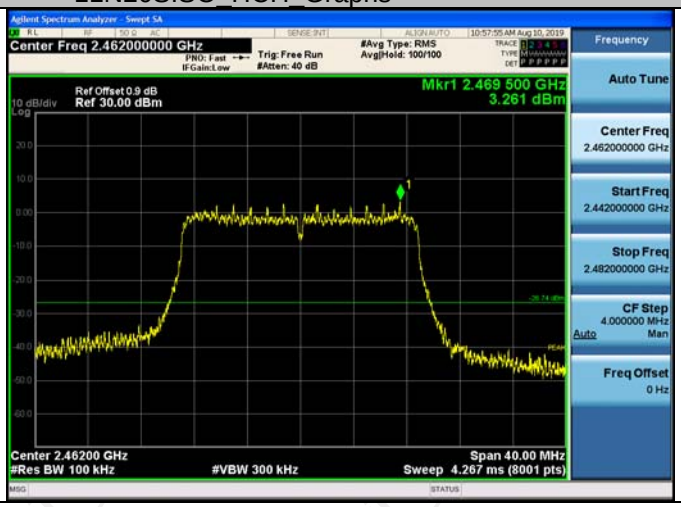

Puw/11N20SISO/HCH		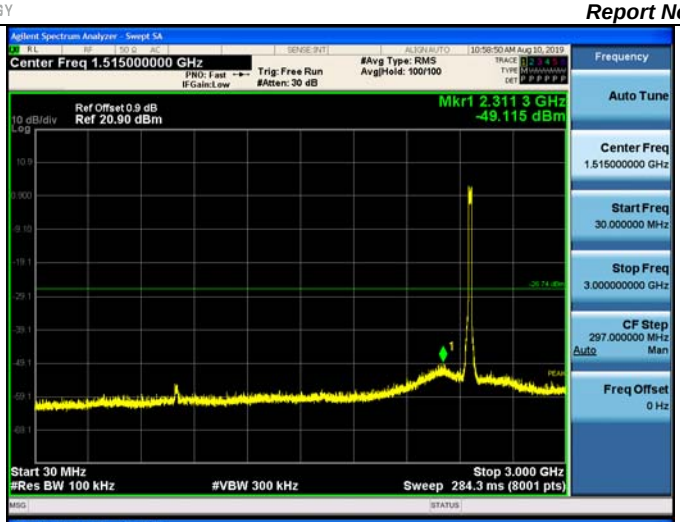 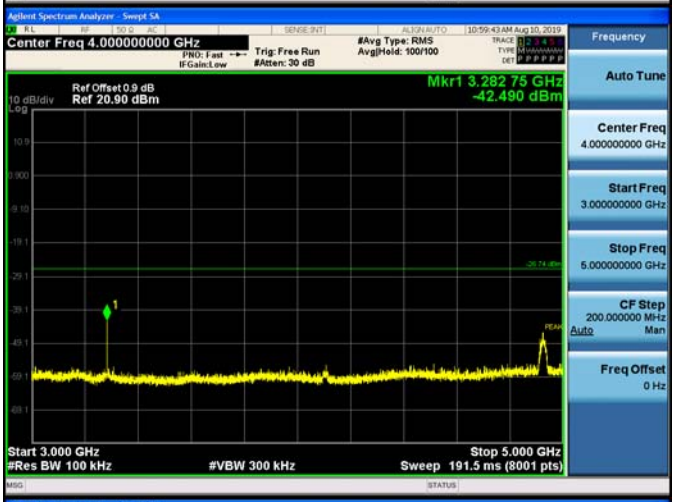 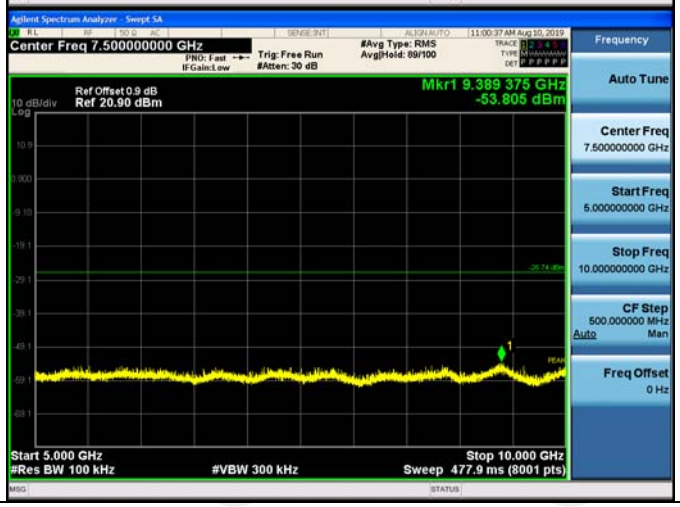	

11N40SISO_LCH_Graphs	
Pref/11N40SISO/LCH	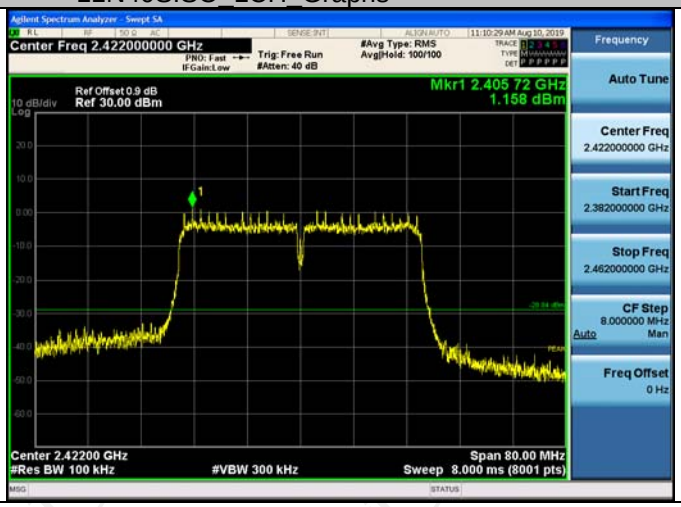

Puw/11N40SISO/LCH		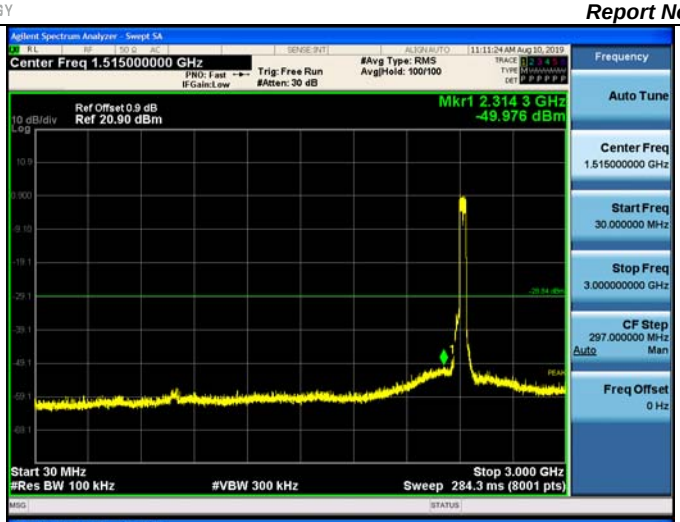 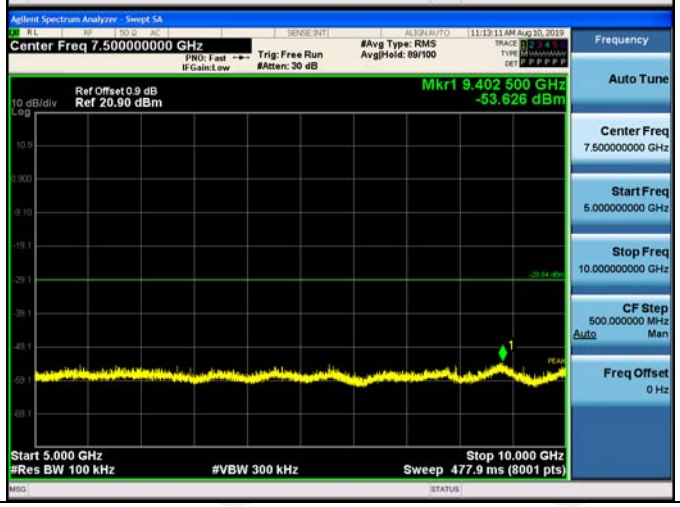	

11N40SISO_MCH_Graphs	
Pref/11N40SISO/MCH	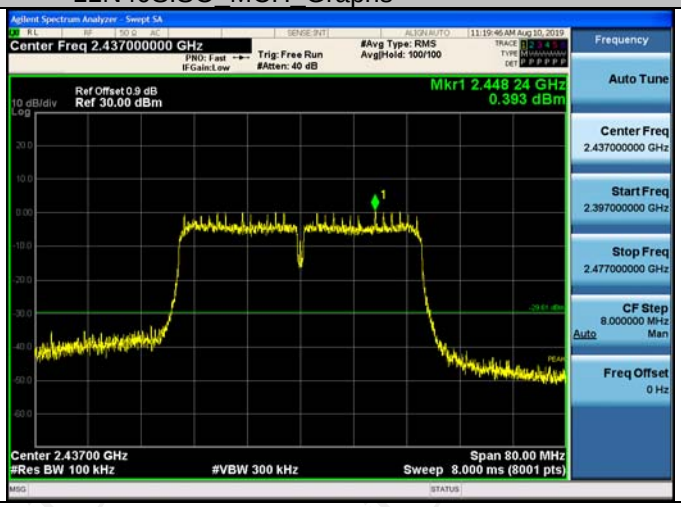

Puw/11N40SISO/MCH		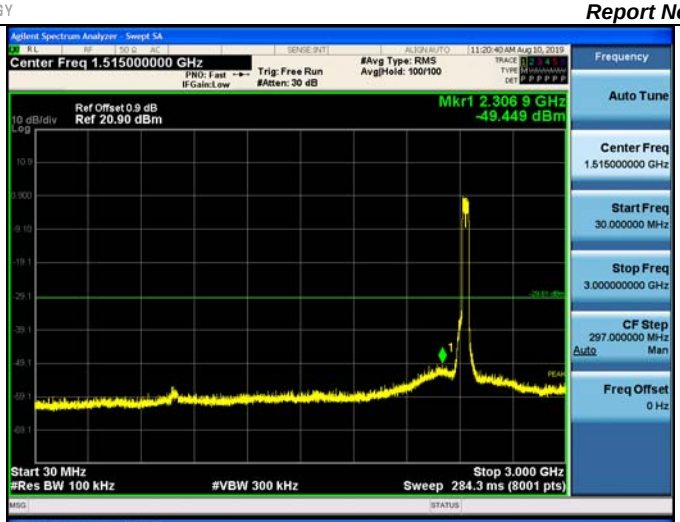 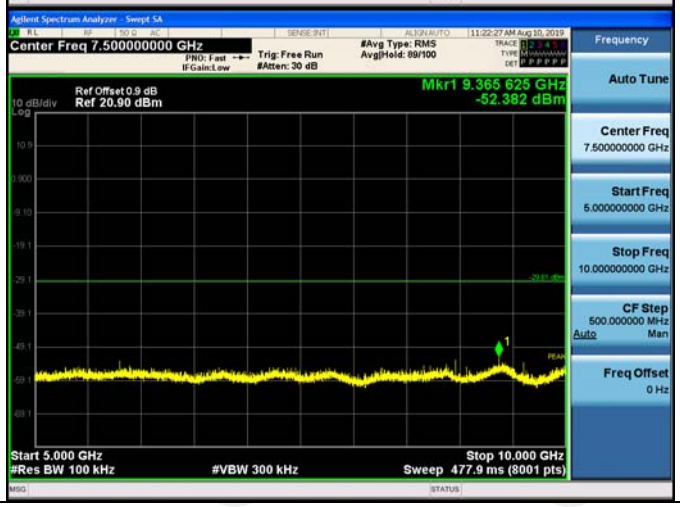	

11N40SISO_HCH_Graphs	
Pref/11N40SISO/HCH	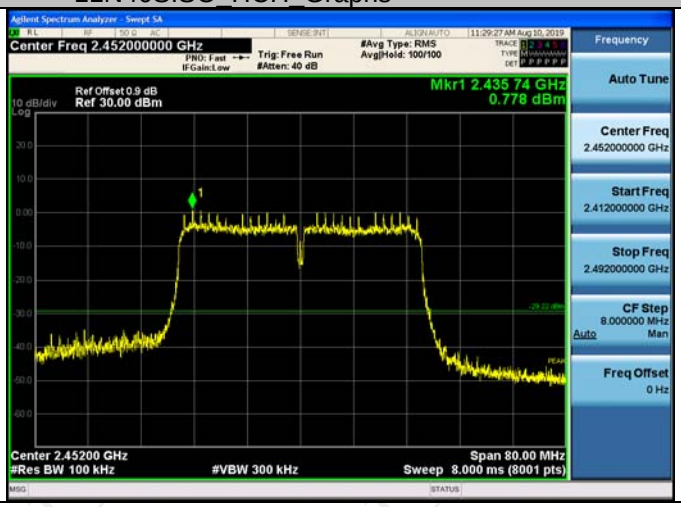

Puw/11N40SISO/HCH		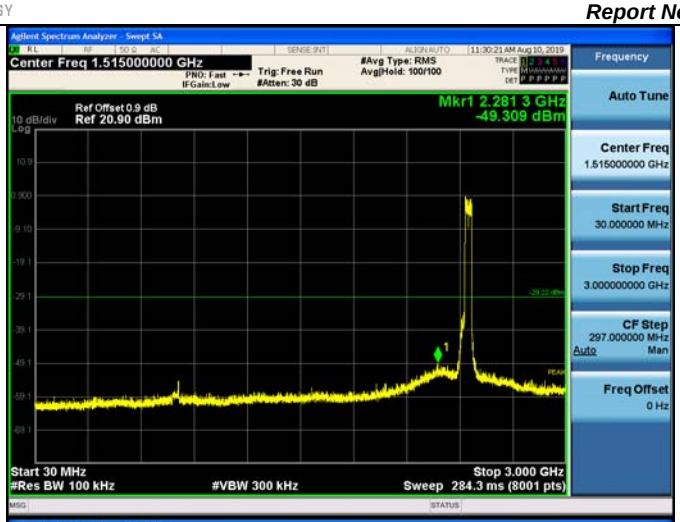 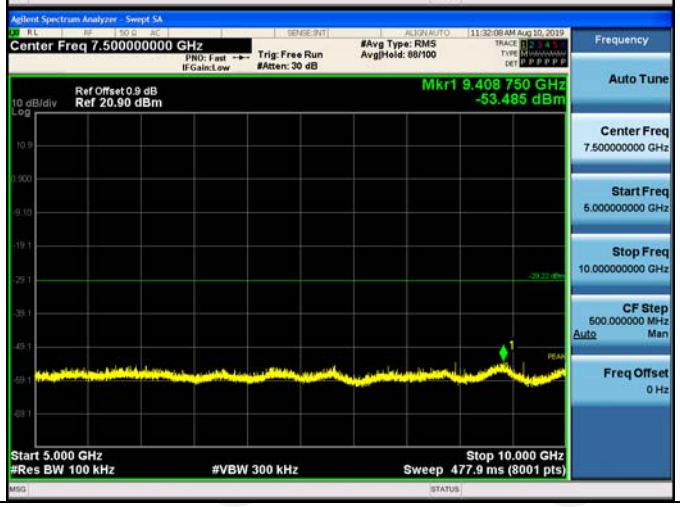	

Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 20.90 dBm
Mkr1 13.401 250 GHz
-51.143 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

Agilent Spectrum Analyzer - Swept SA
Center Freq 20.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 32 dB
#Avg Type: RMS
Avg|Hold: 100/100
Frequency
Auto Tune
Ref Offset 0.9 dB
10 dB/div
Ref 22.90 dBm
Mkr1 24.995 00 GHz
-41.053 dBm
Center Freq
20.000000000 GHz
Start Freq
15.000000000 GHz
Stop Freq
25.000000000 GHz
CF Step
1.000000000 GHz
Auto
Man
Freq Offset
0 Hz
Start 15.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.000 GHz
Sweep 955.7 ms (8001 pts)

Power Spectral Density

Result Table

Mode	Channel	Meas.Level [dBm]	Verdict
11B	LCH	-12.676	PASS
11B	MCH	-12.589	PASS
11B	HCH	-12.362	PASS
11G	LCH	-13.400	PASS
11G	MCH	-13.753	PASS
11G	HCH	-14.364	PASS
11N20SISO	LCH	-13.738	PASS
11N20SISO	MCH	-13.702	PASS
11N20SISO	HCH	-15.821	PASS
11N40SISO	LCH	-16.305	PASS
11N40SISO	MCH	-17.721	PASS
11N40SISO	HCH	-17.125	PASS

Test Graph

Graphs			
11B/LCH			

Hotline: 400-6611-140 Tel: 86-755-27673339 Fax: 86-755-27673332 http://www.tct-lab.com