



FCC ID 2AGS5-IPG

IC: 20934-IPG

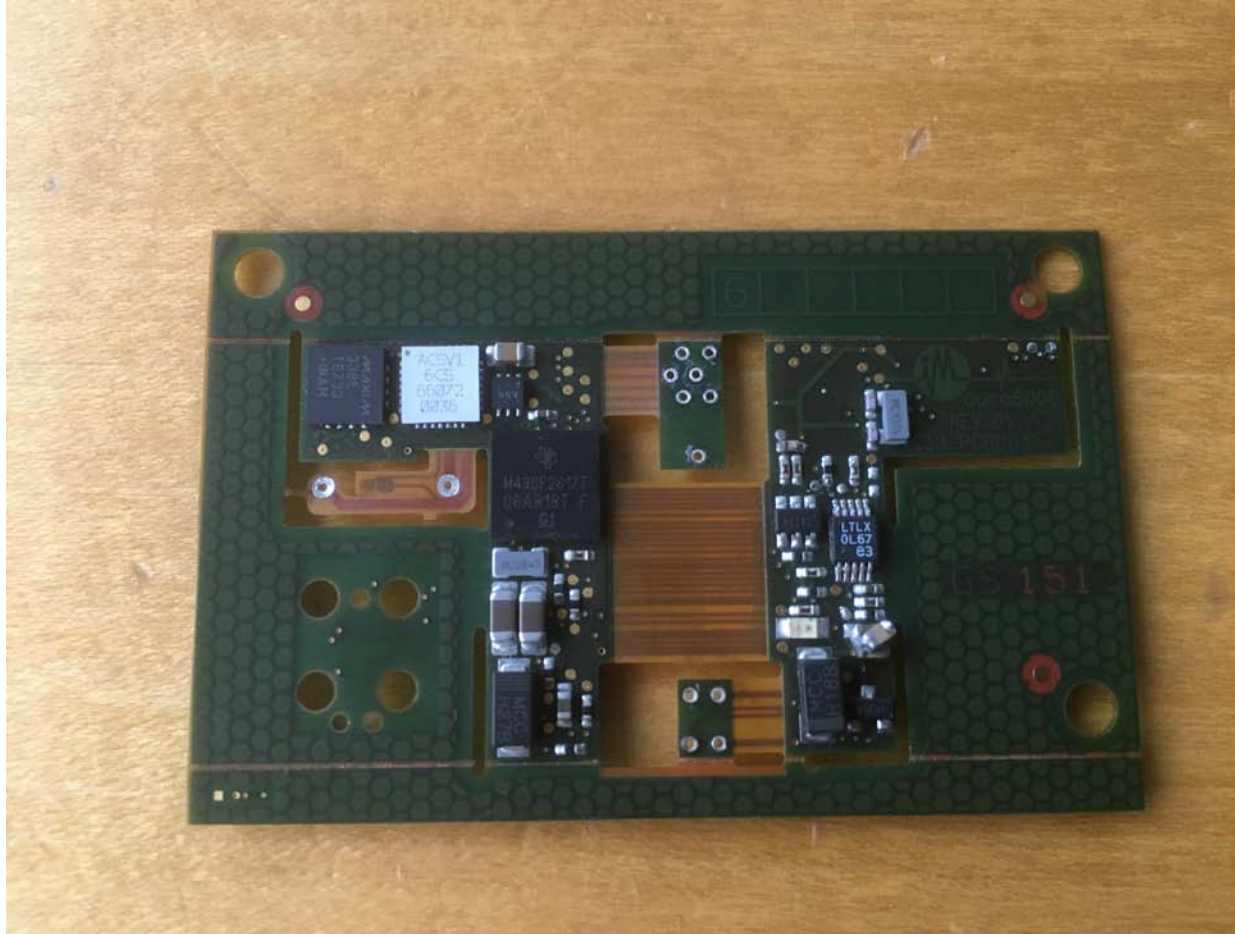

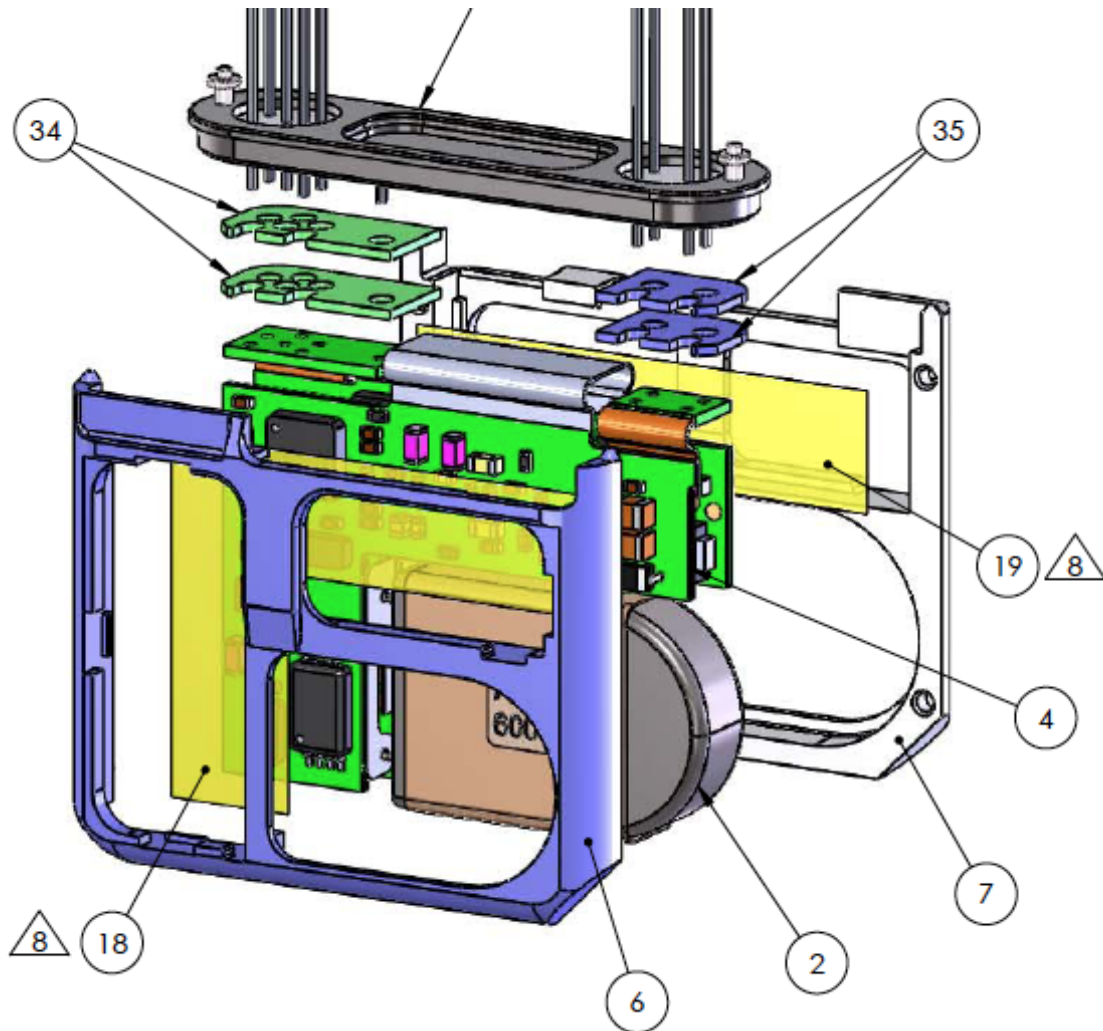

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means
without the written permission of an authorized representative of ImThera Medical, Inc.


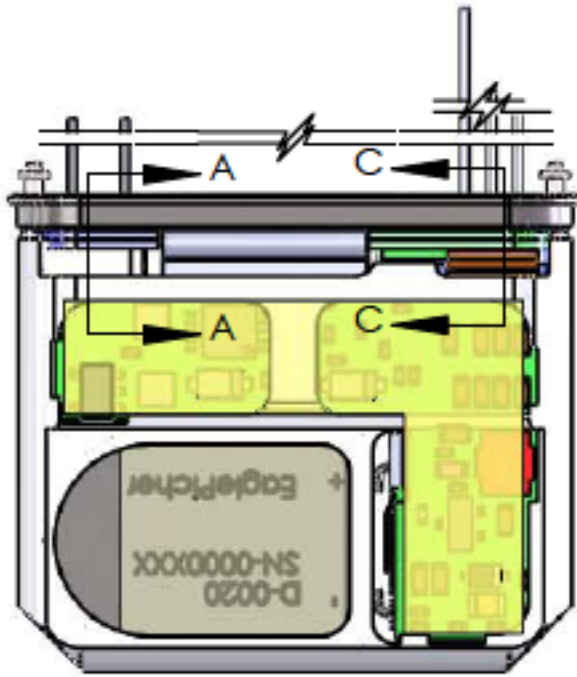


Figure 2 – IPG Internal structure with battery, PCBA, plastic support and feedthrough assembly

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means
without the written permission of an authorized representative of ImThera Medical, Inc.

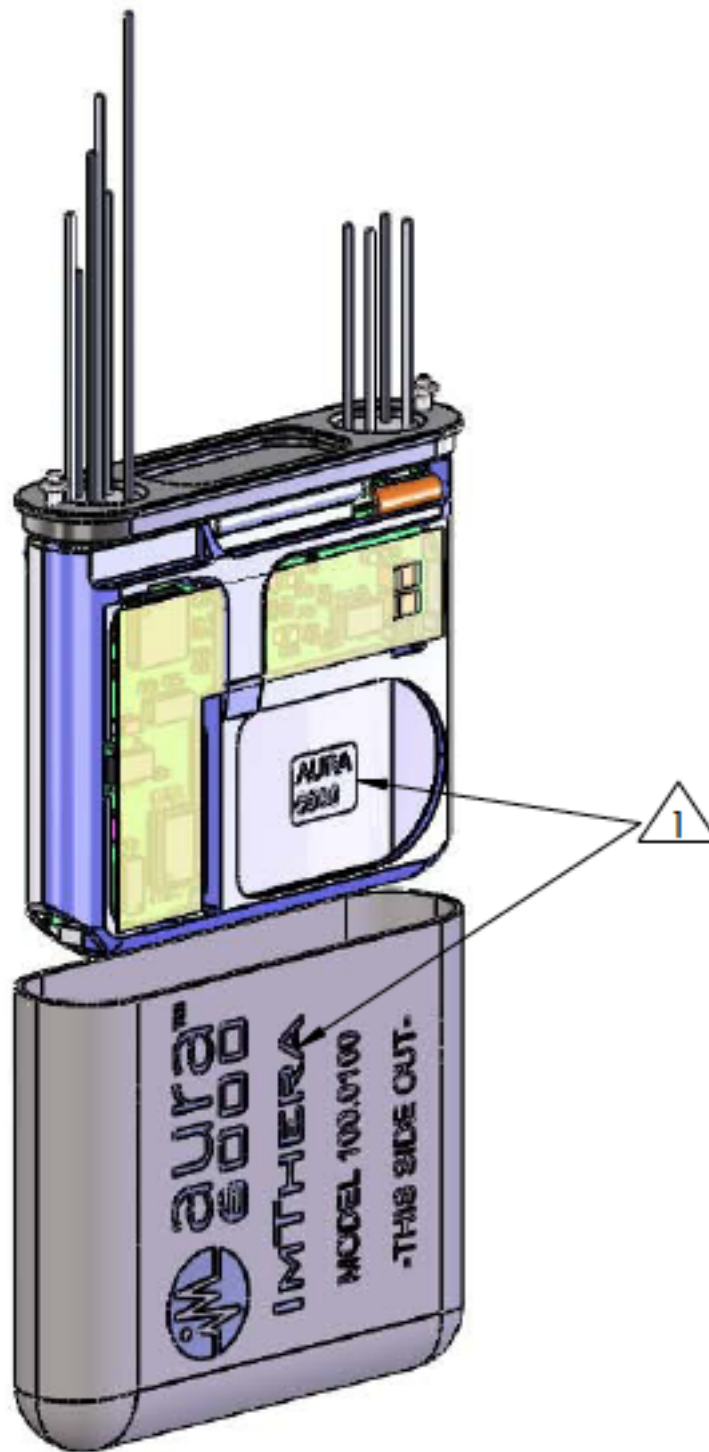

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means without the written permission of an authorized representative of ImThera Medical, Inc.

Figure 3 – IPG Internal Assembly being inserted into titanium can prior to laser weld of feedthrough assembly to can

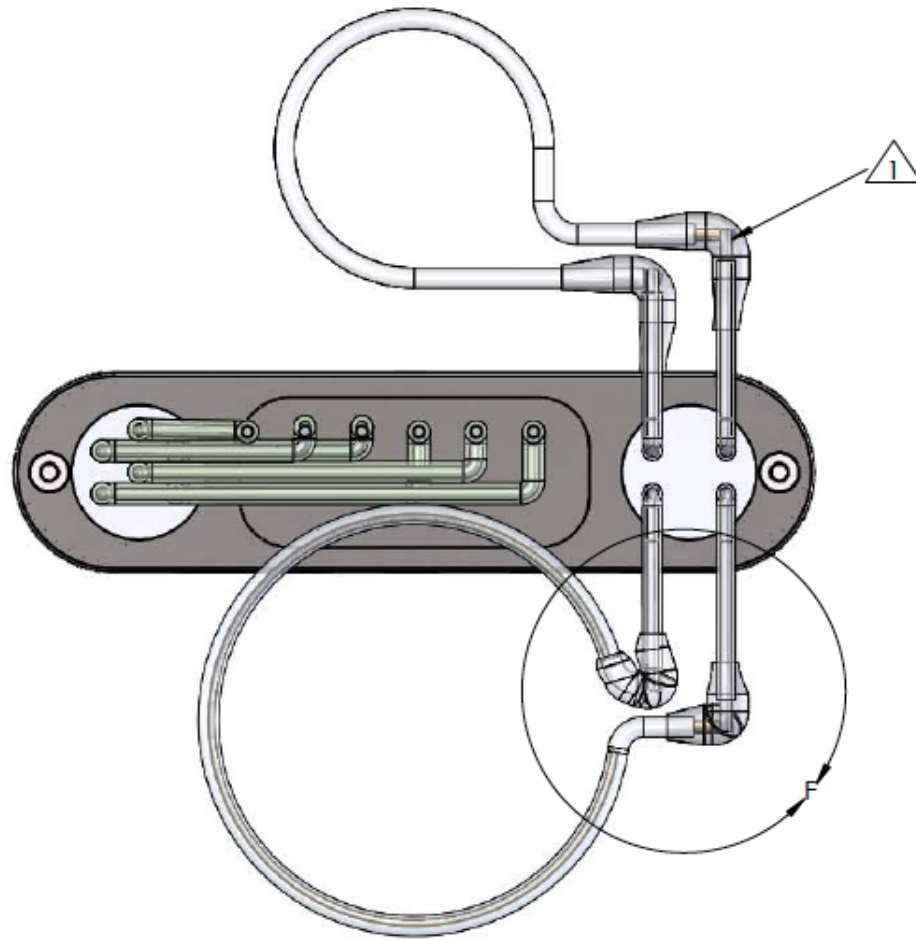


Figure 4 top view of IPG feedthrough assembly; top loop is gold wire RF telemetry antenna; bottom loop is charging coil used to receive inductive charging power.

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means without the written permission of an authorized representative of ImThera Medical, Inc.

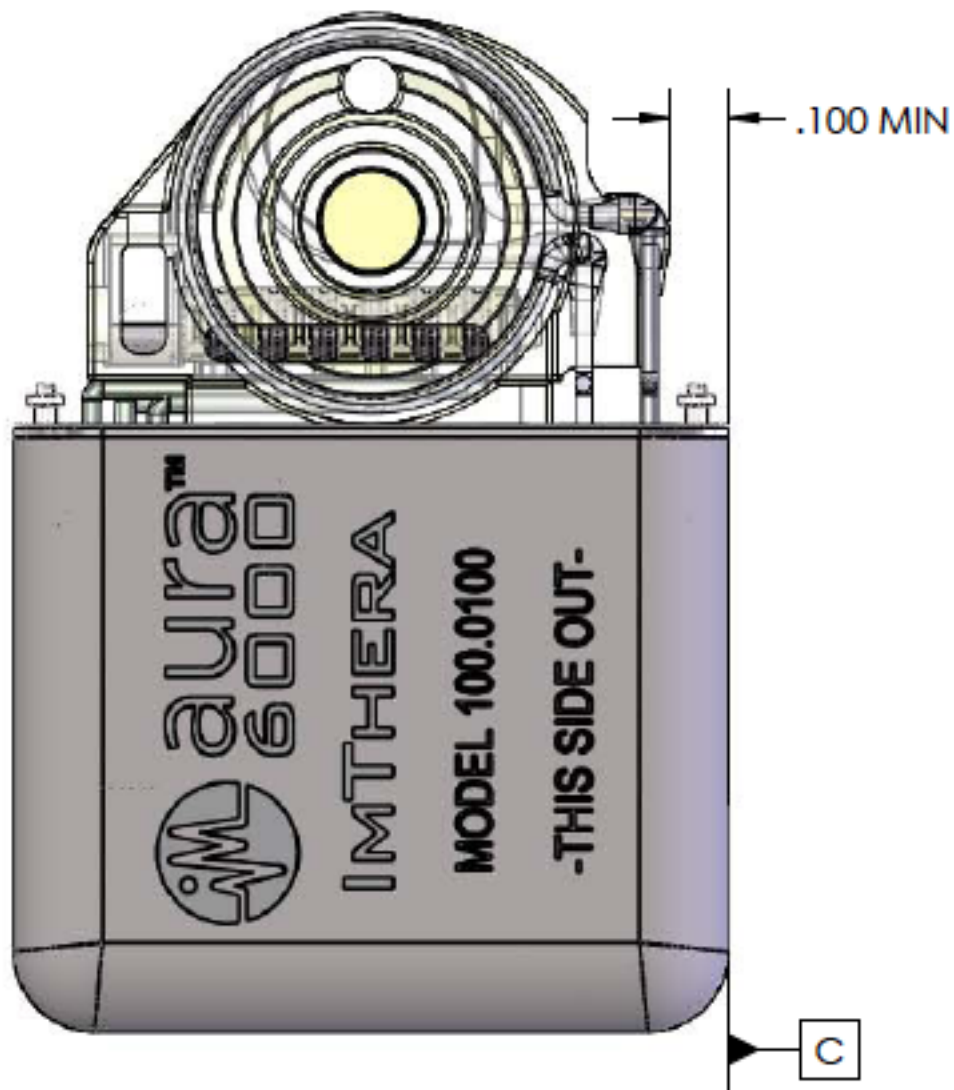


Figure 5 – Front view of IPG with charge coil and magnet visible

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means without the written permission of an authorized representative of ImThera Medical, Inc.

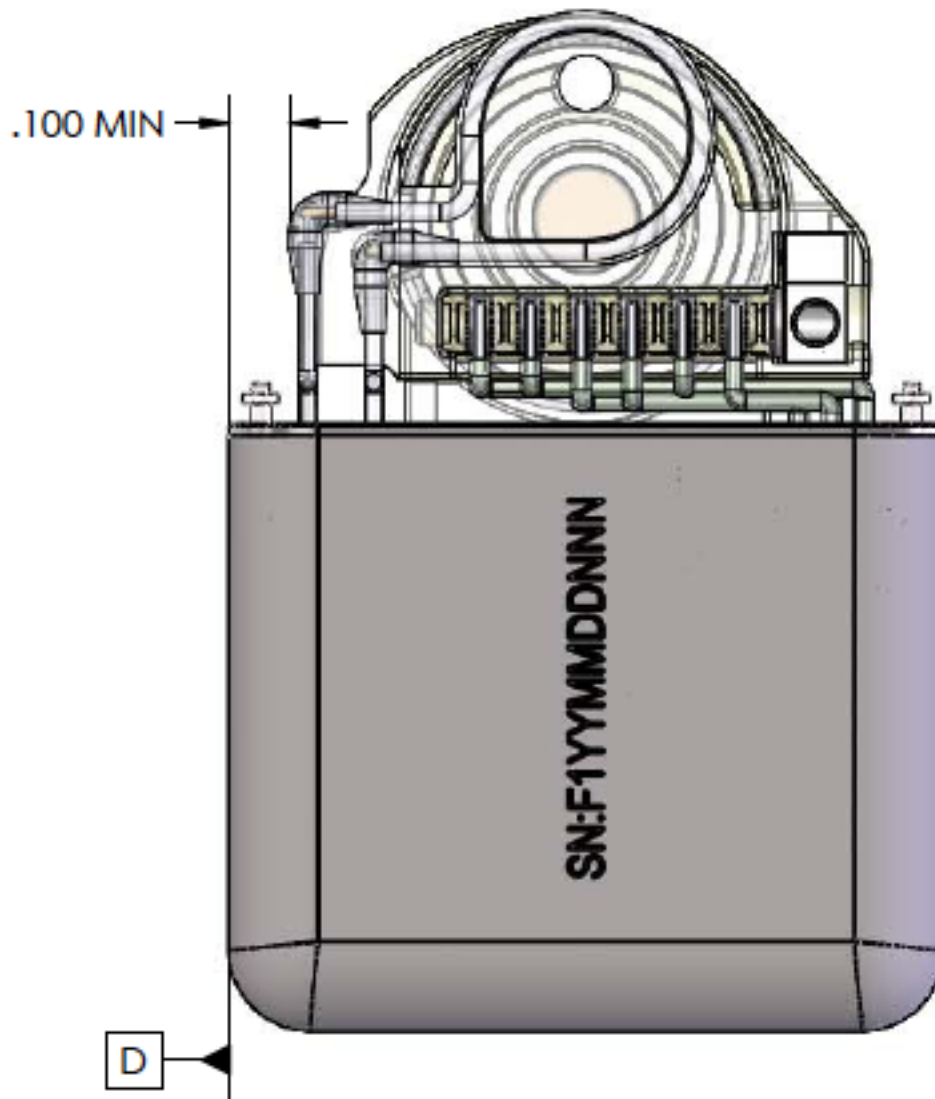


Figure 6 – Rear view of IPG with telemetry coil visible

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means
without the written permission of an authorized representative of ImThera Medical, Inc.

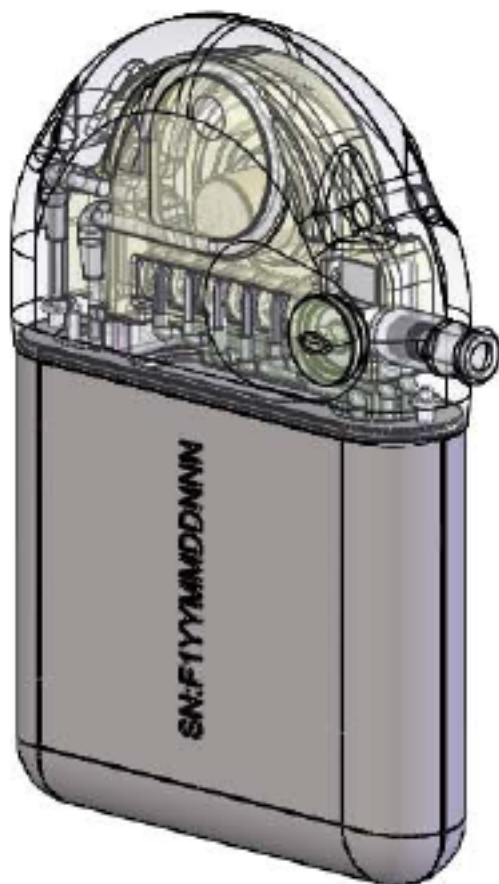


Figure 7 – Completed IPG device

CONFIDENTIAL

May not be reproduced, transmitted or disseminated in any form or by any means
without the written permission of an authorized representative of ImThera Medical, Inc.

