

This document is **CONFIDENTIAL** and contains designs and/or other information that are the property of ImThera Medical, Inc. This document and the designs and/or other information contained therein, may not, in whole or part, be duplicated or disclosed or used for the manufacture of any part(s)disclosed herein, or for any other purpose, without the prior written permission of ImThera Medical, Inc.

SolidWorks DWG


REVISION HISTORY		
REV.	DESCRIPTION	DCN
AA	INITIAL RELEASE	0413
AB	REFERENCE CHANGES PER DCN 0443	0443
AC	CORRECT EC ADDRESS, ADD PRODUCT REGISTRATION STICKER (ITEM 10)	0770

D

C

B

A

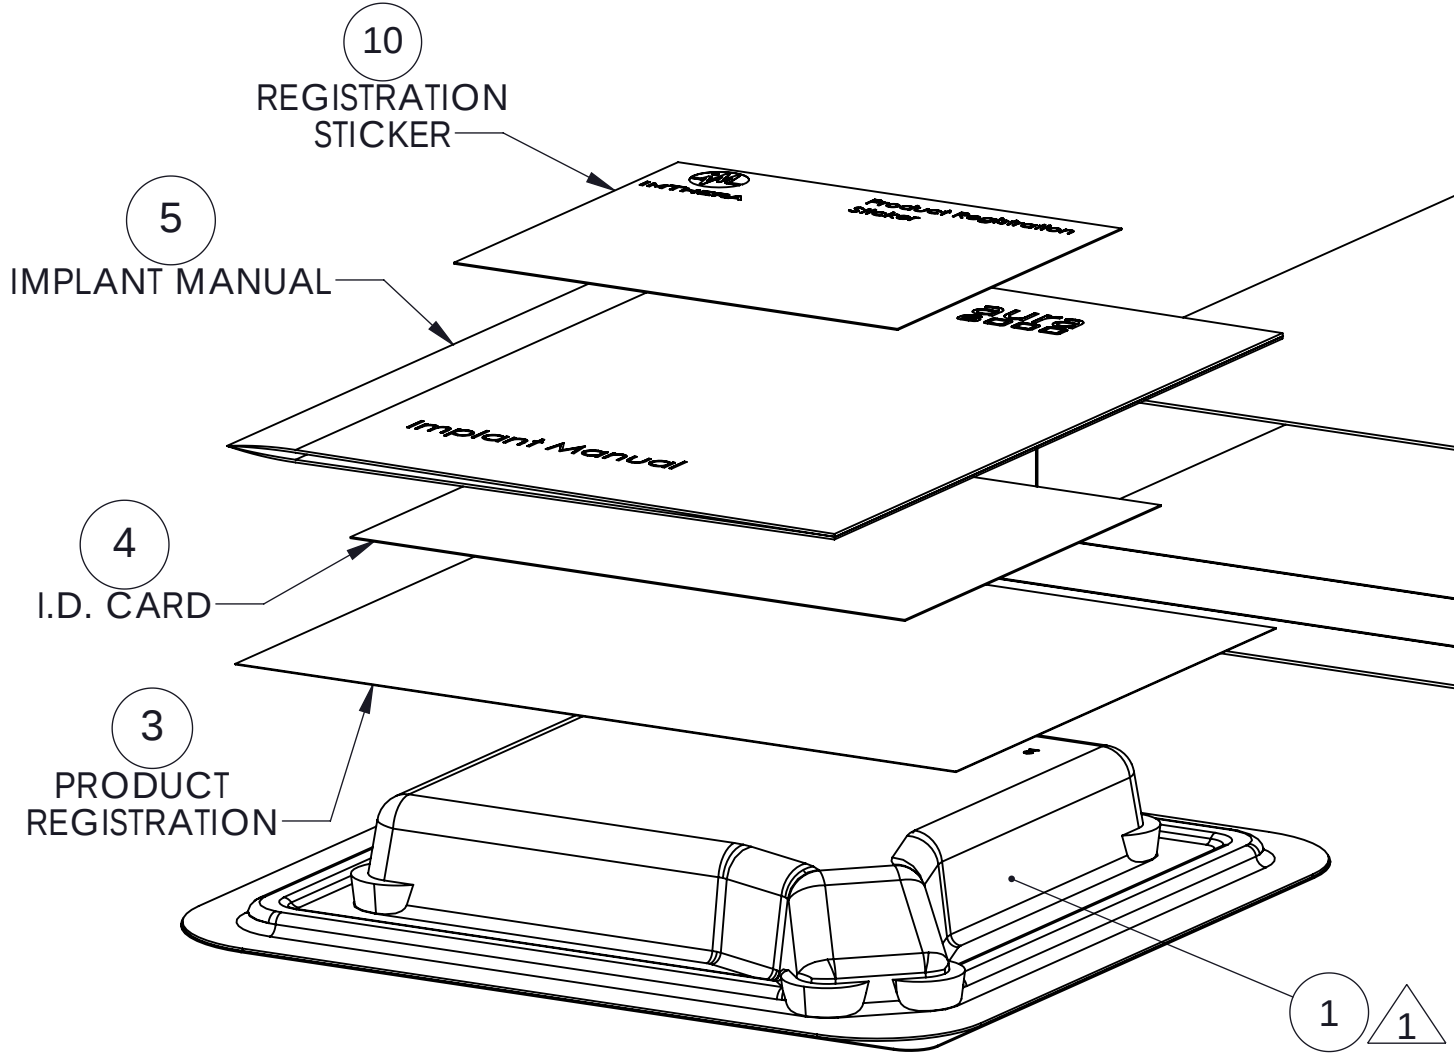

ITEM	PART NO.	DESCRIPTION	QTY
1	SPC-00643-01	POST-STERILE,PACKAGED IPG ASSEMBLY	1
2	T-100440	SHELF BOX	NA
3	REF. DWI-00647-01	PRODUCT REGISTRATION	2
4	REF. DWI-00647-01	TEMPORARY PATIENT I.D. CARD	2
5	REF. DWI-00647-01	IMPLANT MANUAL	2
6	ULINE, P/N: S-9994	TAMPER LABEL	1
7	T-100405	ETO INDICATOR LABEL	NA
8	LBL-00434-02	STERILE SHELF BOX LABEL	NA
9	REF. DWI-00647-01	IDE OVER LABEL	2
10	LBL-00414-01	IPG PRODUCT REGISTRATION STICKER	1

1. ITEM 1 (SPC-00643-01) INCLUDES ITEMS 2 (T-100440), 7 (T-100405) AND 8 (LBL-00434-02). THESE ITEMS ARE RECEIVED AS PART OF THE SPC-00643-01 ASSEMBLY AND ARE NOT INCLUDED IN THE MATERIALS KIT.
2. REFER TO DWI-00647-01 AND CONFIGURATION MATRIX (FRM-00660-01) TO DETERMINE PACKAGE CONTENT AND QUANTITIES.

NOTES: UNLESS OTHERWISE SPECIFIED:

UNLESS OTHERWISE SPECIFIED
ALL DIMS ARE IN INCHES.
ALL DIMS APPLY AFTER FINISH.

TOLERANCES

DECIMALS	.X ± .1	ANGLE	±1°
	.XX ± .01		
	.XXX ± .005		
	.XXXX ± .0005	FRACTION	±1/32

SURFACE FINISH PER ANSI-B46-1 32/✓
BREAK ALL EDGES .005 MAX.
FILLET RADII .005 MAX.

DO NOT SCALE DRAWING

SCALE	N/A	SHEET	1 of 3
-------	-----	-------	--------

IMTHERA MEDICAL, INC.

TITLE

Ship Level, IPG Assembly

DRAWN BY	DATE	SIZE	DRAWING NUMBER	REV
R.Brasc	03JAN13	B	SHP-100.0100-XX	AC

4


3

2

1

D

PRODUCT LITERATURE
STACKED ON BOTTOM
SIDE OF OUTER TRAY

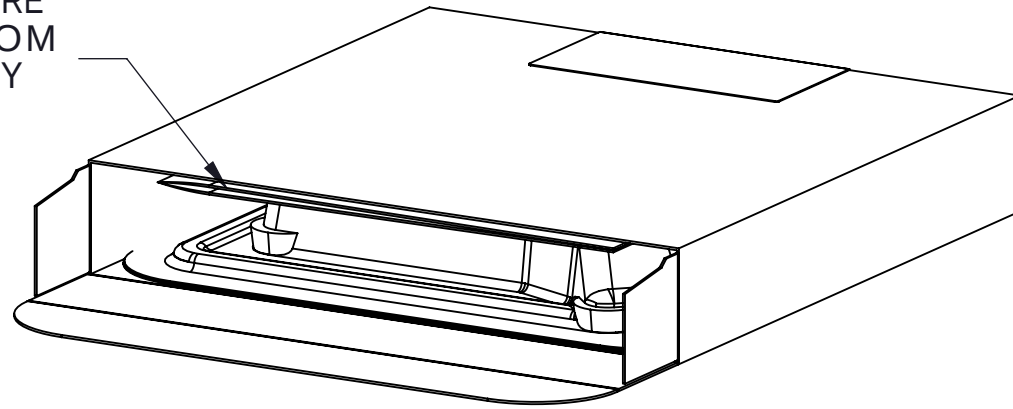


C

WHEN CHARGING, PLACE CHARGE ANTENNA
OVER LABEL LOCKING THE DEVICE MAGNET AND
ANTENNA MAGNET TOGETHER

B

A


6
TAMPER PROOF
LABEL

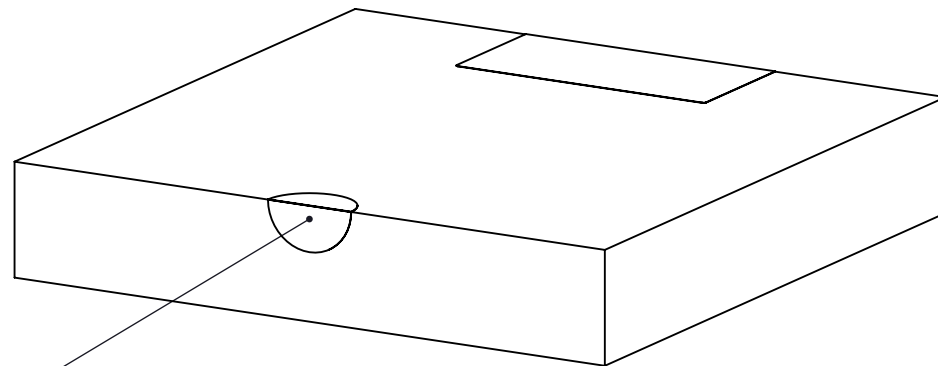

7 1
ETO INDICATOR

8 1
BOX LABEL

SEE PAGE 3 FOR DETAILED
LABEL INSTRUCTIONS

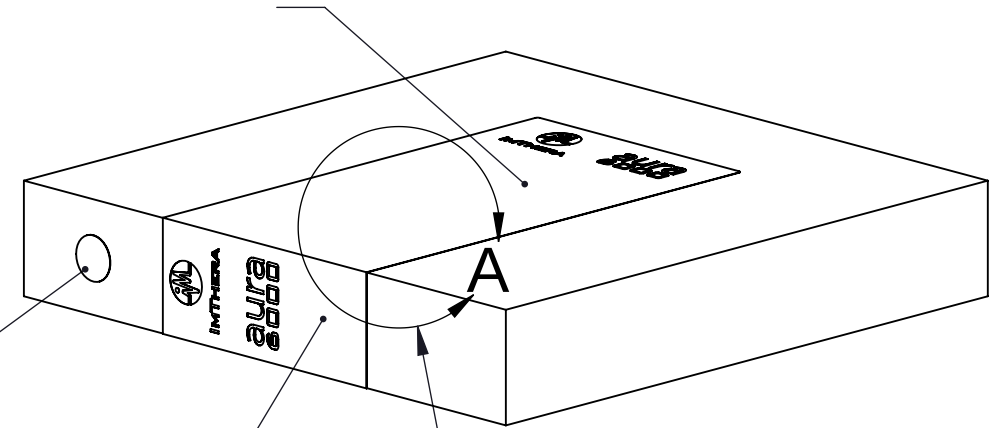

D

C

B

A


1



REF 100.0100

SN

- EN Neurostimulator Kit (IPG)**
Contents: 1 model 100.0100 IPG, accessories and documentation
- DE Neurostimulator Kit (IPG)**
Inhalt: Ein IPG Modell 100.0100, Zubehör und Dokumentation
- ES Conjunto de neuroestimulación (IPG)**
Contiene: un IPG ref 100.0100, accesorios y documentación
- FR Ensemble de neurostimulation (IPG)**
Contenu: 1 IPG modèle 100.0100, accessoires et documentation
- IT Kit Neurostimolatore Impiantabile (IPG)**
Contenuto: 1 IPG modello 100.0100 accessori e documentazione
- PT Kit De Neuroestimulação (IPG)**
Conteúdo: 1 modelo 100.0100 IPG , acessórios e documentação



MADE IN USA FOR EXPORT ONLY CE 0344 2012

Single Use Only

FCC FCC ID: 2AG55-IPG

STERILE EO

10°C 55°C

EC REP

Cormedics Medizintechnik GmbH
Bahnhofstrasse 32
82041 Deisenhofen Germany

ImThera Medical, Inc.
12555 High Bluff Drive, #310
San Diego, CA 92130 USA



Charge every 6 months. Last charge date:

_____	_____
_____	_____
_____	_____