



Appendix A

Detailed System Check Results

1. System Performance Check
System Performance Check 13 MHz
System Performance Check 2450 MHz
System Performance Check 5250 MHz
System Performance Check 5600 MHz
System Performance Check 5750 MHz
System Performance Check 6500 MHz
System Performance Check 10 GHz

Test Laboratory: SGS-SAR Lab

System Check_Head_13MHz

DUT: CLA-13; Type: CLA-13; Serial: SN1032

Communication System: UID 0, CW (0); Frequency: 13 MHz; Duty Cycle: 1:1

Medium: HSL_13; Medium parameters used: $f = 13 \text{ MHz}$; $\sigma = 0.713 \text{ S/m}$; $\epsilon_r = 55.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(15.44, 17.46, 16.16); Calibrated: 2025/11/07
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 2025/09/08
- Phantom: ELI5; Type: ELI5; Serial: 1143
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Configuration/Pin=250mW/Area Scan (8x8x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$
Maximum value of SAR (measured) = 0.142 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 13.74 V/m ; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 0.194 W/kg

SAR(1 g) = 0.107 W/kg ; SAR(10 g) = 0.069 W/kg

Smallest distance from peaks to all points 3 dB below = 15.2 mm

Ratio of SAR at M2 to SAR at M1 = 53.6%

Maximum value of SAR (measured) = 0.185 W/kg

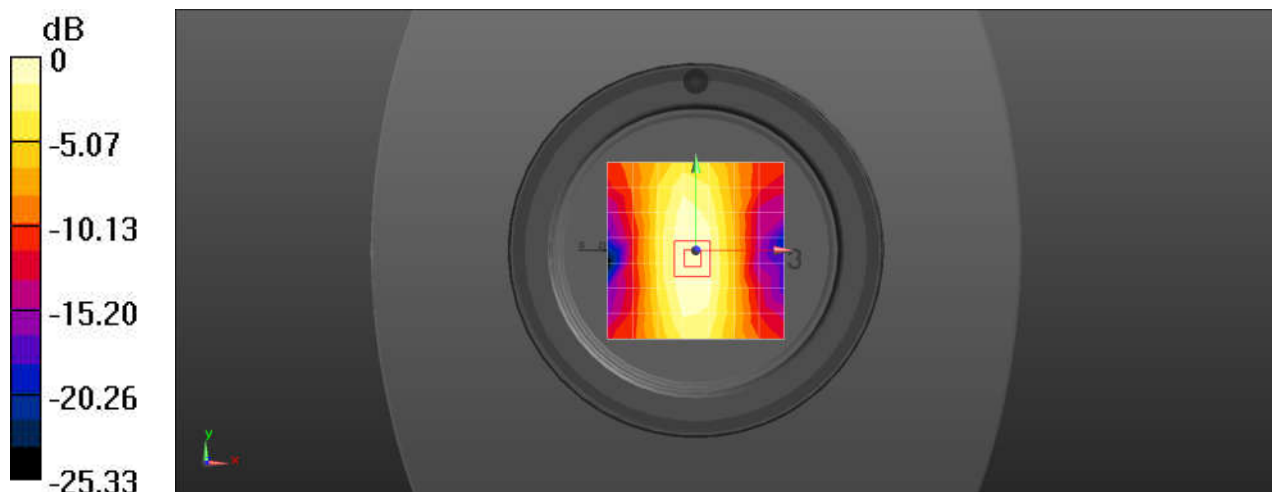

$0 \text{ dB} = 0.185 \text{ W/kg} = -7.33 \text{ dBW/kg}$


System Performance Check 2450MHz

Communication System: ; Frequency: 2450.000
Medium: HSL. Medium parameters used: $f= 2450.000$ MHz; $\sigma= 1.81$ S/m; $\epsilon_r = 38.9$

- DASY8 Configuration:
- Probe: EX3DV4 - SN7838; ConvF(7.55, 7.55, 7.55); Calibrated: 2026-02-02
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1374; Calibrated: 2026-02-02
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2217
 - Measurement Software: cDASY8 V16.4.0.5005

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.5 W/kg; SAR (10g) = 6.41 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 13.2 W/kg; SAR (10g) = 6.16 W/kg;
M2/M1 [%] 81.6
Dist 3dB Peak [mm] 9.3

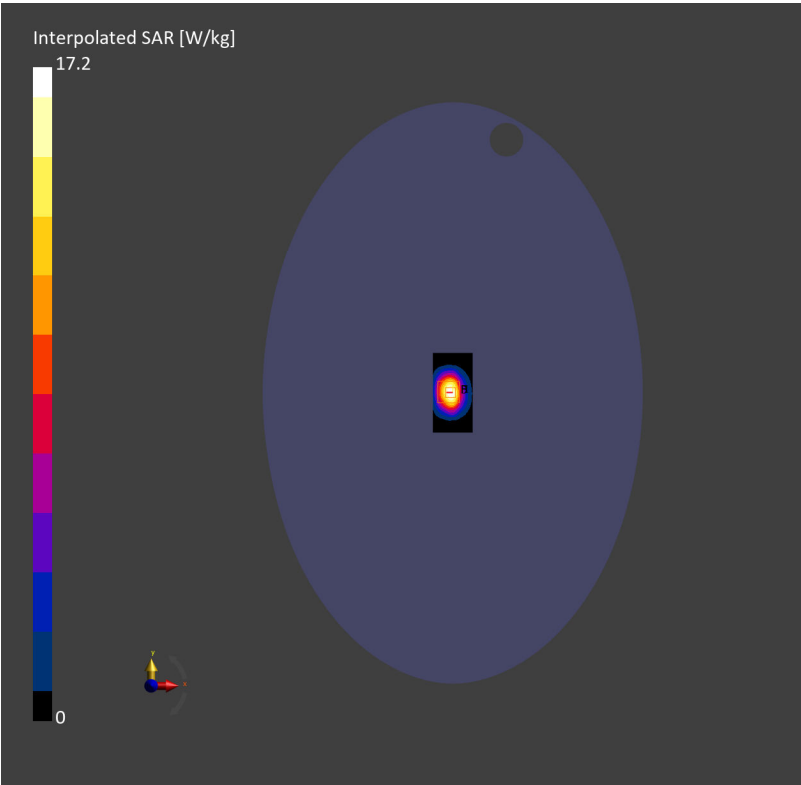


System Performance Check 5250MHz

Communication System: ; Frequency: 5250.000
Medium: HSL. Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.88$ S/m; $\epsilon_r = 36.7$

- DASY8 Configuration:
- Probe: EX3DV4 - SN7838; ConvF(5.35, 5.35, 5.35); Calibrated: 2026-02-02
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1374; Calibrated: 2026-02-02
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2217
 - Measurement Software: cDASY8 V16.4.0.5005

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 8.11 W/kg; SAR (10g) = 2.31 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.07 dB
SAR (1g) = 8.21 W/kg; SAR (10g) = 2.32 W/kg;
M2/M1 [%] 66.5
Dist 3dB Peak [mm] 7.9

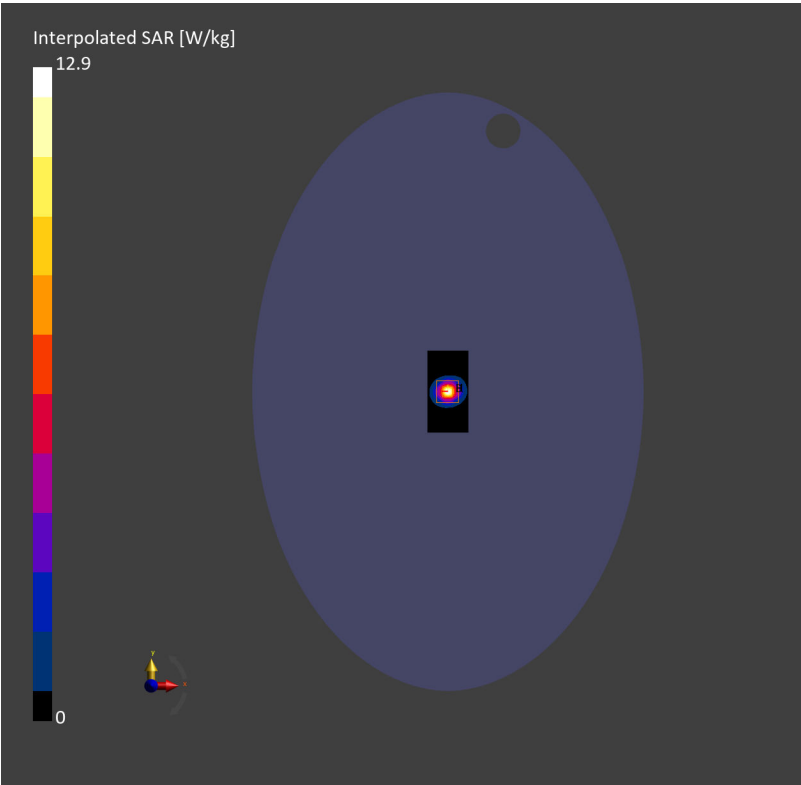


System Performance Check 5600MHz

Communication System: ; Frequency: 5600.000
Medium: HSL. Medium parameters used: $f= 5600.000$ MHz; $\sigma= 5.23$ S/m; $\epsilon_r = 36.3$

- DASY8 Configuration:
- Probe: EX3DV4 - SN7838; ConvF(4.75, 4.75, 4.75); Calibrated: 2026-02-02
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1374; Calibrated: 2026-02-02
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2217
 - Measurement Software: cDASY8 V16.4.0.5005

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 7.88 W/kg; SAR (10g) = 2.15 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.12 dB
SAR (1g) = 8.49 W/kg; SAR (10g) = 2.38 W/kg;
M2/M1 [%] 61.2
Dist 3dB Peak [mm] 7.9

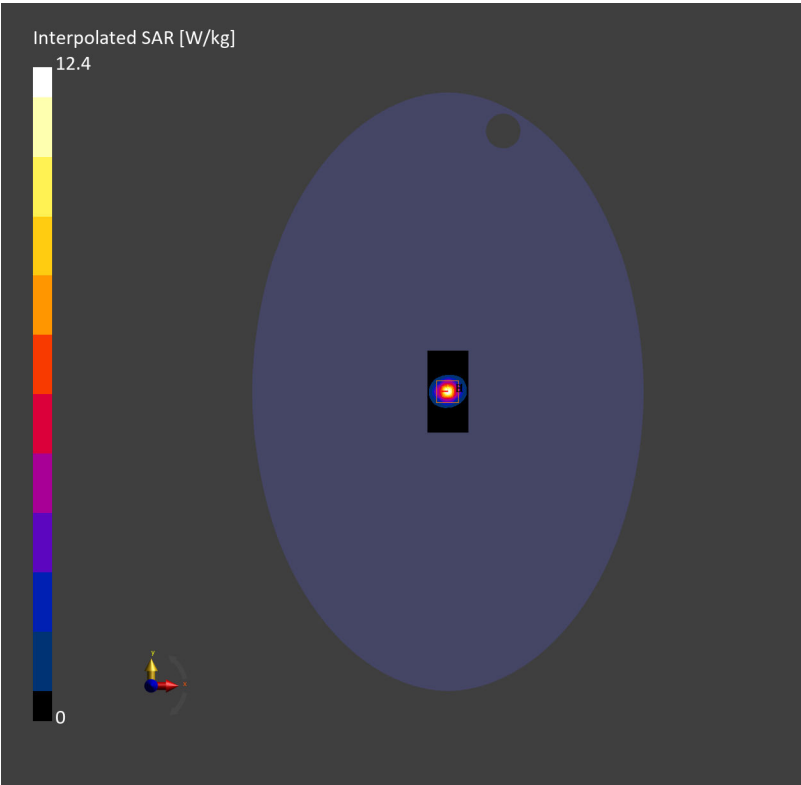


System Performance Check 5750MHz

Communication System: ; Frequency: 5750.000
Medium: HSL. Medium parameters used: $f= 5750.000$ MHz; $\sigma= 5.38$ S/m; $\epsilon_r = 35.9$

- DASY8 Configuration:
- Probe: EX3DV4 - SN7838; ConvF(4.86, 4.86, 4.86); Calibrated: 2026-02-02
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1374; Calibrated: 2026-02-02
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2217
 - Measurement Software: cDASY8 V16.4.0.5005

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 7.66 W/kg; SAR (10g) = 2.23 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.04 dB
SAR (1g) = 7.88 W/kg; SAR (10g) = 2.19 W/kg;
M2/M1 [%] 60.2
Dist 3dB Peak [mm] 7.7

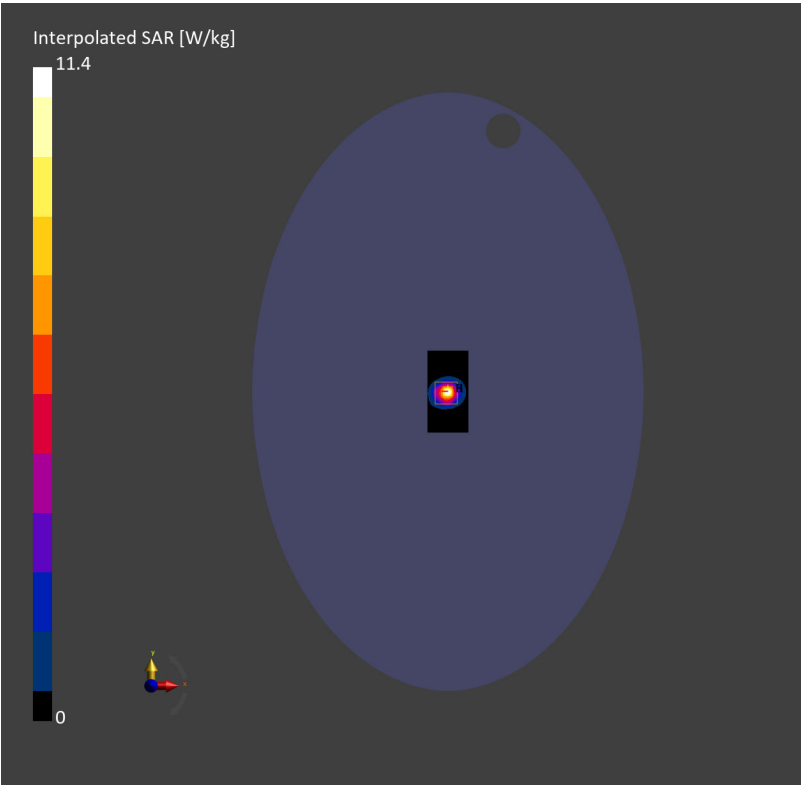


System Performance Check 6500MHz

Communication System: ; Frequency: 6500.000
Medium: HSL. Medium parameters used: $f=6500.000\text{ MHz}$; $\sigma=6.29\text{ S/m}$; $\epsilon_r=35.4$

- DASY8 Configuration:
- Probe: EX3DV4 - SN7838; ConvF(5.46, 5.46, 5.46); Calibrated: 2026-02-02
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1374; Calibrated: 2026-02-02
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2217
 - Measurement Software: cDASY8 V16.4.0.5005

Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm
 $\text{SAR (1g)} = 25.5\text{ W/kg}$; $\text{SAR (8g)} = 5.89\text{ W/kg}$; $\text{SAR (10g)} = 4.95\text{ W/kg}$;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm
Power Drift = 0.07 dB
 $\text{SAR (1g)} = 28.6\text{ W/kg}$; $\text{SAR (8g)} = 6.45\text{ W/kg}$; $\text{SAR (10g)} = 5.22\text{ W/kg}$;
psAPD (4.0cm2, sq) [W/m2] 129
M2/M1 [%] 56.5
Dist 3dB Peak [mm] 5.0

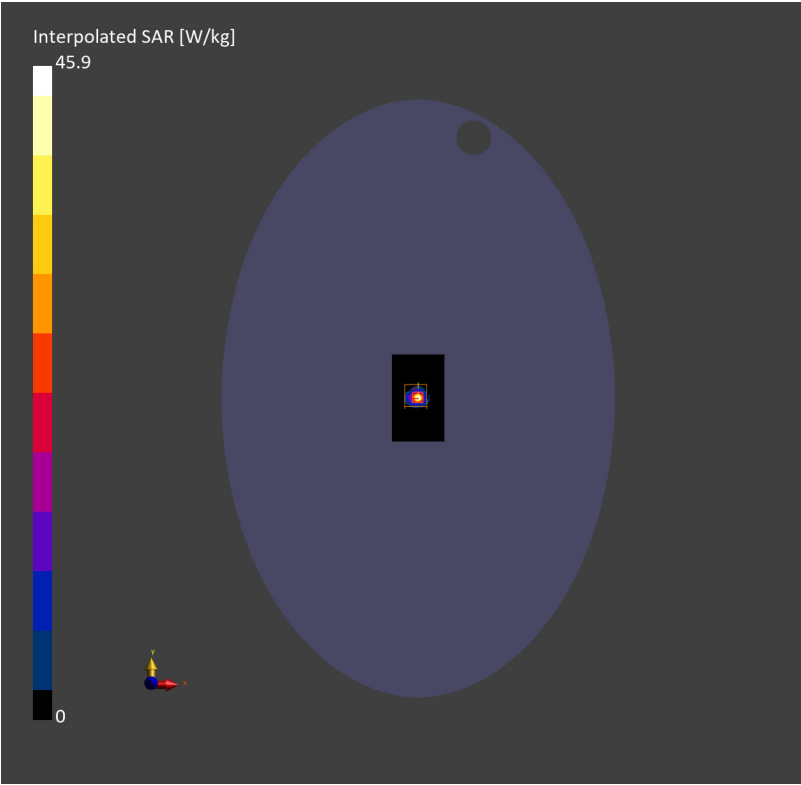

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
10G Source,	100.0 x 100.0 x 100.0	Phone

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup


Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave – 1777	Air –	EUmmWV4 – SN9718_F1–55GHz, 2025–08–04	DAE4 Sn1374, 2026–02–02

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2026–03–15
Avg. Area [cm²]	4.00
psPDn+ [W/m²]	173
psPDtot+ [W/m²]	175
psPDmod+ [W/m²]	179
E _{max} [V/m]	288
Power Drift [dB]	0.06

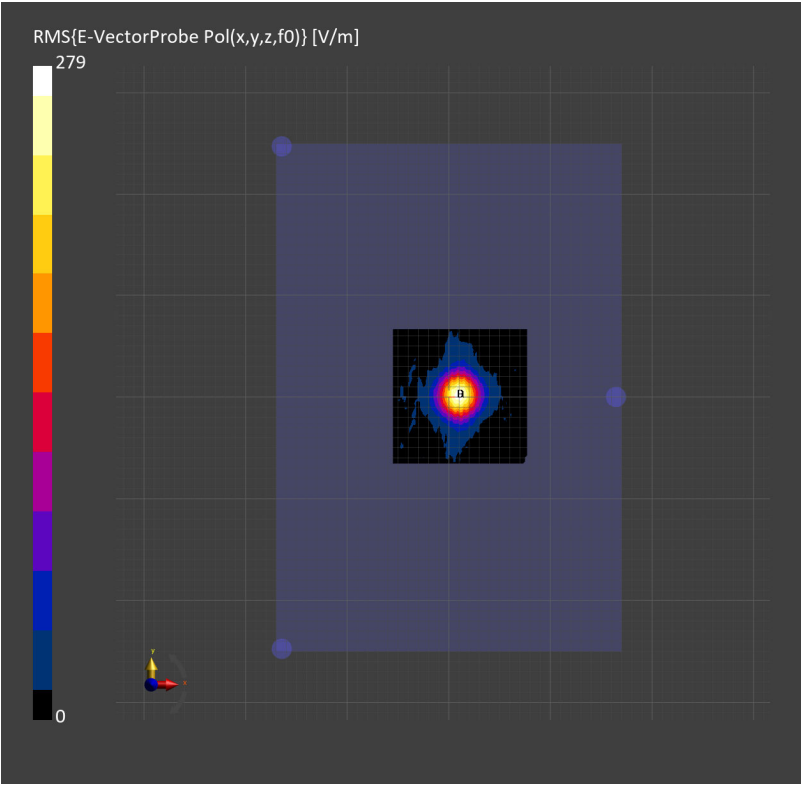



Report No.: SUCR260200011908
Page: 9 of 9

- End of the Appendix -