

APPENDIX

10. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

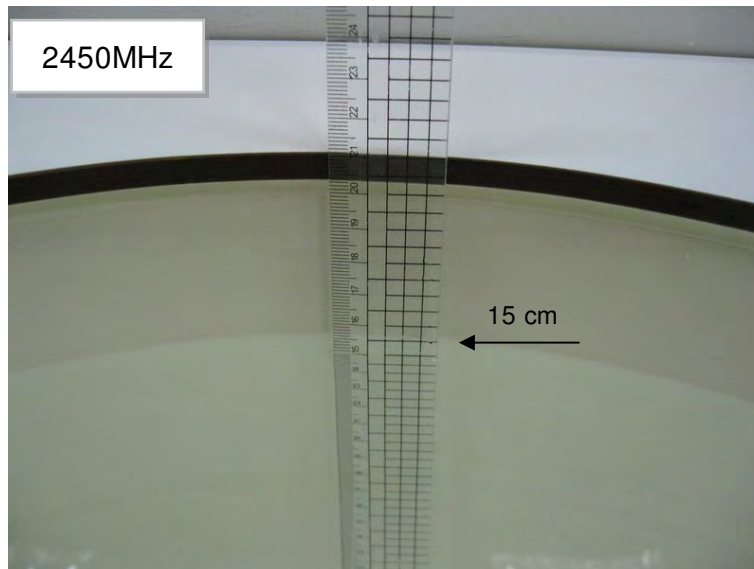


Fig.2

Body - distance between flat phantom and EUT is 0 mm



Fig.3 EUT Inner surface side to flat phantom

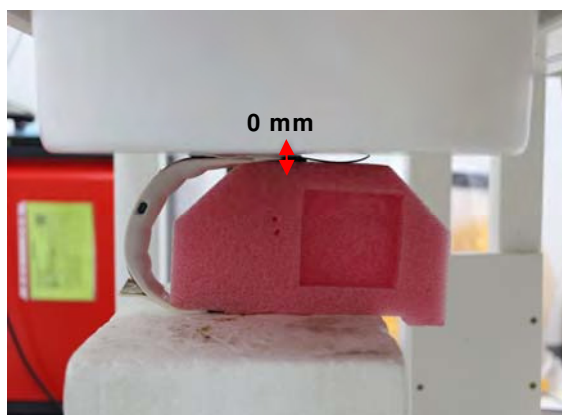


Fig.4 EUT Outer surface side to flat phantom

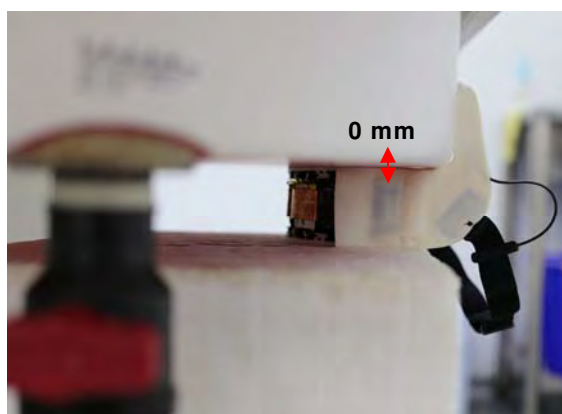


Fig.5 EUT Edge side_1 to flat phantom

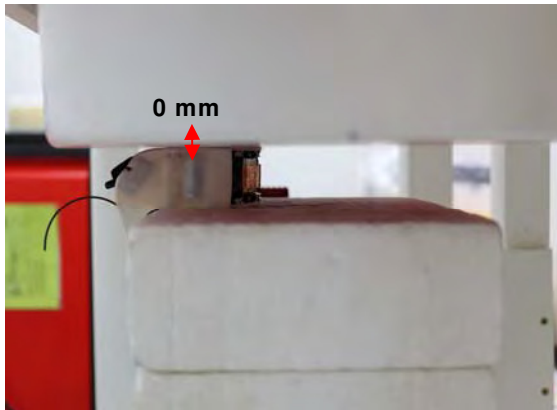


Fig.6 EUT Edge side_2 to flat phantom

11. Photographs of the EUT



Fig.7 Front view of EUT



Fig.8 Back view of EUT

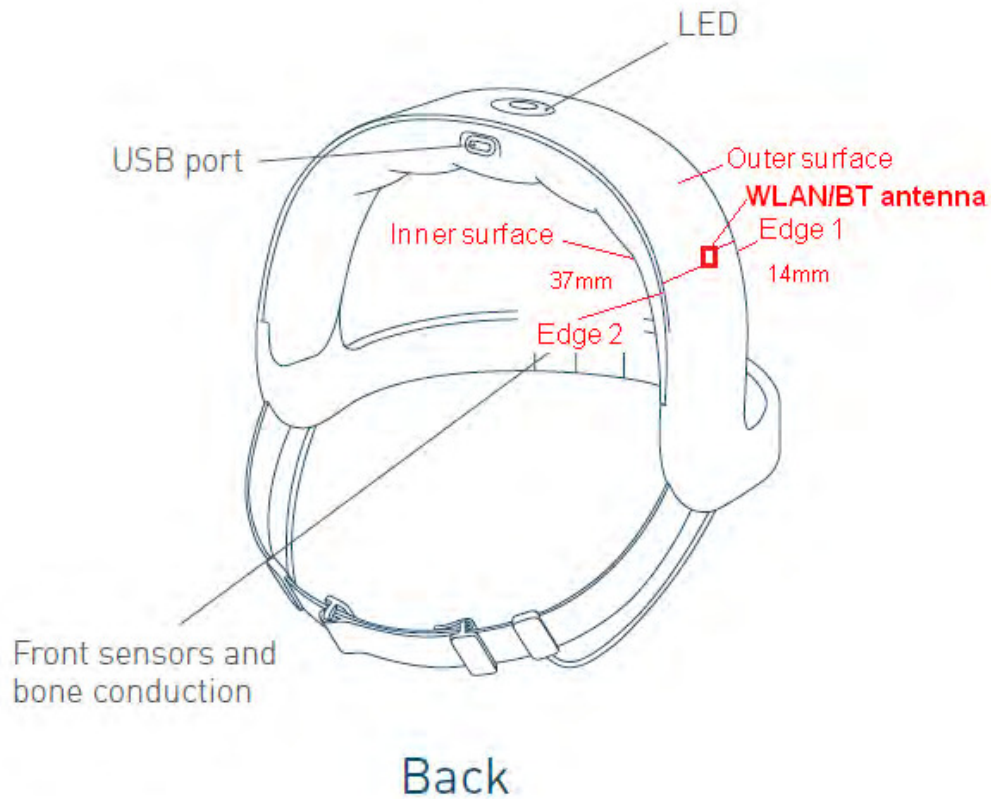


Fig.9 Antenna position of EUT

- End of Report -