
Annex 1 to Test Report # EMCC-150530A, 2016-04-25

PHOTOGRAPHS OF TEST SET-UP

EQUIPMENT UNDER TEST:

Device:	AG501
Serial Number:	03-12-10-24
Equipment Class:	Articulograph
Manufacturer:	Carstens Medizinelektronik GmbH
Address:	Nelkenweg 8 37120 Bovenden Germany
Phone:	+49 5593 1697
Fax:	+49 5593 8791

RELEVANT STANDARD(S): 47 CFR §§ 15.207, 15.209

MEASUREMENT PROCEDURE:

☒ ANSI C63.10-2013 ☐ RSS-Gen Issue 4 ☐ Other



Photo A1-1: Conducted emissions measurement

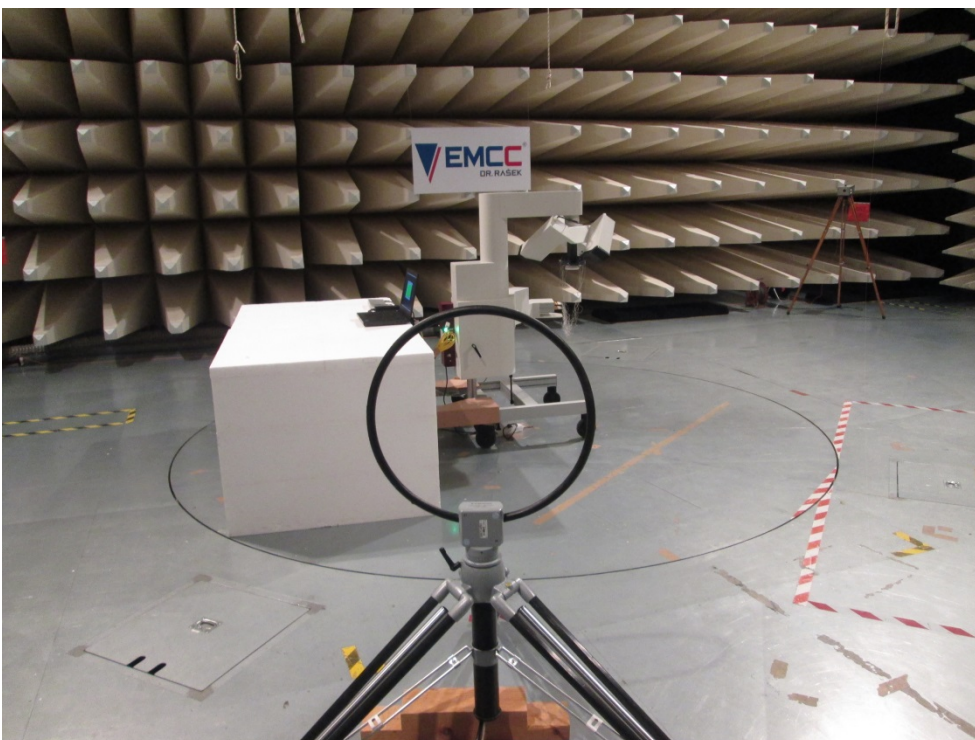


Photo A1-2: Radiated emissions measurement at 3 m distance, 9 kHz – 30 MHz



Photo A1-3: Radiated emissions measurement at 3 m distance, 9 kHz – 30 MHz, reference measurement at open field site

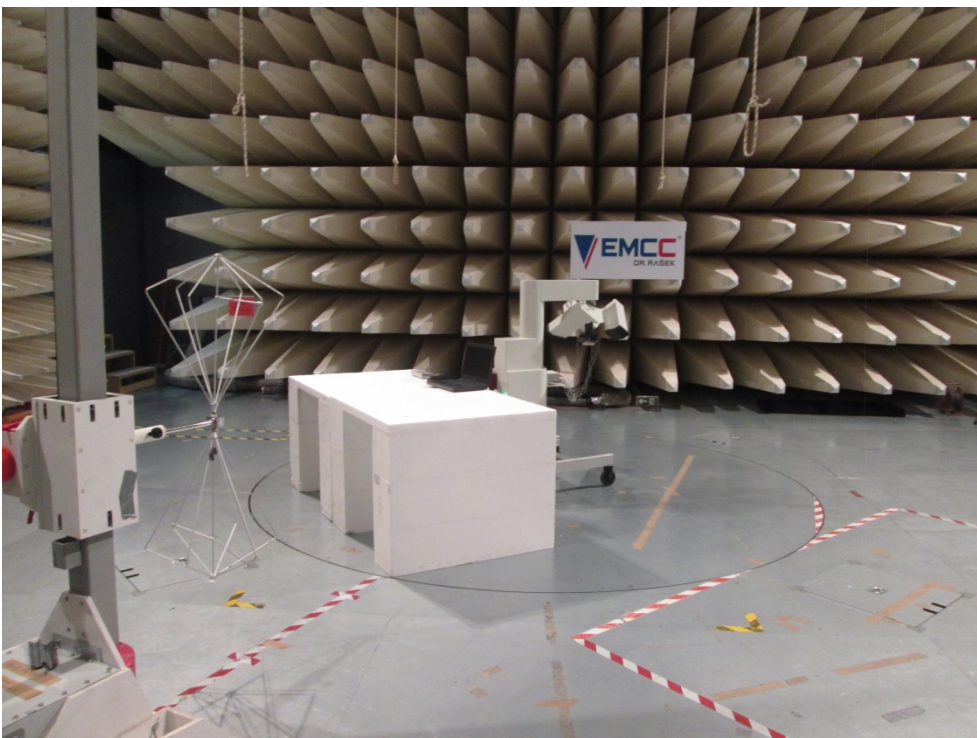


Photo A1-4: Radiated emissions measurement at 3 m distance, 30 MHz – 300 MHz

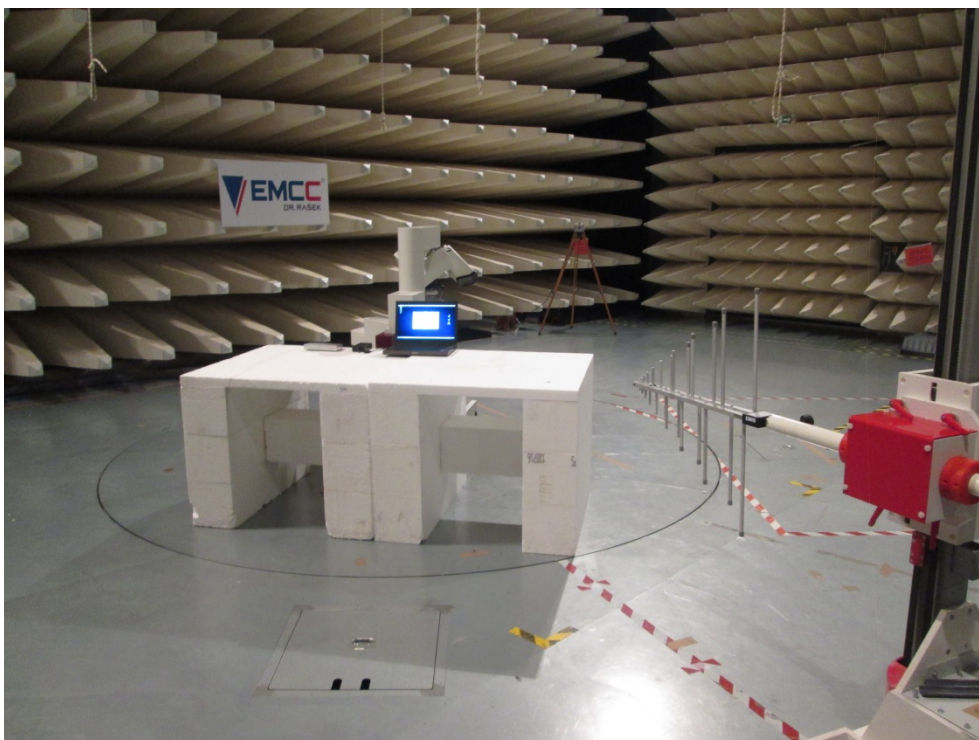


Photo A1-5: Radiated emissions measurement at 3 m distance, 300 MHz – 1000 MHz

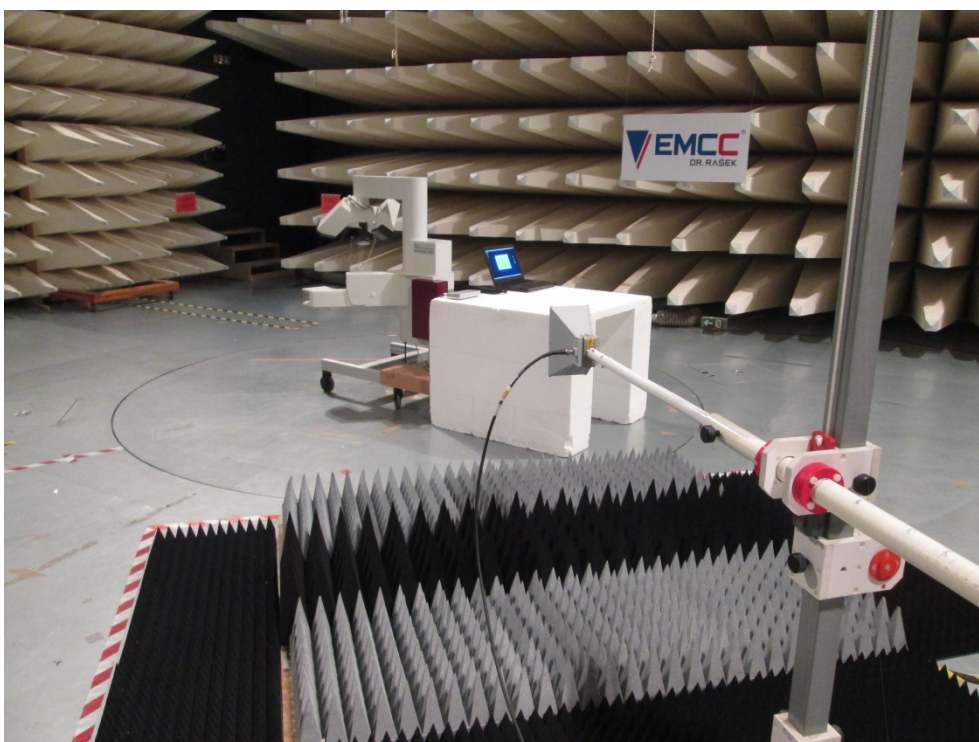


Photo A1-6: Radiated emissions measurement at 3 m distance, 1 GHz – 5 GHz