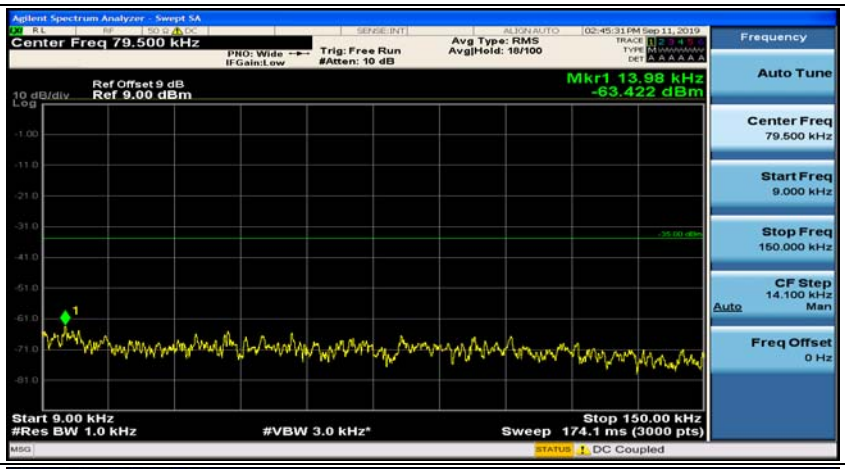

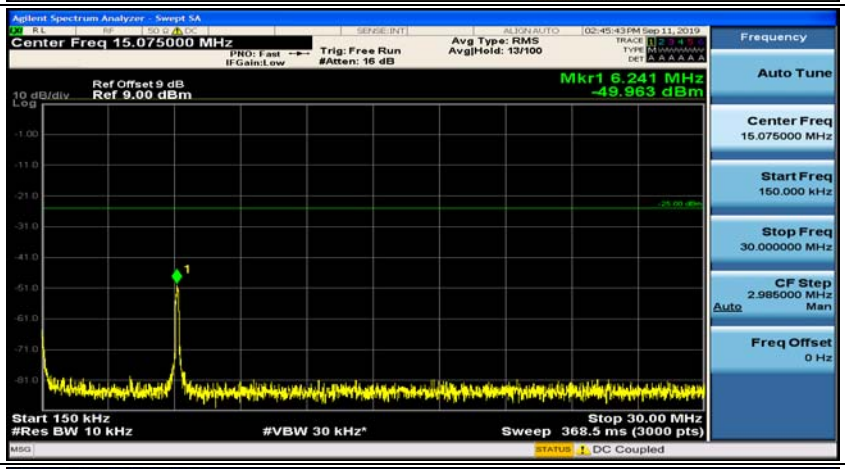

(Channel Bandwidth: 5 MHz)_HCH_16QAM_1RB#24

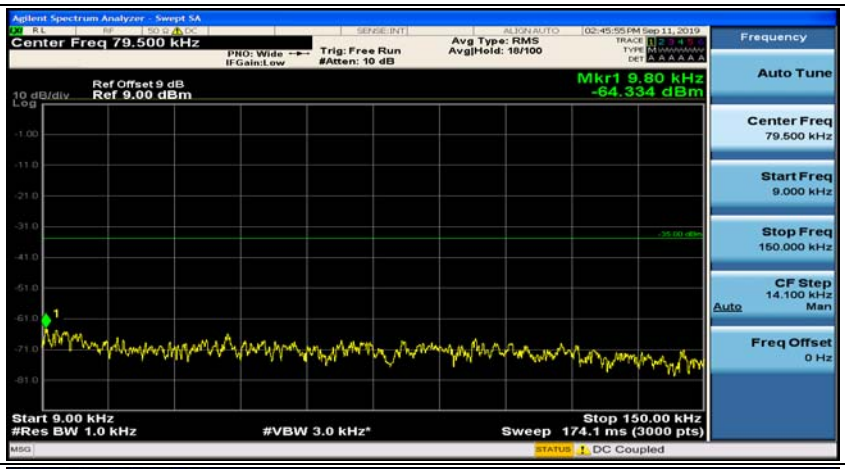
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:45:55 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.80 kHz
-64.334 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

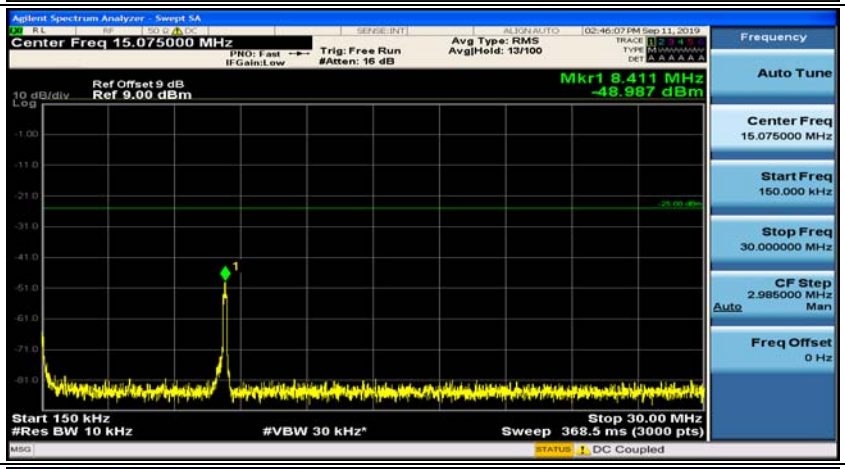
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:46:07 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 8.411 MHz
-48.987 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:46:12 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.822 GHz
-44.443 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz

Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#0
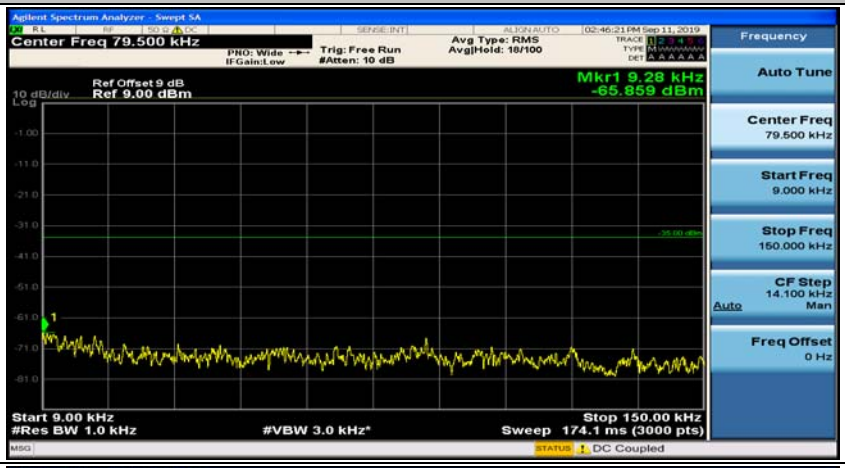
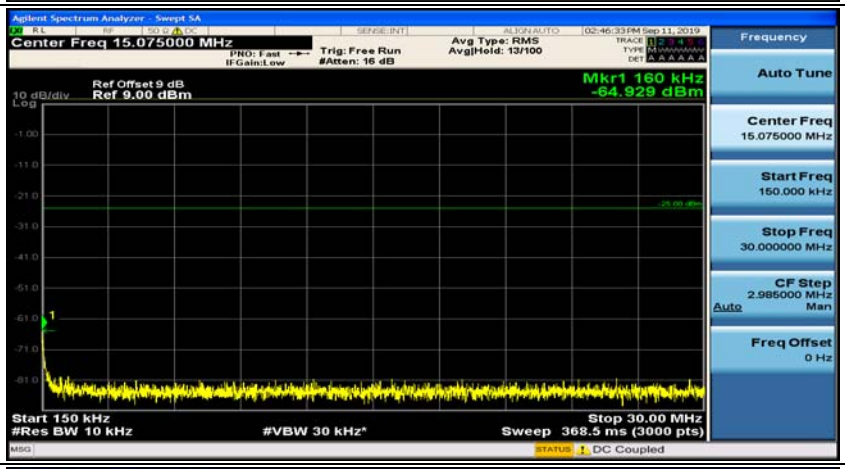
Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#24

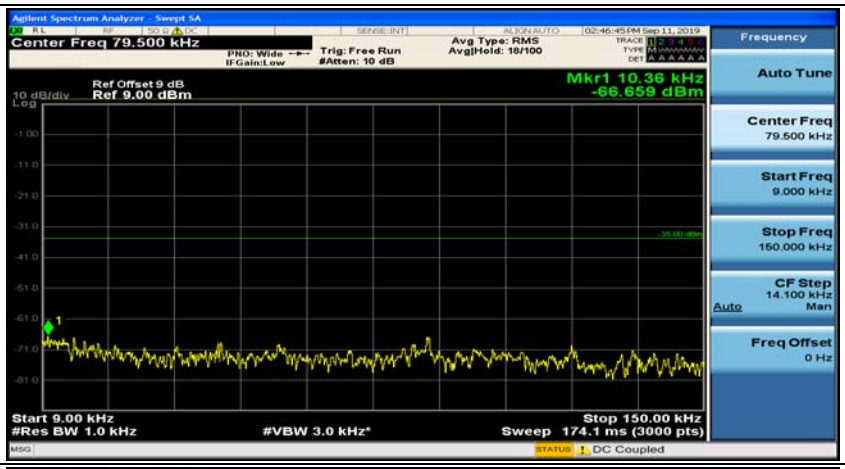

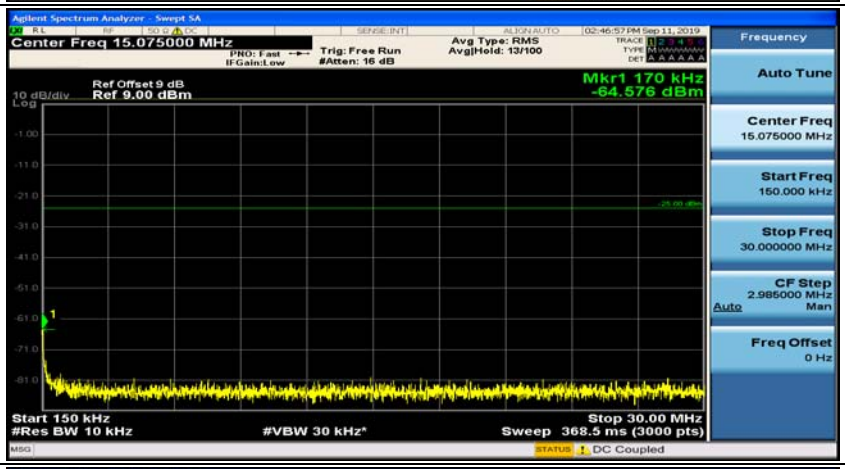

Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#49

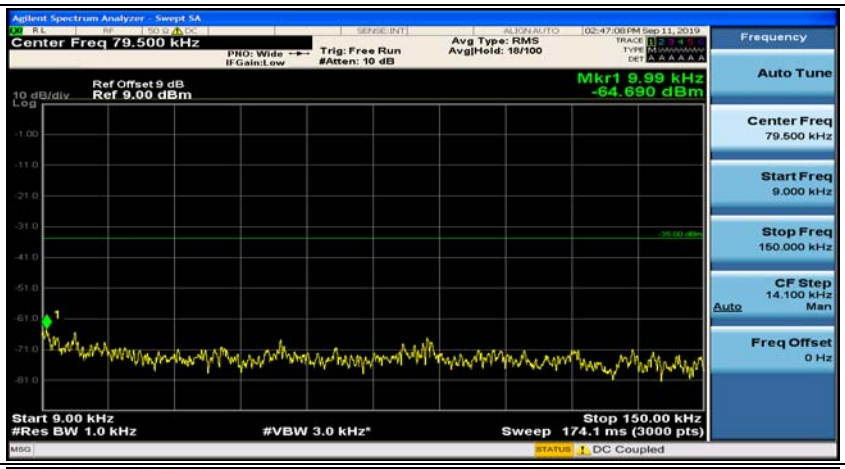
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:47:08 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.99 kHz
-64.690 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

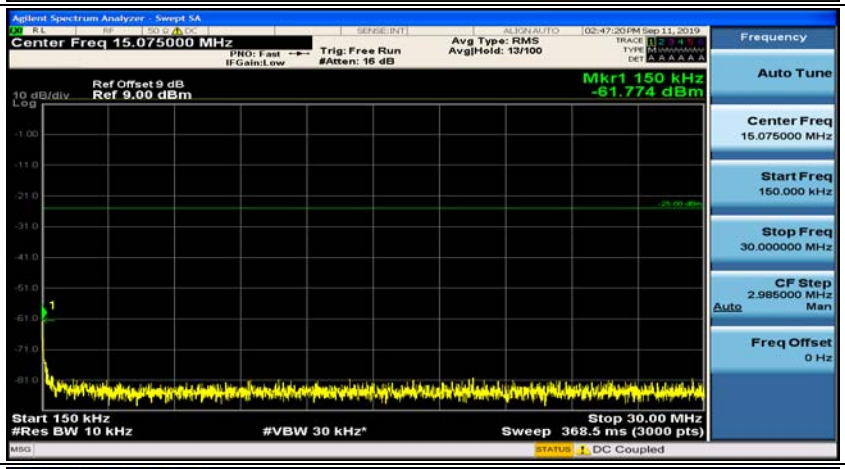
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:47:20 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-61.774 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:47:26 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.848 GHz
-44.890 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#0
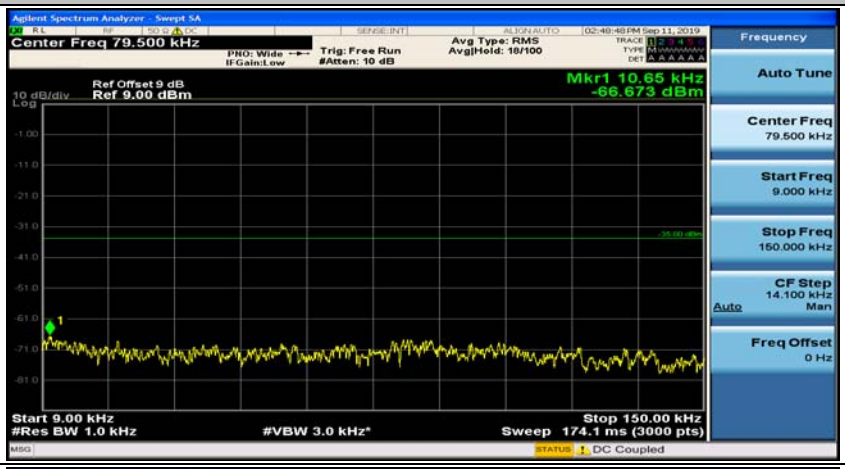
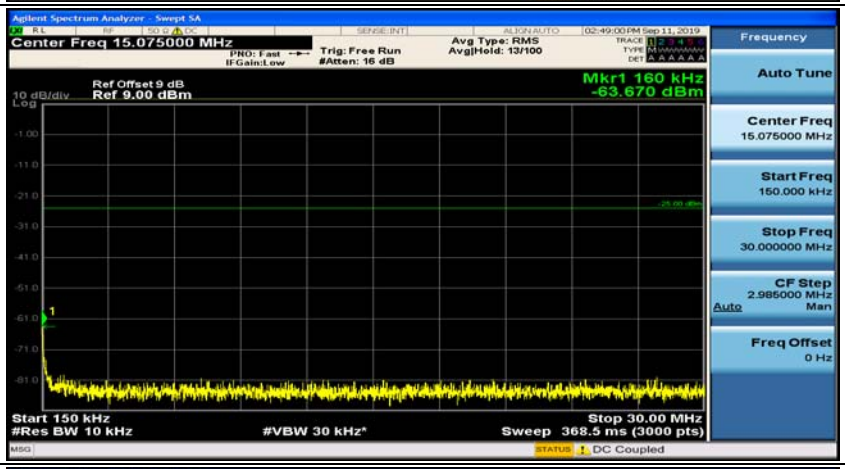
Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#24

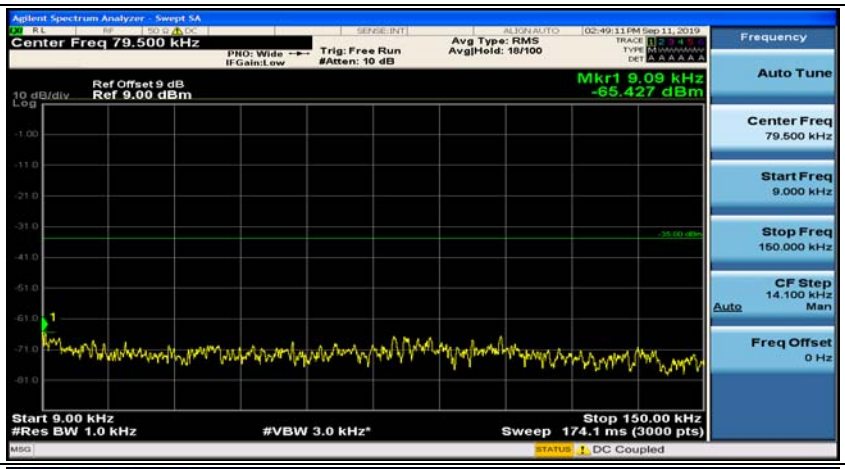

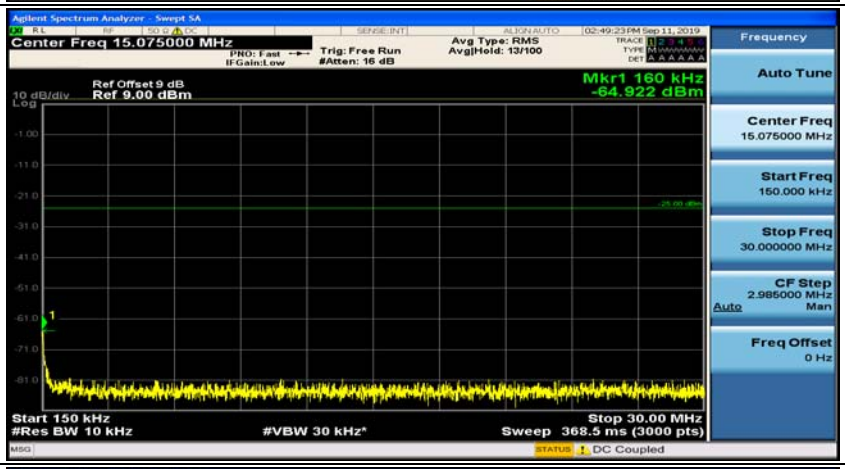

Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#49

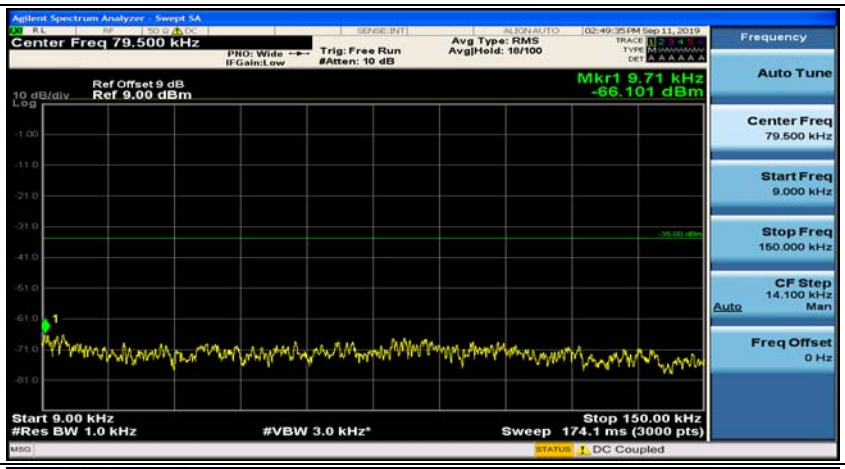
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:49:35 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.71 kHz
-66.101 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

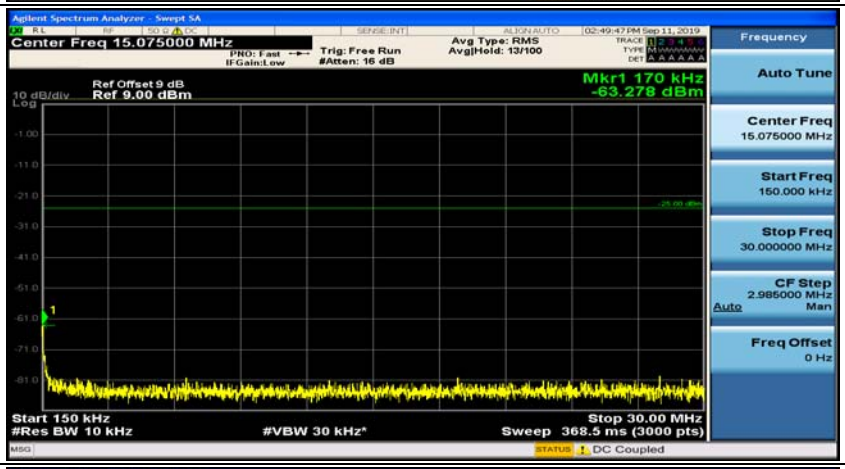
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:49:47 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 170 kHz
-63.279 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 15/100
02:49:52 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.900 GHz
-44.836 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#0
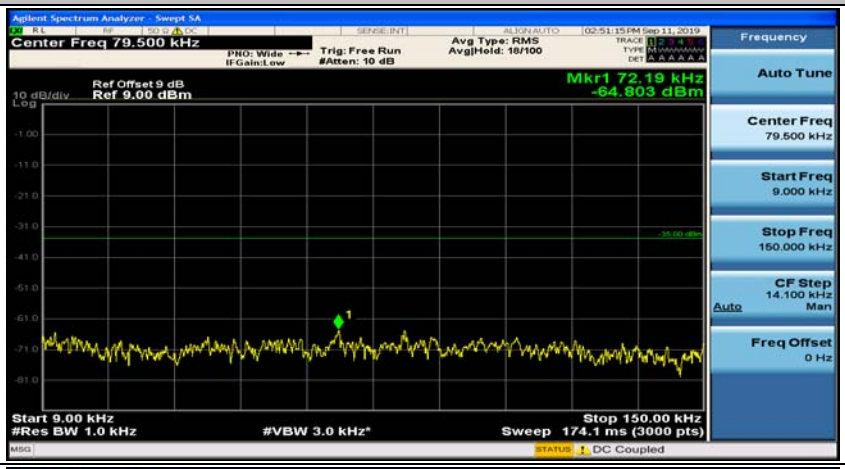
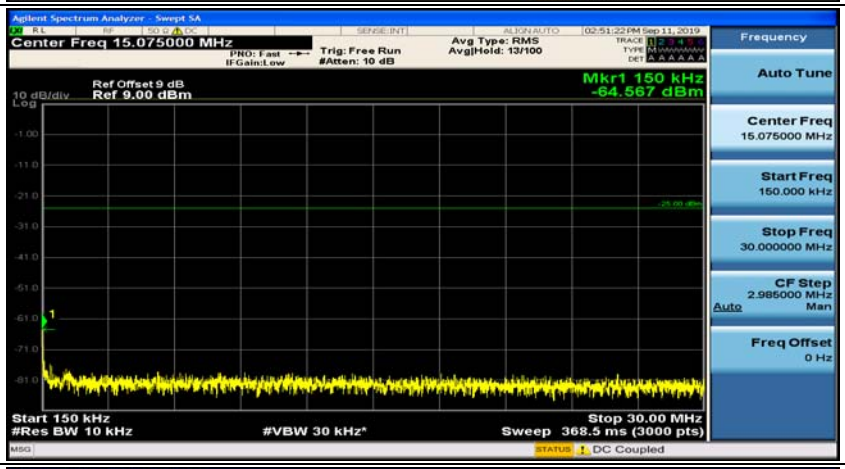
Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#24

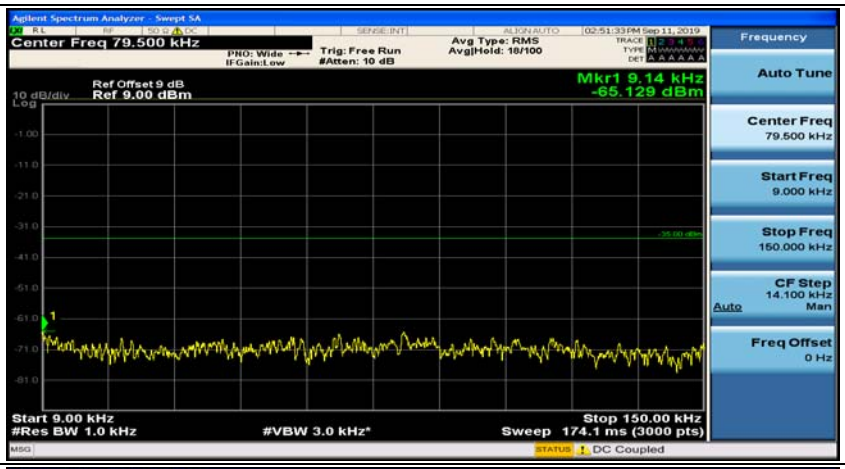

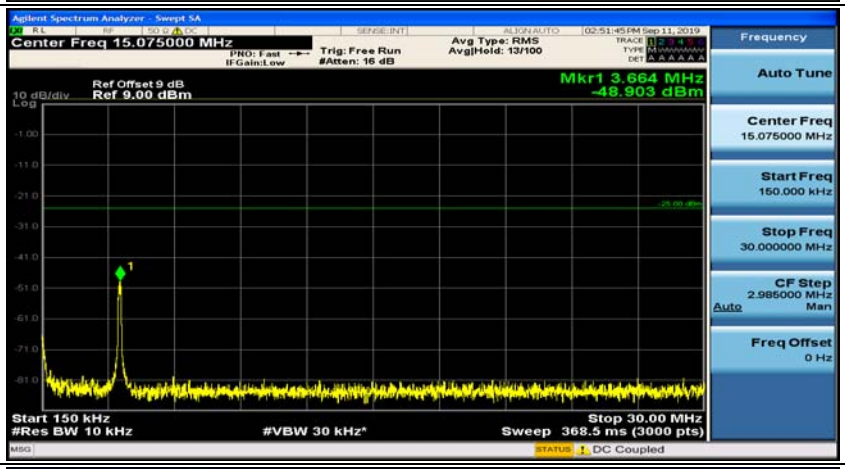

Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#49

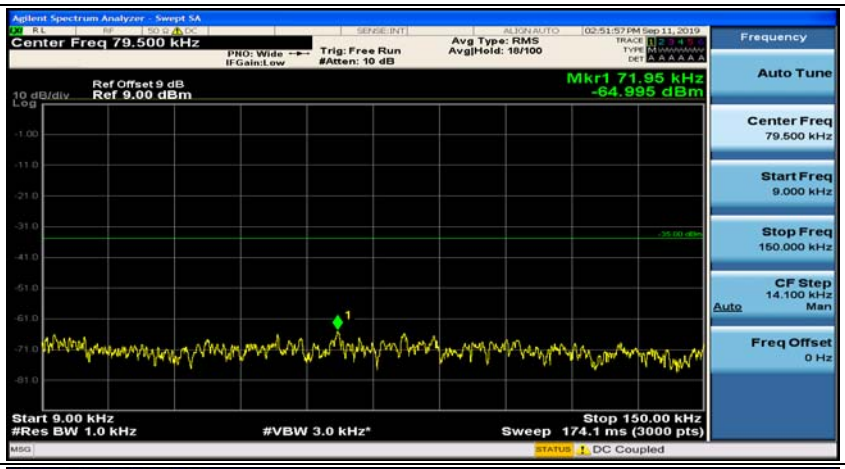
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:51:57 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 71.95 kHz
-64.995 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

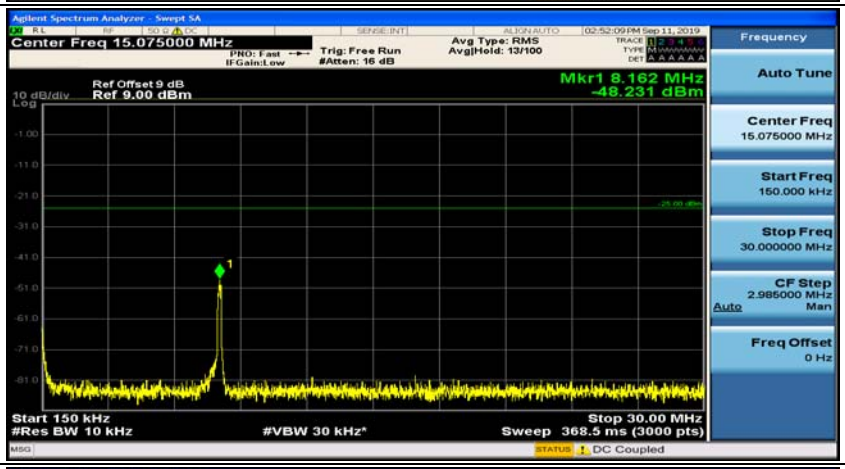
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:52:09 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 8.162 MHz
-48.231 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:52:14 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.840 GHz
-44.679 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Input Overload;ADC over range
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#0
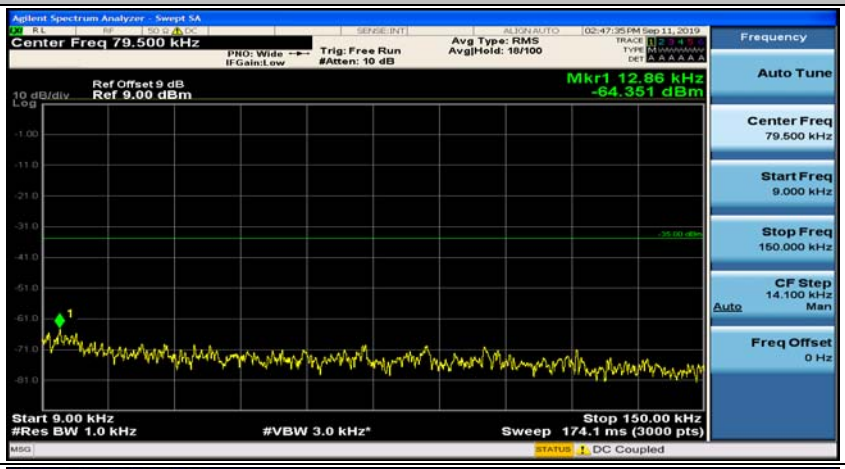
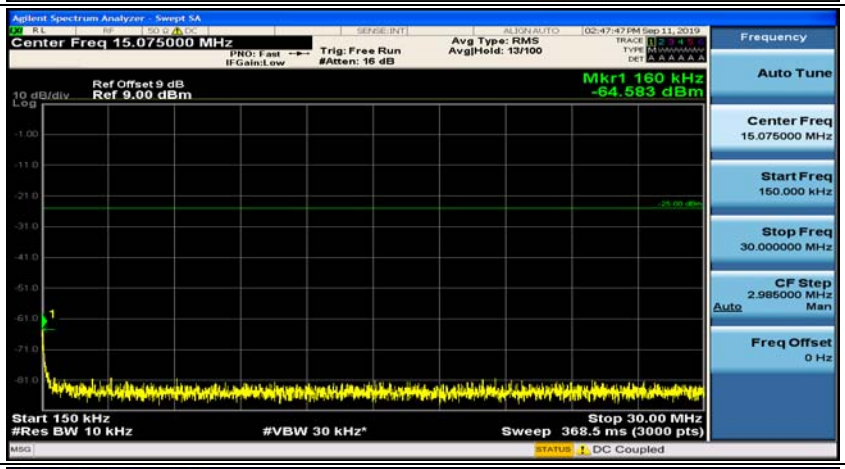
Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#24

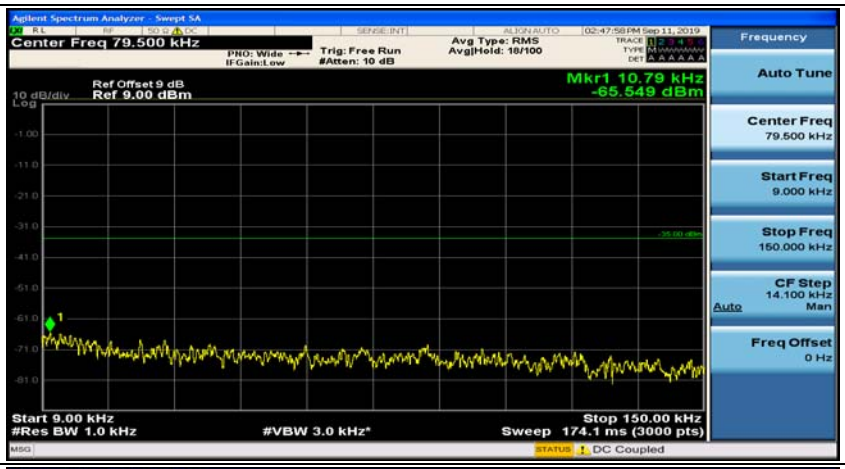

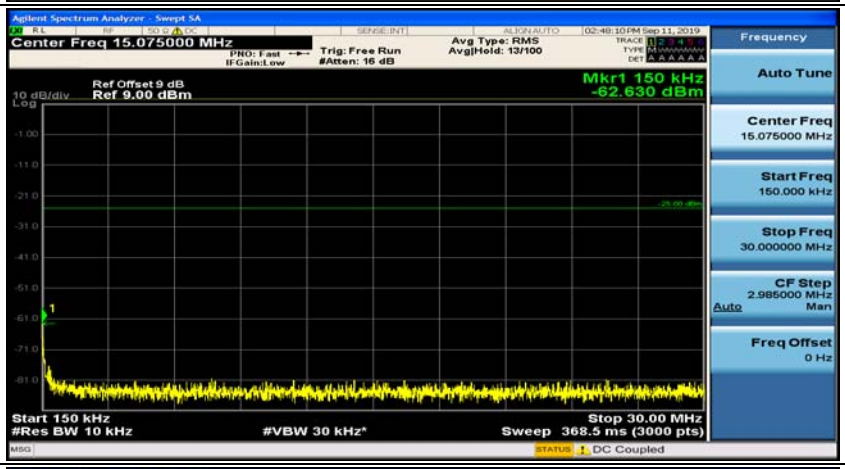

Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#49

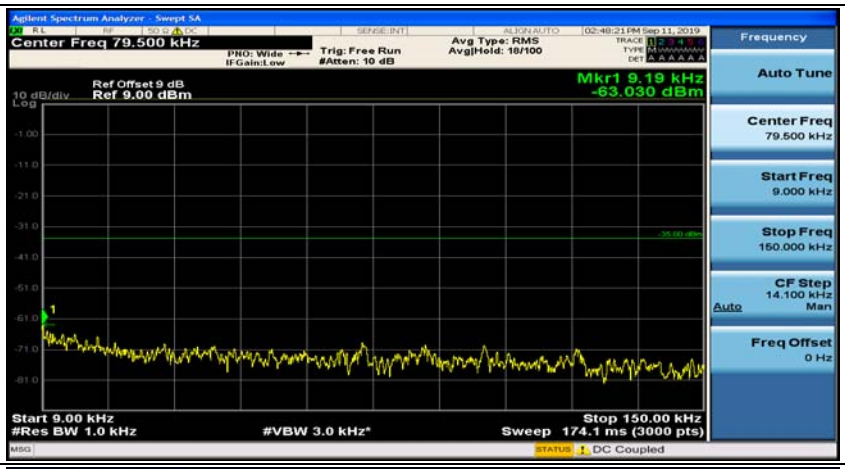
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:48:21 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.19 kHz
-63.030 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

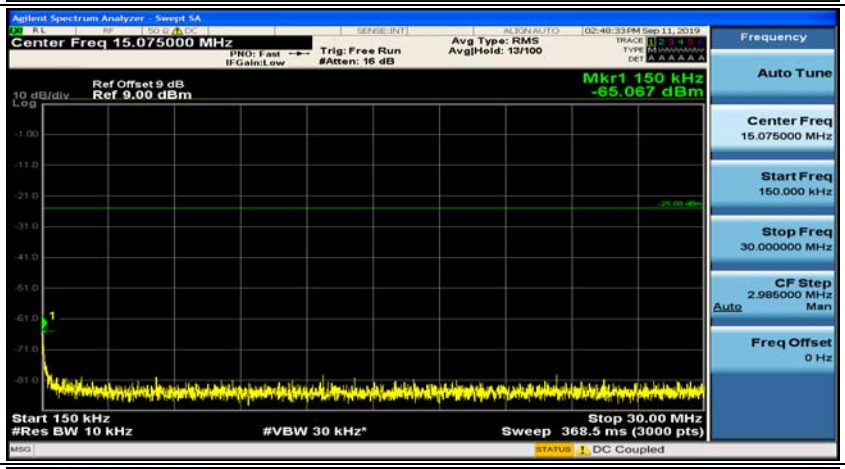
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:48:33 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-65.067 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:48:39 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.892 GHz
-44.869 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_MCH_16QAM_1RB#0
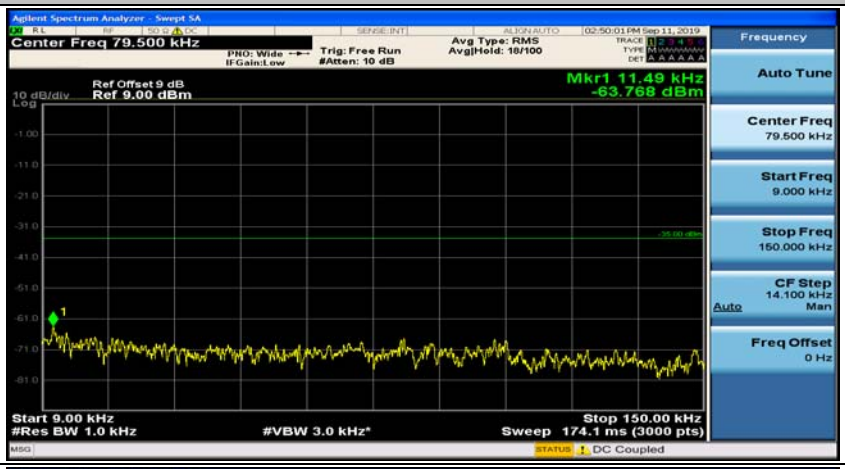
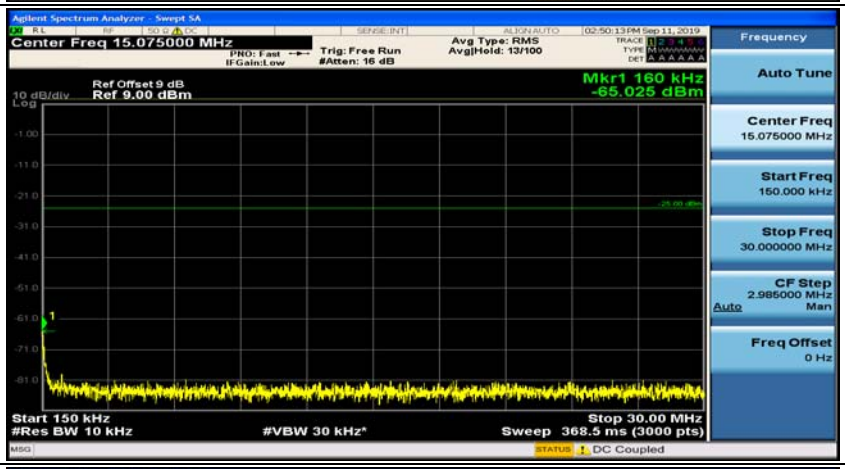
Channel Bandwidth: 10 MHz_MCH_16QAM_1RB#24

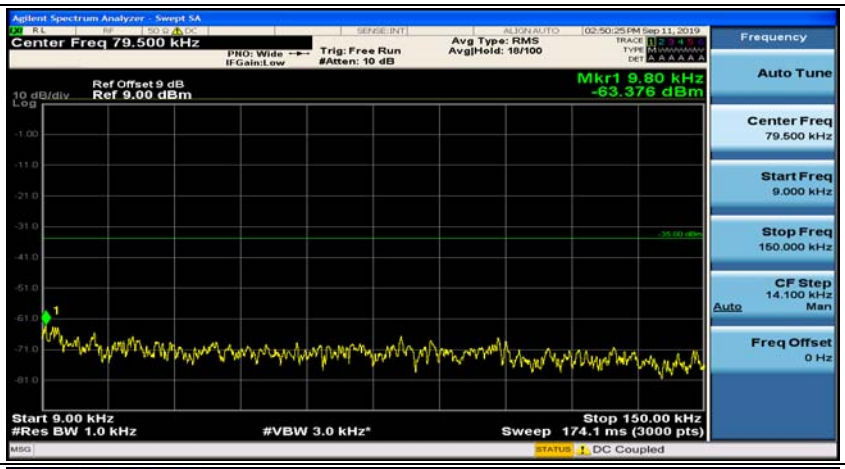

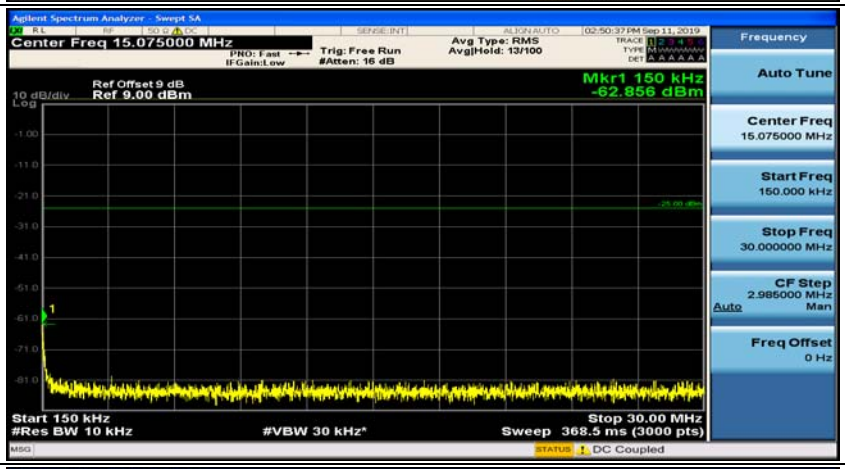

Channel Bandwidth: 10 MHz_MCH_16QAM_1RB#49

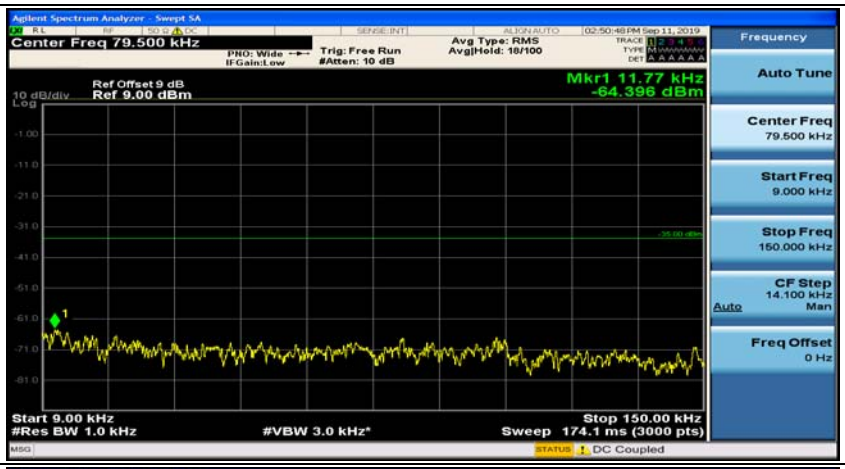
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:50:48 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 11.77 kHz
-64.396 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

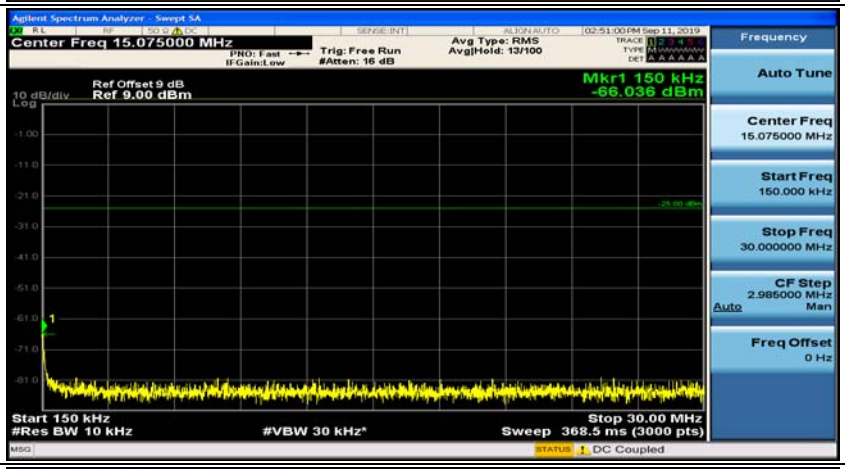
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:51:00 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-66.036 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:51:06 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.805 GHz
-44.093 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_HCH_16QAM_1RB#0
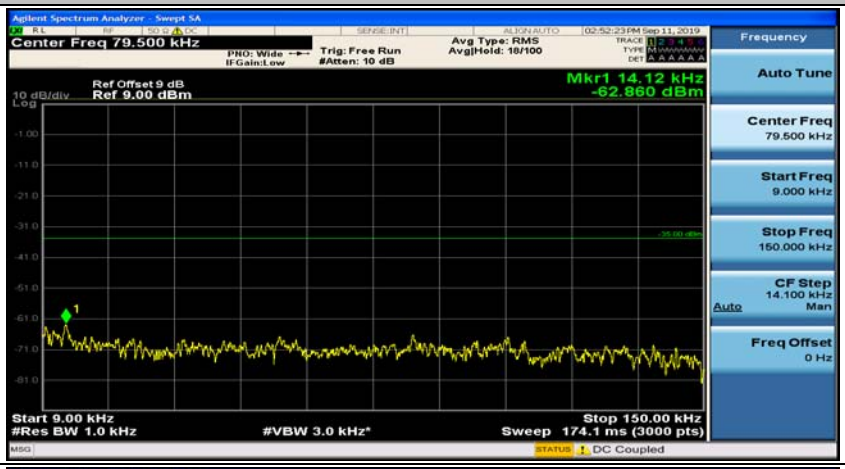
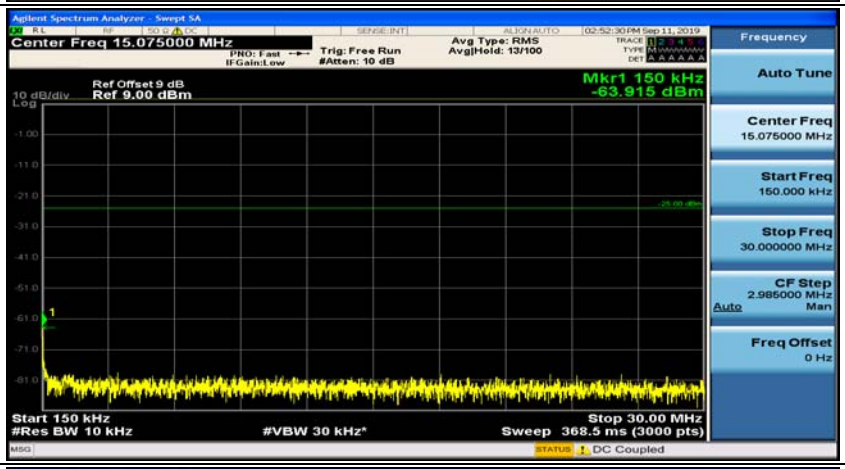
Channel Bandwidth: 10 MHz_HCH_16QAM_1RB#24

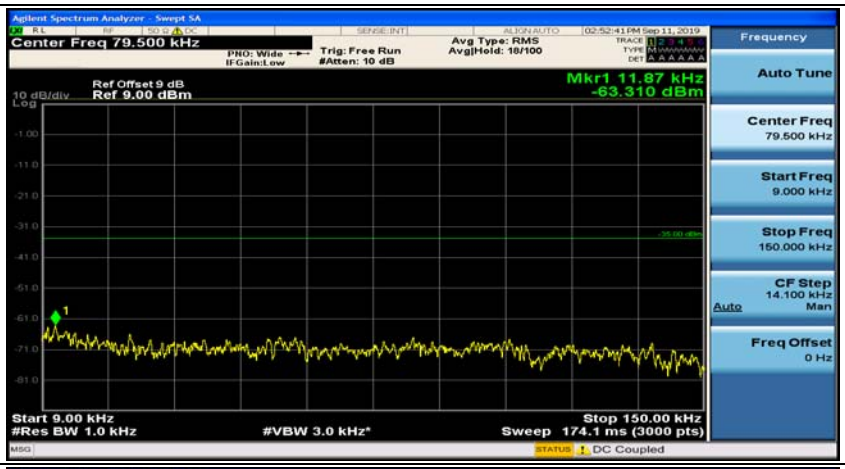

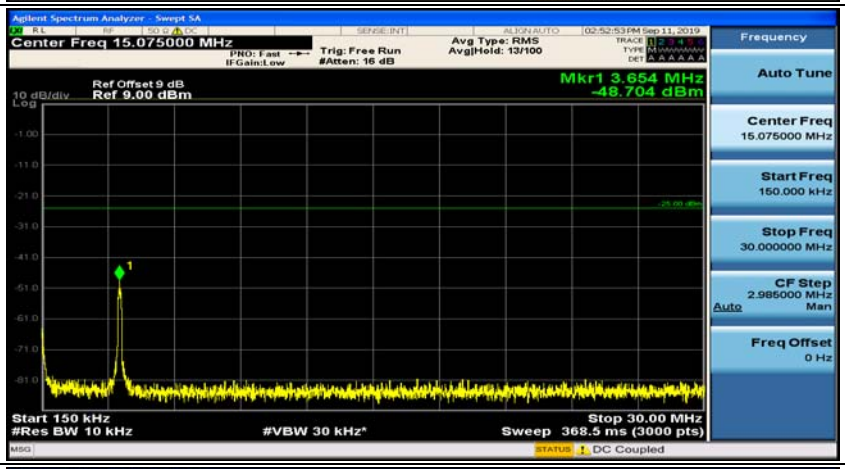

Channel Bandwidth: 10 MHz_HCH_16QAM_1RB#49

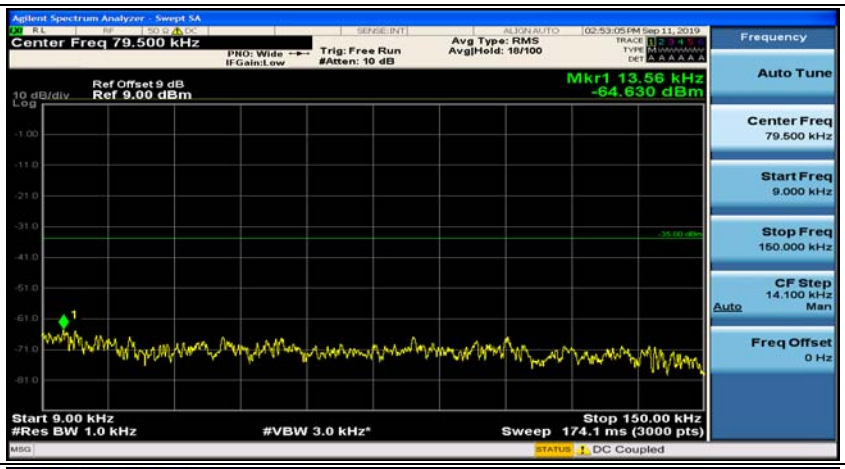
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:53:05 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 13.56 kHz
-64.630 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

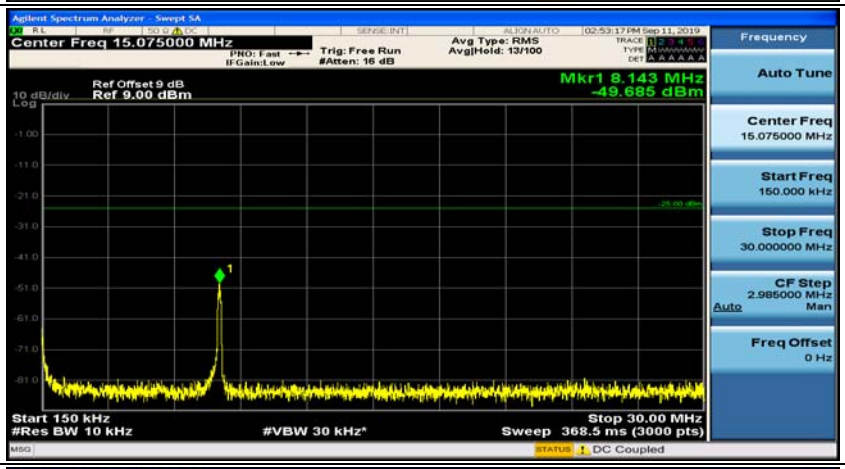
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:53:17 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 8.143 MHz
-49.685 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:53:22 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.883 GHz
-44.462 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 15 MHz

(Channel Bandwidth:15 MHz)_LCH_QPSK_1RB#0

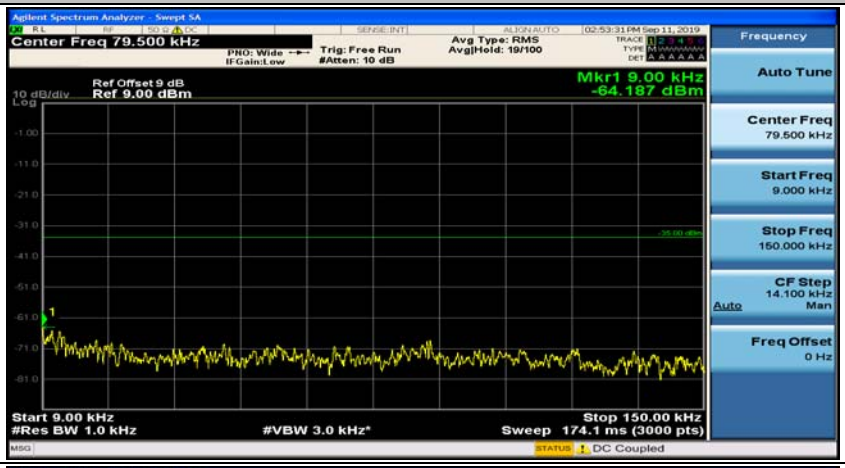

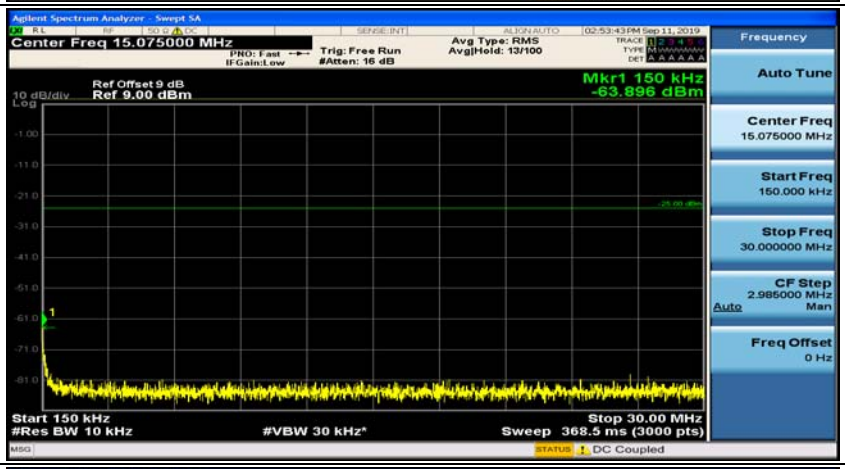

(Channel Bandwidth:15 MHz)_LCH_QPSK_1RB#37

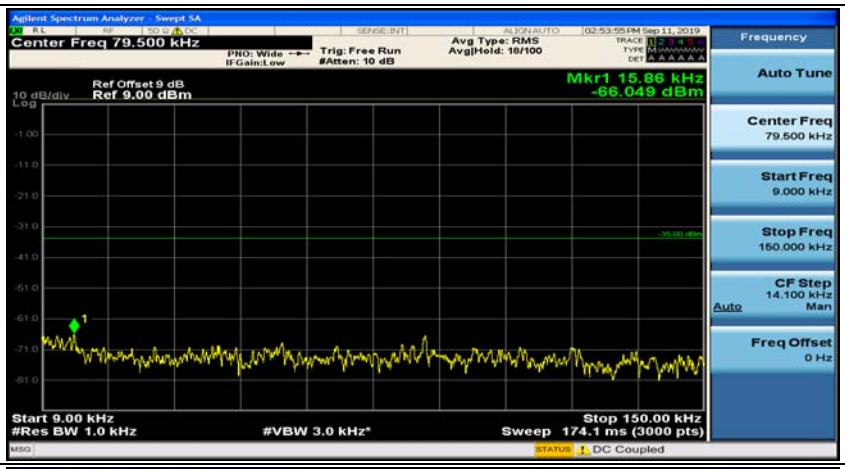

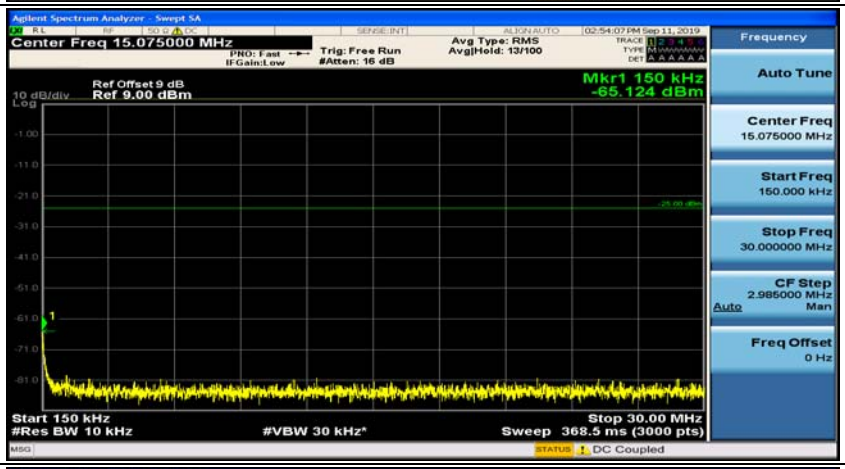

(Channel Bandwidth:15 MHz)_LCH_QPSK_1RB#74

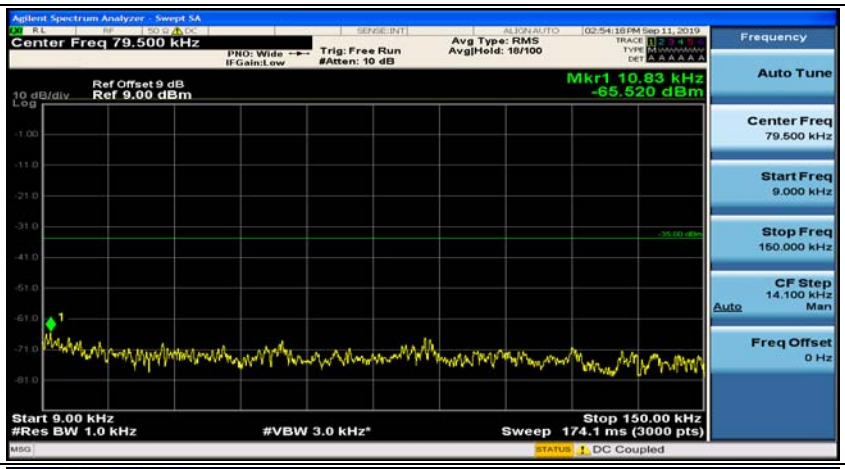
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:54:18 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 10.83 kHz
-65.520 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

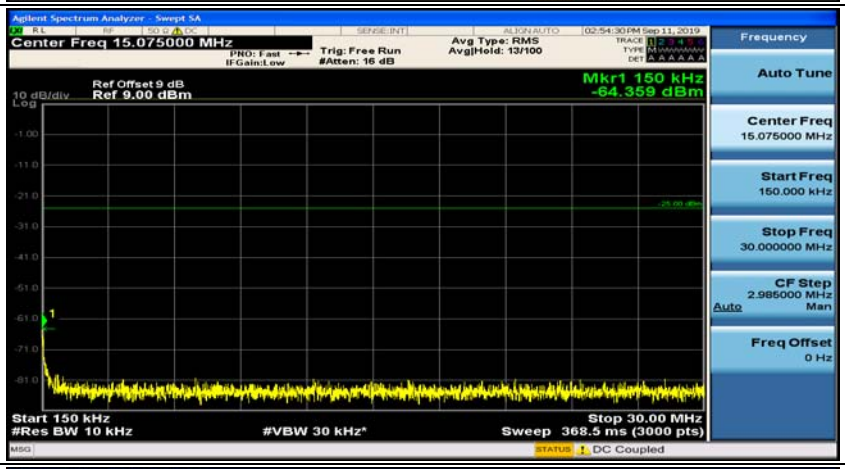
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:54:30 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-64.359 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:54:36 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.805 GHz
-44.818 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_MCH_QPSK_1RB#0
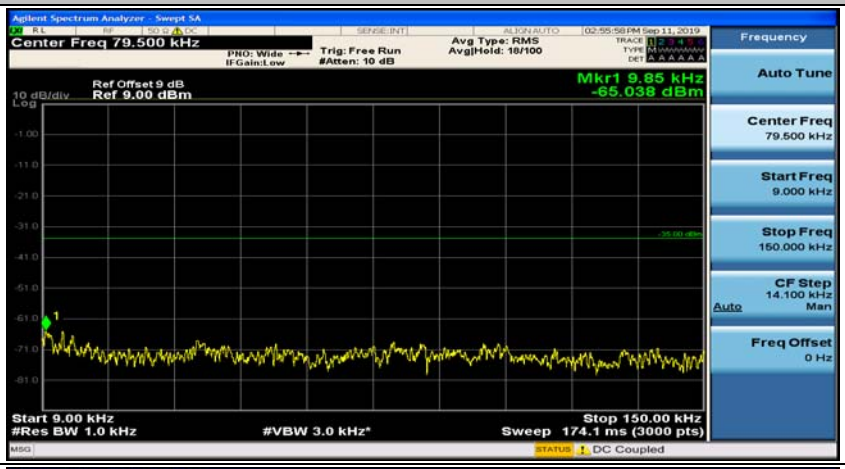
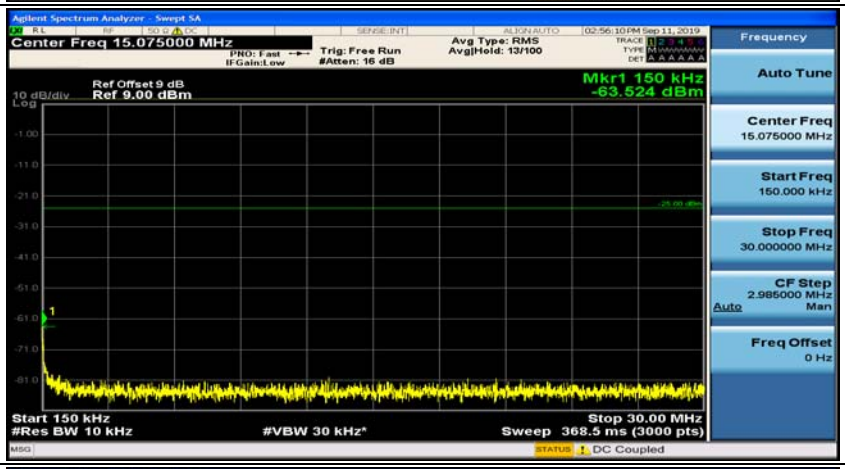
(Channel Bandwidth:15 MHz)_MCH_QPSK_1RB#37

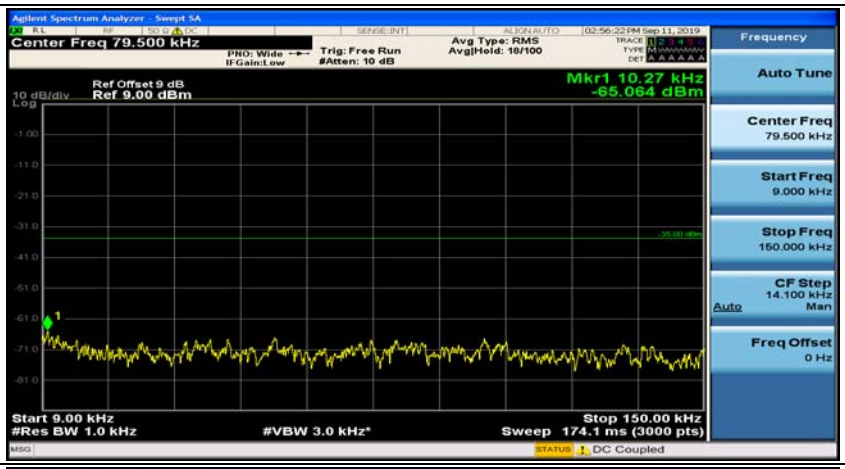

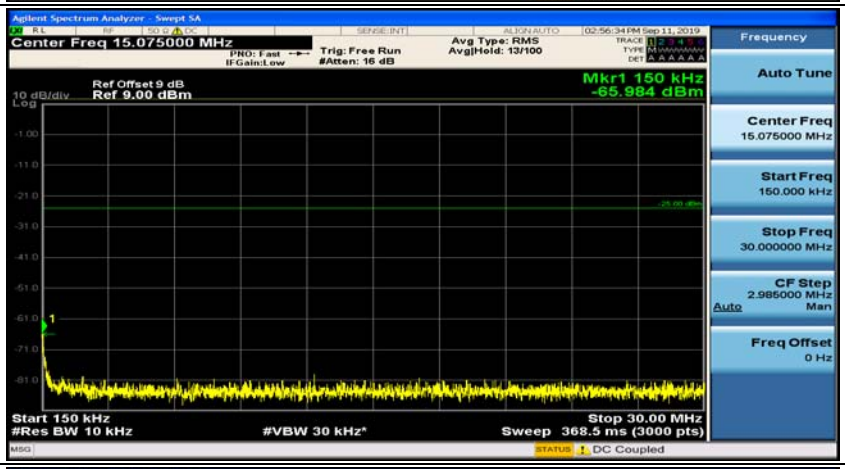

(Channel Bandwidth:15 MHz)_MCH_QPSK_1RB#74

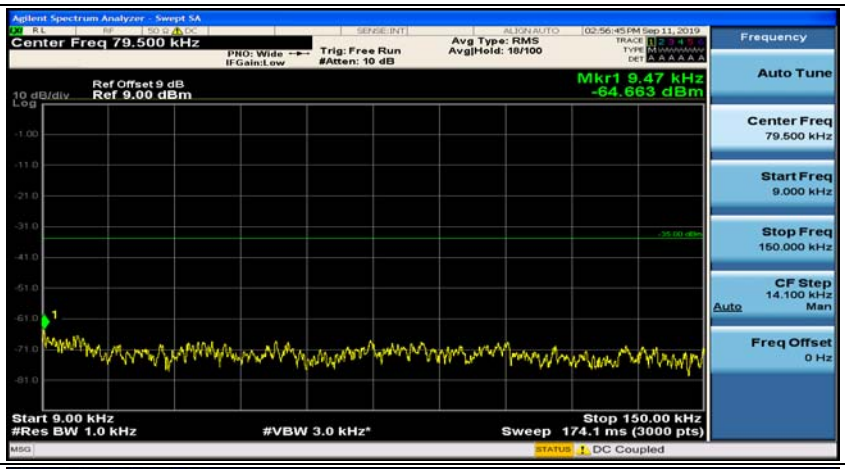
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:56:45 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.47 kHz
-64.663 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

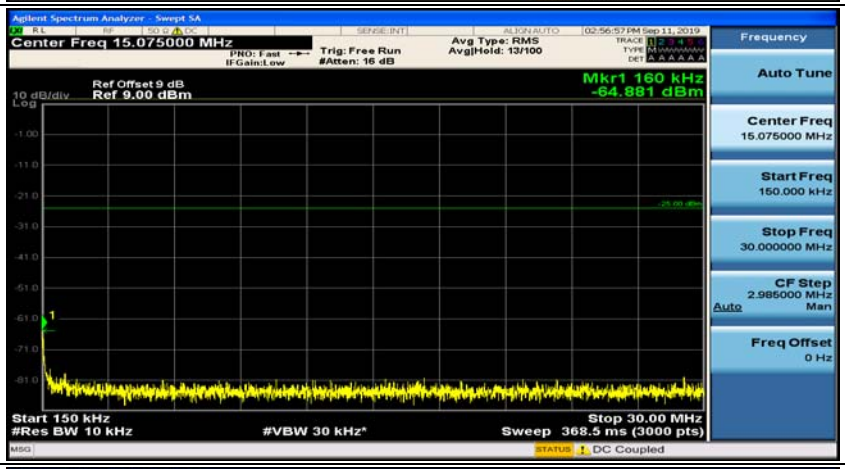
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:56:57 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 160 kHz
-64.881 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:57:03 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.805 GHz
-45.014 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#0

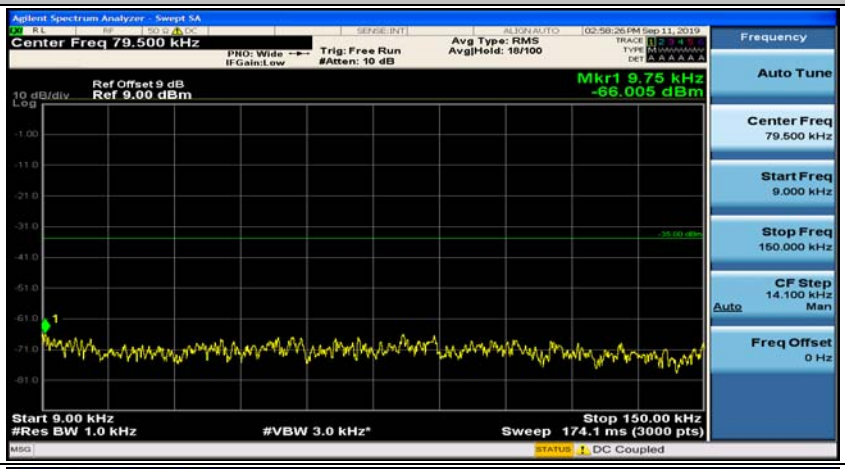

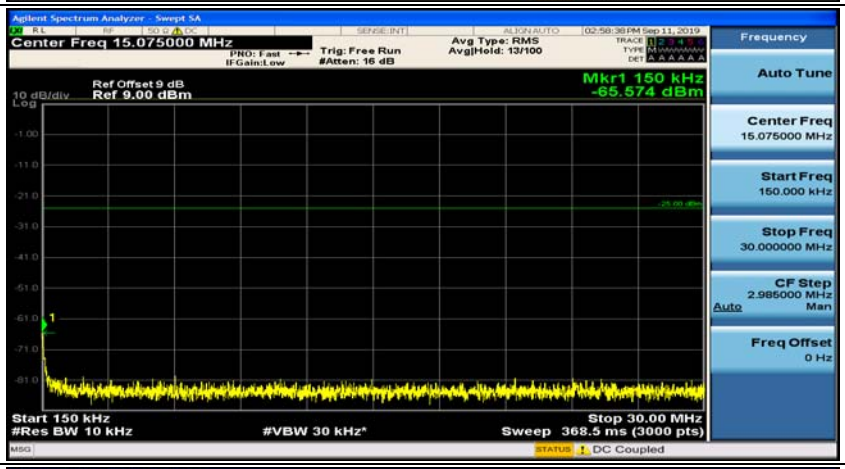

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#37

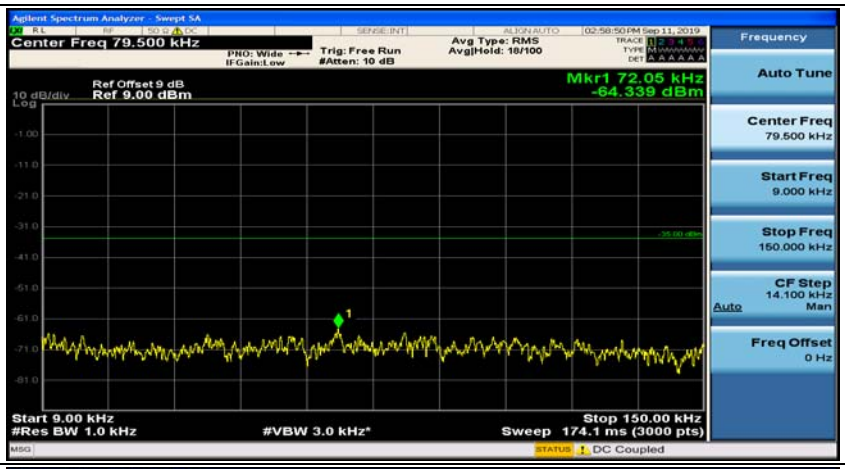

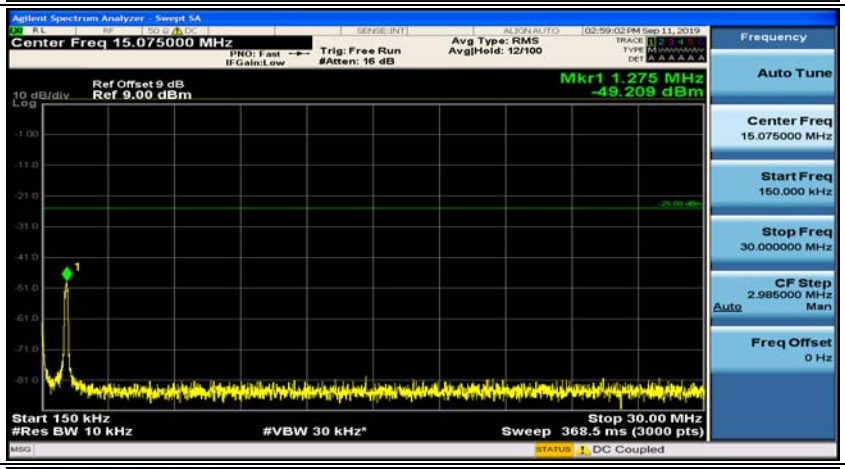

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#74

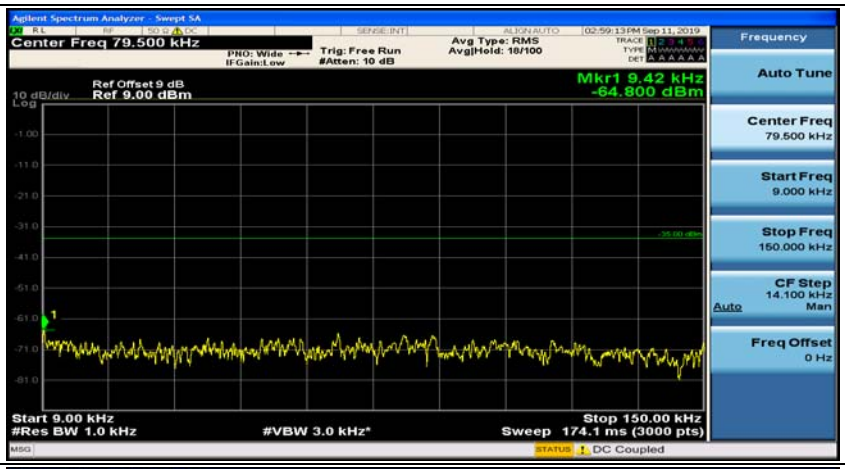
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:59:13 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.42 kHz
-64.800 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

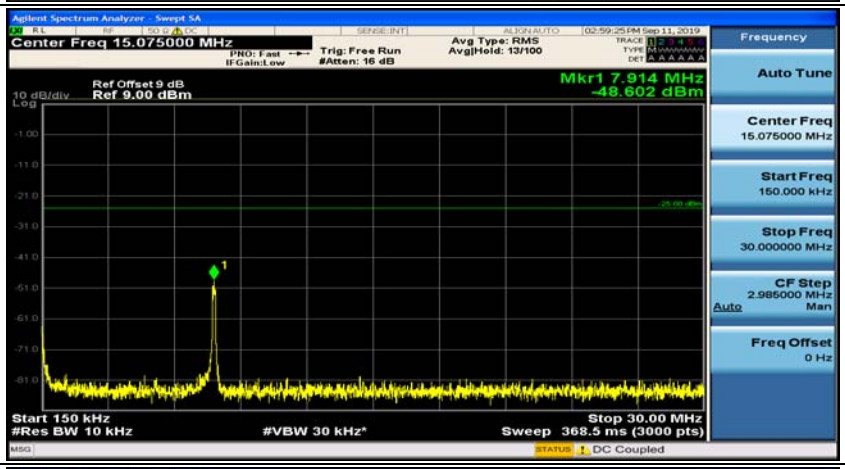
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:59:25 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 7.914 MHz
-48.602 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:59:31 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.840 GHz
-44.507 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#0

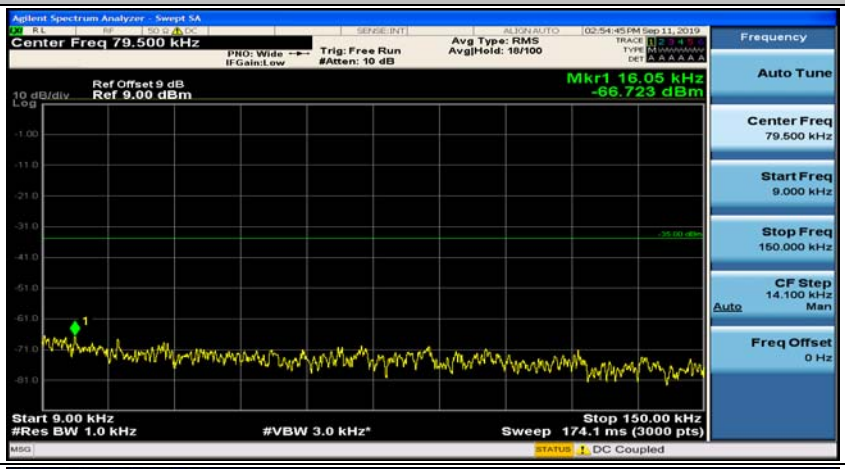

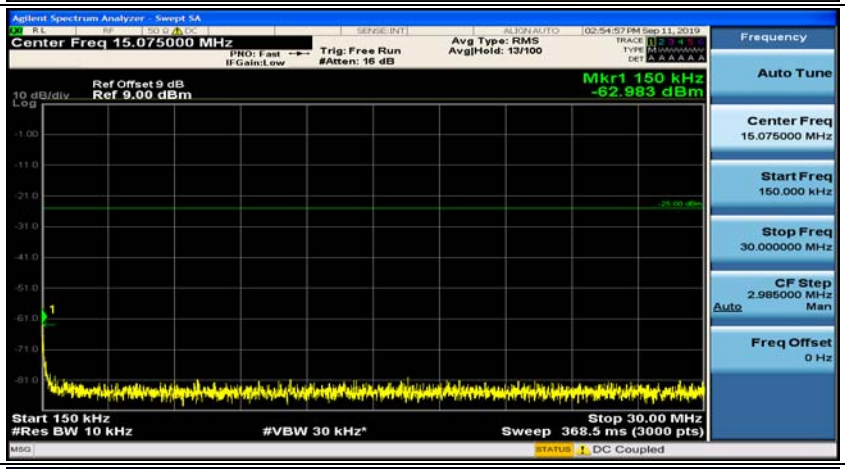

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#37

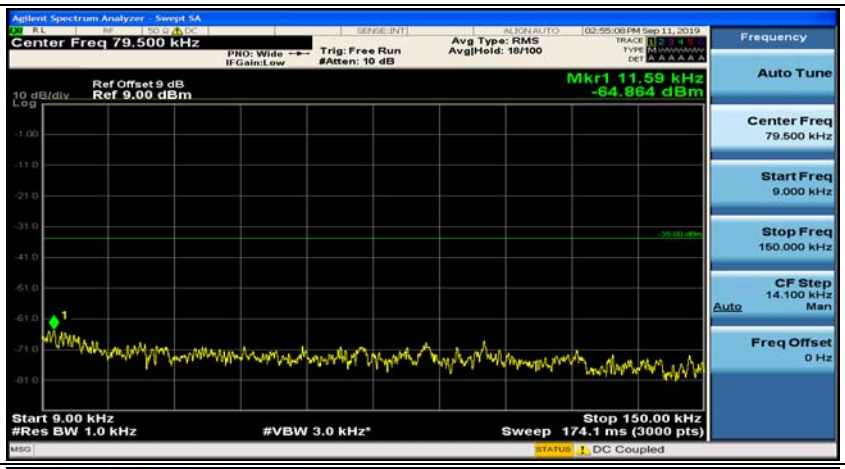

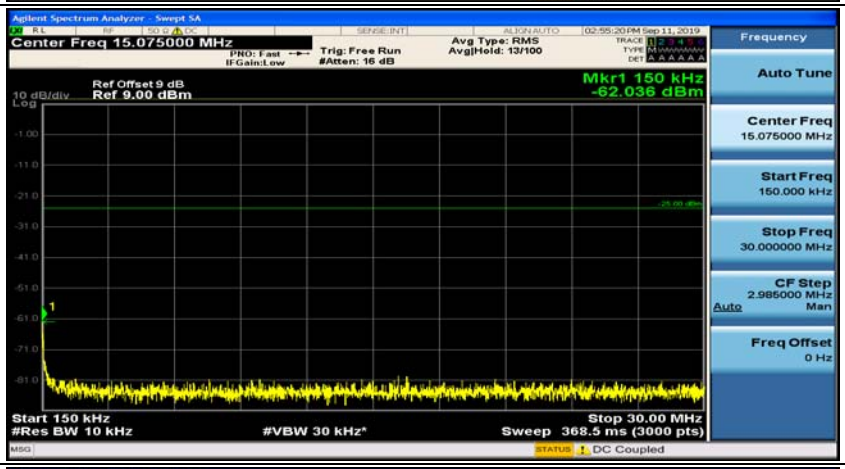

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#74

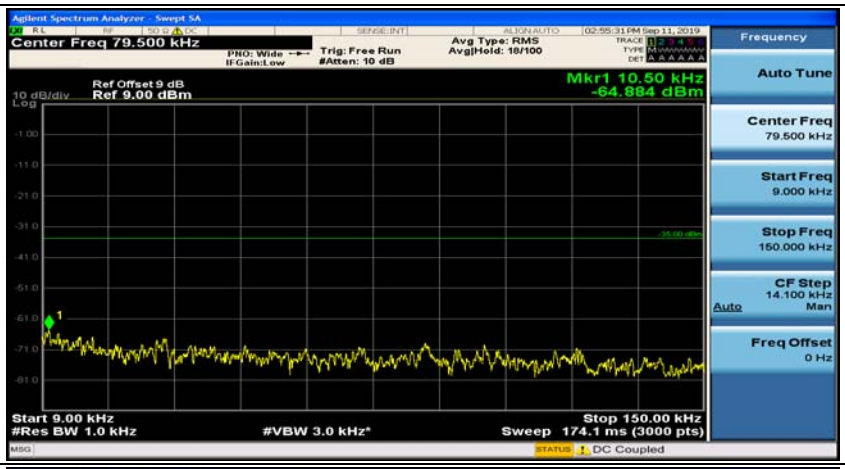
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:55:31 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 10.50 kHz
-64.884 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

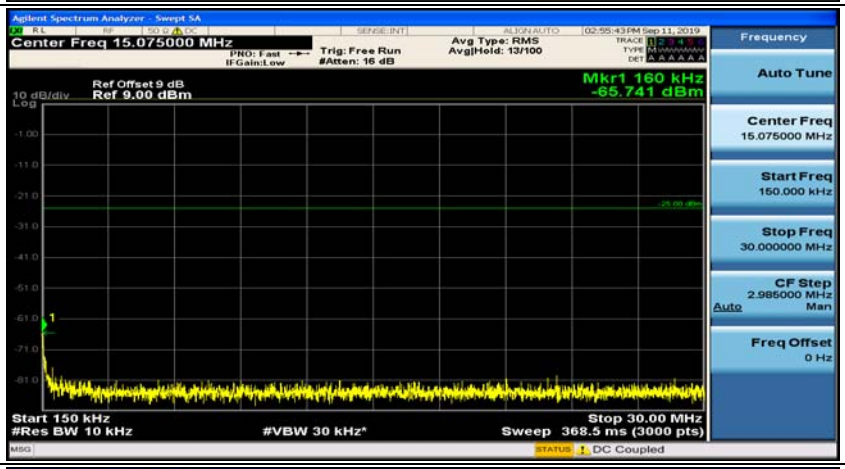
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:55:43 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 160 kHz
-65.741 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:55:49 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.857 GHz
-44.573 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#0

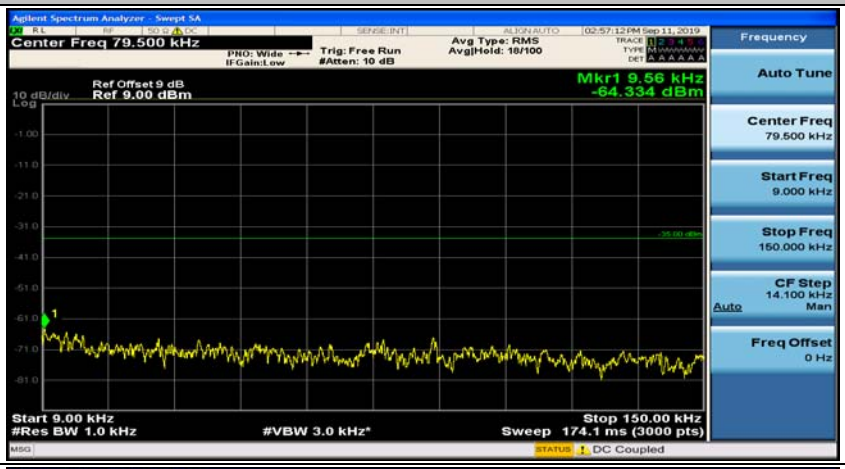

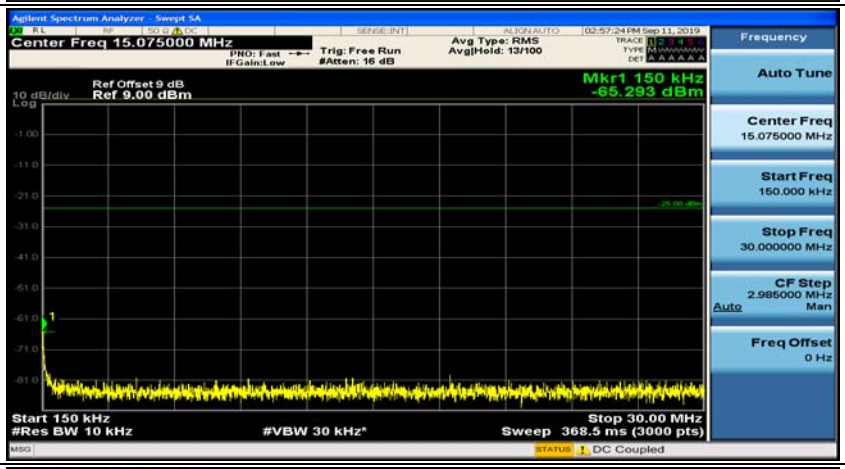

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#37

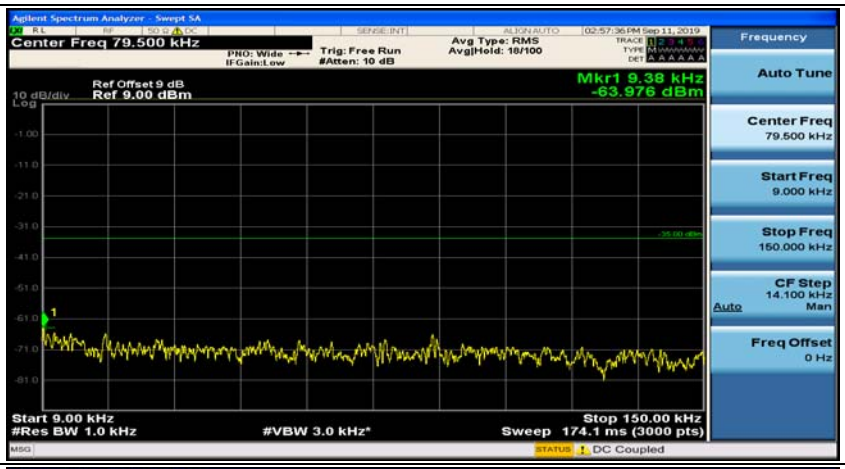

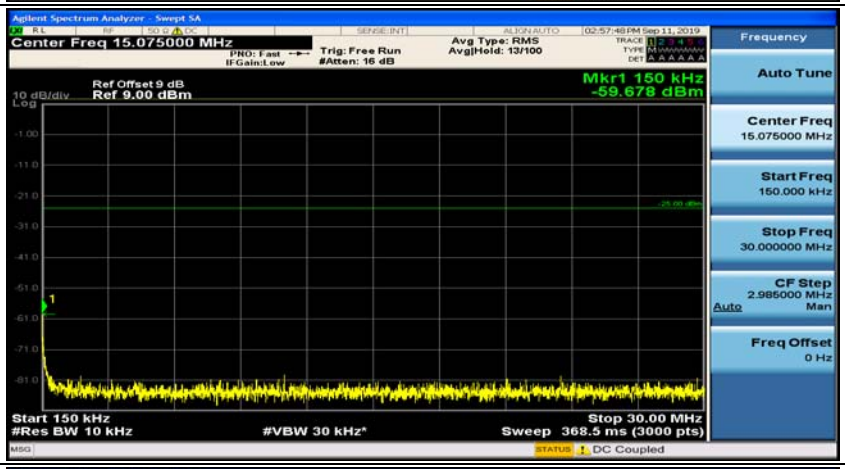

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#74

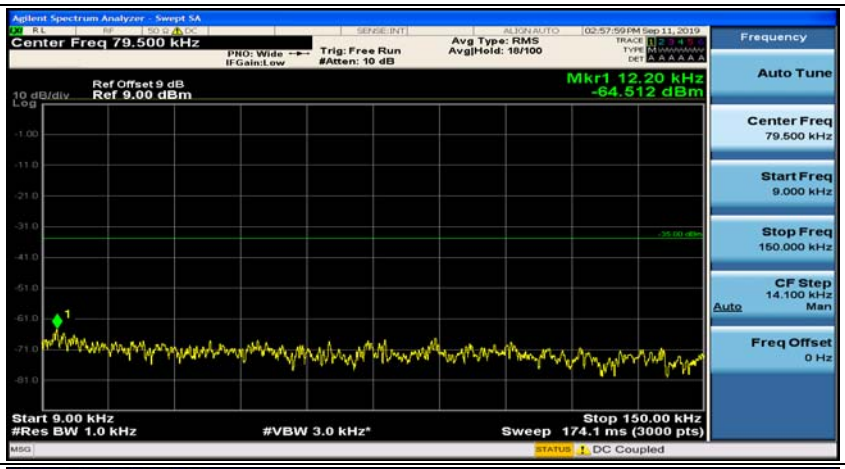
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
02:57:59 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 12.20 kHz
-64.512 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

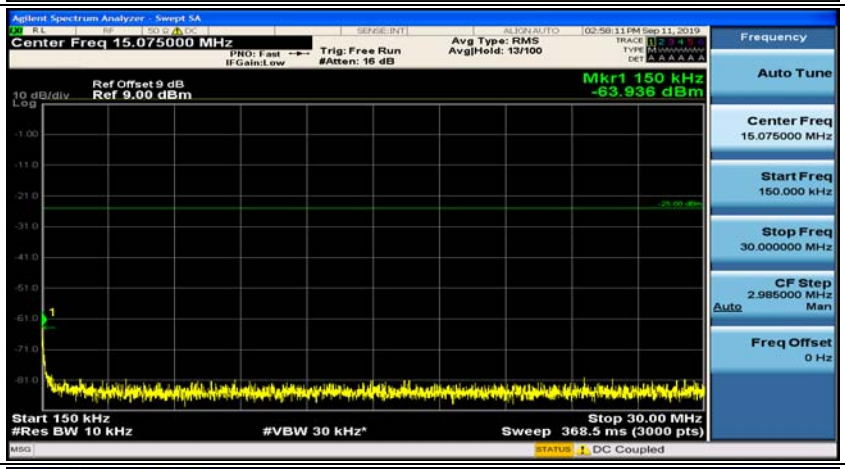
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
02:58:11 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-63.936 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
02:58:17 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.892 GHz
-44.251 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#0

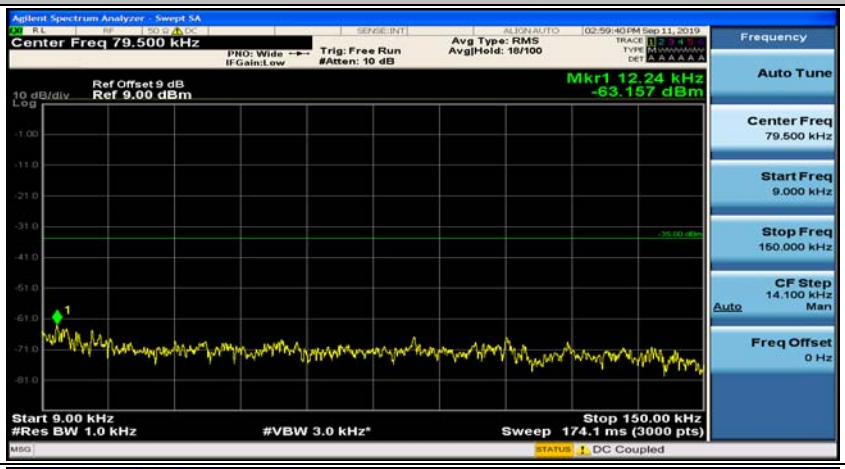

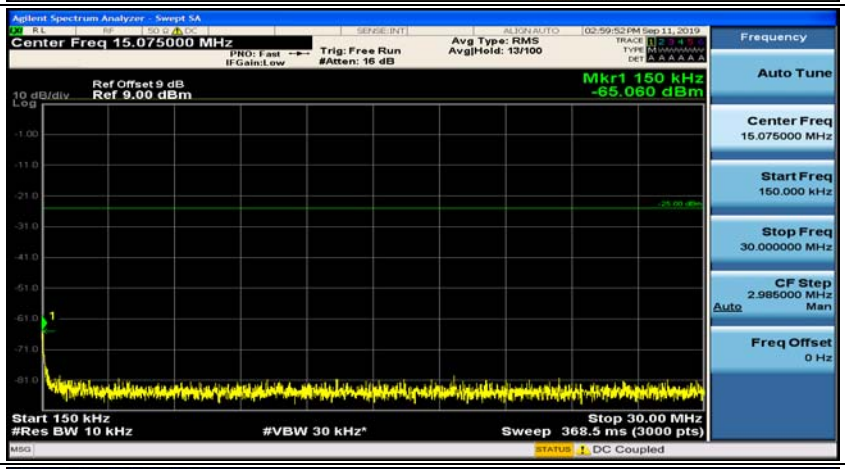

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#37

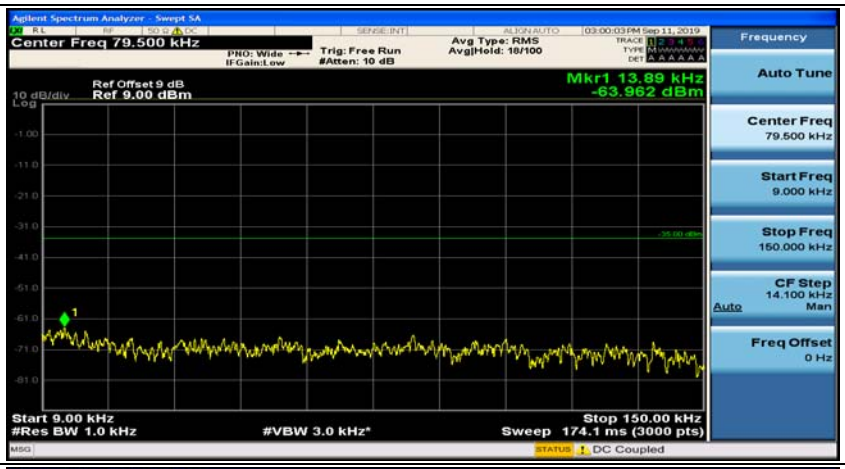

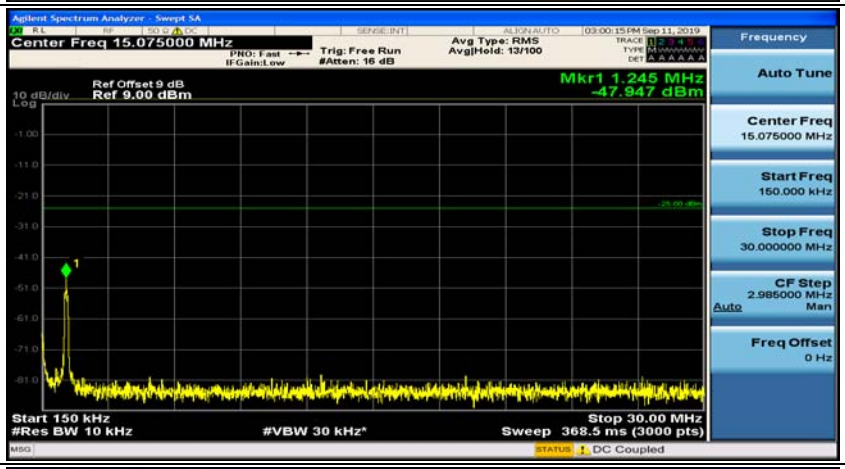

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#74

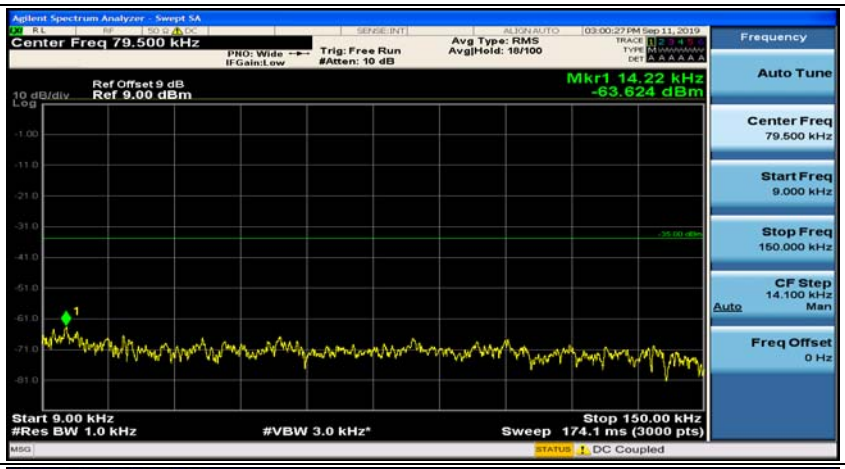
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
03:00:27 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 14.22 kHz
-63.624 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

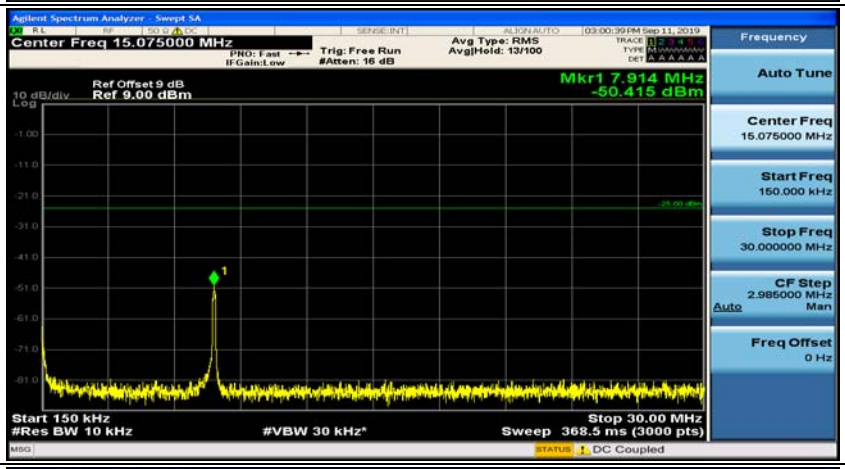
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
03:00:39 PM Sep 11, 2019
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 7.914 MHz
-50.415 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 20 dB
Avg Type: RMS
Avg|Hold: 17/100
03:00:44 PM Sep 11, 2019
Ref Offset 8.95 dB
10 dB/div Ref 18.95 dBm
Log
Mkr2 24.874 GHz
-44.329 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 20 MHz

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#0

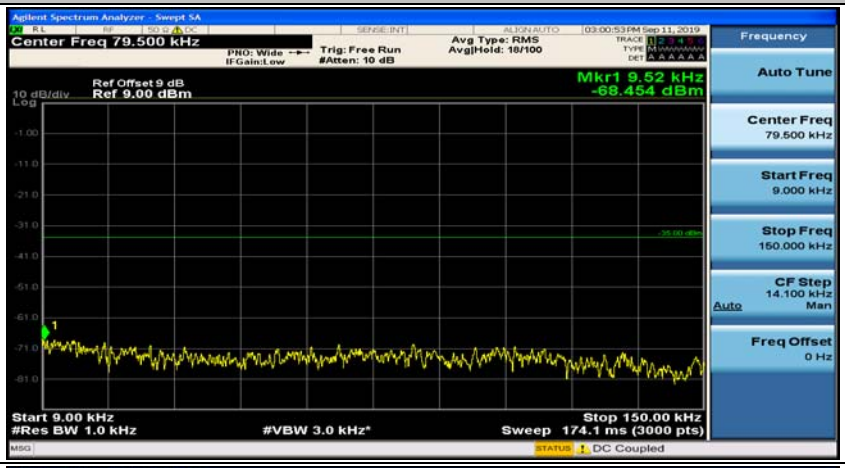

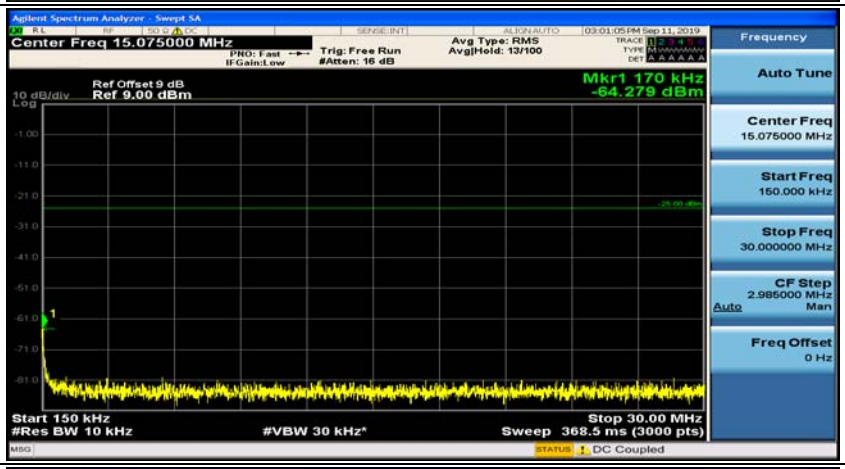

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#49

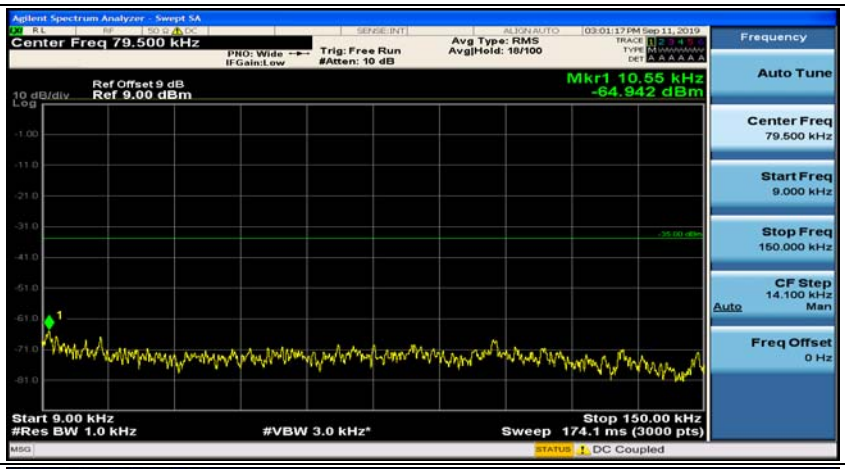

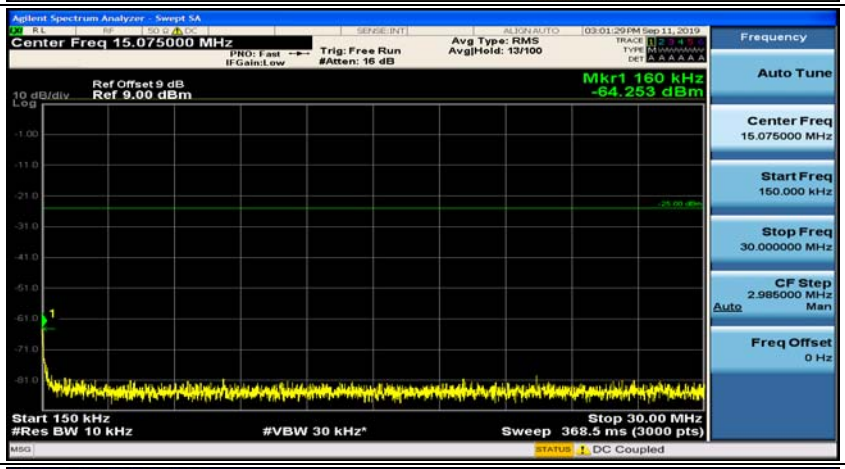

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#99