

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid (Head & Body)

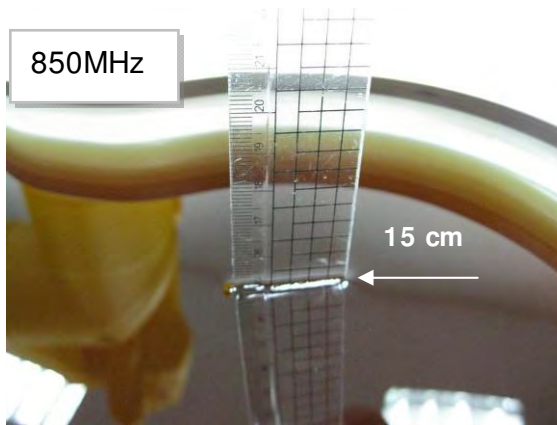


Fig.2.1

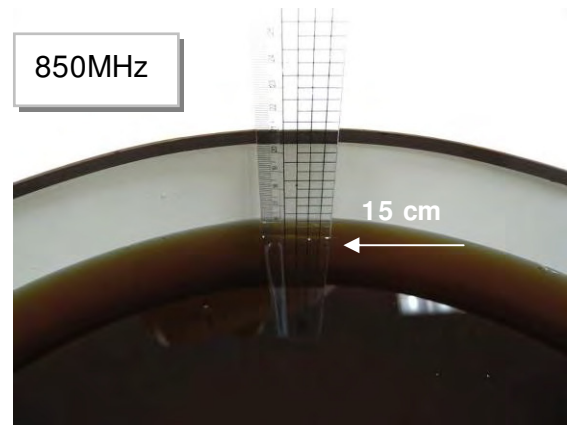


Fig.2.2

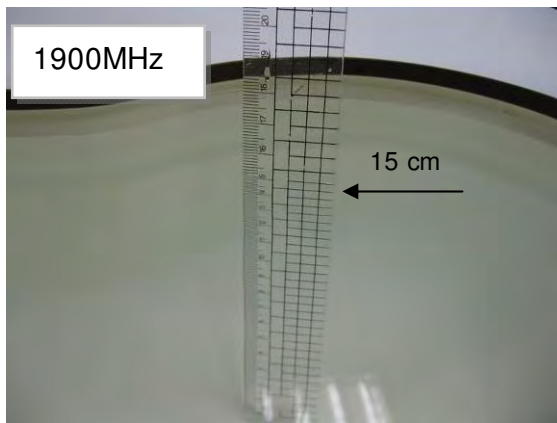


Fig.2.3

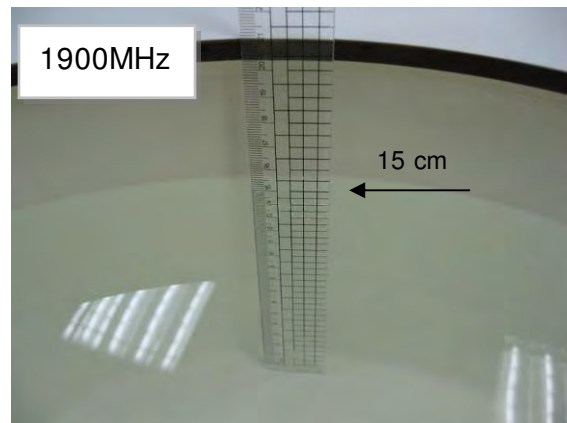


Fig.2.4

Head Mode

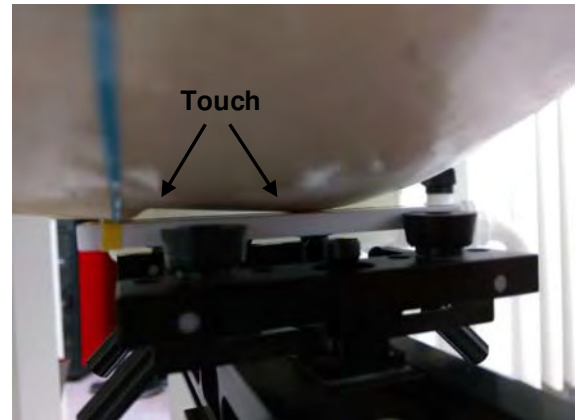
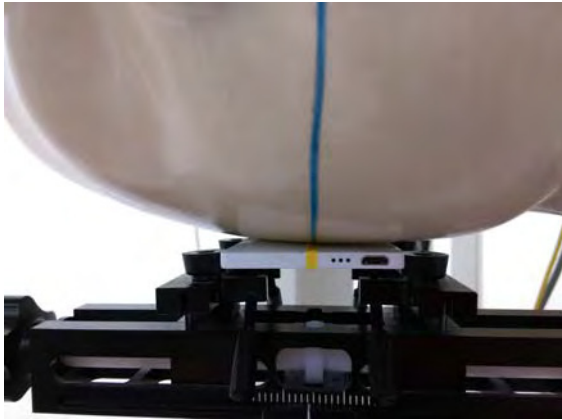


Fig.3 Right Head Section / Cheek-Touch Position

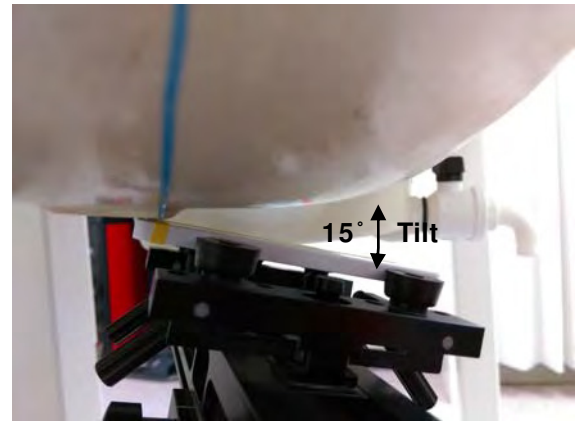
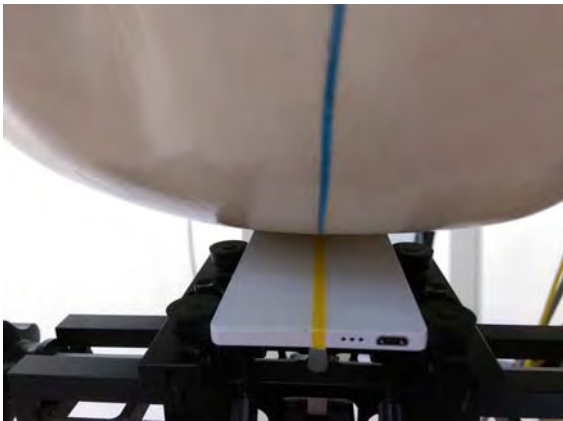


Fig.4 Right Head Section / Ear-Tilt Position(15°)

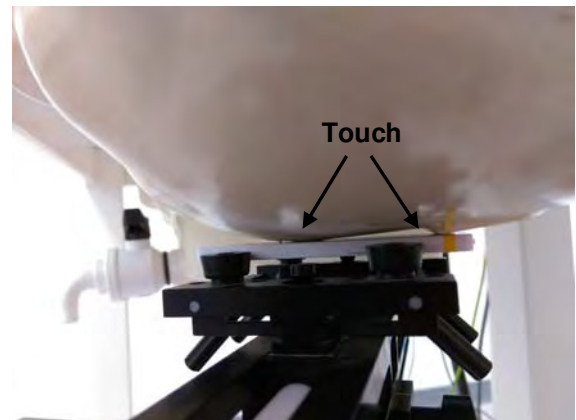
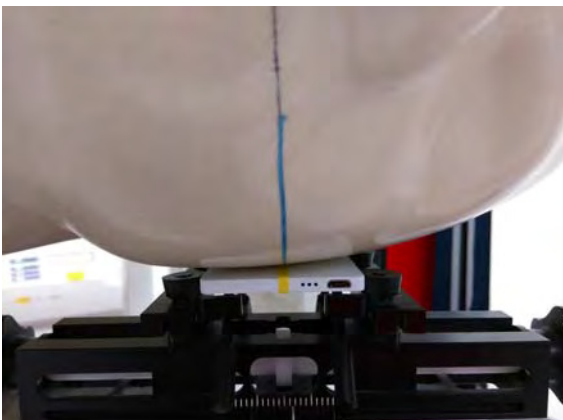


Fig.5 Left Head Section / Cheek-Touch Position

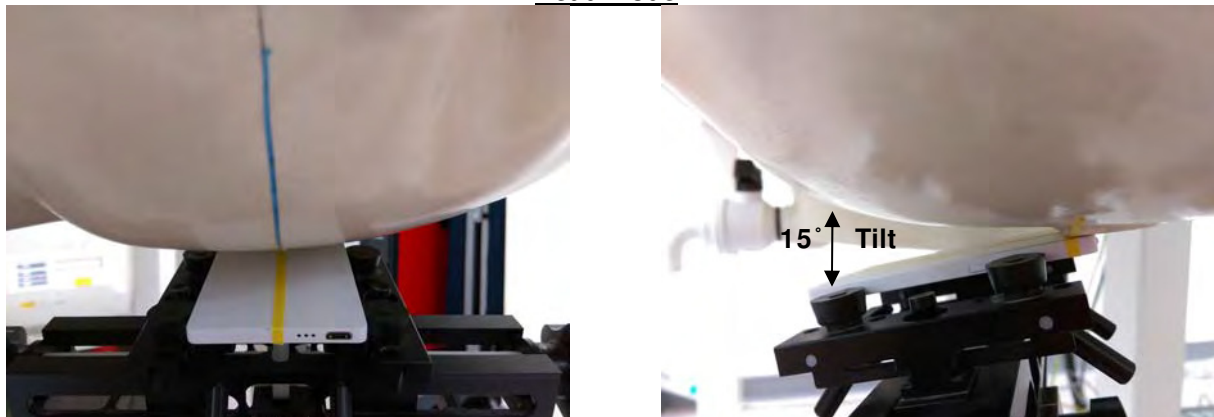
Head Mode

Fig.6 Left Head Section / Ear-Tilt Position(15°)

Body-worn - distance between flat phantom and mobile phone is 10 mm

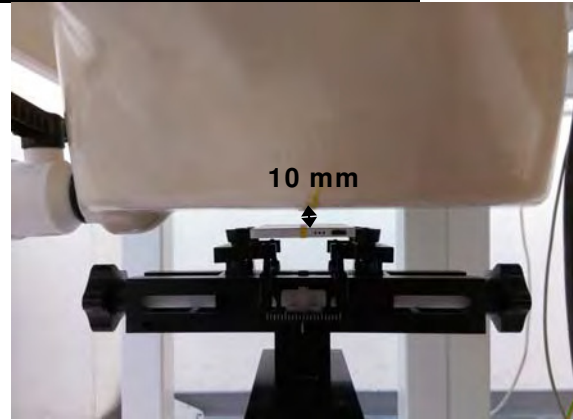


Fig.7 EUT Front side to flat phantom

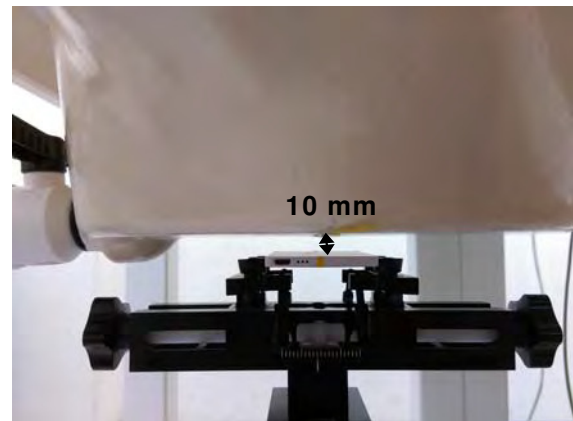


Fig.8 EUT Back side to flat phantom

12. Photographs of the EUT



Fig.9 Front view of EUT



Fig.10 Back view of EUT

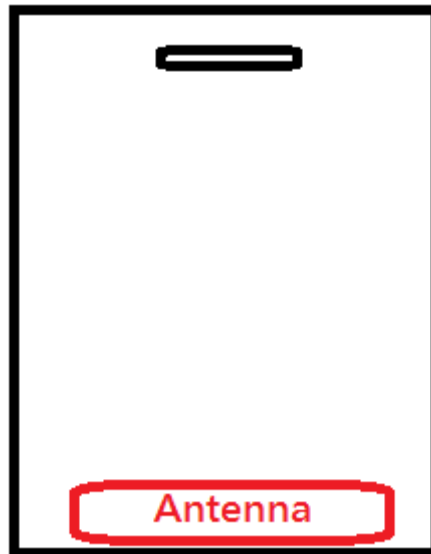


Fig.11 Antenna position of EUT

- End of Report -