



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **WSCT**  
**Shenzhen**

Certificate No. **V-Coil350/85-1035\_Nov24**

## CALIBRATION CERTIFICATE

Object **V-Coil350/85V2 - SN: 1035**

Calibration procedure(s) **QA CAL-47.v13**  
**Calibration Procedure for WPT Verification & Validation Sources**

Calibration date: **November 6, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards  | ID #          | Cal Date (Certificate No.)        | Scheduled Calibration |
|--------------------|---------------|-----------------------------------|-----------------------|
| MAGPy-8H3D+E3D/DAS | SN: 3090/3078 | 22-Aug-24 (MAGPy-8H3D-3090_Aug24) | Aug-25                |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---------------------|------|-----------------------|-----------------|
|---------------------|------|-----------------------|-----------------|

|                | Name        | Function       | Signature |
|----------------|-------------|----------------|-----------|
| Calibrated by: | Jingtian Xi | Project Leader |           |

|              |           |                   |  |
|--------------|-----------|-------------------|--|
| Approved by: | Sven Kühn | Technical Manager |  |
|--------------|-----------|-------------------|--|

Issued: November 13, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

### Glossary:

|     |                           |
|-----|---------------------------|
| WPT | wireless power transfer   |
| V&V | verification & validation |

### Calibration is Performed According to the Following Standards:

- Internal procedure QA CAL-47 Calibration procedure for WPT verification & validation sources from 3 kHz to 10 MHz
- IEC/IEEE 63164, "Assessment methods of the human exposure to electric and magnetic fields from wireless power transfer systems – Models, instrumentation, measurement and computational methods and procedures (Frequency range 3 kHz to 30 MHz)", draft standard, 2023

### Additional Documentation:

- a) cDASY6/DASY8 Module WPT Manual

### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* The V&V source is switched on for at least 30 minutes.
- *Source Positioning:* The V&V source is placed in the center of the UniPV1 phantom such that the source surface is parallel to phantom surface. The probe location used for DUT teaching is the top center of the coil (marked on the source casing). The probe distance is verified using mechanical gauges placed on the source surface.
- *H-field distribution:* H-field is measured in the volume above the V&V source in a rectilinear grid with a uniform grid step of 7.33 mm.

### Calibrated Quantity

- Spatial peak of H-field (RMS value) at  $d$  mm from the DUT surface (extrapolated from measurements)

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

|                   |                   |                                  |
|-------------------|-------------------|----------------------------------|
| Software version  | cDASY6 Module WPT | 2.6.0.5002                       |
|                   | Notebook GUI      | 2.6.0.9                          |
|                   | Sim4Life          | 8.0.1                            |
| Scan setup        | Grid dimensions   | x: 477 mm, y: 389 mm, z: 36.7 mm |
|                   | Grid resolutions  | dx, dy, dz: 7.33 mm              |
| Nominal frequency | 85 kHz            |                                  |

## Calibrated Quantities

| Distance (relative to source surface) (mm) | Peak H-field (A/m) | Uncertainty (k=2) (dB) |
|--------------------------------------------|--------------------|------------------------|
| 0                                          | 208                | 1.13                   |
| 2                                          | 189                | 1.13                   |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Peak values of induced fields<sup>1</sup>

| Distance<br>(relative to<br>source surface)<br>(mm) | Induced<br>peak current<br>density, 1cm <sup>2</sup> area<br>avg. (A/m <sup>2</sup> ) | Induced peak E-field (V/m) |       |                  | peak spatial SAR (mW/kg) |          |
|-----------------------------------------------------|---------------------------------------------------------------------------------------|----------------------------|-------|------------------|--------------------------|----------|
|                                                     |                                                                                       | 2mm cube<br>avg.           | Local | 5mm line<br>avg. | 1g avg.                  | 10g avg. |
| 0                                                   | 2.36                                                                                  | 3.36                       | 3.40  | 3.41             | 6.51                     | 4.82     |
| 2                                                   | 2.22                                                                                  | 3.16                       | 3.19  | 3.20             | 5.81                     | 4.36     |

### Voltage measurement

| Total voltage (V) | Voltages at harmonics (dBc)                                        |
|-------------------|--------------------------------------------------------------------|
| 0.407             | Highest harmonic: -41.1<br>2 <sup>nd</sup> highest harmonic: -48.2 |

<sup>1</sup> determined for a virtual half-space phantom with tissue properties  $\epsilon_r = 55$ ,  $\sigma = 0.75$  S/m,  $\rho = 1000$  kg/m<sup>3</sup> and a 2 mm thick phantom shell

Measurement report

cDASY6 Module WPT Measurement Report

Device under test

Info:  
V-Coil350/85

Serial number:  
1035

Scenario:  
source calibration

Tool info

DASY software version:  
cDASY6 Module WPT 2.6.0.5002

Probe model, serial no. and configuration date:  
MAGPy-8H3D+E3Dv2, WP000230, 2024/08/23

Software version:  
2.0.63, backend: 2.2.22

Scan info

Center location:  
x: -48.08 mm, y: -119.84 mm, z: 36.74 mm

Dimensions:  
x: 477.0 mm, y: 388.8 mm, z: 36.7 mm

Resolution:  
x: 7.33 mm, y: 7.33 mm, z: 7.33 mm

Completed on:  
2024/11/06 18:58:08

Measurement results


Maximum H-field [RMS]:  
MAGNITUDE: 135.93 A/m  
x: 118.90 A/m, y: 31.23 A/m, z: 57.99 A/m

Maximum H-field location relative to DUT:  
x: 157.67 mm, y: 25.67 mm, z: 8.50 mm


Distance to -20.0 dB boundary:  
62.66 mm

Offset relative to DUT:  
x: 0.00 m, y: 0.00 m, z: 1.00 mm

H-field magnitude [RMS] at maximum location

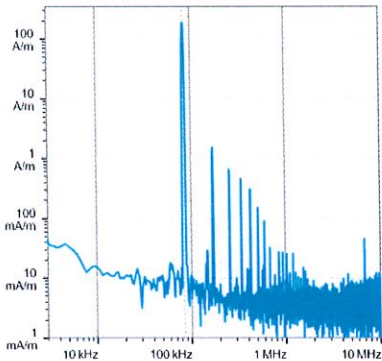

H-field magnitude [RMS] at lowest plane

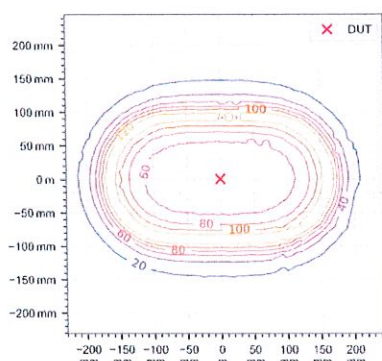

Incident fields and induced fields in the homogeneous phantom at the peak frequency (f = 85.00 kHz,  $\sigma = 0.750\text{ S/m}$ , tissue density =  $1,000\text{ kg/m}^3$ )

| Distance [mm] | Peak incident fields [RMS] | Peak $E_{ind}$ [V/m, RMS] |       |           | Peak $J_{ind}$ [A/m <sup>2</sup> , RMS] | psSAR [mW/kg] |          | H-field extent     | Warnings |                  |                 |
|---------------|----------------------------|---------------------------|-------|-----------|-----------------------------------------|---------------|----------|--------------------|----------|------------------|-----------------|
|               | $H_{inc}$ [A/m]            | Cube avg.                 | Local | Line avg. | Surface avg.                            | 1g avg.       | 10g avg. | -20 dB radius [mm] | Sign     | Vector potential | Boundary effect |
| 0.00          | 208                        | 3.36                      | 3.40  | 3.41      | 2.36                                    | 6.51          | 4.82     | 181                | 1%       | 90%              | 36%             |
| 2.00          | 189                        | 3.16                      | 3.19  | 3.20      | 2.22                                    | 5.81          | 4.36     | 183                | 1%       | 90%              | 38%             |

Compliance evaluation (Field values at the peak frequency) (f=85.00 kHz, )

| Distance [mm] | ICNIRP 2010/2020 |                  |               | ICNIRP 1998      |                                |               | IEEE 2019        |                  |               | FCC              |                  |               | HC Code 6        |                  |               |
|---------------|------------------|------------------|---------------|------------------|--------------------------------|---------------|------------------|------------------|---------------|------------------|------------------|---------------|------------------|------------------|---------------|
|               | RL [RMS]         | BR [RMS]         |               | RL [RMS]         | BR [RMS]                       |               | ERL [RMS]        | DRL [RMS]        |               | MPE [RMS]        | BR [RMS]         |               | RL [RMS]         | BR [RMS]         |               |
|               | $pH_{inc}$ [A/m] | $pE_{ind}$ [V/m] | psSAR [mW/kg] | $pH_{inc}$ [A/m] | $pJ_{ind}$ [A/m <sup>2</sup> ] | psSAR [mW/kg] | $pH_{inc}$ [A/m] | $pE_{ind}$ [V/m] | psSAR [mW/kg] | $pH_{inc}$ [A/m] | $pE_{ind}$ [V/m] | psSAR [mW/kg] | $pH_{inc}$ [A/m] | $pE_{ind}$ [V/m] | psSAR [mW/kg] |
| 0.00          | 208              | 3.36             | 4.82          | 208              | 2.36                           | 4.82          | 208              | 3.41             | 4.82          | 208              | N/A              | 6.51          | 208              | 3.40             | 6.51          |
| 2.00          | 189              | 3.16             | 4.36          | 189              | 2.22                           | 4.36          | 189              | 3.20             | 4.36          | 189              | N/A              | 5.81          | 189              | 3.19             | 5.81          |

Compliance evaluation (Exposure ratios) (ratios in dB)

| Distance [mm] | ICNIRP 2010/2020 |            |       | ICNIRP 1998 |            |       | IEEE 2019  |            |       | FCC        |            |       | HC Code 6  |            |       |
|---------------|------------------|------------|-------|-------------|------------|-------|------------|------------|-------|------------|------------|-------|------------|------------|-------|
|               | RL               | BR         |       | RL          | BR         |       | ERL        | DRL        |       | MPE        | BR         |       | RL         | BR         |       |
|               | $pH_{inc}$       | $pE_{ind}$ | psSAR | $pH_{inc}$  | $pJ_{ind}$ | psSAR | $pH_{inc}$ | $pE_{ind}$ | psSAR | $pH_{inc}$ | $pE_{ind}$ | psSAR | $pH_{inc}$ | $pE_{ind}$ | psSAR |
| 0.00          | NS               | TH         | NS    | N/A         | NS         | TH    | NS         | TH         | NS    | N/A        | N/A        | TH    | NS         | TH         | NS    |
| 0.00          | 19.9             | N/A        | -10.7 | N/A         | 32.4       | 22.9  | N/A        | 2.1        | N/A   | -14.4      | N/A        | 7.26  | N/A        | -10.6      | N/A   |
| 2.00          | 19.1             | N/A        | -11.2 | N/A         | 31.6       | 22.3  | N/A        | 1.3        | N/A   | -14.9      | N/A        | 6.46  | N/A        | -11.1      | N/A   |