

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260320 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.31$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(7.25, 7.53, 7.69); Calibrated: 2026-02-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156-0; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.1 W/kg; SAR (10g) = 5.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 9.15 W/kg; SAR (8g) = 5.56 W/kg; SAR (10g) = 5.17 W/kg

Smallest distance from peaks to all points 3 dB below = 10.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.5 %

TSL Correction: Positive only

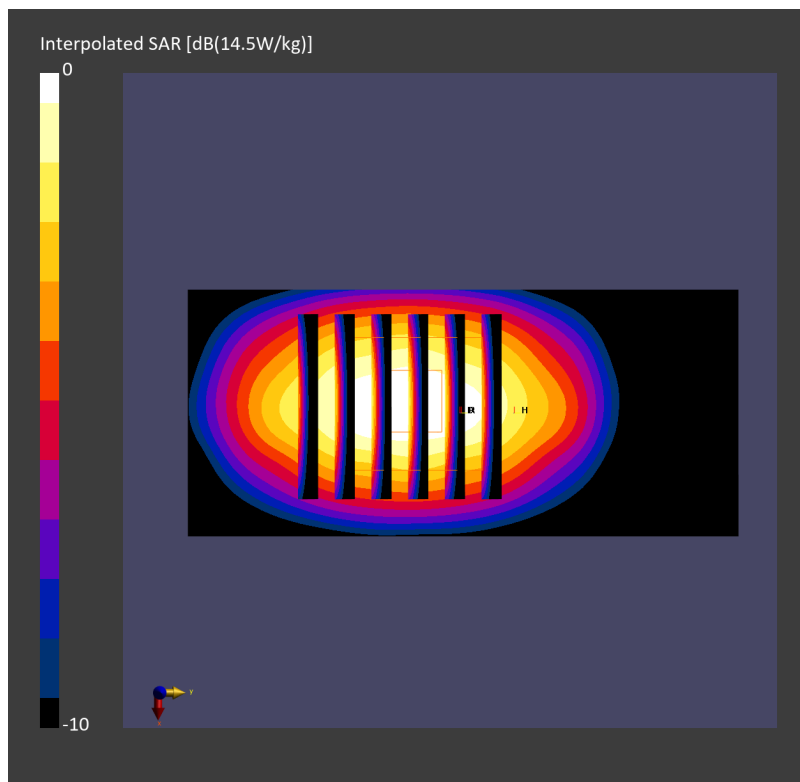

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260320 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(6.54, 6.8, 6.94); Calibrated: 2026-02-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156-0; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.1 W/kg; SAR (10g) = 7.18 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 14.1 W/kg; SAR (8g) = 7.44 W/kg; SAR (10g) = 6.76 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

TSL Correction: Positive only

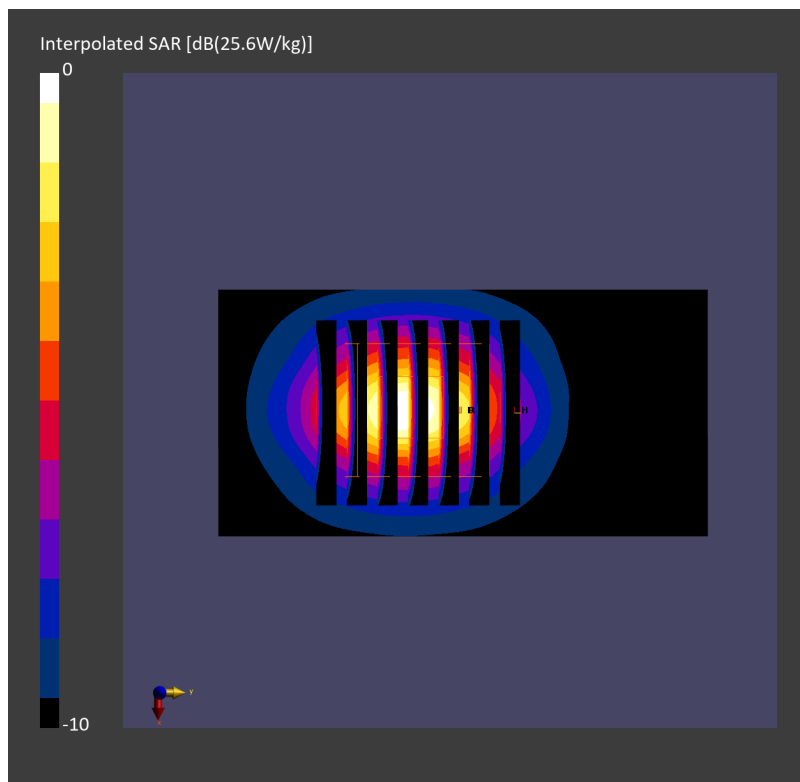

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.32 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.45 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

TSL Correction: Positive only

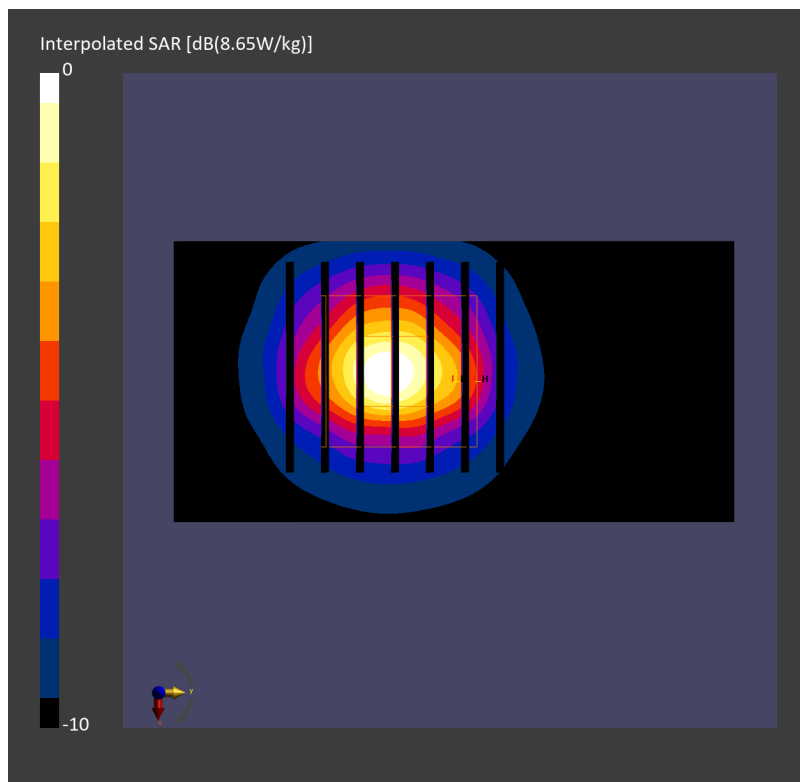

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.80$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.58, 6.79, 6.57); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.13 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

TSL Correction: Positive only

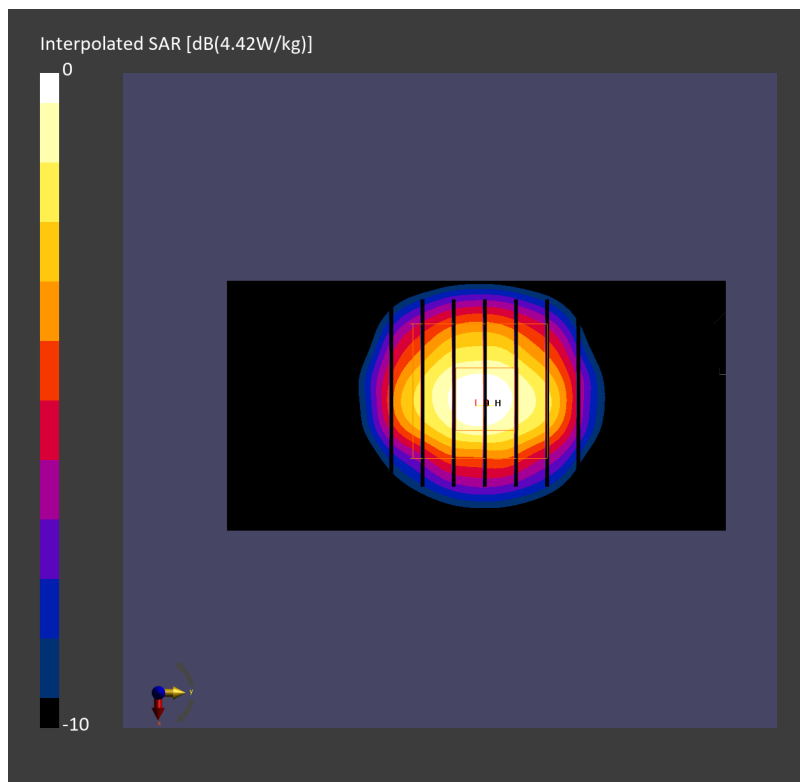

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.58, 6.79, 6.57); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.05 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

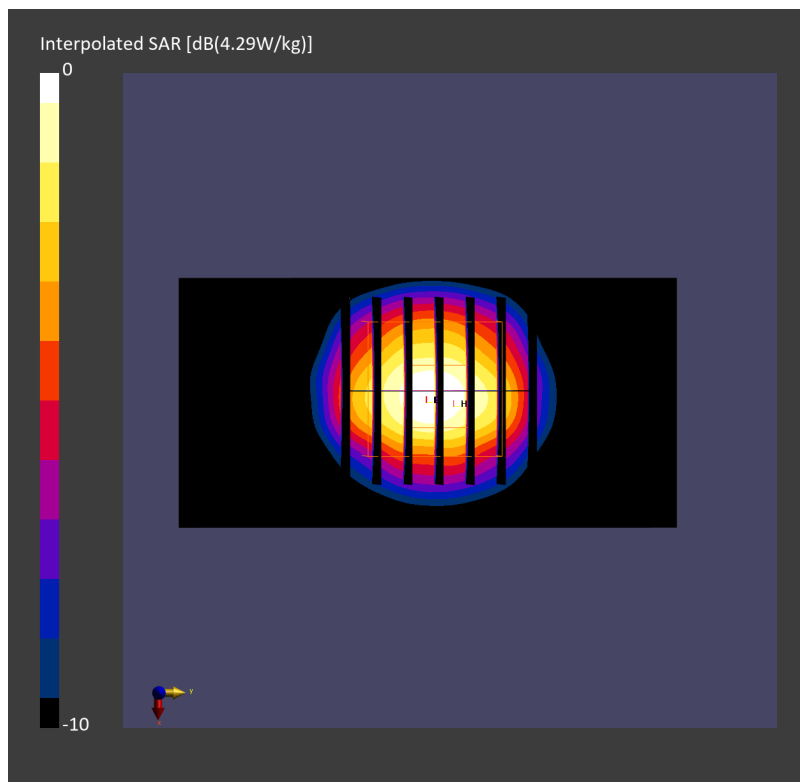

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.43 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 74.6 %

TSL Correction: Positive only

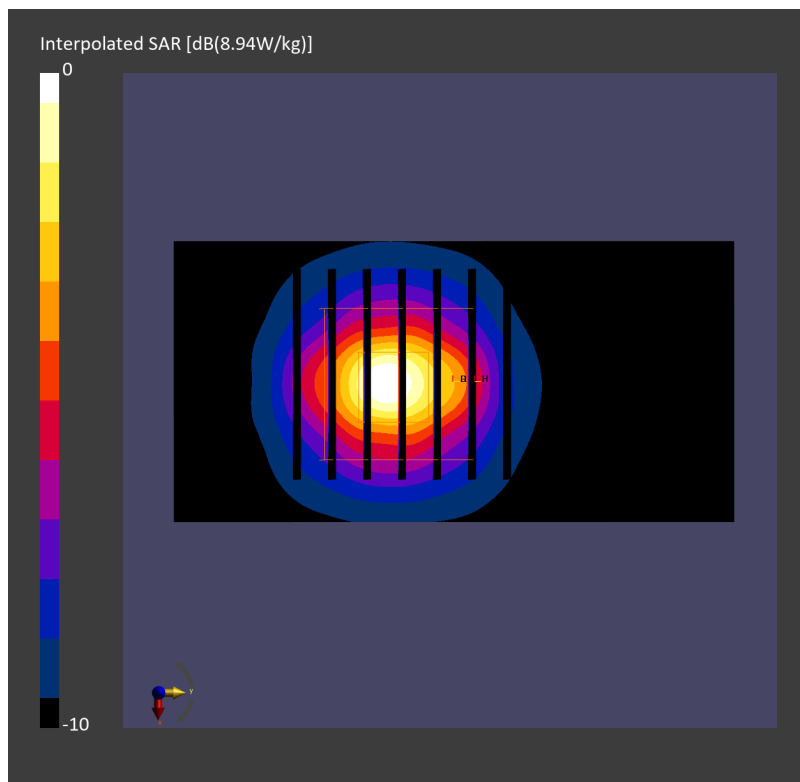

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.72, 6.5); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.61 W/kg; SAR (10g) = 1.28 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.70 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 71.9 %

TSL Correction: Positive only

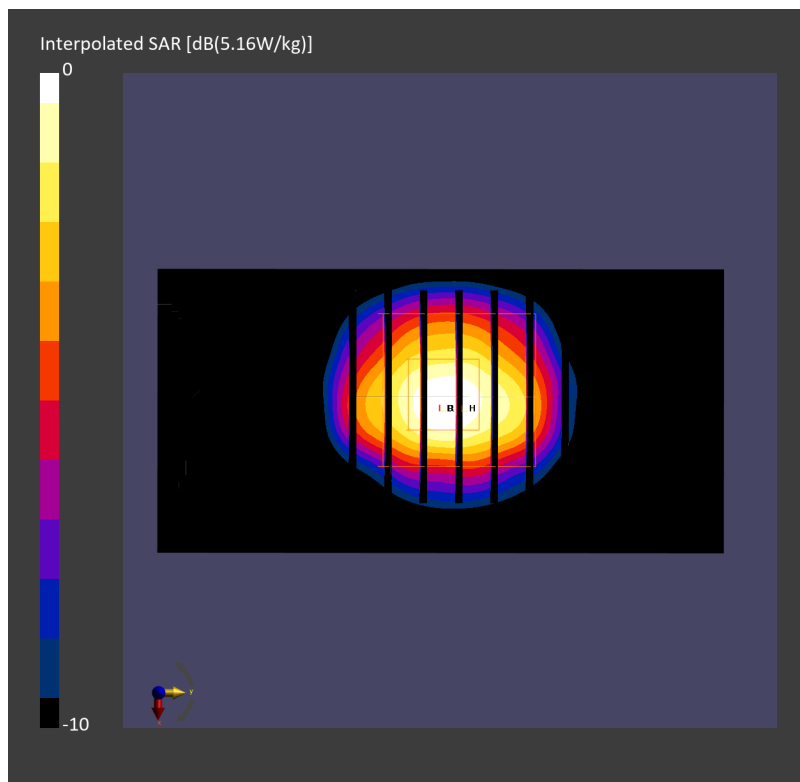

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.72, 6.5); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.47 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.53 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 72.1 %

TSL Correction: Positive only

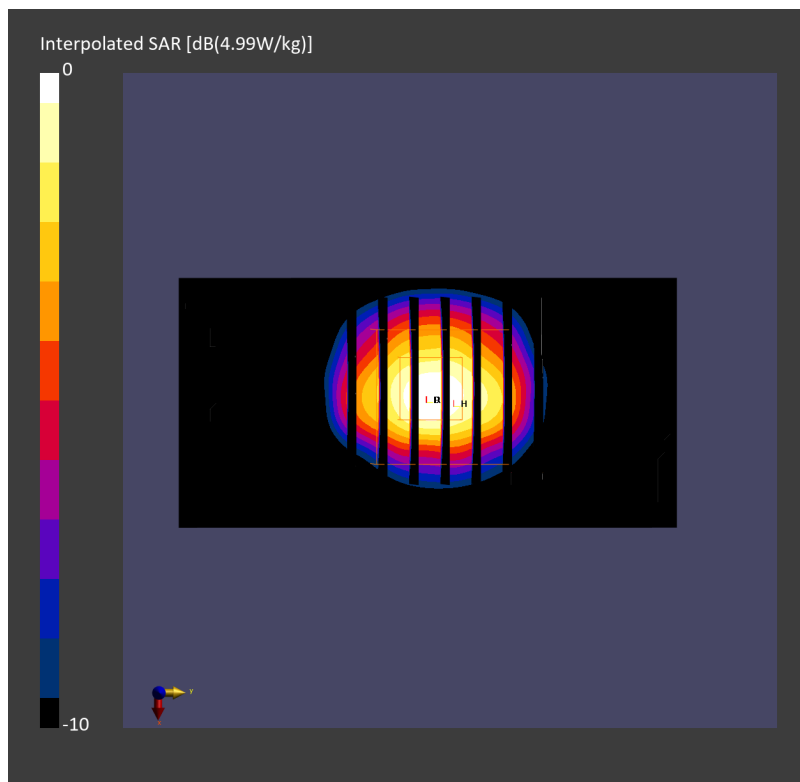

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.02 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.19 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 72.9 %

TSL Correction: Positive only

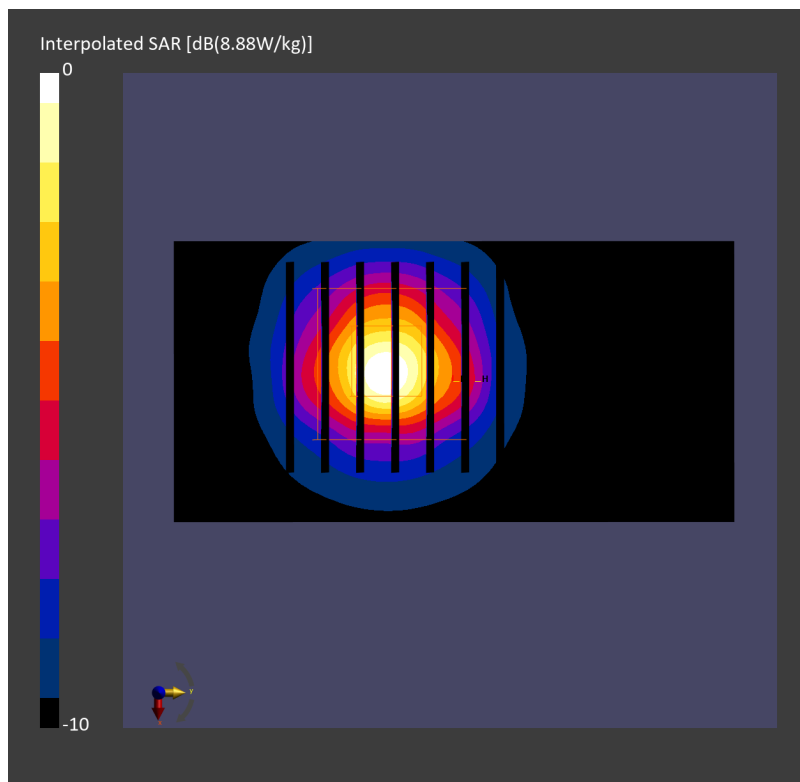

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.20$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.45, 6.66, 6.44); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (40.0 mm x 40.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.0 mm

Ratio of SAR at M2 to SAR at M1 = 71.2 %

TSL Correction: Positive only

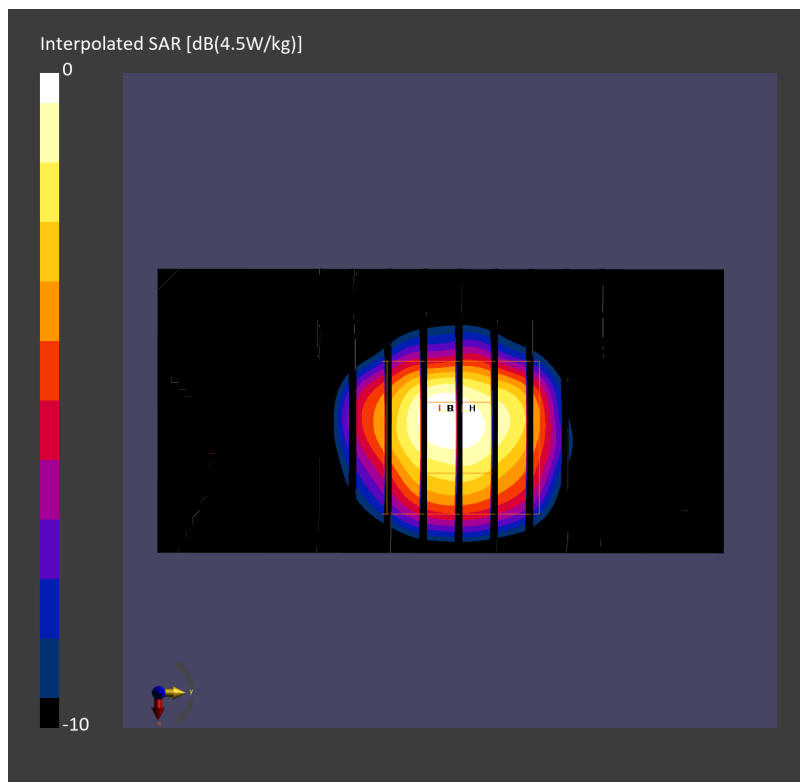

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.05$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.45, 6.66, 6.44); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 71.8 %

TSL Correction: Positive only

