

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260602 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.08, 7.83, 7.89); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.93 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

TSL Correction: Positive only

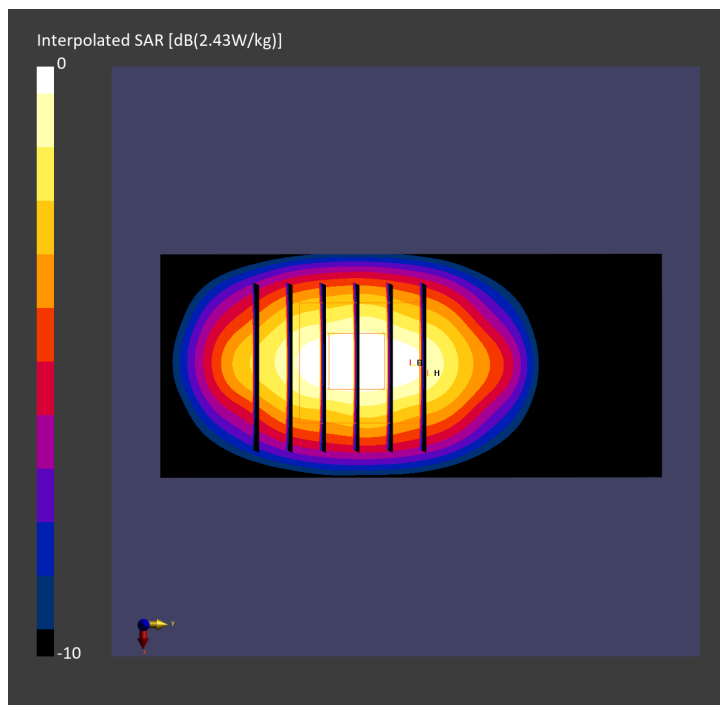

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260603 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.57 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.9 %

TSL Correction: Positive only

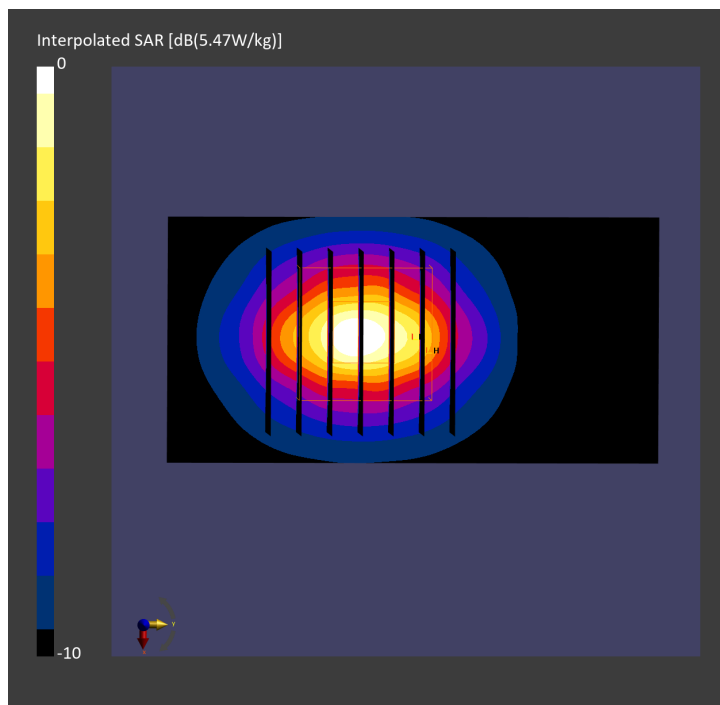

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260604 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.70$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.39 W/kg; SAR (10g) = 1.28 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.34 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

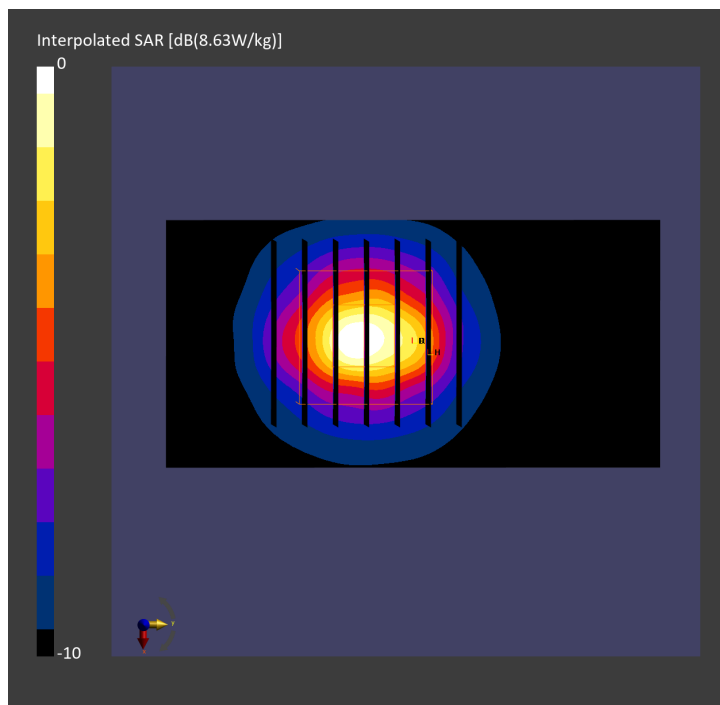

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.78$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.40 W/kg; SAR (10g) = 1.29 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

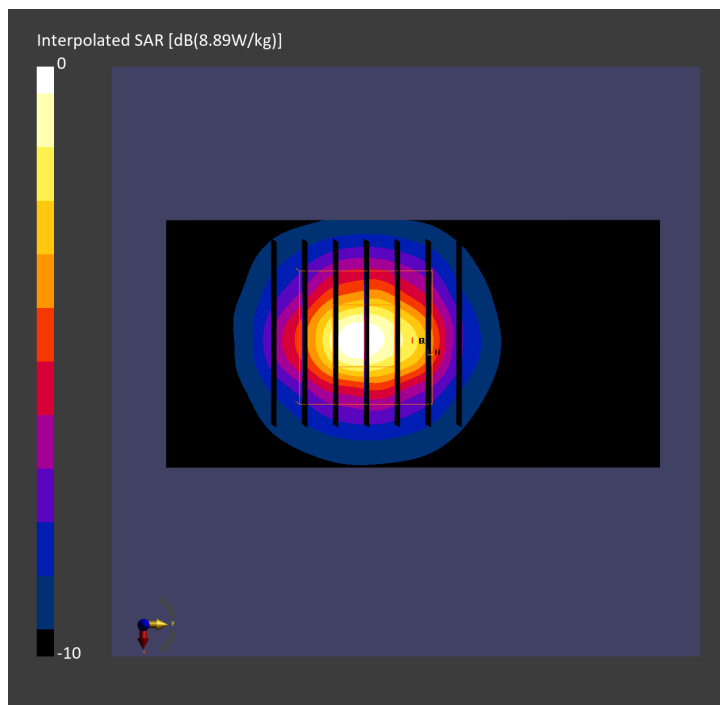

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260604 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.32 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

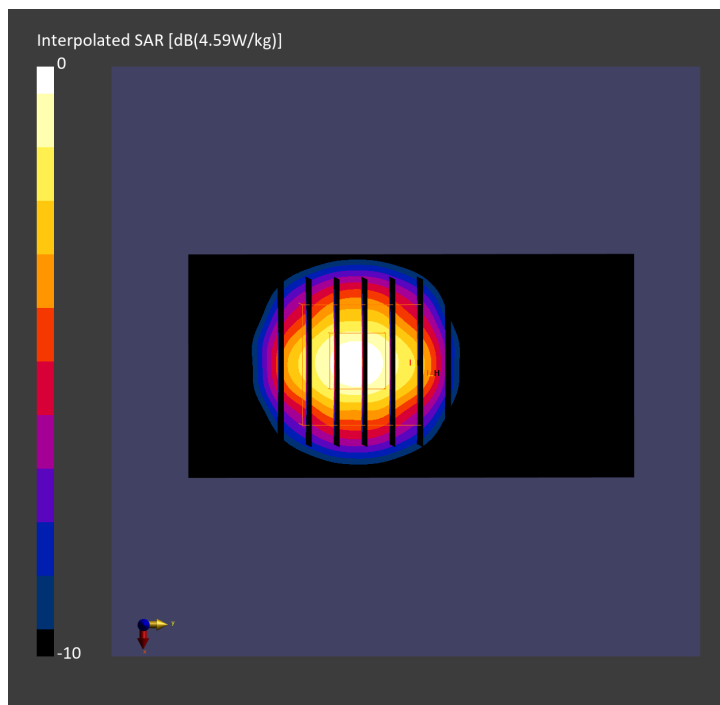

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.43 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.38 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

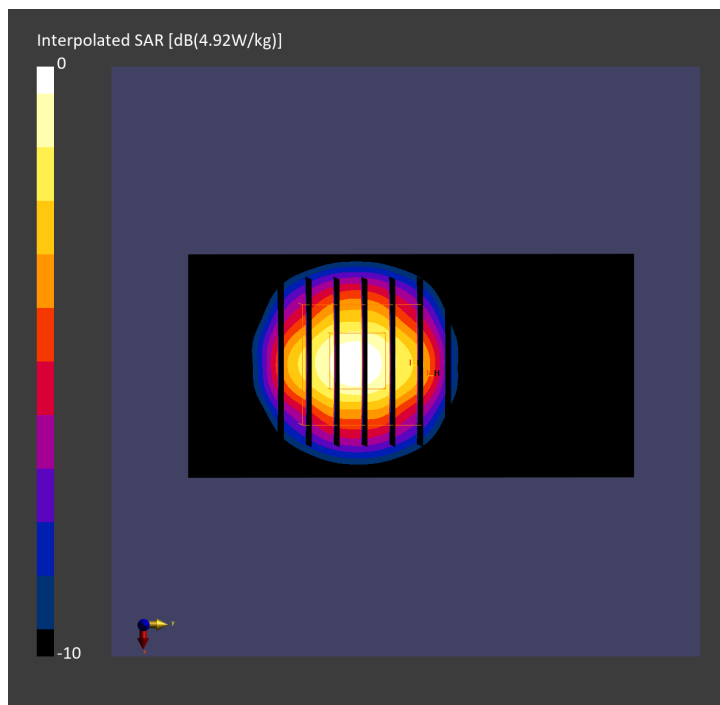

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260604 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.99 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.06 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 71.5 %

TSL Correction: Positive only

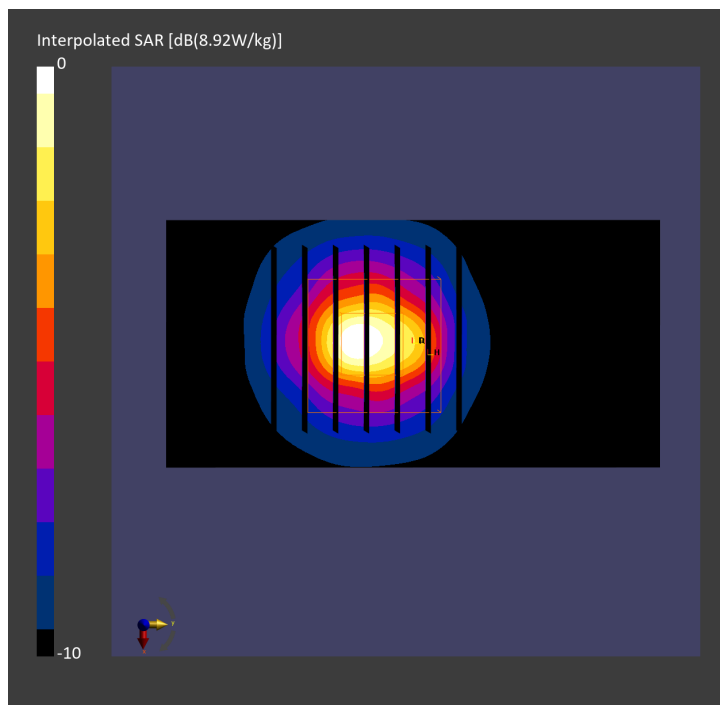

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 72.0 %

TSL Correction: Positive only

