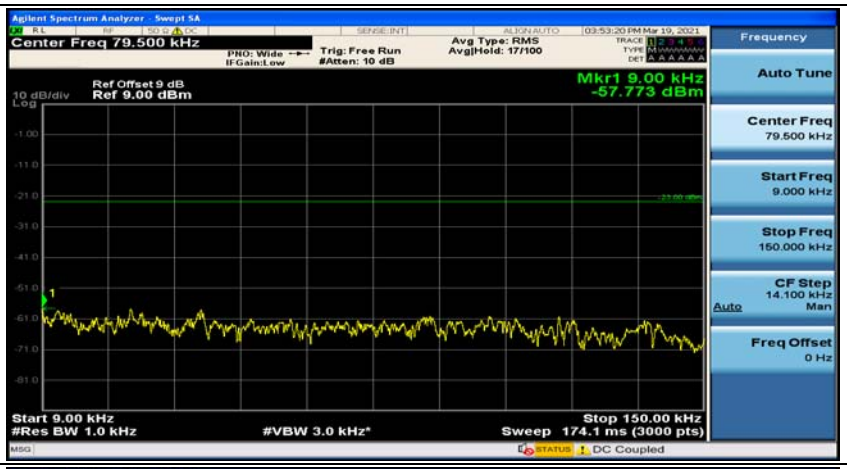
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:53:20 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 9.00 kHz
-57.773 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

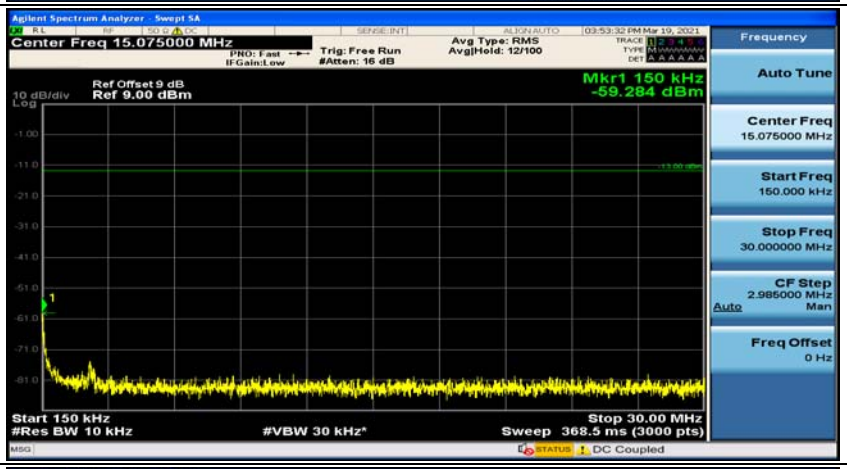
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
03:53:32 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-59.284 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:53:39 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.922 GHz
-29.805 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 3 MHz

(Channel Bandwidth: 3 MHz)_LCH_QPSK_1RB#0

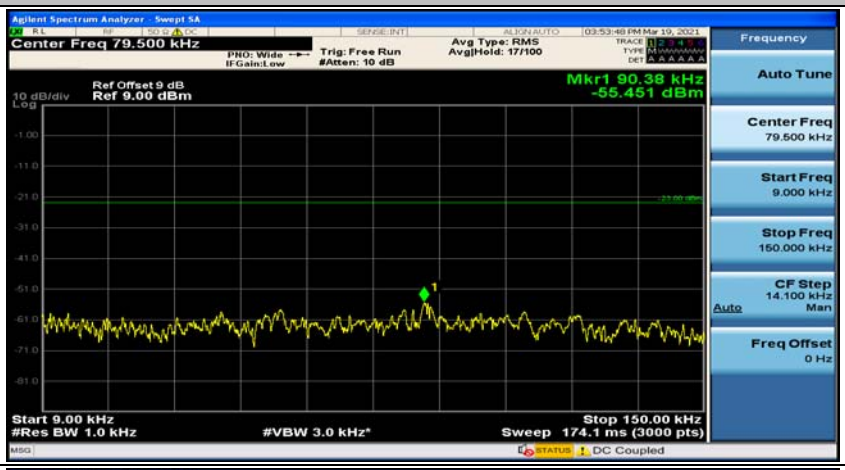

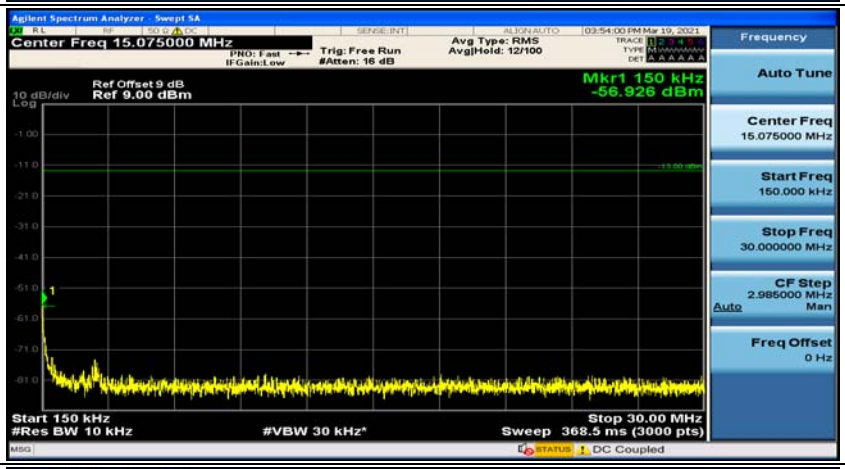

(Channel Bandwidth: 3 MHz)_LCH_QPSK_1RB#7

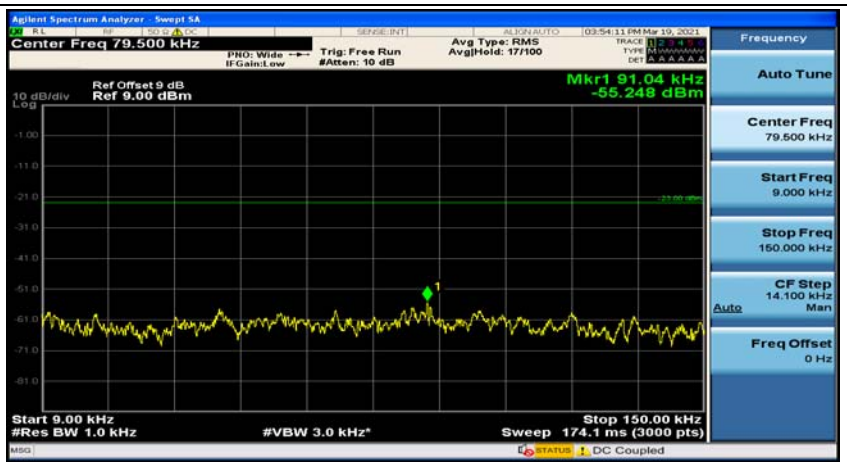
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:54:11 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 91.04 kHz
-55.248 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

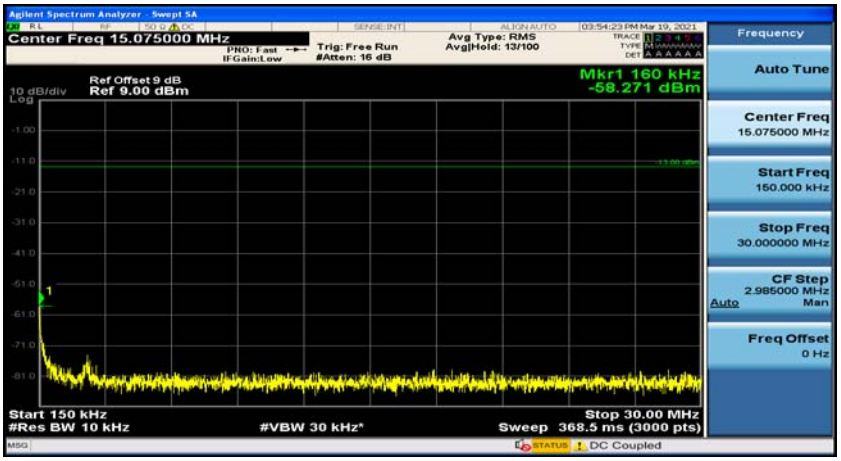
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
03:54:23 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 160 kHz
-58.271 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:54:29 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Mkr2 25.385 GHz
-28.755 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

(Channel Bandwidth: 3 MHz)_MCH_QPSK_1RB#0

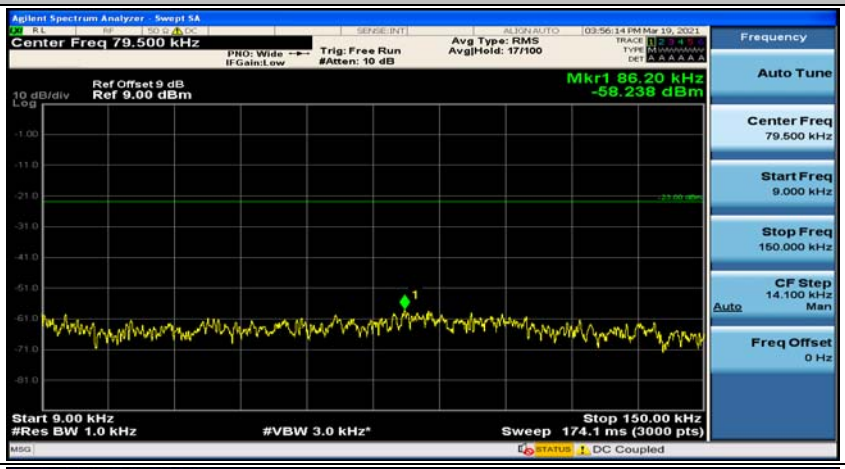

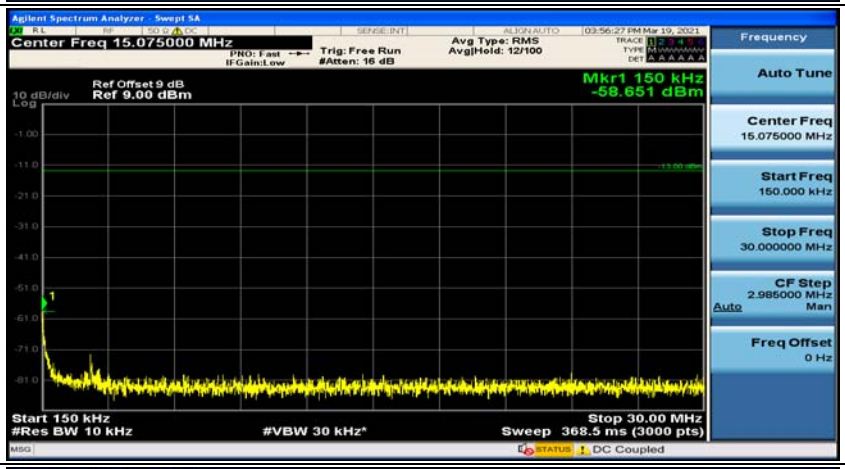

(Channel Bandwidth: 3 MHz)_MCH_QPSK_1RB#7

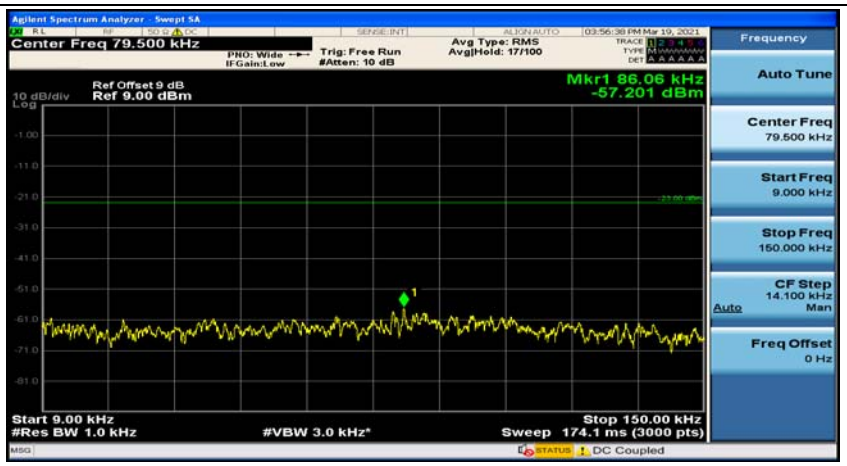
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:56:38 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 86.06 kHz
-57.201 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

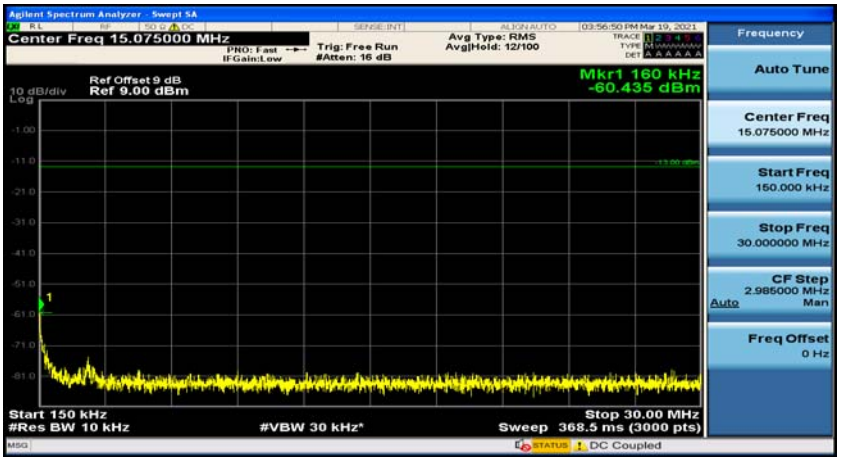
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
03:56:50 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-60.435 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:56:56 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.957 GHz
-29.431 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_HCH_QPSK_1RB#0

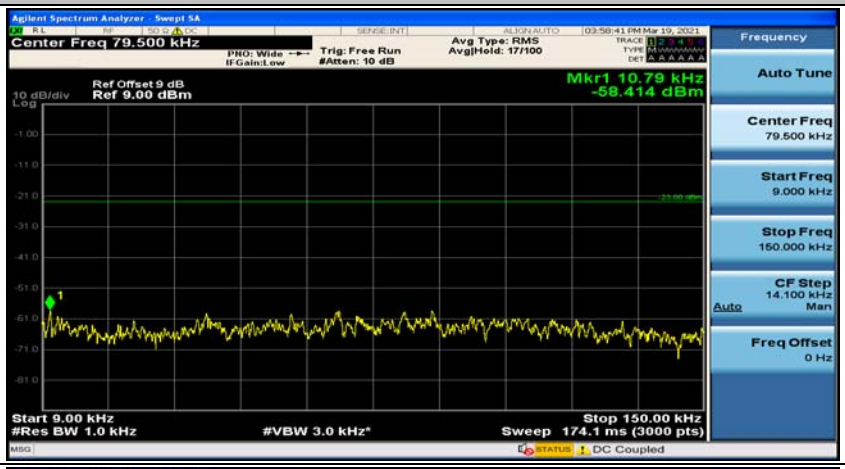

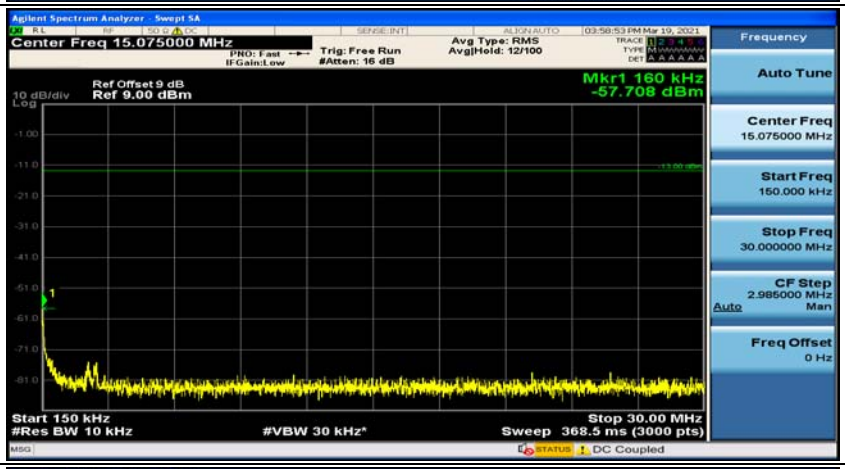

(Channel Bandwidth: 3 MHz)_HCH_QPSK_1RB#7

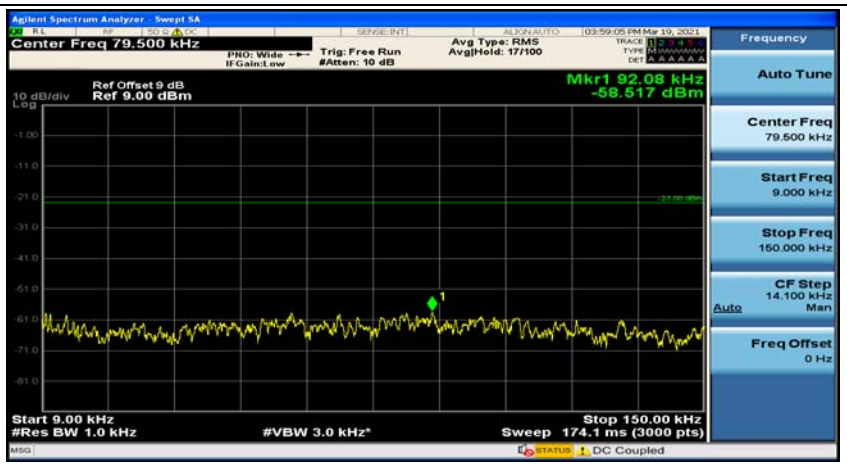
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:59:05 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 92.08 kHz
-58.517 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

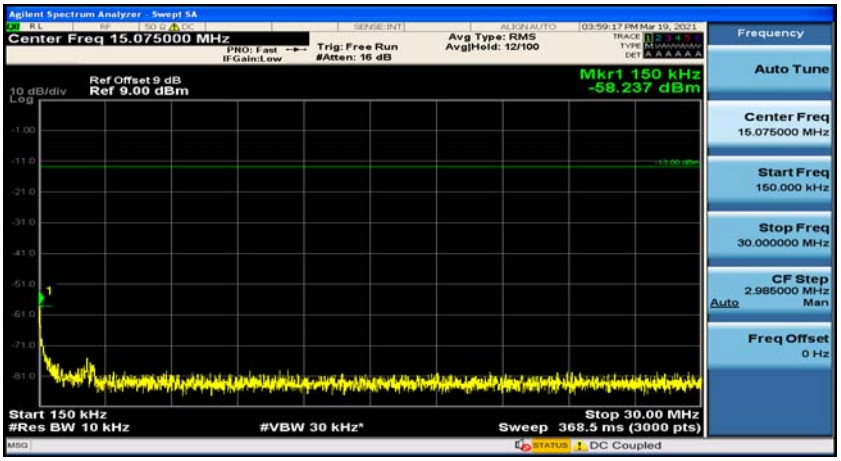
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
03:59:17 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 150 kHz
-58.237 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:59:22 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Mkr2 25.394 GHz
-29.633 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

(Channel Bandwidth: 3 MHz)_LCH_16QAM_1RB#0

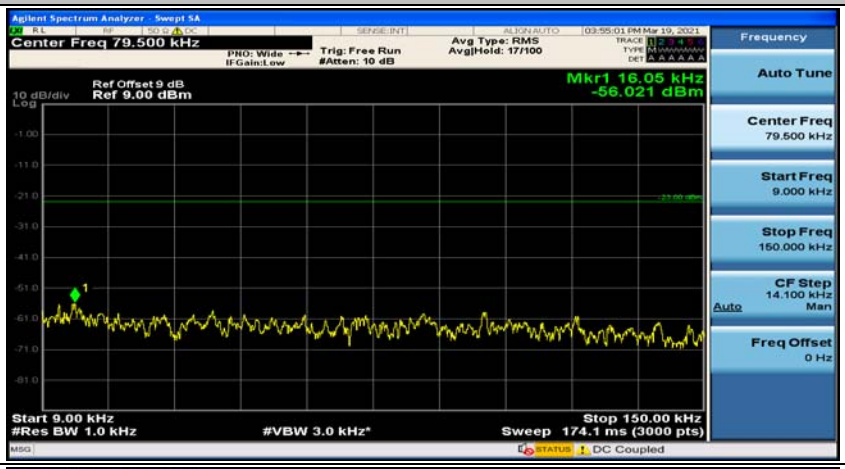

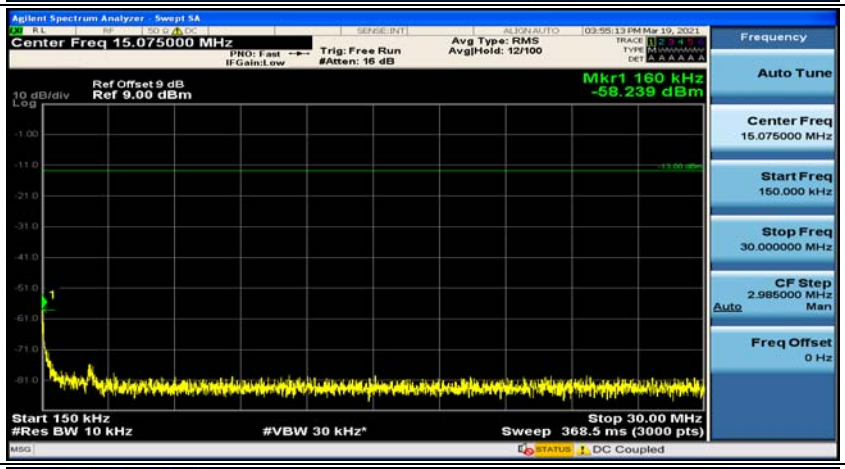

(Channel Bandwidth: 3 MHz)_LCH_16QAM_1RB#7

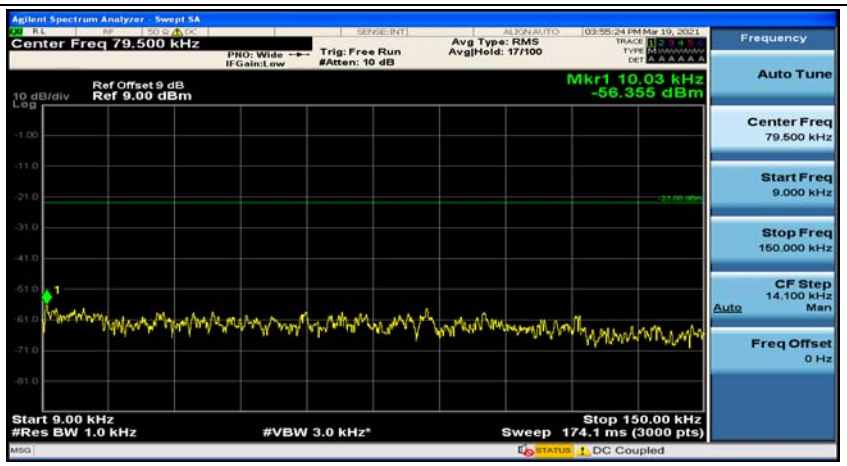
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:55:24 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 10.03 kHz
-56.355 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

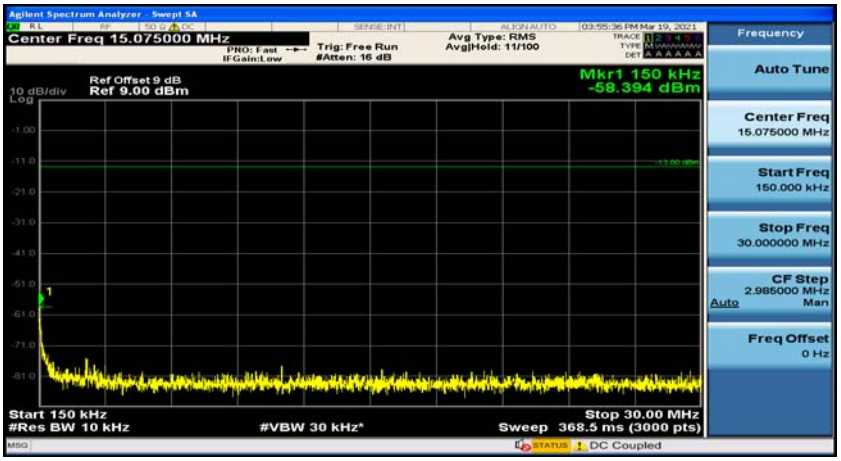
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
03:55:36 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 150 kHz
-58.394 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:55:42 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Mkr2 25.905 GHz
-29.573 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

(Channel Bandwidth: 3 MHz)_MCH_16QAM_1RB#0

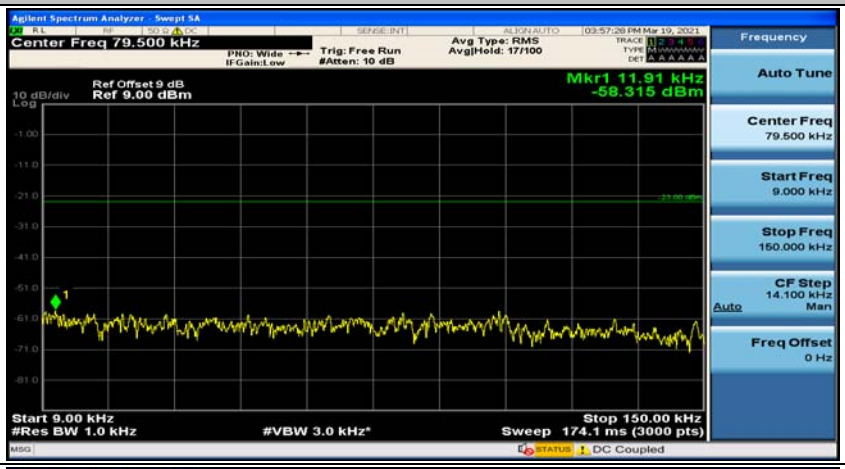

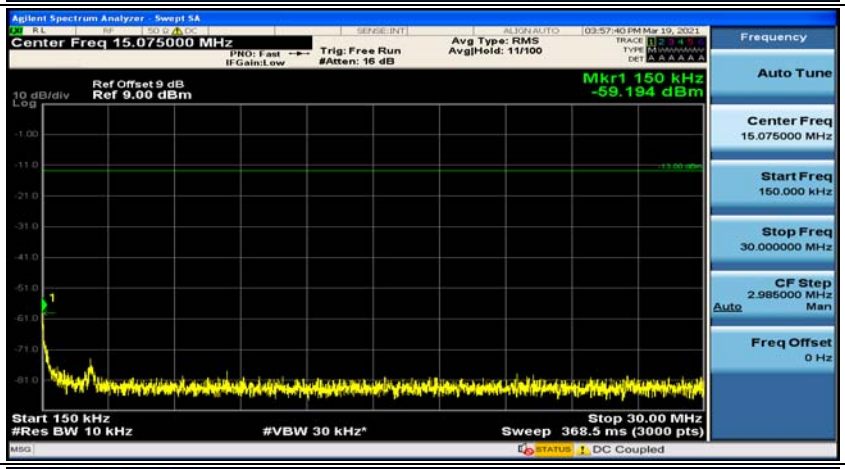

(Channel Bandwidth: 3 MHz)_MCH_16QAM_1RB#7

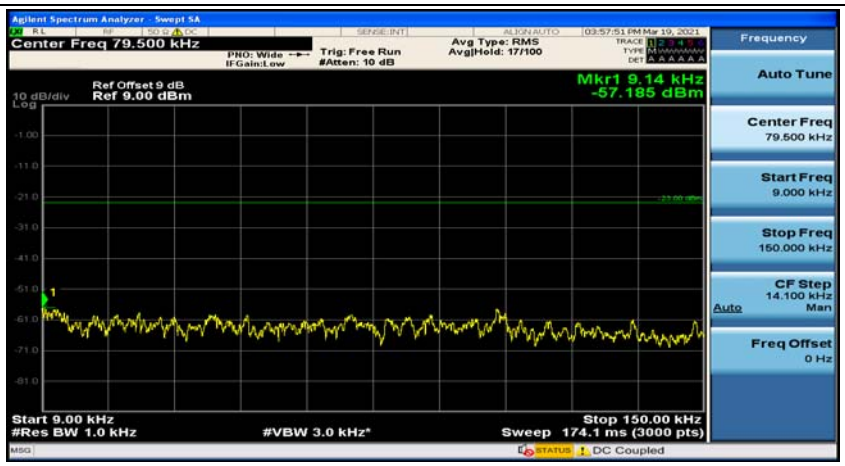
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
03:57:51 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 9.14 kHz
-57.185 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

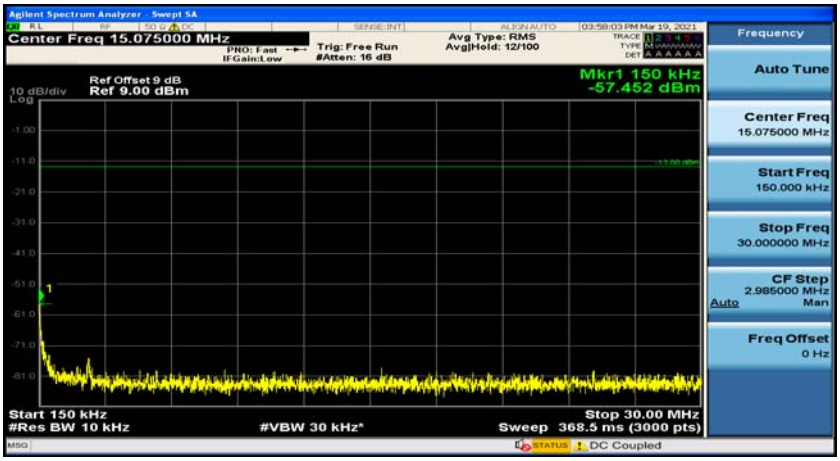
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
03:58:03 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Mkr1 150 kHz
-57.452 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
03:58:09 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Mkr2 25.801 GHz
-29.465 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

(Channel Bandwidth: 3 MHz)_HCH_16QAM_1RB#0

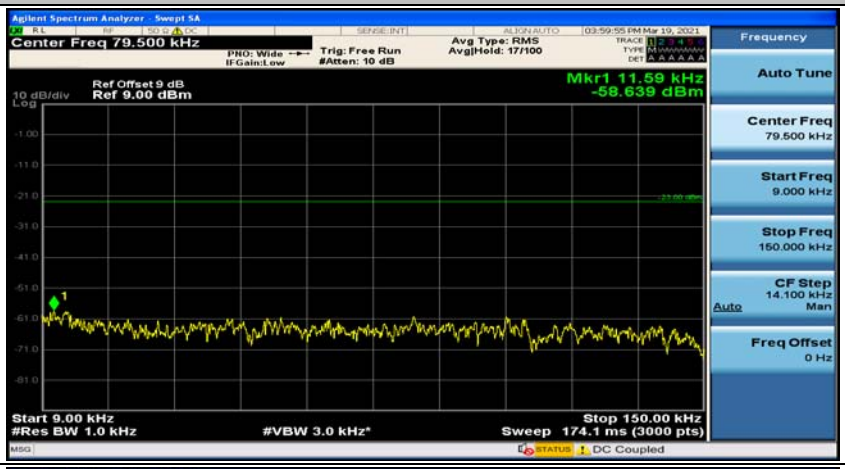

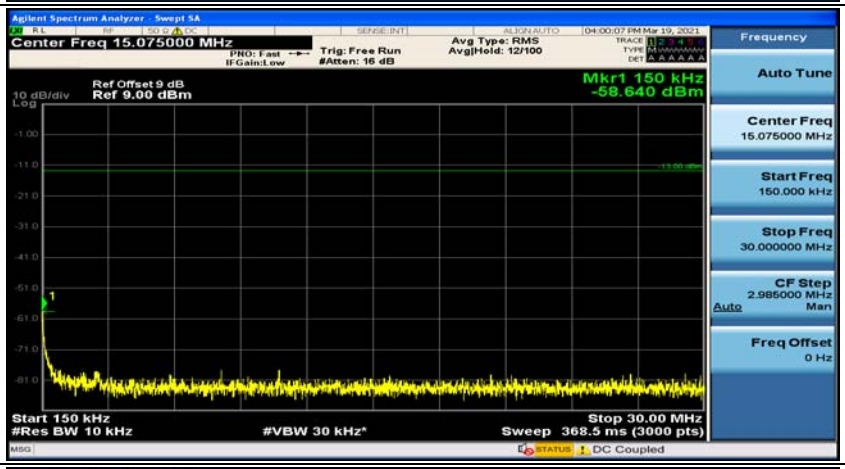

(Channel Bandwidth: 3 MHz)_HCH_16QAM_1RB#7

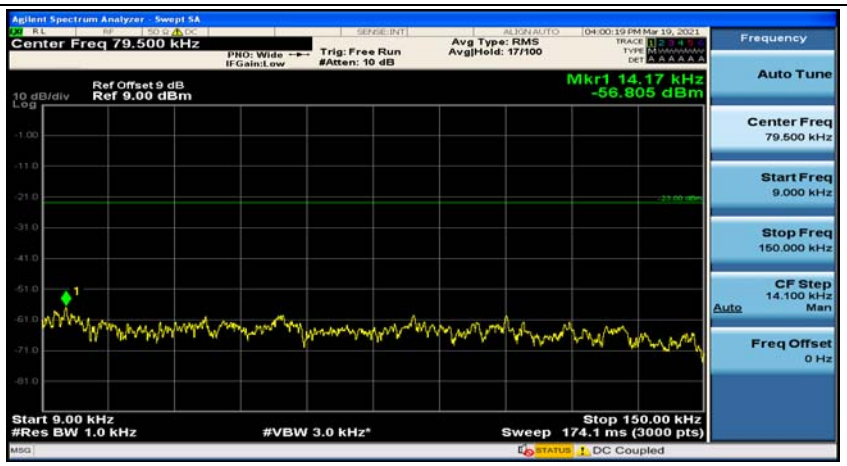
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:00:19 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 14.17 kHz
-56.805 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

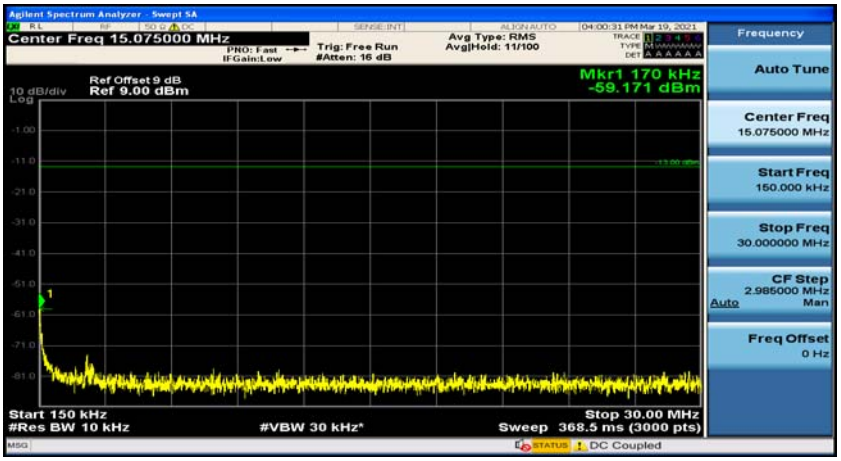
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
04:00:31 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 170 kHz
-59.171 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:00:37 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.498 GHz
-29.807 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 5 MHz

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#0

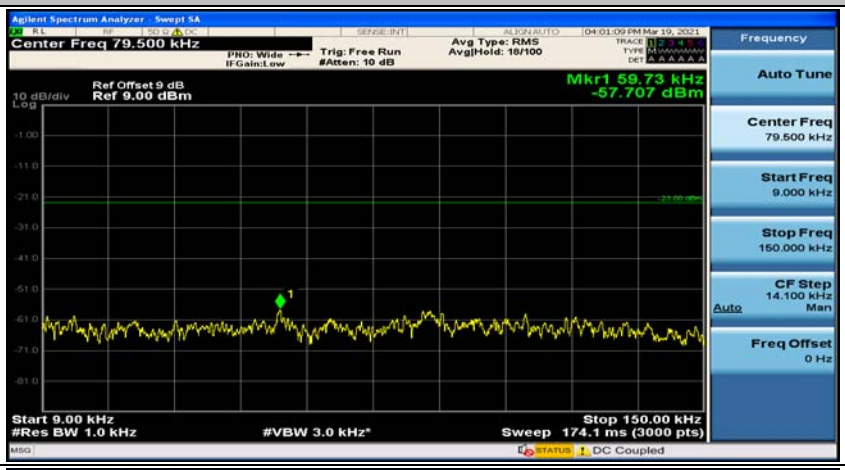

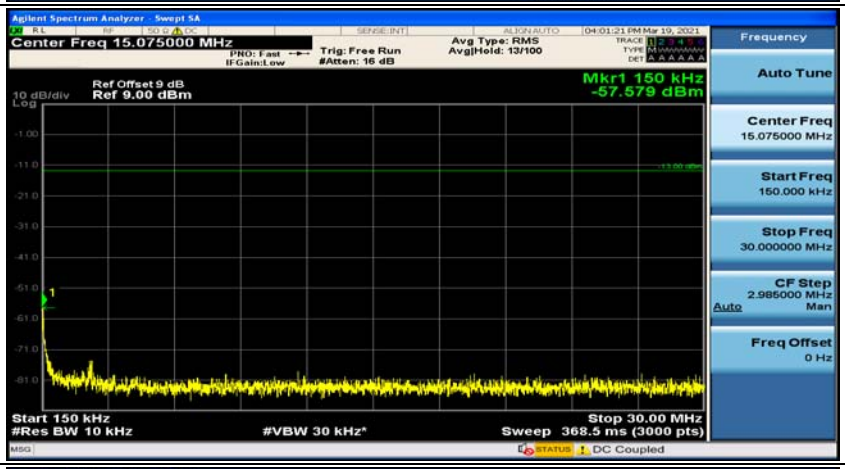

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#12

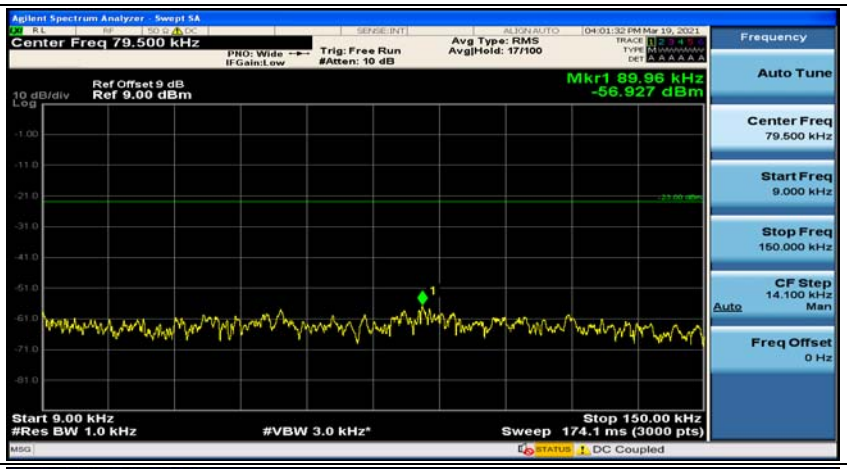

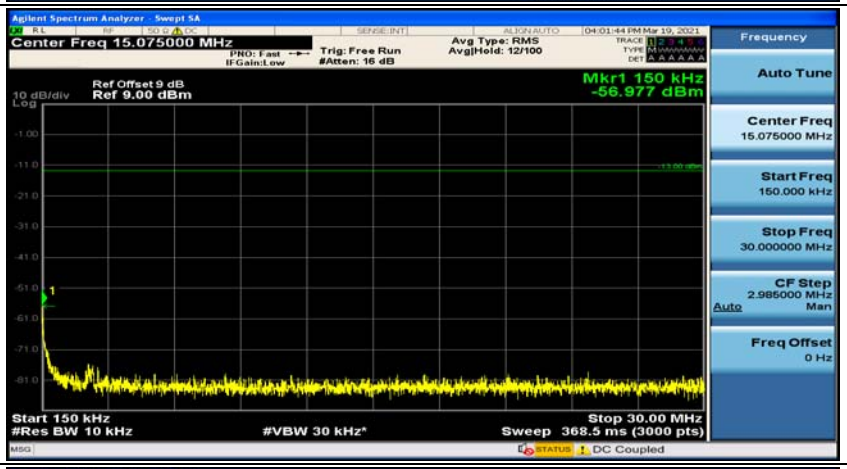

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#24

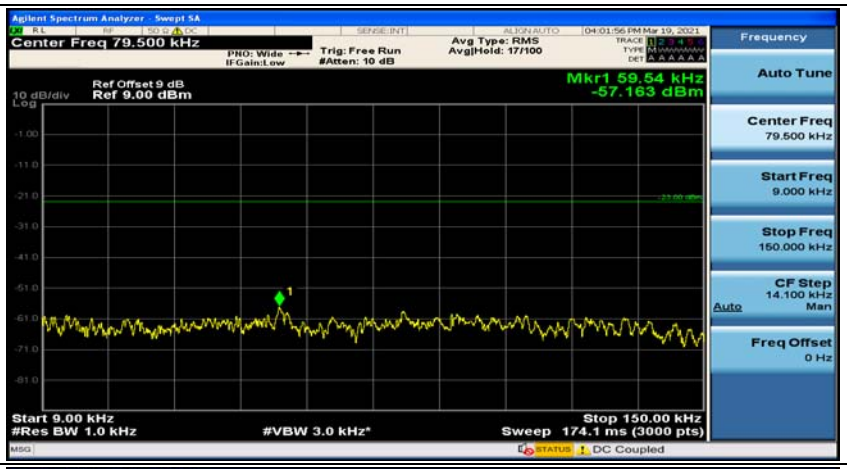
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:01:56 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 59.54 kHz
-57.163 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

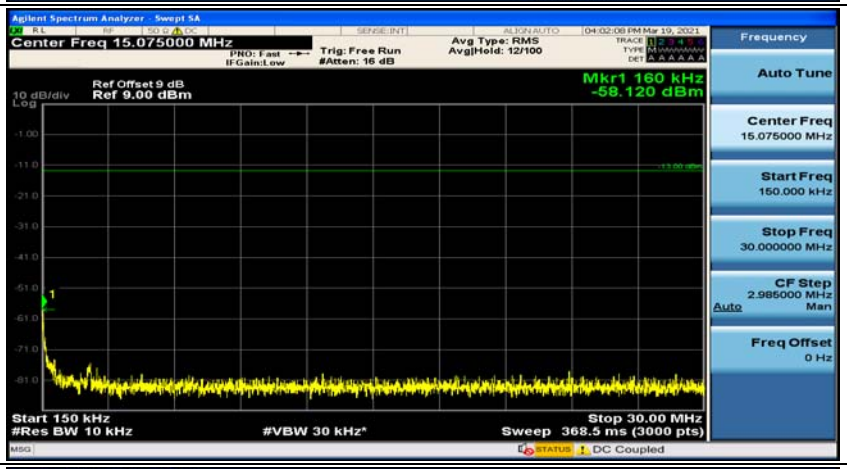
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
04:02:08 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.120 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:02:14 PM Mar 19, 2021
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.532 GHz
-29.381 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#0

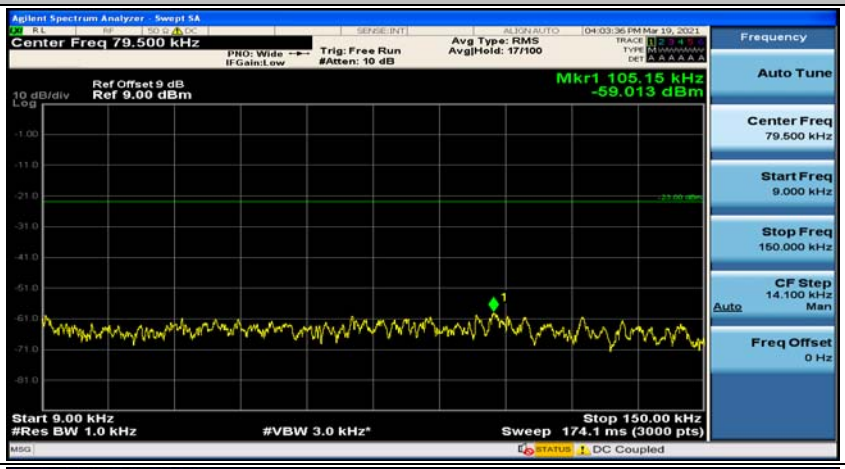

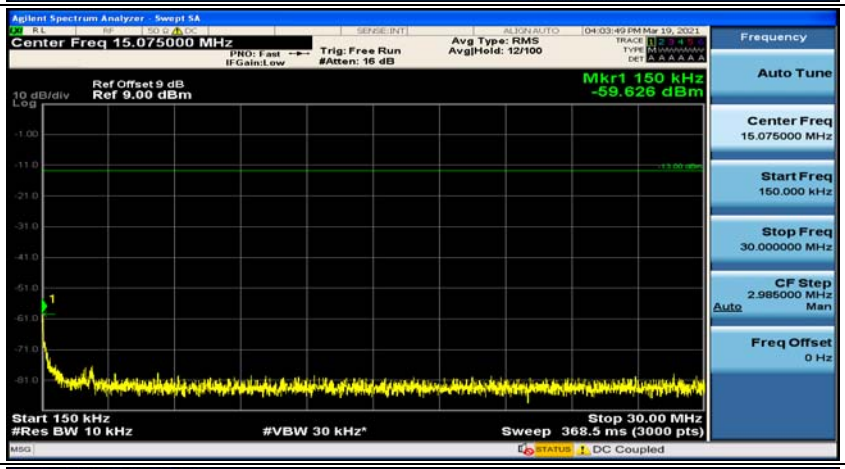

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#12

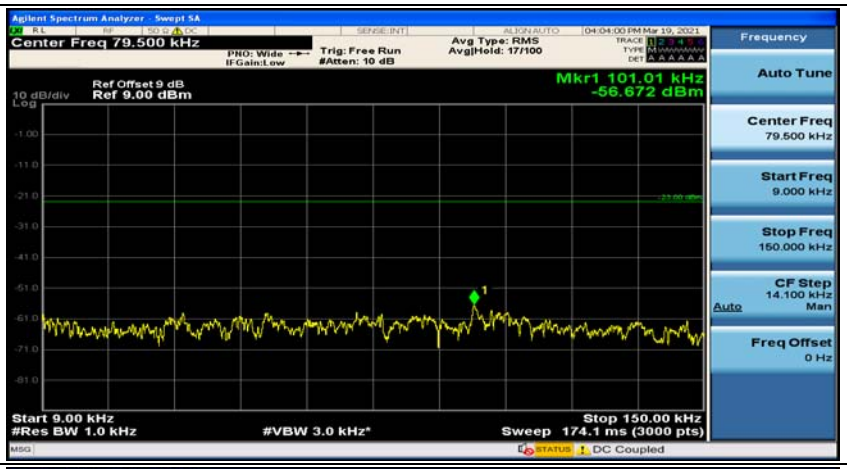

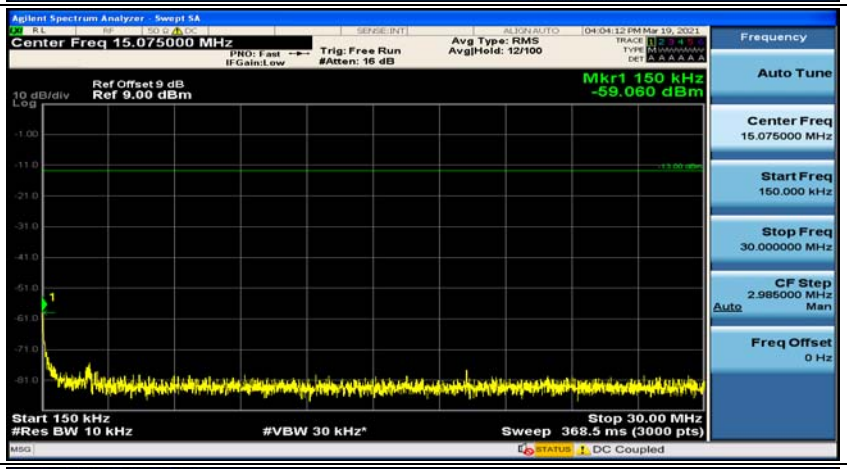

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#24

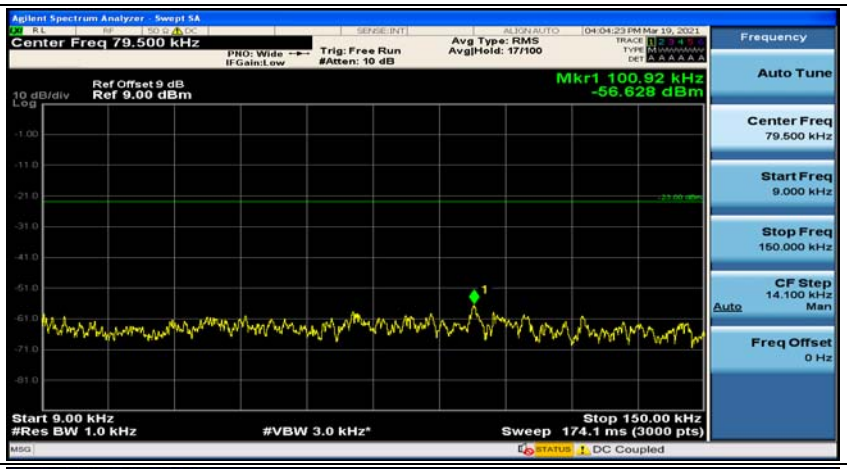
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 100.92 kHz
-56.628 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

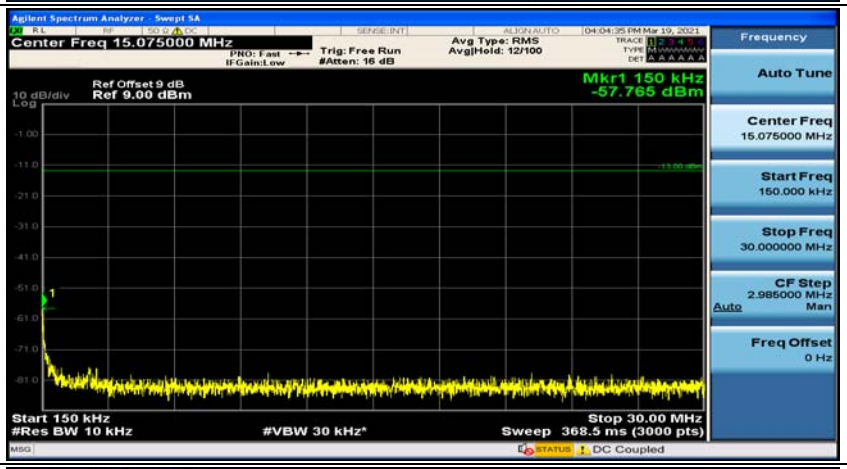
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.765 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.325 GHz
-29.329 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_HCH_QPSK_1RB#0

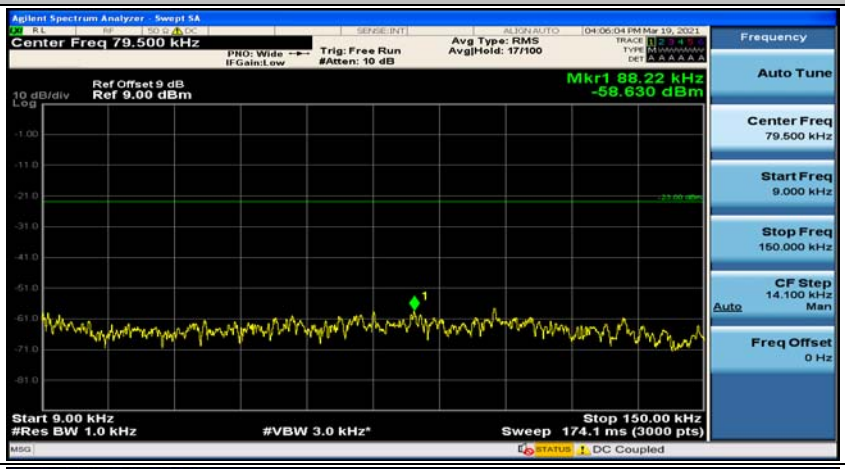

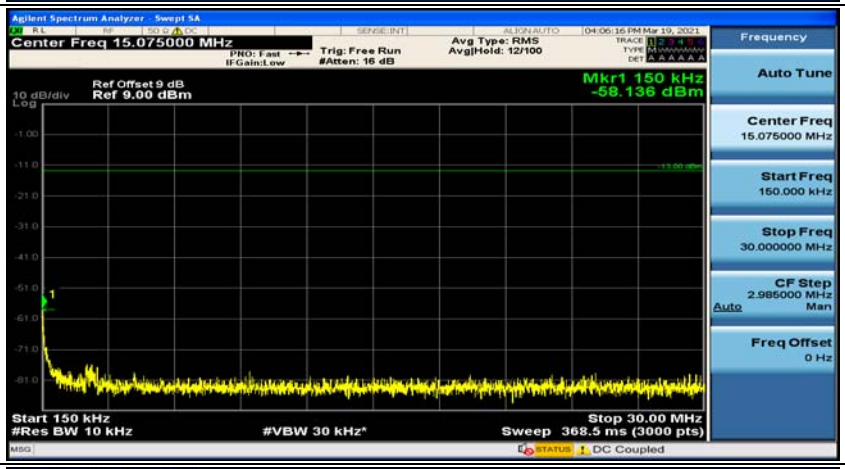

(Channel Bandwidth: 5 MHz)_HCH_QPSK_1RB#12

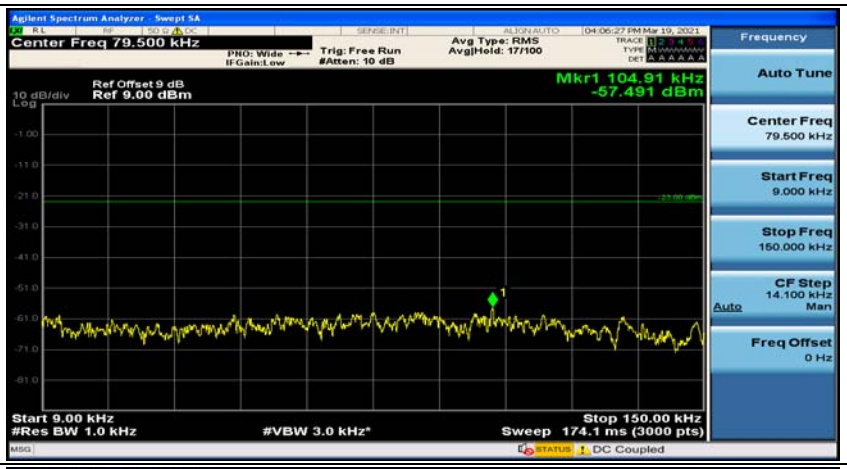

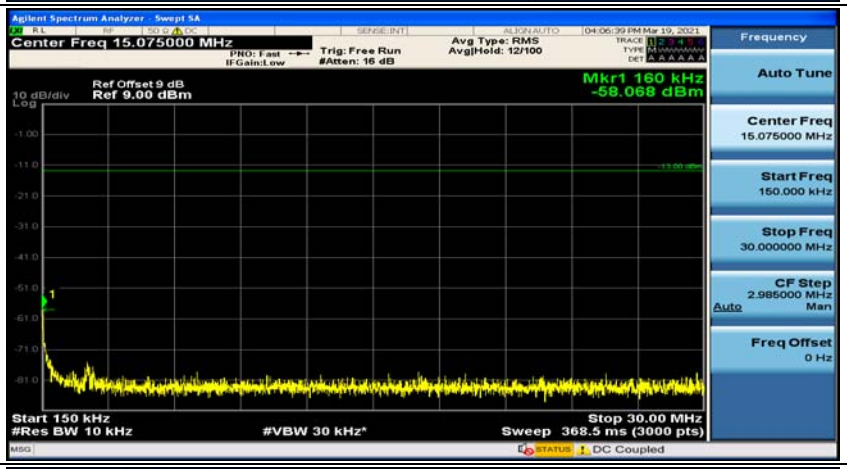

(Channel Bandwidth: 5 MHz)_HCH_QPSK_1RB#24

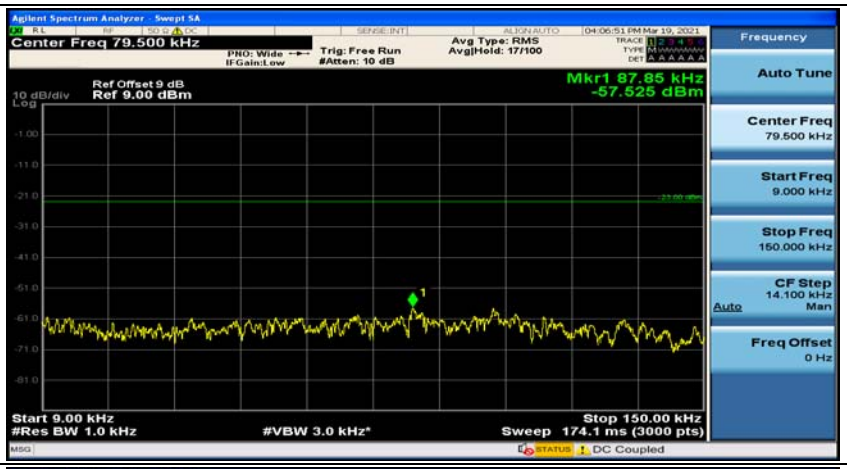
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:06:51 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 87.85 kHz
-57.525 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

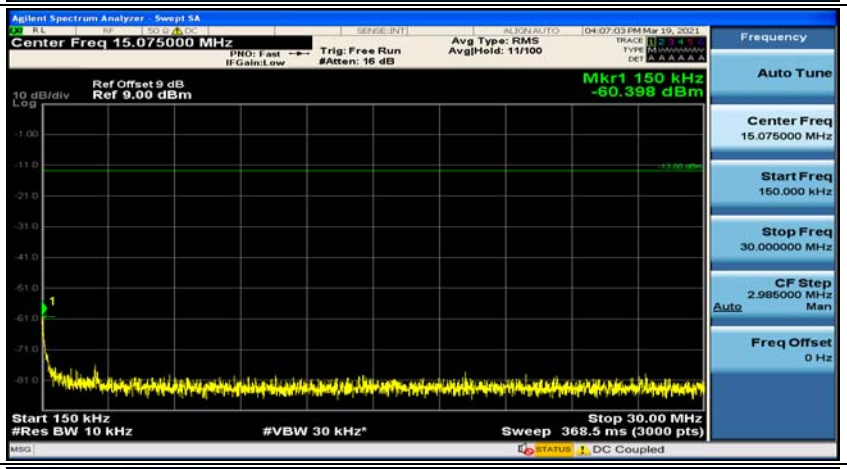
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
04:07:03 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-60.398 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:07:08 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.584 GHz
-29.516 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_LCH_16QAM_1RB#0

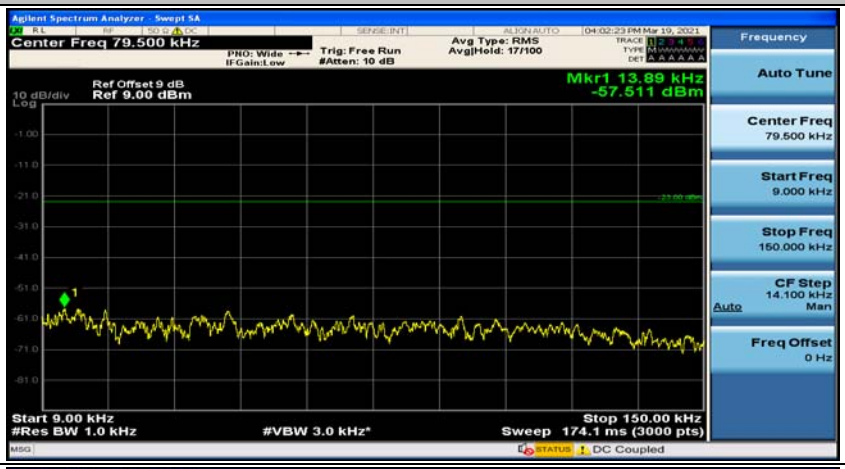

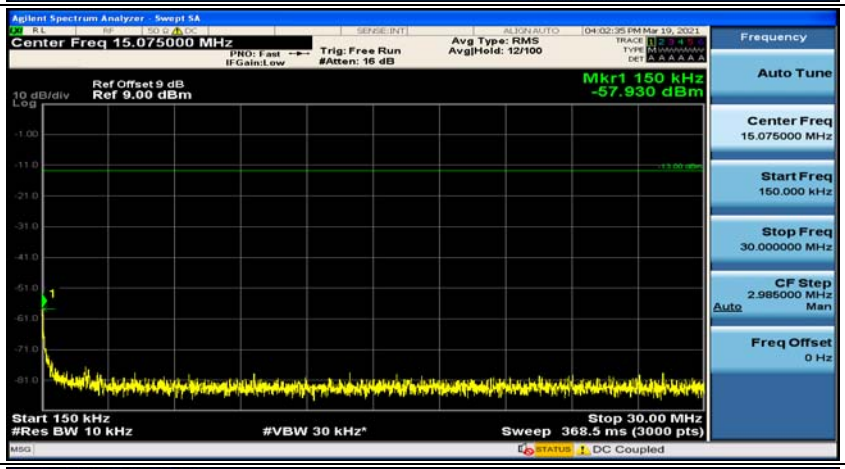

(Channel Bandwidth: 5 MHz)_LCH_16QAM_1RB#12

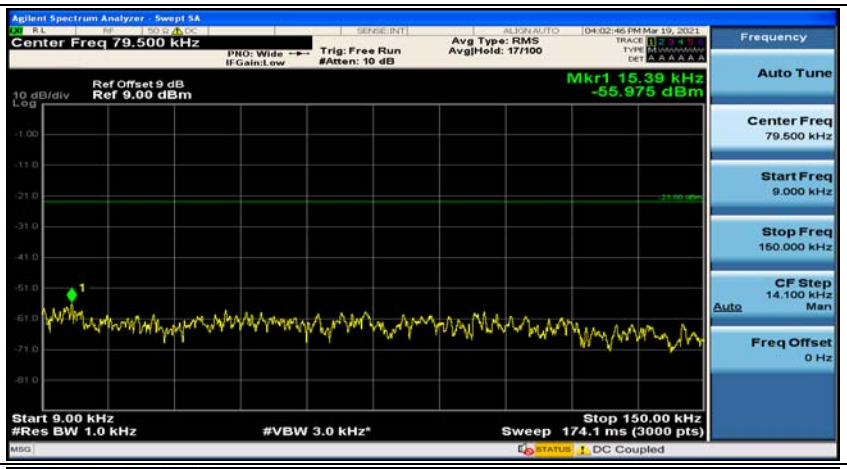

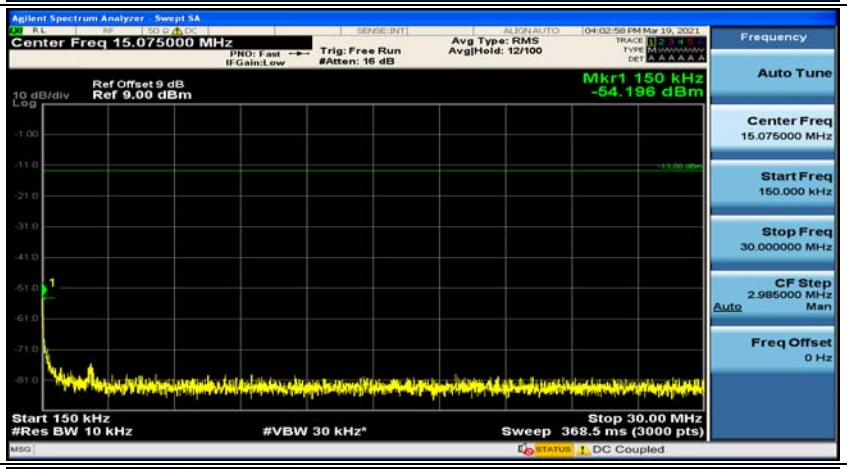

(Channel Bandwidth: 5 MHz)_LCH_16QAM_1RB#24

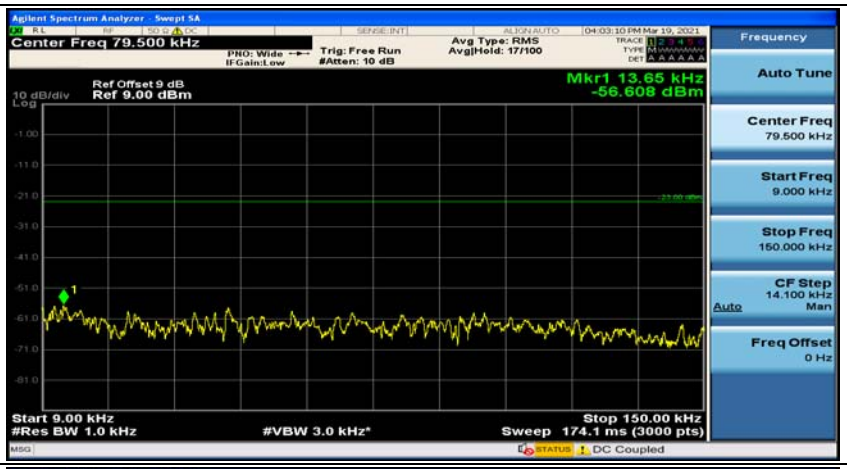
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:03:10 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 13.65 kHz
-56.608 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

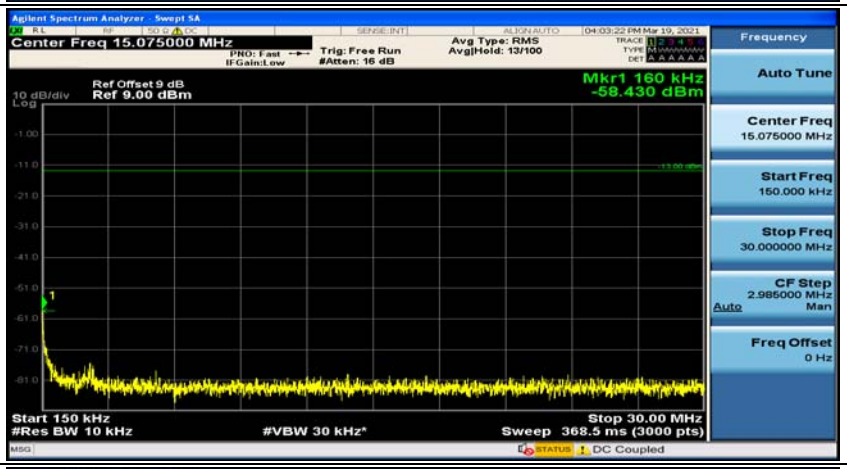
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
04:03:22 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.430 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:03:27 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.558 GHz
-30.017 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_MCH_16QAM_1RB#0

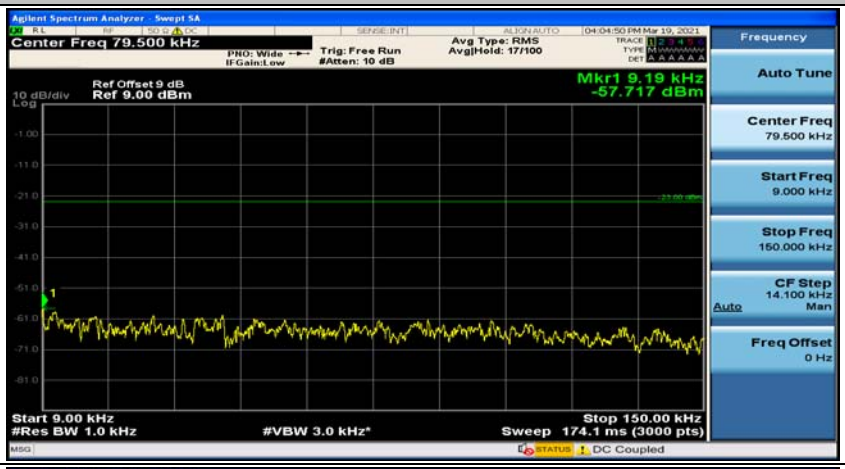

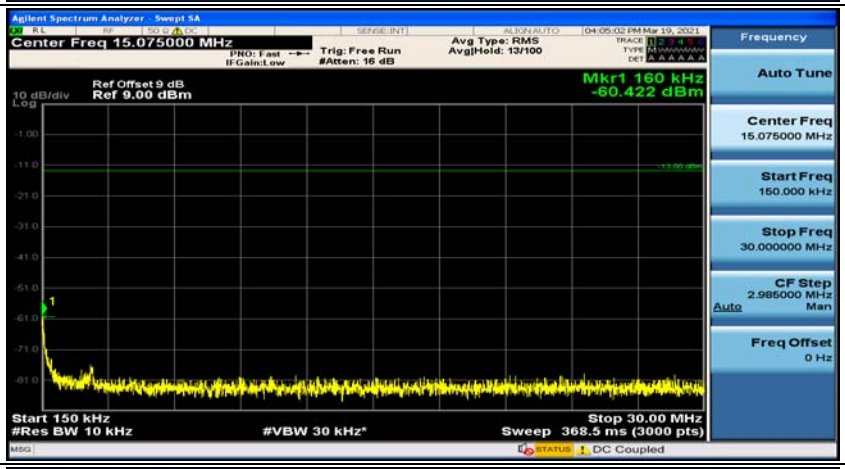

(Channel Bandwidth: 5 MHz)_MCH_16QAM_1RB#12

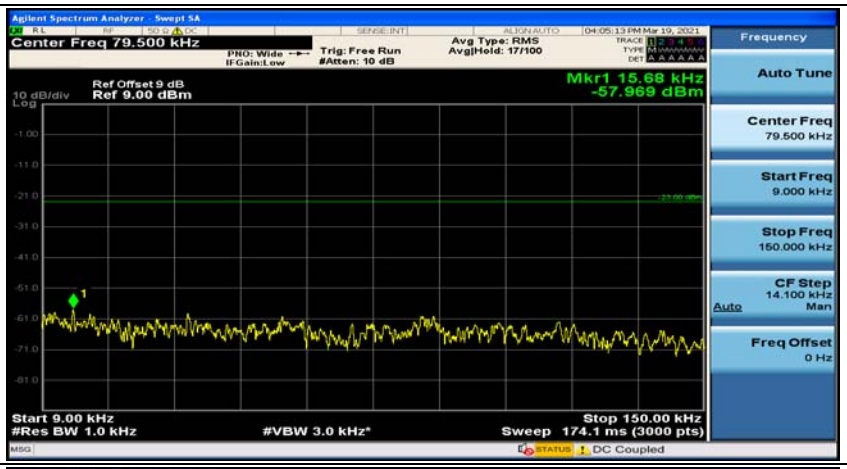

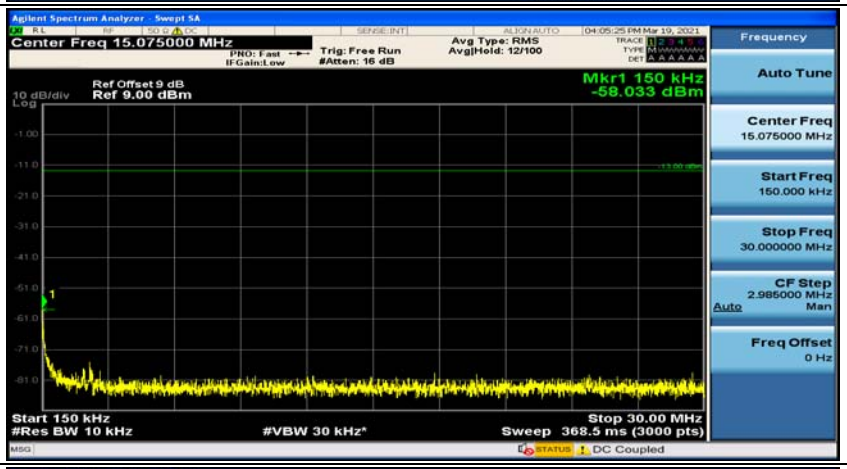

(Channel Bandwidth: 5 MHz)_MCH_16QAM_1RB#24

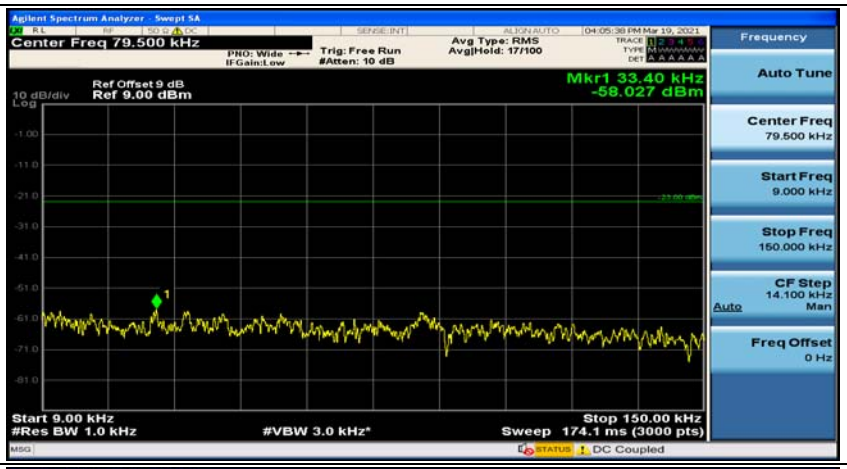
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:05:38 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 33.40 kHz
-58.027 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

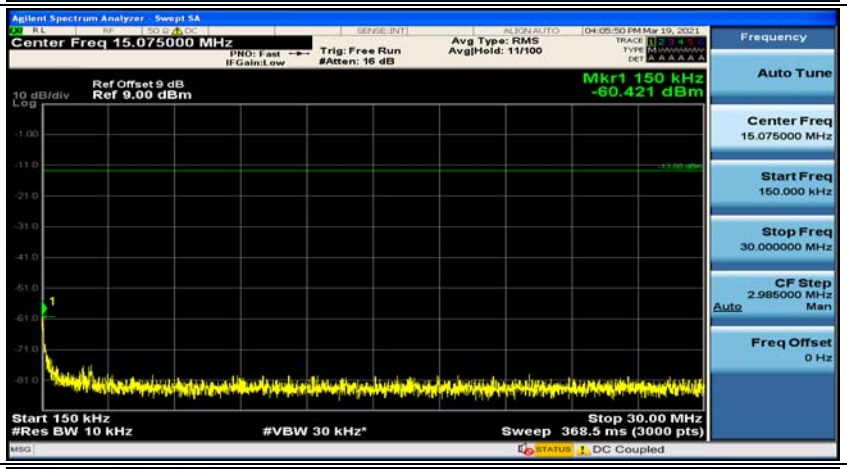
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
04:05:50 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-60.421 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:05:55 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.939 GHz
-29.827 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_HCH_16QAM_1RB#0

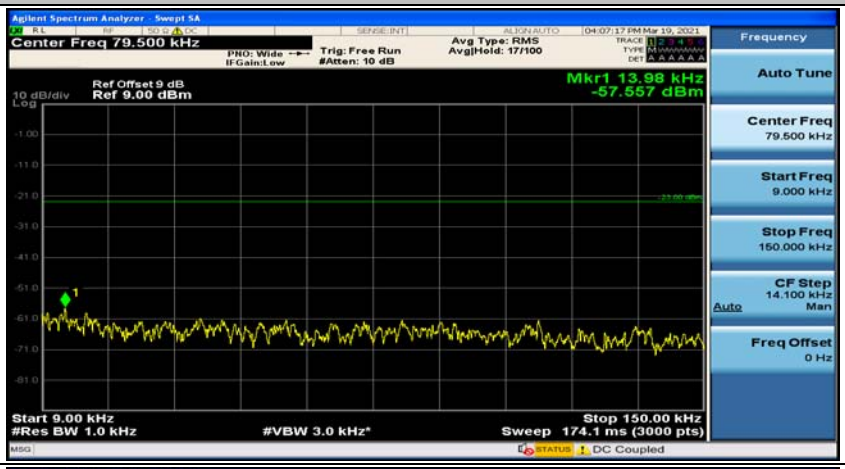

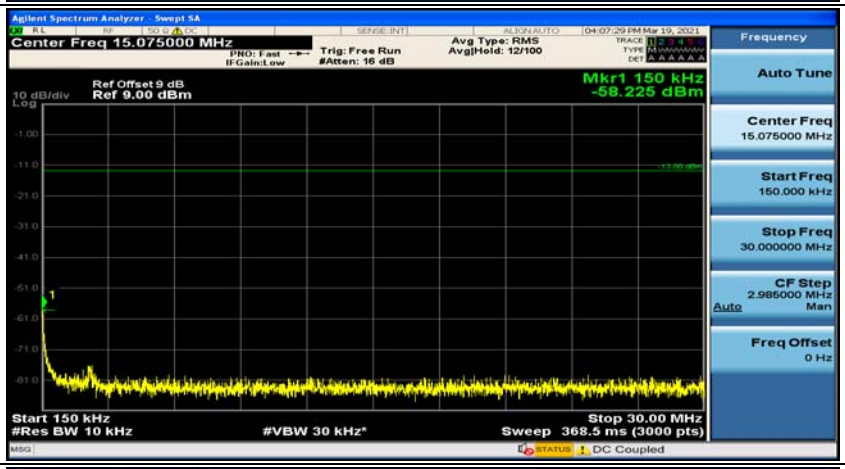

(Channel Bandwidth: 5 MHz)_HCH_16QAM_1RB#12

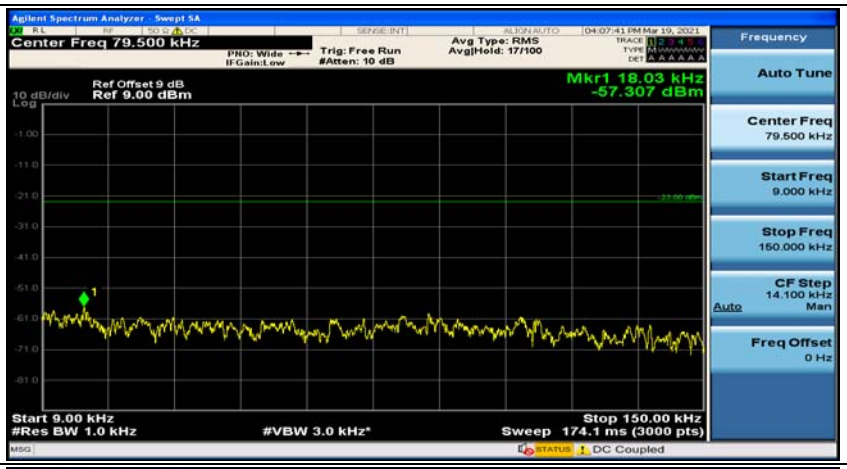

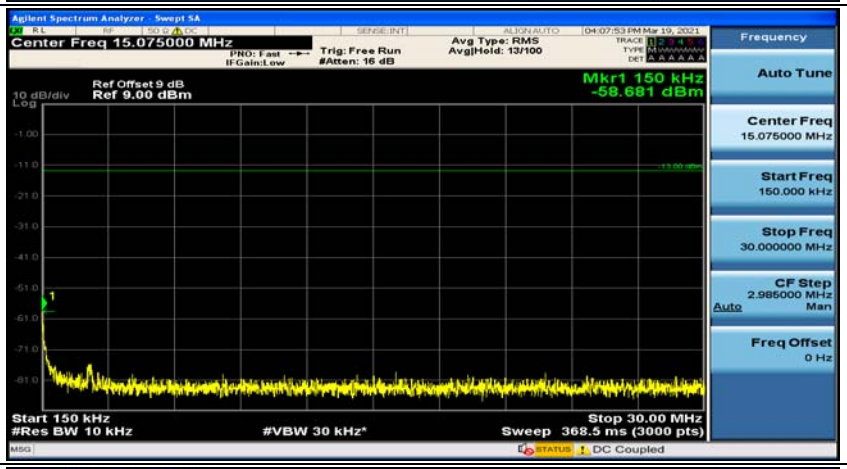

(Channel Bandwidth: 5 MHz)_HCH_16QAM_1RB#24

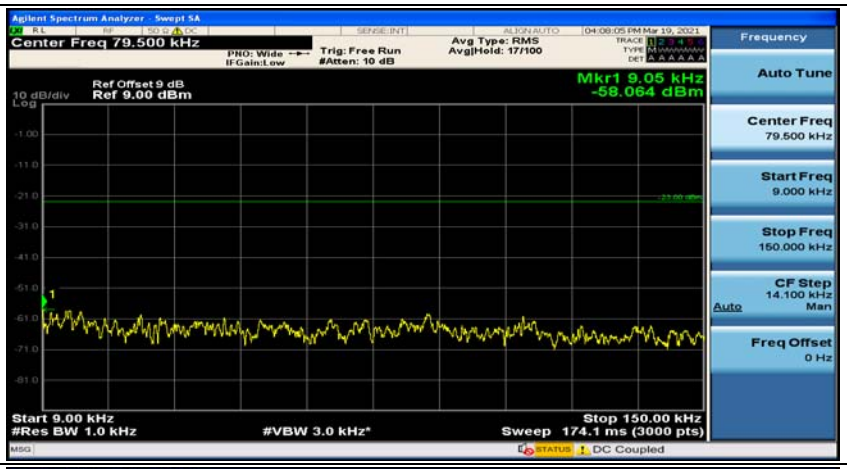
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:08:05 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 9.05 kHz
-58.064 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

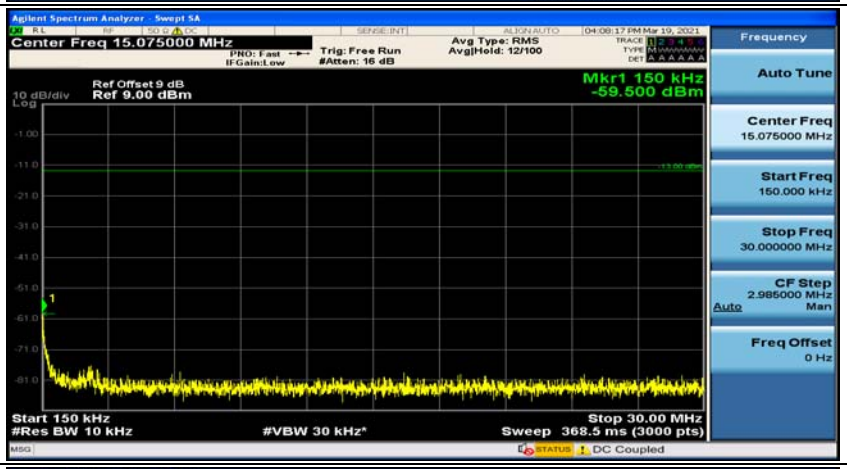
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
04:08:17 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-59.500 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:08:22 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.922 GHz
-29.492 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz

Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#0
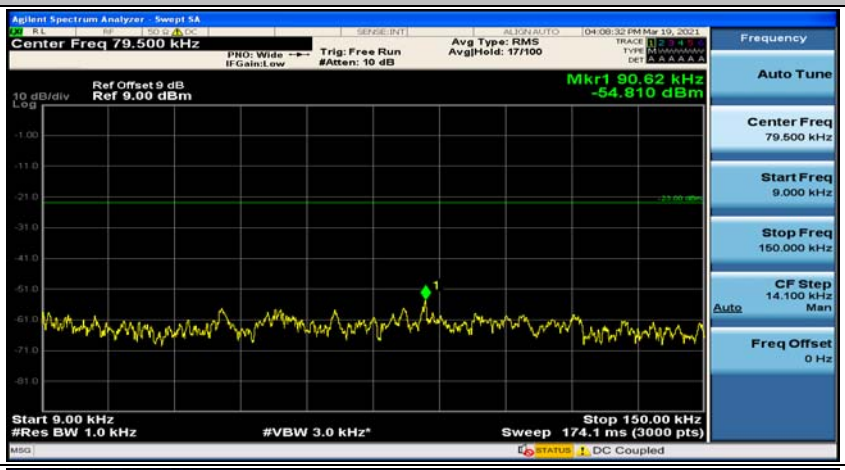
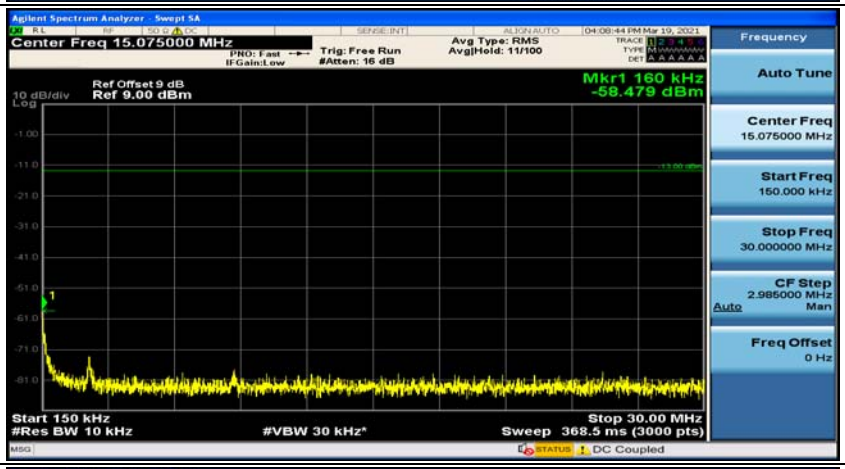
Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#24

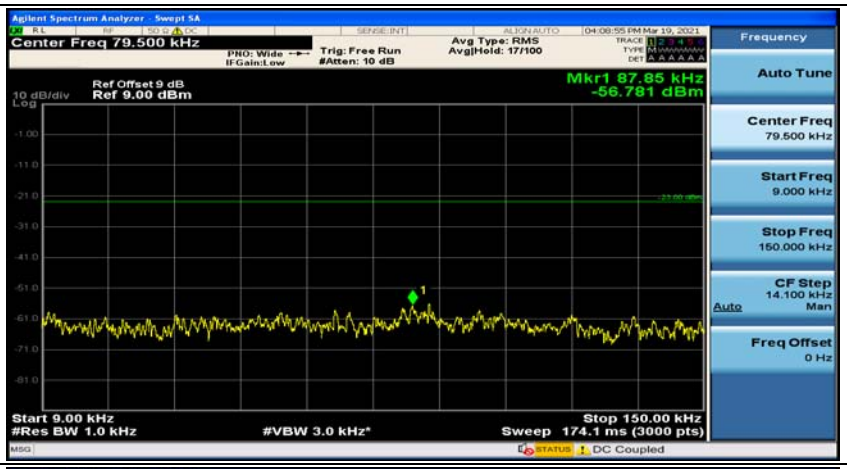

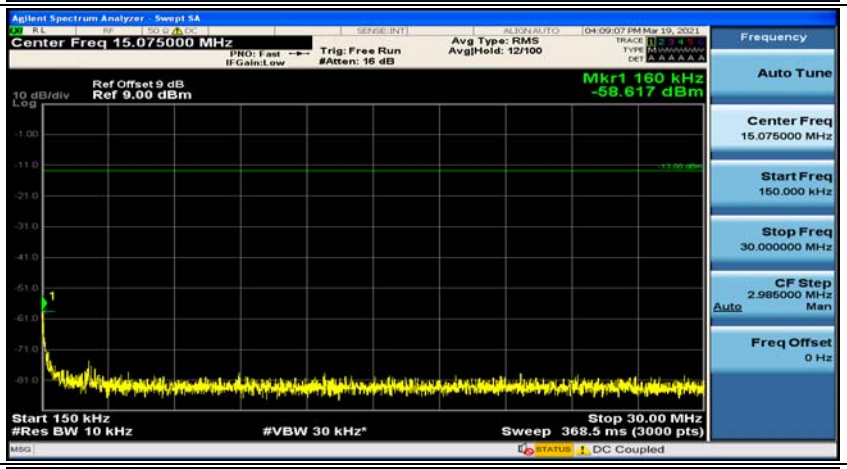

Channel Bandwidth: 10 MHz_LCH_QPSK_1RB#49

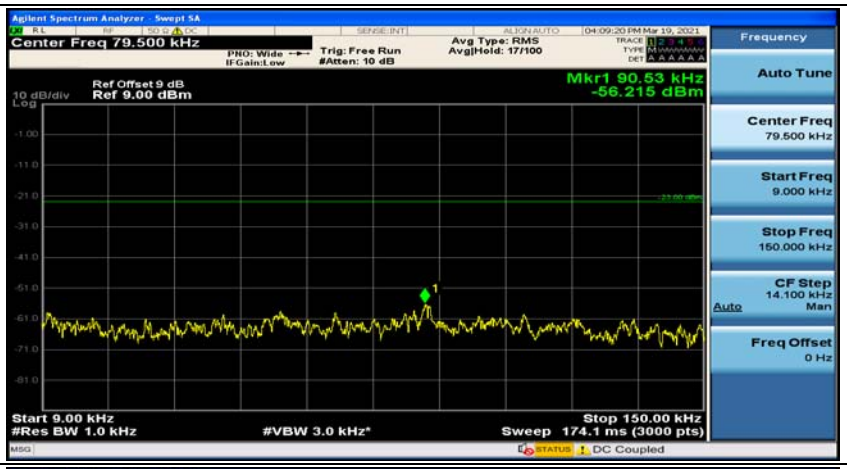
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:09:20 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 90.53 kHz
-56.215 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

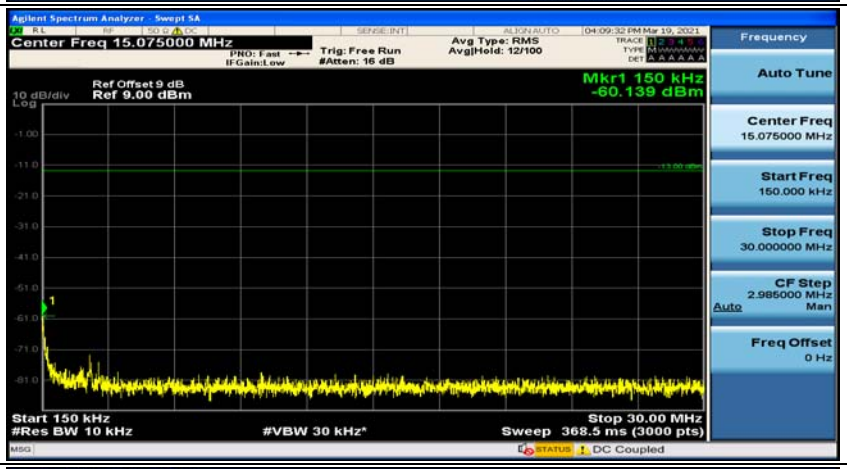
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
04:09:32 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-60.139 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:09:38 PM Mar 19, 2021
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.446 GHz
-29.622 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#0
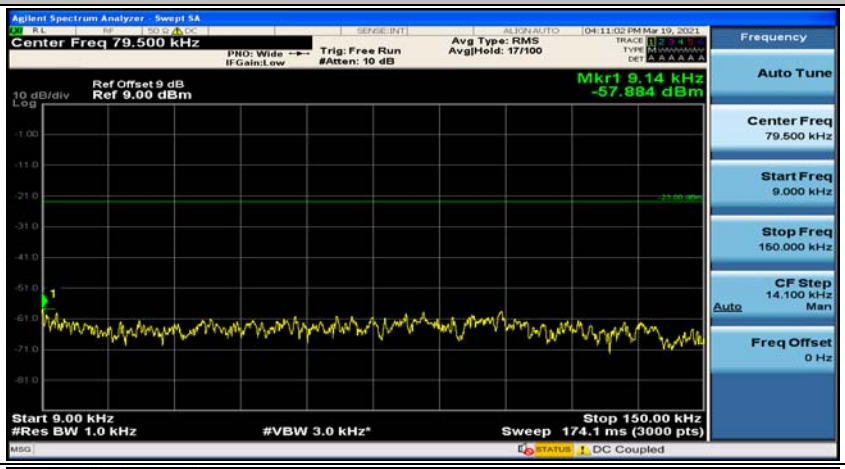
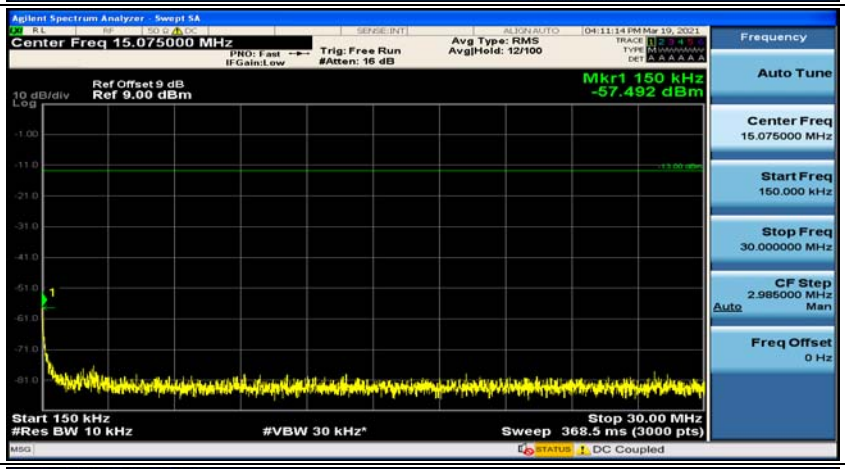
Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#24

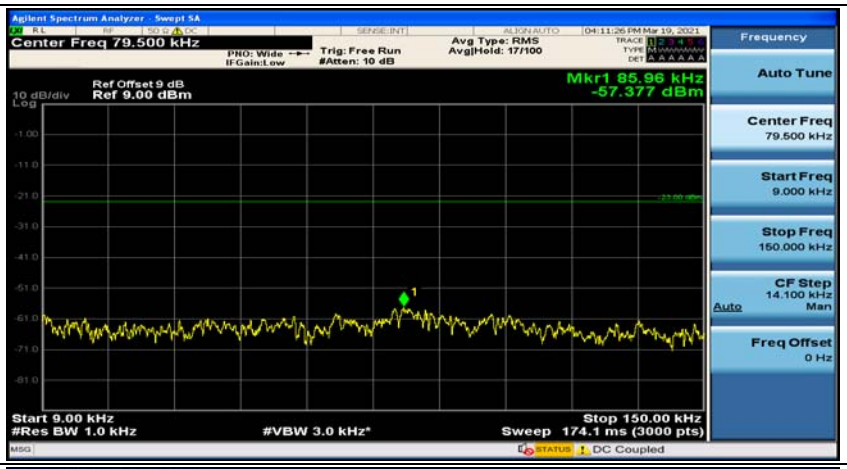

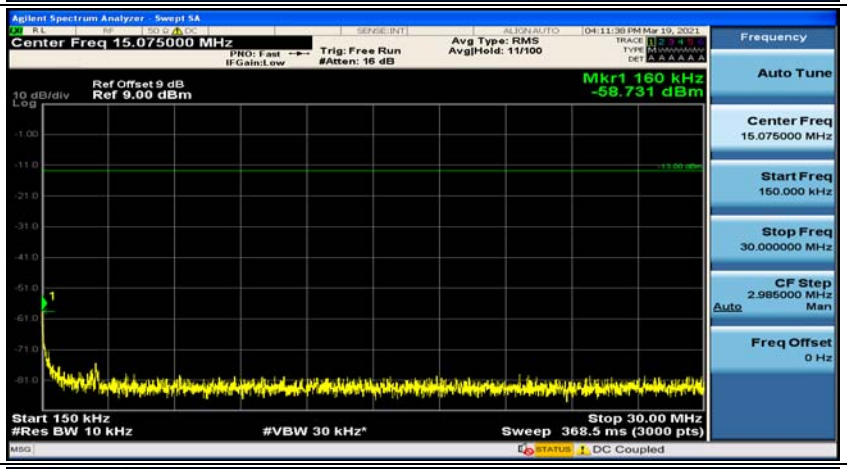

Channel Bandwidth: 10 MHz_MCH_QPSK_1RB#49

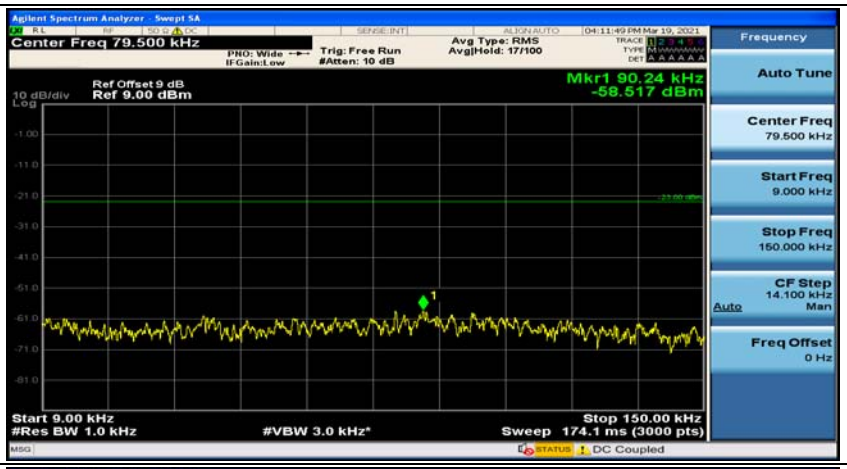
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:11:49 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 90.24 kHz
-58.517 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

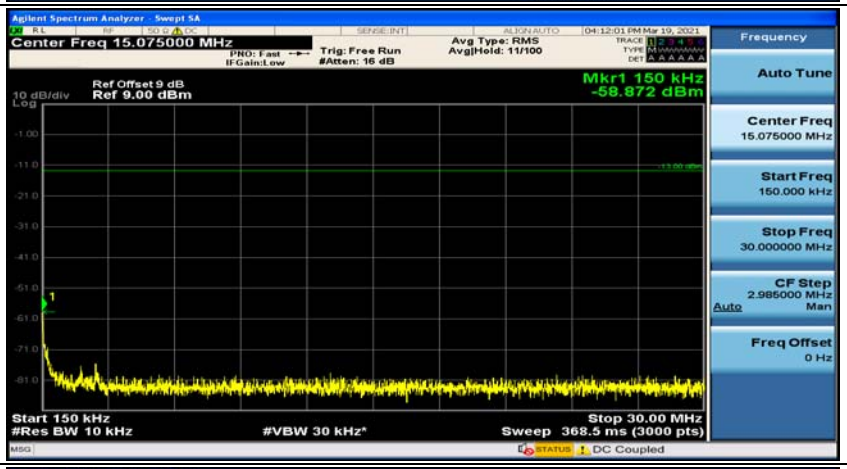
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
04:12:01 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-58.872 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:12:07 PM Mar 19, 2021
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 23.532 GHz
-29.843 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#0
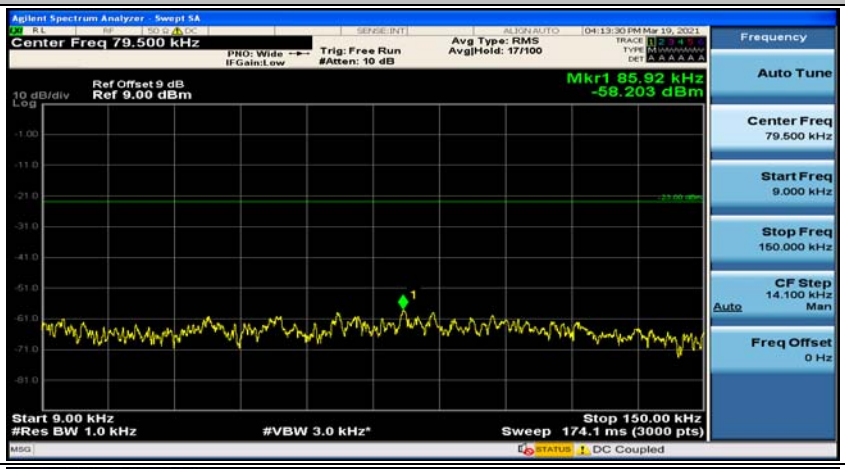
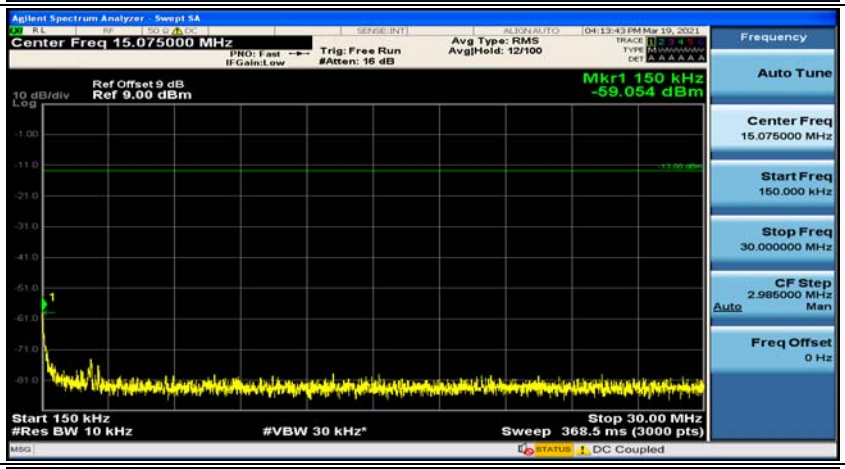
Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#24

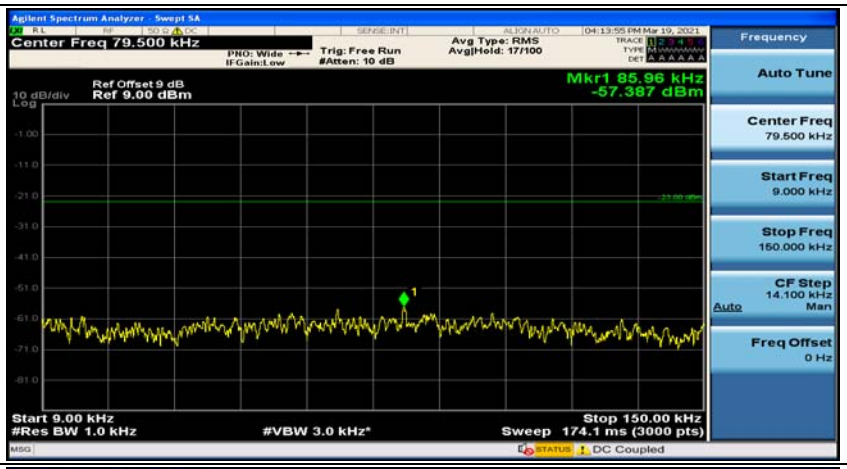

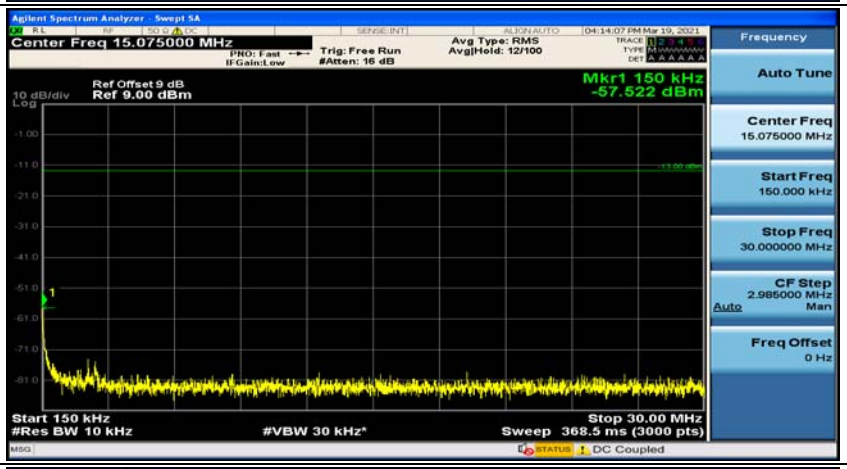

Channel Bandwidth: 10 MHz_HCH_QPSK_1RB#49

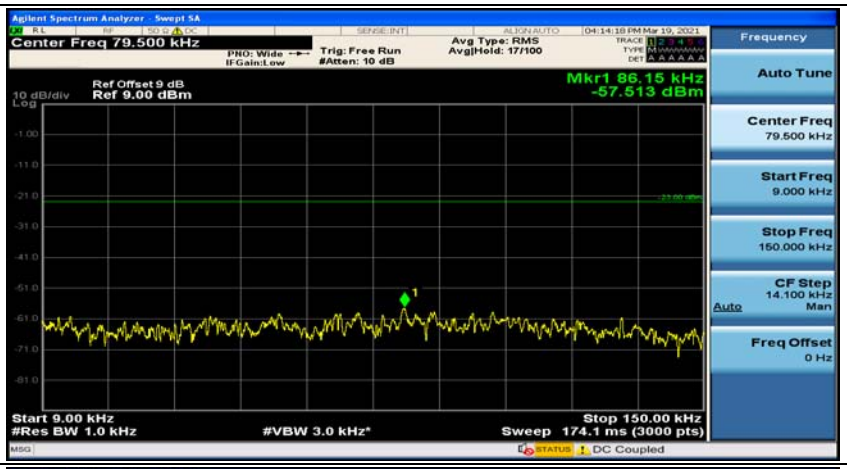
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
04:14:18 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 86.15 kHz
-57.513 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

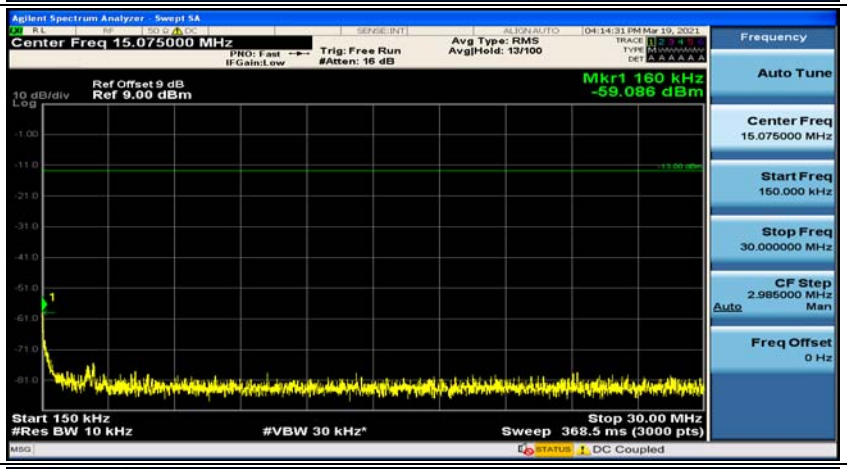
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
04:14:31 PM Mar 19, 2021
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-59.086 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
04:14:36 PM Mar 19, 2021
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.532 GHz
-29.790 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#0
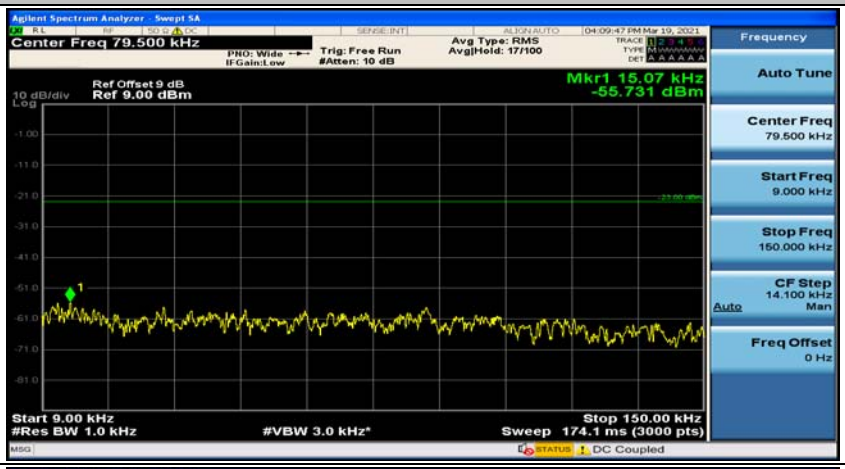
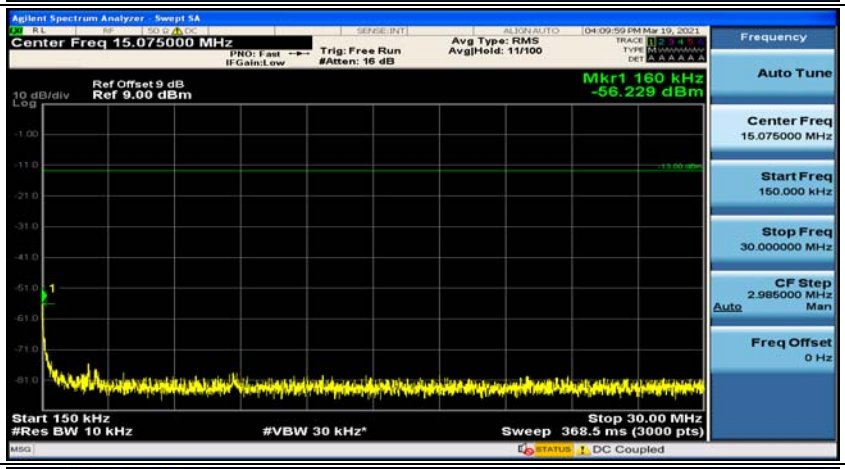
Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#24

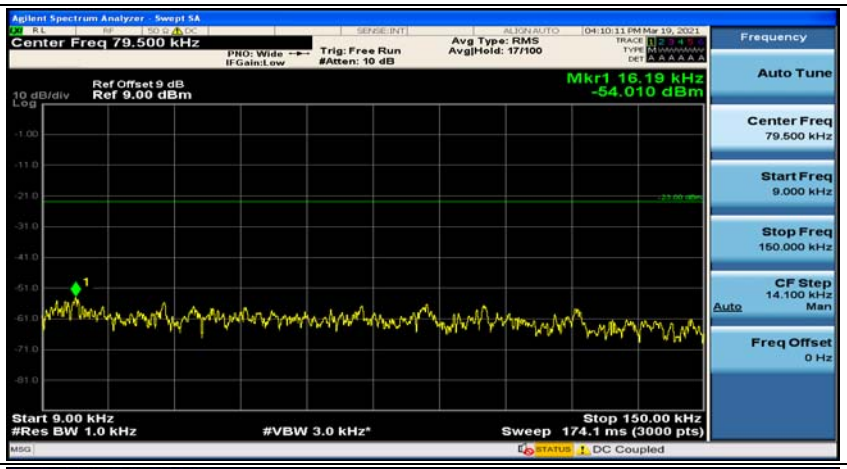

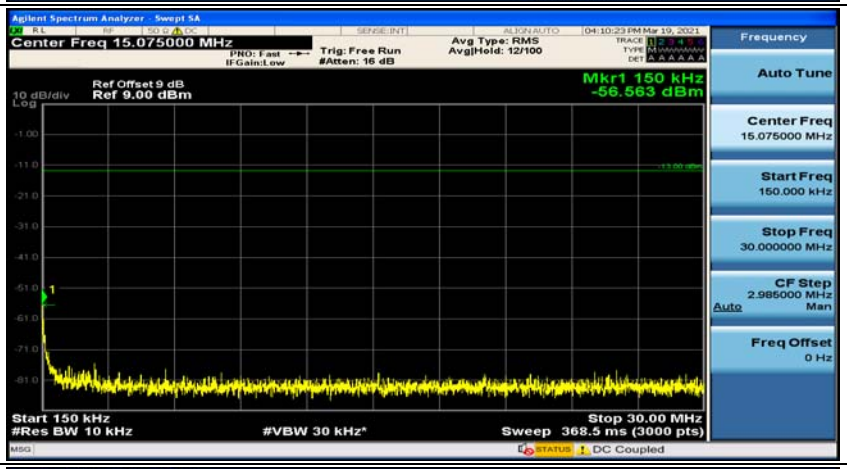

Channel Bandwidth: 10 MHz_LCH_16QAM_1RB#49