

# Test Report No.50121721 001

## Appendix D: Radiated and Mains Spurious Emission Data



(File: 50121721AppendixD)

### Contents



|                                                 |    |
|-------------------------------------------------|----|
| Spurious Emissions, Band Edges, 2.35-2.5G ..... | 2  |
| Spurious Emissions, TX Mode, 1-18G.....         | 6  |
| Spurious Emissions, TX Mode, 18-26G.....        | 12 |
| Spurious Emissions, TX Mode, 30M-1G .....       | 18 |
| Spurious Emissions, TX Mode, 9k-30M .....       | 20 |
| Spurious Emissions, RX Mode, 1-18G .....        | 22 |
| Spurious Emissions, RX Mode, 18-26G .....       | 24 |
| Spurious Emissions, RX Mode, 30M-1G.....        | 26 |
| Spurious Emissions, RX Mode, 9K-30M.....        | 28 |

# Radiated Bandedge (GFSK)

## Low Channel (Hor)

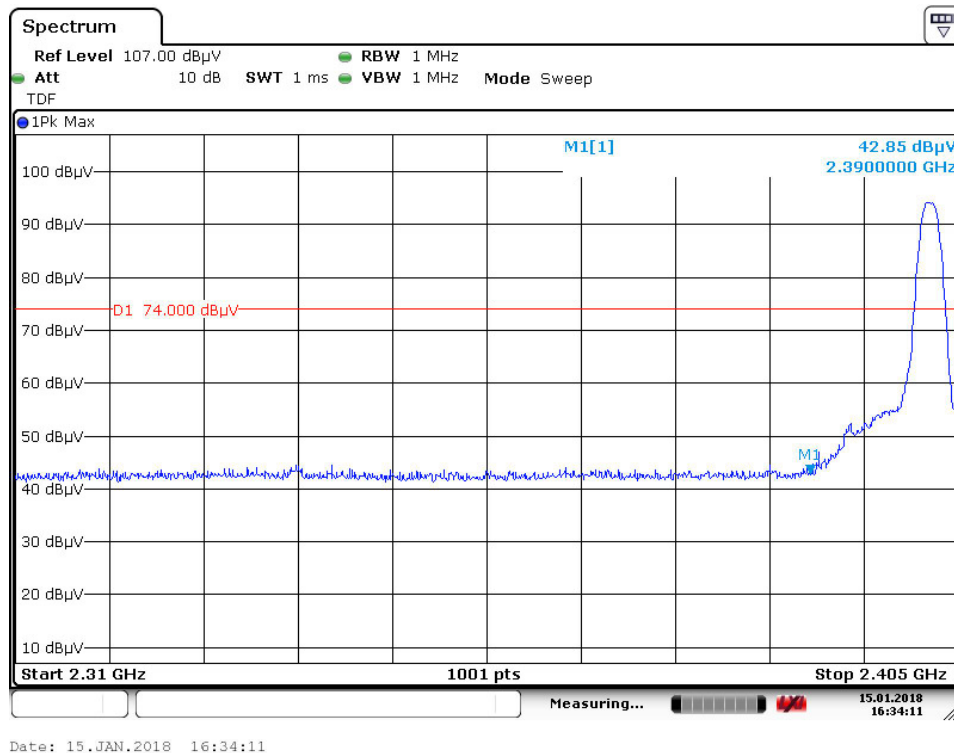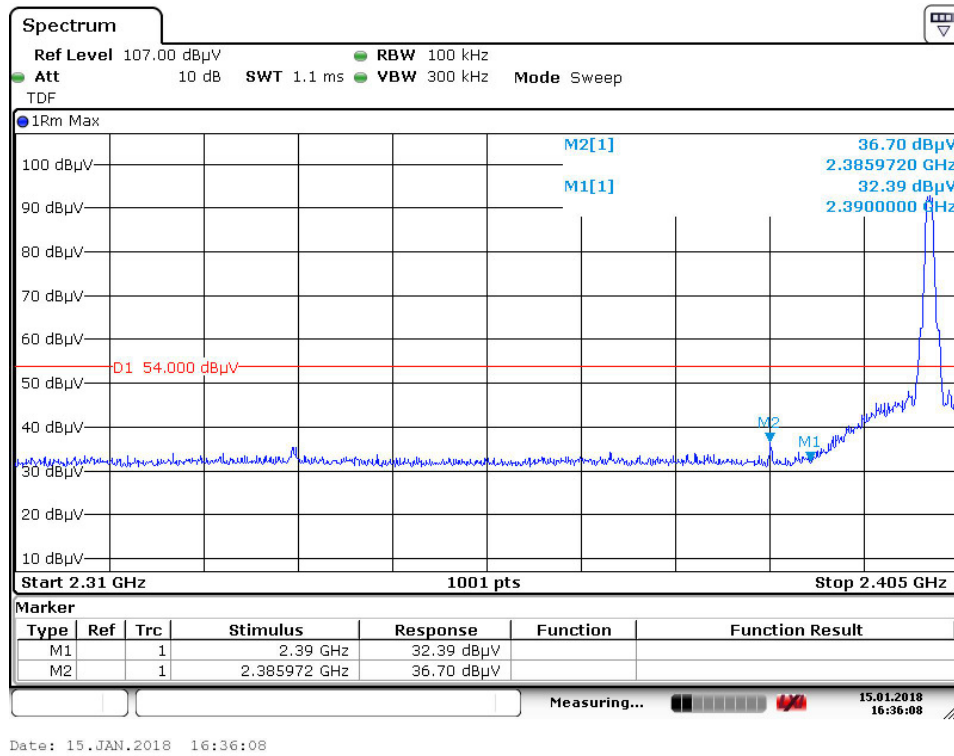



Low Channel (Ver)

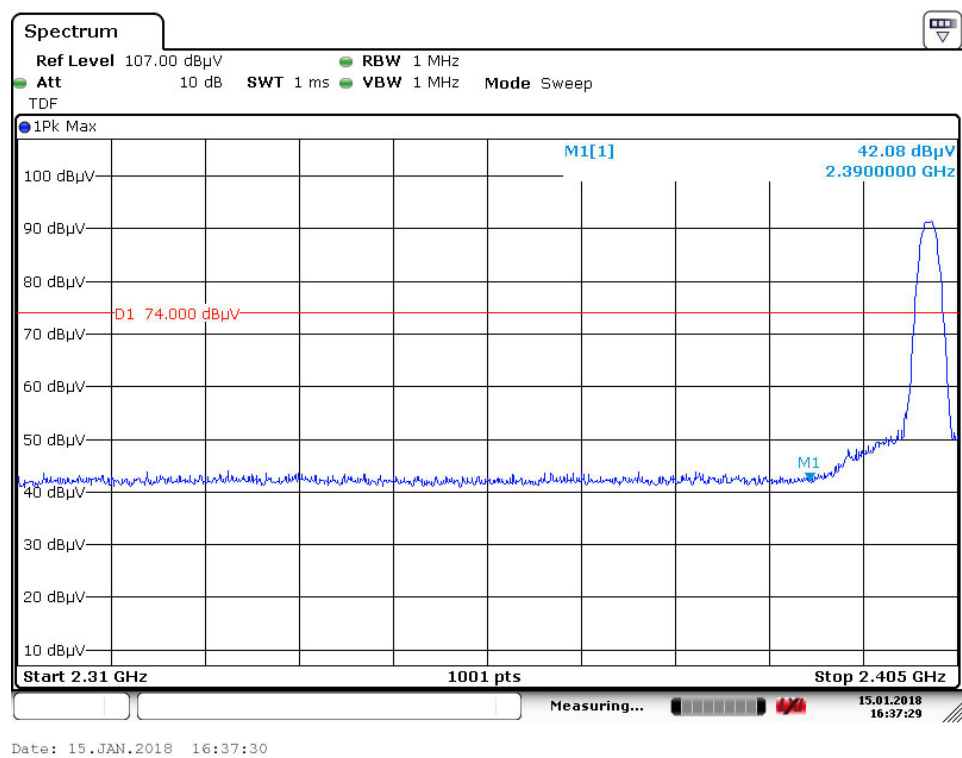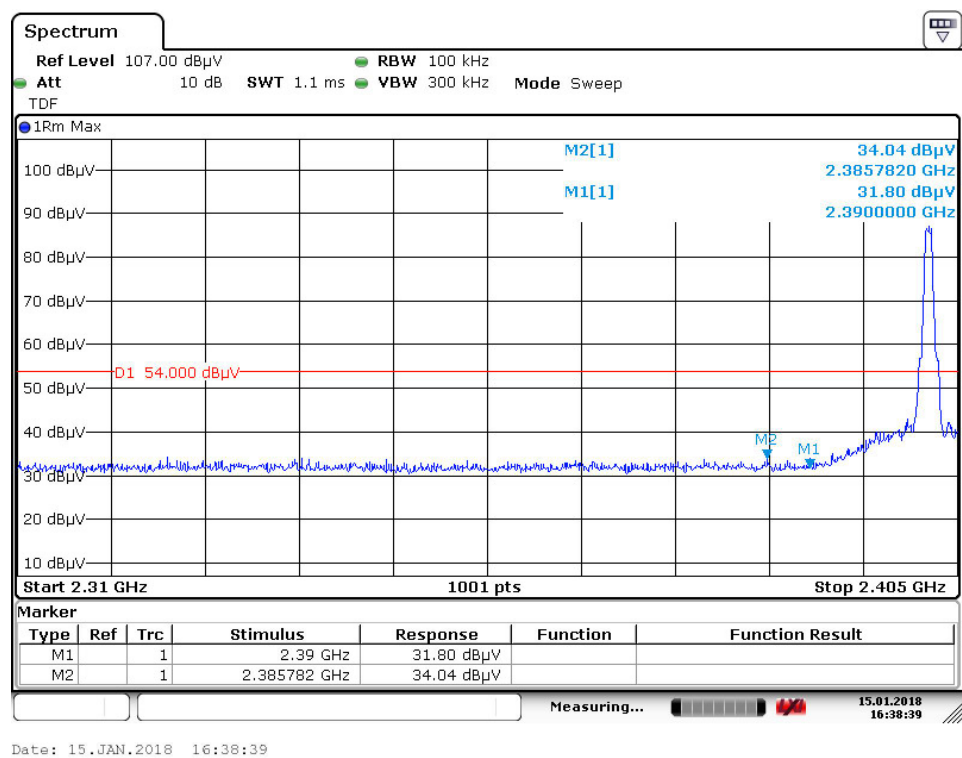

Spurious Emissions, Band Edge, 2.35-2.5G



# Radiated Bandedge (GFSK)

## High Channel (Hor)

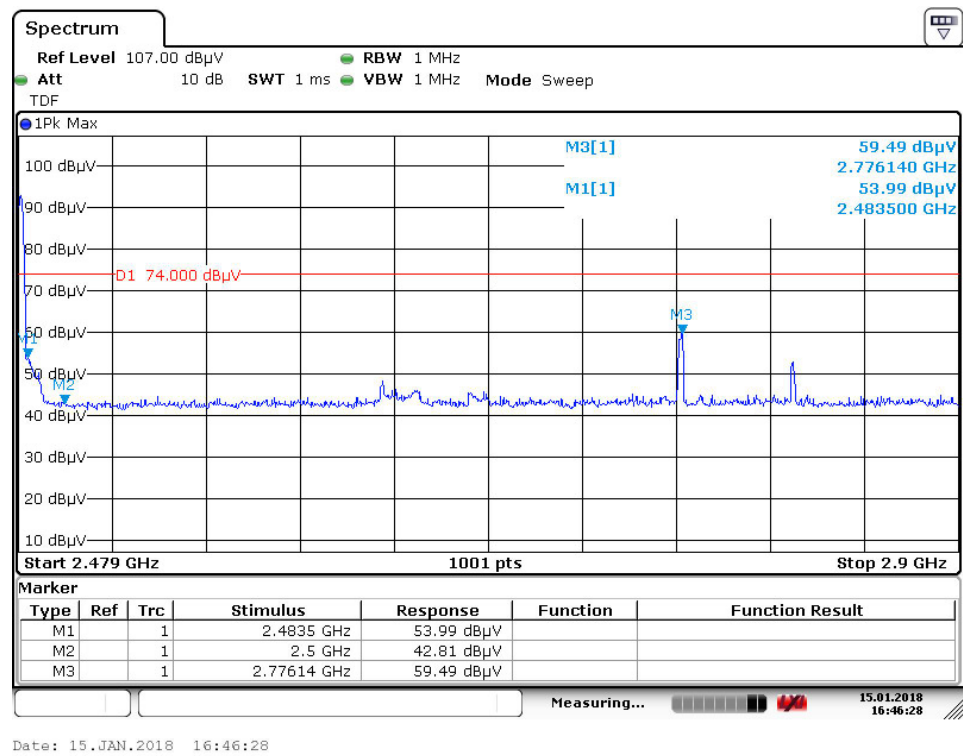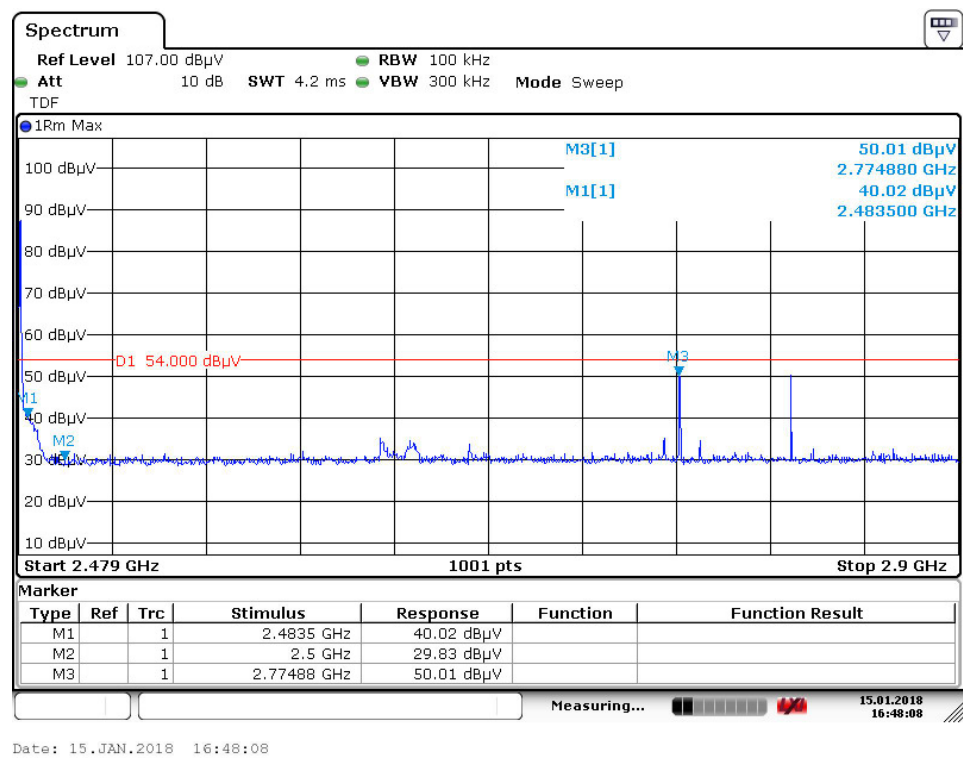

## Spurious Emissions, Band Edge, 2.35-2.5G

High Channel (Ver)

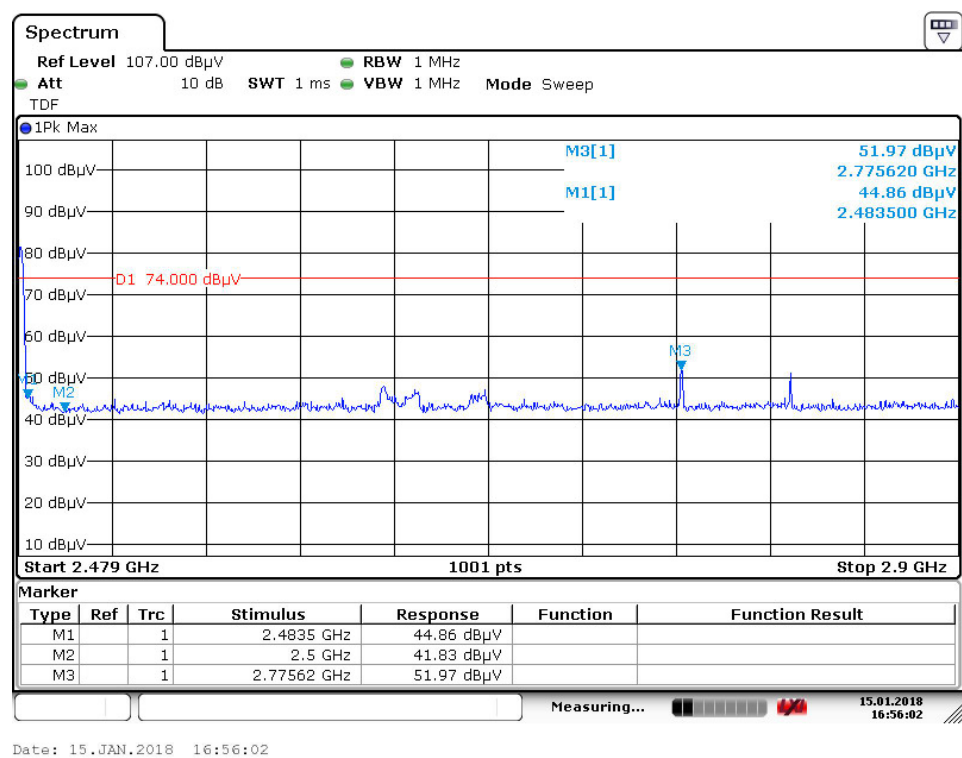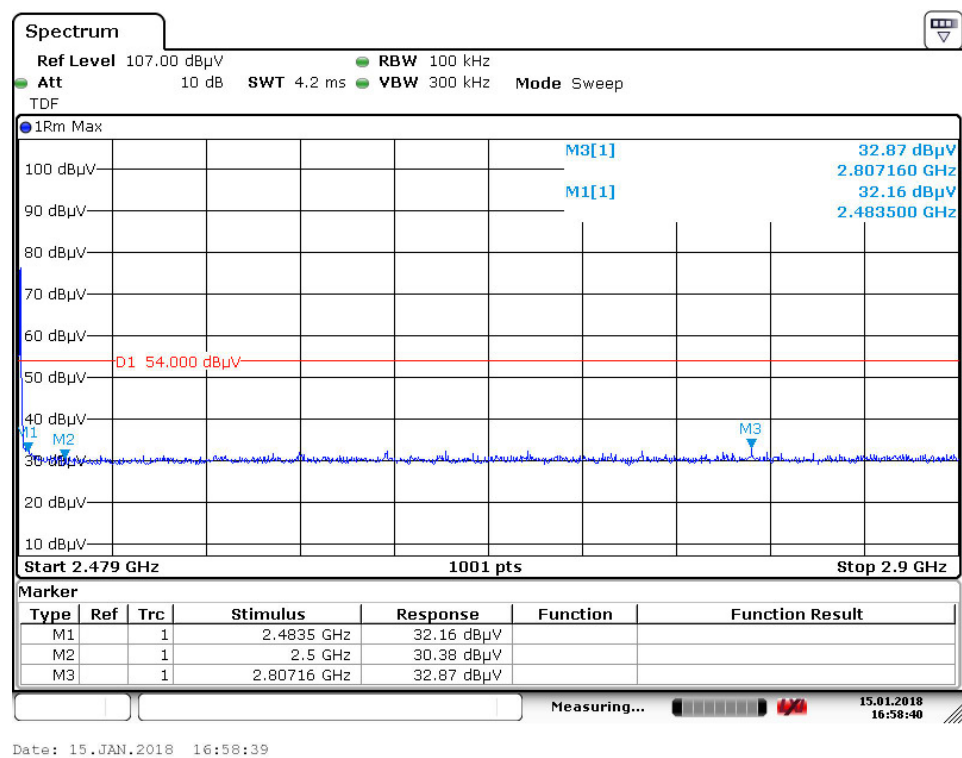

Spurious Emissions, Band Edge, 2.35-2.5G


# Spurious Emissions, TX Mode, 1-18G



**TUV Rheinland Taiwan Ltd.**

11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105


Tel:+886-2172-7000 fax:+886-2528-0018

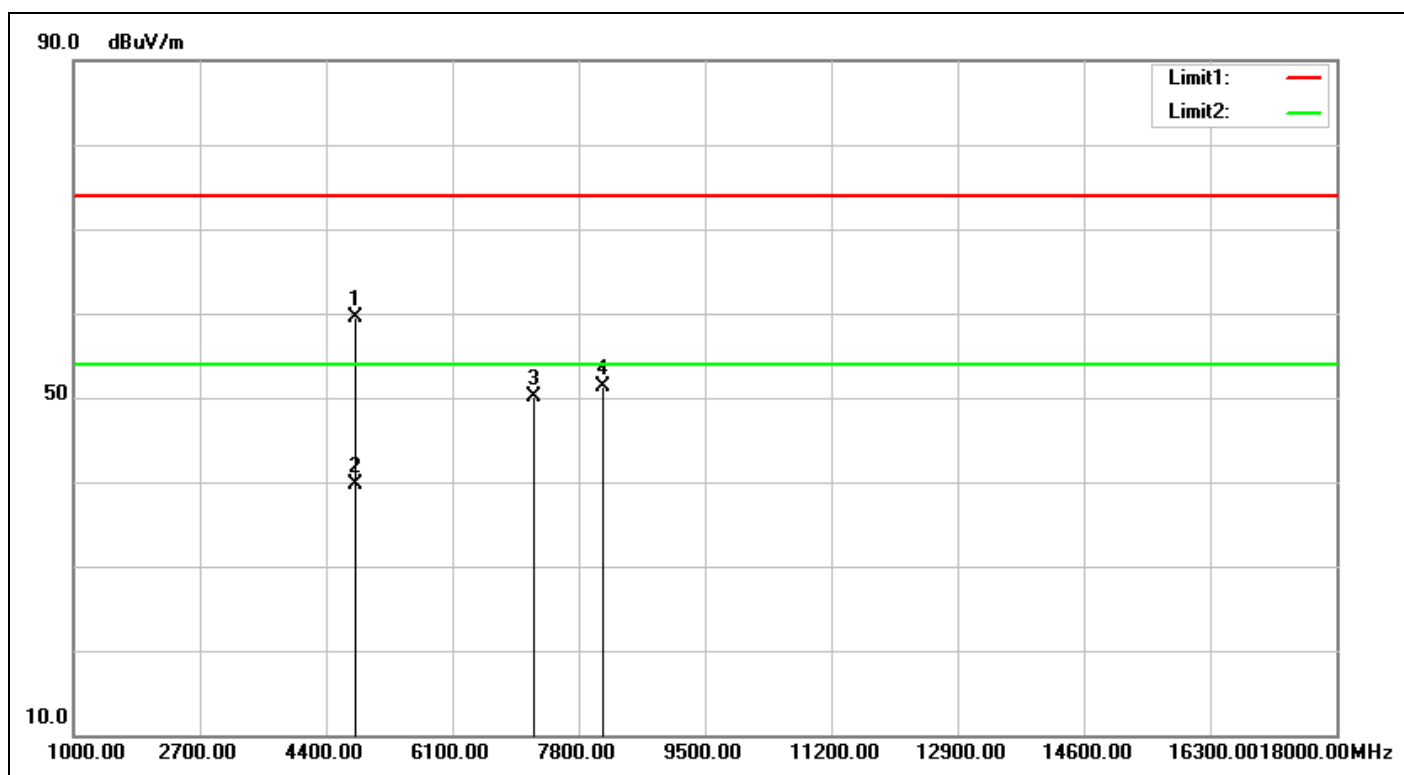

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 17:01:35 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2402-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |


| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 4804.000        | -2.72         | 62.17          | 59.45          | 74.00          | -14.55      | peak | 100         | 178         |        |
| 2   | 4804.000        | -2.72         | 42.38          | 39.66          | 54.00          | -14.34      | AVG  | 100         | 178         |        |
| 3   | 7206.000        | 5.25          | 44.88          | 50.13          | 74.00          | -23.87      | peak |             | 0           |        |
| 4   | 8123.000        | 5.96          | 45.28          | 51.24          | 74.00          | -22.76      | peak | 100         | 78          |        |

# Spurious Emissions, TX Mode, 1-18G

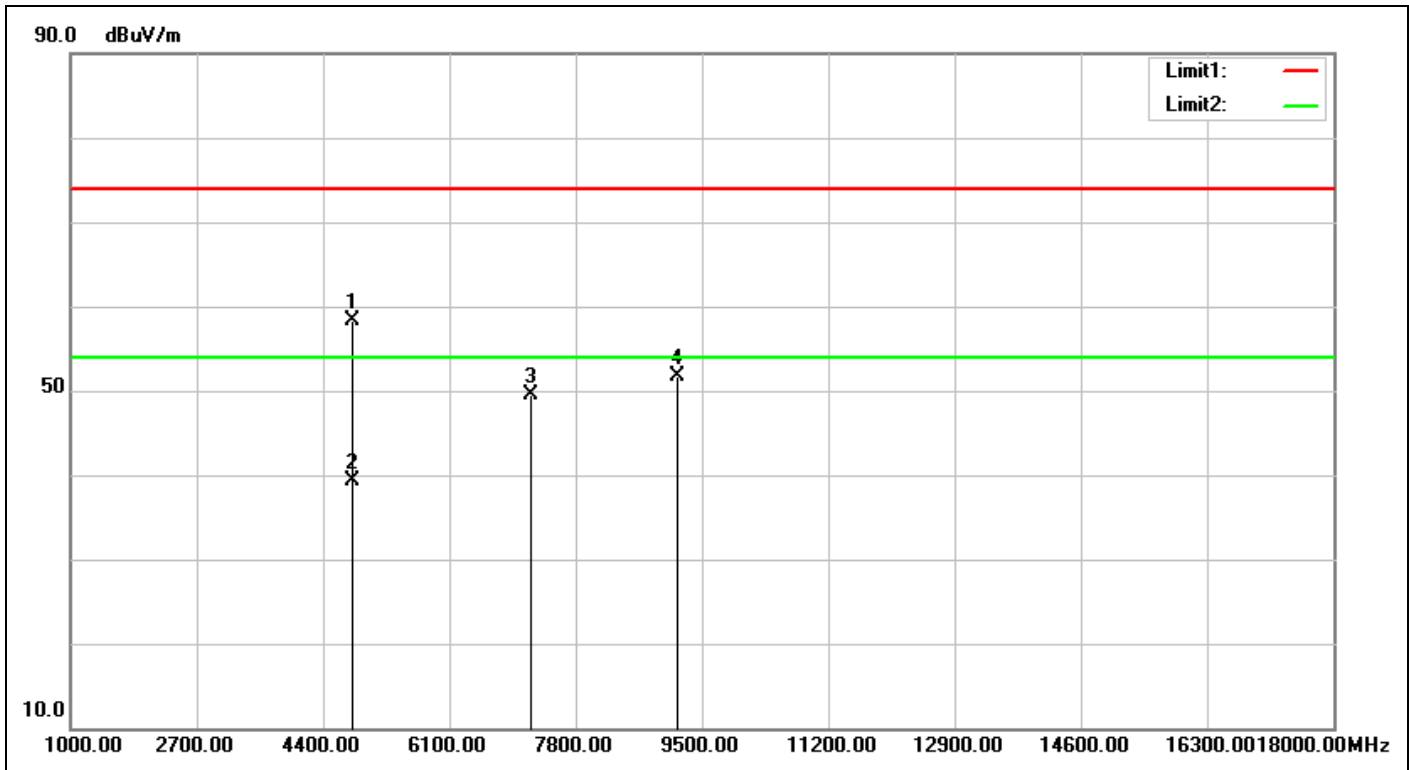


|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:02:38</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65 %</b>        |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2402-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 4804.000        | -2.72         | 61.01          | 58.29          | 74.00          | -15.71      | peak | 100         | 229           |        |
| 2   | 4804.000        | -2.72         | 42.06          | 39.34          | 54.00          | -14.66      | AVG  | 100         | 229           |        |
| 3   | 7206.000        | 5.25          | 44.28          | 49.53          | 74.00          | -24.47      | peak |             |               |        |
| 4   | 9160.000        | 6.48          | 45.17          | 51.65          | 74.00          | -22.35      | peak | 100         | 213           |        |

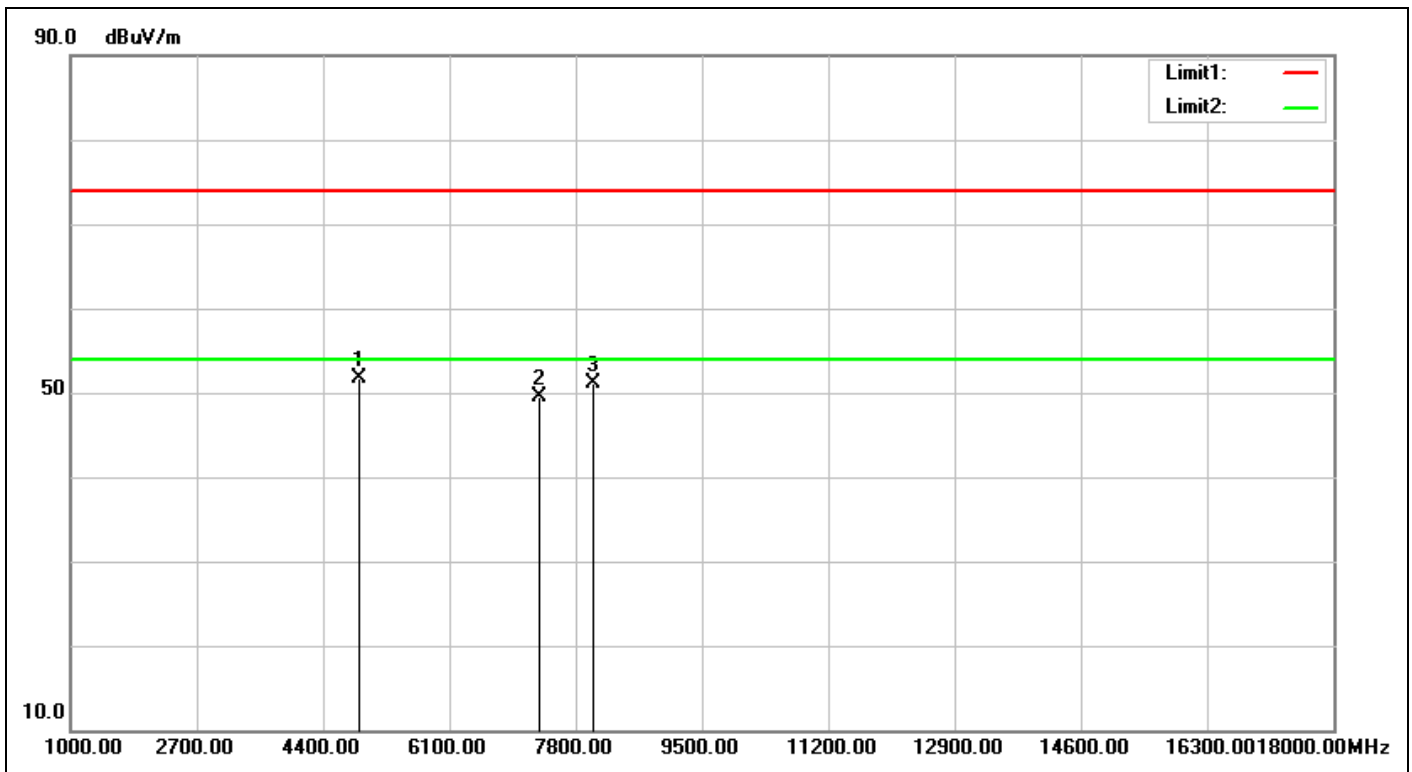


|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Horizontal</b>         |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:11:11</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 4880.000        | -2.50         | 54.25          | 51.75          | 74.00          | -22.25      | peak | 100         | 167           |        |
| 2   | 7320.000        | 5.54          | 44.02          | 49.56          | 74.00          | -24.44      | peak |             |               |        |
| 3   | 8038.000        | 5.86          | 45.27          | 51.13          | 74.00          | -22.87      | peak | 100         | 114           |        |

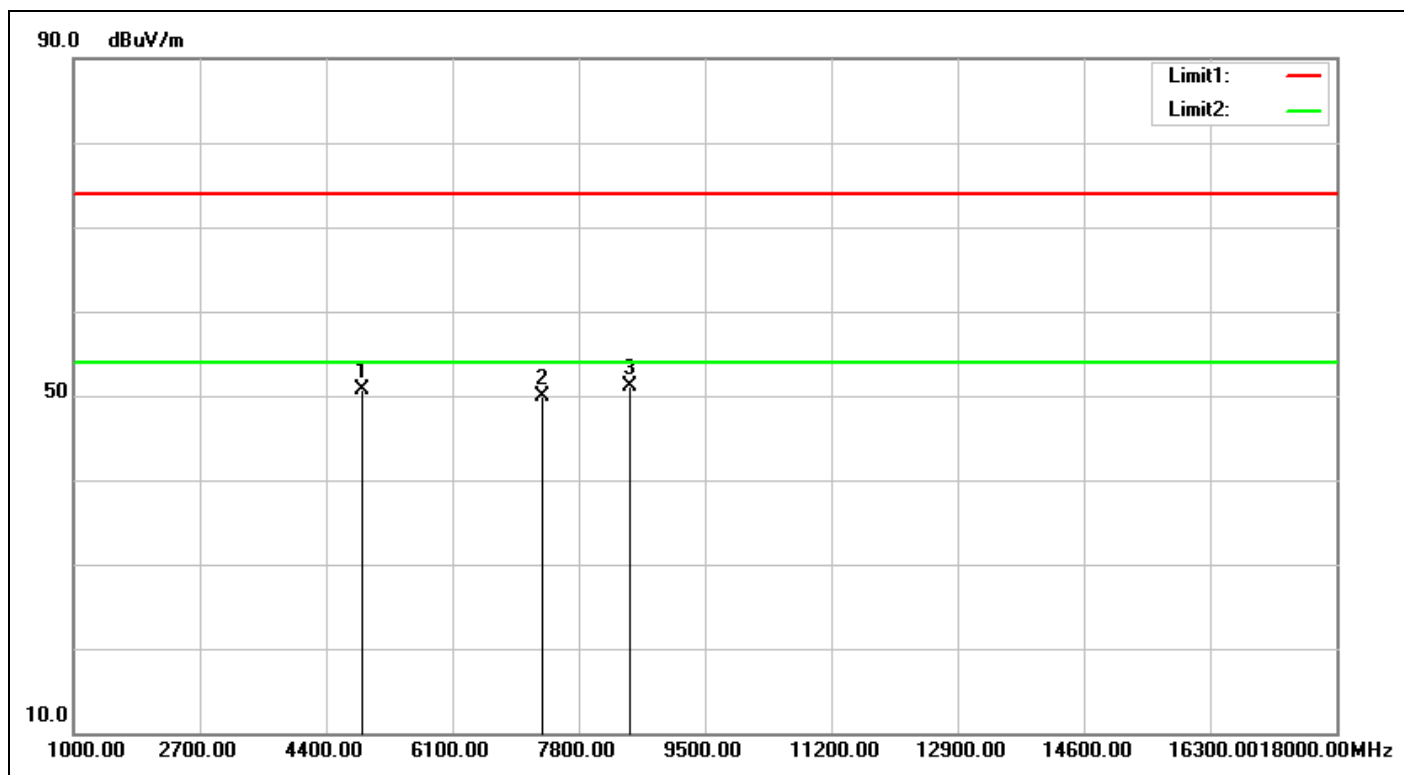


|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:12:14</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 4880.000        | -2.50         | 53.12          | 50.62          | 74.00          | -23.38      | peak | 100         | 3             |        |
| 2   | 7320.000        | 5.54          | 44.38          | 49.92          | 74.00          | -24.08      | peak |             |               |        |
| 3   | 8480.000        | 6.35          | 44.75          | 51.10          | 74.00          | -22.90      | peak | 100         | 146           |        |

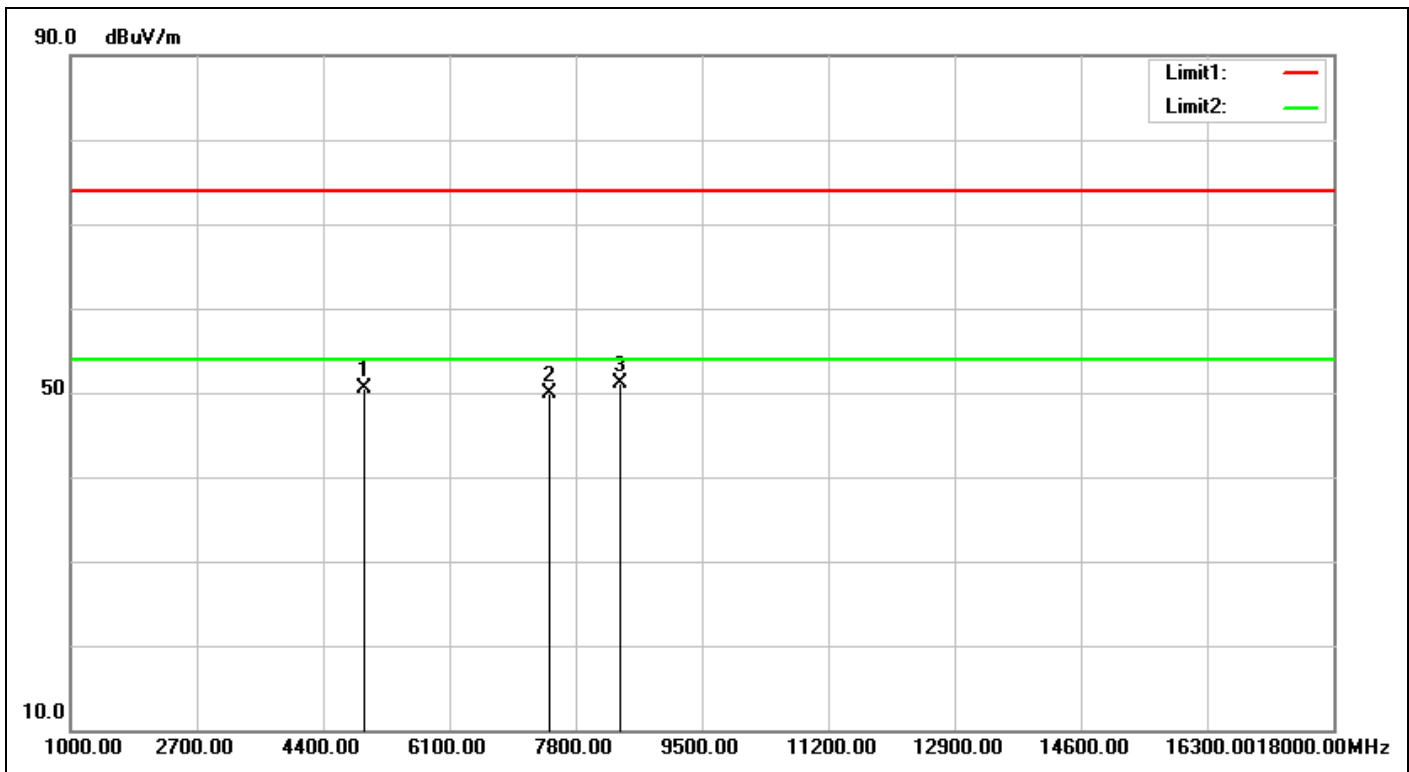

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Horizontal</b>         |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:16:12</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65 %</b>        |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2480-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 4960.000        | -2.28         | 52.70          | 50.42          | 74.00          | -23.58      | peak | 100         | 78            |        |
| 2   | 7440.000        | 5.84          | 44.09          | 49.93          | 74.00          | -24.07      | peak |             |               |        |
| 3   | 8395.000        | 6.26          | 44.93          | 51.19          | 74.00          | -22.81      | peak | 100         | 0             |        |

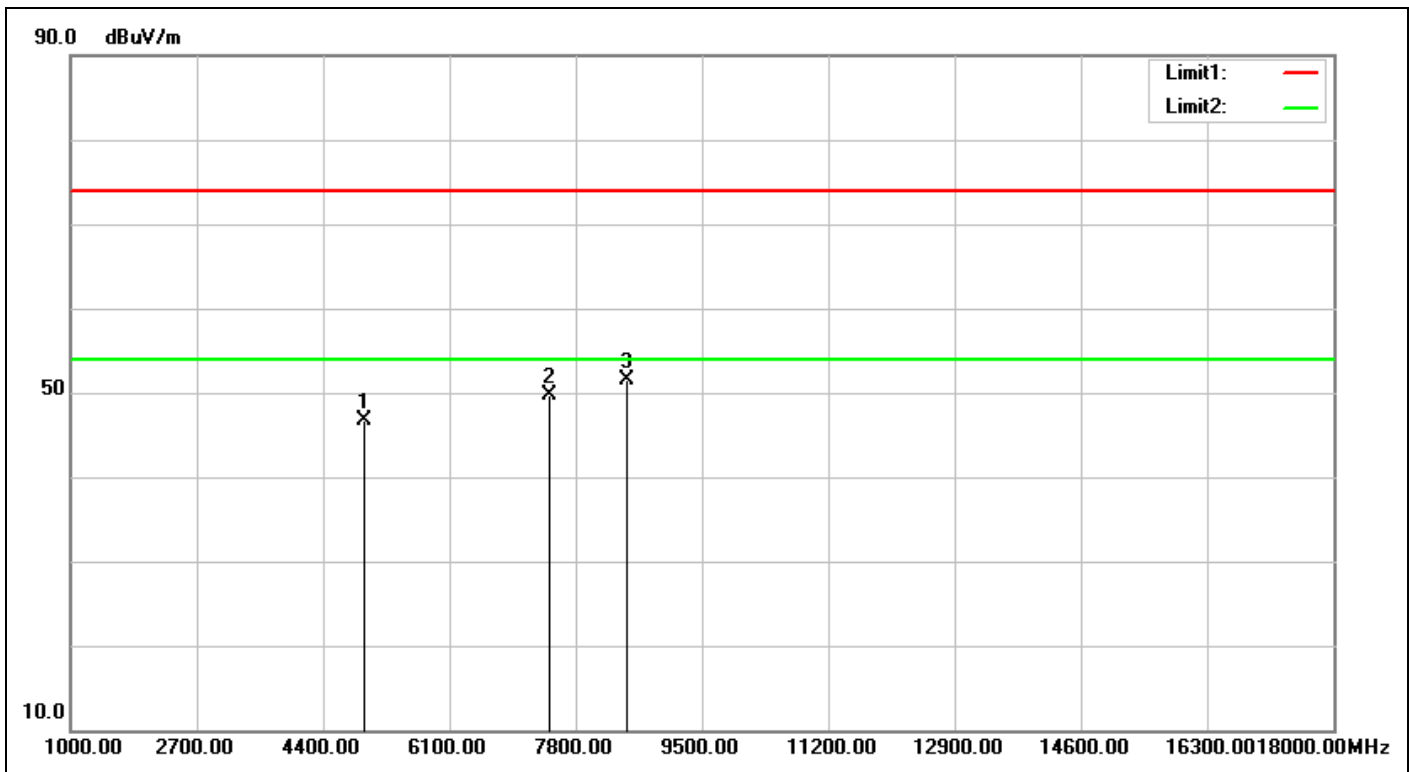

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:17:15</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2480-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 4960.000        | -2.28         | 48.98          | 46.70          | 74.00          | -27.30      | peak |             |               |        |
| 2   | 7440.000        | 5.84          | 43.91          | 49.75          | 74.00          | -24.25      | peak |             |               |        |
| 3   | 8480.000        | 6.35          | 45.19          | 51.54          | 74.00          | -22.46      | peak | 100         | 265           |        |


# Spurious Emissions, TX Mode, 18-26G



**TUV Rheinland Taiwan Ltd.**


11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105

Tel:+886-2172-7000 fax:+886-2528-0018

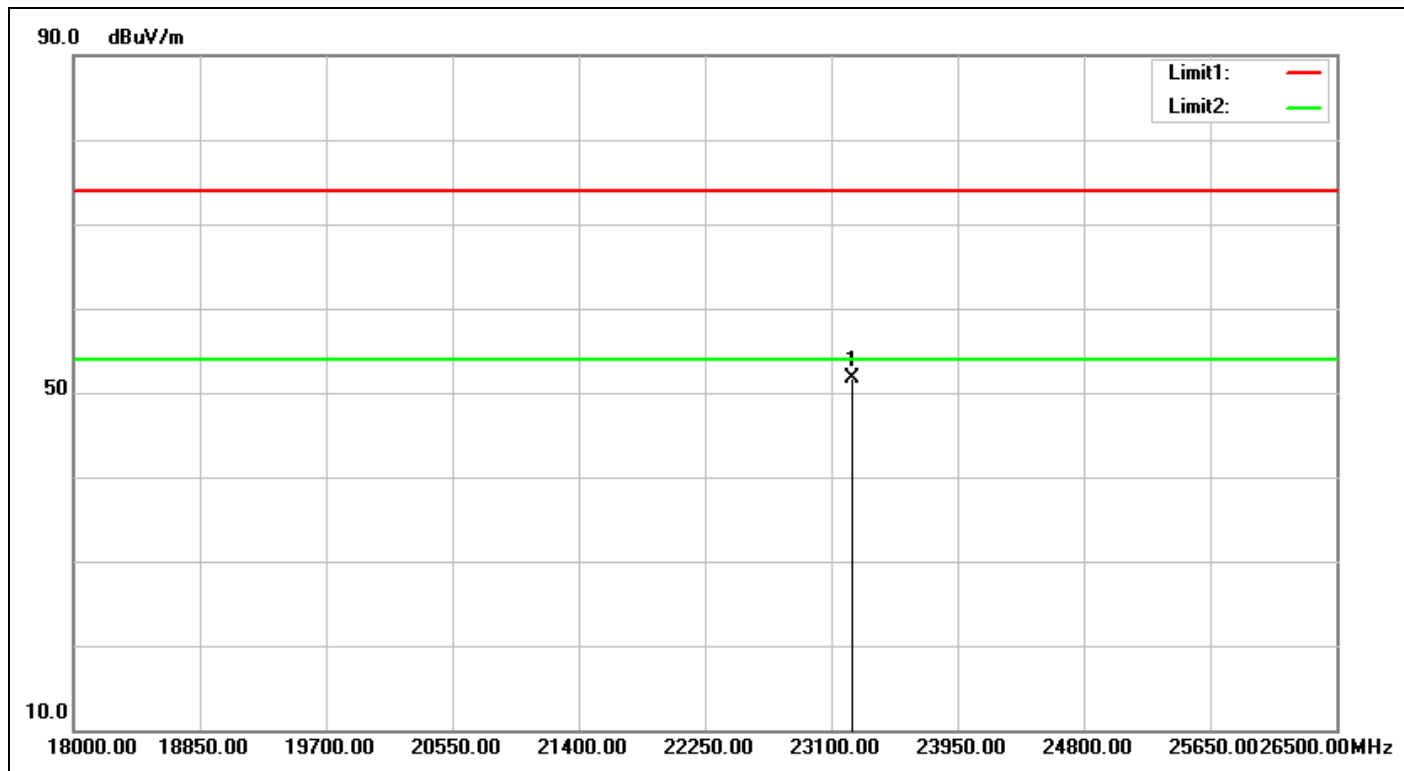


|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 18:55:16 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2402-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 23244.500       | 33.61         | 18.05          | 51.66          | 74.00          | -22.34      | peak |             | 0           |        |

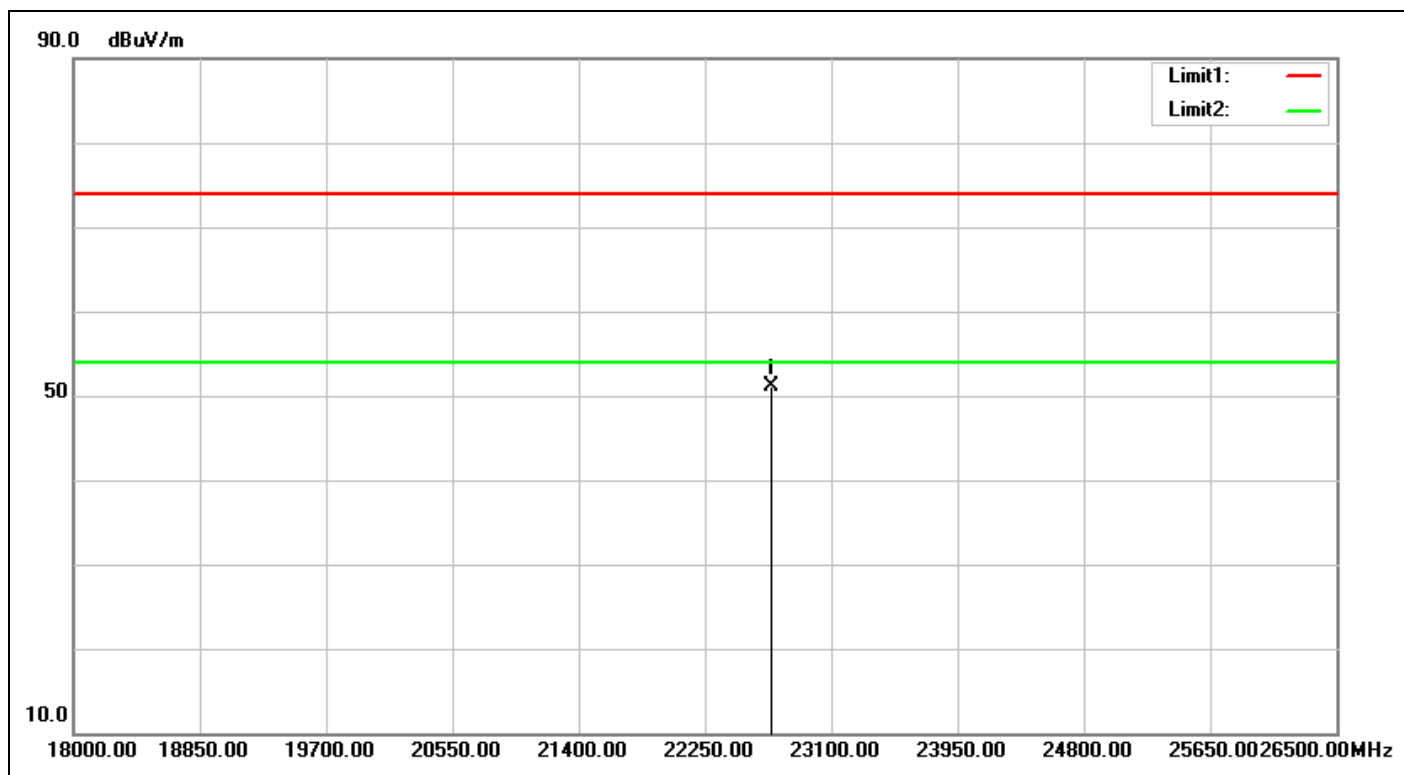


|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Vertical           |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 18:56:26 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2402-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 22692.000       | 33.26         | 17.90          | 51.16          | 74.00          | -22.84      | peak |             |               |        |

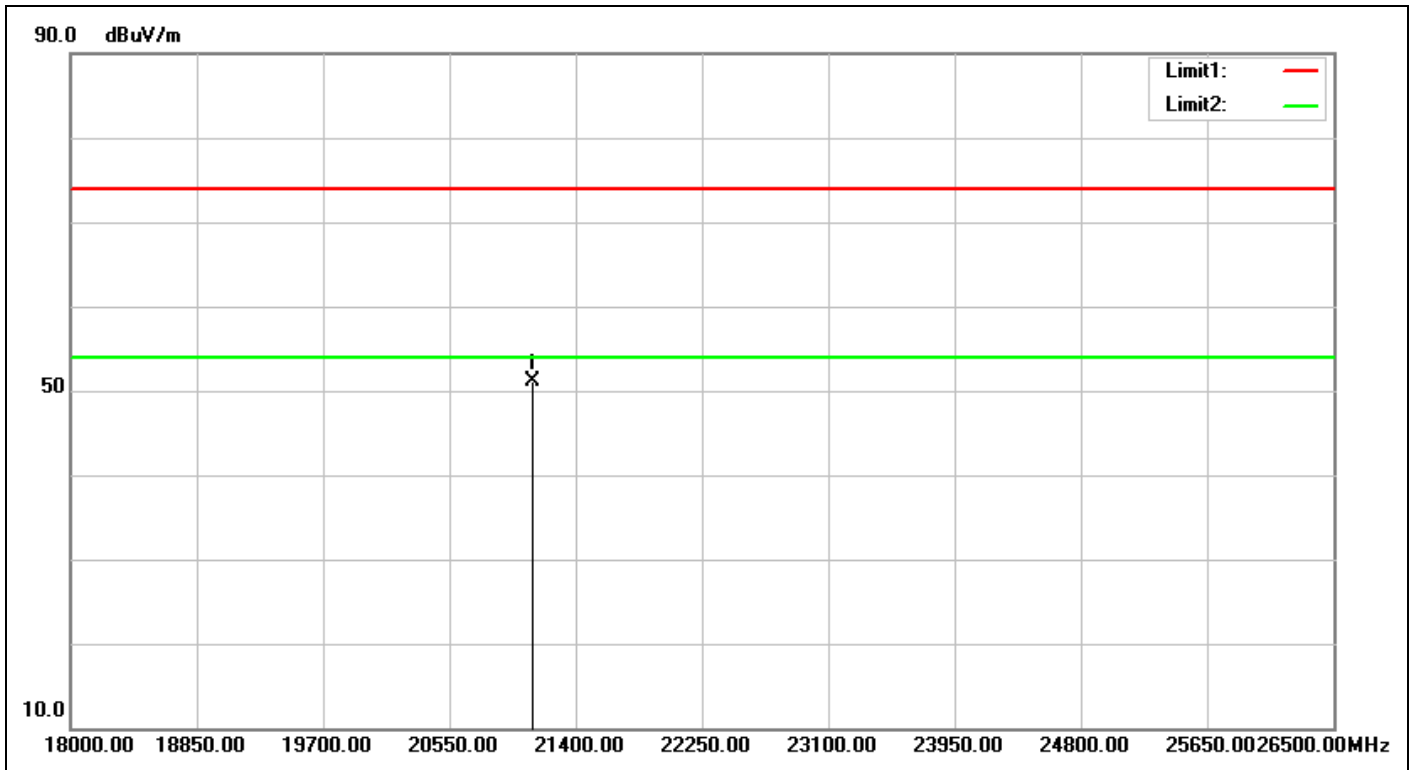


|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Horizontal</b>         |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 18:56:55</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65 %</b>        |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 21111.000       | 33.08         | 18.12          | 51.20          | 74.00          | -22.80      | peak |             |               |        |

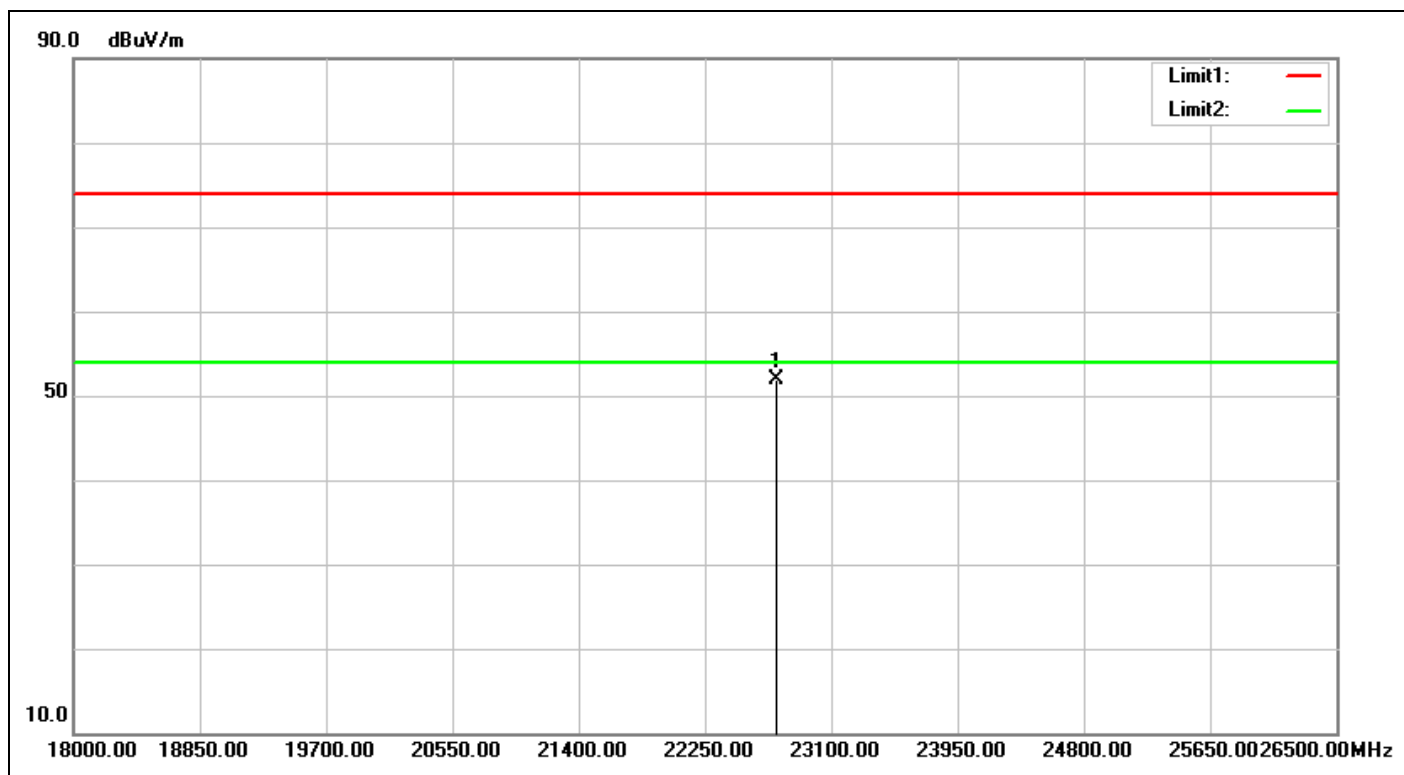


|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Vertical           |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 18:57:15 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 22734.500       | 33.27         | 18.56          | 51.83          | 74.00          | -22.17      | peak |             |               |        |

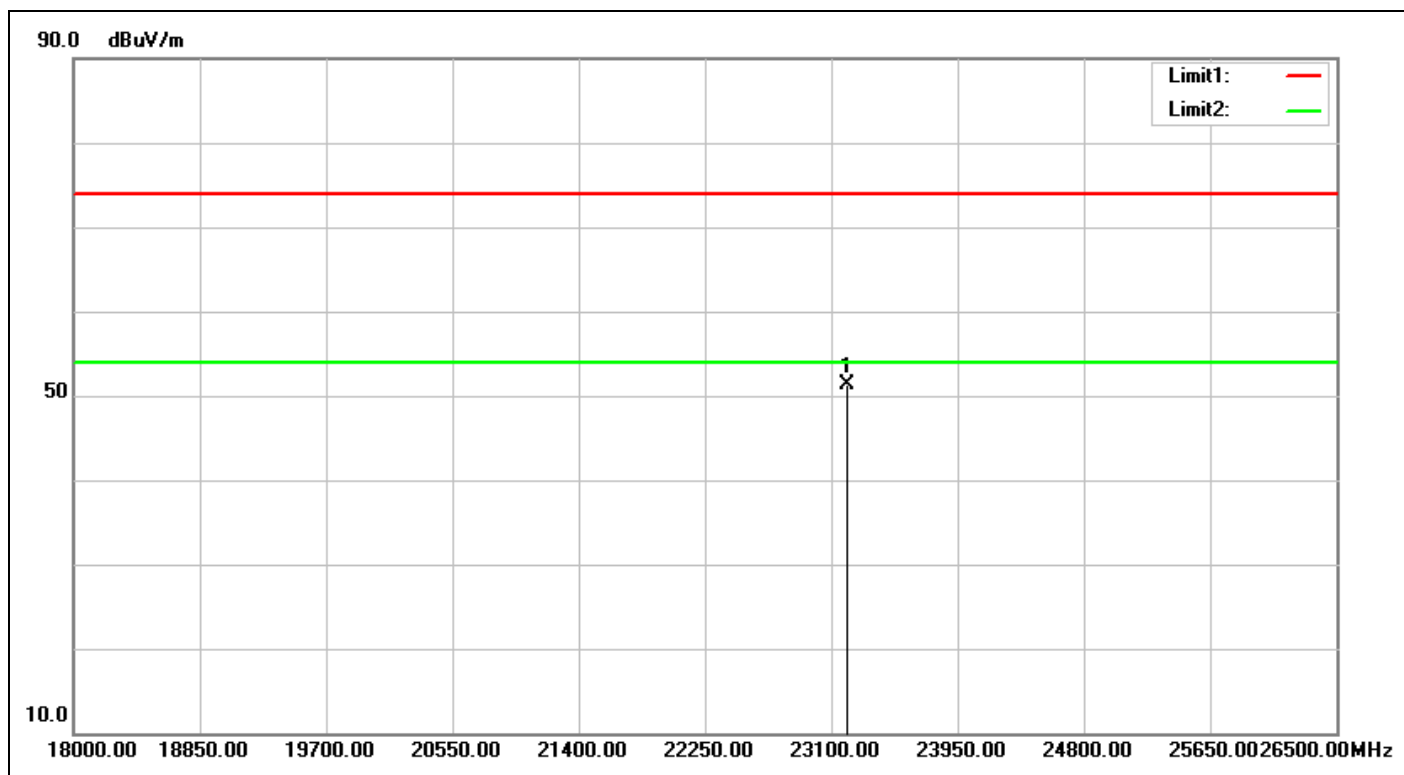

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 18:57:40 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2480-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 23202.000       | 33.57         | 17.66          | 51.23          | 74.00          | -22.77      | peak |             |               |        |

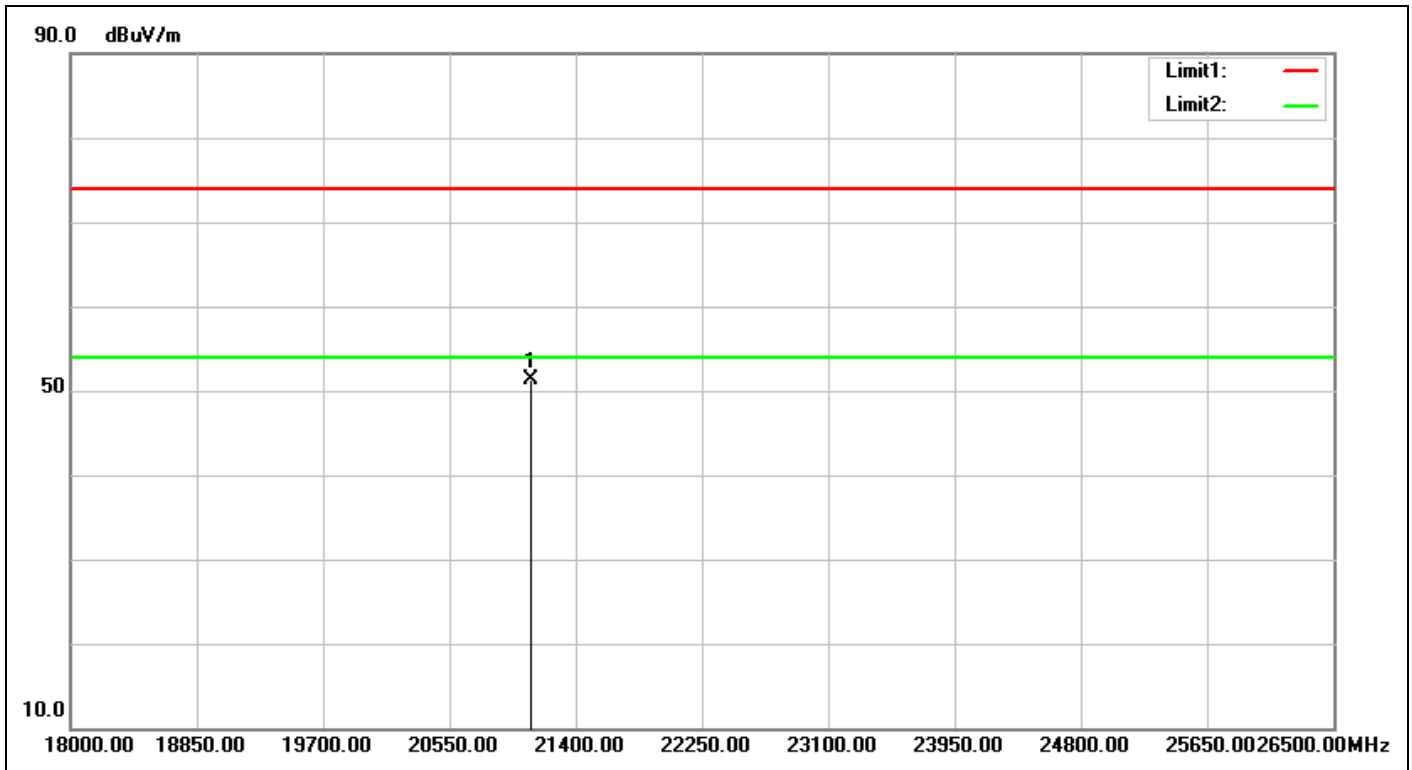

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 18:58:03</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65 %</b>        |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2480-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 21102.500       | 33.07         | 18.27          | 51.34          | 74.00          | -22.66      | peak |             |               |        |


# Spurious Emissions, TX Mode, 30M-1G



**TUV Rheinland Taiwan Ltd.**

11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105


Tel:+886-2172-7000 fax:+886-2528-0018

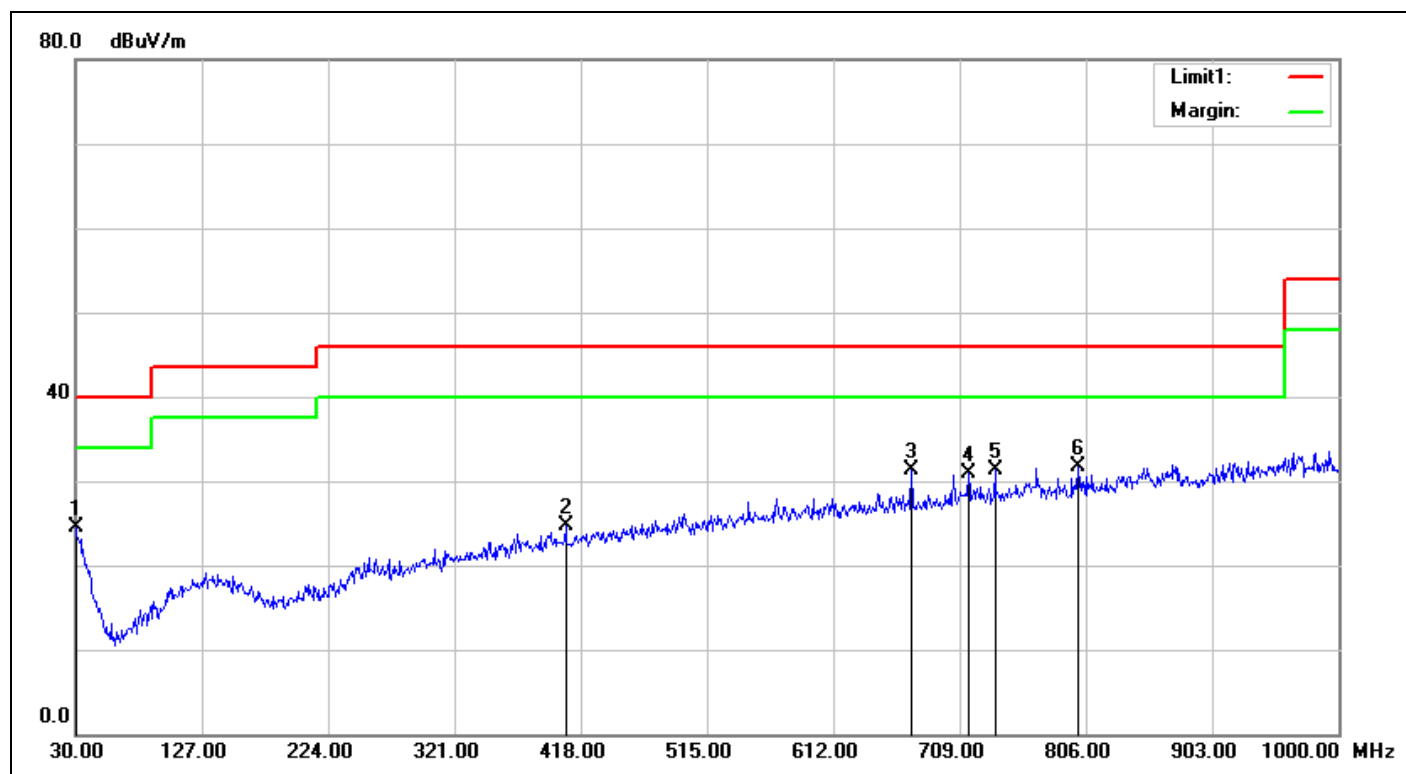

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Class B 3M Radiation                  | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 20:19:58 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 30.0000         | -0.25         | 24.82          | 24.57          | 40.00          | -15.43      | QP   | 100         | 155         |        |
| 2   | 406.3600        | -2.37         | 27.06          | 24.69          | 46.00          | -21.31      | QP   | 100         | 309         |        |
| 3   | 672.1400        | 0.85          | 30.46          | 31.31          | 46.00          | -14.69      | QP   | 100         | 75          |        |
| 4   | 715.7900        | 1.62          | 29.27          | 30.89          | 46.00          | -15.11      | QP   | 100         | 158         |        |
| 5   | 736.1600        | 2.06          | 29.30          | 31.36          | 46.00          | -14.64      | QP   | 100         | 248         |        |
| 6   | 800.1799        | 2.77          | 28.89          | 31.66          | 46.00          | -14.34      | QP   | 100         | 272         |        |

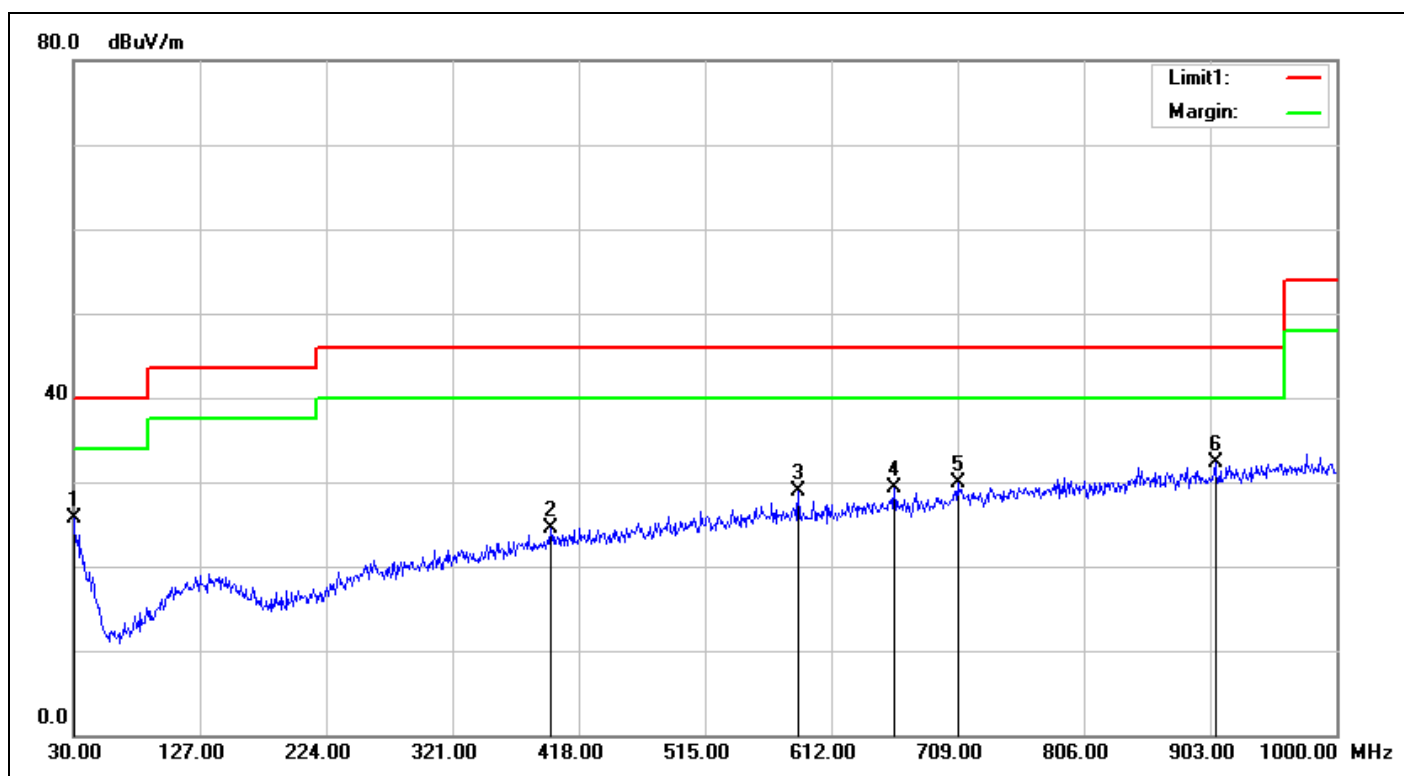

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Class B 3M Radiation                  | Ant. Polarization: | Vertical           |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 20:21:02 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 30.0000         | -0.25         | 25.93          | 25.68          | 40.00          | -14.32      | QP   | 100         | 274         |        |
| 2   | 396.6600        | -2.49         | 26.94          | 24.45          | 46.00          | -21.55      | QP   | 100         | 317         |        |
| 3   | 586.7800        | -0.06         | 28.92          | 28.86          | 46.00          | -17.14      | QP   | 100         | 346         |        |
| 4   | 660.5000        | 0.69          | 28.52          | 29.21          | 46.00          | -16.79      | QP   | 100         | 131         |        |
| 5   | 709.0000        | 1.47          | 28.49          | 29.96          | 46.00          | -16.04      | QP   | 100         | 11          |        |
| 6   | 906.8800        | 4.26          | 27.99          | 32.25          | 46.00          | -13.75      | QP   | 100         | 0           |        |


# Spurious Emissions, TX Mode, 9k-30M



**TUV Rheinland Taiwan Ltd.**

11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105


Tel:+886-2172-7000 fax:+886-2528-0018

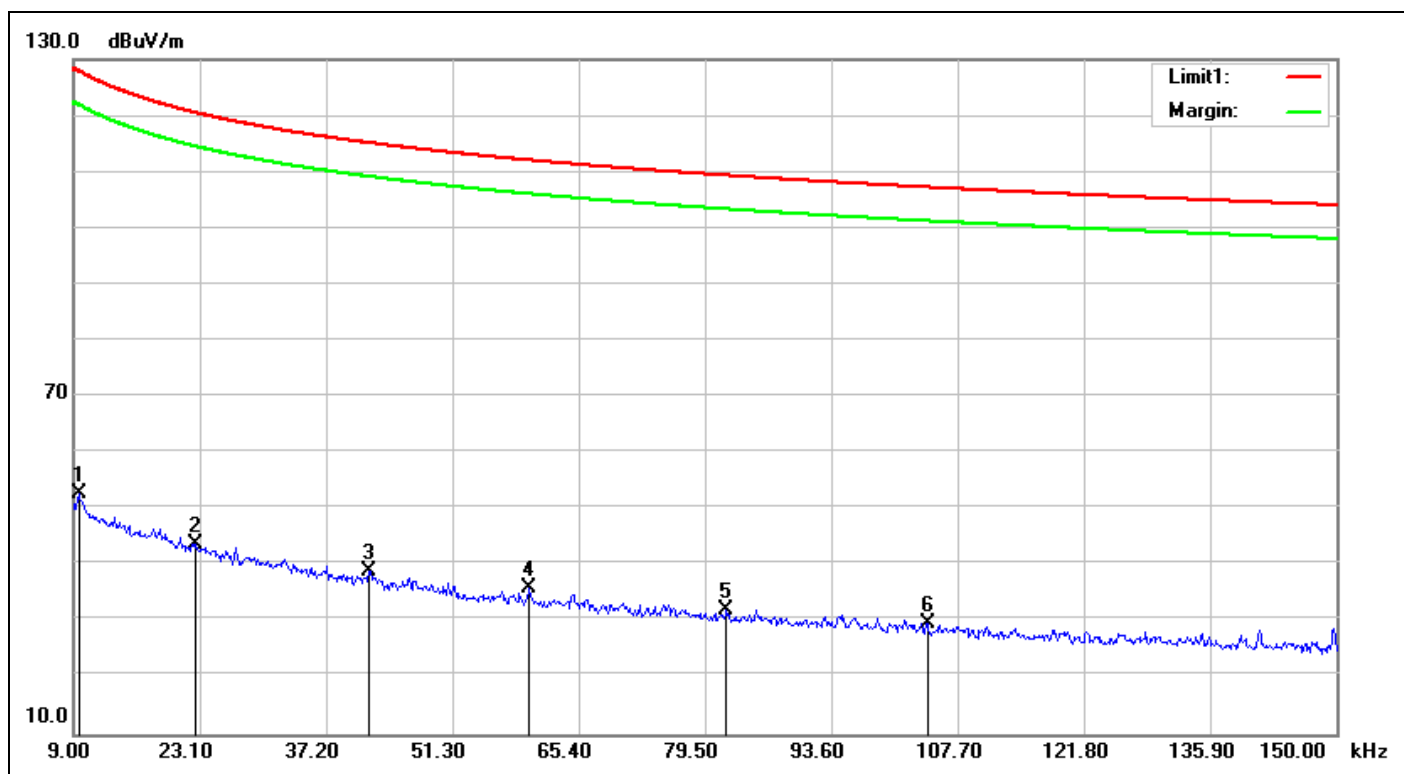

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC2.8_9k-1G_3m                           | Ant. Polarization: |                    |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 20:43:27 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-TX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 0.0095          | 19.73         | 32.88          | 52.61          | 128.03         | -75.42      | QP   | 100         | 272         |        |
| 2   | 0.0226          | 20.06         | 23.67          | 43.73          | 120.51         | -76.78      | QP   | 100         | 352         |        |
| 3   | 0.0419          | 19.71         | 19.22          | 38.93          | 115.15         | -76.22      | QP   | 100         | 27          |        |
| 4   | 0.0599          | 19.37         | 16.64          | 36.01          | 112.05         | -76.04      | QP   | 100         | 163         |        |
| 5   | 0.0818          | 19.24         | 12.83          | 32.07          | 109.34         | -77.27      | QP   | 100         | 189         |        |
| 6   | 0.1043          | 19.13         | 10.60          | 29.73          | 107.23         | -77.50      | QP   | 100         | 128         |        |

## Spurious Emissions, TX Mode, 9k-30M

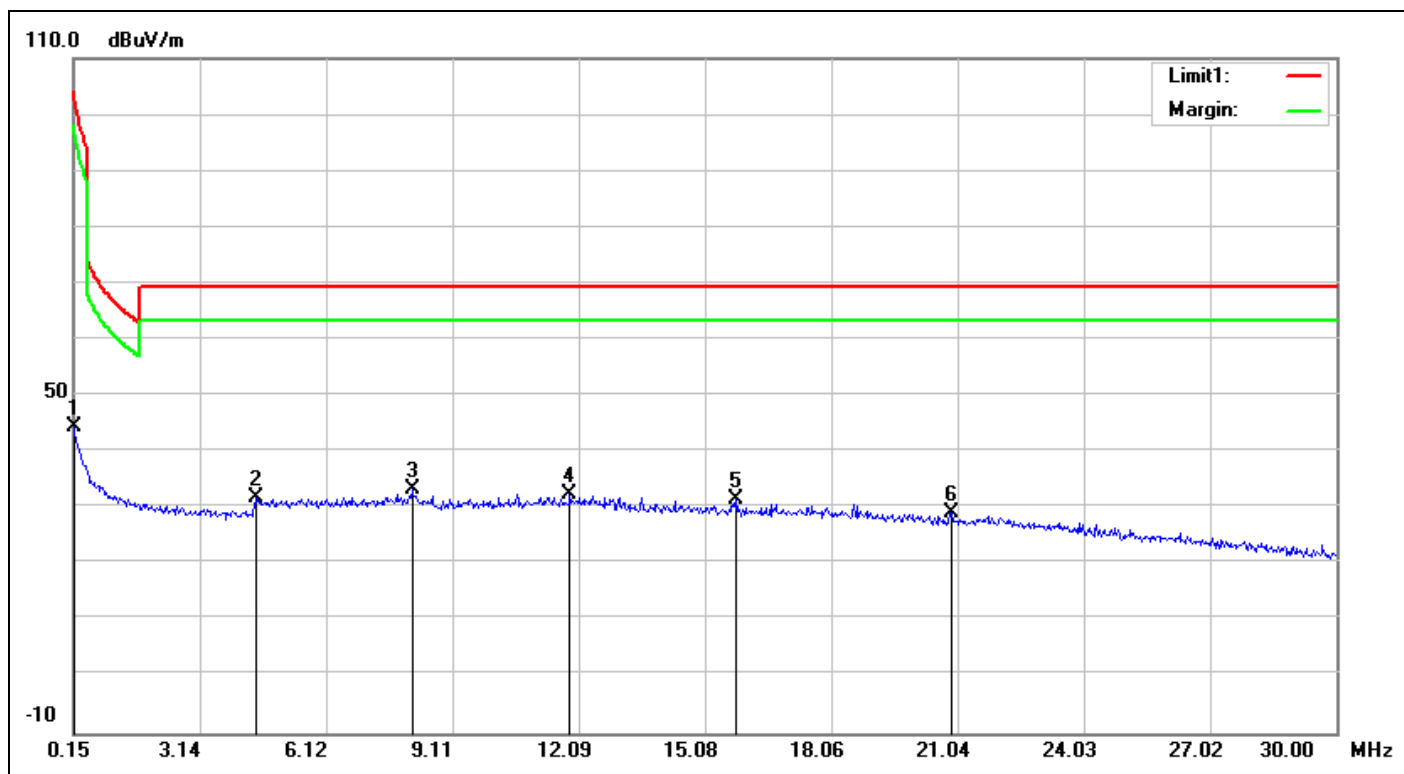

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC2.8_9k-1G_3m</b>                           | <b>Ant. Polarization:</b>  |                           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 20:49:17</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-TX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 0.1500          | 19.08         | 25.26          | 44.34          | 104.08         | -59.74      | QP   | 100         | 205           |        |
| 2   | 4.4782          | 19.44         | 12.52          | 31.96          | 69.50          | -37.54      | QP   | 100         | 197           |        |
| 3   | 8.1498          | 20.05         | 13.18          | 33.23          | 69.50          | -36.27      | QP   | 100         | 69            |        |
| 4   | 11.8810         | 20.55         | 11.85          | 32.40          | 69.50          | -37.10      | QP   | 100         | 261           |        |
| 5   | 15.8212         | 21.25         | 10.45          | 31.70          | 69.50          | -37.80      | QP   | 100         | 144           |        |
| 6   | 20.8957         | 22.04         | 7.02           | 29.06          | 69.50          | -40.44      | QP   | 100         | 174           |        |


# Spurious Emissions, RX Mode, 1-18G



**TUV Rheinland Taiwan Ltd.**

11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105


Tel:+886-2172-7000 fax:+886-2528-0018

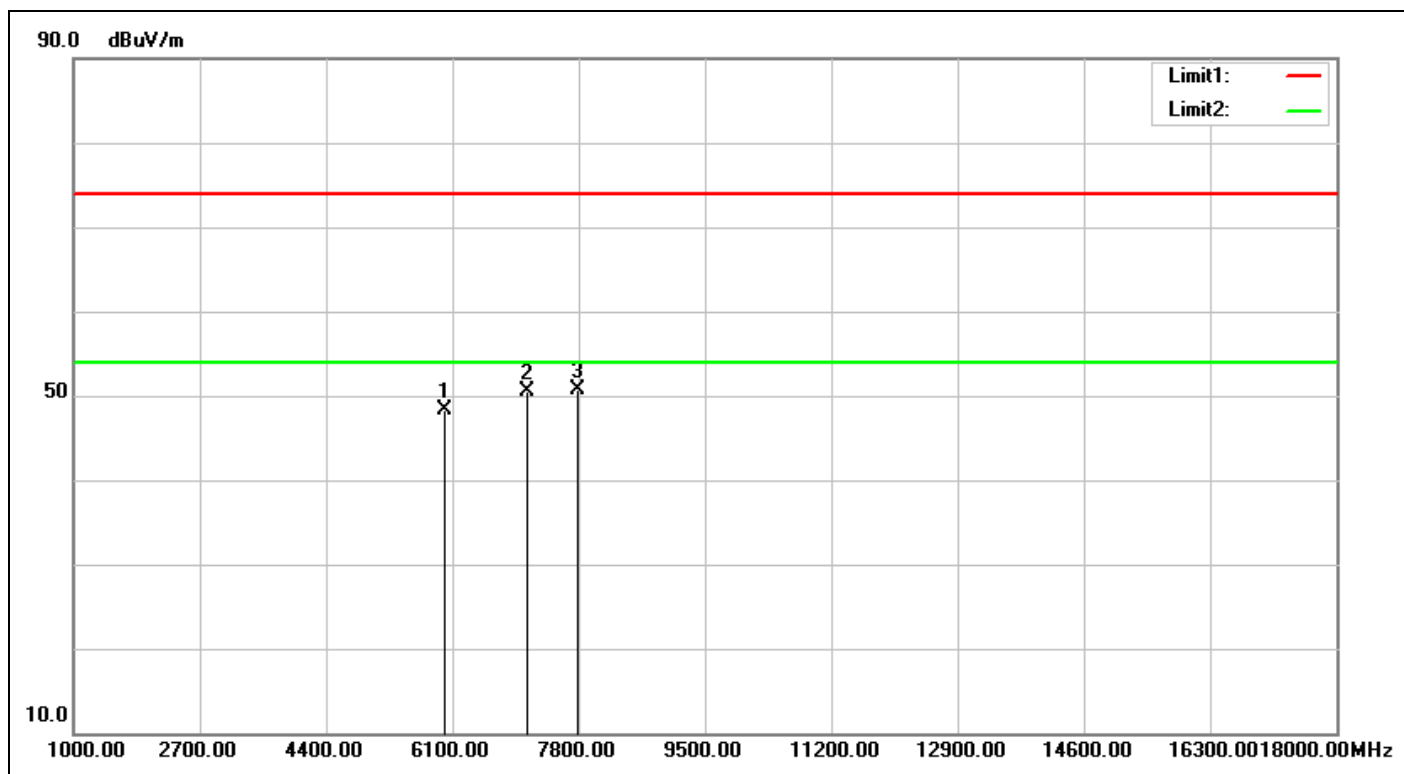

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 17:24:05 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-RX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 5998.000        | 2.34          | 46.06          | 48.40          | 74.00          | -25.60      | peak | 100         | 20          |        |
| 2   | 7103.000        | 3.95          | 46.50          | 50.45          | 74.00          | -23.55      | peak | 100         | 355         |        |
| 3   | 7783.000        | 4.86          | 45.93          | 50.79          | 74.00          | -23.21      | peak | 100         | 180         |        |

# Spurious Emissions, RX Mode, 1-18G

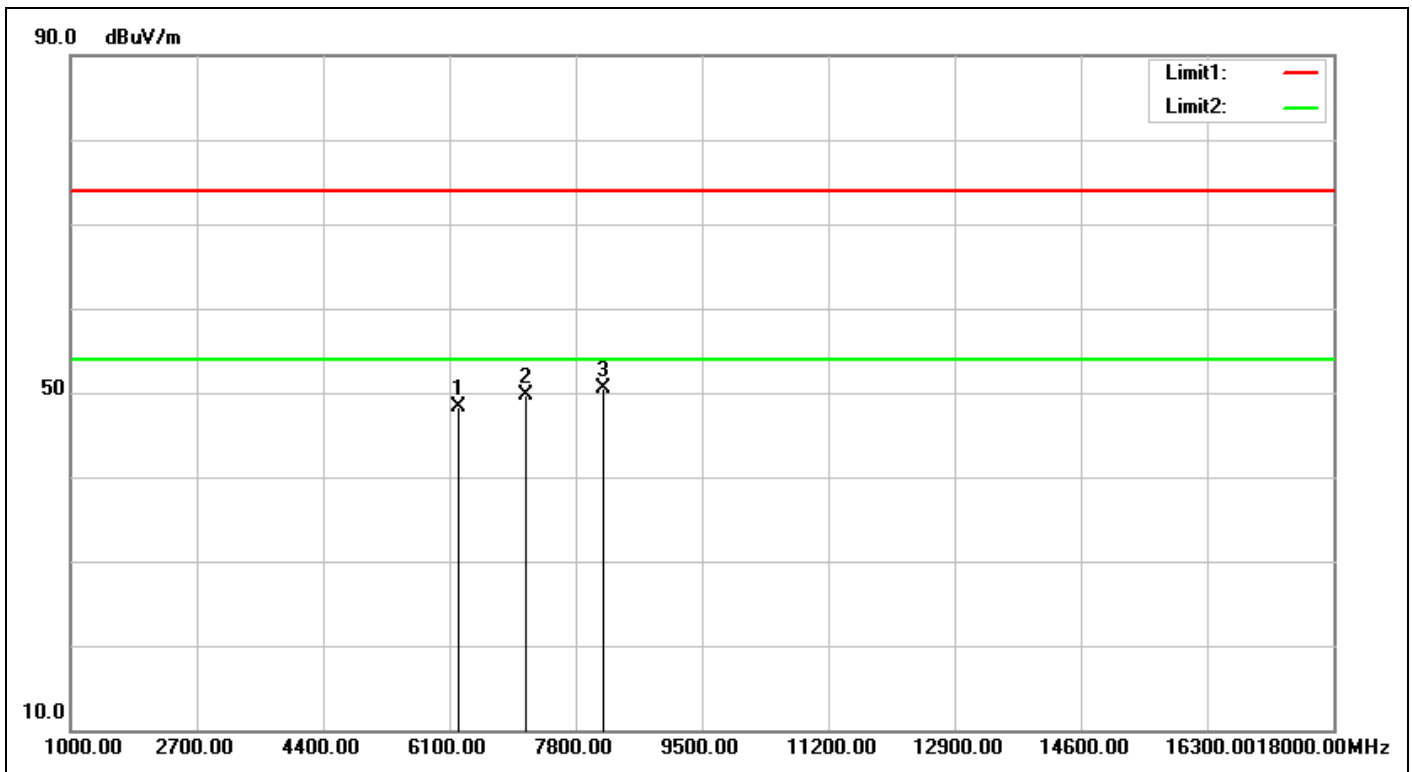

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Above 1G PEAK</b>                         | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 17:25:08</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-RX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 6219.000        | 3.22          | 45.13          | 48.35          | 74.00          | -25.65      | peak | 100         | 5             |        |
| 2   | 7120.000        | 3.99          | 45.81          | 49.80          | 74.00          | -24.20      | peak | 100         | 307           |        |
| 3   | 8174.000        | 4.98          | 45.48          | 50.46          | 74.00          | -23.54      | peak | 100         | 360           |        |


# Spurious Emissions, RX Mode, 18-26G



**TUV Rheinland Taiwan Ltd.**


**11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105**

Tel:+886-2172-7000 fax:+886-2528-0018

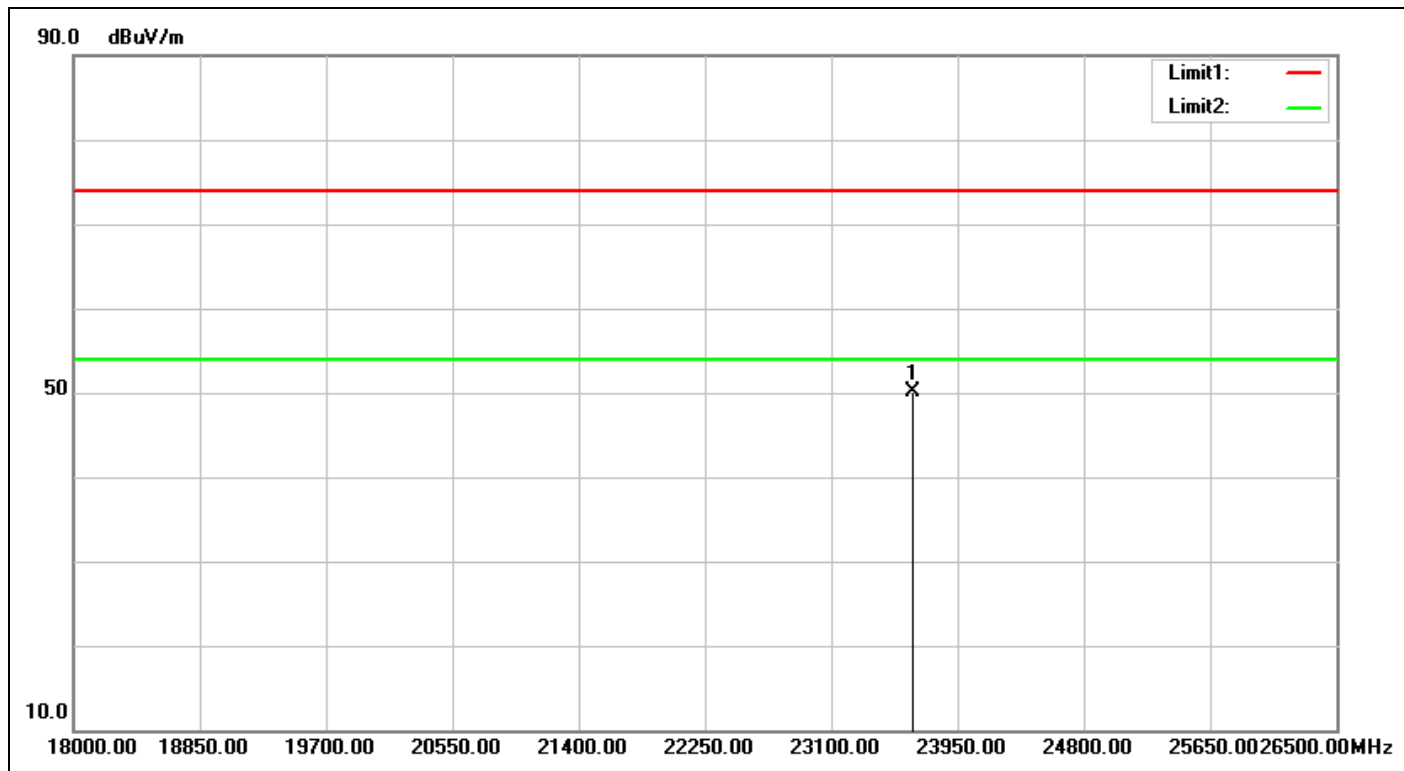

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Horizontal         |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 19:01:07 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-RX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 23652.500       | 32.71         | 17.42          | 50.13          | 74.00          | -23.87      | peak |             | 0           |        |

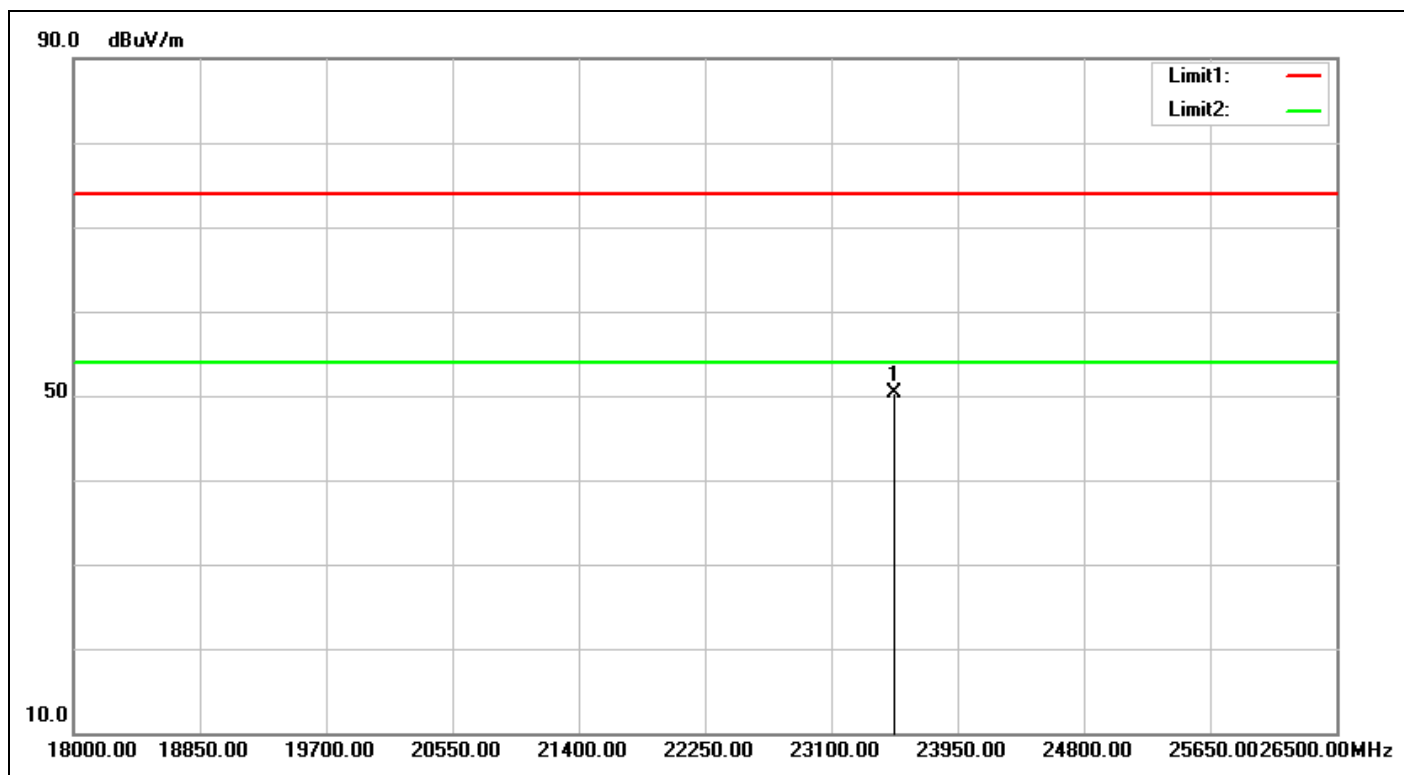

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC Above 1G PEAK                         | Ant. Polarization: | Vertical           |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 19:01:29 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%)  | 22(°C)/65 %        |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-RX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 23525.000       | 32.81         | 17.56          | 50.37          | 74.00          | -23.63      | peak |             |               |        |


# Spurious Emissions, RX Mode, 30M-1G



**TUV Rheinland Taiwan Ltd.**


11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105

Tel:+886-2172-7000 fax:+886-2528-0018

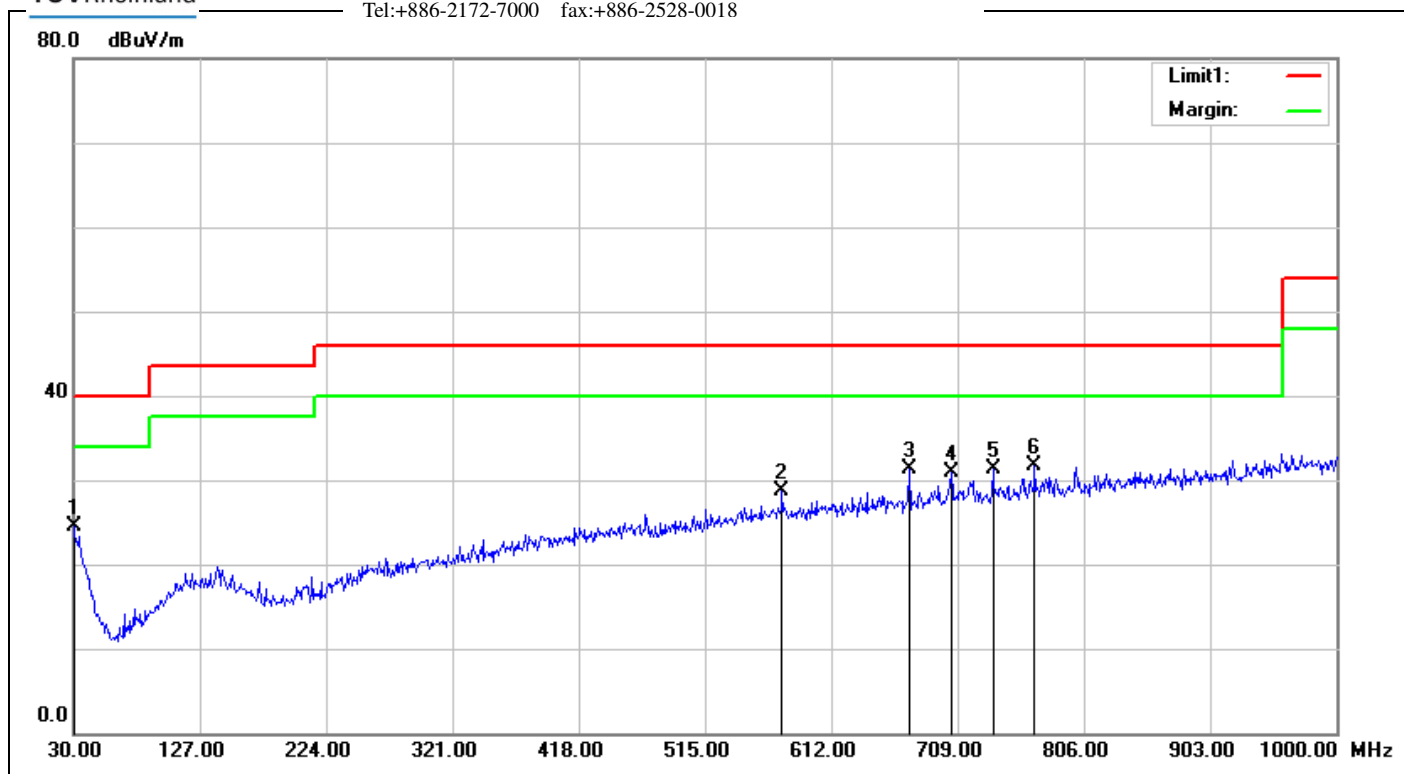

|                |  |                                           |  |  |  |                    |  |                    |  |  |
|----------------|--|-------------------------------------------|--|--|--|--------------------|--|--------------------|--|--|
| Service No.:   |  | 114072368                                 |  |  |  | Test Distance:     |  | 3m                 |  |  |
| Test Standard: |  | NCC Class B 3M Radiation                  |  |  |  | Ant. Polarization: |  | Horizontal         |  |  |
| Test item:     |  | Radiation Emission                        |  |  |  | Test Time:         |  | 2018/1/15 20:24:29 |  |  |
| Applicant:     |  | General Life Biotechnology Co., Ltd.      |  |  |  | Test Rating:       |  | DC 3V              |  |  |
| Product:       |  | BeneCheck Supreme Multi-Monitoring System |  |  |  | Temp.(℃)/Hum.(%)   |  | 22(℃)/65%          |  |  |
| Model No.:     |  | SEE REPORT NO: 50121721 APPENDIX I        |  |  |  | Test Engineer:     |  | Curry Chen         |  |  |
| Test Mode:     |  | 2440-RX                                   |  |  |  |                    |  |                    |  |  |
| Remark:        |  |                                           |  |  |  |                    |  |                    |  |  |

| No. | Frequency<br>(MHz) | Factor<br>(dB/m) | Reading<br>(dBuV) | Level<br>(dBuV/m) | Limit<br>(dBuV/m) | Margin<br>(dB) | Det. | Height<br>(cm) | Azimuth<br>( ° ) | Remark |
|-----|--------------------|------------------|-------------------|-------------------|-------------------|----------------|------|----------------|------------------|--------|
| 1   | 30.0000            | -0.25            | 24.80             | 24.55             | 40.00             | -15.45         | QP   | 100            | 313              |        |
| 2   | 574.1700           | -0.20            | 28.85             | 28.65             | 46.00             | -17.35         | QP   | 100            | 276              |        |
| 3   | 672.1400           | 0.85             | 30.50             | 31.35             | 46.00             | -14.65         | QP   | 100            | 219              |        |
| 4   | 704.1500           | 1.35             | 29.46             | 30.81             | 46.00             | -15.19         | QP   | 100            | 59               |        |
| 5   | 736.1600           | 2.06             | 29.29             | 31.35             | 46.00             | -14.65         | QP   | 100            | 53               |        |
| 6   | 768.1700           | 2.51             | 29.24             | 31.75             | 46.00             | -14.25         | QP   | 100            | 240              |        |

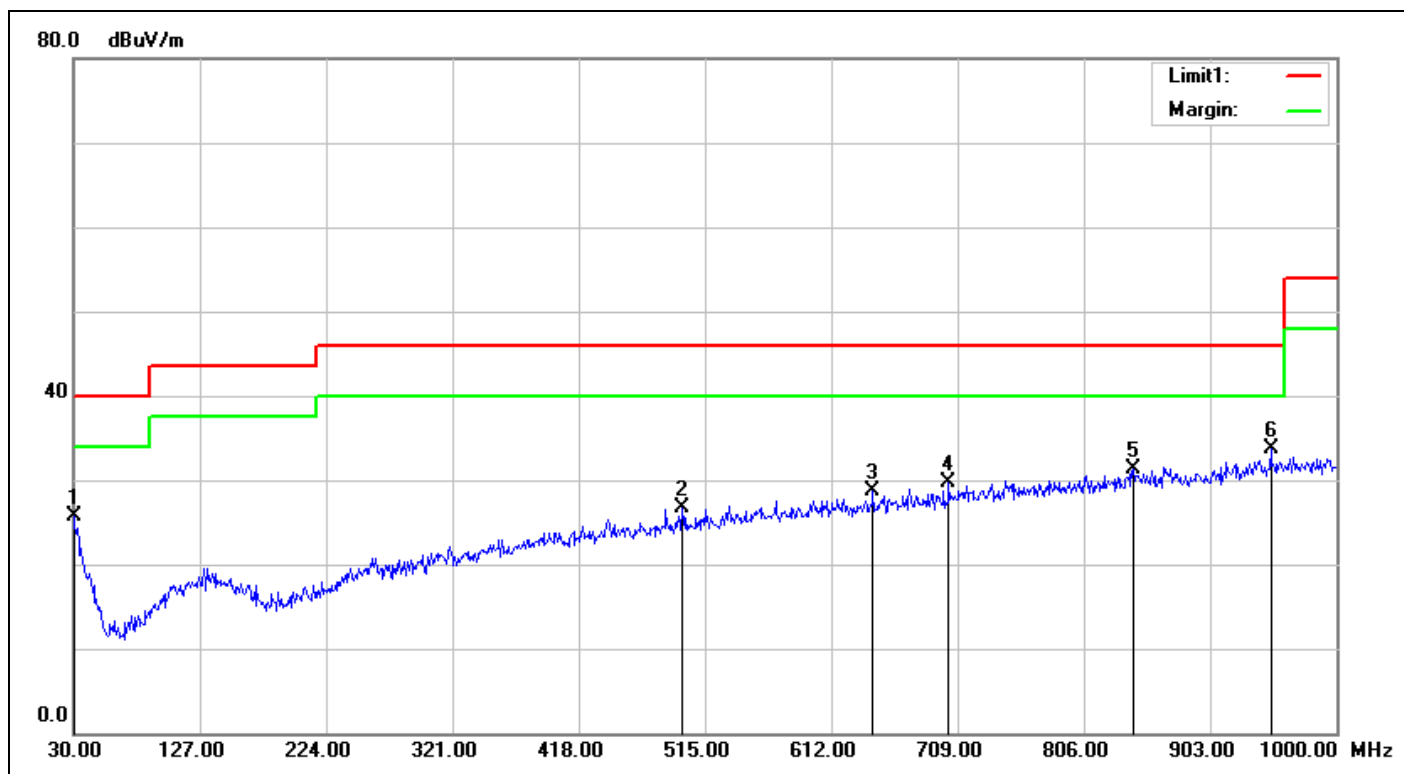

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC Class B 3M Radiation</b>                  | <b>Ant. Polarization:</b>  | <b>Vertical</b>           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 20:25:32</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-RX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 30.0000         | -0.25         | 25.95          | 25.70          | 40.00          | -14.30      | QP   | 100         | 157           |        |
| 2   | 497.5400        | -1.21         | 27.94          | 26.73          | 46.00          | -19.27      | QP   | 100         | 99            |        |
| 3   | 644.0100        | 0.47          | 28.21          | 28.68          | 46.00          | -17.32      | QP   | 100         | 184           |        |
| 4   | 702.2100        | 1.31          | 28.43          | 29.74          | 46.00          | -16.26      | QP   | 100         | 216           |        |
| 5   | 843.8300        | 3.60          | 27.65          | 31.25          | 46.00          | -14.75      | QP   | 100         | 115           |        |
| 6   | 949.5600        | 5.48          | 28.30          | 33.78          | 46.00          | -12.22      | QP   | 100         | 266           |        |


# Spurious Emissions, RX Mode, 9K-30M



**TUV Rheinland Taiwan Ltd.**

11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105


Tel:+886-2172-000 fax:+886-2528-0018

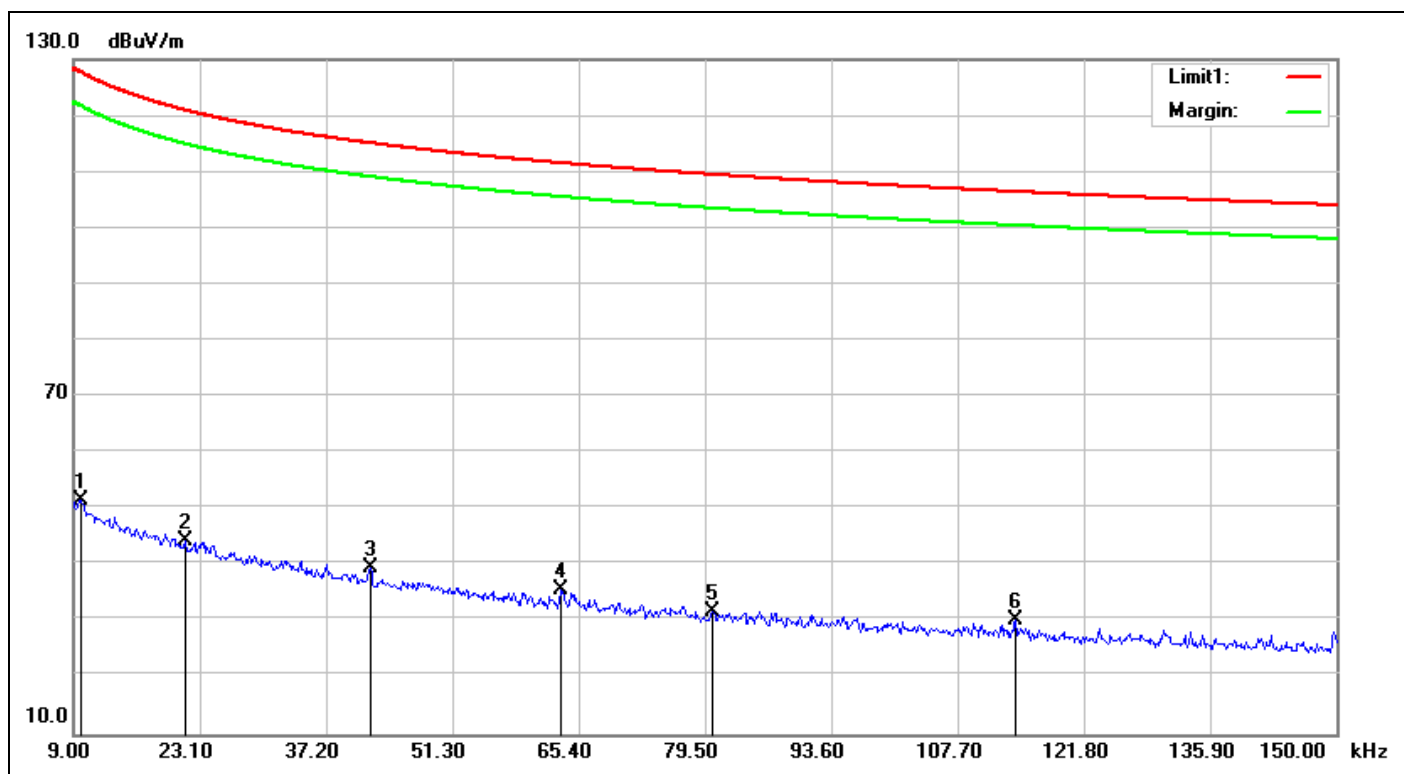

|                |                                           |                    |                    |
|----------------|-------------------------------------------|--------------------|--------------------|
| Service No.:   | 114072368                                 | Test Distance:     | 3m                 |
| Test Standard: | NCC2.8_9k-1G_3m                           | Ant. Polarization: |                    |
| Test item:     | Radiation Emission                        | Test Time:         | 2018/1/15 20:44:30 |
| Applicant:     | General Life Biotechnology Co., Ltd.      | Test Rating:       | DC 3V              |
| Product:       | BeneCheck Supreme Multi-Monitoring System | Temp.(°C)/Hum.(%): | 22(°C)/65%         |
| Model No.:     | SEE REPORT NO: 50121721 APPENDIX I        | Test Engineer:     | Curry Chen         |
| Test Mode:     | 2440-RX                                   |                    |                    |
| Remark:        |                                           |                    |                    |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth (°) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|-------------|--------|
| 1   | 0.0098          | 19.85         | 31.85          | 51.70          | 127.76         | -76.06      | QP   | 100         | 200         |        |
| 2   | 0.0215          | 20.05         | 24.24          | 44.29          | 120.94         | -76.65      | QP   | 100         | 258         |        |
| 3   | 0.0421          | 19.71         | 19.93          | 39.64          | 115.11         | -75.47      | QP   | 100         | 260         |        |
| 4   | 0.0634          | 19.35         | 16.33          | 35.68          | 111.55         | -75.87      | QP   | 100         | 189         |        |
| 5   | 0.0803          | 19.25         | 12.54          | 31.79          | 109.50         | -77.71      | QP   | 100         | 136         |        |
| 6   | 0.1142          | 19.12         | 11.01          | 30.13          | 106.44         | -76.31      | QP   | 100         | 356         |        |

## Spurious Emissions, RX Mode, 9k-30M

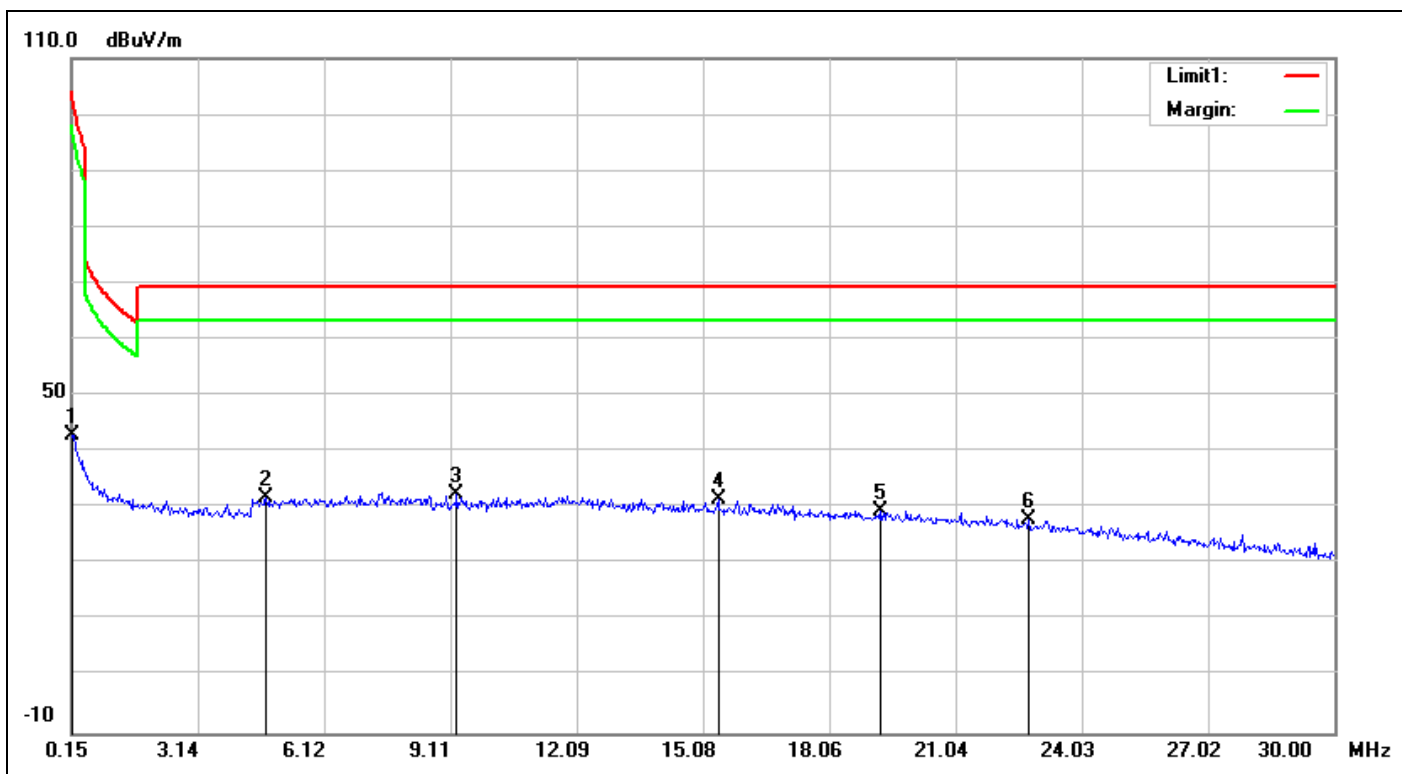

|                       |                                                  |                            |                           |
|-----------------------|--------------------------------------------------|----------------------------|---------------------------|
| <b>Service No.:</b>   | <b>114072368</b>                                 | <b>Test Distance:</b>      | <b>3m</b>                 |
| <b>Test Standard:</b> | <b>NCC2.8_9k-1G_3m</b>                           | <b>Ant. Polarization:</b>  |                           |
| <b>Test item:</b>     | <b>Radiation Emission</b>                        | <b>Test Time:</b>          | <b>2018/1/15 20:50:21</b> |
| <b>Applicant:</b>     | <b>General Life Biotechnology Co., Ltd.</b>      | <b>Test Rating:</b>        | <b>DC 3V</b>              |
| <b>Product:</b>       | <b>BeneCheck Supreme Multi-Monitoring System</b> | <b>Temp.(°C)/Hum.(%)</b> : | <b>22(°C)/65%</b>         |
| <b>Model No.:</b>     | <b>SEE REPORT NO: 50121721 APPENDIX I</b>        | <b>Test Engineer:</b>      | <b>Curry Chen</b>         |
| <b>Test Mode:</b>     | <b>2440-RX</b>                                   |                            |                           |
| <b>Remark:</b>        |                                                  |                            |                           |

| No. | Frequency (MHz) | Factor (dB/m) | Reading (dBuV) | Level (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Det. | Height (cm) | Azimuth ( ° ) | Remark |
|-----|-----------------|---------------|----------------|----------------|----------------|-------------|------|-------------|---------------|--------|
| 1   | 0.1500          | 19.08         | 23.95          | 43.03          | 104.08         | -61.05      | QP   | 100         | 104           |        |
| 2   | 4.7469          | 19.60         | 12.19          | 31.79          | 69.50          | -37.71      | QP   | 100         | 115           |        |
| 3   | 9.2543          | 20.15         | 12.24          | 32.39          | 69.50          | -37.11      | QP   | 100         | 194           |        |
| 4   | 15.4332         | 21.18         | 10.48          | 31.66          | 69.50          | -37.84      | QP   | 100         | 97            |        |
| 5   | 19.2540         | 21.85         | 7.72           | 29.57          | 69.50          | -39.93      | QP   | 100         | 192           |        |
| 6   | 22.7763         | 22.17         | 5.73           | 27.90          | 69.50          | -41.60      | QP   | 100         | 91            |        |