



Annex B Test Setup Photos

Next to mouth

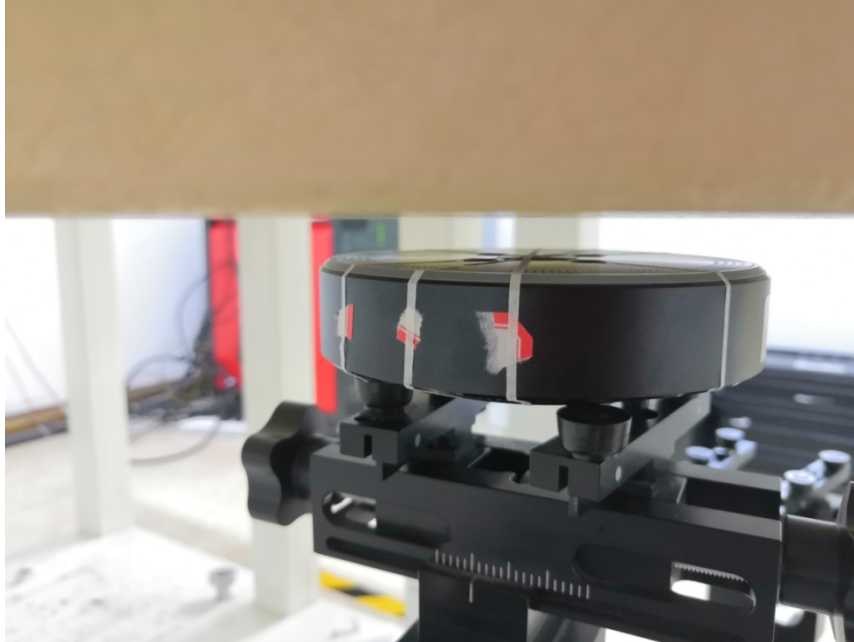


Top Side

(Test distance: 10mm, Thickness of EUT: 15mm)

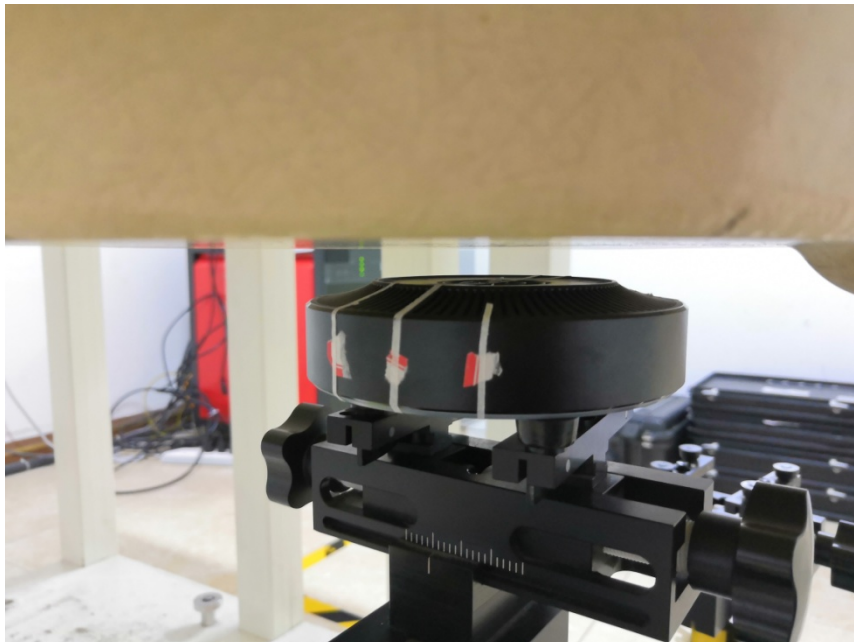


Bottom Side

(Test distance: 10mm, Thickness of EUT: 15 mm)

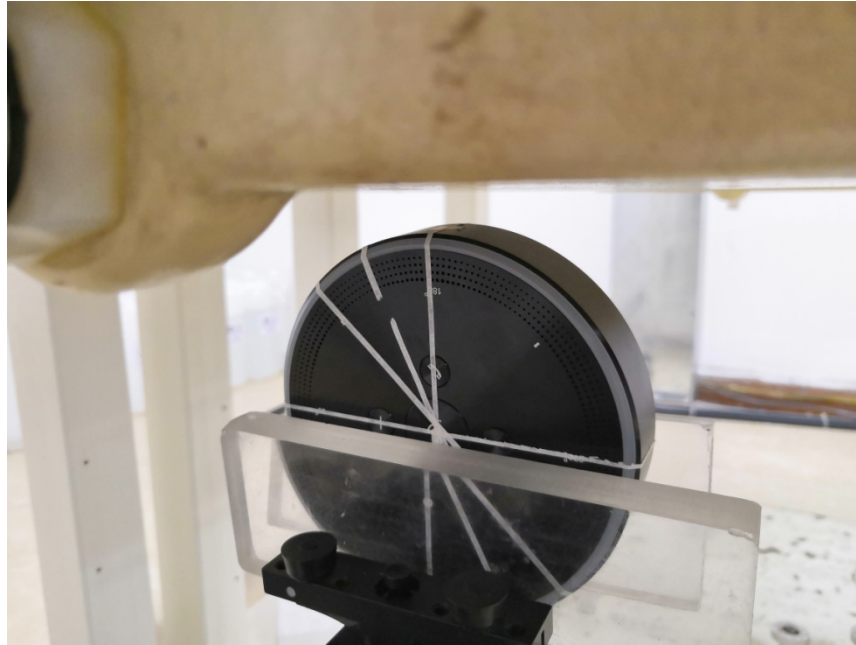

Top Side

(Test distance: 10mm, Thickness of EUT: 15mm)

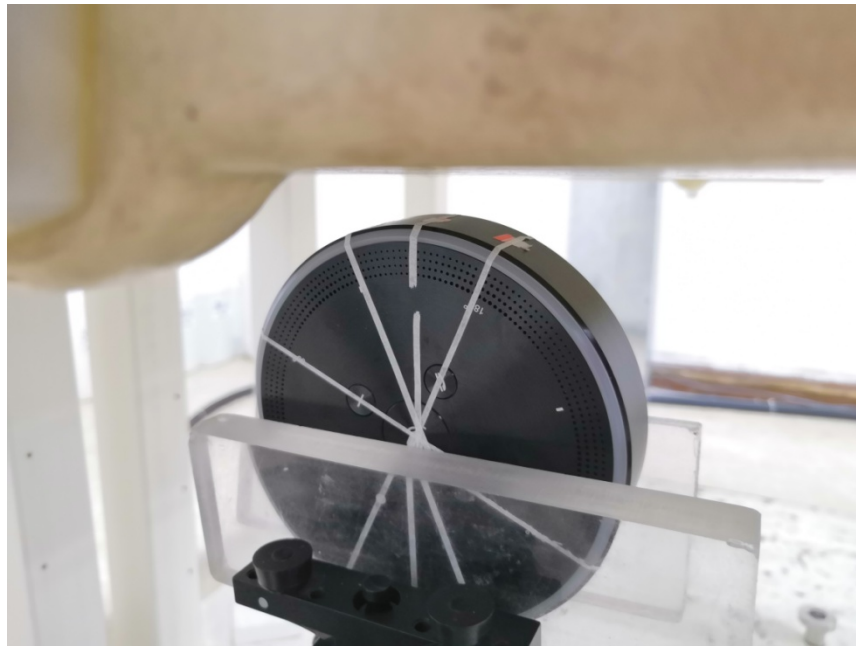

Left Side 1

(Test distance: 10mm, Thickness of EUT: 15mm)



Left Side 2


(Test distance: 10mm, Thickness of EUT: 15mm)

Body



Top Side

(Test distance: 5mm, Thickness of EUT: 15mm)

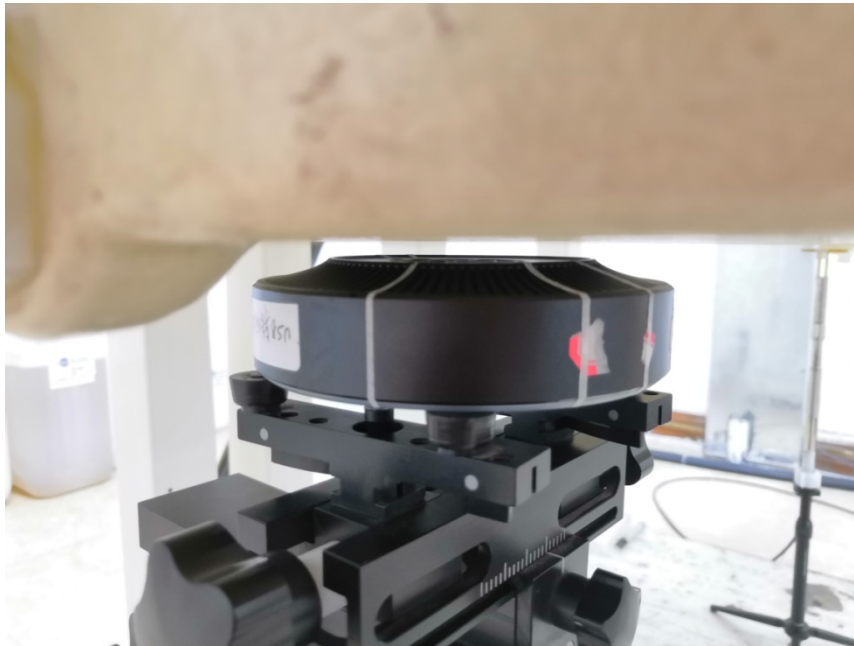

Bottom Side

(Test distance: 5mm, Thickness of EUT: 15 mm)



Top Side

(Test distance: 5mm, Thickness of EUT: 15mm)



Left Side 1


(Test distance: 5mm, Thickness of EUT: 15mm)



Left Side 2


(Test distance: 5mm, Thickness of EUT: 15mm)

Extremity

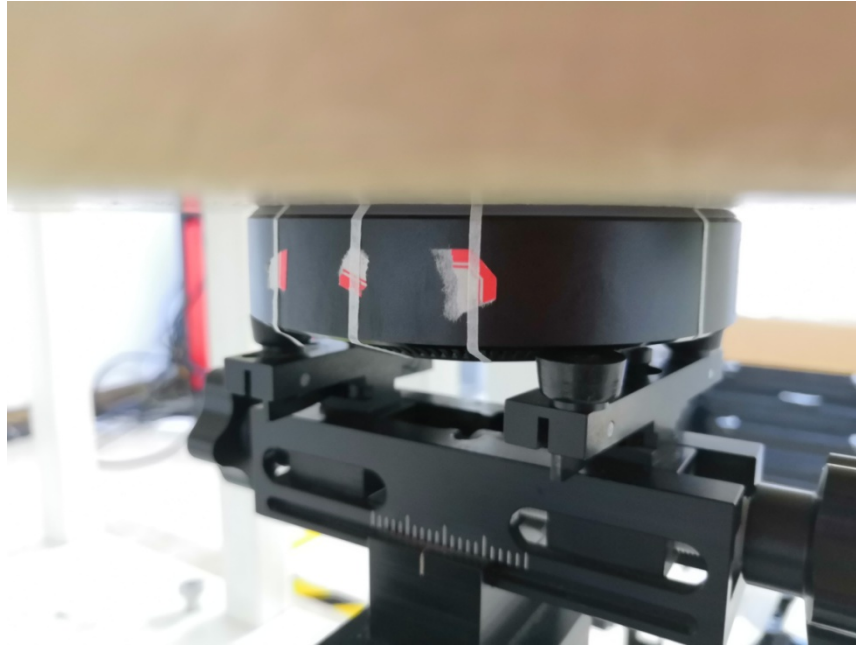

Top Side

(Test distance: 0mm, Thickness of EUT: 15mm)

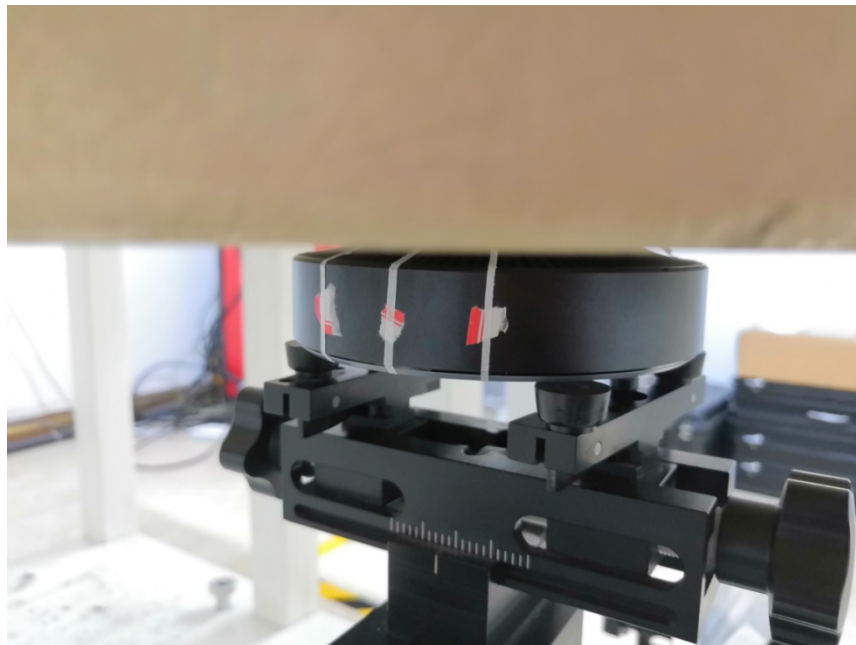

Bottom Side

(Test distance: 0mm, Thickness of EUT: 15 mm)




Top Side

(Test distance: 0mm, Thickness of EUT: 15mm)



Left Side 1

(Test distance: 0mm, Thickness of EUT: 15mm)

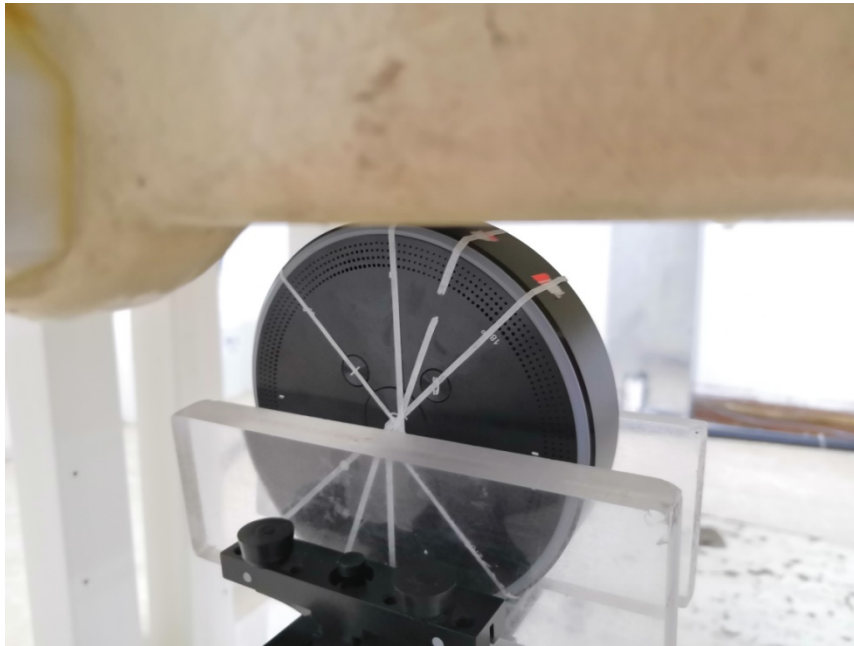

Left Side 2

(Test distance: 0mm, Thickness of EUT: 15mm)