

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

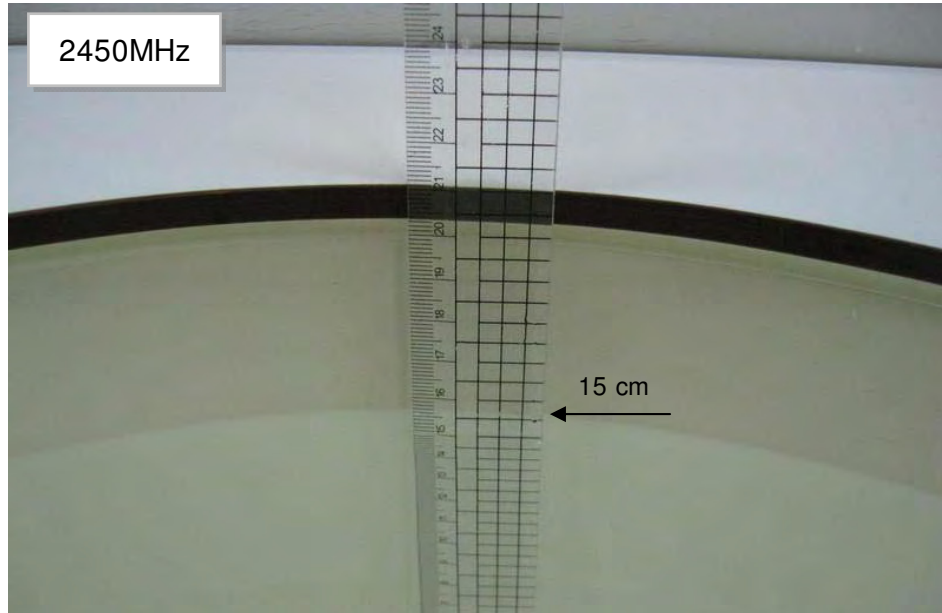


Fig.2

Body - distance between flat phantom and EUT is 0 mm

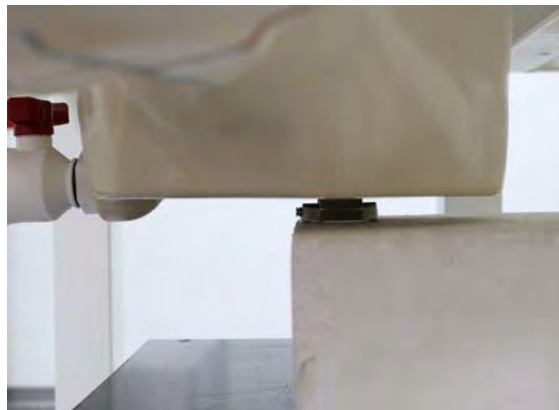
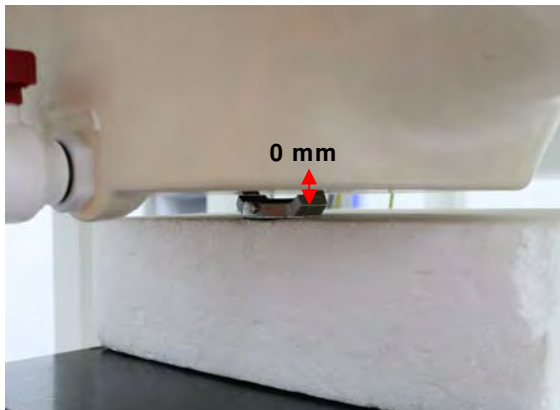


Fig.3 Configuration 1: remove the watchband and make the watch's back touch against the flat phantom

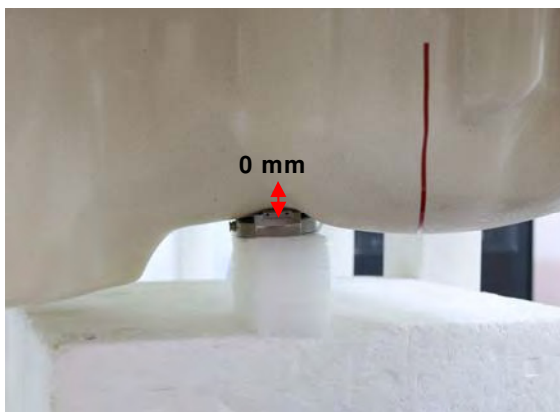


Fig.4 Configuration 2: remove the watchband and make the watch's back touch against the neck phantom area

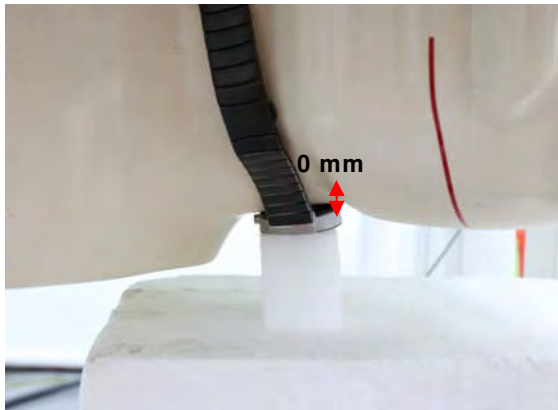


Fig.5 Configuration 3: remove the one side's watchband and make the watch's back touch against the neck phantom area

12. Photographs of the EUT

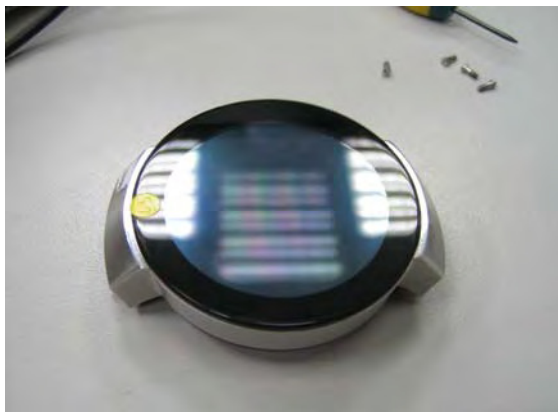


Fig.6 EUT

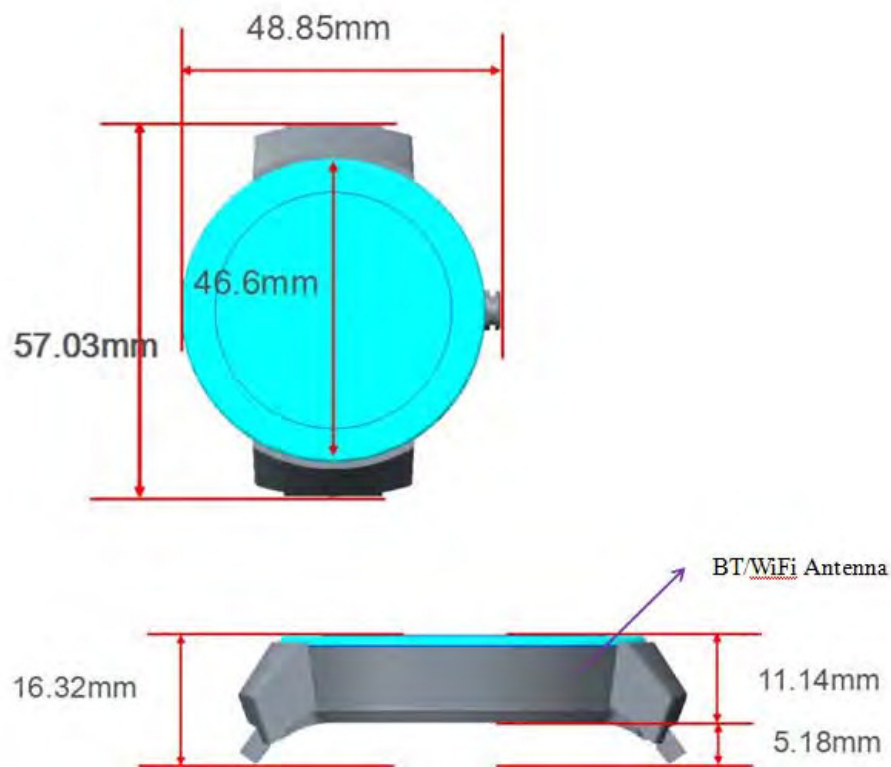


Fig.7 Antenna location

- End of Report -