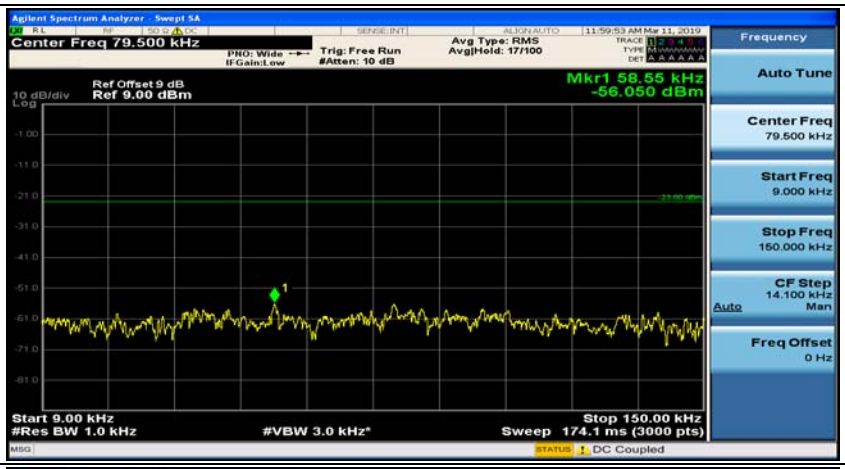
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
11:59:53 AM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 58.55 kHz
-56.050 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

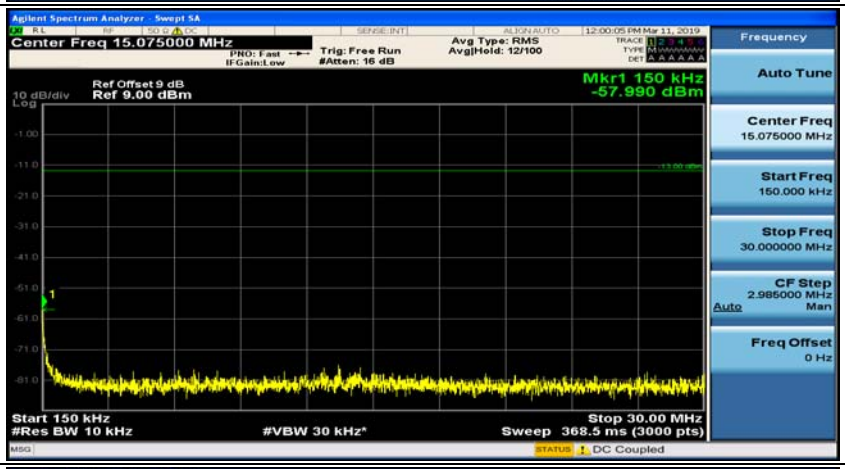
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:00:05 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.990 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

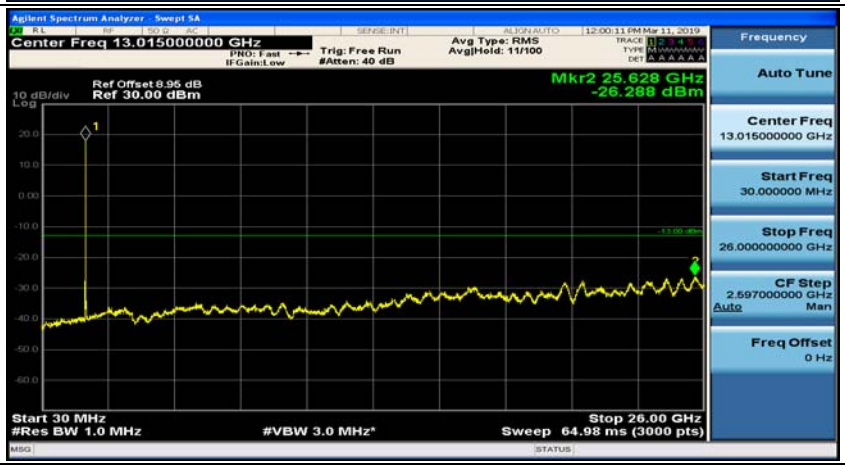
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:00:11 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.628 GHz
-26.288 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#0

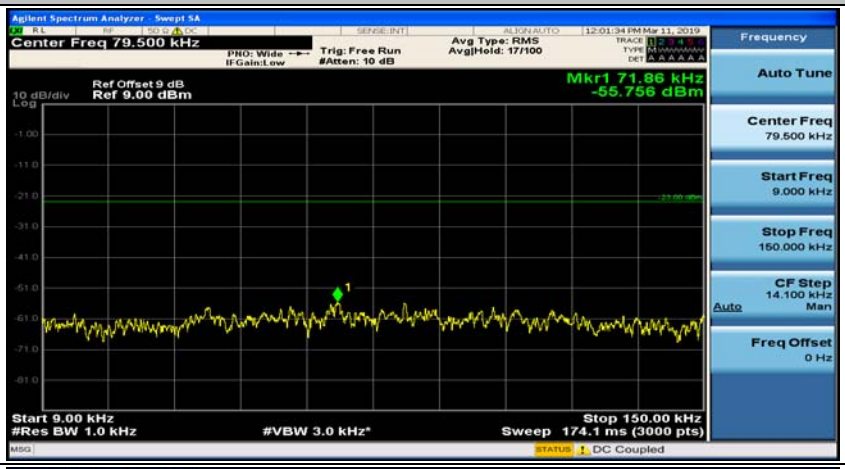

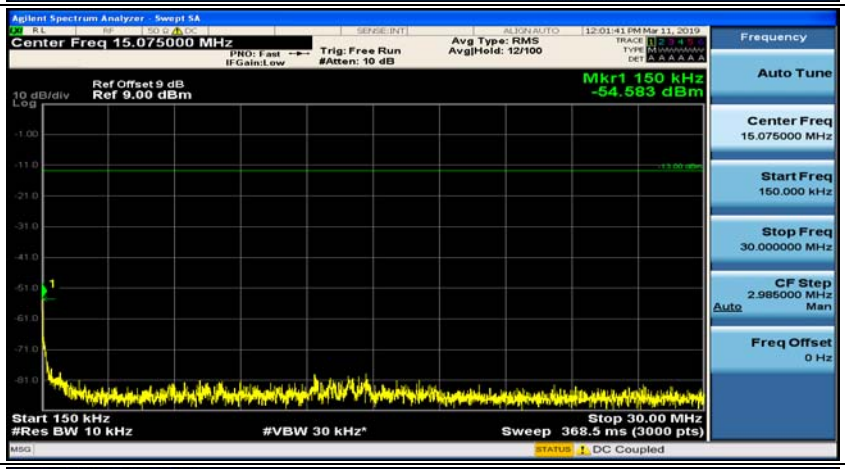

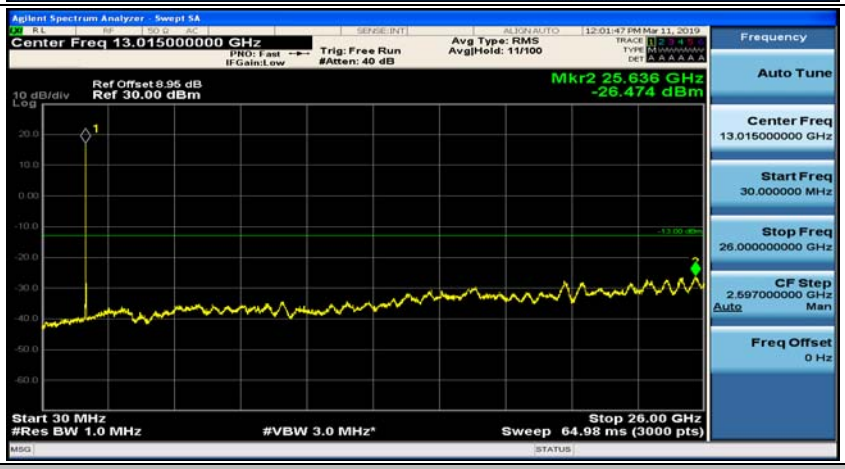

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#37

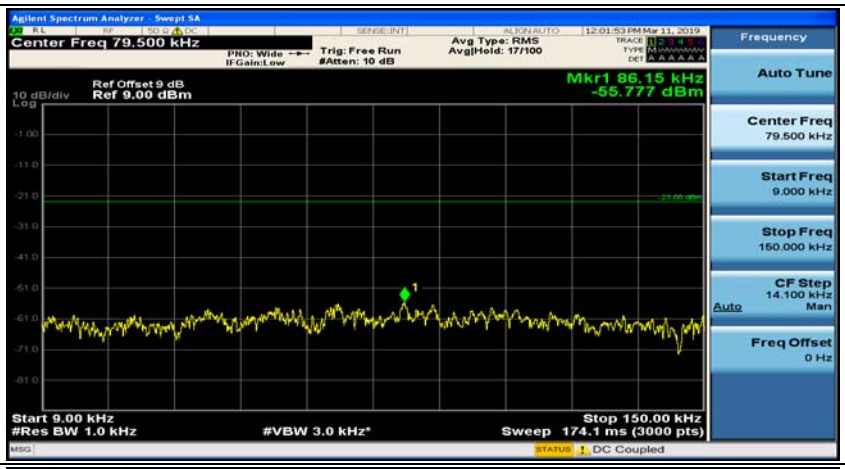

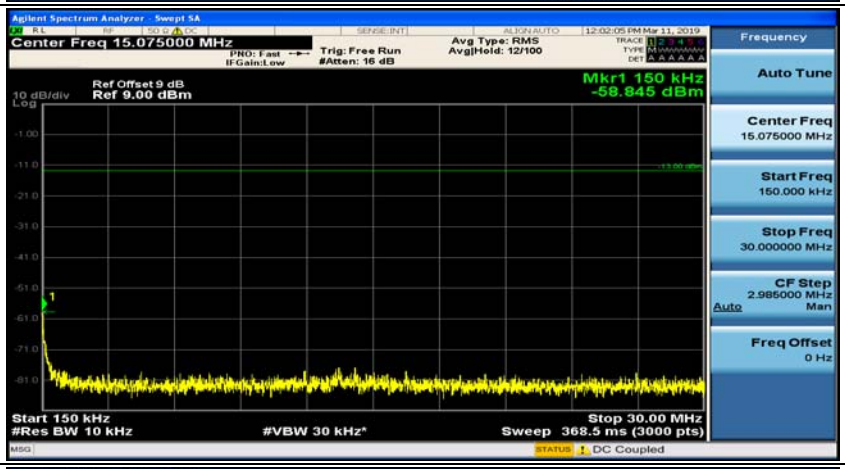

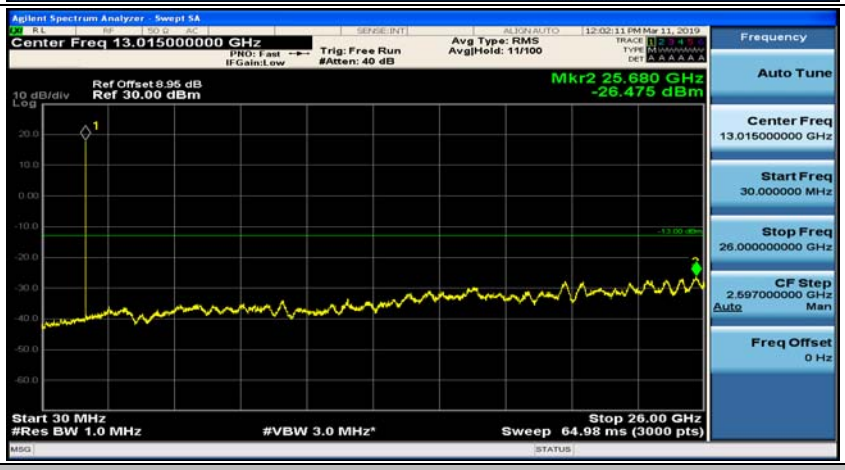

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#74

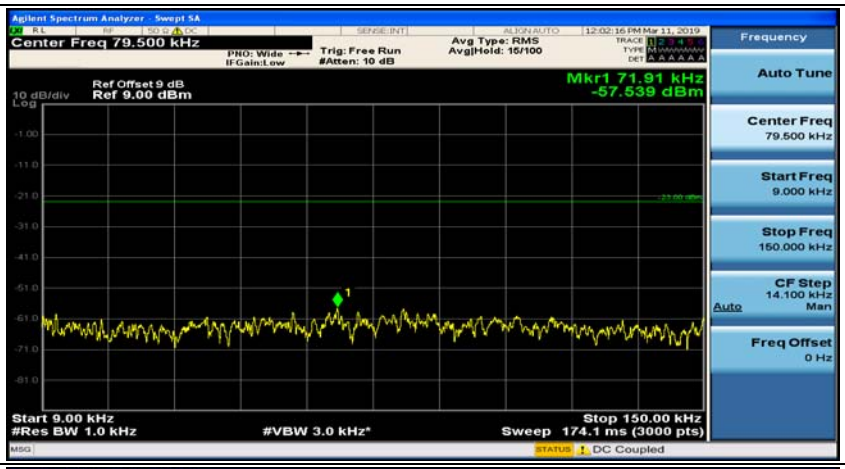
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 15/100
12:02:16 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 71.91 kHz
-57.539 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

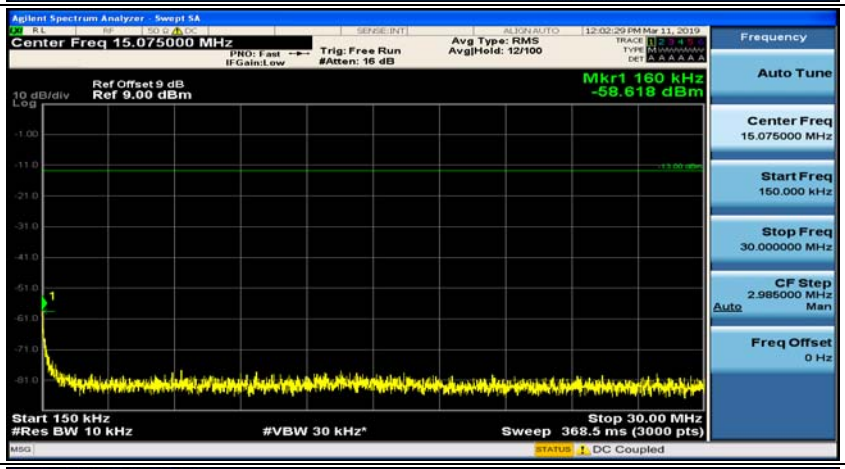
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:02:29 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.618 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

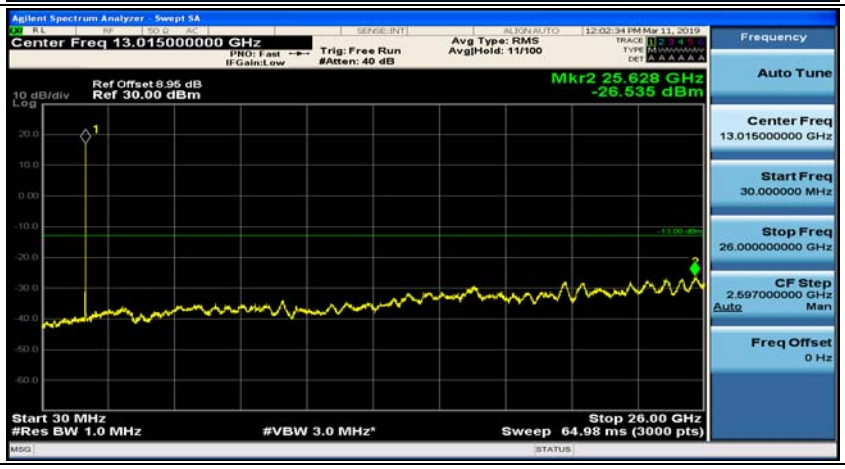
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:02:34 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.628 GHz
-26.535 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#0

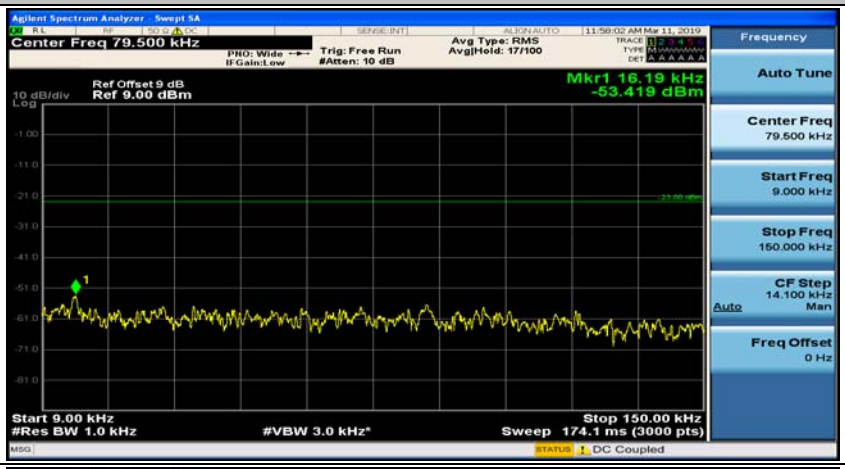

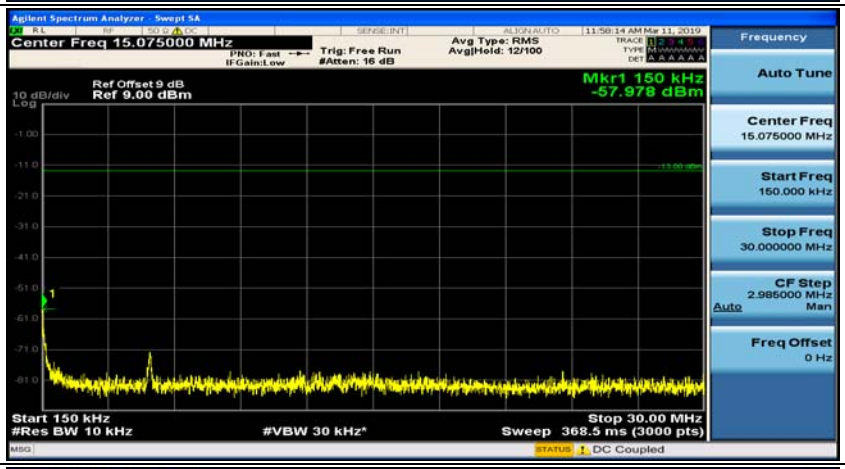

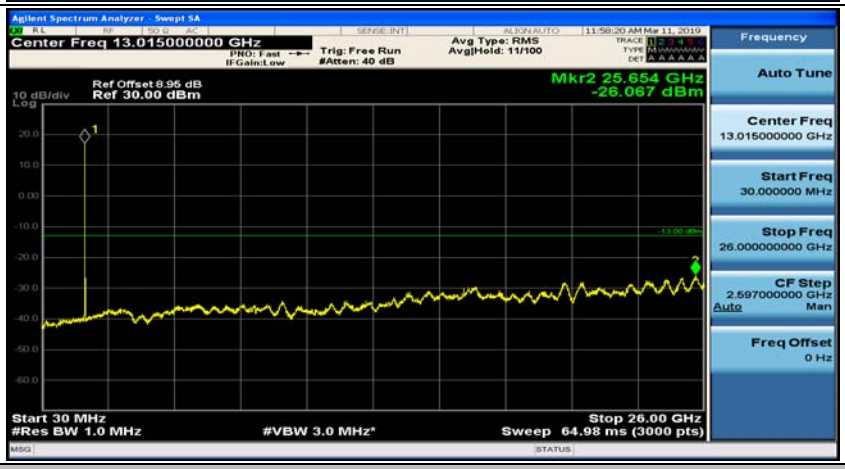

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#37

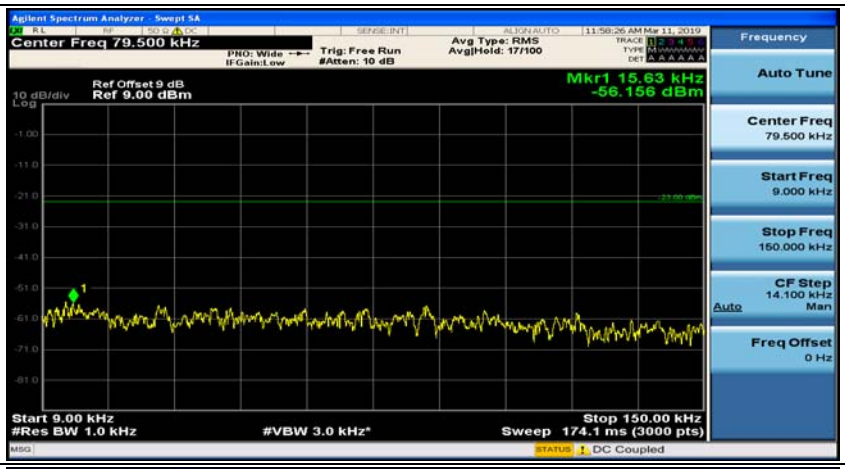

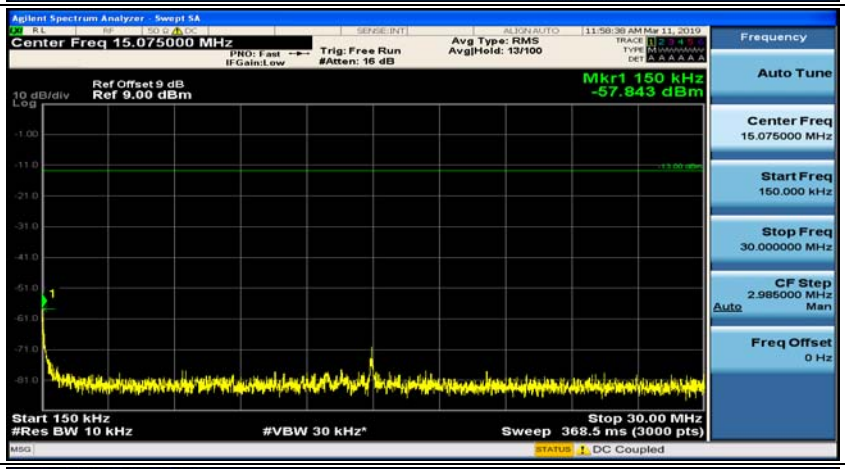

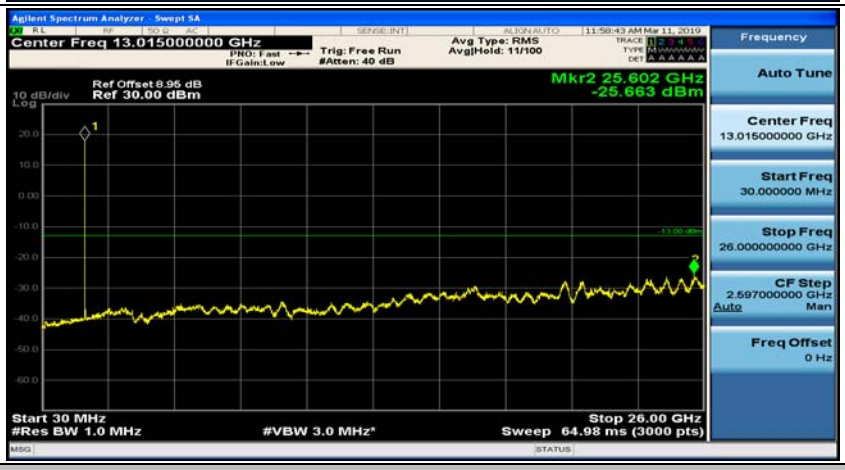

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#74

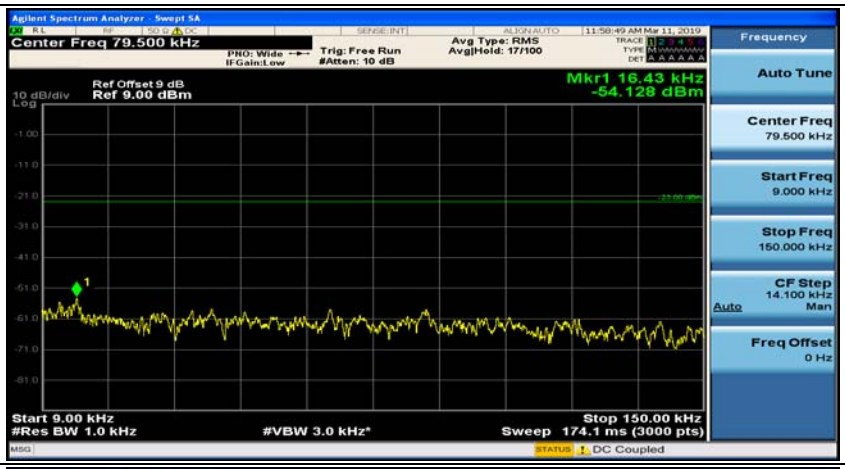
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
11:58:49 AM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 16.43 kHz
-54.128 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

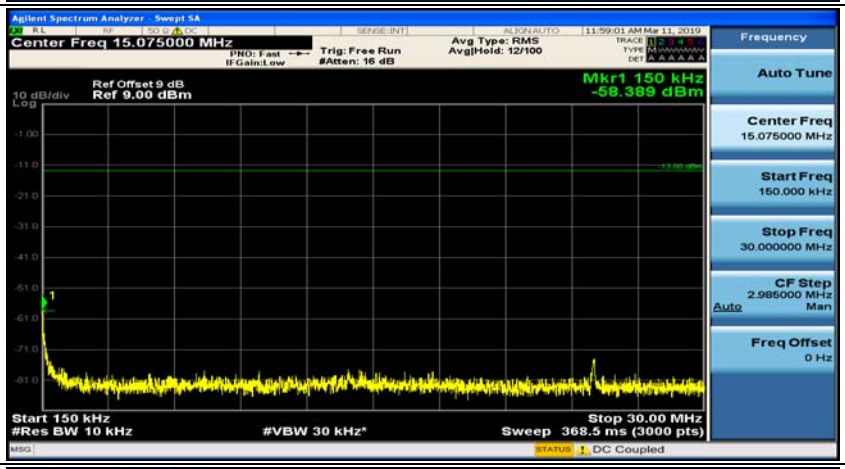
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
11:59:01 AM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-58.389 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

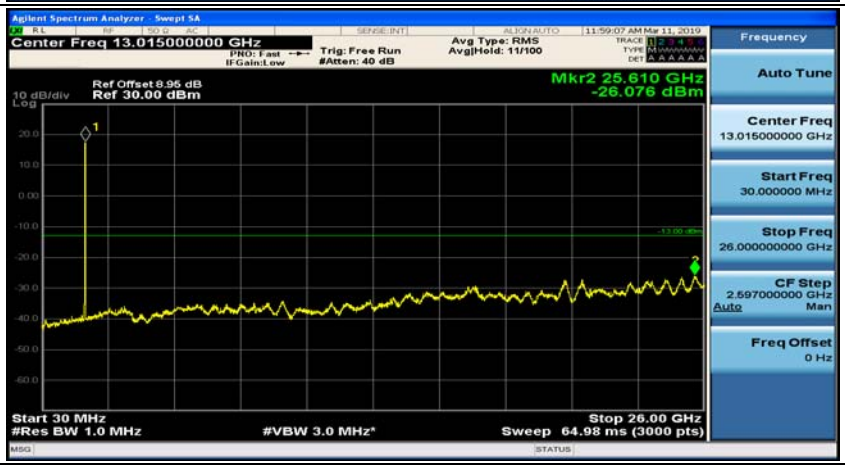
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
11:59:07 AM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.610 GHz
-26.076 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#0

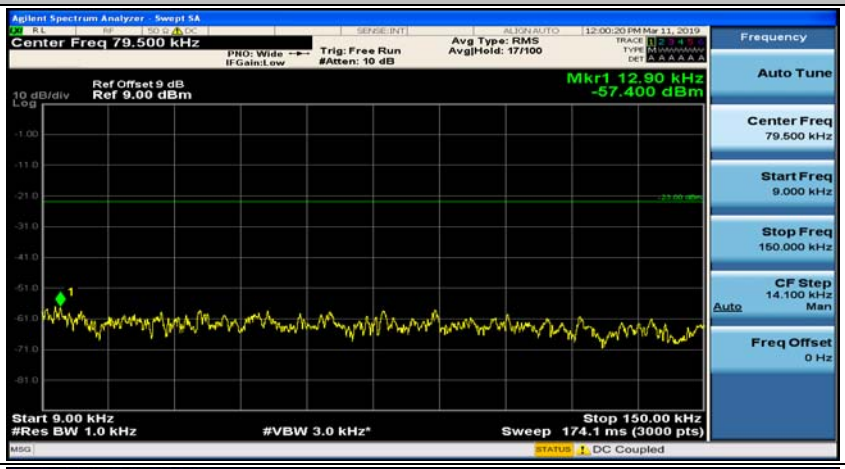

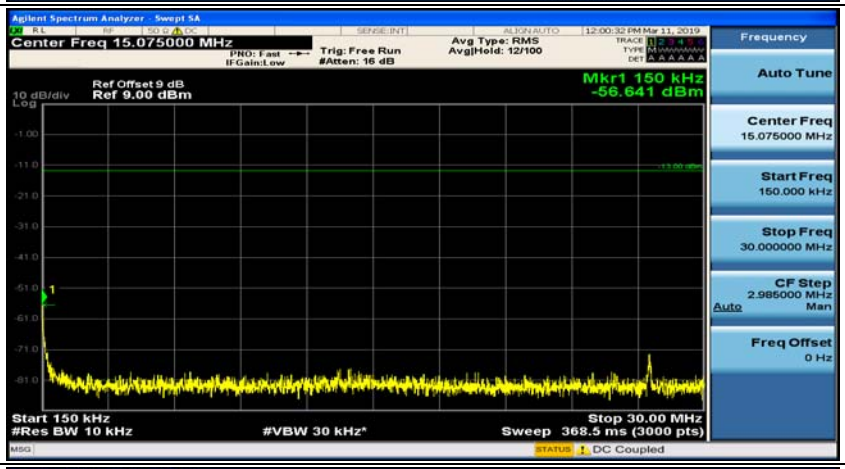

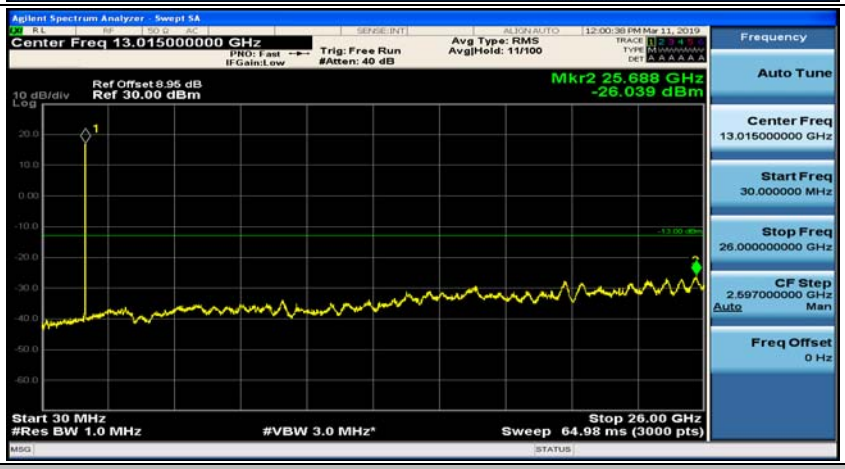

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#37

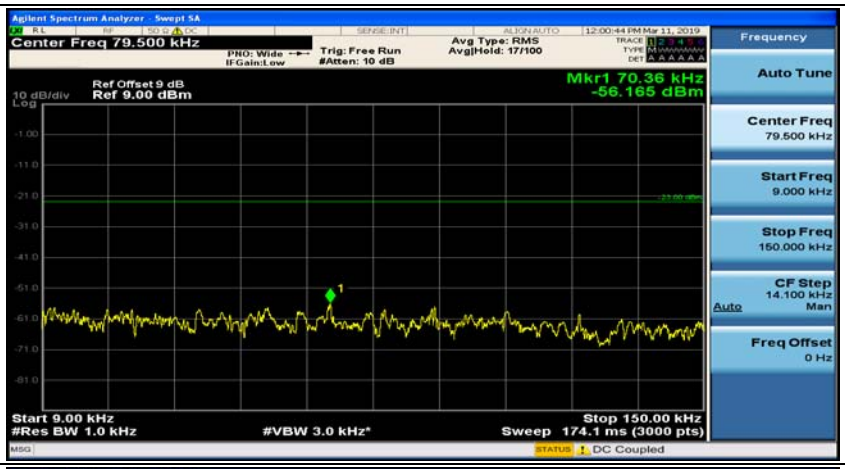

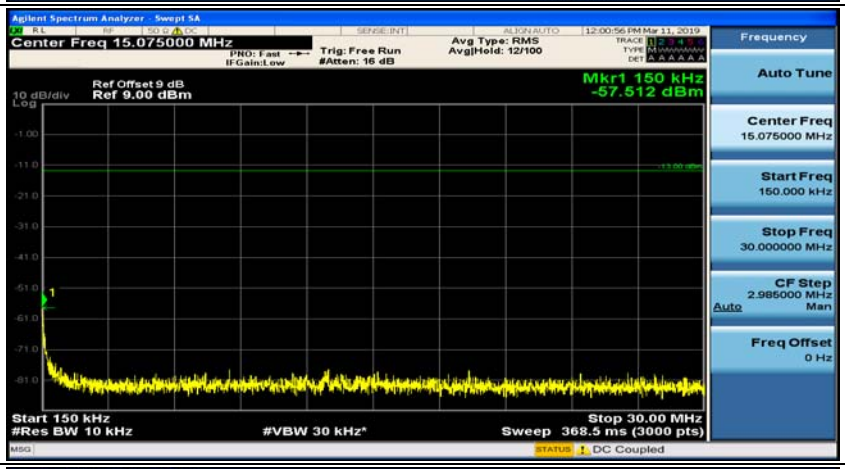

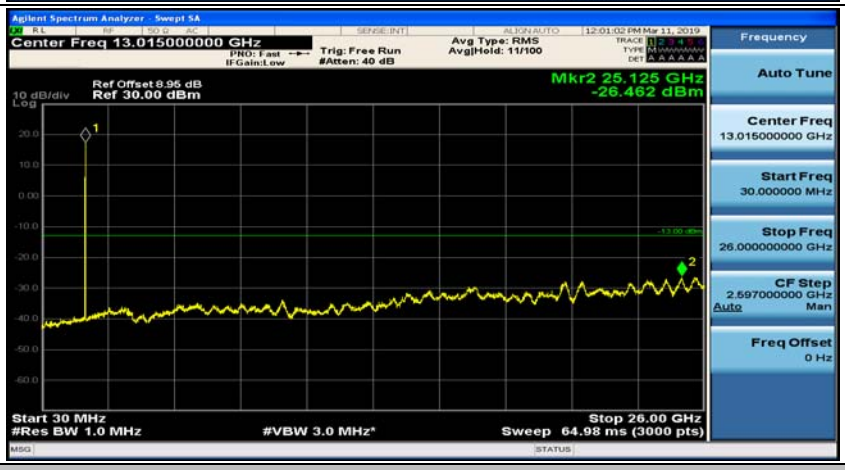

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#74

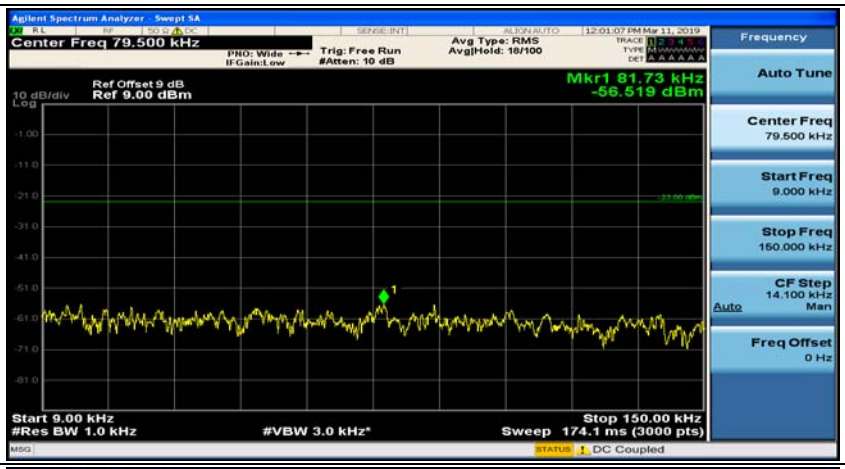
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 18/100
12:01:07 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 81.73 kHz
-56.519 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

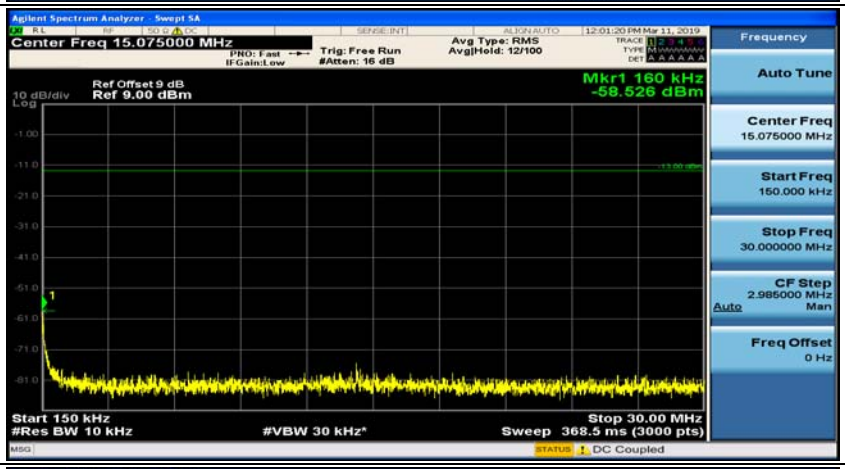
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:01:20 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.526 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

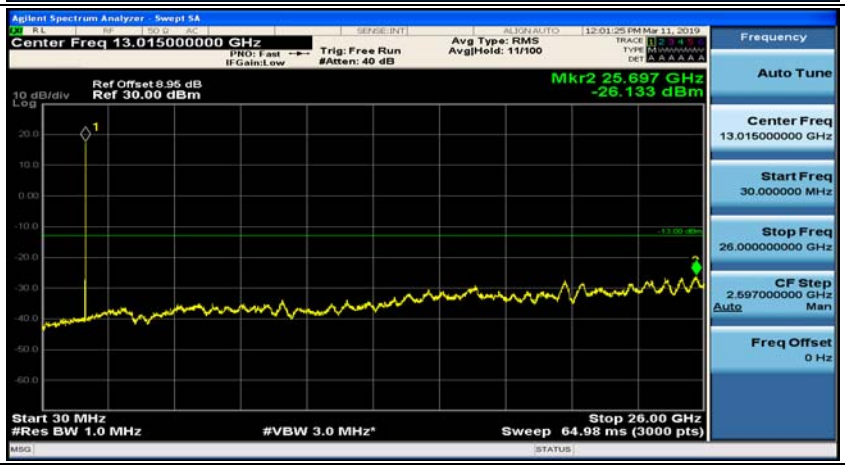
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:01:25 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.697 GHz
-26.133 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#0

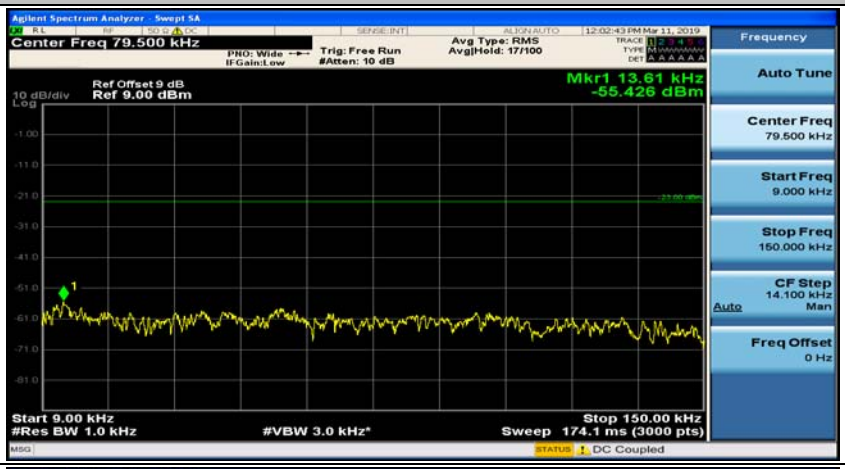

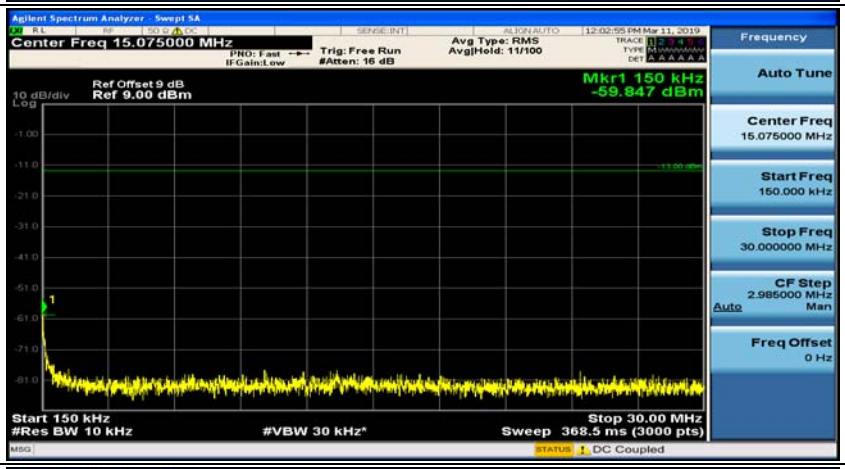

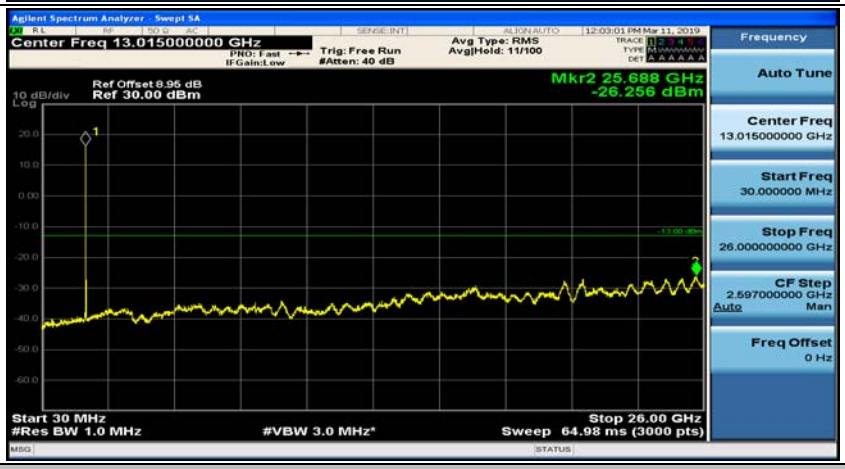

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#37

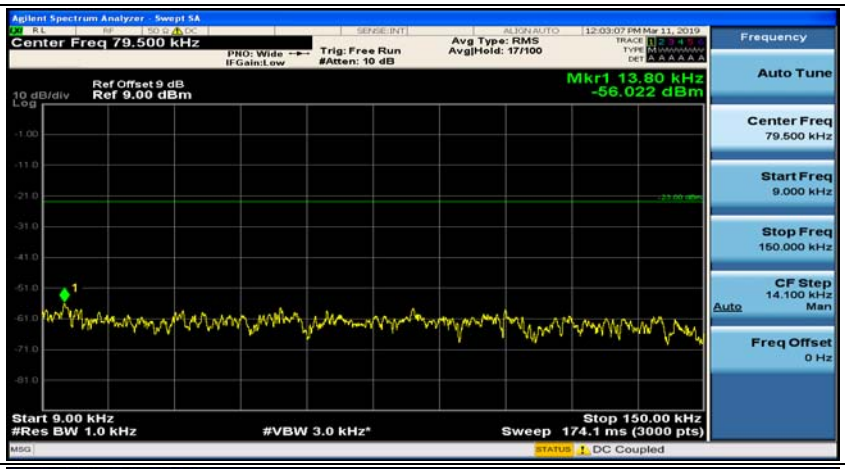

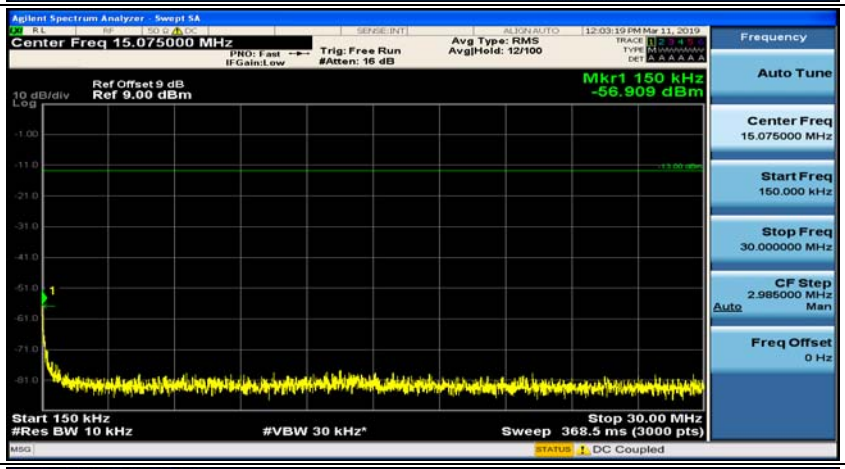

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#74

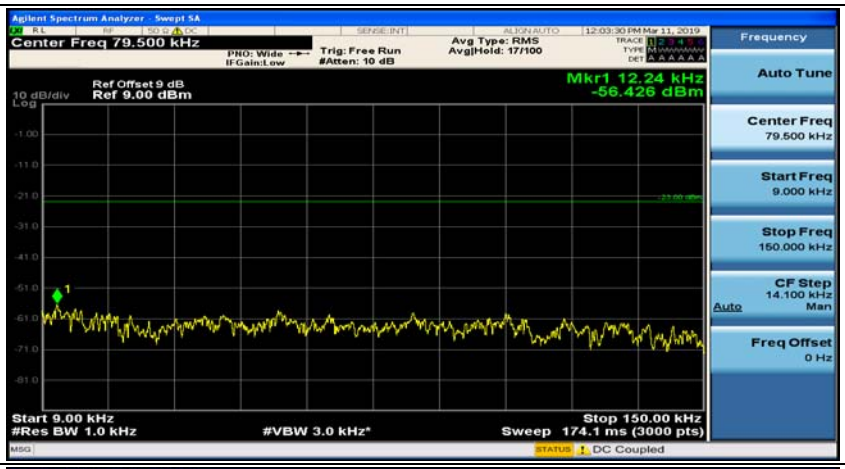
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:03:30 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 12.24 kHz
-56.426 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

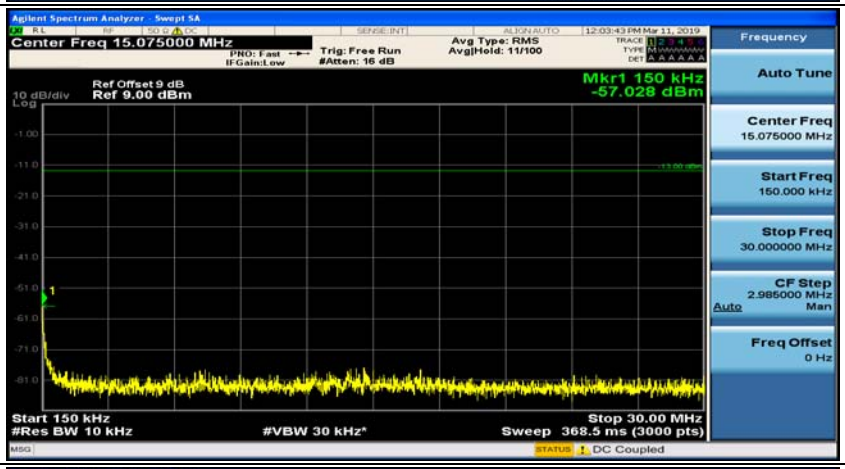
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
12:03:43 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.028 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

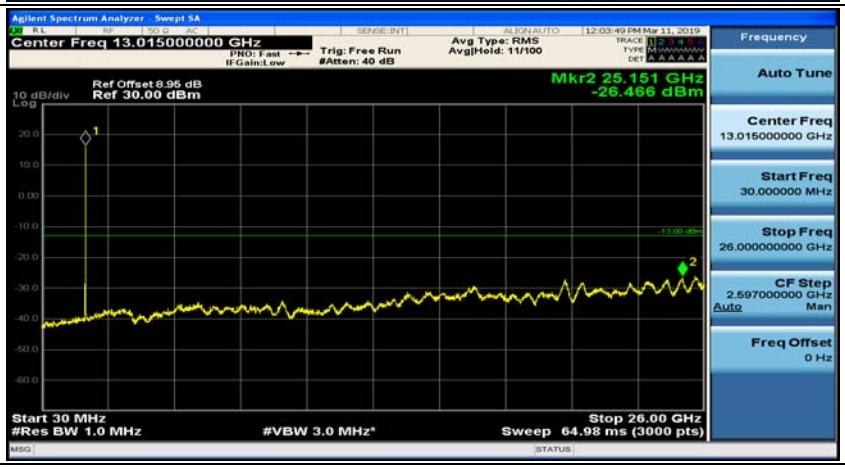
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:03:49 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.151 GHz
-26.466 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 20 MHz

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#0

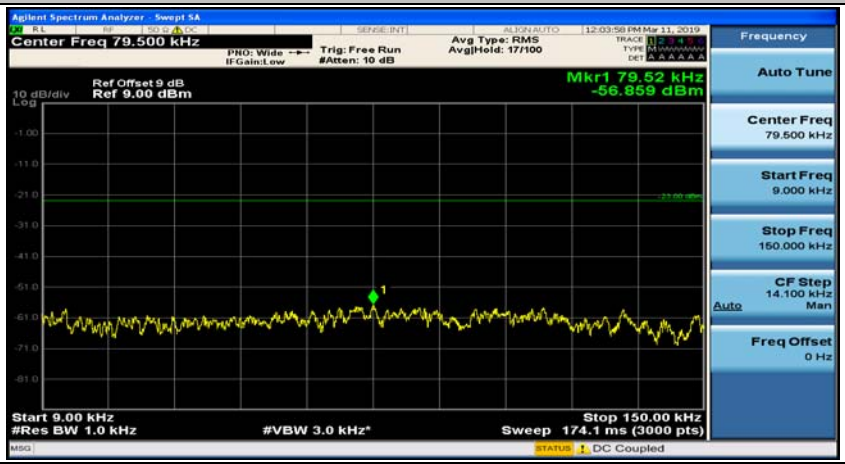

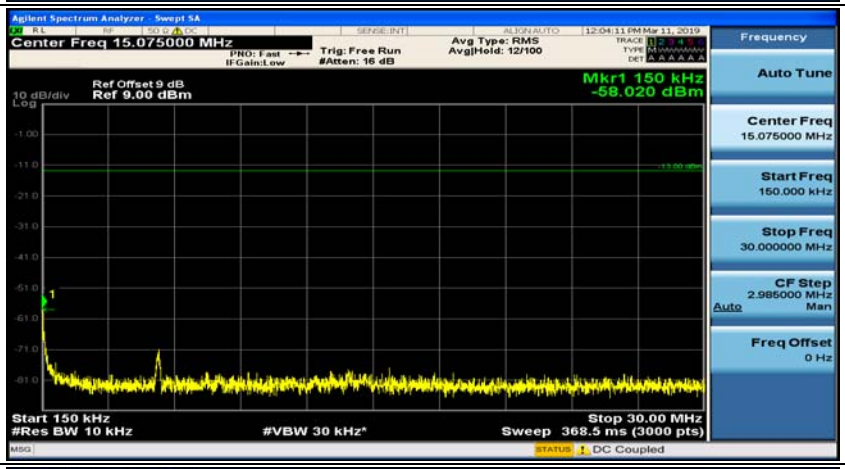

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#49

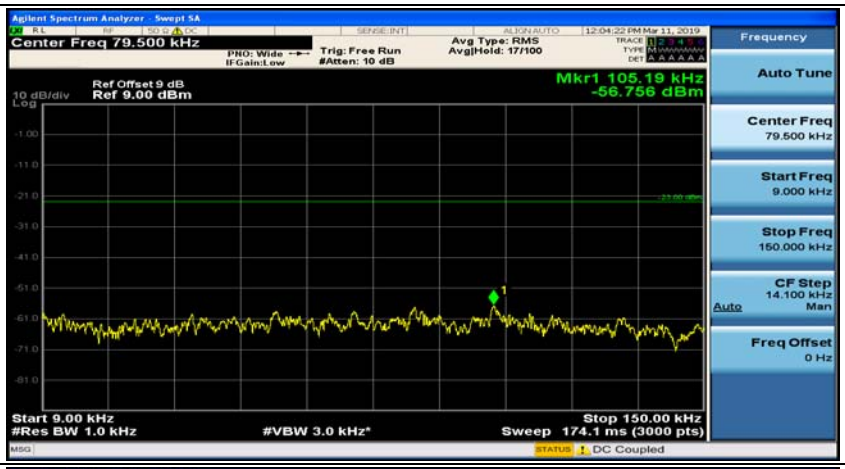

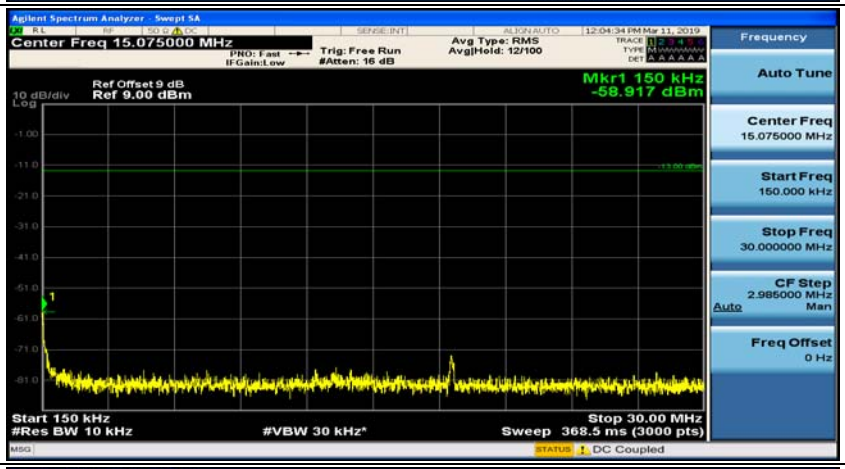

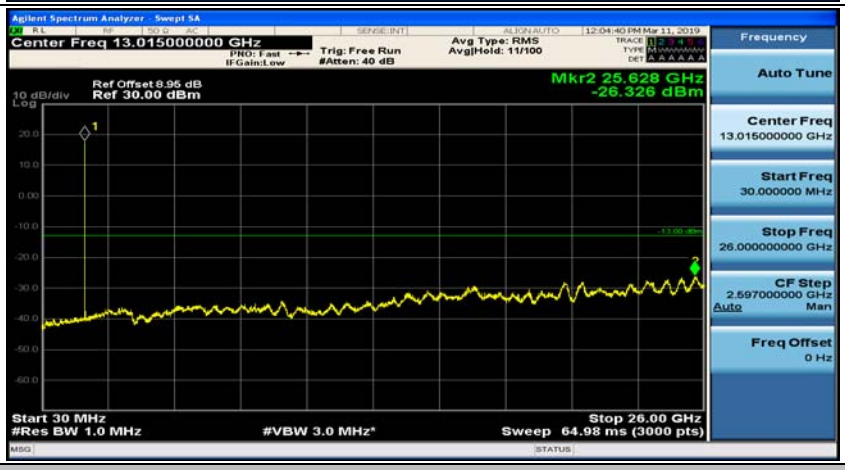

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#99

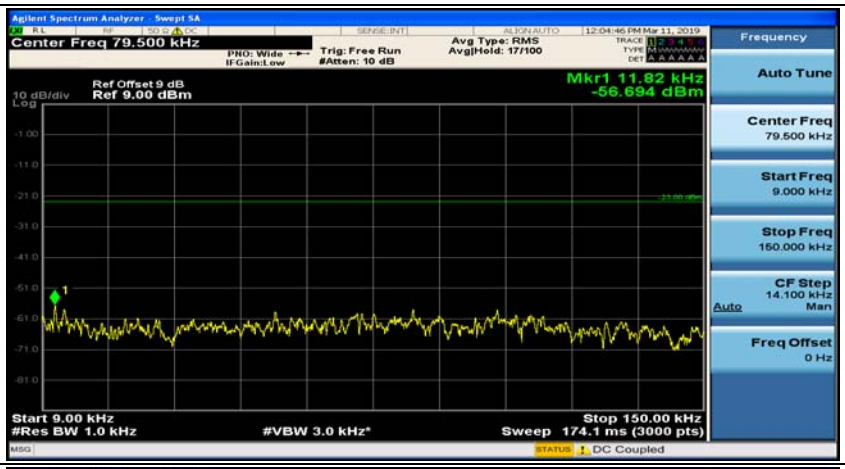
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:04:46 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 11.82 kHz
-56.694 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

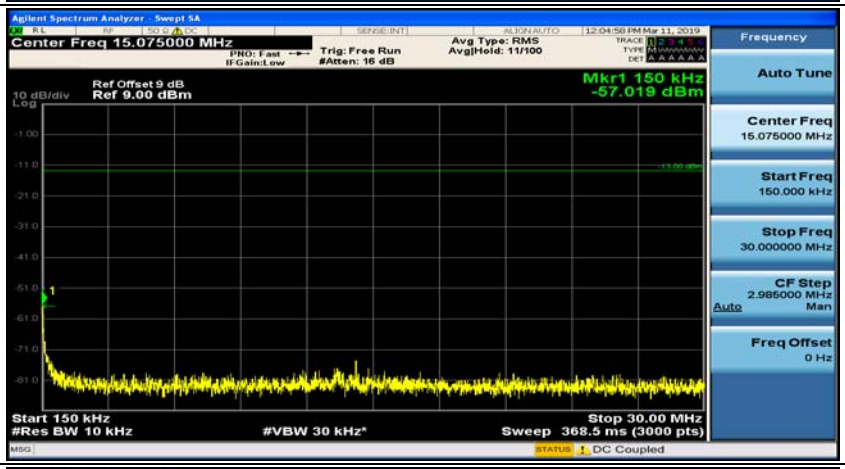
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
12:04:58 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.019 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

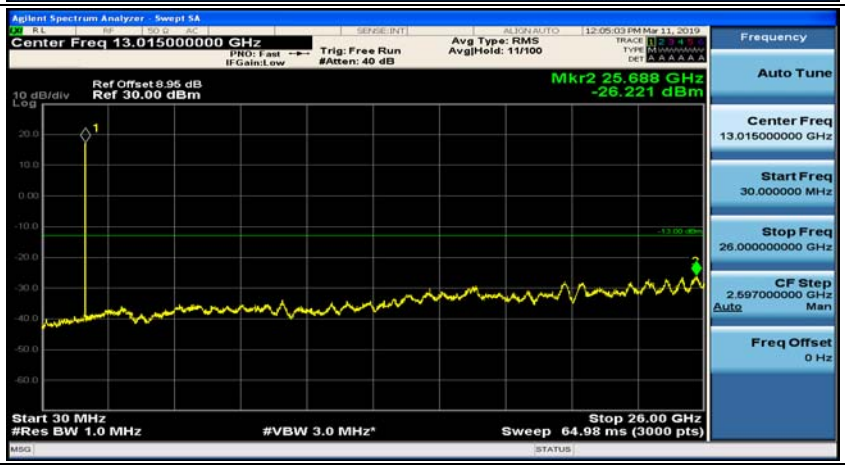
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:05:03 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.688 GHz
-26.221 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#0

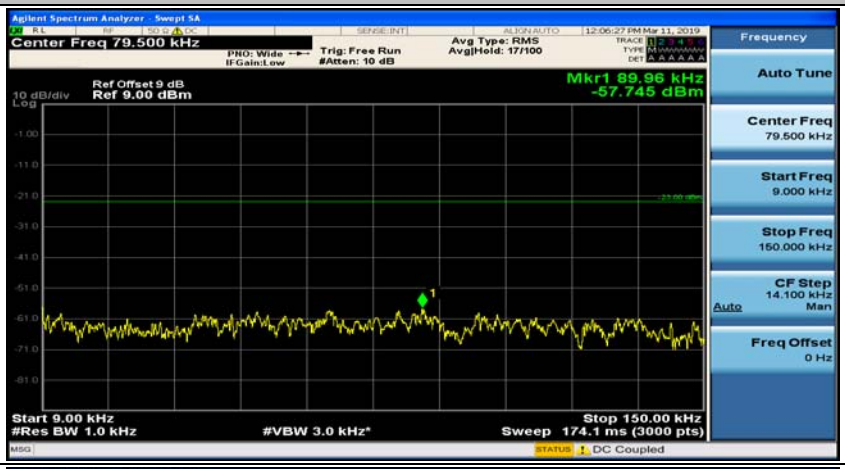

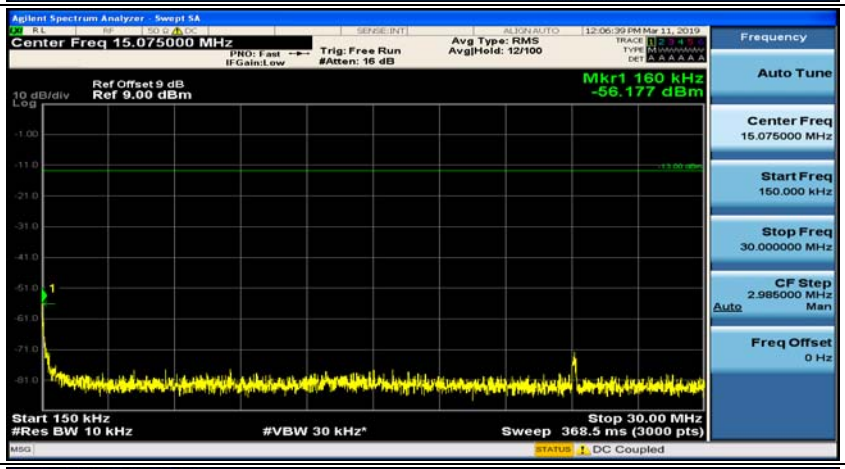

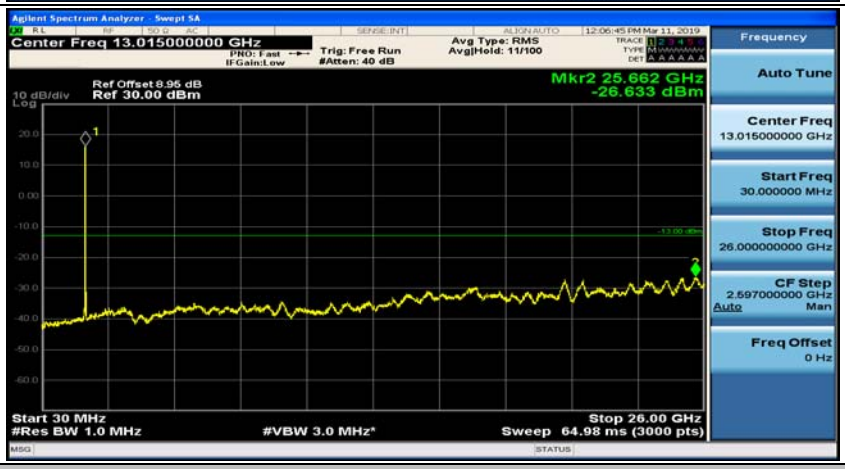

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#49

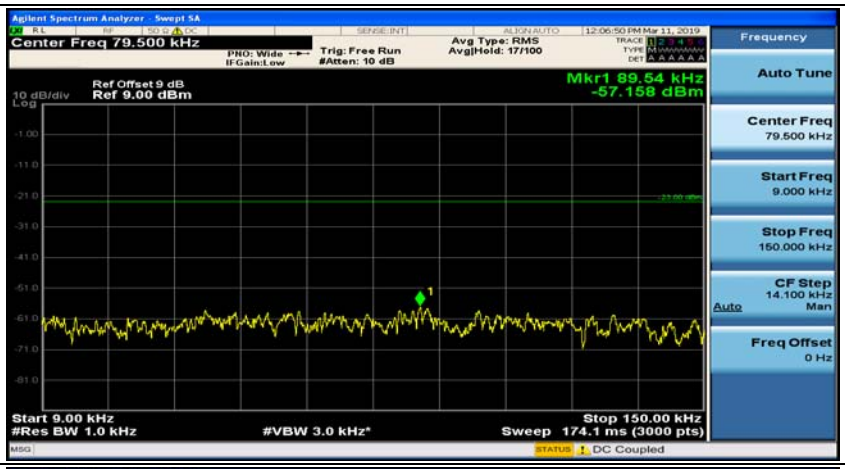

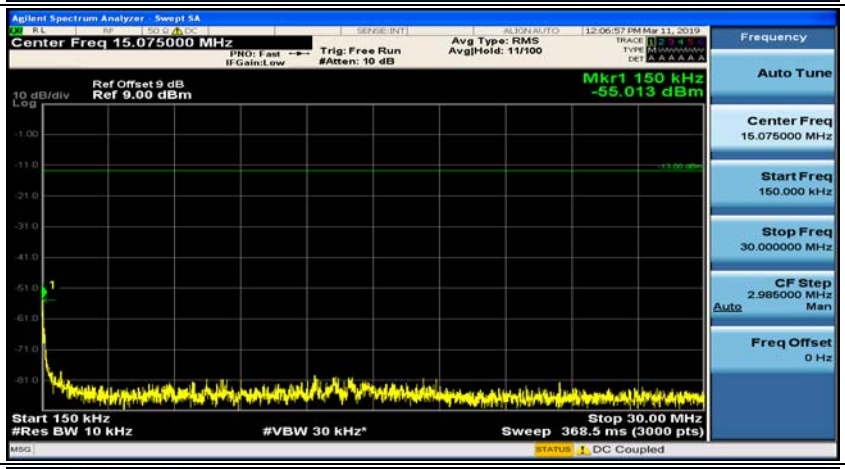

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#99

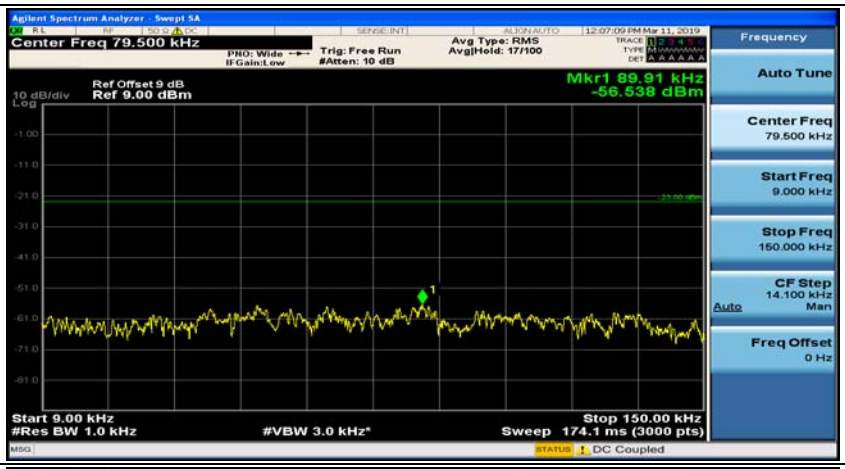
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:07:09 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 89.91 kHz
-56.538 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

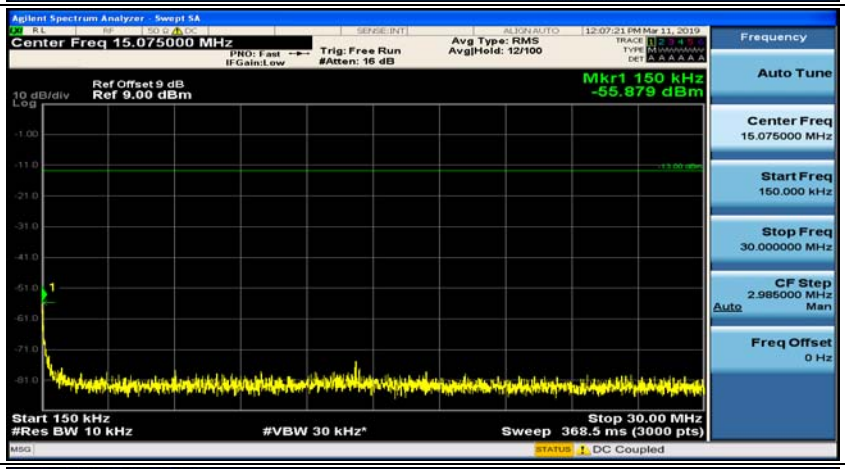
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:07:21 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-55.879 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

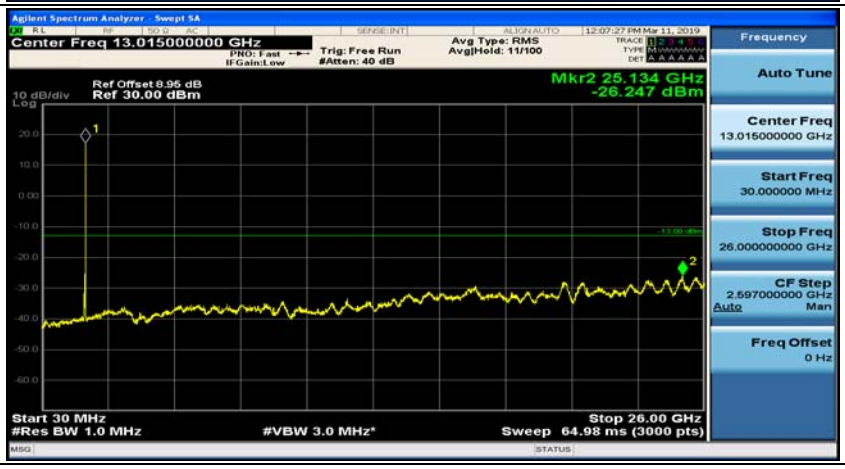
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:07:27 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.134 GHz
-26.247 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#0

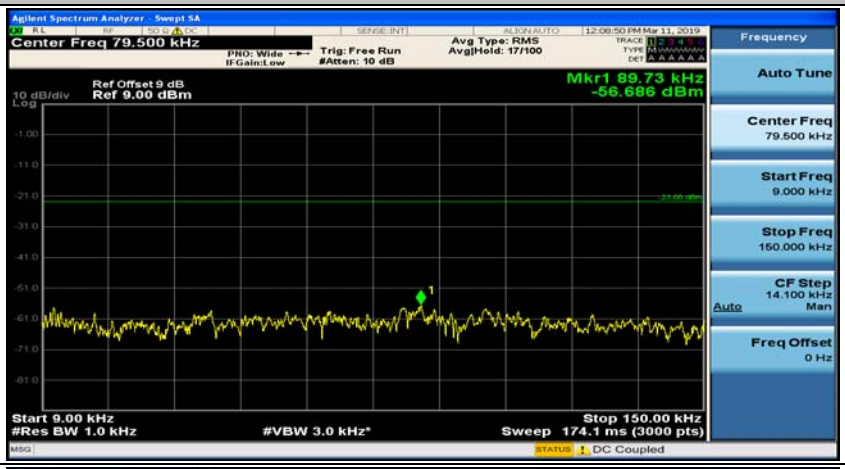

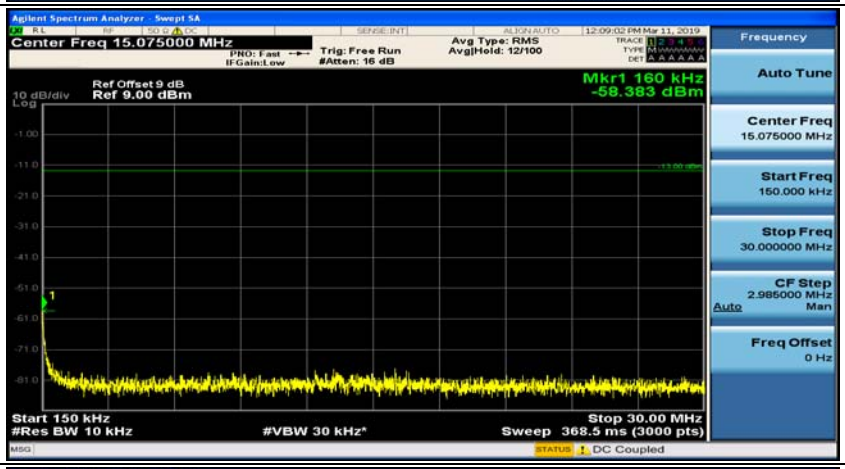

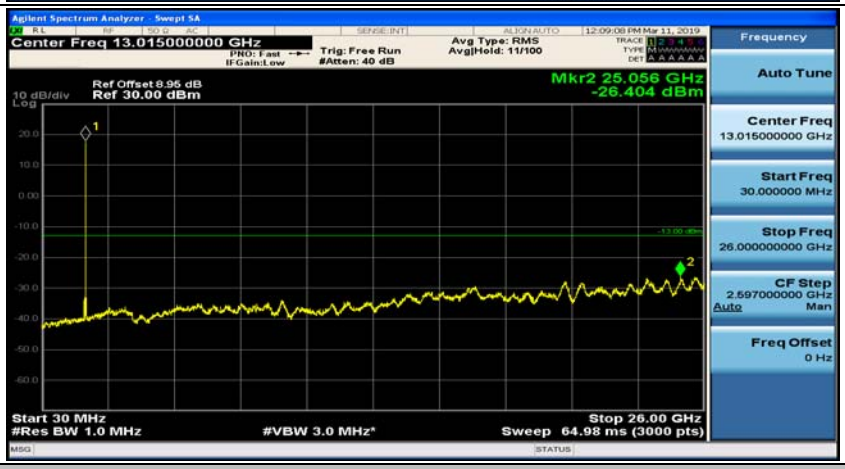

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#49

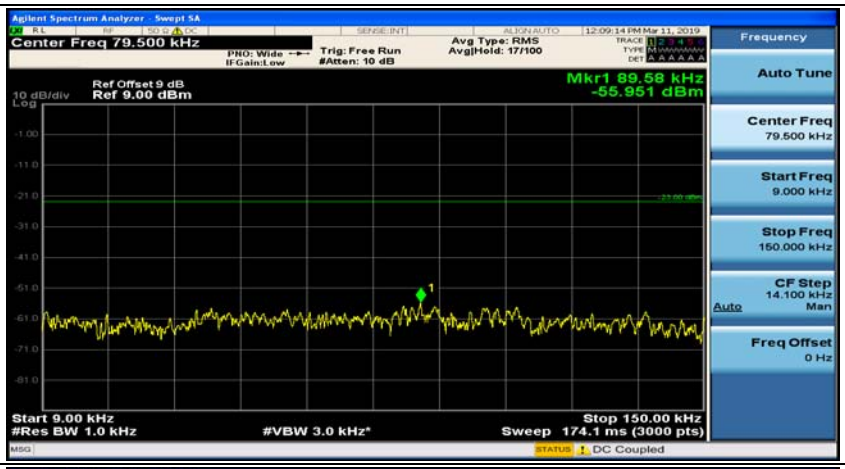

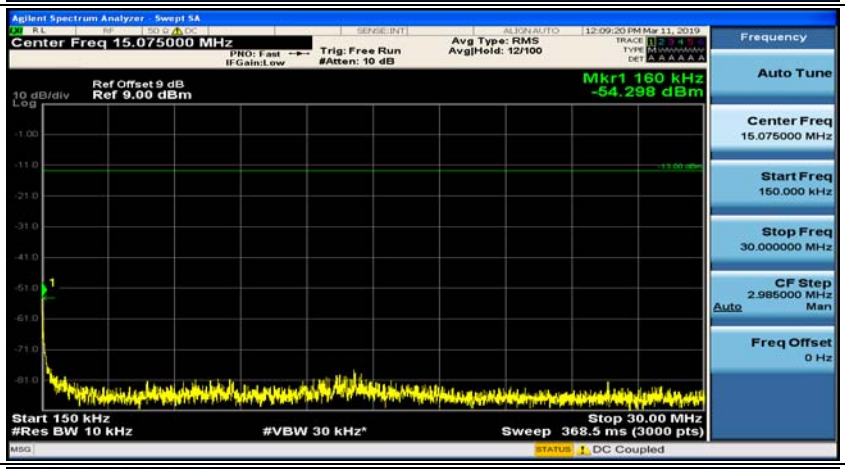

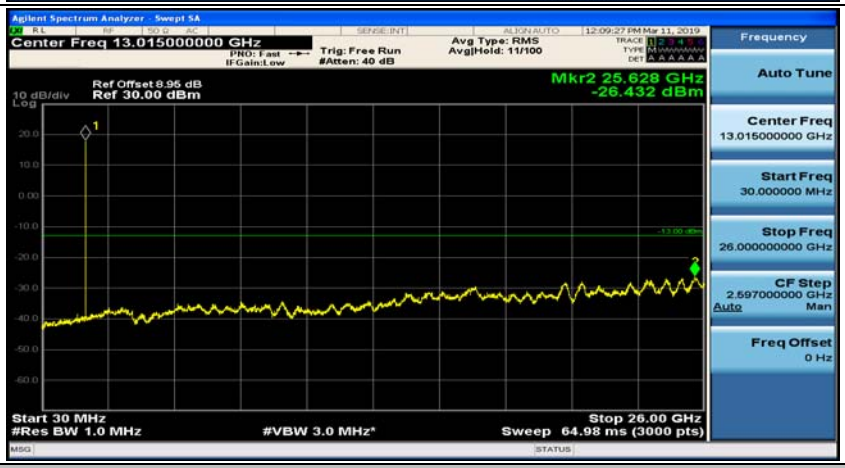

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#99

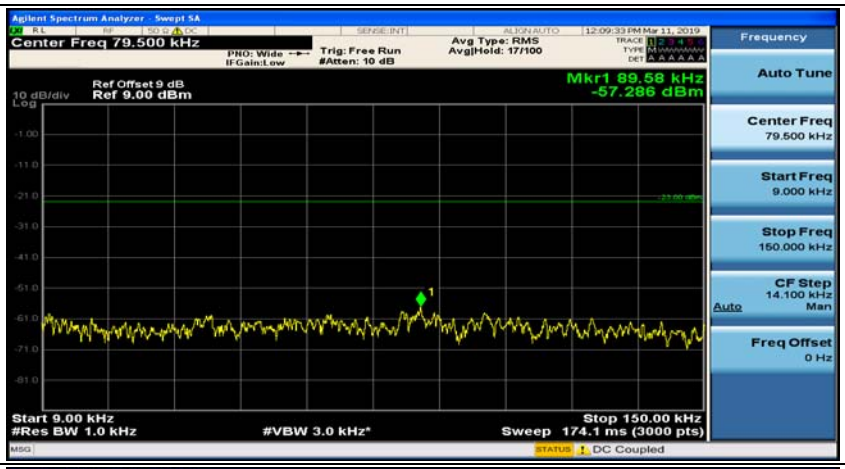
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:09:33 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 89.58 kHz
-57.286 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

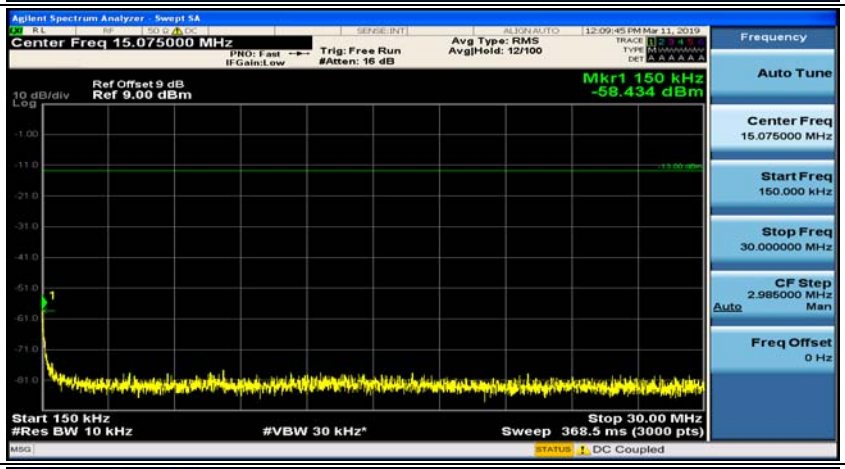
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:09:45 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-58.434 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

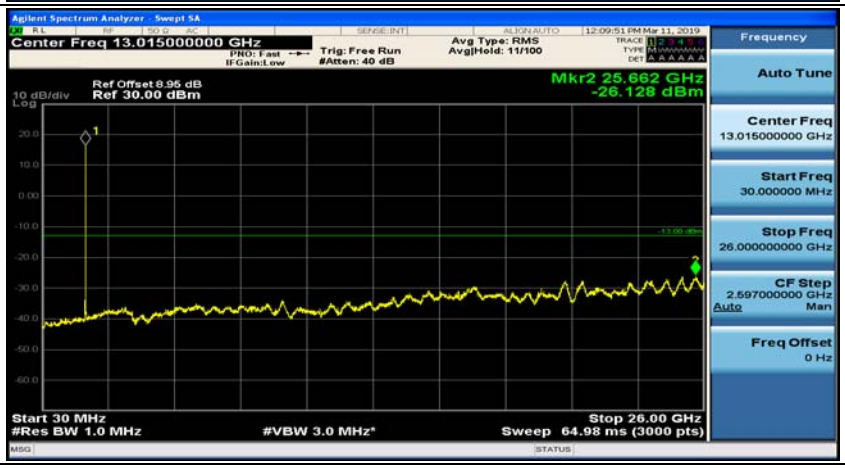
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:09:51 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.662 GHz
-26.128 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#0

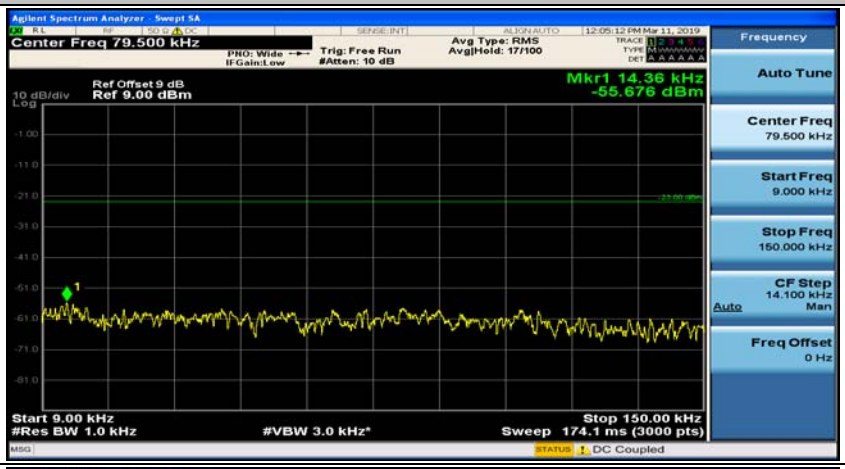

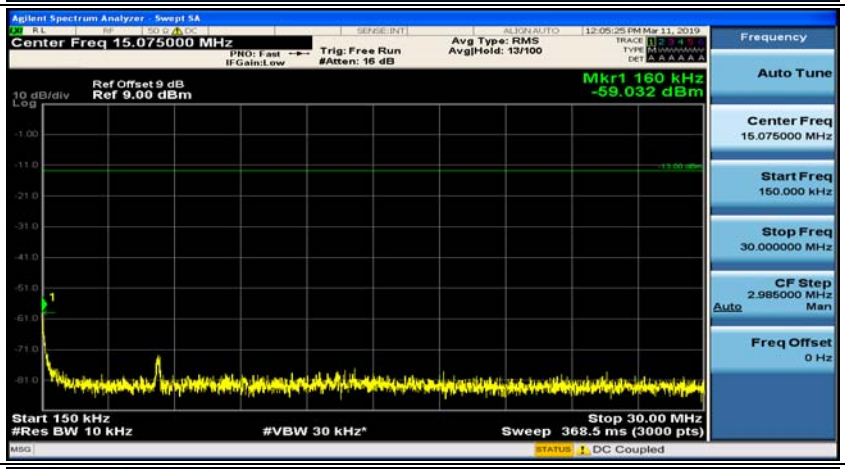

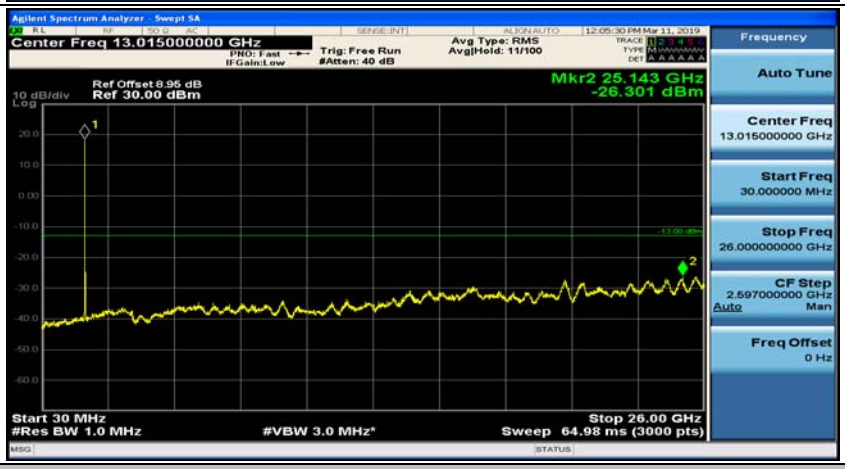

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#49

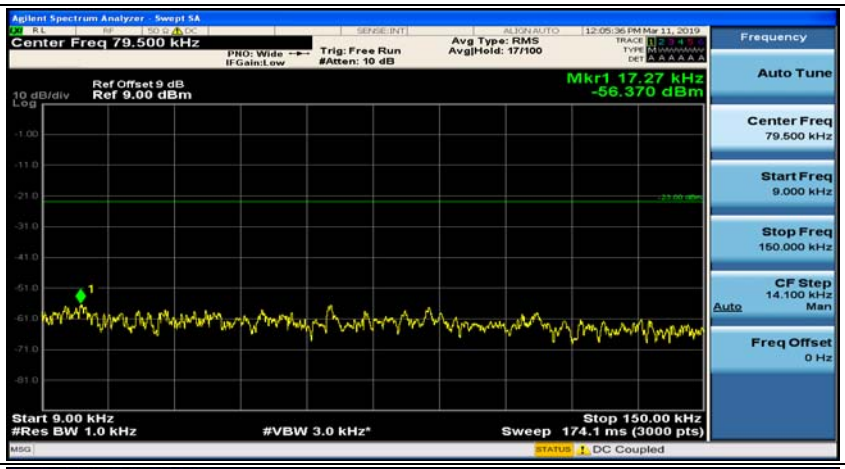

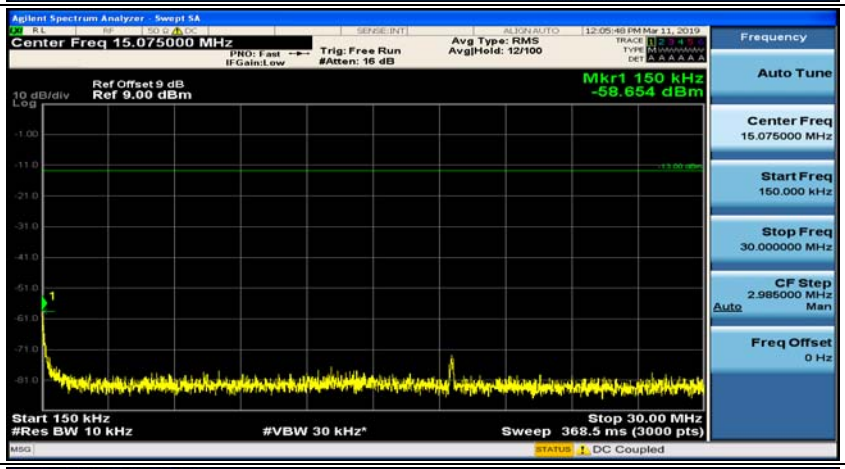

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#99

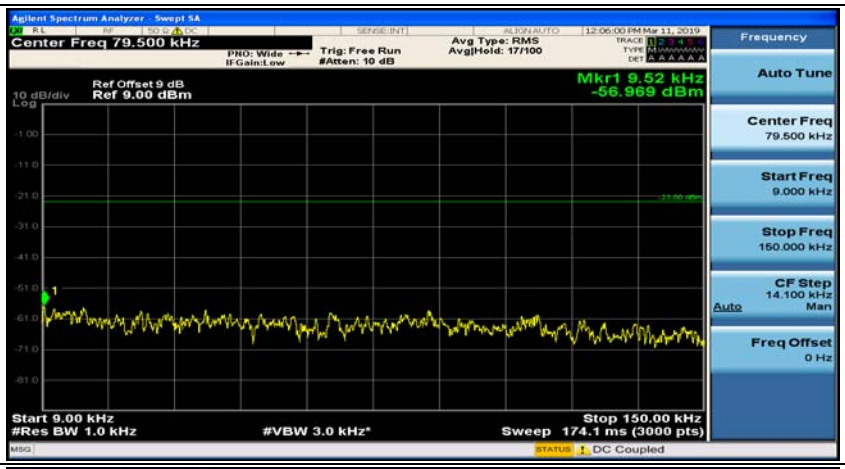
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:06:00 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 9.52 kHz
-56.969 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

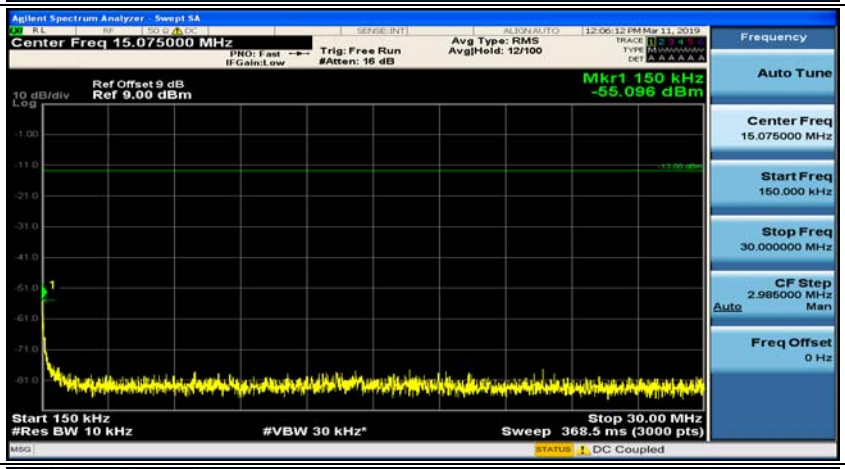
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:06:12 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-55.096 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:06:18 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.654 GHz
-26.388 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#0

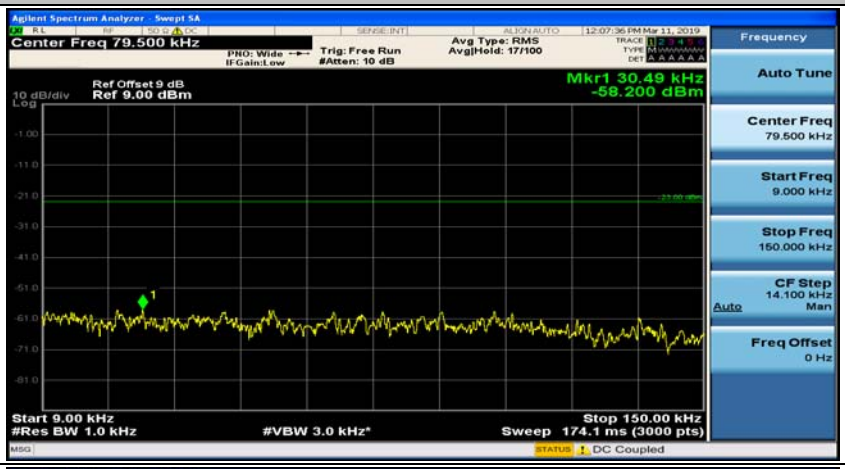

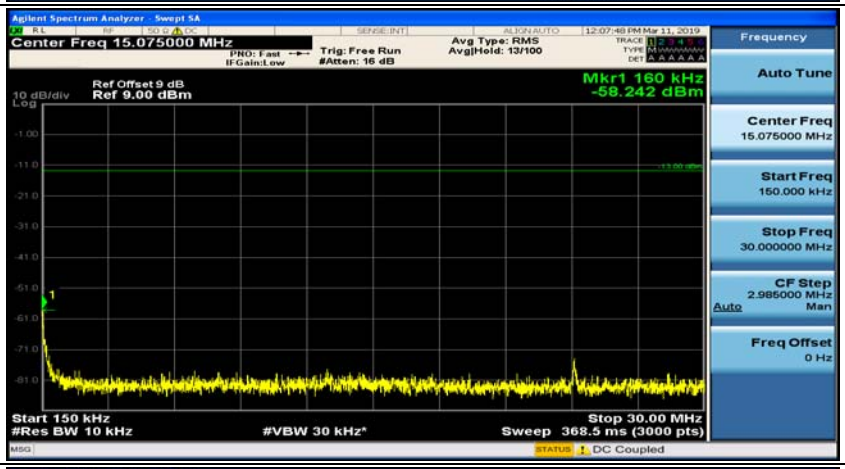

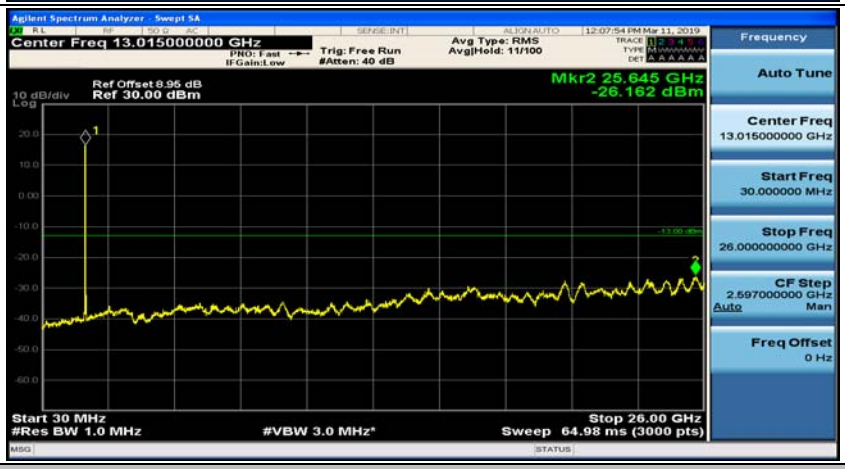

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#49

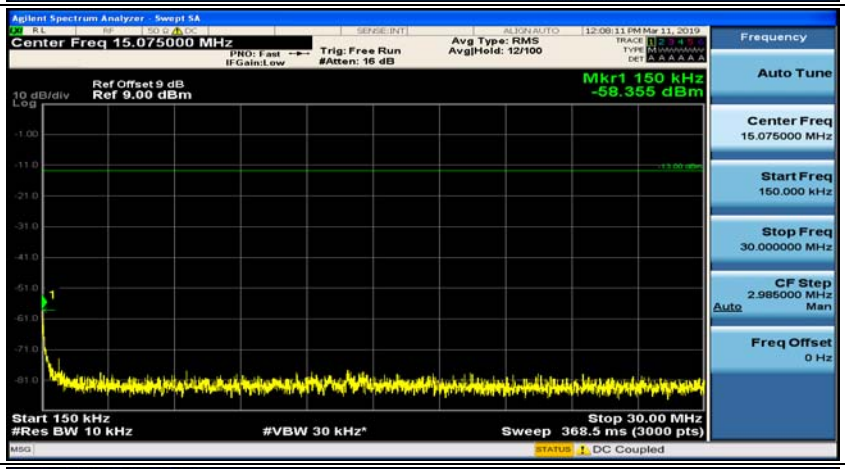

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#99

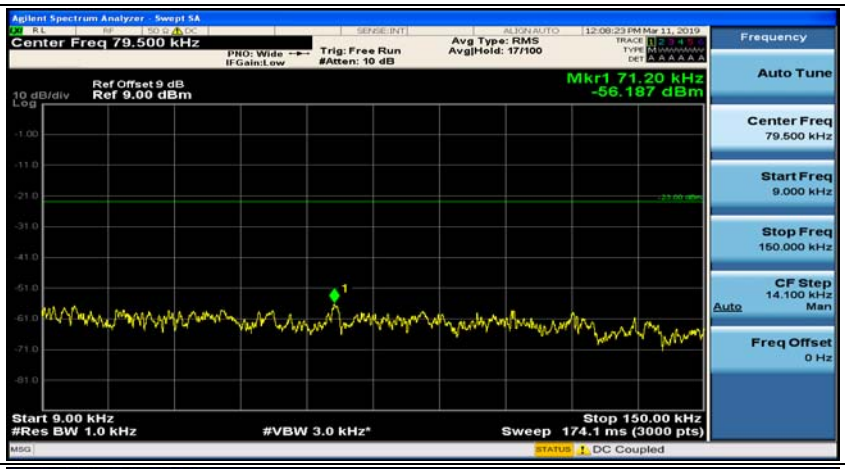
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:08:23 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 71.20 kHz
-56.187 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

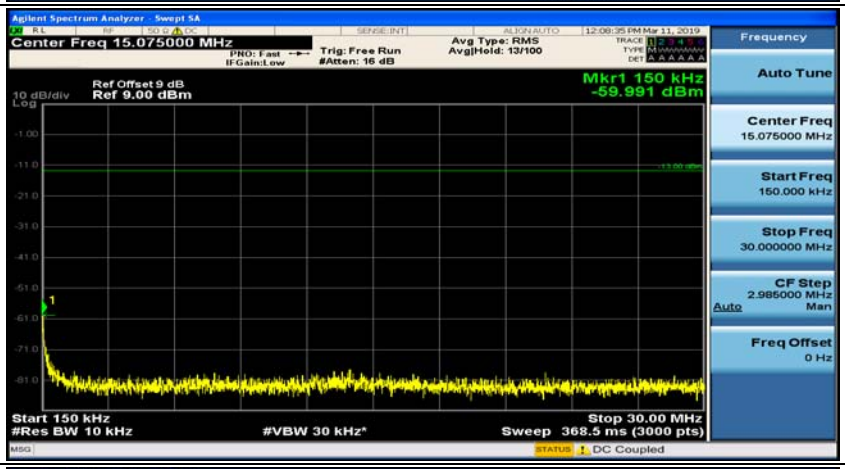
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
12:08:35 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-59.991 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

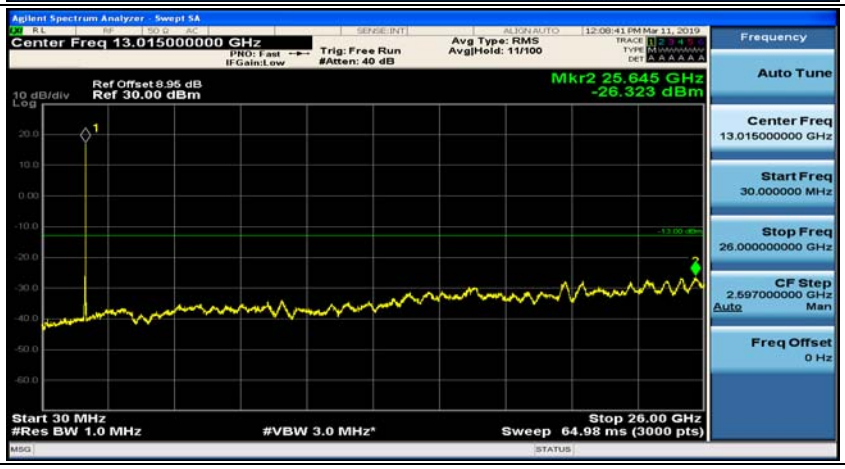
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:08:41 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.645 GHz
-26.323 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#0

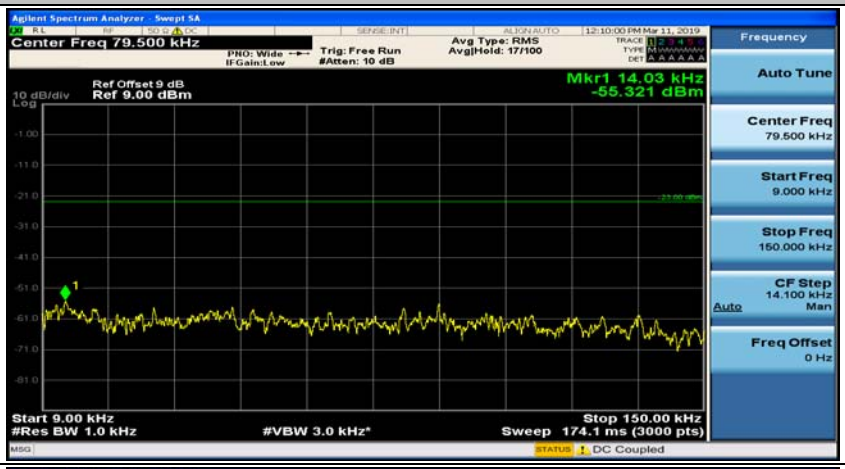

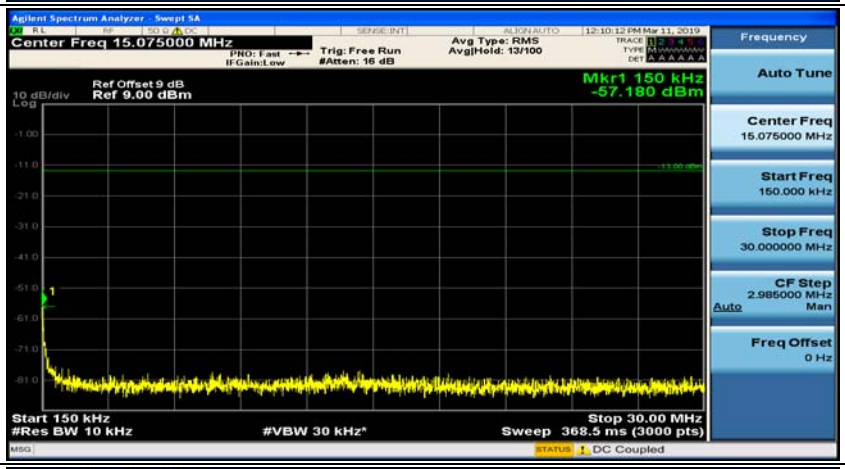

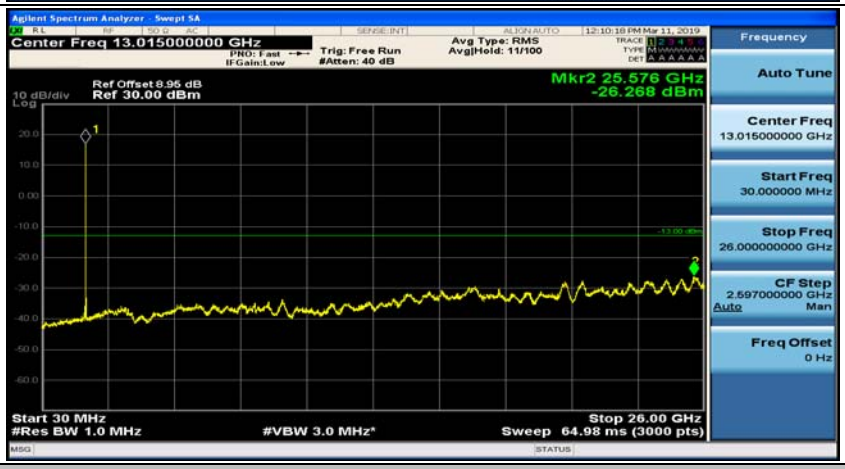

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#49

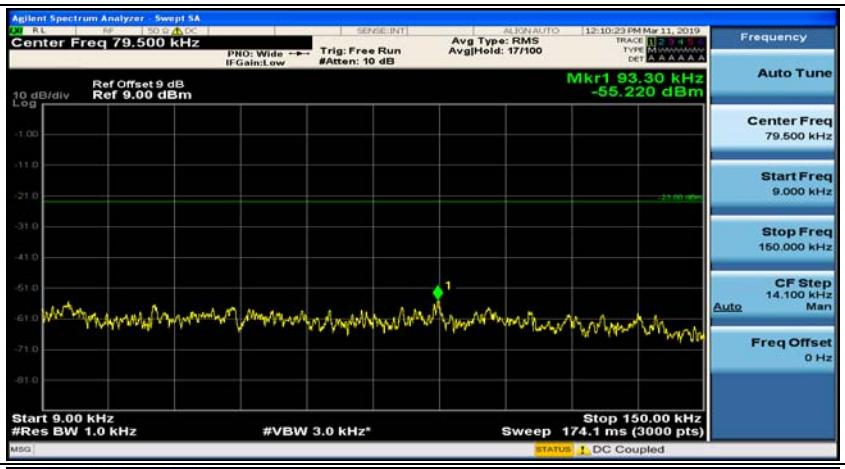

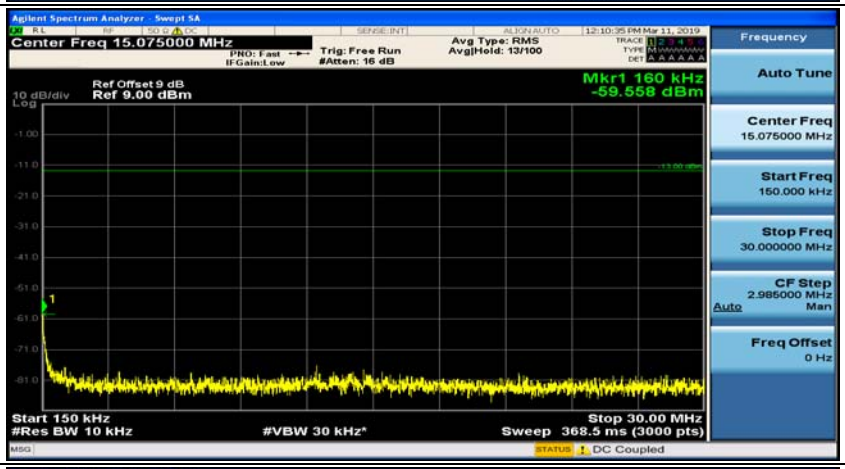

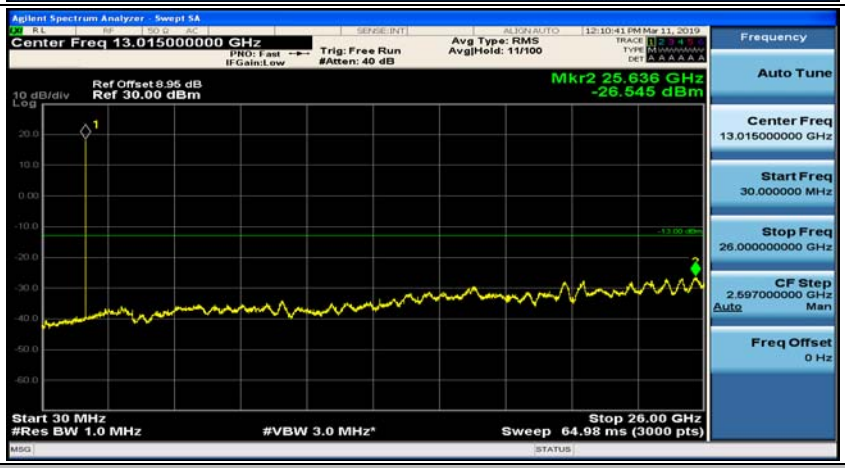

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#99

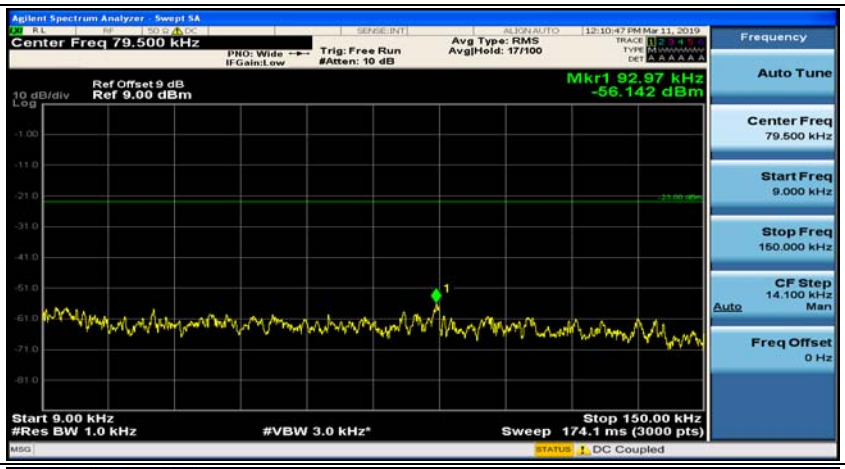
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:10:47 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 92.97 kHz
-56.142 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

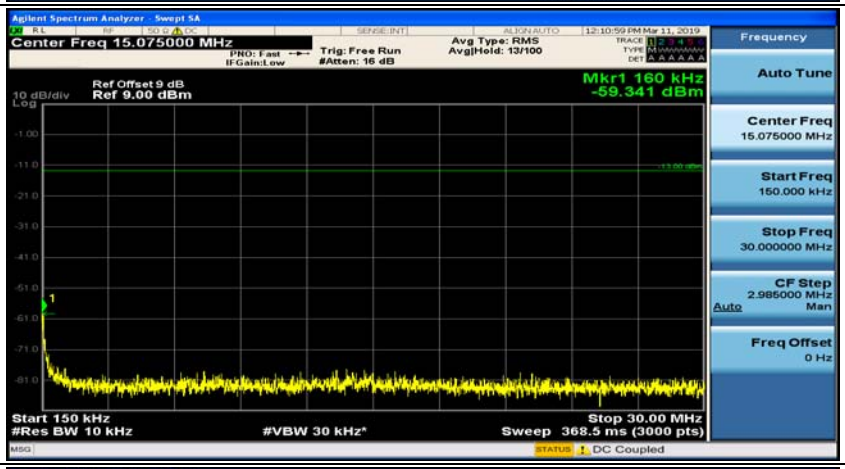
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
12:10:59 PM Mar 11, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-59.341 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

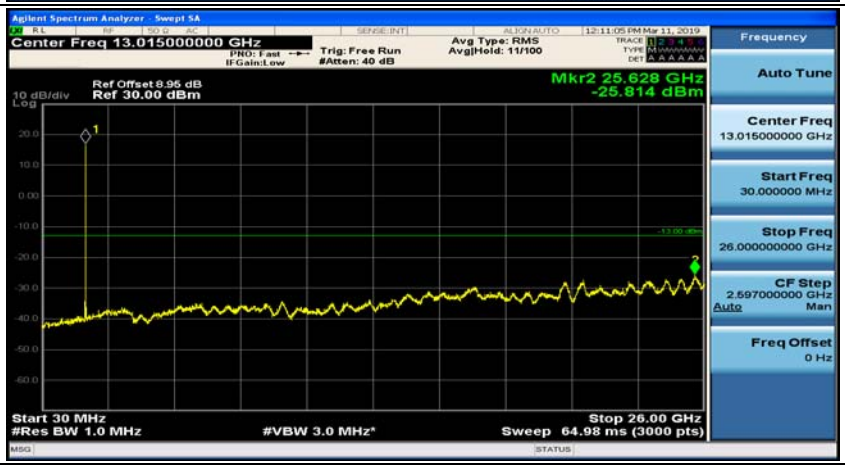
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:11:05 PM Mar 11, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.628 GHz
-25.814 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Appendix F: Frequency Stability

Test Result

Channel Bandwidth: 1.4 MHz

Channel Bandwidth: 1.4 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	2.05	0.001198	± 2.5	PASS
		VN	TN	3.01	0.001760	± 2.5	PASS
		VH	TN	4.39	0.002566	± 2.5	PASS
	MCH	VL	TN	2.48	0.001431	± 2.5	PASS
		VN	TN	2	0.001154	± 2.5	PASS
		VH	TN	-1.74	-0.001004	± 2.5	PASS
	HCH	VL	TN	4.04	0.002303	± 2.5	PASS
		VN	TN	-0.22	-0.000125	± 2.5	PASS
		VH	TN	-0.58	-0.000331	± 2.5	PASS
16QAM	LCH	VL	TN	1.18	0.000690	± 2.5	PASS
		VN	TN	-1.9	-0.001111	± 2.5	PASS
		VH	TN	0.77	0.000450	± 2.5	PASS
	MCH	VL	TN	4.6	0.002655	± 2.5	PASS
		VN	TN	4.19	0.002418	± 2.5	PASS
		VH	TN	4.94	0.002851	± 2.5	PASS
	HCH	VL	TN	4.71	0.002685	± 2.5	PASS
		VN	TN	2.81	0.001602	± 2.5	PASS
		VH	TN	0.07	0.000040	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	1.89	0.001105	± 2.5	PASS
		VN	-20	-0.51	-0.000298	± 2.5	PASS
		VN	-10	-1.38	-0.000807	± 2.5	PASS
		VN	0	4.15	0.002426	± 2.5	PASS
		VN	10	-0.12	-0.000070	± 2.5	PASS
		VN	20	1.2	0.000701	± 2.5	PASS
		VN	30	4.01	0.002344	± 2.5	PASS
		VN	40	3.72	0.002175	± 2.5	PASS
		VN	50	2	0.001169	± 2.5	PASS
	MCH	VN	-30	-0.93	-0.000537	± 2.5	PASS

		VN	-20	1.25	0.000722	± 2.5	PASS
		VN	-10	2.07	0.001195	± 2.5	PASS
		VN	0	0.17	0.000098	± 2.5	PASS
		VN	10	0.67	0.000387	± 2.5	PASS
		VN	20	0.22	0.000127	± 2.5	PASS
		VN	30	-1.38	-0.000797	± 2.5	PASS
		VN	40	3.74	0.002159	± 2.5	PASS
		VN	50	3.25	0.001876	± 2.5	PASS
	HCH	VN	-30	1.61	0.000918	± 2.5	PASS
		VN	-20	4.42	0.002520	± 2.5	PASS
		VN	-10	1.23	0.000701	± 2.5	PASS
		VN	0	-1.88	-0.001072	± 2.5	PASS
		VN	10	1.89	0.001077	± 2.5	PASS
		VN	20	-1.66	-0.000946	± 2.5	PASS
		VN	30	1.66	0.000946	± 2.5	PASS
		VN	40	2.14	0.001220	± 2.5	PASS
		VN	50	-0.48	-0.000274	± 2.5	PASS
16QAM	LCH	VN	-30	2.15	0.001257	± 2.5	PASS
		VN	-20	2.14	0.001251	± 2.5	PASS
		VN	-10	3.16	0.001847	± 2.5	PASS
		VN	0	4.58	0.002677	± 2.5	PASS
		VN	10	4.64	0.002712	± 2.5	PASS
		VN	20	4.26	0.002490	± 2.5	PASS
		VN	30	4.93	0.002882	± 2.5	PASS
		VN	40	3.02	0.001765	± 2.5	PASS
		VN	50	0.64	0.000374	± 2.5	PASS
	MCH	VN	-30	2.77	0.001579	± 2.5	PASS
		VN	-20	1.97	0.001123	± 2.5	PASS
		VN	-10	-0.01	-0.000006	± 2.5	PASS
		VN	0	-0.38	-0.000217	± 2.5	PASS
		VN	10	-0.46	-0.000262	± 2.5	PASS
		VN	20	4.02	0.002292	± 2.5	PASS
		VN	30	-0.09	-0.000051	± 2.5	PASS
		VN	40	-1.98	-0.001129	± 2.5	PASS
		VN	50	1.32	0.000752	± 2.5	PASS
	HCH	VN	-30	3.77	0.002149	± 2.5	PASS
		VN	-20	3.51	0.002001	± 2.5	PASS
		VN	-10	4.34	0.002474	± 2.5	PASS
		VN	0	1.25	0.000713	± 2.5	PASS
		VN	10	3.03	0.001727	± 2.5	PASS
		VN	20	0.11	0.000063	± 2.5	PASS

		VN	30	3.03	0.001727	± 2.5	PASS
		VN	40	3.15	0.001796	± 2.5	PASS
		VN	50	-1.23	-0.000701	± 2.5	PASS

Channel Bandwidth: 3 MHz

Channel Bandwidth: 3 MHz+							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	3.89	0.002273	± 2.5	PASS
		VN	TN	1.22	0.000713	± 2.5	PASS
		VH	TN	-1.26	-0.000736	± 2.5	PASS
	MCH	VL	TN	-1.33	-0.000768	± 2.5	PASS
		VN	TN	2.73	0.001576	± 2.5	PASS
		VH	TN	3.18	0.001835	± 2.5	PASS
	HCH	VL	TN	-1.8	-0.001027	± 2.5	PASS
		VN	TN	-1.05	-0.000599	± 2.5	PASS
		VH	TN	-1.19	-0.000679	± 2.5	PASS
16QAM	LCH	VL	TN	-0.94	-0.000549	± 2.5	PASS
		VN	TN	4.56	0.002664	± 2.5	PASS
		VH	TN	0.58	0.000339	± 2.5	PASS
	MCH	VL	TN	4.96	0.002863	± 2.5	PASS
		VN	TN	0.35	0.000202	± 2.5	PASS
		VH	TN	-0.1	-0.000058	± 2.5	PASS
	HCH	VL	TN	-1.28	-0.000730	± 2.5	PASS
		VN	TN	0.31	0.000177	± 2.5	PASS
		VH	TN	-0.49	-0.000279	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	4.95	0.002892	± 2.5	PASS
		VN	-20	3.15	0.001840	± 2.5	PASS
		VN	-10	-1.84	-0.001075	± 2.5	PASS
		VN	0	-0.58	-0.000339	± 2.5	PASS
		VN	10	4.99	0.002916	± 2.5	PASS
		VN	20	1.62	0.000947	± 2.5	PASS
		VN	30	4.61	0.002694	± 2.5	PASS
		VN	40	3.08	0.001800	± 2.5	PASS
		VN	50	3.35	0.001957	± 2.5	PASS
	MCH	VN	-30	-0.44	-0.000254	± 2.5	PASS
		VN	-20	4.92	0.002840	± 2.5	PASS

		VN	-10	-0.8	-0.000462	± 2.5	PASS
		VN	0	0.6	0.000346	± 2.5	PASS
		VN	10	2.42	0.001397	± 2.5	PASS
		VN	20	0.03	0.000017	± 2.5	PASS
		VN	30	0.16	0.000092	± 2.5	PASS
		VN	40	-0.2	-0.000115	± 2.5	PASS
		VN	50	3.49	0.002014	± 2.5	PASS
	HCH	VN	-30	0.96	0.000547	± 2.5	PASS
		VN	-20	2.48	0.001414	± 2.5	PASS
		VN	-10	3.67	0.002093	± 2.5	PASS
		VN	0	1.84	0.001049	± 2.5	PASS
		VN	10	1.5	0.000855	± 2.5	PASS
		VN	20	-1	-0.000570	± 2.5	PASS
		VN	30	0.46	0.000262	± 2.5	PASS
		VN	40	2.87	0.001637	± 2.5	PASS
		VN	50	-0.38	-0.000217	± 2.5	PASS
QPSK	LCH	VN	-30	0.05	0.000029	± 2.5	PASS
		VN	-20	-1.4	-0.000808	± 2.5	PASS
		VN	-10	4.42	0.002551	± 2.5	PASS
		VN	0	3.77	0.002176	± 2.5	PASS
		VN	10	3.51	0.002026	± 2.5	PASS
		VN	20	0.89	0.000514	± 2.5	PASS
		VN	30	3.57	0.002061	± 2.5	PASS
		VN	40	3.53	0.002038	± 2.5	PASS
		VN	50	3.32	0.001916	± 2.5	PASS
	MCH	VN	-30	4.08	0.002327	± 2.5	PASS
		VN	-20	4.15	0.002367	± 2.5	PASS
		VN	-10	0.96	0.000547	± 2.5	PASS
		VN	0	-1.5	-0.000855	± 2.5	PASS
		VN	10	3.7	0.002110	± 2.5	PASS
		VN	20	-1.96	-0.001118	± 2.5	PASS
		VN	30	-1.56	-0.000890	± 2.5	PASS
		VN	40	1.35	0.000770	± 2.5	PASS
		VN	50	4.07	0.002321	± 2.5	PASS
	HCH	VN	-30	4.4	0.002509	± 2.5	PASS
		VN	-20	1.42	0.000810	± 2.5	PASS
		VN	-10	4.81	0.002743	± 2.5	PASS
		VN	0	3.4	0.001939	± 2.5	PASS
		VN	10	3.26	0.001859	± 2.5	PASS
		VN	20	1.81	0.001032	± 2.5	PASS
		VN	30	-1.05	-0.000599	± 2.5	PASS

		VN	40	-1.98	-0.001129	± 2.5	PASS
		VN	50	2.83	0.001614	± 2.5	PASS

Channel Bandwidth: 5 MHz

Channel Bandwidth: 5 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	-1.41	-0.000823	± 2.5	PASS
		VN	TN	1.03	0.000601	± 2.5	PASS
		VH	TN	-0.33	-0.000193	± 2.5	PASS
	MCH	VL	TN	4.17	0.002407	± 2.5	PASS
		VN	TN	4.88	0.002817	± 2.5	PASS
		VH	TN	4.34	0.002505	± 2.5	PASS
	HCH	VL	TN	4.72	0.002693	± 2.5	PASS
		VN	TN	-1.64	-0.000936	± 2.5	PASS
		VH	TN	3.69	0.002106	± 2.5	PASS
16QAM	LCH	VL	TN	1.63	0.000952	± 2.5	PASS
		VN	TN	3.23	0.001886	± 2.5	PASS
		VH	TN	-0.55	-0.000321	± 2.5	PASS
	MCH	VL	TN	2.27	0.001310	± 2.5	PASS
		VN	TN	0.16	0.000092	± 2.5	PASS
		VH	TN	-1.56	-0.000900	± 2.5	PASS
	HCH	VL	TN	0	0.000000	± 2.5	PASS
		VN	TN	3.04	0.001735	± 2.5	PASS
		VH	TN	1.5	0.000856	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	0.02	0.000012	± 2.5	PASS
		VN	-20	2.54	0.001483	± 2.5	PASS
		VN	-10	1.73	0.001010	± 2.5	PASS
		VN	0	-0.35	-0.000204	± 2.5	PASS
		VN	10	3.84	0.002242	± 2.5	PASS
		VN	20	-1.42	-0.000829	± 2.5	PASS
		VN	30	1.74	0.001016	± 2.5	PASS
		VN	40	4.24	0.002476	± 2.5	PASS
		VN	50	0.99	0.000578	± 2.5	PASS
	MCH	VN	-30	-0.14	-0.000081	± 2.5	PASS
		VN	-20	0.8	0.000462	± 2.5	PASS
		VN	-10	1.63	0.000941	± 2.5	PASS

		VN	0	2.79	0.001610	± 2.5	PASS
		VN	10	4.76	0.002747	± 2.5	PASS
		VN	20	0.27	0.000156	± 2.5	PASS
		VN	30	-1.42	-0.000820	± 2.5	PASS
		VN	40	1.89	0.001091	± 2.5	PASS
		VN	50	-1.96	-0.001131	± 2.5	PASS
	HCH	VN	-30	3.4	0.001940	± 2.5	PASS
		VN	-20	0.79	0.000414	± 2.5	PASS
		VN	-10	0.97	0.000509	± 2.5	PASS
		VN	0	0.65	0.000341	± 2.5	PASS
		VN	10	-1.35	-0.000708	± 2.5	PASS
		VN	20	-0.46	-0.000241	± 2.5	PASS
		VN	30	0.69	0.000362	± 2.5	PASS
		VN	40	4.88	0.002558	± 2.5	PASS
		VN	50	2.79	0.001463	± 2.5	PASS
16QAM	LCH	VN	-30	-1.09	-0.000629	± 2.5	PASS
		VN	-20	-1.68	-0.000970	± 2.5	PASS
		VN	-10	2.88	0.001662	± 2.5	PASS
		VN	0	4.73	0.002730	± 2.5	PASS
		VN	10	-0.3	-0.000173	± 2.5	PASS
		VN	20	-0.99	-0.000571	± 2.5	PASS
		VN	30	3.74	0.002159	± 2.5	PASS
		VN	40	0.71	0.000410	± 2.5	PASS
		VN	50	2.36	0.001362	± 2.5	PASS
	MCH	VN	-30	-0.51	-0.000291	± 2.5	PASS
		VN	-20	4.29	0.002448	± 2.5	PASS
		VN	-10	4.51	0.002573	± 2.5	PASS
		VN	0	4.01	0.002288	± 2.5	PASS
		VN	10	1.45	0.000827	± 2.5	PASS
		VN	20	4.57	0.002608	± 2.5	PASS
		VN	30	1.45	0.000827	± 2.5	PASS
		VN	40	4.37	0.002494	± 2.5	PASS
		VN	50	-0.54	-0.000308	± 2.5	PASS
	HCH	VN	-30	3.84	0.002013	± 2.5	PASS
		VN	-20	2.45	0.001284	± 2.5	PASS
		VN	-10	3.4	0.001782	± 2.5	PASS
		VN	0	0.37	0.000194	± 2.5	PASS
		VN	10	3.96	0.002076	± 2.5	PASS
		VN	20	1.23	0.000645	± 2.5	PASS
		VN	30	3.95	0.002071	± 2.5	PASS
		VN	40	3.1	0.001625	± 2.5	PASS

		VN	50	-1.55	-0.000813	± 2.5	PASS

Channel Bandwidth: 10 MHz

Channel Bandwidth: 10 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	2.57	0.001499	± 2.5	PASS
		VN	TN	0.13	0.000076	± 2.5	PASS
		VH	TN	-1.97	-0.001149	± 2.5	PASS
	MCH	VL	TN	0.29	0.000167	± 2.5	PASS
		VN	TN	-0.46	-0.000266	± 2.5	PASS
		VH	TN	3.89	0.002245	± 2.5	PASS
	HCH	VL	TN	-1.14	-0.000651	± 2.5	PASS
		VN	TN	2.41	0.001377	± 2.5	PASS
		VH	TN	3.33	0.001903	± 2.5	PASS
16QAM	LCH	VL	TN	2.67	0.001557	± 2.5	PASS
		VN	TN	2.94	0.001714	± 2.5	PASS
		VH	TN	-1.74	-0.001015	± 2.5	PASS
	MCH	VL	TN	0.55	0.000317	± 2.5	PASS
		VN	TN	3.81	0.002199	± 2.5	PASS
		VH	TN	-0.27	-0.000156	± 2.5	PASS
	HCH	VL	TN	2.28	0.001303	± 2.5	PASS
		VN	TN	0.95	0.000543	± 2.5	PASS
		VH	TN	-0.35	-0.000200	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
16QAM	LCH	VN	-30	3.26	0.001901	± 2.5	PASS
		VN	-20	-0.23	-0.000134	± 2.5	PASS
		VN	-10	3.79	0.002210	± 2.5	PASS
		VN	0	3.07	0.001790	± 2.5	PASS
		VN	10	-0.02	-0.000012	± 2.5	PASS
		VN	20	4.01	0.002338	± 2.5	PASS
		VN	30	4.87	0.002840	± 2.5	PASS
		VN	40	-0.87	-0.000507	± 2.5	PASS
		VN	50	3.66	0.002134	± 2.5	PASS
	MCH	VN	-30	-0.93	-0.000537	± 2.5	PASS
		VN	-20	0.94	0.000543	± 2.5	PASS
		VN	-10	1.69	0.000975	± 2.5	PASS
		VN	0	-0.12	-0.000069	± 2.5	PASS

		VN	10	1.43	0.000825	± 2.5	PASS
		VN	20	3.67	0.002118	± 2.5	PASS
		VN	30	3.06	0.001766	± 2.5	PASS
		VN	40	4.75	0.002742	± 2.5	PASS
		VN	50	2.76	0.001593	± 2.5	PASS
	HCH	VN	-30	-0.46	-0.000263	± 2.5	PASS
		VN	-20	2.98	0.001703	± 2.5	PASS
		VN	-10	2.73	0.001560	± 2.5	PASS
		VN	0	-0.18	-0.000103	± 2.5	PASS
		VN	10	4.01	0.002291	± 2.5	PASS
		VN	20	-0.98	-0.000560	± 2.5	PASS
		VN	30	1.37	0.000783	± 2.5	PASS
		VN	40	2.33	0.001331	± 2.5	PASS
		VN	50	2.04	0.001166	± 2.5	PASS
QPSK	LCH	VN	-30	3.63	0.002095	± 2.5	PASS
		VN	-20	4.01	0.002315	± 2.5	PASS
		VN	-10	2.99	0.001726	± 2.5	PASS
		VN	0	-1.65	-0.000952	± 2.5	PASS
		VN	10	2.8	0.001616	± 2.5	PASS
		VN	20	4.91	0.002834	± 2.5	PASS
		VN	30	0.72	0.000416	± 2.5	PASS
		VN	40	4.63	0.002672	± 2.5	PASS
		VN	50	4.3	0.002482	± 2.5	PASS
	MCH	VN	-30	-1.34	-0.000766	± 2.5	PASS
		VN	-20	-0.56	-0.000320	± 2.5	PASS
		VN	-10	4.9	0.002800	± 2.5	PASS
		VN	0	2.47	0.001411	± 2.5	PASS
		VN	10	-0.77	-0.000440	± 2.5	PASS
		VN	20	4.76	0.002720	± 2.5	PASS
		VN	30	0.35	0.000200	± 2.5	PASS
		VN	40	-1.11	-0.000634	± 2.5	PASS
		VN	50	1.92	0.001097	± 2.5	PASS
	HCH	VN	-30	-0.99	-0.000566	± 2.5	PASS
		VN	-20	-0.73	-0.000417	± 2.5	PASS
		VN	-10	3.07	0.001754	± 2.5	PASS
		VN	0	2.24	0.001280	± 2.5	PASS
		VN	10	3.4	0.001943	± 2.5	PASS
		VN	20	2.11	0.001206	± 2.5	PASS
		VN	30	4.26	0.002434	± 2.5	PASS
		VN	40	3.49	0.001994	± 2.5	PASS
		VN	50	4.85	0.002771	± 2.5	PASS

Channel Bandwidth: 15 MHz

Channel Bandwidth: 15 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	0.69	0.000402	± 2.5	PASS
		VN	TN	4.35	0.002533	± 2.5	PASS
		VH	TN	3.49	0.002032	± 2.5	PASS
	MCH	VL	TN	-0.52	-0.000300	± 2.5	PASS
		VN	TN	0.81	0.000468	± 2.5	PASS
		VH	TN	1.87	0.001079	± 2.5	PASS
	HCH	VL	TN	1.67	0.000956	± 2.5	PASS
		VN	TN	1.18	0.000675	± 2.5	PASS
		VH	TN	0.28	0.000160	± 2.5	PASS
16QAM	LCH	VL	TN	-0.3	-0.000175	± 2.5	PASS
		VN	TN	1.48	0.000862	± 2.5	PASS
		VH	TN	2.05	0.001194	± 2.5	PASS
	MCH	VL	TN	4.4	0.002540	± 2.5	PASS
		VN	TN	0.89	0.000514	± 2.5	PASS
		VH	TN	4.24	0.002447	± 2.5	PASS
	HCH	VL	TN	1.17	0.000670	± 2.5	PASS
		VN	TN	0.96	0.000549	± 2.5	PASS
		VH	TN	-1.47	-0.000841	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	1.38	0.000803	± 2.5	PASS
		VN	-20	0.7	0.000408	± 2.5	PASS
		VN	-10	2.08	0.001211	± 2.5	PASS
		VN	0	0.32	0.000186	± 2.5	PASS
		VN	10	2.22	0.001293	± 2.5	PASS
		VN	20	3.7	0.002154	± 2.5	PASS
		VN	30	2.89	0.001683	± 2.5	PASS
		VN	40	-0.22	-0.000128	± 2.5	PASS
		VN	50	4.85	0.002824	± 2.5	PASS
	MCH	VN	-30	0.38	0.000219	± 2.5	PASS
		VN	-20	2.55	0.001472	± 2.5	PASS
		VN	-10	-0.37	-0.000214	± 2.5	PASS
		VN	0	-0.29	-0.000167	± 2.5	PASS
		VN	10	-1.13	-0.000652	± 2.5	PASS
		VN	20	2.53	0.001460	± 2.5	PASS

		VN	30	1.84	0.001062	± 2.5	PASS
		VN	40	2.53	0.001460	± 2.5	PASS
		VN	50	-1.81	-0.001045	± 2.5	PASS
	HCH	VN	-30	3.26	0.001866	± 2.5	PASS
		VN	-20	1.09	0.000624	± 2.5	PASS
		VN	-10	3.29	0.001883	± 2.5	PASS
		VN	0	-1.86	-0.001064	± 2.5	PASS
		VN	10	1.72	0.000984	± 2.5	PASS
		VN	20	-1.44	-0.000824	± 2.5	PASS
		VN	30	-0.78	-0.000446	± 2.5	PASS
		VN	40	2.36	0.001351	± 2.5	PASS
		VN	50	4.24	0.002426	± 2.5	PASS
QPSK	LCH	VN	-30	-0.14	-0.000081	± 2.5	PASS
		VN	-20	-0.33	-0.000190	± 2.5	PASS
		VN	-10	3.83	0.002211	± 2.5	PASS
		VN	0	4.22	0.002436	± 2.5	PASS
		VN	10	2.33	0.001345	± 2.5	PASS
		VN	20	0.5	0.000289	± 2.5	PASS
		VN	30	2.02	0.001166	± 2.5	PASS
		VN	40	-0.65	-0.000375	± 2.5	PASS
		VN	50	-0.52	-0.000300	± 2.5	PASS
	MCH	VN	-30	1.79	0.001024	± 2.5	PASS
		VN	-20	-1.08	-0.000618	± 2.5	PASS
		VN	-10	2.44	0.001396	± 2.5	PASS
		VN	0	-0.2	-0.000114	± 2.5	PASS
		VN	10	4.88	0.002793	± 2.5	PASS
		VN	20	2.79	0.001597	± 2.5	PASS
		VN	30	1.84	0.001053	± 2.5	PASS
		VN	40	1.41	0.000807	± 2.5	PASS
		VN	50	-1.21	-0.000692	± 2.5	PASS
	HCH	VN	-30	0.7	0.000401	± 2.5	PASS
		VN	-20	2.67	0.001528	± 2.5	PASS
		VN	-10	3.35	0.001917	± 2.5	PASS
		VN	0	0.9	0.000515	± 2.5	PASS
		VN	10	3.44	0.001969	± 2.5	PASS
		VN	20	2.31	0.001322	± 2.5	PASS
		VN	30	-0.37	-0.000212	± 2.5	PASS
		VN	40	4.24	0.002426	± 2.5	PASS
		VN	50	3.13	0.001791	± 2.5	PASS

Channel Bandwidth: 20 MHz

Channel Bandwidth: 20 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	4.95	0.002878	± 2.5	PASS
		VN	TN	1.31	0.000762	± 2.5	PASS
		VH	TN	0.86	0.000500	± 2.5	PASS
	MCH	VL	TN	-1.42	-0.000820	± 2.5	PASS
		VN	TN	2.43	0.001403	± 2.5	PASS
		VH	TN	4.12	0.002378	± 2.5	PASS
	HCH	VL	TN	-1.96	-0.001123	± 2.5	PASS
		VN	TN	4.06	0.002327	± 2.5	PASS
		VH	TN	4.74	0.002716	± 2.5	PASS
16QAM	LCH	VL	TN	0.1	0.000058	± 2.5	PASS
		VN	TN	4.83	0.002808	± 2.5	PASS
		VH	TN	3.39	0.001971	± 2.5	PASS
	MCH	VL	TN	1.73	0.000999	± 2.5	PASS
		VN	TN	3.93	0.002268	± 2.5	PASS
		VH	TN	4.55	0.002626	± 2.5	PASS
	HCH	VL	TN	1.93	0.001106	± 2.5	PASS
		VN	TN	-0.58	-0.000332	± 2.5	PASS
		VH	TN	2.63	0.001507	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	1.6	0.000930	± 2.5	PASS
		VN	-20	2.56	0.001488	± 2.5	PASS
		VN	-10	2.62	0.001523	± 2.5	PASS
		VN	0	1.79	0.001041	± 2.5	PASS
		VN	10	3.23	0.001878	± 2.5	PASS
		VN	20	3.73	0.002169	± 2.5	PASS
		VN	30	1.31	0.000762	± 2.5	PASS
		VN	40	4.22	0.002453	± 2.5	PASS
		VN	50	-1.86	-0.001081	± 2.5	PASS
	MCH	VN	-30	4.61	0.002661	± 2.5	PASS
		VN	-20	1.1	0.000635	± 2.5	PASS
		VN	-10	-1.69	-0.000975	± 2.5	PASS
		VN	0	4.86	0.002805	± 2.5	PASS
		VN	10	-1.84	-0.001062	± 2.5	PASS
		VN	20	4.9	0.002828	± 2.5	PASS

		VN	30	4.67	0.002696	± 2.5	PASS
		VN	40	2.74	0.001582	± 2.5	PASS
		VN	50	0.78	0.000450	± 2.5	PASS
	HCH	VN	-30	4.32	0.002476	± 2.5	PASS
		VN	-20	4.98	0.002854	± 2.5	PASS
		VN	-10	-1.13	-0.000648	± 2.5	PASS
		VN	0	4.81	0.002756	± 2.5	PASS
		VN	10	1.9	0.001089	± 2.5	PASS
		VN	20	-1.51	-0.000865	± 2.5	PASS
		VN	30	-0.6	-0.000344	± 2.5	PASS
		VN	40	-1.34	-0.000768	± 2.5	PASS
		VN	50	1.27	0.000728	± 2.5	PASS
QPSK	LCH	VN	-30	3.59	0.002072	± 2.5	PASS
		VN	-20	1.51	0.000872	± 2.5	PASS
		VN	-10	2.4	0.001385	± 2.5	PASS
		VN	0	3.23	0.001864	± 2.5	PASS
		VN	10	-0.11	-0.000063	± 2.5	PASS
		VN	20	-1.2	-0.000693	± 2.5	PASS
		VN	30	2.1	0.001212	± 2.5	PASS
		VN	40	-1.26	-0.000727	± 2.5	PASS
		VN	50	-1.6	-0.000924	± 2.5	PASS
	MCH	VN	-30	-1.99	-0.001140	± 2.5	PASS
		VN	-20	-0.91	-0.000521	± 2.5	PASS
		VN	-10	2.64	0.001513	± 2.5	PASS
		VN	0	-1.68	-0.000963	± 2.5	PASS
		VN	10	0.3	0.000172	± 2.5	PASS
		VN	20	1.33	0.000762	± 2.5	PASS
		VN	30	-1.88	-0.001077	± 2.5	PASS
		VN	40	-1.14	-0.000653	± 2.5	PASS
		VN	50	-0.69	-0.000395	± 2.5	PASS
	HCH	VN	-30	0.87	0.000499	± 2.5	PASS
		VN	-20	2.17	0.001244	± 2.5	PASS
		VN	-10	1.13	0.000648	± 2.5	PASS
		VN	0	1.6	0.000917	± 2.5	PASS
		VN	10	1.33	0.000762	± 2.5	PASS
		VN	20	-0.76	-0.000436	± 2.5	PASS
		VN	30	-1.46	-0.000837	± 2.5	PASS
		VN	40	3.66	0.002097	± 2.5	PASS
		VN	50	1.57	0.000900	± 2.5	PASS