

Table of Contents

1.	TRANSMITTER SPURIOUS EMISSIONS	2
1.1	TRANSMITTER SPURIOUS EMISSIONS, BELOW 1GHz.	2
1.2	U-NII-1 BAND:	4
1.3	U-NII-3 BAND:	24

1. Transmitter Spurious Emissions

Note:

1. Testing is carried out with frequency rang 9kHz to the tenth harmonics. And it verified that the emssions above 18GHz are just floor-nises, no need to report it.
2. The highest emissions are the fundamental waves, the emissions more than 20dB below the limits not recorded.
3. All modes for required channel tested, only the worst-case reported.

1.1 Transmitter Spurious Emissions, Below 1GHz



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104


Test Site: PSI EMC Lab-3m Chamber
EUT: 3D scanner
M/N: EinScan Medixa
Test Mode: a 5200MHz
Test Voltage: DC 8.4V
Note:

Polarization: **Horizontal**
Distance: 3m
Test Engineer: Felix

Temperature: 26 °C
Humidity: 54 %RH

Radiated Emission Measurement

Test Date: 2025/9/11 13:40:47

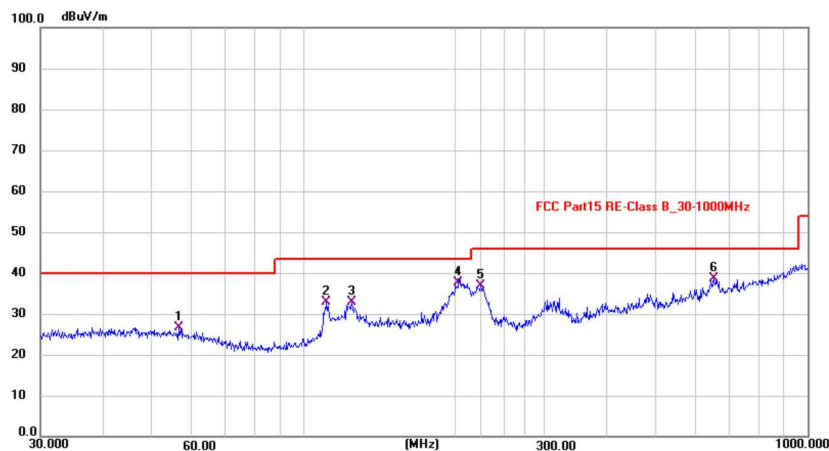

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	56.3947	13.06	13.65	26.71	40.00	-13.29	QP	150	42	P	
2	110.9570	20.43	12.53	32.96	43.50	-10.54	QP	150	318	P	
3	124.5690	19.22	13.73	32.95	43.50	-10.55	QP	150	59	P	
4 *	202.8103	25.95	11.60	37.55	43.50	-5.95	QP	150	77	P	
5	224.5192	24.78	12.09	36.87	46.00	-9.13	QP	150	134	P	
6	651.9415	15.51	23.14	38.65	46.00	-7.35	QP	150	325	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 3 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5200MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 13:45:18

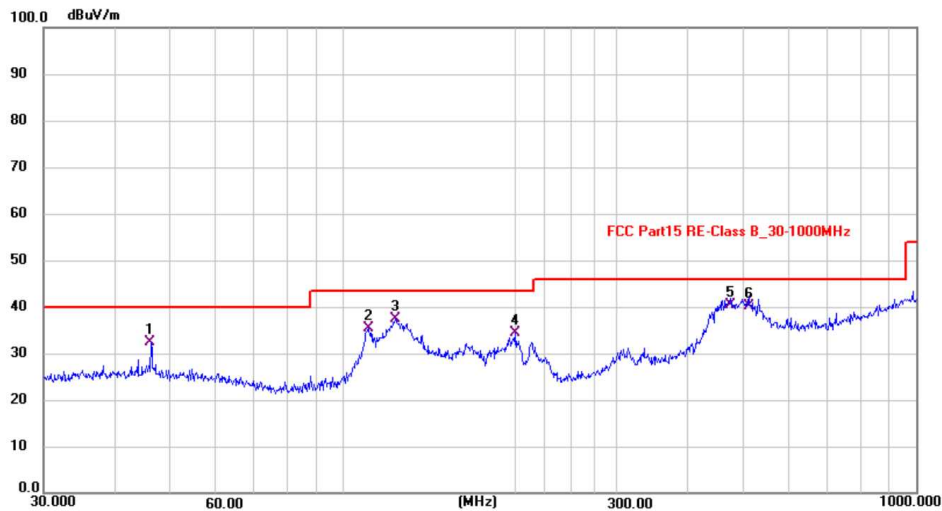

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	46.1779	18.03	14.45	32.48	40.00	-7.52	QP	150	42	P	
2	110.9570	22.96	12.53	35.49	43.50	-8.01	QP	150	184	P	
3	123.2651	23.66	13.66	37.32	43.50	-6.18	QP	150	20	P	
4	199.9855	22.89	11.55	34.44	43.50	-9.06	QP	150	335	P	
5 *	473.8346	21.12	19.14	40.26	46.00	-5.74	QP	150	31	P	
6	510.0434	20.20	19.92	40.12	46.00	-5.88	QP	150	226	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

File: FCC 30-1000MHz 5\Data :#4

Page: 1

Engineer Signature:

1.2 U-NII-1 Band:




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: 3D scanner	Distance: 3m	Humidity: 54 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: a 5180MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 11:00:52

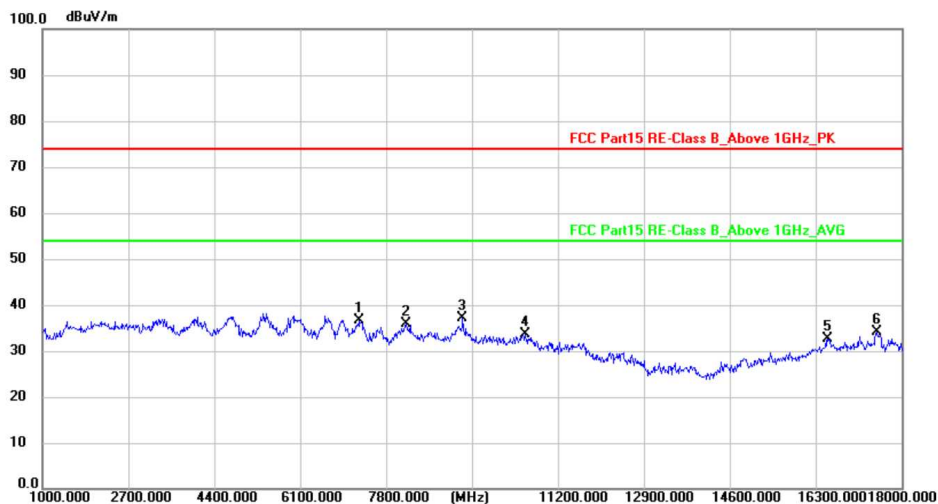

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	7273.000	45.42	-8.77	36.65	74.00	-37.35	peak	150	360	P	
2	8203.750	44.31	-8.31	36.00	74.00	-38.00	peak	150	360	P	
3 *	9315.125	44.15	-7.03	37.12	74.00	-36.88	peak	150	360	P	
4	10554.000	38.93	-5.39	33.54	74.00	-40.46	peak	150	360	P	
5	16552.875	31.97	0.54	32.51	74.00	-41.49	peak	150	360	P	
6	17511.250	33.23	0.93	34.16	74.00	-39.84	peak	150	360	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 5 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5180MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:05:54

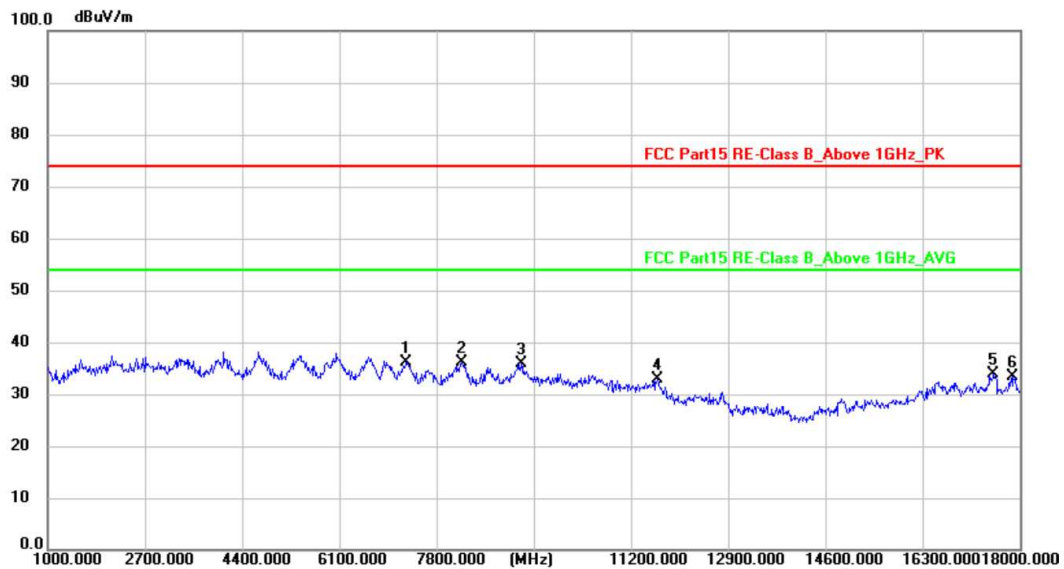

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7283.625	45.01	-8.76	36.25	74.00	-37.75	peak	150	123	P	
2	8256.875	44.28	-8.24	36.04	74.00	-37.96	peak	150	123	P	
3	9279.000	43.01	-7.06	35.95	74.00	-38.05	peak	150	123	P	
4	11671.750	37.13	-4.28	32.85	74.00	-41.15	peak	150	123	P	
5	17543.125	32.85	0.92	33.77	74.00	-40.23	peak	150	123	P	
6	17883.125	32.49	0.77	33.26	74.00	-40.74	peak	150	123	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B

CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 6 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5200MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:10:30

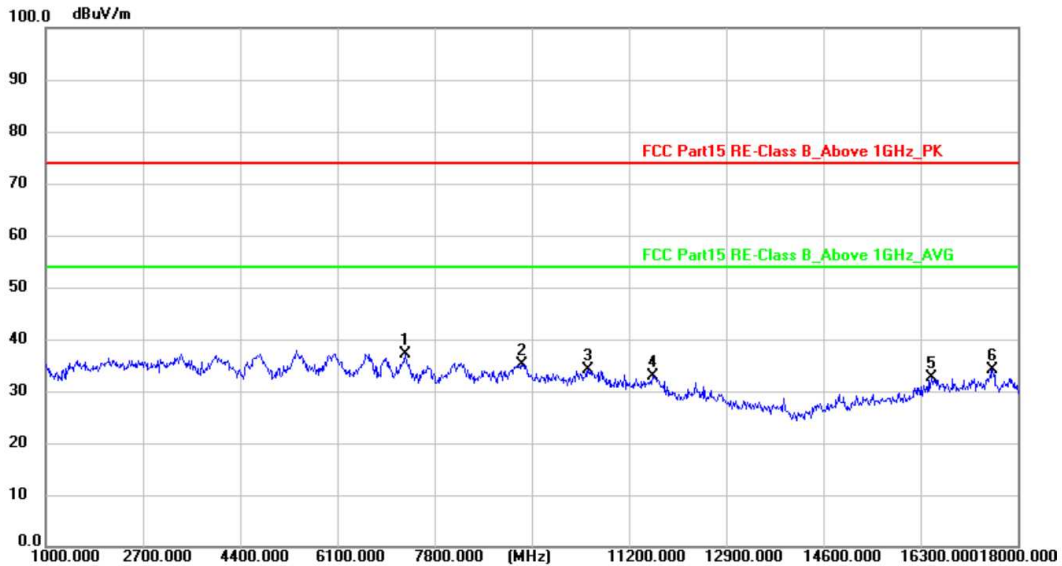

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7290.000	45.97	-8.76	37.21	74.00	-36.79	peak	150	238	P	
2	9338.500	42.03	-6.99	35.04	74.00	-38.96	peak	150	238	P	
3	10494.500	39.54	-5.48	34.06	74.00	-39.94	peak	150	238	P	
4	11625.000	37.21	-4.30	32.91	74.00	-41.09	peak	150	238	P	
5	16495.500	32.20	0.46	32.66	74.00	-41.34	peak	150	238	P	
6	17572.875	33.21	0.89	34.10	74.00	-39.90	peak	150	238	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 7 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5200MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:15:46

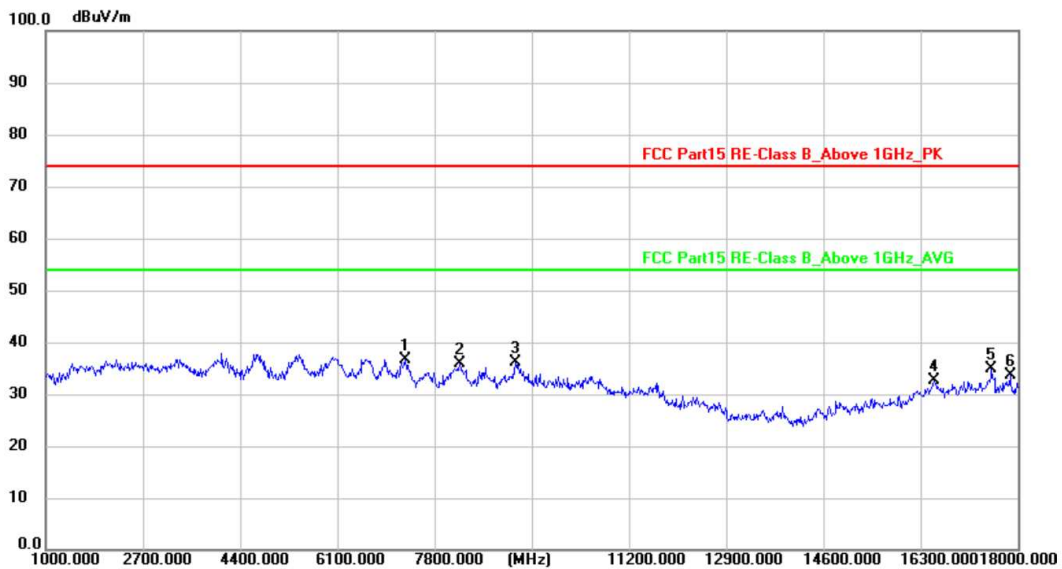

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7294.250	45.41	-8.76	36.65	74.00	-37.35	peak	150	74	P	
2	8256.875	44.09	-8.24	35.85	74.00	-38.15	peak	150	74	P	
3	9213.125	43.40	-7.15	36.25	74.00	-37.75	peak	150	74	P	
4	16540.125	32.13	0.53	32.66	74.00	-41.34	peak	150	74	P	
5	17553.750	33.94	0.91	34.85	74.00	-39.15	peak	150	74	P	
6	17872.500	32.76	0.75	33.51	74.00	-40.49	peak	150	74	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 8 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5240MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:20:46

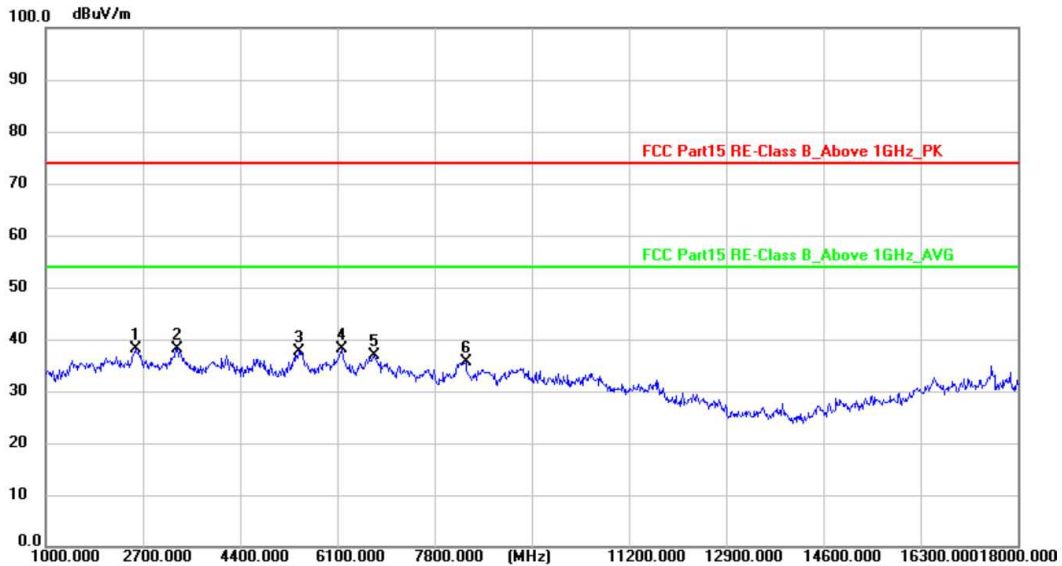

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	2566.125	53.53	-15.47	38.06	74.00	-35.94	peak	150	336	P	
2 *	3299.250	52.64	-14.46	38.18	74.00	-35.82	peak	150	154	P	
3	5441.250	48.42	-10.78	37.64	74.00	-36.36	peak	150	69	P	
4	6187.125	47.46	-9.36	38.10	74.00	-35.90	peak	150	83	P	
5	6748.125	45.87	-9.02	36.85	74.00	-37.15	peak	150	321	P	
6	8358.875	43.71	-8.13	35.58	74.00	-38.42	peak	150	104	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 9 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: 3D scanner	Distance: 3m	Humidity: 54 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: a 5240MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 11:25:30

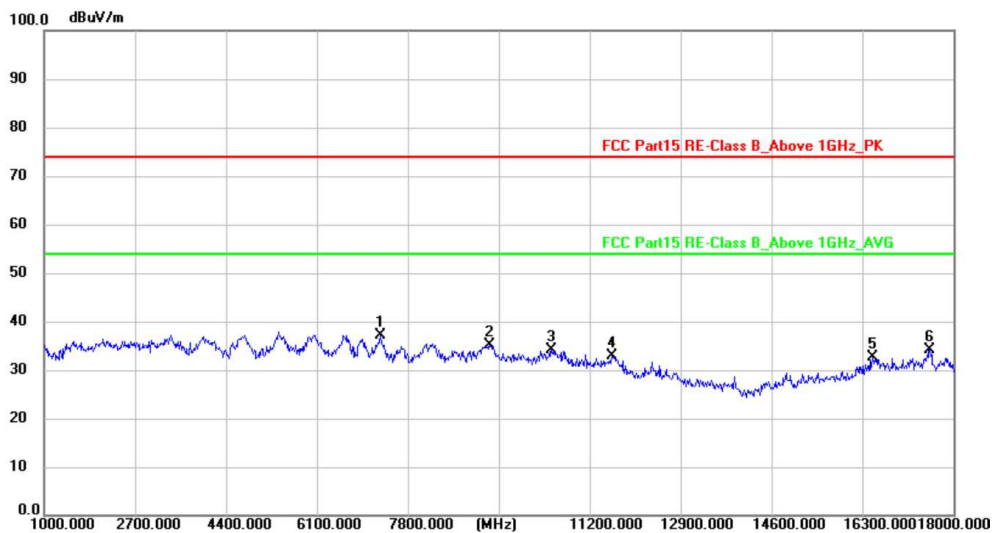

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7290.000	45.97	-8.76	37.21	74.00	-36.79	peak	150	39	P	
2	9338.500	42.03	-6.99	35.04	74.00	-38.96	peak	150	133	P	
3	10494.500	39.54	-5.48	34.06	74.00	-39.94	peak	150	290	P	
4	11625.000	37.21	-4.30	32.91	74.00	-41.09	peak	150	42	P	
5	16495.500	32.20	0.46	32.66	74.00	-41.34	peak	150	147	P	
6	17572.875	33.21	0.89	34.10	74.00	-39.90	peak	150	144	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 10 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5180MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 15:35:36



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5147.988	63.99	-17.47	46.52	54.00	-7.48	AVG	150	150	P	
2	5150.000	61.70	-17.45	44.25	54.00	-9.75	AVG	150	125	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 11 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5180MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 15:40:04

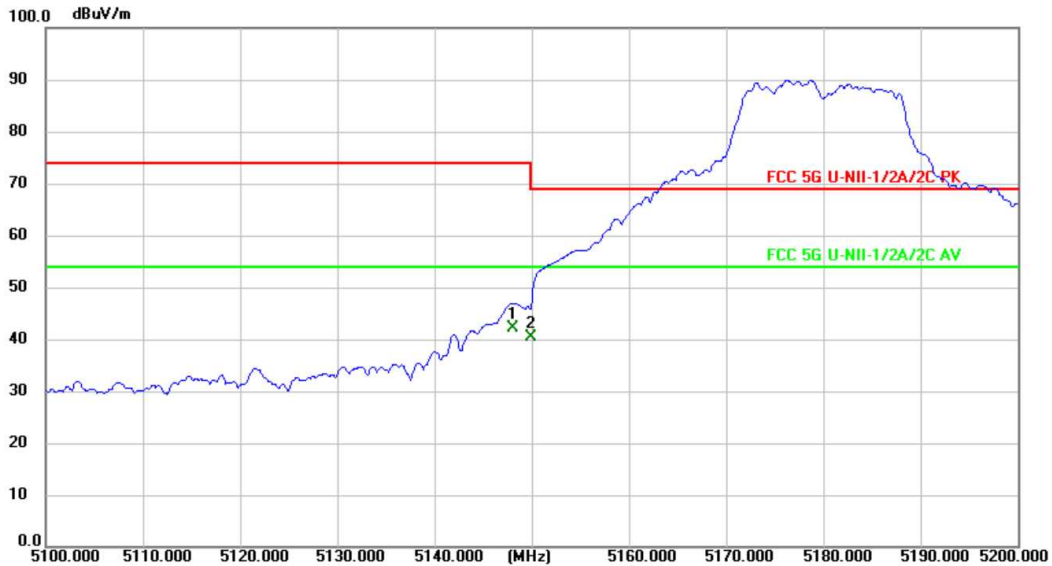

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5148.150	59.67	-17.47	42.20	54.00	-11.80	AVG	150	250	P	
2	5150.000	57.71	-17.45	40.26	54.00	-13.74	AVG	150	125	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 12 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5240MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 15:45:16

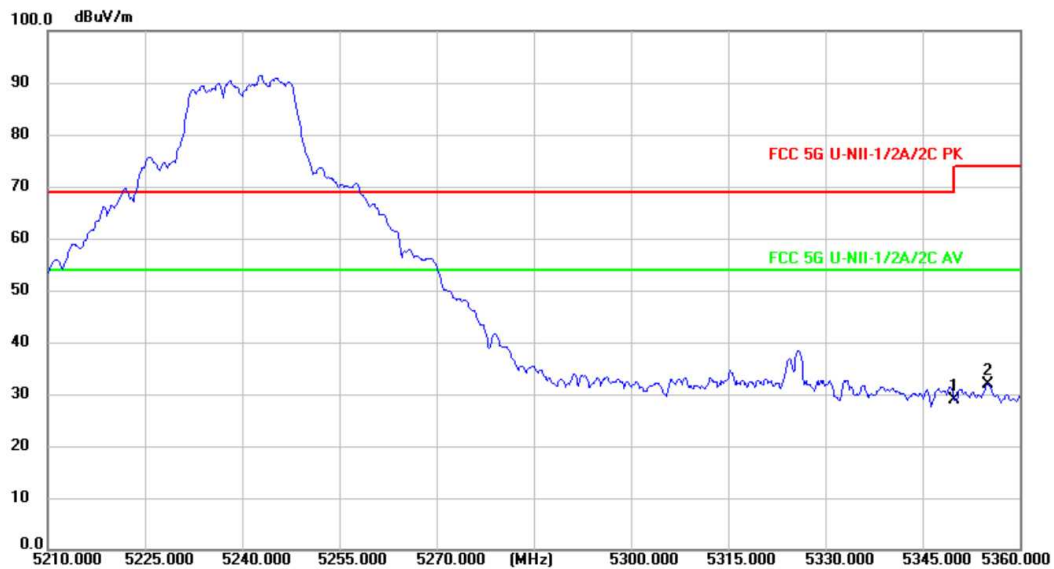

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5350.000	45.80	-16.99	28.81	68.82	-40.01	peak	150	208	P	
2	5355.163	48.94	-16.98	31.96	74.00	-42.04	peak	150	115	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 13 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5240MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 15:50:21



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5350.000	52.40	-16.99	35.41	68.82	-33.41	peak	150	314	P	
2	5356.250	55.31	-16.98	38.33	74.00	-35.67	peak	150	215	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 14 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5180MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 15:55:09

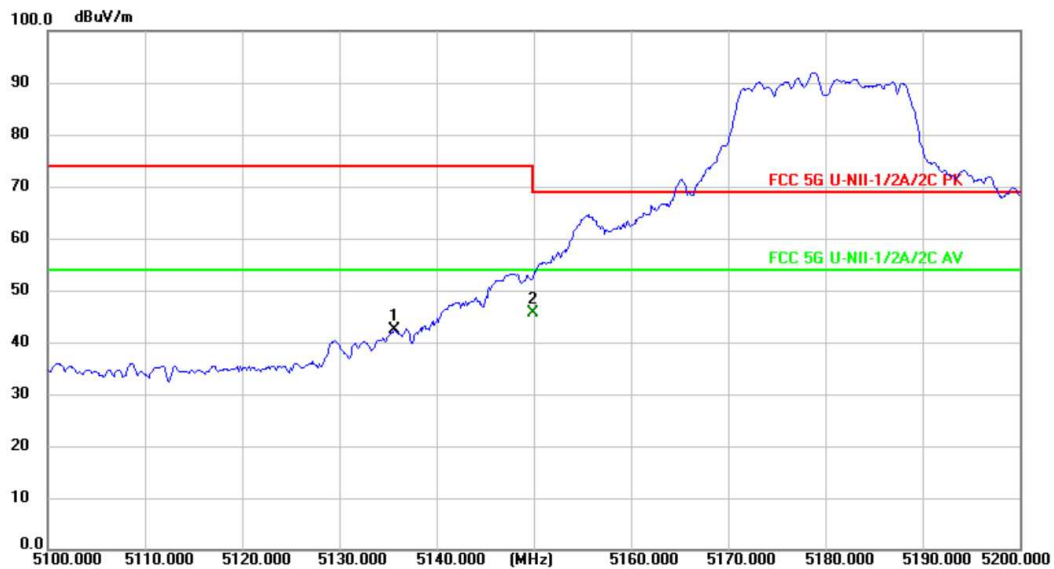

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5135.600	59.87	-17.48	42.39	74.00	-31.61	peak	150	226	P	
2 *	5150.000	63.07	-17.45	45.62	54.00	-8.38	AVG	150	215	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 15 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5180MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:00:37

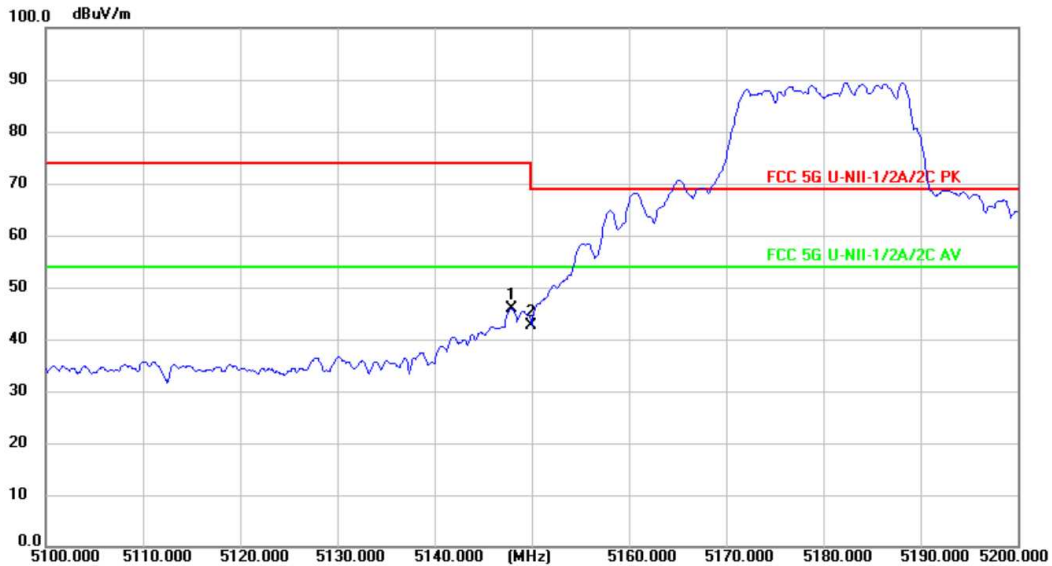

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5147.925	63.45	-17.47	45.98	74.00	-28.02	peak	150	215	P	
2 *	5150.000	60.04	-17.45	42.59	68.82	-26.23	peak	150	360	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 16 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5240MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:05:05



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5350.000	52.83	-16.99	35.84	68.82	-32.98	peak	150	315	P	
2	5356.719	53.89	-16.98	36.91	74.00	-37.09	peak	150	255	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B

CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 17 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5240MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:10:03

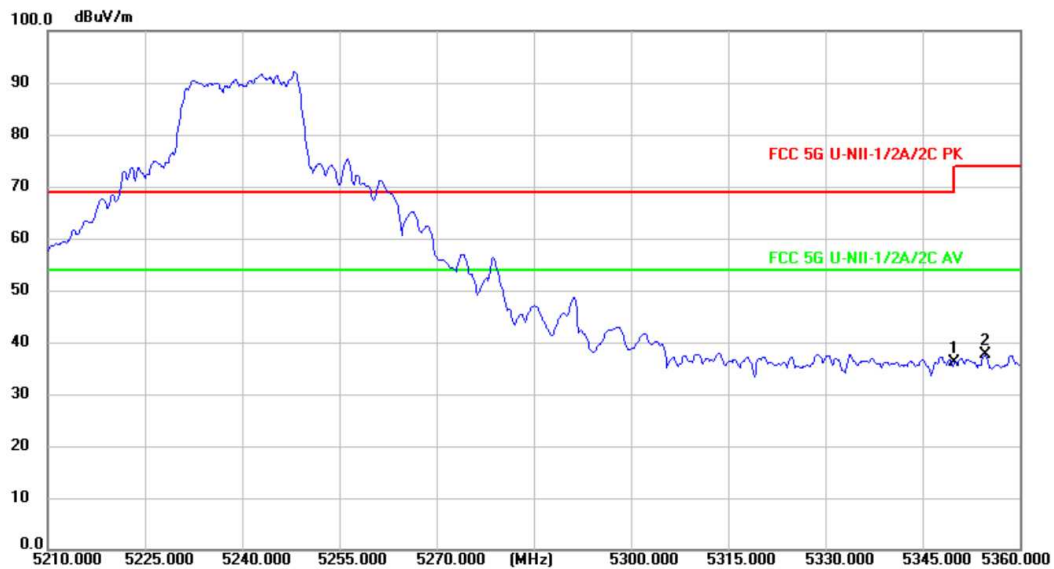

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5350.000	53.19	-16.99	36.20	68.82	-32.62	peak	150	348	P	
2	5354.675	54.57	-16.98	37.59	74.00	-36.41	peak	150	214	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 18 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5190MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:15:43



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5127.180	58.76	-17.50	41.26	54.00	-12.74	AVG	150	205	P	
2 *	5150.000	61.71	-17.45	44.26	54.00	-9.74	AVG	150	115	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 19 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5190MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:20:28



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5136.220	61.76	-17.48	44.28	54.00	-9.72	AVG	150	155	P	
2 *	5150.000	66.40	-17.45	48.95	54.00	-5.05	AVG	150	56	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 20 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5230MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:25:43



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5321.320	57.75	-17.06	40.69	68.82	-28.13	peak	150	206	P	
2	5350.680	55.26	-16.98	38.28	74.00	-35.72	peak	150	115	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 21 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5230MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:30:15



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5350.000	57.33	-16.99	40.34	68.82	-28.48	peak	150	315	P	
2	5357.820	59.43	-16.97	42.46	74.00	-31.54	peak	150	159	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit