

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 22 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: ax80 5210MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:35:39

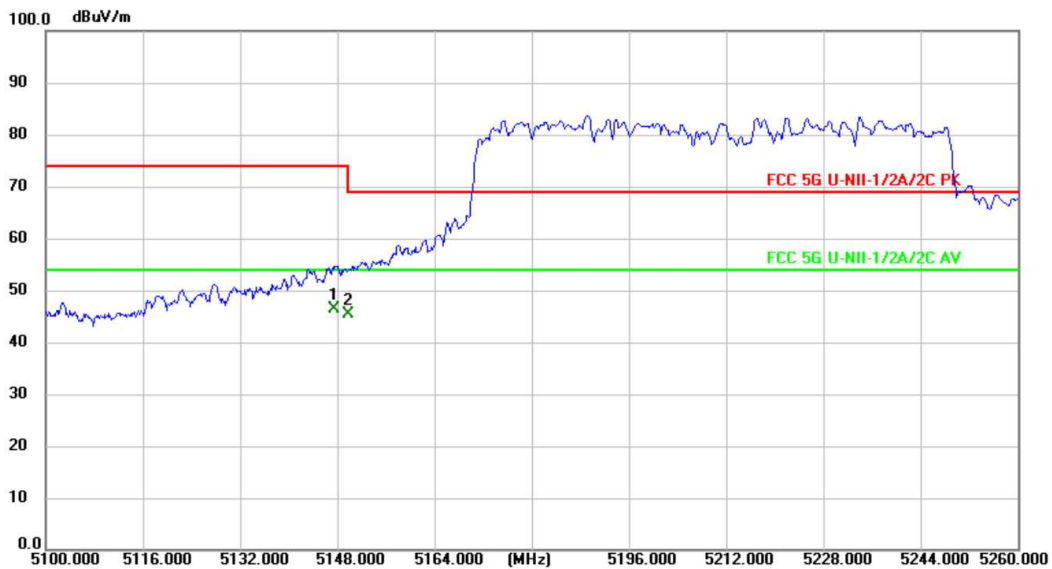

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5147.760	63.89	-17.47	46.42	54.00	-7.58	AVG	150	152	P	
2	5150.000	62.80	-17.45	45.35	54.00	-8.65	AVG	150	305	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 23 of 43



Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: ax80 5210MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:40:39



No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5142.780	60.72	-17.47	43.25	54.00	-10.75	AVG	150	208	P	
2 *	5150.000	62.01	-17.45	44.56	54.00	-9.44	AVG	150	126	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

1.3 U-NII-3 Band:




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 26 °C
EUT: 3D scanner	Distance: 3m	Humidity: 54 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: a 5745MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 11:30:30

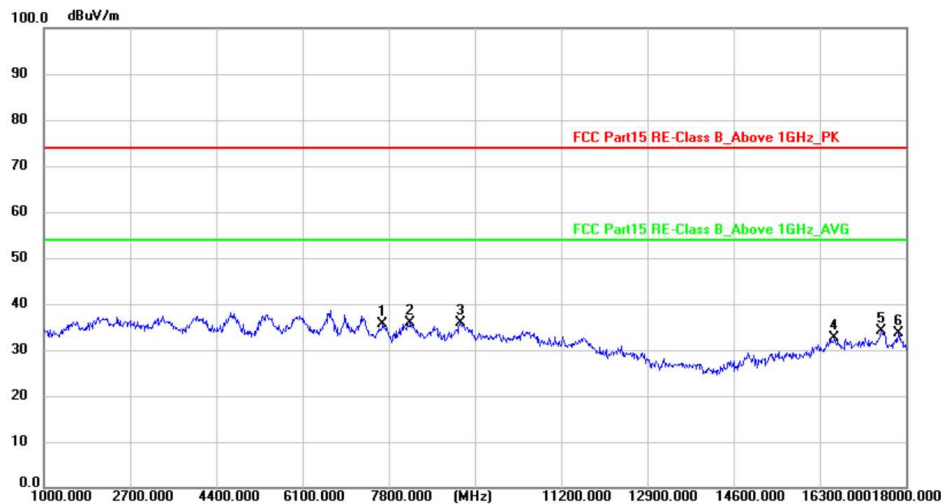

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	7685.250	44.27	-8.63	35.64	74.00	-38.36	peak	150	130	P	
2	8239.875	44.11	-8.26	35.85	74.00	-38.15	peak	150	225	P	
3 *	9221.625	43.00	-7.13	35.87	74.00	-38.13	peak	150	84	P	
4	16603.875	32.03	0.62	32.65	74.00	-41.35	peak	150	280	P	
5	17511.250	33.17	0.93	34.10	74.00	-39.90	peak	150	130	P	
6	17855.500	32.76	0.77	33.53	74.00	-40.47	peak	150	175	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 25 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5745MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:35:47

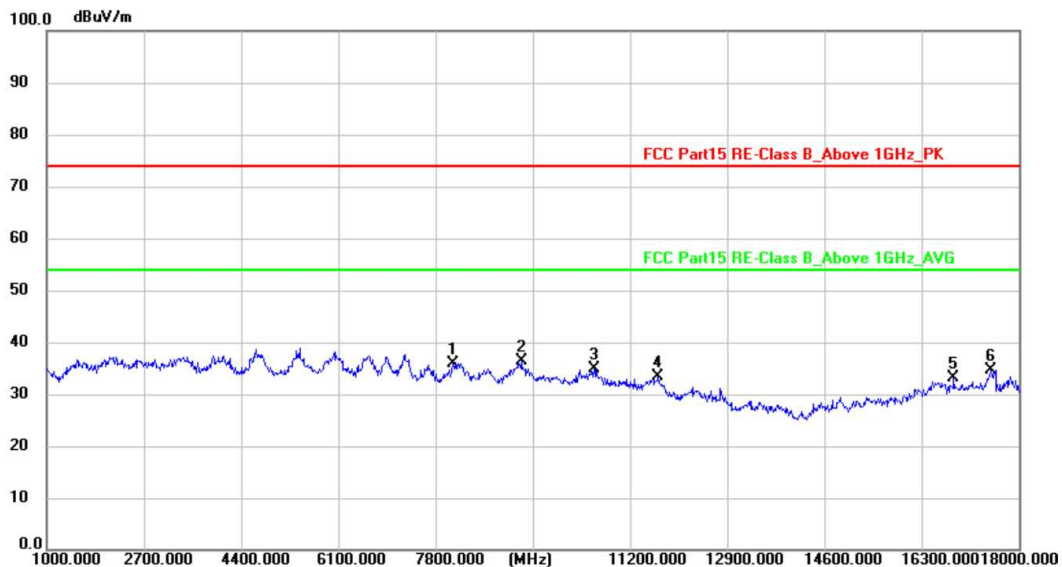

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	8116.625	44.19	-8.40	35.79	74.00	-38.21	peak	150	320	P	
2 *	9300.250	43.44	-7.04	36.40	74.00	-37.60	peak	150	174	P	
3	10579.500	40.25	-5.36	34.89	74.00	-39.11	peak	150	39	P	
4	11695.125	37.67	-4.26	33.41	74.00	-40.59	peak	150	320	P	
5	16863.125	32.04	0.98	33.02	74.00	-40.98	peak	150	83	P	
6	17517.625	33.76	0.92	34.68	74.00	-39.32	peak	150	0	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: 3D scanner	Distance: 3m	Humidity: 54 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: a 5785MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 11:40:16

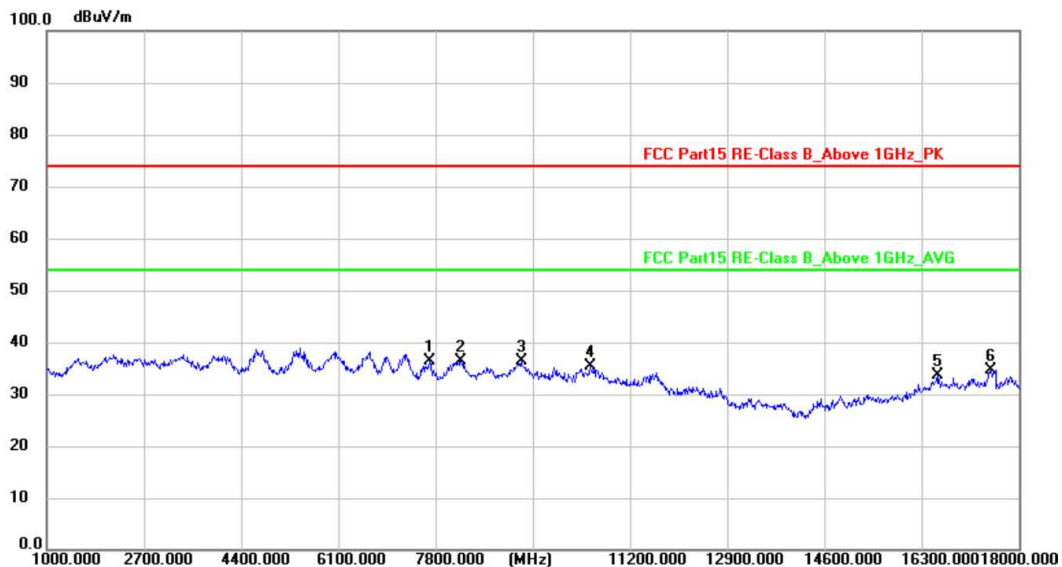

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	7708.625	44.96	-8.63	36.33	74.00	-37.67	peak	150	222	P	
2	8242.000	44.58	-8.26	36.32	74.00	-37.68	peak	150	114	P	
3 *	9300.250	43.44	-7.04	36.40	74.00	-37.60	peak	150	270	P	
4	10503.000	40.80	-5.47	35.33	74.00	-38.67	peak	150	312	P	
5	16580.500	33.07	0.58	33.65	74.00	-40.35	peak	150	298	P	
6	17517.625	33.76	0.92	34.68	74.00	-39.32	peak	150	27	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 27 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5785MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:45:33

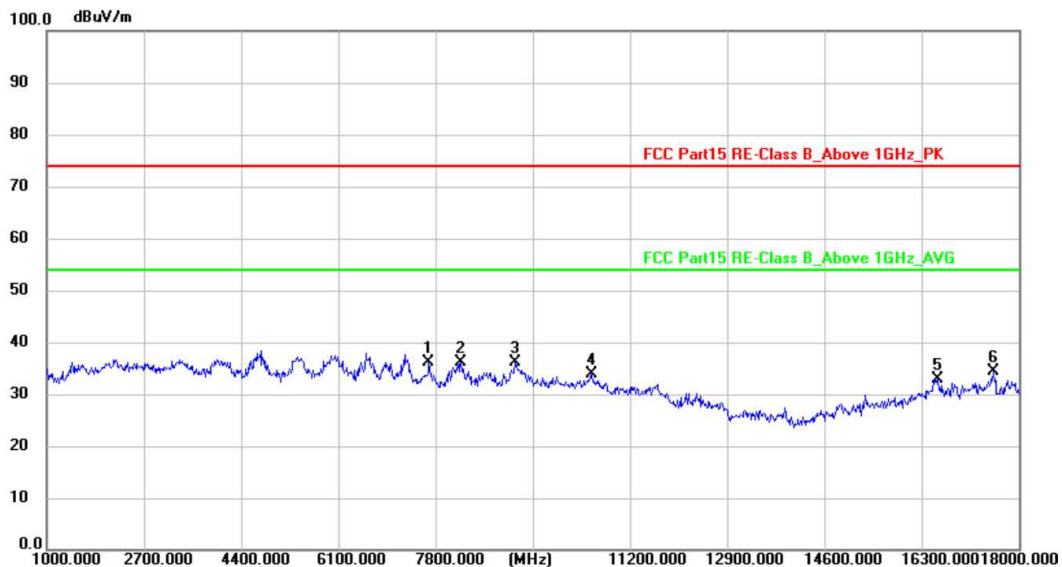

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	7695.875	44.85	-8.63	36.22	74.00	-37.78	peak	150	200	P	
2	8246.250	44.28	-8.26	36.02	74.00	-37.98	peak	150	205	P	
3	9206.750	43.25	-7.16	36.09	74.00	-37.91	peak	150	349	P	
4	10539.125	39.37	-5.42	33.95	74.00	-40.05	peak	150	221	P	
5	16589.000	32.35	0.60	32.95	74.00	-41.05	peak	150	237	P	
6	17564.375	33.58	0.90	34.48	74.00	-39.52	peak	150	213	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 28 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 26 °C
EUT: 3D scanner Distance: 3m Humidity: 54 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5825MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 11:50:33

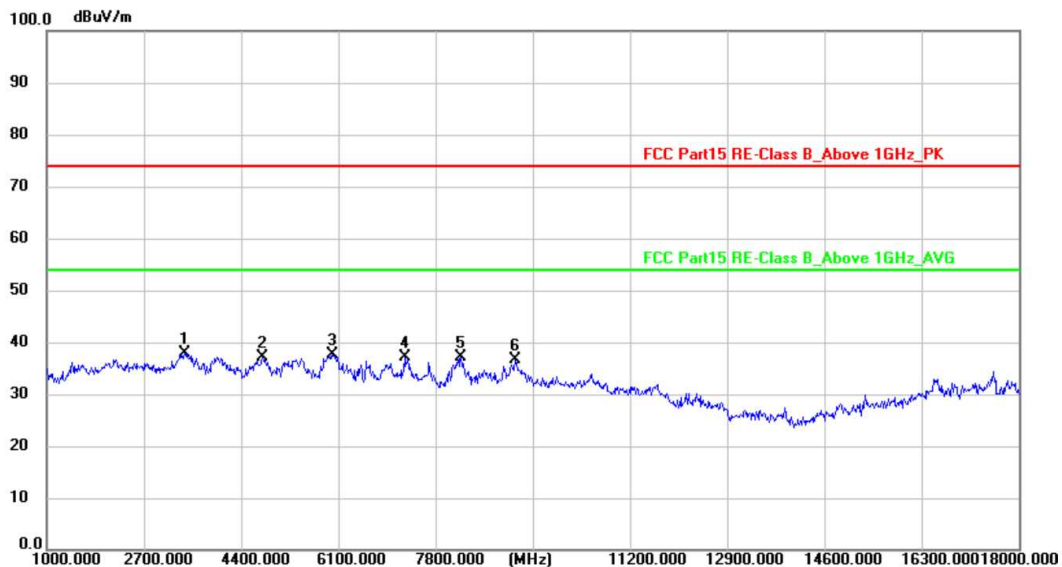

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	3420.375	52.18	-14.26	37.92	74.00	-36.08	peak	150	213	P	
2	4776.125	49.27	-12.14	37.13	74.00	-36.87	peak	150	38	P	
3	6006.500	47.08	-9.48	37.60	74.00	-36.40	peak	150	351	P	
4	7258.125	45.82	-8.77	37.05	74.00	-36.95	peak	150	74	P	
5	8246.250	45.28	-8.26	37.02	74.00	-36.98	peak	150	334	P	
6	9206.750	43.75	-7.16	36.59	74.00	-37.41	peak	150	269	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 29 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Vertical	Temperature: 26 °C
EUT: 3D scanner	Distance: 3m	Humidity: 54 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: a 5825MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 11:55:16

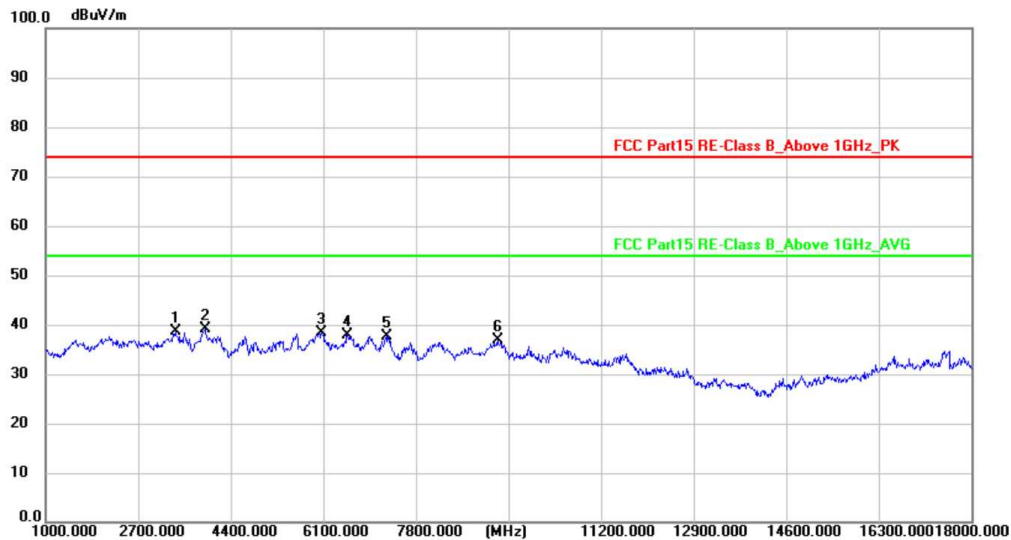

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	3390.625	52.82	-14.31	38.51	74.00	-35.49	peak	150	39	P	
2 *	3932.500	52.66	-13.43	39.23	74.00	-34.77	peak	150	111	P	
3	6074.500	47.70	-9.43	38.27	74.00	-35.73	peak	150	47	P	
4	6554.750	46.95	-9.12	37.83	74.00	-36.17	peak	150	105	P	
5	7270.875	46.36	-8.77	37.59	74.00	-36.41	peak	150	74	P	
6	9300.250	43.94	-7.04	36.90	74.00	-37.10	peak	150	83	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 30 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5745MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:45:49

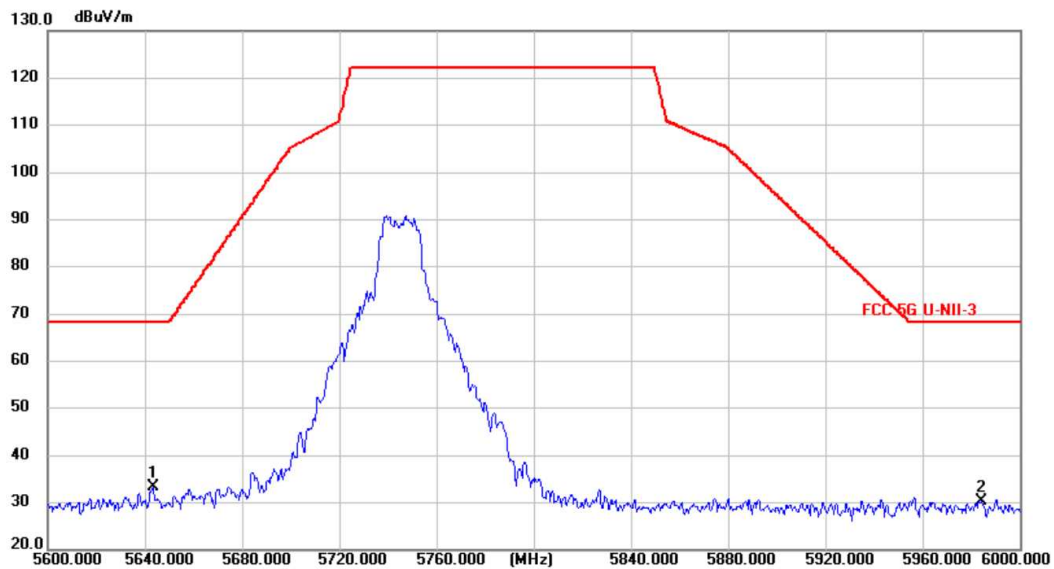

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5643.400	49.61	-16.32	33.29	68.20	-34.91	peak	150	205	P	
2	5984.550	45.82	-15.53	30.29	68.20	-37.91	peak	150	114	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 31 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5745MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:50:55

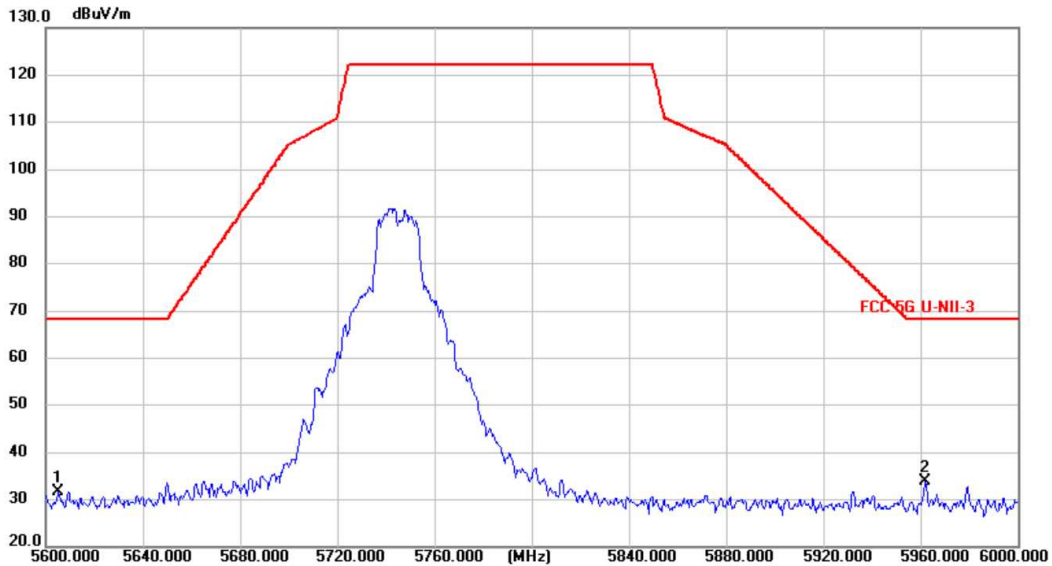

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5605.300	48.10	-16.41	31.69	68.20	-36.51	peak	150	315	P	
2 *	5962.100	49.41	-15.59	33.82	68.20	-34.38	peak	150	360	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 32 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5825MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 16:55:38

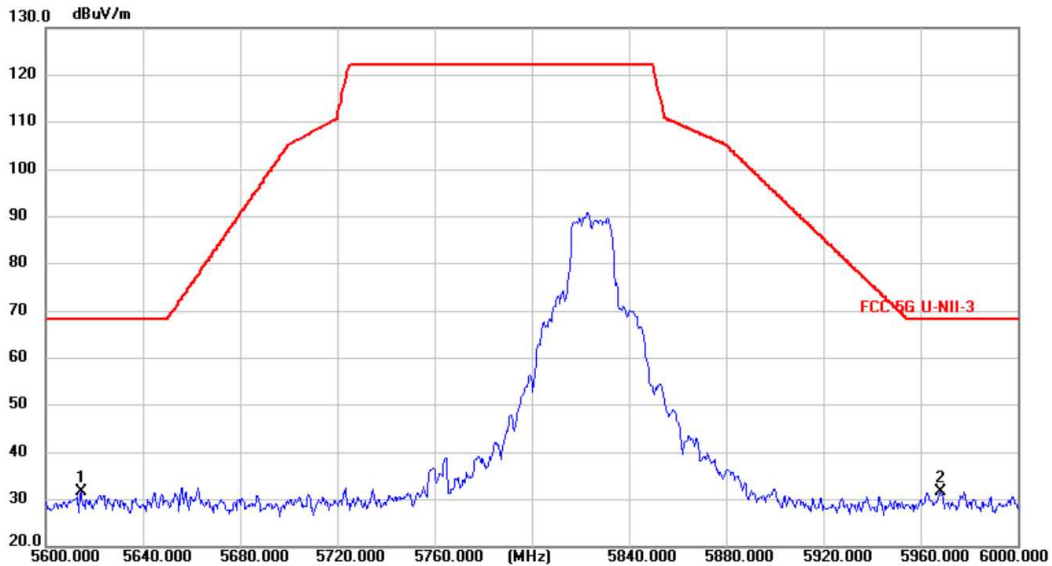

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5614.500	48.02	-16.39	31.63	68.20	-36.57	peak	150	105	P	
2 *	5968.150	47.20	-15.57	31.63	68.20	-36.57	peak	150	215	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 33 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: a 5825MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:00:26

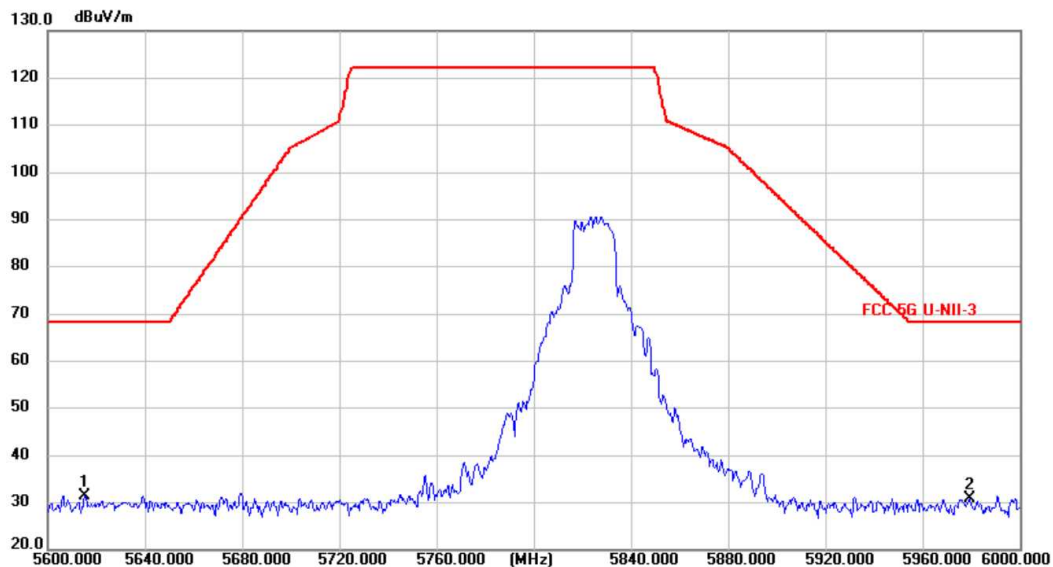

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5615.500	47.93	-16.39	31.54	68.20	-36.66	peak	150	287	P	
2	5979.600	46.47	-15.55	30.92	68.20	-37.28	peak	150	318	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 34 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5745MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:05:59

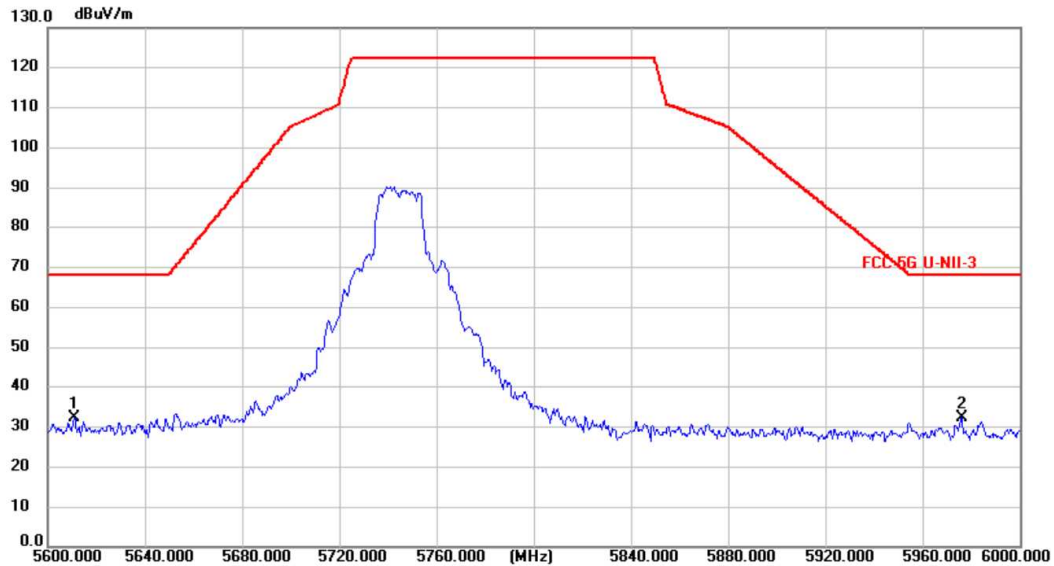

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5611.100	48.84	-16.40	32.44	68.20	-35.76	peak	150	315	P	
2	5976.050	47.99	-15.56	32.43	68.20	-35.77	peak	150	274	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 35 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5745MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:10:27

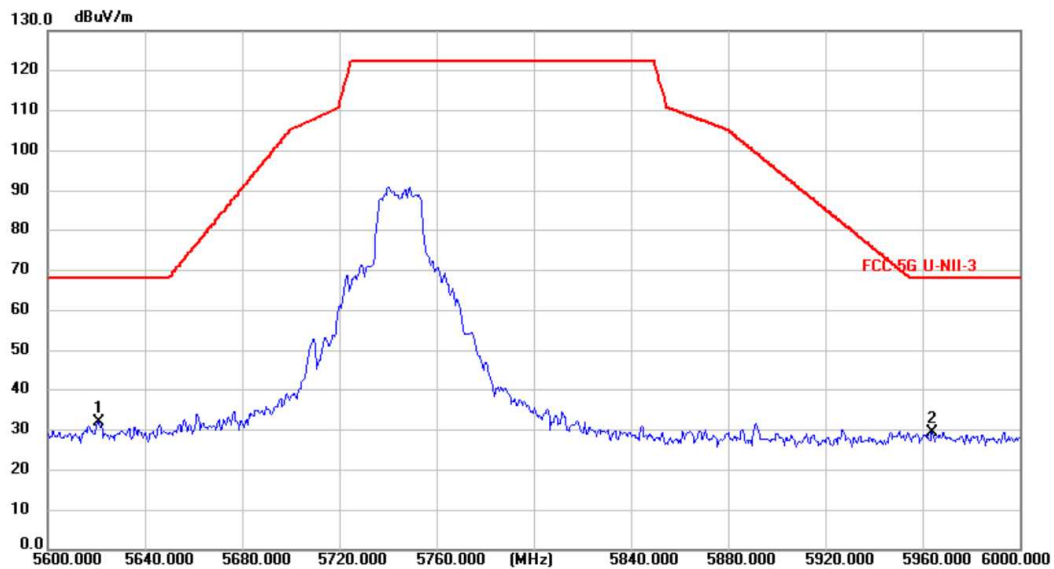

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5620.950	48.46	-16.37	32.09	68.20	-36.11	peak	150	354	P	
2	5964.100	45.03	-15.59	29.44	68.20	-38.76	peak	150	108	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 36 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5825MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:15:34

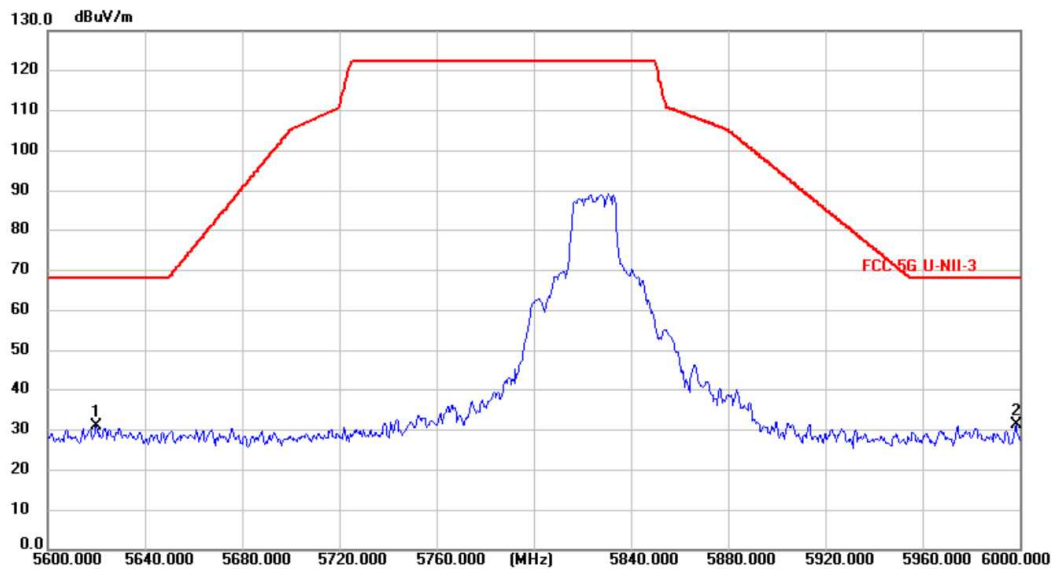

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1	5620.050	47.32	-16.37	30.95	68.20	-37.25	peak	150	318	P	
2 *	5998.450	46.80	-15.50	31.30	68.20	-36.90	peak	150	264	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 37 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n20 5825MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:20:59

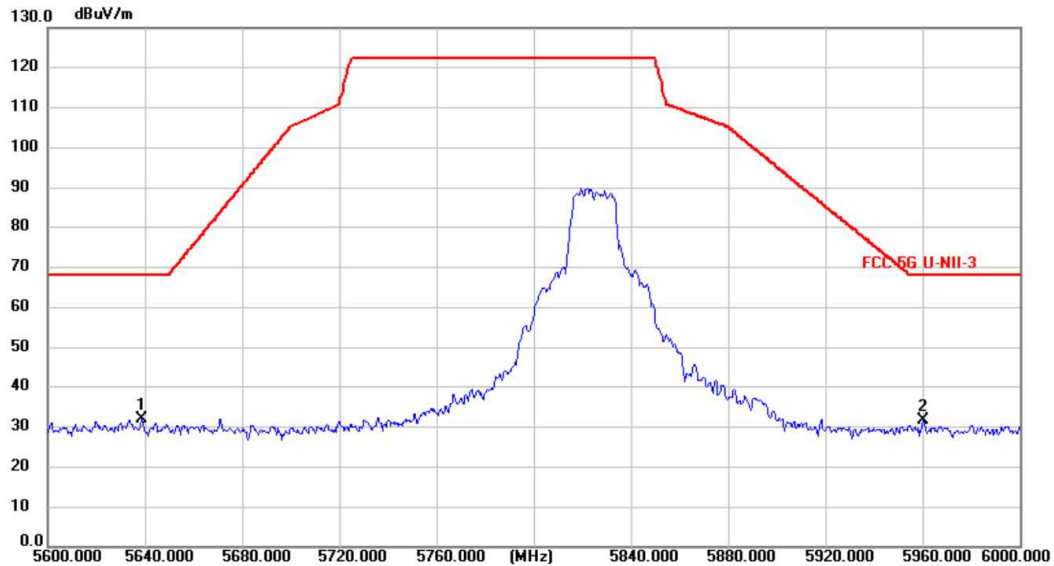

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5638.900	48.37	-16.33	32.04	68.20	-36.16	peak	150	168	P	
2	5960.500	47.37	-15.59	31.78	68.20	-36.42	peak	150	124	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber	Polarization: Horizontal	Temperature: 24 °C
EUT: 3D scanner	Distance: 3m	Humidity: 56 %RH
M/N: EinScan Medixa	Test Engineer: Felix	
Test Mode: n40 5755MHz		
Test Voltage: DC 8.4V		
Note:		

Radiated Emission Measurement

Test Date: 2025/9/11 17:25:32

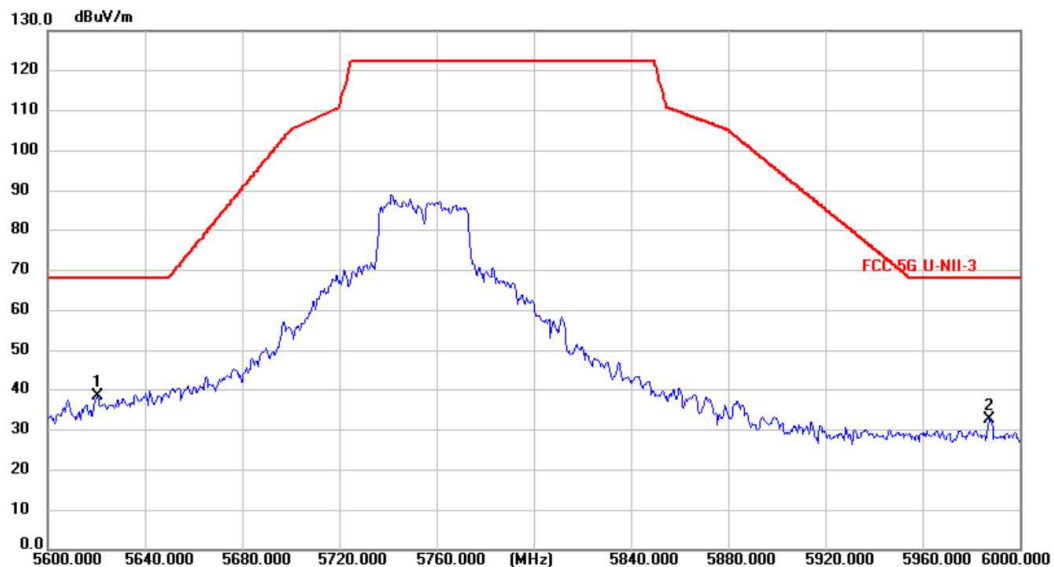

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5620.600	54.73	-16.37	38.36	68.20	-29.84	peak	150	315	P	
2	5987.900	48.19	-15.53	32.66	68.20	-35.54	peak	150	205	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 39 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5755MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:30:31

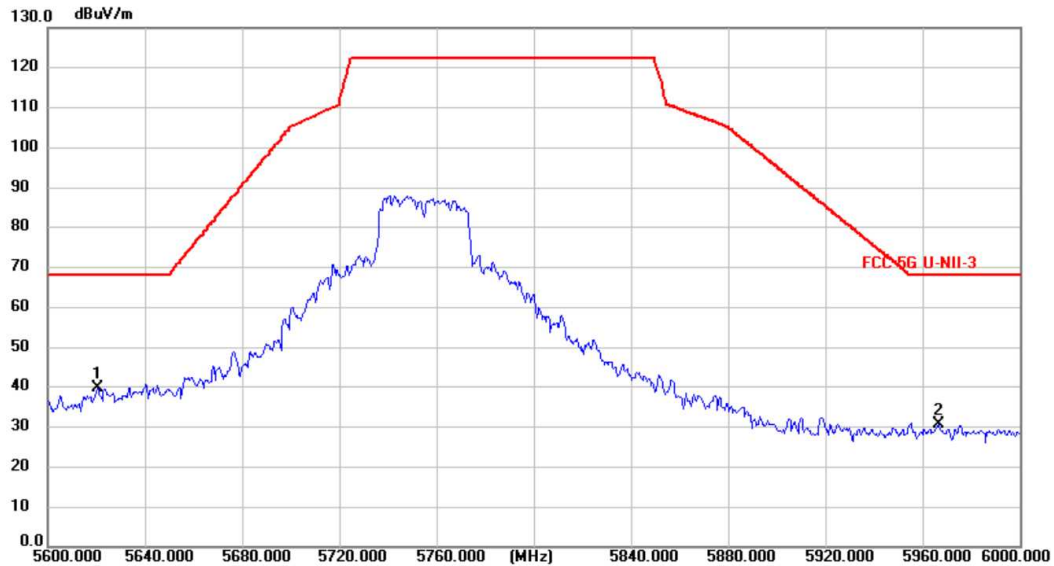

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5620.600	56.04	-16.37	39.67	68.20	-28.53	peak	150	308	P	
2	5966.650	46.23	-15.57	30.66	68.20	-37.54	peak	150	123	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 40 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5795MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:35:38

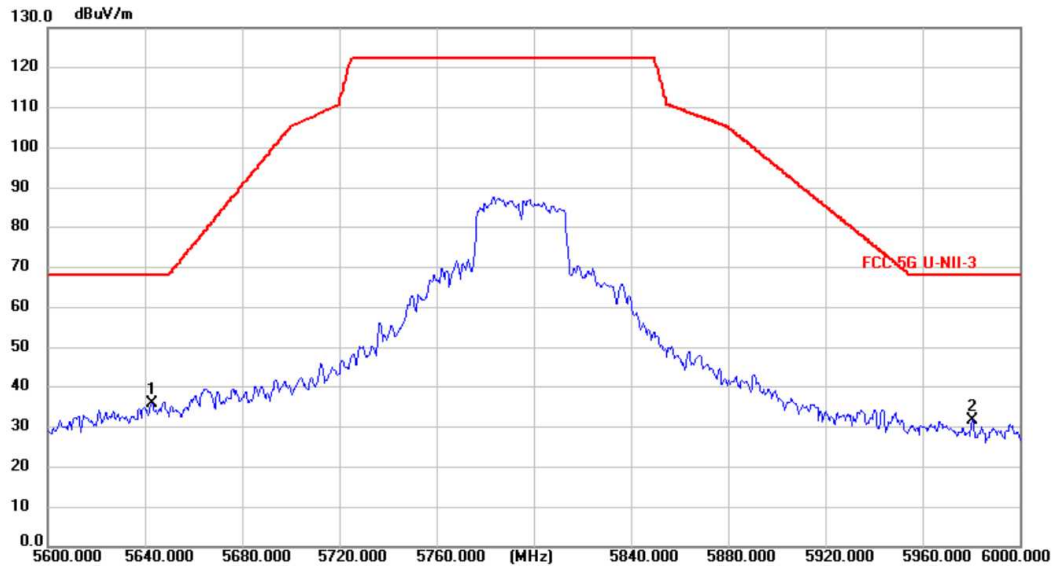

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5643.050	52.26	-16.32	35.94	68.20	-32.26	peak	150	211	P	
2	5980.750	47.19	-15.55	31.64	68.20	-36.56	peak	150	54	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 41 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: n40 5795MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:40:46

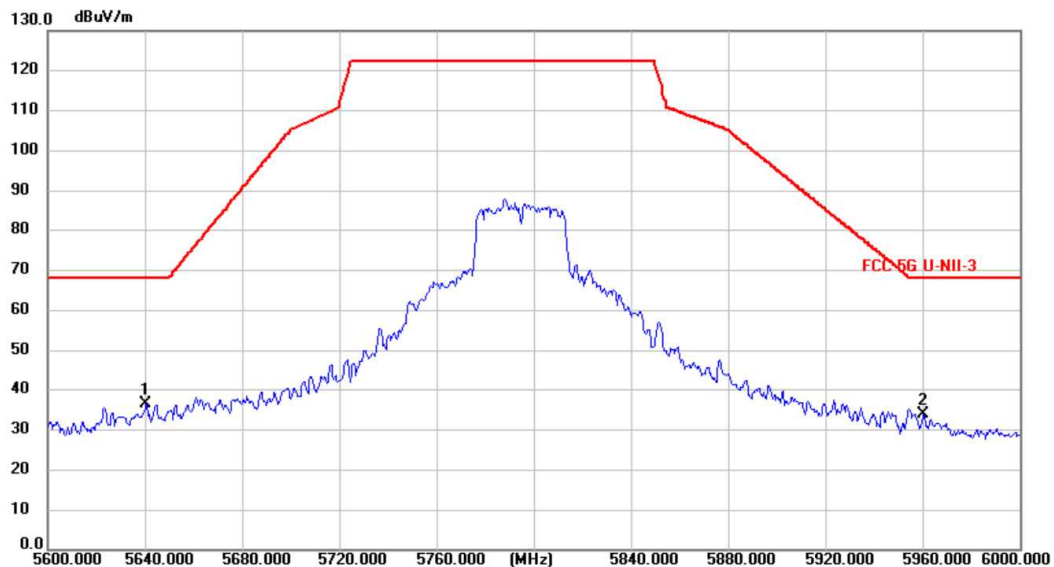

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5640.750	52.74	-16.33	36.41	68.20	-31.79	peak	150	308	P	
2	5960.550	49.64	-15.59	34.05	68.20	-34.15	peak	150	155	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002



Prüfbericht - Produkte
Test Report - Products

Page 42 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Horizontal** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: ax80 5775MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:45:47

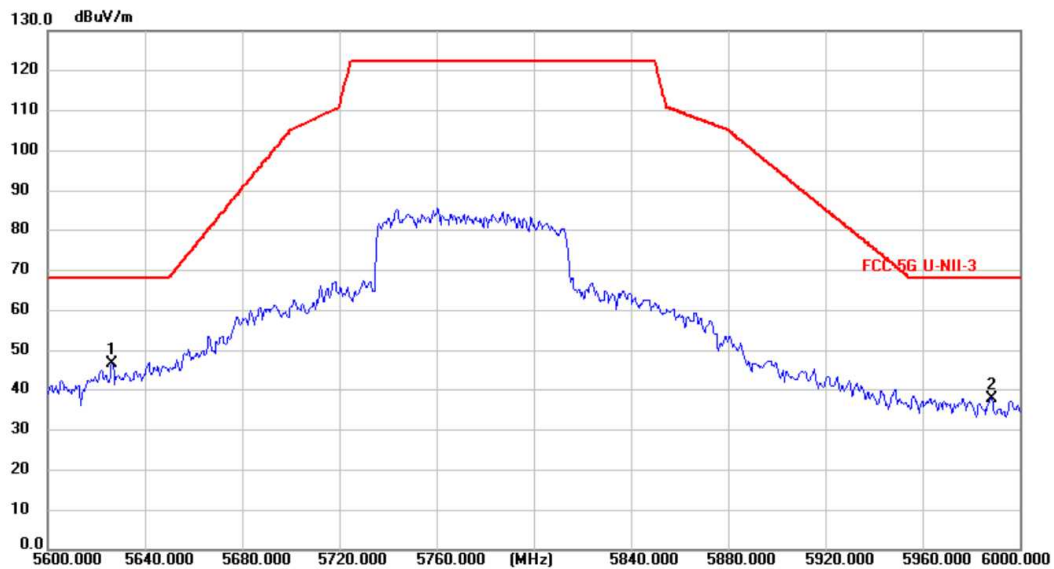

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5626.650	62.87	-16.36	46.51	68.20	-21.69	peak	150	218	P	
2	5988.400	53.53	-15.53	38.00	68.20	-30.20	peak	150	165	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit

Appendix B
CN25OGF0 002

Prüfbericht - Produkte
Test Report - Products

Page 43 of 43




Shenzhen PSI Testing Co., Ltd.
1-2F, Building 5, Yudafu Industrial Park, No. 10, Xingye West Road,
Shajing Street, Bao'an District, Shenzhen, Guangdong, China 518104

Test Site: PSI EMC Lab-3m Chamber Polarization: **Vertical** Temperature: 24 °C
EUT: 3D scanner Distance: 3m Humidity: 56 %RH
M/N: EinScan Medixa Test Engineer: Felix
Test Mode: ax80 5775MHz
Test Voltage: DC 8.4V
Note:

Radiated Emission Measurement

Test Date: 2025/9/11 17:50:17

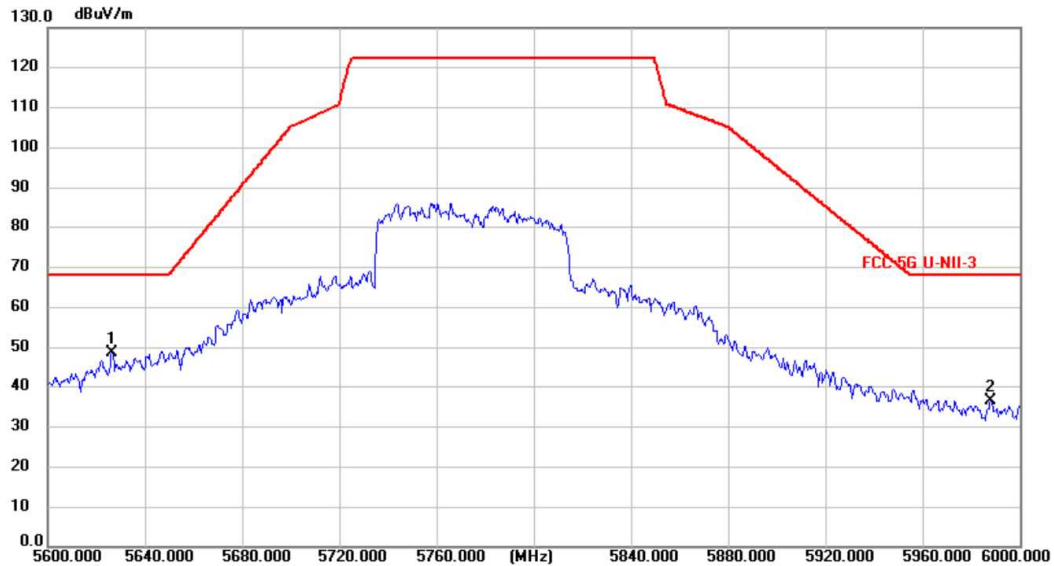

No.	Frequency (MHz)	Reading (dBuV)	Factor (dB/m)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Height (cm)	Azimuth (deg.)	P/F	Remark
1 *	5626.600	64.90	-16.36	48.54	68.20	-19.66	peak	150	205	P	
2	5988.150	52.21	-15.53	36.68	68.20	-31.52	peak	150	360	P	

Note: *:Maximum data x:Over limit !:over margin Level = Reading + Factor Margin = Level - Limit