


Impedance Plot for D450V3-SN:1113


450 Head

Calibrated impedance: $59.2\Omega + 0.9j\Omega$; Measurement impedance: $58.4\Omega + 3.7j\Omega$ (within 5Ω)

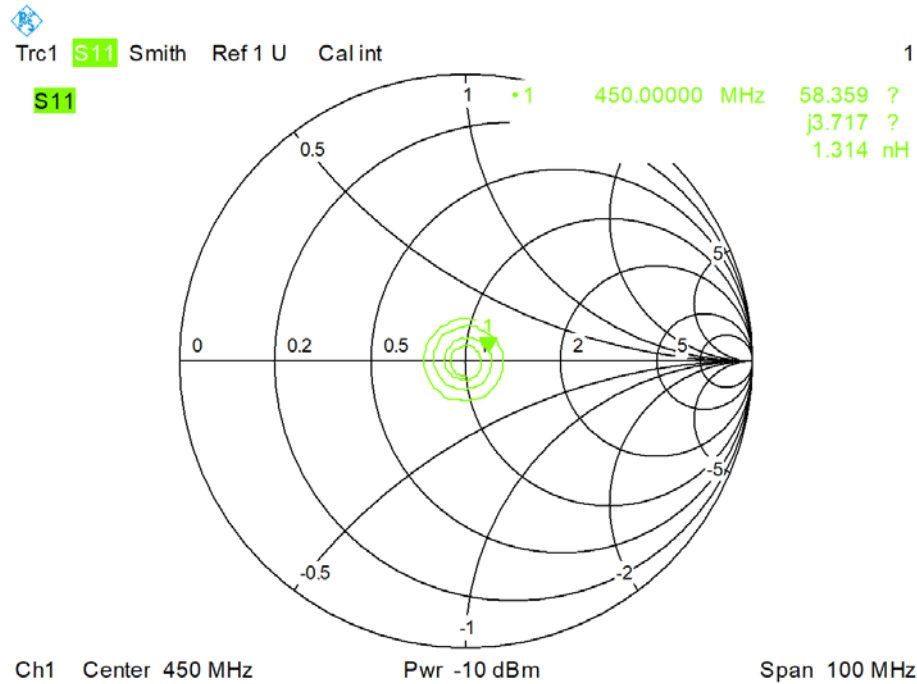

Date: 5.FEB.2026 15:26:43

Calibrated return loss: -21.5dB; Measurement return loss: -22.5dB (within 20%)

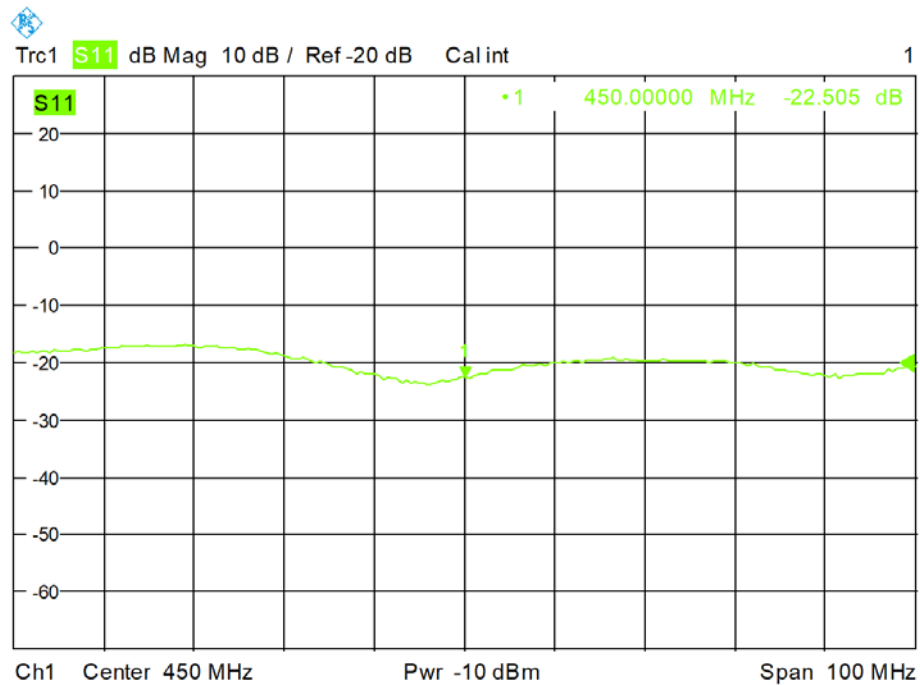

Date: 5.FEB.2026 15:20:00