

Test Report

FCC ID:2ANB8-T1

Date of issue: Jun. 26, 2017

Report Number:	MTi170811E069
Sample Description:	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment
Model(s):	T1, T1 Pro, M1
Applicant:	Getwell Health Technology (Wuhu) Co., Ltd.
Address:	4th Building, Service outsourcing park, new and high-tech zone, Yijiang District, Wuhu, Anhui
Date of Test:	Jun. 10, 2017 to Jun. 26, 2017

Shenzhen Microtest Co., Ltd.
<http://www.mttest.com>



This test report is valid for the tested samples only. It cannot be reproduced except in full without prior written consent of Shenzhen Microtest Co., Ltd.

Tel: (86-755) 88850135

Fax: (86-755) 88850136

Web: <http://www.mttest.com>

E-mail: mti@51mti.com

Address: No.102A & 302A, East Block, Hengfang Industrial Park, Xingye Road, Xixiang, Bao'an District, Shenzhen, Guangdong, China

TEST RESULT CERTIFICATION	
Applicant's name	Getwell Health Technology (Wuhu) Co., Ltd.
Address	4th Building,Service outsourcing park, new and high-tech zone, Yijiang District,Wuhu, Anhui
Manufacture's Name	Getwell Health Technology (Wuhu) Co., Ltd.
Address	4th Building,Service outsourcing park, new and high-tech zone, Yijiang District,Wuhu, Anhui
Product name	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment
Model and/or type reference :	T1
Serial Model	T1 Pro, M1
Standards	FCC Part15.247
Test procedure	ANSI C63.4-2014 ;ANSI C63.10-2013

This device described above has been tested by Shenzhen Toby Technology Co., Ltd. and the test results show that the equipment under test (EUT) is in compliance with the FCC requirements. And it is applicable only to the tested sample identified in the report.

Tested by:

Amy Lu

Amy Lu

Jun. 26, 2017

Reviewed by:

Smith Chen

Smith Chen

Jun. 26, 2017

Approved by:

Tom Xue

Tom Xue

Jun. 26, 2017

Table of Contents	Page
1 . SUMMARY OF TEST RESULTS	5
1.1 TEST FACILITY	6
1.2 MEASUREMENT UNCERTAINTY	6
2 . GENERAL INFORMATION	7
2.1 GENERAL DESCRIPTION OF EUT	7
2.2 DESCRIPTION OF TEST MODES	8
2.3 BLOCK DIGRAM SHOWING THE CONFIGURATION OF SYSTEM TESTED	9
2.4 DESCRIPTION OF SUPPORT UNITS(CONDUCTED MODE)	10
2.5 EQUIPMENTS LIST FOR ALL TEST ITEMS	11
3 . EMC EMISSION TEST	12
3.1 CONDUCTED EMISSION MEASUREMENT	12
3.1.1 POWER LINE CONDUCTED EMISSION LIMITS	12
3.1.2 TEST PROCEDURE	13
3.1.3 DEVIATION FROM TEST STANDARD	13
3.1.4 TEST SETUP	13
3.1.5 EUT OPERATING CONDITIONS	13
3.1.6 TEST RESULTS	14
3.2 RADIATED EMISSION MEASUREMENT	16
3.2.1 RADIATED EMISSION LIMITS	16
3.2.2 TEST PROCEDURE	16
3.2.3 DEVIATION FROM TEST STANDARD	17
3.2.4 TEST SETUP	18
3.2.5 EUT OPERATING CONDITIONS	19
3.2.6 TEST RESULTS (BETWEEN 9KHZ – 30 MHZ)	20
3.2.7 TEST RESULTS (BETWEEN 30MHZ – 1GHZ)	21
3.2.8 TEST RESULTS (1G-25GHZ)	22
4 . POWER SPECTRAL DENSITY TEST	24
4.1 APPLIED PROCEDURES / LIMIT	24
4.1.1 TEST PROCEDURE	24
4.1.2 DEVIATION FROM STANDARD	24
4.1.3 TEST SETUP	24
4.1.4 EUT OPERATION CONDITIONS	24
4.1.5 TEST RESULTS	25
5 . BANDWIDTH TEST	27
5.1 APPLIED PROCEDURES / LIMIT	27

Table of Contents	Page
5.1.1 TEST PROCEDURE	27
5.1.2 DEVIATION FROM STANDARD	27
5.1.3 TEST SETUP	27
5.1.4 EUT OPERATION CONDITIONS	27
5.1.5 TEST RESULTS	28
6 . PEAK OUTPUT POWER TEST	30
6.1 APPLIED PROCEDURES / LIMIT	30
6.1.1 TEST PROCEDURE	30
6.1.2 DEVIATION FROM STANDARD	30
6.1.3 TEST SETUP	30
6.1.4 EUT OPERATION CONDITIONS	30
6.1.5 TEST RESULTS	31
7 . 100 KHZ BANDWIDTH OF FREQUENCY BAND EDGE	32
7.1 DEVIATION FROM STANDARD	32
7.2 TEST SETUP	32
7.3 EUT OPERATION CONDITIONS	32
7.4 TEST RESULTS	33
8 . ANTENNA REQUIREMENT	35
8.1 STANDARD REQUIREMENT	35
8.2 EUT ANTENNA	35

1. SUMMARY OF TEST RESULTS

Test procedures according to the technical standards:

FCC Part15 (15.247) , Subpart C			
Standard Section	Test Item	Judgment	Remark
15.207	Conducted Emission	PASS	
15.247 (a)(2)	6dB Bandwidth	PASS	
15.247 (b)	Peak Output Power	PASS	
15.247 (c)	Radiated Spurious Emission	PASS	
15.247 (d)	Power Spectral Density	PASS	
15.205	Band Edge Emission	PASS	
15.203	Antenna Requirement	PASS	

NOTE:

(1) "N/A" denotes test is not applicable in this Test Report

1.1 TEST FACILITY

Shenzhen Toby Technology Co., Ltd.

Add.: 10/F.,A Block, Jiada R&D Bldg., No.5 Songpingshan, Road, Science&Technology Park,
Shenzhen, 518057

FCC Registration No.:811562

1.2 MEASUREMENT UNCERTAINTY

The reported uncertainty of measurement $y \pm U$, where expanded uncertainty U is based on a standard uncertainty multiplied by a coverage factor of $k=2$, providing a level of confidence of approximately **95 %**.

No.	Item	Uncertainty
1	Conducted Emission Test	$\pm 1.38\text{dB}$
2	RF power, conducted	$\pm 0.16\text{dB}$
3	Spurious emissions, conducted	$\pm 0.21\text{dB}$
4	All emissions, radiated(<1G)	$\pm 4.68\text{dB}$
5	All emissions, radiated(>1G)	$\pm 4.89\text{dB}$
6	Temperature	$\pm 0.5^{\circ}\text{C}$
7	Humidity	$\pm 2\%$

2. GENERAL INFORMATION

2.1 GENERAL DESCRIPTION OF EUT

Equipment	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	
Trade Name		
Model Name	T1	
Serial Model	T1 Pro , M1	
Model Difference	Packing accessory, color and pattern are difference	
Product Description	The EUT is a Getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	
	Operation Frequency:	BLE 2402-2480MHz
	Modulation Type:	GFSK
	Bit Rate of Transmitter	1Mbps
	Number Of Channel	40
	Antenna Designation:	Please see Note 3.
	Output Power(Conducted):	BLE: 1.09 dBm (Max.)
	Antenna Gain (dBi)	2dBi
Based on the application, features, or specification exhibited in User's Manual, the EUT is considered as an ITE/Computing Device. More details of EUT technical specification, please refer to the User's Manual.		
Channel List	Please refer to the Note 2.	
Power source:	DC 5V from adapter	
Adapter information:	Model:SK12G-0500100U Input:AC100-240V 50/60Hz 0.2A Max Output:DC 5V 1A	
Battery	DC 3.7V by battery	
Connecting I/O Port(s)	Please refer to the User's Manual	

Note:

1. For a more detailed features description, please refer to the manufacturer's specifications or the User's Manual.
- 2.

Channel List for BLE							
Channel	Frequency (MHz)	Channel	Frequency (MHz)	Channel	Frequency (MHz)	Channel	Frequency (MHz)
01	2402	--	---	20	2440	38	2476
02	2404	--	---	--	---	39	2478
03	2406	19	2438	--	---	40	2480

3.

Table for Filed Antenna

Ant	Brand	Model Name	Antenna Type	Connector	Gain (dBi)	NOTE
A	N/A	N/A	External antenna	/	2	BT Antenna

2.2 DESCRIPTION OF TEST MODES

To investigate the maximum EMI emission characteristics generates from EUT, the test system was pre-scanning tested base on the consideration of following EUT operation mode or test configuration mode which possible have effect on EMI emission level. Each of these EUT operation mode(s) or test configuration mode(s) mentioned above was evaluated respectively.

Pretest Mode	Description
Mode 1	BLE CH1/ CH20/ CH40
Mode 2	TX Mode


For Conducted Emission	
Final Test Mode	Description
Mode 2	TX Mode

For Radiated Emission	
Final Test Mode	Description
Mode 1	BLE CH1/ CH20/ CH40

Note:


- (1) The measurements are performed at the highest, middle, lowest available channels.
- (2) The measurements are performed at all Bit Rate of Transmitter, the worst data was reported

2.3 BLOCK DIGRAM SHOWING THE CONFIGURATION OF SYSTEM TESTED

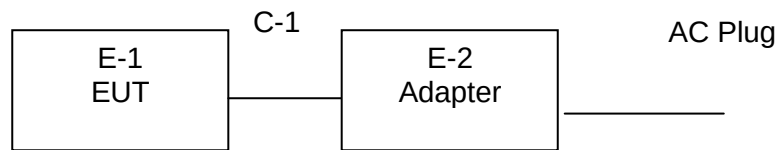

2.4 DESCRIPTION OF SUPPORT UNITS(CONDUCTED MODE)

The EUT has been tested as an independent unit together with other necessary accessories or support units. The following support units or accessories were used to form a representative test configuration during the tests.

Item	Equipment	Brand	Model/Type No.	Series No.	Note
E-1	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment		T1	N/A	EUT
E-2	/	/	/	/	

Item	Shielded Type	Ferrite Core	Length	Note
C-1	NO	NO	1.0m	
C-2	NO	NO	0.8m	

Note:

- (1) The support equipment was authorized by Declaration of Confirmation.
- (2) For detachable type I/O cable should be specified the length in cm in 『Length』 column.

2.5 EQUIPMENTS LIST FOR ALL TEST ITEMS

Equipment	Manufacturer	Model	Serial No.	Calibration Due
Universal Radio Communication Tester	Rohde&schwarz	CMU200	114587	2017/11/4
Spectrum analyzer	Agilent	E4407B	MY41441082	2017/11/4
Dc Power Supply	GW	GPR-6030D	/	2017/11/4
Temperature & Humidity Chamber	GIANT FORCE	GTH-056P	GF-94454-1	2017/11/14
Broadband TRILOG Antenna	Schwarabeck	VULB9163	9163-872	2017/11/14
Horn Antenna	Schwarzbeck	BBHA 9120 D	9120D-1145	2017/11/14
Amplifier	HP	8447D	3113A06150	2017/11/4
Amplifier	Agilent	8449B	3008A02400	2017/7/4
Test Receiver	Schwarabeck	ESPI7	100314	2017/11/4
Spectrum analyzer	Agilent	E4407B	MY41441082	2017/11/4
Signal Generator	R&S	SMT 06	832080/007	2017/11/4
Broadband TRILOG Antenna	Schwarabeck	VULB9163	9163-872	2017/11/14
Horn Antenna	Schwarzbeck	BBHA 9120 D	9120D-1145	2017/11/14
Amplifier	HP	8447D	3113A06150	2017/11/4
Amplifier	Agilent	8449B	3008A02400	2017/7/4
Test Receiver	Schwarabeck	ESPI	100314	2017/11/4
Spectrum analyzer	Agilent	E4407B	MY41441082	2017/11/4
LISN	R&S	ENV216	1001131	2017/9/25
Test Cable	United Microwave	57793	1m	2017/12/05
Test Cable	United Microwave	A30A30-5006	10m	2017/12/05

Note: the calibration interval of the above test instruments is 12 months and the calibrations are traceable to international system unit (SI).

3. EMC EMISSION TEST

3.1 CONDUCTED EMISSION MEASUREMENT

3.1.1 POWER LINE CONDUCTED EMISSION Limits (Frequency Range 150KHz-30MHz)

FREQUENCY (MHz)	Class A (dBuV)		Class B (dBuV)		Standard
	Quasi-peak	Average	Quasi-peak	Average	
0.15 -0.5	79.00	66.00	66 - 56 *	56 - 46 *	CISPR
0.50 -5.0	73.00	60.00	56.00	46.00	CISPR
5.0 -30.0	73.00	60.00	60.00	50.00	CISPR

0.15 -0.5	79.00	66.00	66 - 56 *	56 - 46 *	FCC
0.50 -5.0	73.00	60.00	56.00	46.00	FCC
5.0 -30.0	73.00	60.00	60.00	50.00	FCC

Note:

- (1) The tighter limit applies at the band edges.
- (2) The limit of " * " marked band means the limitation decreases linearly with the logarithm of the frequency in the range.

The following table is the setting of the receiver

Receiver Parameters	Setting
Attenuation	10 dB
Start Frequency	0.15 MHz
Stop Frequency	30 MHz
IF Bandwidth	9 kHz


3.1.2 TEST PROCEDURE

- The EUT was placed 0.8 meters from the horizontal ground plane with EUT being connected to the power mains through a line impedance stabilization network (LISN). All other support equipments powered from additional LISN(s). The LISN provide 50 Ohm/ 50uH of coupling impedance for the measuring instrument.
- Interconnecting cables that hang closer than 40 cm to the ground plane shall be folded back and forth in the center forming a bundle 30 to 40 cm long.
- I/O cables that are not connected to a peripheral shall be bundled in the center. The end of the cable may be terminated, if required, using the correct terminating impedance. The overall length shall not exceed 1 m.
- LISN at least 80 cm from nearest part of EUT chassis.
- For the actual test configuration, please refer to the related Item –EUT Test Photos.

3.1.3 DEVIATION FROM TEST STANDARD

No deviation

3.1.4 TEST SETUP

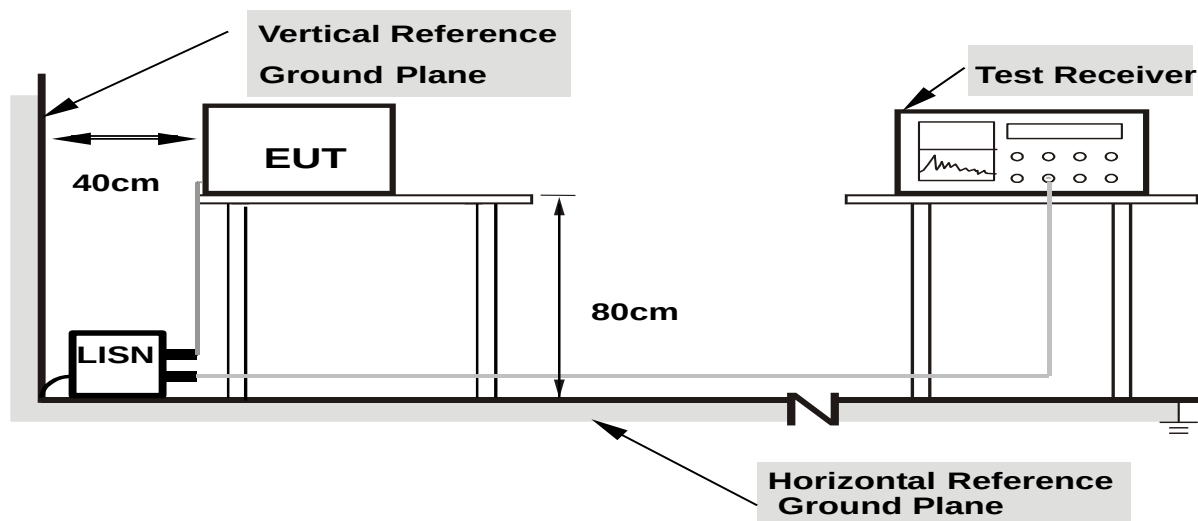

Note: 1.Support units were connected to second LISN.


2.Both of LISNs (AMN) are 80 cm from EUT and at least 80 from other units and other metal planes

3.1.5 EUT OPERATING CONDITIONS

The EUT was configured for testing in a typical fashion (as a customer would normally use it). The EUT has been programmed to continuously transmit during test. This operating condition was tested and used to collect the included data.


3.1.6 TEST RESULTS

Temperature :	26 °C	Relative Humidity :	54%
Pressure :	1010hPa	Phase :	L
Test Voltage :	DC 5Vfrom adapter AC 120V/60Hz	Test Mode :	Mode 5

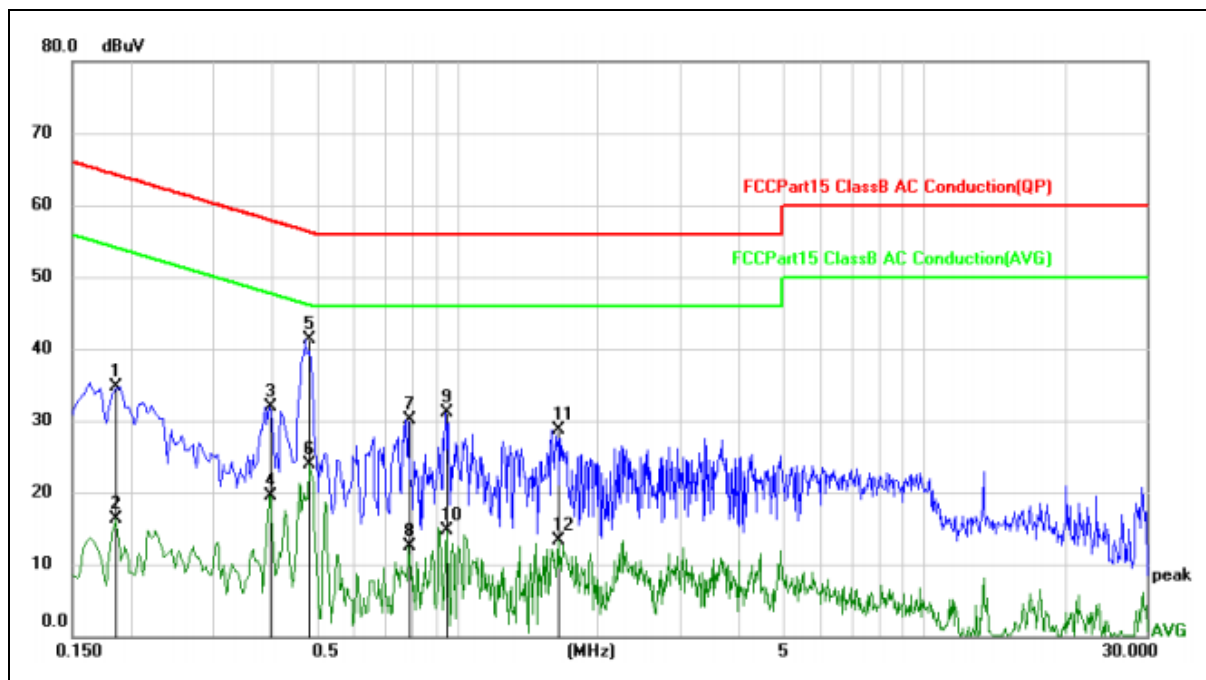

No.	Mk.	Freq. MHz	Reading Level dBuV	Correct Factor dB	Measure- ment dBuV	Limit dBuV	Over dB	Detector	Comment
1		0.1860	34.64	-0.03	34.61	64.21	-29.60	QP	
2		0.1860	16.24	-0.03	16.21	54.21	-38.00	AVG	
3		0.3975	31.98	-0.03	31.95	57.91	-25.96	QP	
4		0.3975	19.57	-0.03	19.54	47.91	-28.37	AVG	
5	*	0.4830	41.37	-0.03	41.34	56.29	-14.95	QP	
6		0.4830	23.90	-0.03	23.87	46.29	-22.42	AVG	
7		0.7890	30.07	-0.03	30.04	56.00	-25.96	QP	
8		0.7890	12.58	-0.03	12.55	46.00	-33.45	AVG	
9		0.9510	31.19	-0.04	31.15	56.00	-24.85	QP	
10		0.9510	14.82	-0.04	14.78	46.00	-31.22	AVG	
11		1.6485	28.77	-0.04	28.73	56.00	-27.27	QP	
12		1.6485	13.35	-0.04	13.31	46.00	-32.69	AVG	

Temperature :	26 °C	Relative Humidity :	54%
Pressure :	1010hPa	Phase :	N
Test Voltage :	DC 5Vfrom adapter AC 120V/60Hz	Test Mode :	Mode 5

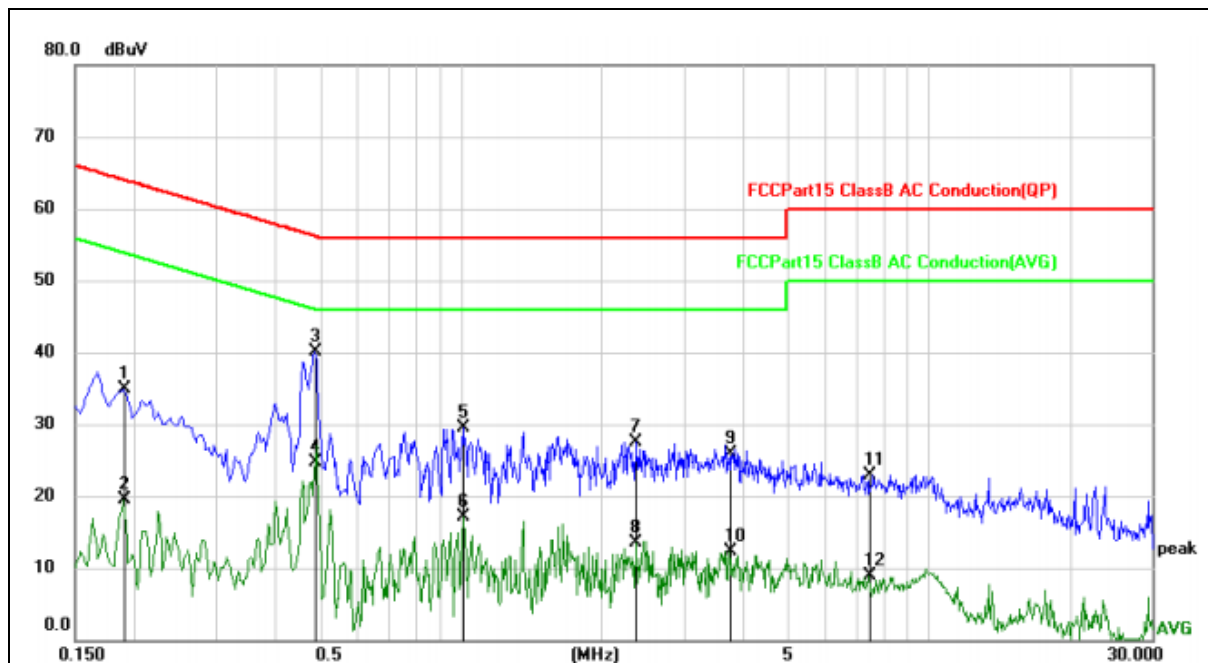

No.	Mk.	Freq. MHz	Reading Level dBμV	Correct Factor dB	Measure- ment dBμV	Limit dBμV	Over dB	Detector	Comment
1		0.1905	34.97	-0.03	34.94	64.01	-29.07	QP	
2		0.1905	19.62	-0.03	19.59	54.01	-34.42	AVG	
3	*	0.4889	40.12	-0.03	40.09	56.19	-16.10	QP	
4		0.4889	24.69	-0.03	24.66	46.19	-21.53	AVG	
5		1.0140	29.52	-0.04	29.48	56.00	-26.52	QP	
6		1.0140	17.12	-0.04	17.08	46.00	-28.92	AVG	
7		2.3640	27.49	-0.05	27.44	56.00	-28.56	QP	
8		2.3640	13.52	-0.05	13.47	46.00	-32.53	AVG	
9		3.7455	25.98	-0.05	25.93	56.00	-30.07	QP	
10		3.7455	12.41	-0.05	12.36	46.00	-33.64	AVG	
11		7.4715	22.89	-0.05	22.84	60.00	-37.16	QP	
12		7.4715	8.98	-0.05	8.93	50.00	-41.07	AVG	

3.2 RADIATED EMISSION MEASUREMENT

3.2.1 RADIATED EMISSION LIMITS (Frequency Range 9kHz-1000MHz)

20dBc in any 100 kHz bandwidth outside the operating frequency band. In case the emission fall within the restricted band specified on 15.205(a), then the 15.209(a) limit in the table below has to be followed.

Frequencies (MHz)	Field Strength (micроволts/meter)	Measurement Distance (meters)
0.009~0.490	2400/F(KHz)	300
0.490~1.705	24000/F(KHz)	30
1.705~30.0	30	30
30~88	100	3
88~216	150	3
216~960	200	3
Above 960	500	3

Spectrum Parameter	Setting
Attenuation	Auto
Start Frequency	1000 MHz
Stop Frequency	10th carrier harmonic
RB / VB (emission in restricted band)	1 MHz / 1 MHz for Peak, 1 MHz / 10Hz for Average

Receiver Parameter	Setting
Attenuation	Auto
Start ~ Stop Frequency	9kHz~150kHz / RB 200Hz for QP
Start ~ Stop Frequency	150kHz~30MHz / RB 9kHz for QP
Start ~ Stop Frequency	30MHz~1000MHz / RB 120kHz for QP

3.2.2 TEST PROCEDURE

- The measuring distance of at 3 m shall be used for measurements at frequency up to 1GHz. For frequencies above 1GHz, any suitable measuring distance may be used.
- The EUT was placed on the top of a rotating table 0.8 meters above the ground at a 3 meter open area test site. The table was rotated 360 degrees to determine the position of the highest radiation.
- The height of the equipment or of the substitution antenna shall be 0.8 m; the height of the test antenna shall vary between 1 m to 4 m. Both horizontal and vertical polarizations of the antenna are set to make the measurement.
- The initial step in collecting conducted emission data is a spectrum analyzer peak detector mode pre-scanning the measurement frequency range. Significant peaks are then marked and then Quasi Peak detector mode re-measured.
- If the Peak Mode measured value compliance with and lower than Quasi Peak Mode Limit, the EUT shall be deemed to meet QP Limits and then no additional QP Mode measurement performed.

f. For the actual test configuration, please refer to the related Item –EUT Test Photos.

Note:


Both horizontal and vertical antenna polarities were tested
and performed pretest to three orthogonal axis. The worst case emissions were reported

3.2.3 DEVIATION FROM TEST STANDARD


No deviation

3.2.4 TEST SETUP


(A) Radiated Emission Test-Up Frequency Below 30MHz

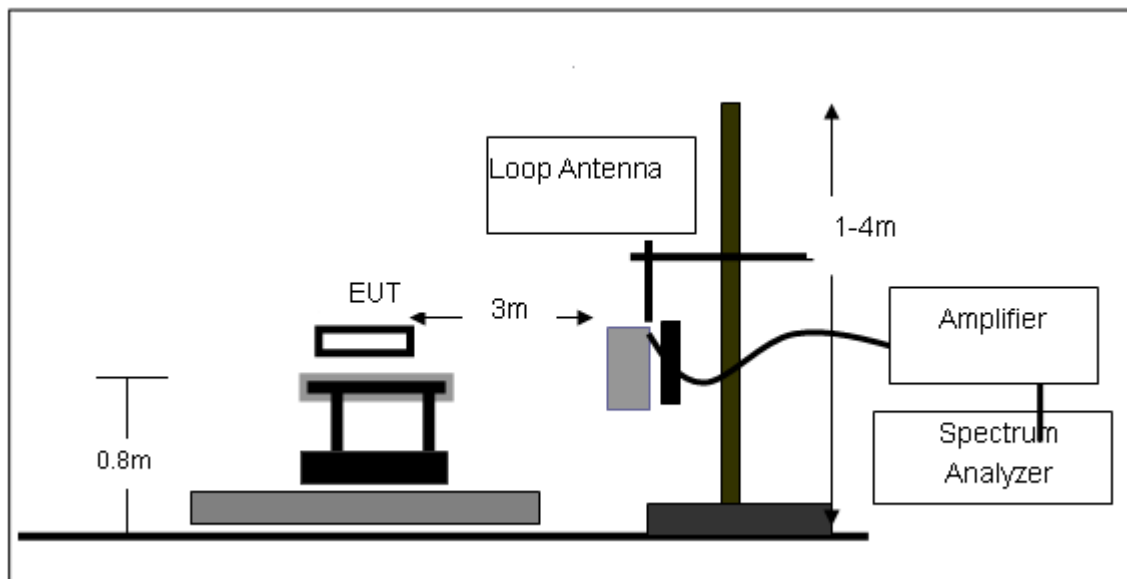

(B) Radiated Emission Test-Up Frequency 30MHz~1GHz

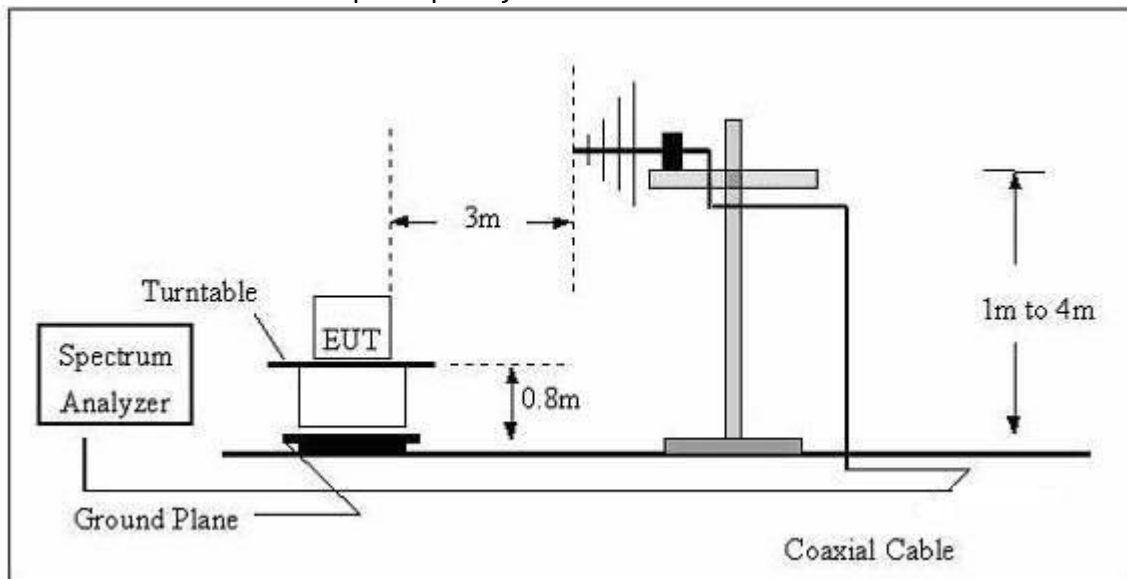

(C) Radiated Emission Test-Up Frequency Above 1GHz

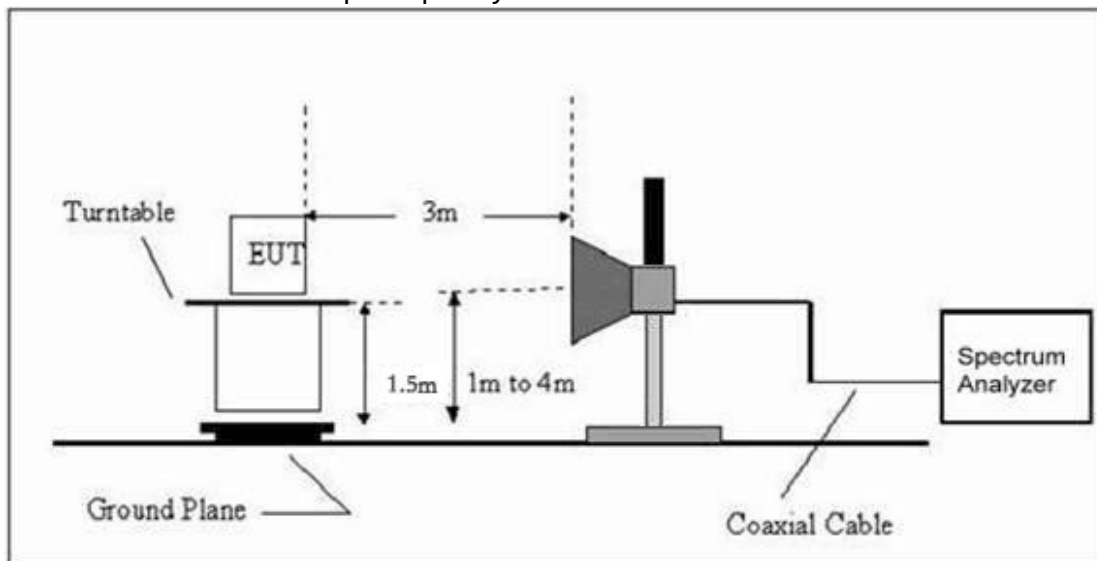

3.2.5 EUT OPERATING CONDITIONS

The EUT tested system was configured as the statements of 2.4 Unless otherwise a special operating condition is specified in the follows during the testing.

3.2.6 TEST RESULTS (BETWEEN 9KHZ – 30 MHZ)

EUT:	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name. :	T1
Temperature:	22℃	Relative Humidity:	55%
Pressure:	1010 hPa	Test Voltage :	DC 3.7V by battery
Test Mode :	TX	Polarization :	--

Freq.	Reading	Limit	Margin	State
(MHz)	(dBuV/m)	(dBuV/m)	(dB)	P/F
--	--	--	--	PASS
--	--	--	--	PASS

NOTE:

The amplitude of spurious emissions which are attenuated by more than 20dB below the permissible value has no need to be reported.

Distance extrapolation factor = $40 \log (\text{specific distance/test distance})$ (dB);

Limit line = specific limits(dBuv) + distance extrapolation factor.

3.2.7 TEST RESULTS (BETWEEN 30MHZ – 1GHZ)

EUT :	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name :	T1
Temperature :	22℃	Relative Humidity:	55%
Pressure:	1010 hPa	Test Voltage :	DC 3.7V by battery
Test Mode :	TX		

Polar (H/V)	Frequency	Meter Reading	Factor	Emission Level	Limits	Margin	Detector Type
	(MHz)	(dBuV)	(dB)	(dBuV/m)	(dBuV/m)	(dB)	
V	44.5868	27.57	-12.77	14.80	40.00	-25.20	QP
V	56.9912	24.51	-13.71	10.80	40.00	-29.20	QP
V	107.1337	24.74	-14.44	10.30	43.50	-33.20	QP
V	235.8164	23.31	-12.51	10.80	46.00	-35.20	QP
V	419.1081	25.17	-8.27	16.90	46.00	-29.10	QP
V	785.0935	24.92	-3.02	21.90	46.00	-24.10	QP
H	50.5860	25.74	-12.74	13.00	40.00	-27.00	QP
H	101.6443	25.13	-14.43	10.70	43.50	-32.80	QP
H	251.1804	25.20	-12.00	13.20	46.00	-32.80	QP
H	373.3112	25.40	-9.10	16.30	46.00	-29.70	QP
H	517.2480	25.88	-6.78	19.10	46.00	-26.90	QP
H	699.3046	26.73	-4.23	22.50	46.00	-23.50	QP
Remark: Absolute Level= ReadingLevel+ Factor, Margin= Absolute Level- Limit Factor = Antenna Factor + Cable Loss – Pre-amplifier. Factor added by measurement software automatically							

3.2.8 TEST RESULTS (1G-25GHZ)

BLE

Normal Voltage

Polar (H/V)	Frequency	Meter Reading	Factor	Emission Level	Limits	Margin	Detector Type
	(MHz)	(dBuV)	(dB)	(dBuV/m)	(dBuV/m)	(dB)	
Low Channel (2402 MHz)							
Vertical	2491.777	59.74	-10.48	49.26	74	24.74	Pk
Horizontal	2498.247	56.64	-13.37	43.27	74	30.73	Pk
Vertical	4804.184	56.63	-8.42	48.21	74	25.79	Pk
Horizontal	4804.184	56.95	-4.14	52.81	74	21.19	Pk
Vertical	1485.838	60.44	-15.71	44.73	74	29.27	Pk
Vertical	1636.784	60.13	-14.3	45.83	74	28.17	Pk
Vertical	2095.928	58.94	-10.03	48.91	74	25.09	Pk
Horizontal	1074.301	60.67	-18.82	41.85	74	32.15	Pk
Horizontal	1483.178	59.66	-18.58	41.08	74	32.92	Pk
Horizontal	1895.832	56.68	-15.63	41.05	74	32.95	Pk
Mid Channel (2440 MHz)							
Vertical	2474.777	56.52	-10.89	45.63	74	28.37	Pk
Horizontal	2474.144	57.05	-10.2	46.85	74	27.15	Pk
Vertical	4880.425	56.68	-5.87	50.81	74	23.19	Pk
Horizontal	4880.979	57.01	-6.99	50.02	74	23.98	Pk
Vertical	1433.535	63.42	-16.04	47.38	74	26.62	Pk
Vertical	1636.784	60.75	-15.47	45.28	74	28.72	Pk
Vertical	2284.166	54.49	-12.44	42.05	74	31.95	Pk
Horizontal	1280.515	60.15	-19.07	41.08	74	32.92	Pk
Horizontal	1636.784	58.98	-16.62	42.36	74	31.64	Pk
Horizontal	1892.438	59.1	-15.28	43.82	74	30.18	Pk
High Channel (2480 MHz MHz)							
Vertical	2453.883	57.02	-11.16	45.86	74	28.14	Pk
Horizontal	2453.839	57.02	-10.64	46.38	74	27.62	Pk
Vertical	4960.325	53.94	-4.4	49.54	74	24.46	Pk
Horizontal	4960.683	54.12	-2.84	51.28	74	22.72	Pk
Vertical	1187.688	58.05	-17.88	40.17	74	33.83	Pk
Vertical	1636.784	56.86	-15.61	41.25	74	32.75	Pk
Vertical	2084.693	54.45	-13.39	41.06	74	32.94	Pk
Horizontal	1534.540	57.11	-17.48	39.63	74	34.37	Pk
Horizontal	1786.985	56.82	-16.57	40.25	74	33.75	Pk
Horizontal	1892.438	56.7	-15.62	41.08	74	32.92	Pk

BAND EDGE(Radiated)

Frequency (MHz)	Meter Reading (dBμV)	Factor (dB)	Emission Level (dBμV/m)	Limits (dBμV/m)	Margin (dB)	Detector Type	Comment
BLE							
2390	58.02	-12.76	45.26	74	28.74	peak	Vertical
2390	58.48	-14.25	44.23	74	29.77	peak	Horizontal
2483.5	57.7	-12.02	45.68	74	28.32	peak	Vertical
2483.5	56.06	-12	44.06	74	29.94	peak	Horizontal

NOTE: The PK value is less than the AV value, AV value is not required.

4. POWER SPECTRAL DENSITY TEST

4.1 APPLIED PROCEDURES / LIMIT

FCC Part15 (15.247) , Subpart C				
Section	Test Item	Limit	Frequency Range (MHz)	Result
15.247	Power Spectral Density	8 dBm (in any 3KHz)	2400-2483.5	PASS

4.1.1 TEST PROCEDURE

1. Set analyzer center frequency to DTS channel center frequency.
2. Set the span to 1.5 times the DTS channel bandwidth.
3. Set the RBW ≥ 3 kHz.
4. Set the VBW $\geq 3 \times$ RBW.
5. Detector = peak.
6. Sweep time = auto couple.
7. Trace mode = max hold.
8. Allow trace to fully stabilize.
9. Use the peak marker function to determine the maximum amplitude level.
10. If measured value exceeds limit, reduce RBW (no less than 3 kHz) and repeat.

4.1.2 DEVIATION FROM STANDARD

No deviation.

4.1.3 TEST SETUP




4.1.4 EUT OPERATION CONDITIONS



The EUT tested system was configured as the statements of 2.1 Unless otherwise a special operating condition is specified in the follows during the testing.

4.1.5 TEST RESULTS

EUT :	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name :	T1
Temperature :	22℃	Relative Humidity:	55%
Pressure :	1015 hPa	Test Voltage :	DC 3.7V by battery
Test Mode :	TX Mode /CH01, CH20, CH40		

Frequency	Power Density (dBm)	Limit (dBm)	Result
2402 MHz	-20.821	8	PASS
2440 MHz	-19.799	8	PASS
2480 MHz	-18.853	8	PASS

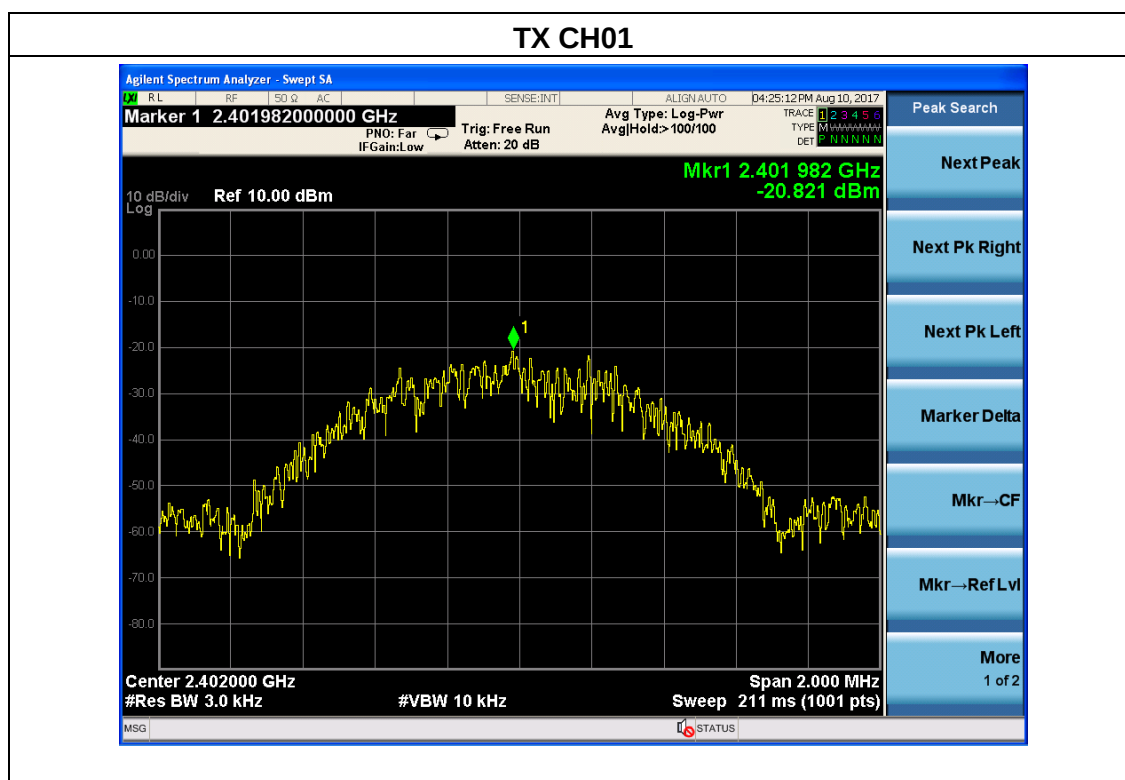

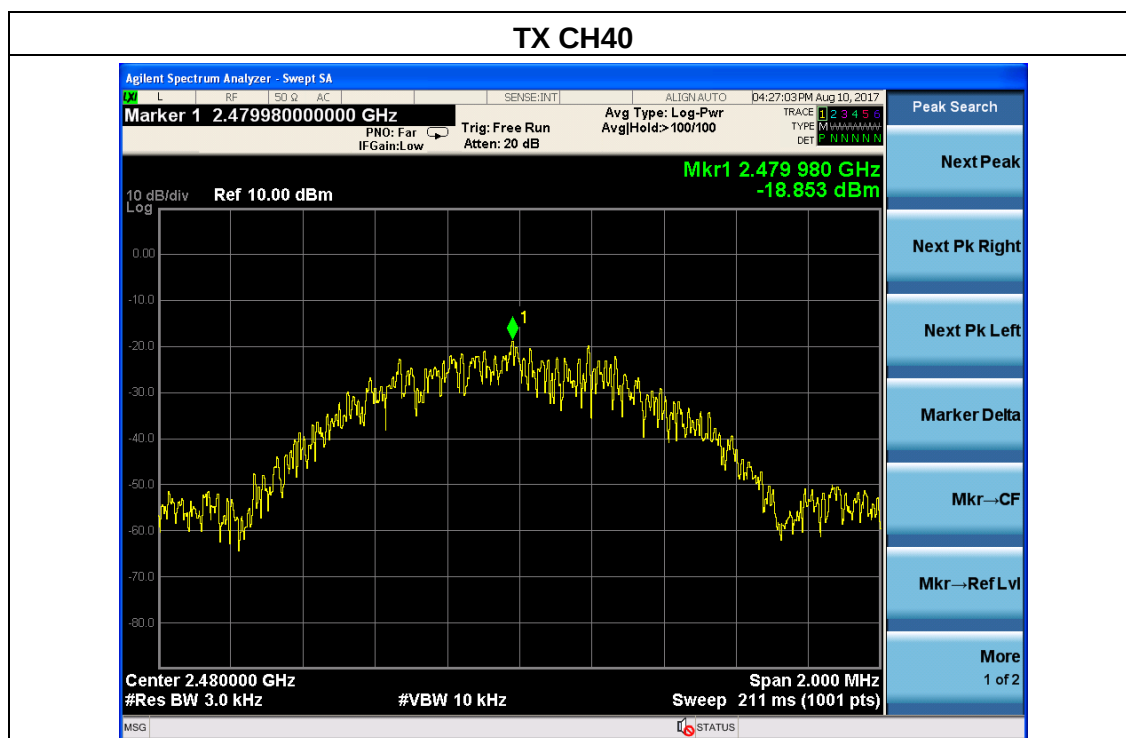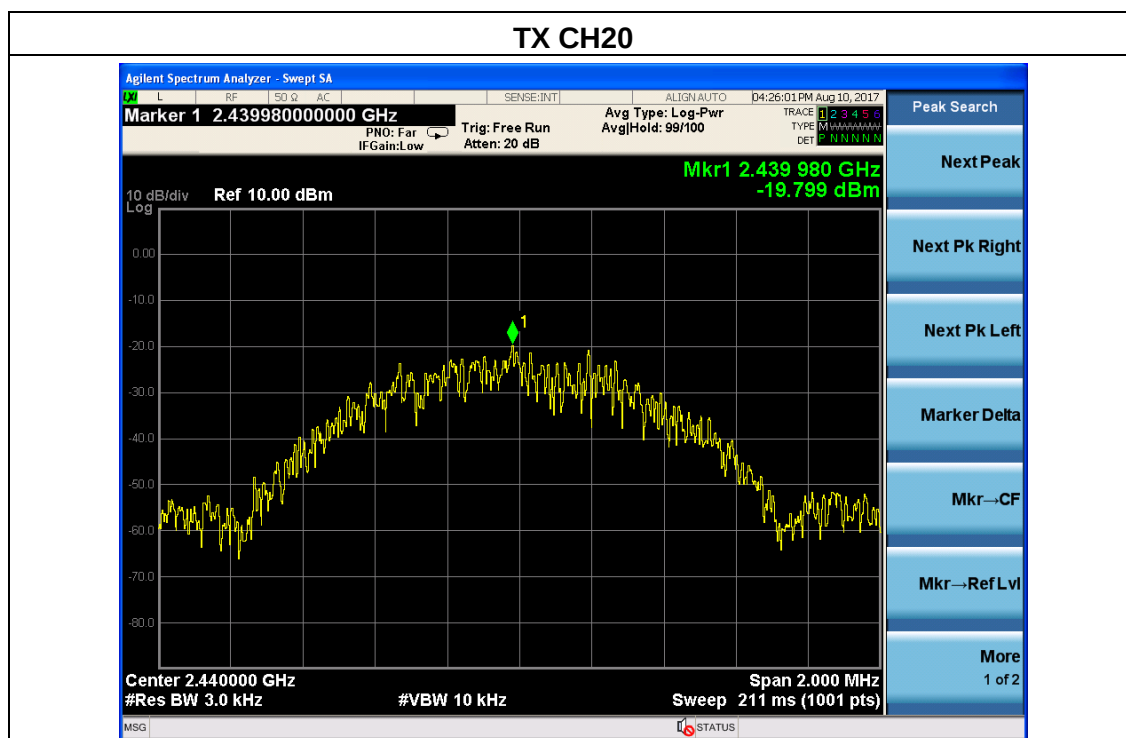

5. BANDWIDTH TEST

5.1 APPLIED PROCEDURES / LIMIT

FCC Part15 (15.247) , Subpart C				
Section	Test Item	Limit	Frequency Range (MHz)	Result
15.247(a)(2)	Bandwidth	$\geq 500\text{KHz}$ (6dB bandwidth)	2400-2483.5	PASS

5.1.1 TEST PROCEDURE

1. Set RBW= 100 kHz.
2. Set the video bandwidth (VBW) $\geq 3 \times \text{RBW}$.
3. Detector = Peak.
4. Trace mode = max hold.
5. Sweep = auto couple.
6. Allow the trace to stabilize.
7. Measure the maximum width of the emission that is constrained by the frequencies associated with the two outermost amplitude points (upper and lower) that are attenuated by 6 dB relative to the maximum level measured in the fundamental emission.

5.1.2 DEVIATION FROM STANDARD

No deviation.

5.1.3 TEST SETUP




5.1.4 EUT OPERATION CONDITIONS

The EUT tested system was configured as the statements of 2.4 Unless otherwise a special operating condition is specified in the follows during the testing.

5.1.5 TEST RESULTS

EUT :	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name :	T1
Temperature :	22℃	Relative Humidity:	55%
Pressure :	1012 hPa	Test Voltage :	DC 3.7V by battery
Test Mode :	TX Mode /CH01, CH20, CH40		

Channel	Frequency (MHz)	6dB bandwidth (KHz)	Limit (kHz)	Result
Low	2402	687.2	500	Pass
Middle	2440	686.4	500	Pass
High	2480	687.1	500	Pass

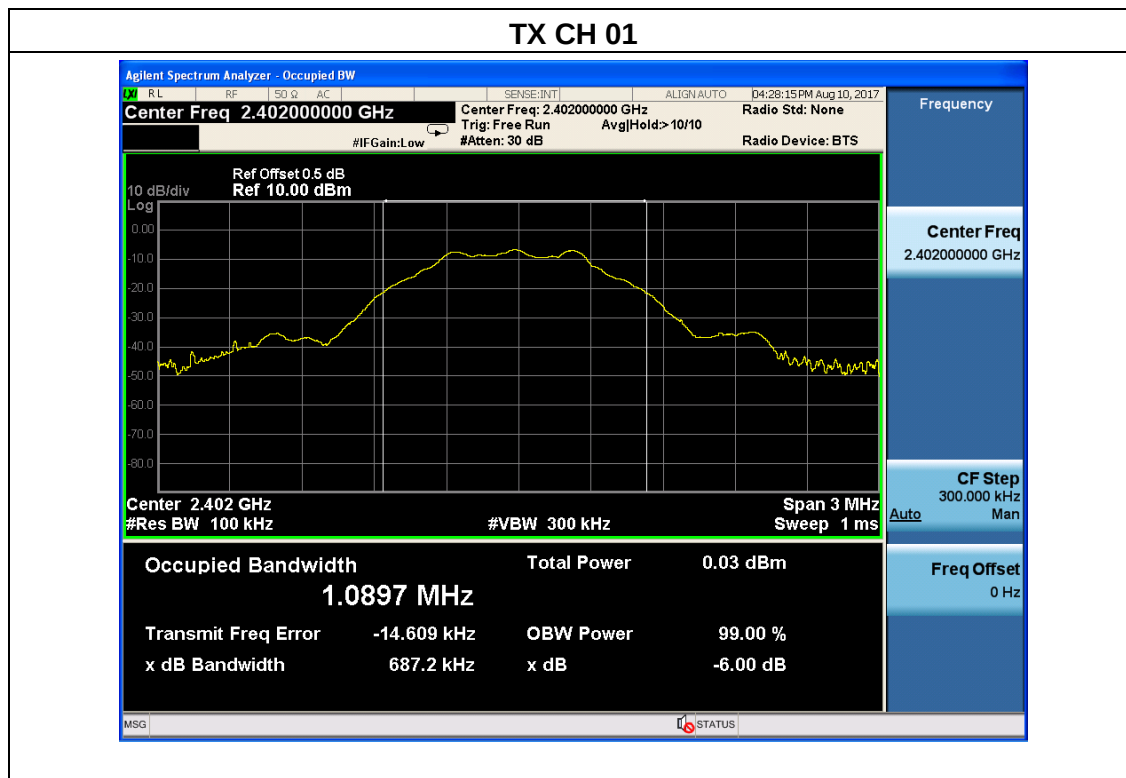

TX CH 20



TX CH 40



6. PEAK OUTPUT POWER TEST

6.1 APPLIED PROCEDURES / LIMIT

FCC Part15 (15.247) , Subpart C				
Section	Test Item	Limit	Frequency Range (MHz)	Result
15.247(b)(3)	Peak Output Power	1 watt or 30dBm	2400-2483.5	PASS

6.1.1 TEST PROCEDURE

- a. The EUT was directly connected to the Power meter

6.1.2 DEVIATION FROM STANDARD

No deviation.

6.1.3 TEST SETUP



6.1.4 EUT OPERATION CONDITIONS

The EUT tested system was configured as the statements of 2.4 Unless otherwise a special operating condition is specified in the follows during the testing.

6.1.5 TEST RESULTS

EUT :	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name :	T1
Temperature :	22℃	Relative Humidity:	55%
Pressure :	1012 hPa	Test Voltage :	DC 3.7V by battery
Test Mode :	TX Mode /CH01, CH20, CH40		

TX BLE Mode			
Test Channe	Frequency	Maximum Conducted Output Power(PK)	LIMIT
	(MHz)	(dBm)	dBm
CH01	2402	1.09	30
CH20	2440	0.42	30
CH40	2480	0.26	30

///

7. 100 KHZ BANDWIDTH OF FREQUENCY BAND EDGE

APPLICABLE STANDARD

In any 100 kHz bandwidth outside the frequency band in which the spread spectrum or digitally modulated intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement, provided the transmitter demonstrates compliance with the peak conducted power limits. If the transmitter complies with the conducted power limits based on the use of RMS averaging over a time interval, as permitted under paragraph (b)(3) of this section, the attenuation required under this paragraph shall be 30 dB instead of 20 dB. Attenuation below the general limits specified in §15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in §15.205(a), must also comply with the radiated emission limits specified in §15.209(a) (see §15.205(c)).

TEST PROCEDURE

- Check the calibration of the measuring instrument using either an internal calibrator or a known signal from an external generator.
- Position the EUT without connection to measurement instrument. Turn on the EUT and connect its antenna terminal to measurement instrument via a low loss cable. Then set it to any one measured frequency within its operating range, and make sure the instrument is operated in its linear range.
- Set RBW to 100 kHz and VBW of spectrum analyzer to 300 kHz with a convenient frequency span including 100 kHz bandwidth from band edge.
- Measure the highest amplitude appearing on spectral display and set it as a reference level. Plot the graph with marking the highest point and edge frequency.
- Repeat above procedures until all measured frequencies were complete.

7.1 DEVIATION FROM STANDARD

No deviation.

7.2 TEST SETUP



7.3 EUT OPERATION CONDITIONS


The EUT tested system was configured as the statements of 2.4 Unless otherwise a special operating condition is specified in the follows during the testing.

7.4 TEST RESULTS

EUT :	getwell Aerobic capacity assessment and muscle oxygen monitoring equipment	Model Name :	T1
Temperature :	22℃	Relative Humidity:	55%
Pressure :	1012 hPa	Test Voltage :	DC 3.7V by battery

Frequency Band	Delta Peak to band emission (dBc)	> Limit (dBc)	Result
BLE mode			
Left-band	-39.57	20	Pass
Right-band	48.69	20	Pass

BLE: Band Edge, Left Side

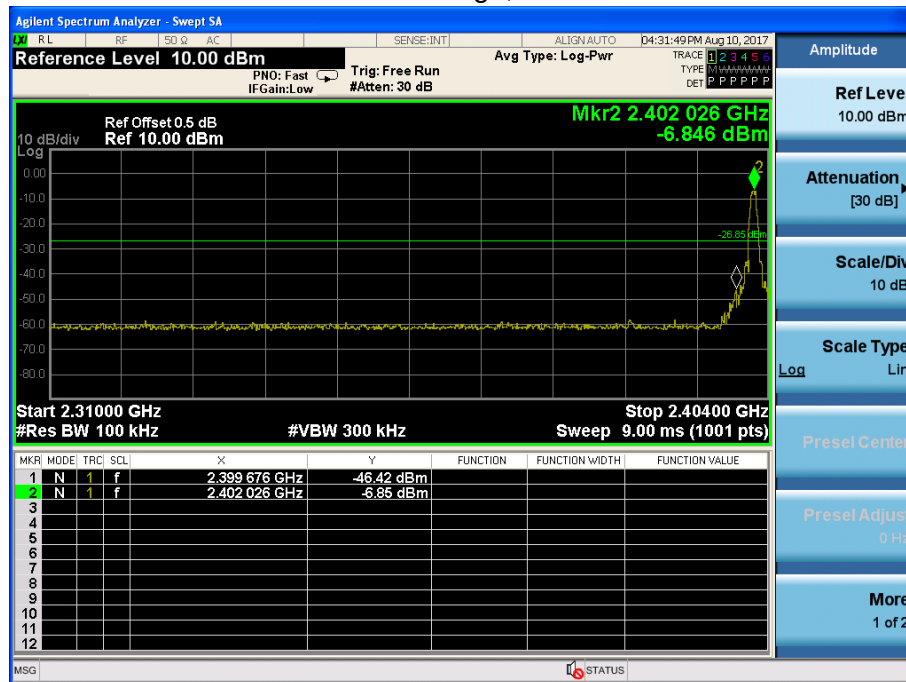

BLE: Band Edge, Right Side



8. ANTENNA REQUIREMENT

8.1 STANDARD REQUIREMENT

15.203 requirement: For intentional device, according to 15.203: an intentional radiator shall be designed to ensure that no antenna other than that furnished by the responsible party shall be used with the device.

8.2 EUT ANTENNA

The EUT antenna is Integral antenna.

----END OF REPORT----