Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

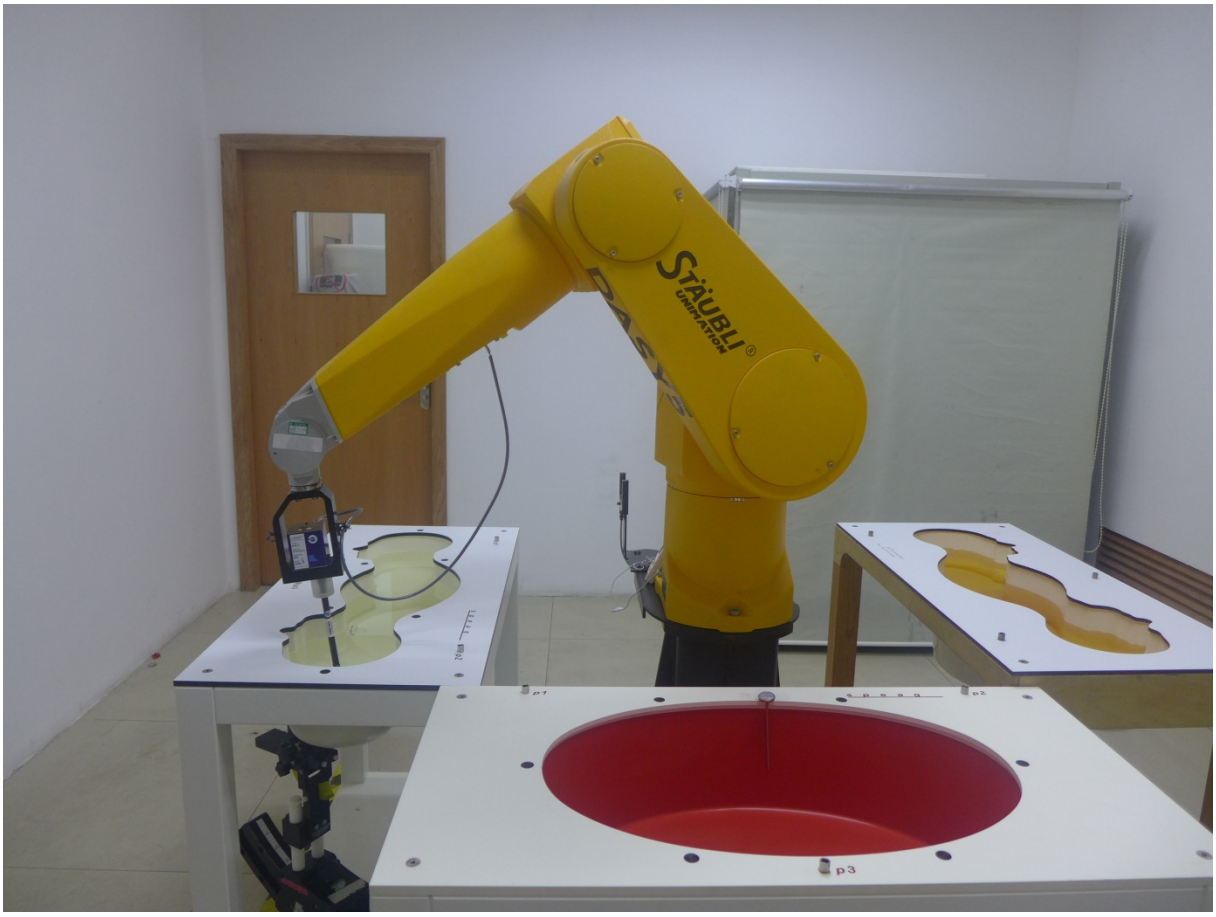

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
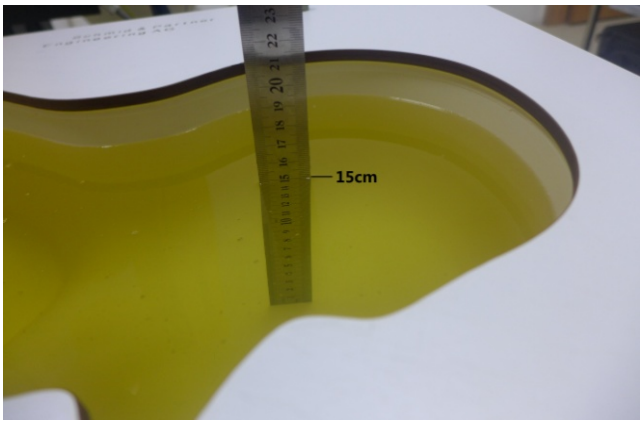	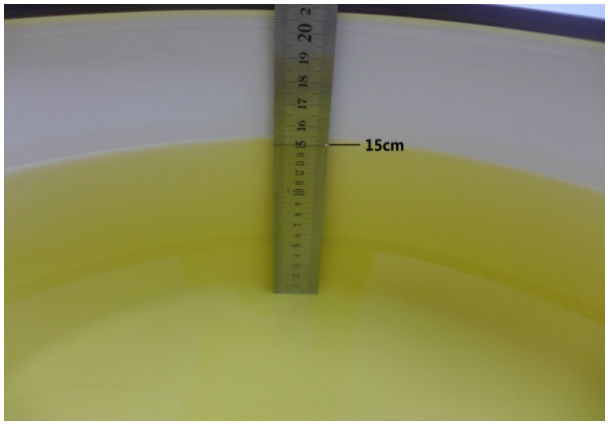
Photo 3: Tissue Simulant Liquid for Head 835	**Photo 4: Tissue Simulant Liquid for Body 835**
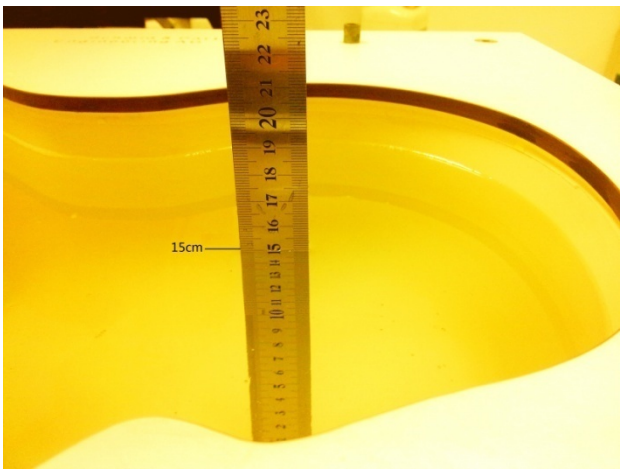	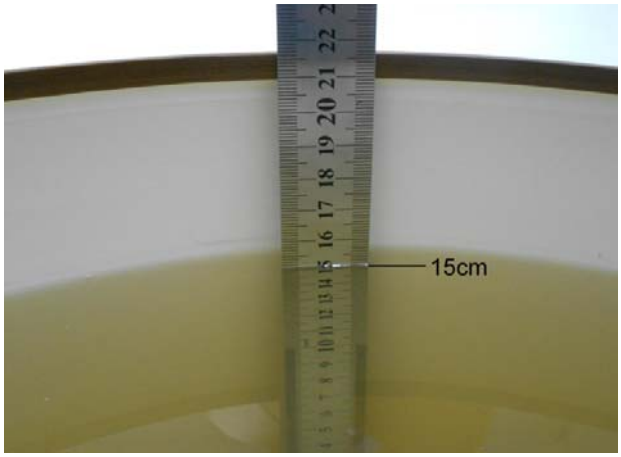

Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
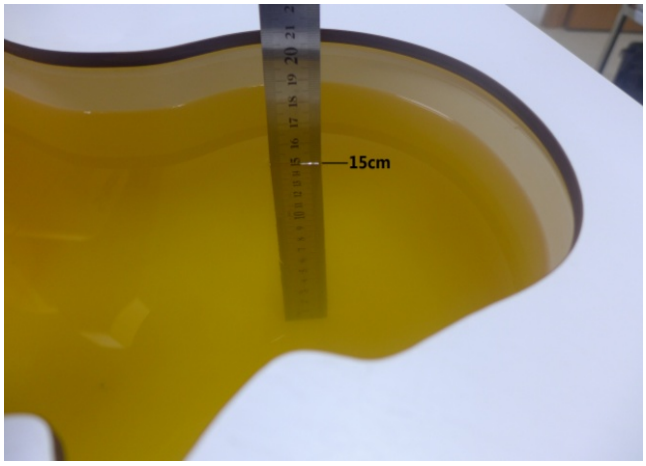	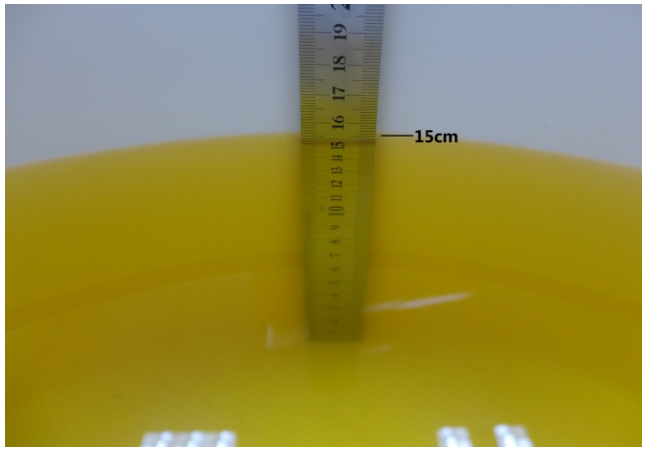
Photo 7: Tissue Simulant Liquid for Head 1900	**Photo 8: Tissue Simulant Liquid for Body 1900**
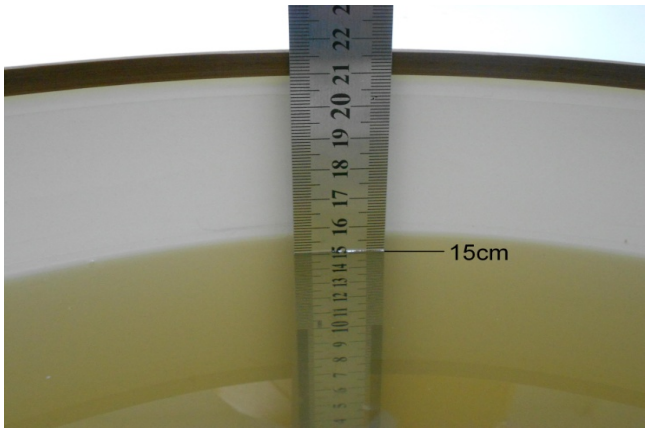	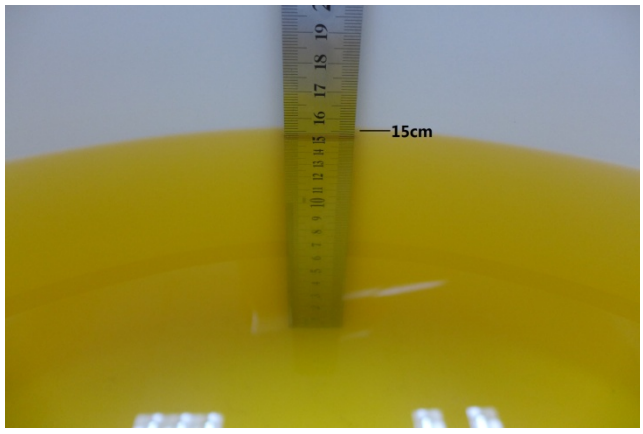

Photo 9: Tissue Simulant Liquid for Head 5G	Photo 10: Tissue Simulant Liquid for Body 5G
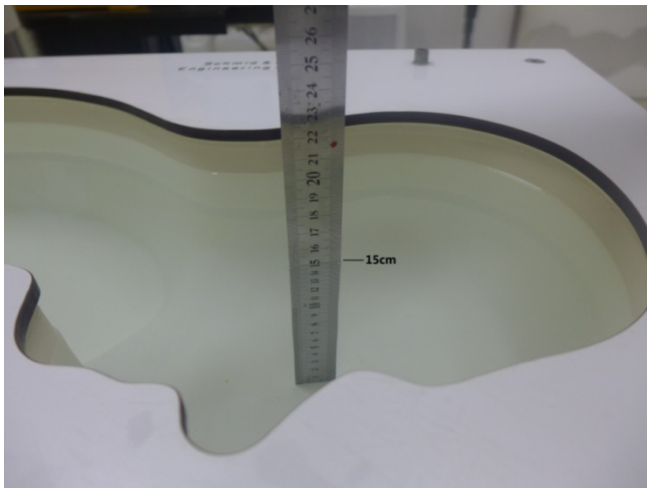	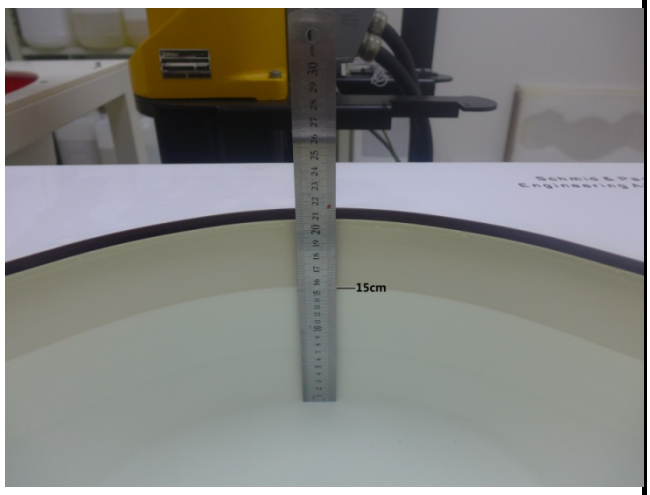

3. Photographs of EUT test position

Photo 11: Left touch cheek	Photo 12: Left tilted 15 degree
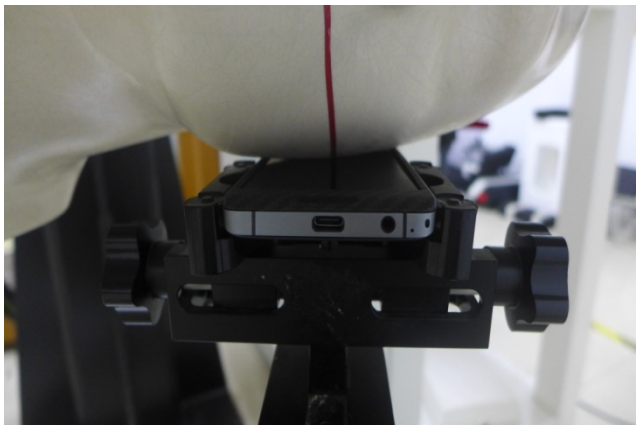	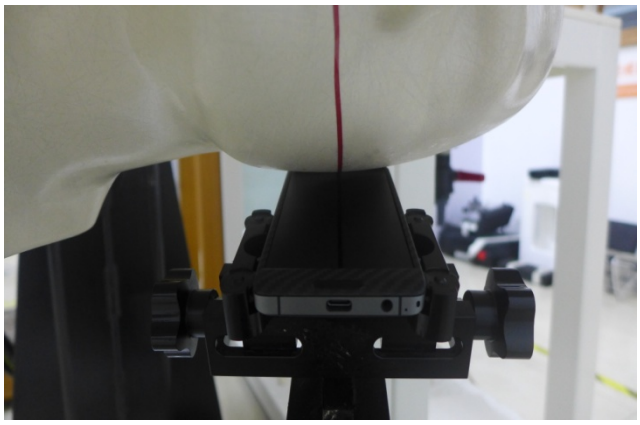
Photo 13: Right touch cheek	**Photo 14: Right tilted 15 degree**
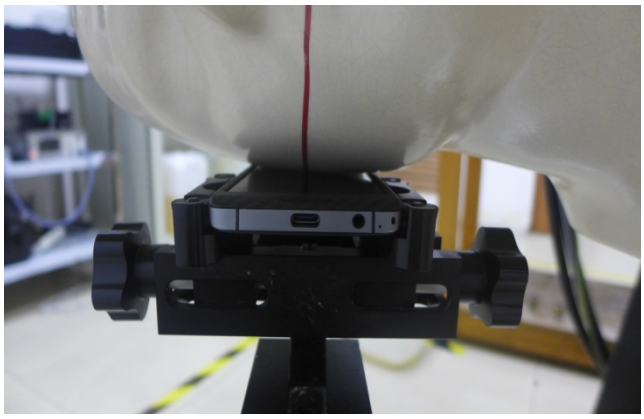	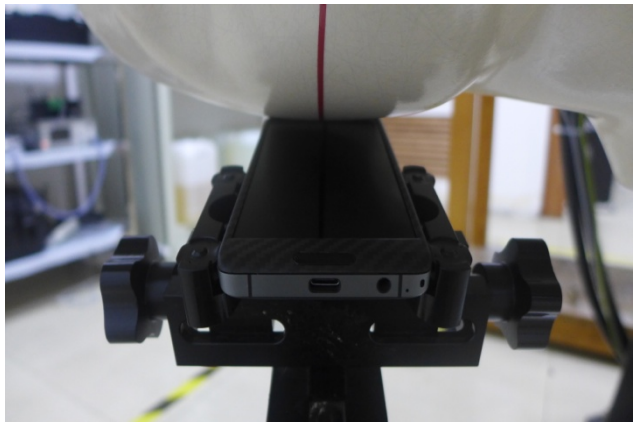
Photo 15: Front side 15mm	**Photo 16: Back side 15mm**

Photo 17: Front side 10mm	Photo 18: Back side 10mm
	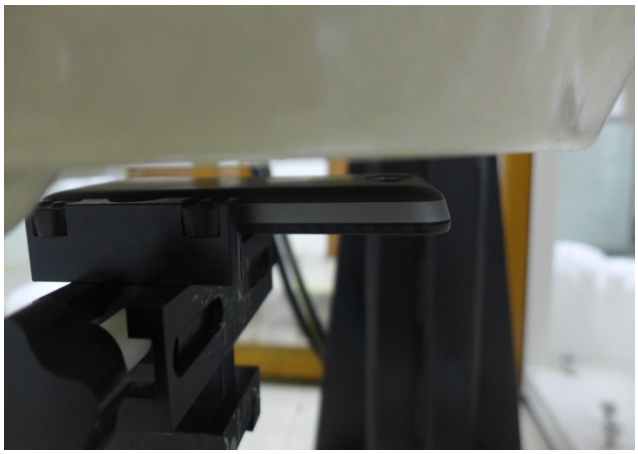
Photo 19: Left side 10mm	**Photo 20: Right side 10mm**
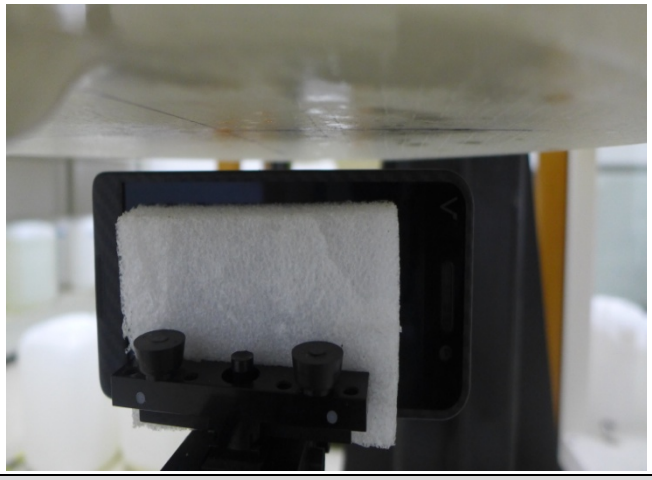	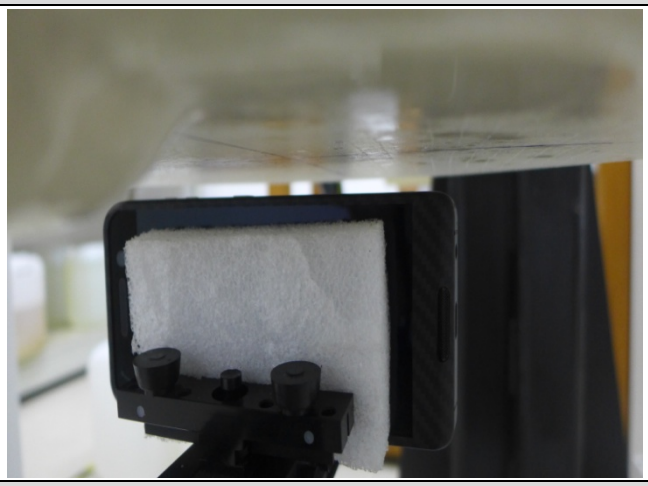
Photo 21: Top side 10mm	**Photo 22: Bottom side 10mm**
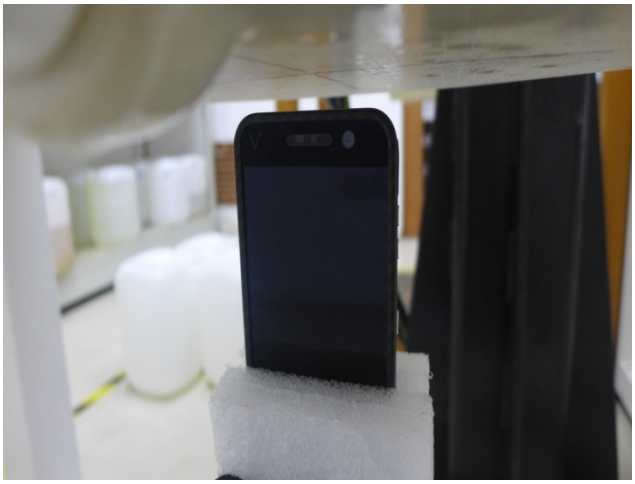	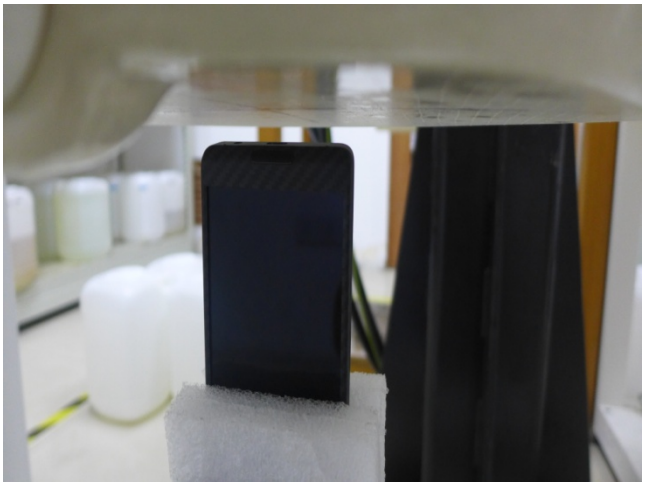

4. EUT Constructional Details

Photo 23: Front View	Photo 24: Back View
Photo 25: Accessory	**N/A**
	N/A