


ES3DV3 Sn:3127



Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

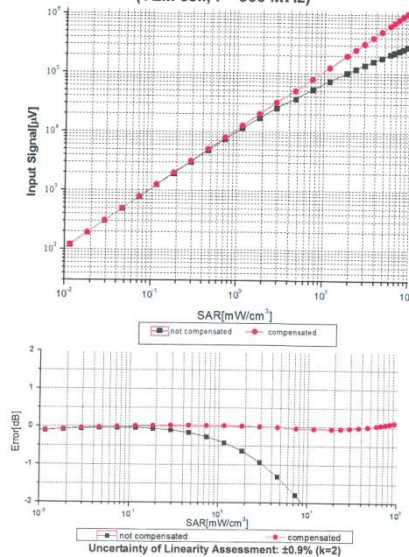


Certificate No: Z17-97142

Page 9 of 12




Conversion Factor Assessment

f=900 MHz, WGLS R9(H_convF) f=1810 MHz, WGLS R22(H_convF)

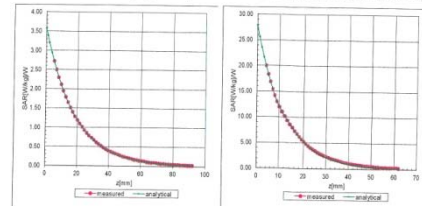

Deviation from Isotropy in Liquid

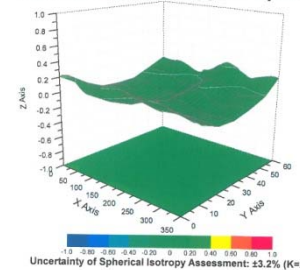

Certificate No: Z17-97142

Page 10 of 12



DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	165.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	10mm
Tip Diameter	4mm
Probe Tip to Sensor X Calibration Point	2mm
Probe Tip to Sensor Y Calibration Point	2mm
Probe Tip to Sensor Z Calibration Point	2mm
Recommended Measurement Distance from Surface	3mm

Certificate No: Z17-97142

Page 11 of 12



Appendix: Modulation Calibration Parameters

UID	Communication System Name	PAR	A dB	B dB-μV	C	VR mV	Unc ^h (k=2)
0	CW	0.00	X 0.0 Y 0.0 Z 0.0	0.0 0.0 0.0	1.0 1.0 1.0	282.3 280.9 275.1	±2.5%
10012	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	1.87	X 2.77 Y 2.75 Z 2.71	68.02 68.05 67.79	18.46 18.52 18.25	143.0 145.0 142.3	±1.8%
10100	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	5.67	X 6.13 Y 6.15 Z 6.09	66.4 66.49 66.32	18.97 19.06 18.90	141.9 144.2 140.9	±1.9%
10108	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	5.80	X 6.09 Y 6.10 Z 6.05	66.24 66.33 66.19	19.07 19.15 19.05	139.5 141.5 138.0	±1.9%
10154	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	5.75	X 5.81 Y 5.82 Z 5.79	65.85 65.92 65.89	18.93 19.01 18.97	136.1 137.8 134.7	±1.9%
10169	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	5.73	X 4.84 Y 4.82 Z 4.80	65.92 65.98 66.00	19.20 19.27 19.29	130.8 131.3 129.1	±1.9%
10175	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	5.72	X 4.88 Y 4.83 Z 4.79	66.14 66.08 66.02	19.40 19.33 19.29	131.6 130.9 129.3	±1.9%
10297	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	5.81	X 6.19 Y 6.13 Z 6.14	66.61 66.43 66.52	19.42 19.26 19.33	141.9 140.7 139.6	±1.9%

Certificate No: Z17-97142

Page 12 of 12

EX3DV4 Sn:3708

TTL Calibration Laboratory
In Collaboration with
CNAS
Add: No. 31 Xuyuan Road, Baifu District, Beijing, 100191, China
Tel: +86-10-42304633-2218 Fax: +86-10-42304633-2209
E-mail: cti@ttllab.com.cn http://www.ttllab.com

Client: **SRTC** Certificate No: **Z17-97214**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:3708**

Calibration Procedure(s): **FF-Z11-004-01**
Calibration Procedures for Dosimetric E-field Probe

Calibration date: **November 07, 2017**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±1)°C and humidity<70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter	NRP2	101919 27-Jun-17 (CTTL No.J17X05857)	Jun-18
Power sensor	NRP-Z91	101547 27-Jun-17 (CTTL No.J17X05857)	Jun-18
Power sensor	NRP-Z91	101548 27-Jun-17 (CTTL No.J17X05857)	Jun-18
Reference 10dB Attenuator	18N5RW-10dB	13-Mar-16 (CTTL No.J16X01547)	Mar-18
Reference 20dB Attenuator	18N5RW-20dB	13-Mar-16 (CTTL No.J16X01548)	Mar-18
Reference Probe EX3DV4	SN 3617	23-Jan-17 (SPEAG No EX3-3617_Jan17)	Jan-18
DAE4	SN 549	13-Dec-16 (SPEAG No DAE4-549_Dec16)	Dec-17

Secondary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator MG370DA	620102805	27-Jun-17 (CTTL No.J17X05858)	Jun-18
Network Analyzer E5071C	MY48110673	13-Jan-17 (CTTL No.J17X06285)	Jan-18

Calibrated by: **Yu Zongying** SAR Test Engineer

Reviewed by: **Lin Hai** SAR Test Engineer

Approved by: **Qi Diaryuan** SAR Project Leader

Issued: November 06, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97214

Page 1 of 12

TTL Calibration Laboratory
In Collaboration with
CNAS
Add: No. 31 Xuyuan Road, Baifu District, Beijing, 100191, China
Tel: +86-10-42304633-2218 Fax: +86-10-42304633-2209
E-mail: cti@ttllab.com.cn http://www.ttllab.com

Glossary:

TSL: tissue simulating liquid
NORM_{x,y,z}: sensitivity in free space
ConvF: sensitivity in TSL / NORM_{x,y,z}
DCP: diode compression point
CF: crest factor (1/duty_cycle) of the RF signal
A,B,C,D: modulation dependent linearization parameters
Polarization θ : θ rotation around probe axis
Polarization ϕ : ϕ rotation around an axis that is in the plane normal to probe axis (at measurement center), $\phi=0$ is normal to probe axis
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2016
d) K2B 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization ($\theta=0$ (H500MHz in TEM-cell, $\theta=1800$ MHz: waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E^2 field uncertainty inside TSL (see below ConvF).
- NORM_{x,y,z} = NORM_{x,y,z} * Frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.3. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A_{x,y,z}, B_{x,y,z}, C_{x,y,z}, V₀, μ , A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f>300MHz) and inside waveguide using analytical field distributions based on power measurements for f>300MHz. The same setups are used for assessment of the parameters applied for boundary compensation (shape, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from 50MHz to 100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_{x,y,z} (no uncertainty required).

Certificate No: Z17-97214

Page 2 of 12



Probe EX3DV4

SN: 3708

Calibrated: November 07, 2017
Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system)

Certificate No: Z17-97214

Page 3 of 12



DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3708

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ₀ (V/m) ^A	0.19	0.36	0.44	±10.0%
DCP(mV) ^B	95.1	102.7	105.5	

Modulation Calibration Parameters

UID	Communication System Name	A dB	B dB/μV	C dB	D dB	VR mV	Unc ^E (k=2)
0	CW	X 0.0	0.0	1.0	0.00	95.9	±3.1%
		Y 0.0	0.0	1.0		149.0	
		Z 0.0	0.0	1.0		169.4	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiply by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm₀ X, Y, Z do not effect the E^2 field uncertainty inside TSL (see Page 6 and Page 9).
^B Numerical linearization parameter: uncertainty not required.
^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: Z17-97214

Page 4 of 12

EX3DV4 Sn:3708



DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3708

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Relative Permittivity ¹	Conductivity [S/m]	ConvF X	ConvF Y	ConvF Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)
900	41.5	0.97	9.07	9.07	9.07	0.15	1.37	±12.1%
1810	40.0	1.40	7.77	7.77	7.77	0.24	1.04	±12.1%
2000	40.0	1.40	7.80	7.80	7.80	0.28	0.88	±12.1%
2450	39.2	1.80	7.19	7.19	7.19	0.34	1.03	±12.1%
5200	36.0	4.66	5.64	5.64	5.64	0.40	1.35	±13.3%
5300	35.9	4.76	5.43	5.43	5.43	0.40	1.35	±13.3%
5500	35.6	4.96	5.03	5.03	5.03	0.40	1.50	±13.3%
5600	35.5	5.07	4.89	4.89	4.89	0.40	1.60	±13.3%
5800	35.3	5.27	5.03	5.03	5.03	0.45	1.45	±13.3%

¹ Frequency validity above 300 MHz of a 100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to 50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is a 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to a 110 MHz.

² At frequency below 3 GHz, the validity of tissue parameters (x and y) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (x and y) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

³ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below a 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z17-97214

Page 3 of 12



DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3708

Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz]	Relative Permittivity ¹	Conductivity [S/m]	ConvF X	ConvF Y	ConvF Z	Alpha ²	Depth ³ (mm)	Unc. (k=2)
900	56.0	1.05	9.18	9.16	9.16	0.17	1.40	±12.1%
1810	53.3	1.52	7.70	7.70	7.70	0.20	1.13	±12.1%
2000	53.3	1.52	7.76	7.76	7.76	0.14	1.60	±12.1%
2450	52.7	1.95	7.30	7.30	7.30	0.66	0.70	±12.1%
5200	49.0	5.30	4.79	4.79	4.79	0.45	1.80	±13.3%
5300	48.9	5.42	4.56	4.56	4.56	0.45	1.80	±13.3%
5500	48.6	5.65	4.17	4.17	4.17	0.50	1.75	±13.3%
5600	48.5	5.77	4.10	4.10	4.10	0.50	1.60	±13.3%
5800	48.2	6.00	4.19	4.19	4.19	0.55	1.85	±13.3%

¹ Frequency validity above 300 MHz of a 100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to 50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is a 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to a 110 MHz.

² At frequency below 3 GHz, the validity of tissue parameters (x and y) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (x and y) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


³ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below a 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z17-97214

Page 4 of 12



Frequency Response of E-Field (TEM-Cell: IF110 EXX, Waveguide: R22)

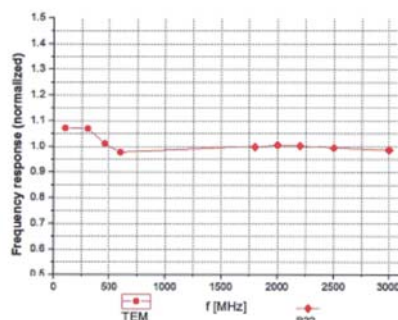

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No: Z17-97214



Page 7 of 12



Receiving Pattern (Φ, θ=0°)

f=600 MHz, TEM


f=1800 MHz, R22

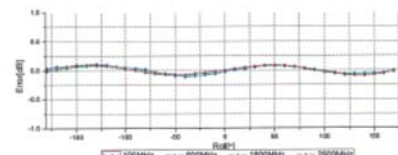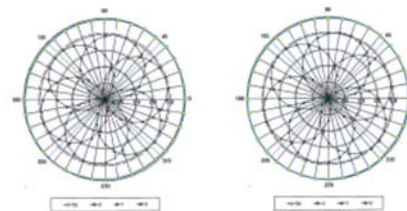

Certificate No: Z17-97214


Page 8 of 12

EX3DV4 Sn:3708

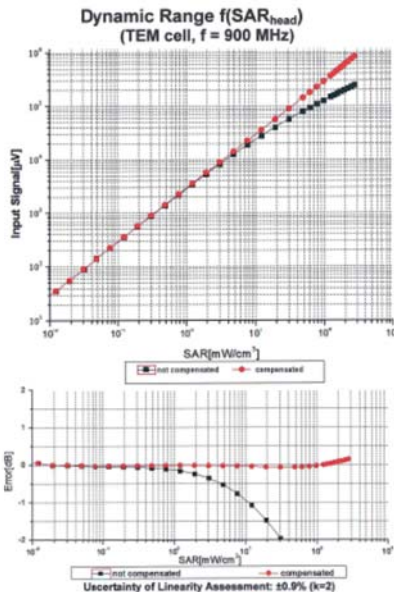

Certificate No: Z17-97214

Page 9 of 12

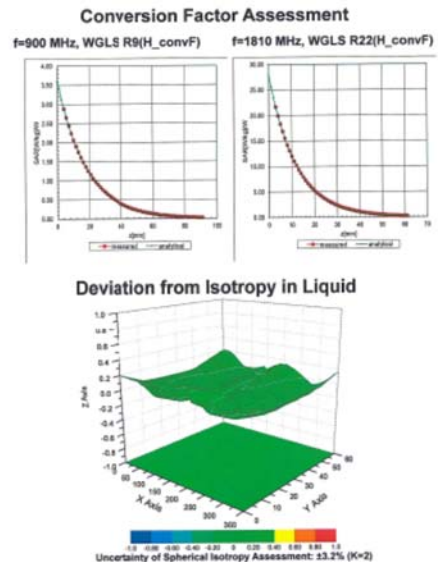

Certificate No: Z17-97214

Page 10 of 12



DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3708

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	177.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Certificate No: Z17-97214

Page 11 of 12



Appendix (Additional assessments outside the scope of FCC approved dual-logo scope)

Modulation Calibration Parameters

UID	Communication System Name	PAR	A	B	C	VR	Unc ¹
0	CW	0.00	X 0.0 0.0 1.0	Y 0.0 0.0 1.0	Z 0.0 0.0 1.0	95.9	±3.1%
10011	UMTS-FDD (WCDMA)	2.91	X 2.97 64.29 16.82	Y 3.15 66.44 17.98	Z 3.21 67.23 18.44	147.4	±1.8%
10021	GSM-FDD (TDMA GMSK)	9.39	X 0.95 57.62 9.60	Y 1.22 59.57 9.93	Z 1.13 59.66 9.94	48.2	±2.4%
10062	IEEE 802.11a/b Wi-Fi 5 GHz (OFDM 6 Mbps)	8.68	X 9.01 65.22 19.38	Y 8.26 63.95 18.73	Z 8.53 64.77 19.13	92.1	±2.1%

Certificate No: Z17-97214

Page 12 of 12

D750V3 Sn:1101

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

中国认可
国际互认
校准
CALIBRATION
CNAS L6570

Client: **SRTC** Certificate No: **Z17-97134**

CALIBRATION CERTIFICATE

Object: **D750V3 - SN: 1101**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **September 13, 2017**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRV-D	102196	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
Power sensor NRV-Z5	100596	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
Reference Probe EX30V4	SN 7433	28-Sep-16(SPEAG, No EX3-7433_Sep16)	Sep-17
DAE4	SN 1331	19-Jan-17(CTTL-SPEAG, No Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No.J17X00286)	Jan-18
Network Analyzer E5071C	MY46111013	13-Jan-17 (CTTL, No.J17X00286)	Jan-18

Calibrated by: **Zhao Jing** Function: **SAR Test Engineer** Signature:

Reviewed by: **Yu Zongying** Function: **SAR Test Engineer** Signature:

Approved by: **Qi Dianyan** Function: **SAR Project Leader** Signature:

Issued: September 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97134

Page 1 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
d) KDB655664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:
e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:
• **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• **SAR measured:** SAR measured at the stated antenna input power.
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97134

Page 2 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY52	52.10.0.1446
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.88 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.05 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	8.26 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.34 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	5.39 mW / g ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.95 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.15 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	8.69 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.42 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	5.73 mW / g ± 18.7 % (k=2)

Certificate No: Z17-97134

Page 3 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.com

Appendix (Additional assessments outside the scope of CNAS L6570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.90 ± 0.24jΩ
Return Loss	- 28.4dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.0Ω; 2.22jΩ
Return Loss	- 30.6dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.136 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z17-97134

Page 4 of 8


D750V3 Sn:1101



DASY5 Validation Report for Head TSL Date: 09.13.2017
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1101
Communication System: UTD 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 750$ MHz; $\sigma = 0.879$ S/m; $\epsilon_r = 41.54$; $\rho = 1000$ kg/m³
Phantom section: Left Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(10.01, 10.01, 10.01); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 53.10 V/m; Power Drift = -0.05 dB
Peak SAR (extrapolated) = 3.17 W/kg
SAR(1 g) = 2.05 W/kg; SAR(10 g) = 1.34 W/kg
Maximum value of SAR (measured) = 2.77 W/kg

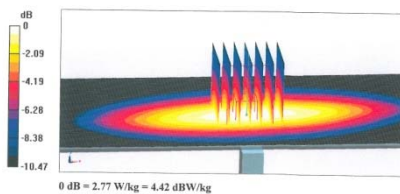


Certificate No: Z17-97134

Page 5 of 8



Impedance Measurement Plot for Head TSL

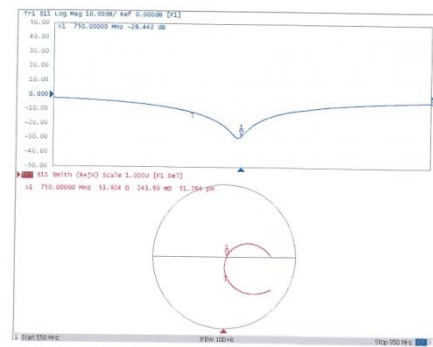

Certificate No: Z17-97134


Page 6 of 8



DASY5 Validation Report for Body TSL Date: 09.13.2017
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1101
Communication System: UTD 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 750$ MHz; $\sigma = 0.946$ S/m; $\epsilon_r = 55.41$; $\rho = 1000$ kg/m³
Phantom section: Center Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(9.83, 9.83, 9.83); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 53.35 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 3.27 W/kg
SAR(1 g) = 2.15 W/kg; SAR(10 g) = 1.42 W/kg
Maximum value of SAR (measured) = 2.88 W/kg

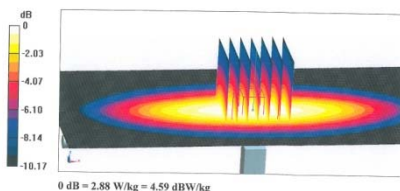


Certificate No: Z17-97134

Page 7 of 8



Impedance Measurement Plot for Body TSL

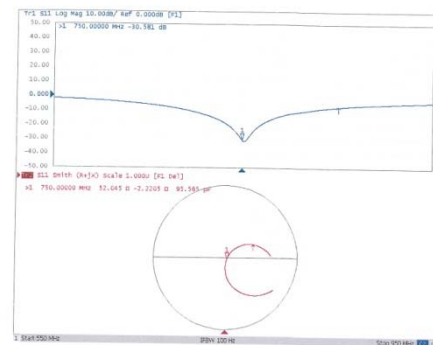

Certificate No: Z17-97134

Page 8 of 8

D835V2 Sn:4d023

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

中国认可
国际互认
校准
CALIBRATION
CNAS L0570

Client: **SRTC** Certificate No: **Z17-97135**

CALIBRATION CERTIFICATE

Object: **D835V2 - SN: 4d023**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **September 13, 2017**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRV-D	102196	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Power sensor NRV-Z5	100590	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG No.EK3-7433_Sep16)	Sep-17
DAE4	SN 1331	19-Jan-17(CTTL-SPEAG No.Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL No.J17X00286)	Jan-18
Network Analyzer ES071C	MY46110673	13-Jan-17 (CTTL No.J17X00285)	Jan-18

Calibrated by: **Zhao Jing** SAR Test Engineer Signature: *[Signature]*

Reviewed by: **Yu Zongying** SAR Test Engineer Signature: *[Signature]*

Approved by: **Qi Dianyuan** SAR Project Leader Signature: *[Signature]*

Issued: September 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: Z17-97135

Page 1 of 8

Glossary:
TSL tissue simulating liquid
ConvF sensitivity in TSL / NORMx.y.z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB855664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

- dASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement, multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97135

Page 2 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

Measurement Conditions
dASY system configuration, as far as not given on page 1.

DASY Version	DASY2	52.10.0.1446
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S 1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	0.90 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.35 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	9.37 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.52 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.06 mW / g ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.7 ± 6 %	0.96 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.34 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	9.47 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.53 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	6.17 mW / g ± 18.7 % (k=2)

Certificate No: Z17-97135

Page 3 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.0Q-2.79jQ
Return Loss	-30.7dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.6Q-3.61jQ
Return Loss	-25.8dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.495 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.


Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z17-97135


Page 4 of 8

D835V2 Sn:4d023

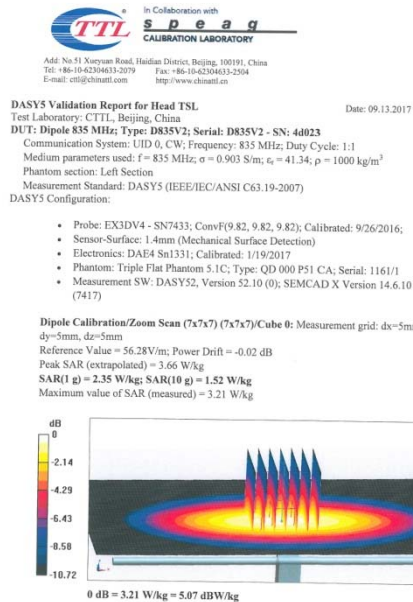


Certificate No: Z17-97135

Page 5 of 8

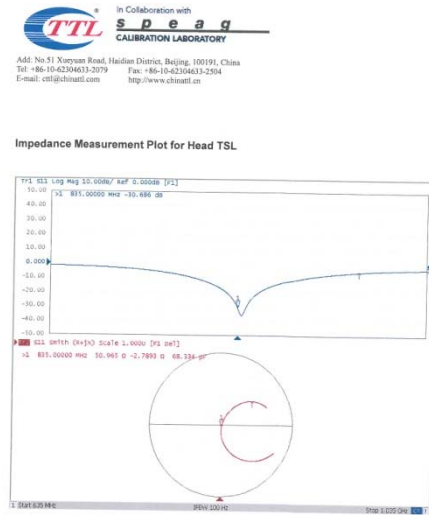


Certificate No: Z17-97135

Page 6 of 8

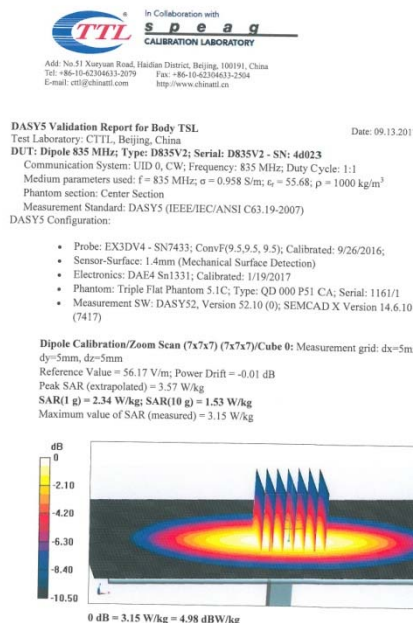

Certificate No: Z17-97135

Page 7 of 8

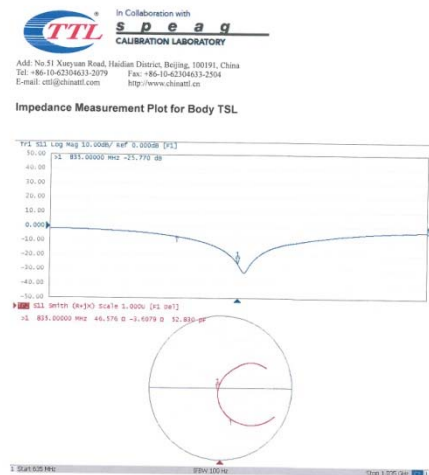

Certificate No: Z17-97135

Page 8 of 8

D1800V2 Sn:2d084

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatitl.cn

中国认可
国际互认
校准
CNAS
CALIBRATION
CNAS L0570

Client: **SRTC** Certificate No: **Z17-97138**

CALIBRATION CERTIFICATE

Object: D1800V2 - SN: 2d084

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: September 15, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	102196	02-Mar-17 (CTTL, No J17X01254)	Mar-18
Power sensor NRP-Z91	100596	02-Mar-17 (CTTL, No J17X01254)	Mar-18
Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG, No EX3-7433_Sep16)	Sep-17
DAE4	SN 1331	19-Jan-17(CTTL-SPEAG, No Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No J17X00286)	Jan-18
Network Analyzer E5071C	MY46110673	13-Jan-17 (CTTL, No J17X00286)	Jan-18

Calibrated by: Name: Zhao Jing Function: SAR Test Engineer Signature: [Signature]

Reviewed by: Yu Zongying SAR Test Engineer [Signature]

Approved by: Qi Danyuan SAR Project Leader [Signature]

Issued: September 18, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97138

Page 1 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatitl.cn

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:
e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:
• **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• **SAR measured:** SAR measured at the stated antenna input power.
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97138

Page 2 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatitl.cn

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.0.1446
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S 1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.4 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.79 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	38.9 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.12 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.4 mW / g ± 18.7 % (k=2)

Body TSL parameters
The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.8 ± 6 %	1.50 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.84 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	39.7 mW / g ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.18 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.8 mW / g ± 18.7 % (k=2)

Certificate No: Z17-97138

Page 3 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatitl.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.3Ω - 1.55Ω
Return Loss	- 35.4dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.0Ω - 1.32Ω
Return Loss	- 27.1dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.316 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z17-97138

Page 4 of 8


D1800V2 Sn:2d084



DASY5 Validation Report for Head TSL Date: 09.15.2017
 Test Laboratory: CCTL, Beijing, China
DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d084
 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 1800 \text{ MHz}$; $\sigma = 1.423 \text{ S/m}$; $\tau = 40.37$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Left Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(7.97, 7.97, 7.97); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASYS2, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:
dx=5mm, dy=5mm, dz=5mm
Reference Value = 93.90 V/m; Power Drift = 0.01 dB
Peak SAR (extrapolated) = 18.7 W/kg
SAR(1 g) = 9.79 W/kg; SAR(10 g) = 5.12 W/kg
Maximum value of SAR (measured) = 15.5 W/kg

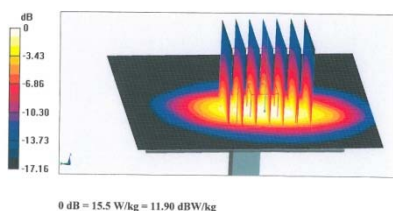


Certificate No: Z17-97138

Page 5 of 8




Impedance Measurement Plot for Head TSL

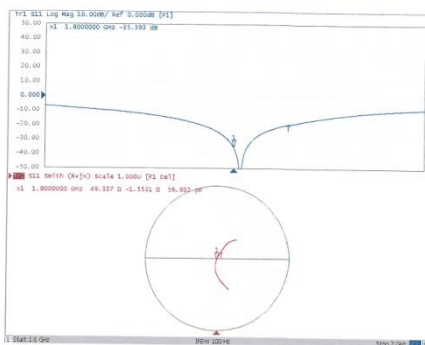

Certificate No: Z17-97138


Page 6 of 8



DASY5 Validation Report for Body TSL Date: 09/14/2017
 Test Laboratory: CTTI, Beijing, China
DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2c0d84
 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 1800 \text{ MHz}$; $\sigma = 1.503 \text{ S/m}$; $\epsilon_r = 53.79$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Center Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(7.75, 7.75, 7.75); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 SN1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7413)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:
dx=5mm, dy=5mm, dz=5mm
Reference Value = 97.57 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 18.0 W/kg
SAR(1 g) = 9.84 W/kg; SAR(10 g) = 5.18 W/kg
Maximum value of SAR (measured) = 15.2 W/kg

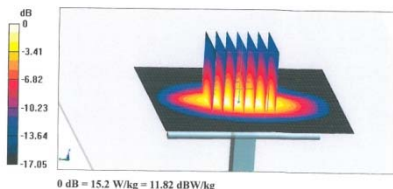


Certificate No: Z17-97138

Page 7 of 8



Impedance Measurement Plot for Body TSL

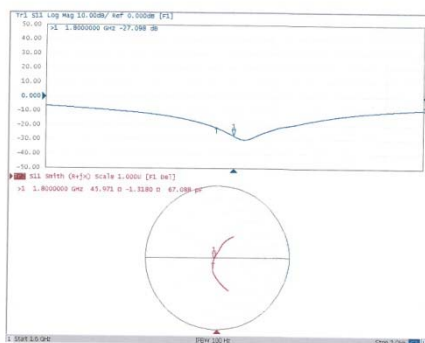

Certificate No: Z17-97138

Page 8 of 8

D2000V2 Sn:1009

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.31 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4236403-2079 Fax: +86-10-4236403-2504
E-mail: ttl@ttltest.com http://www.ttltest.cn

Client: **SRTC** Certificate No: **Z18-97021**

CALIBRATION CERTIFICATE

Object: D2000V2 - SN: 1009

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: February 1, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate

All calibrations have been conducted in the closed laboratory facility, environment temperature(23±1)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter: NRV-D	102188	02-Mar-17 (CTTL, No. J17AD1254)	Mar-18
Power sensor: NRV-Z5	100569	02-Mar-17 (CTTL, No. J17AD1254)	Mar-18
Reference Probe: EX3DV4	SN 7464	12-Sep-17 (SPEAG, No. EX3-7464_Sep17)	Sep-18
DAE4	SN 1225	02-Oct-17 (SPEAG, No. DAE4-1525_Oct17)	Oct-18

Secondary Standards	ID #	Cal Date/Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator: E4438C	MY49211430	23-Jan-18 (CTTL, No. J18AC0960)	Jan-19
Network Analyzer: E5071C	MY48110673	24-Jan-18 (CTTL, No. J18AC0961)	Jan-19

Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hai	SAR Test Engineer	
Approved by:	Qi Diayuan	SAR Project Leader	

Issued: February 4, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-97021

Page 1 of 6

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.31 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4236403-2079 Fax: +86-10-4236403-2504
E-mail: ttl@ttltest.com http://www.ttltest.cn

Client: **SRTC** Certificate No: **Z18-97021**

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORM.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices-Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2018
c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 300MHz to 6GHz)", March 2010
d) KDB665664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

e) DASYS4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z18-97021

Page 2 of 6

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.31 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4236403-2079 Fax: +86-10-4236403-2504
E-mail: ttl@ttltest.com http://www.ttltest.cn

Measurement Conditions

SAR test configuration, as far as not given on page 1

DASY Version	DASY52	52.10.0.1448
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mS/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.9 ± 0.5	1.42 mS/m ± 0.5 %
Head TSL temperature change during test	<1.0 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm² (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	40.3 mW/g ± 18.3 % (k=2)
SAR averaged over 10 cm² (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.17 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	20.4 mW/g ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mS/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.8 ± 0.5	1.58 mS/m ± 0.5 %
Body TSL temperature change during test	<1.0 °C	—	—

SAR result with Body TSL

SAR averaged over 1 cm² (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.3 mW/g
SAR for nominal Body TSL parameters	normalized to 1W	40.3 mW/g ± 18.4 % (k=2)
SAR averaged over 10 cm² (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.18 mW/g
SAR for nominal Body TSL parameters	normalized to 1W	20.4 mW/g ± 18.7 % (k=2)

Certificate No: Z18-97021

Page 3 of 6

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.31 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4236403-2079 Fax: +86-10-4236403-2504
E-mail: ttl@ttltest.com http://www.ttltest.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.60 - 2.06j
Return Loss	-33.6dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.30 - 1.63j
Return Loss	-27.6dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.047 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The central dipole length is still according to the standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	
	SPEAG

Certificate No: Z18-97021

Page 4 of 6


D2000V2 Sn:1009



DASY5 Validation Report for Head TSL Date: 02.01.2018
Test Laboratory: CTTI, Beijing, China
DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1009
Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2000$ MHz; $\alpha = 1.416$ S/m; $\sigma = 38.89$; $\rho = 1000$ kg/m³
Phantom section: Left Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8.39, 8.39, 8.39); Calibrated: 9/12/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1525; Calibrated: 10/2/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)Cube 0; Measurement grid:
 $d_x=5$ mm, $d_y=5$ mm, $d_z=5$ mm
Reference Value = 95.48 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 19.7 W/kg
SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.17 W/kg
Maximum value of SAR (measured) = 16.2 W/kg

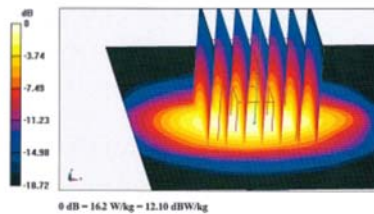


Certificate No: Z18-97021

Page 7 of 8



Impedance Measurement Plot for Head TSL

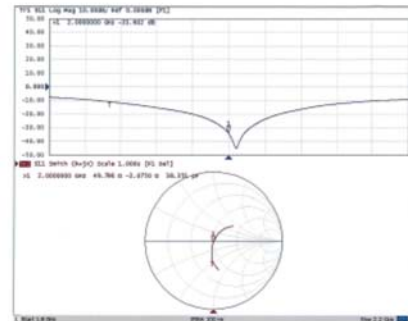

Certificate No: Z18-97021


Page 8 of 8



DASY5 Validation Report for Body TSL Date: 02.01.2018
Test Laboratory: CTTI, Beijing, China
DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1009
Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2000$ MHz; $\alpha = 1.564$ S/m; $\sigma = 51.80$; $\rho = 1000$ kg/m³
Phantom section: Center Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8.24, 8.24, 8.24); Calibrated: 9/12/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1525; Calibrated: 10/2/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)Cube 0; Measurement grid:
 $d_x=5$ mm, $d_y=5$ mm, $d_z=5$ mm
Reference Value = 93.84 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 19.7 W/kg
SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.18 W/kg
Maximum value of SAR (measured) = 16.3 W/kg

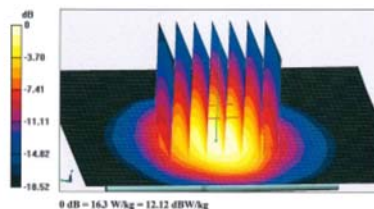


Certificate No: Z18-97021

Page 7 of 8



Impedance Measurement Plot for Body TSL

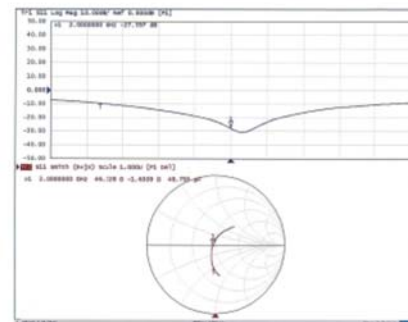

Certificate No: Z18-97021

Page 8 of 8

D2450V2 Sn:738

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

中国认可
国际互认
校准
CNAS L6570

Client: **SRTC** Certificate No: **Z17-97140**

CALIBRATION CERTIFICATE

Object: D2450V2 - SN: 738

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: September 18, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	102196	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Power sensor NRVS Z5	100596	02-Mar-17 (CTTL No.J17X01254)	Mar-18
Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG No EX3-7433_Sep16)	Sep-17
D4E4	SN 1331	10-Jan-17(CTTL-SPEAG No Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL No.J17X00286)	Jan-18
Network Analyzer E5071C	MY46110673	13-Jan-17 (CTTL No.J17X00286)	Jan-18

Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Yu Zongying	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: September 21, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97140

Page 1 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB85664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97140

Page 2 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.0.1448
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.79 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

	Condition	
SAR averaged over 1 cm ³ (1 g) of Head TSL	250 mW input power	13.1 mW / g
SAR measured	normalized to 1W	52.4 mW / g ± 18.8 % (k=2)
SAR for nominal Head TSL parameters	Condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL	250 mW input power	6.10 mW / g
SAR measured	normalized to 1W	24.4 mW / g ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.5 ± 6 %	1.95 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	---	---

SAR result with Body TSL

	Condition	
SAR averaged over 1 cm ³ (1 g) of Body TSL	250 mW input power	13.2 mW / g
SAR measured	normalized to 1W	52.3 mW / g ± 18.8 % (k=2)
SAR for nominal Body TSL parameters	Condition	
SAR averaged over 10 cm ³ (10 g) of Body TSL	250 mW input power	6.10 mW / g
SAR measured	normalized to 1W	24.3 mW / g ± 18.7 % (k=2)

Certificate No: Z17-97140

Page 3 of 8

In Collaboration with
TTL **SPEAG**
CALIBRATION LABORATORY

Address: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.3Ω ± 5.92Ω
Return Loss	- 24.5dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.6Ω ± 6.39Ω
Return Loss	- 23.1dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.268 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG

Certificate No: Z17-97140

Page 4 of 8


D2450V2 Sn:738



DASY5 Validation Report for Head TSL
Test Laboratory: CTTL, Beijing, China
Date: 09.18.2017
DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 738
Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.788$ S/m; $\epsilon_r = 38.67$; $\rho = 1000$ kg/m³
Phantom section: Left Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(745, 745, 745); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 102.1 V/m; Power Drift = -0.01 dB
Peak SAR (extrapolated) = 27.8 W/kg
SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.1 W/kg
Maximum value of SAR (measured) = 22.0 W/kg

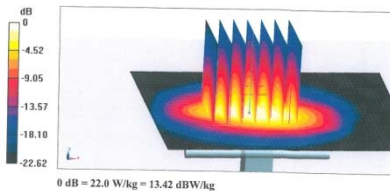


Certificate No: Z17-97140

Page 5 of 8



Impedance Measurement Plot for Head TSL

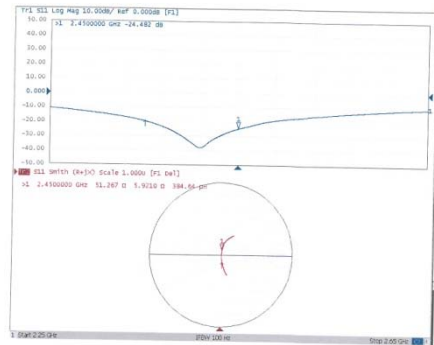

Certificate No: Z17-97140


Page 6 of 8



DASY5 Validation Report for Body TSL
Test Laboratory: CTTL, Beijing, China
Date: 09.18.2017
DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 738
Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.983$ S/m; $\epsilon_r = 52.51$; $\rho = 1000$ kg/m³
Phantom section: Center Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7433; ConvF(746, 746, 746); Calibrated: 9/26/2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 96.41 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 27.8 W/kg
SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.1 W/kg
Maximum value of SAR (measured) = 22.3 W/kg

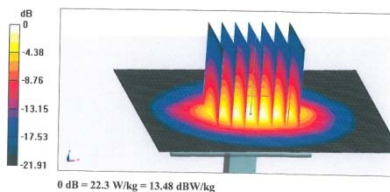


Certificate No: Z17-97140

Page 7 of 8



Impedance Measurement Plot for Body TSL

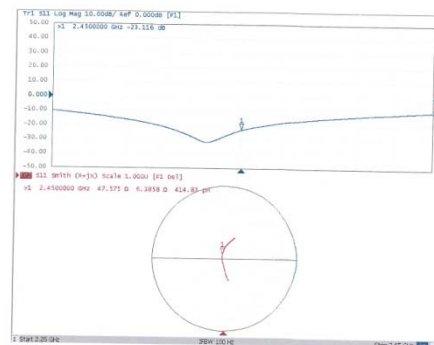

Certificate No: Z17-97140

Page 8 of 8

D5GHzV2 Sn:1079

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

Client: **SRTC** Certificate No: **Z17-97133**

CALIBRATION CERTIFICATE

Object: **D5GHzV2 - SN: 1079**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **September 25, 2017**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(2±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	102196	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
Power sensor NRP-Z91	100596	02-Mar-17 (CTTL, No.J17X01254)	Mar-18
ReferenceProbe EX3DV4	SN 3846	13-Jan-17(CTTL-SPEAG, No.Z16-97251)	Jan-18
D4E4	SN 1331	19-Jan-17(CTTL-SPEAG, No.Z17-97015)	Jan-18

Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No.J17X00286)	Jan-18
NetworkAnalyzer E5071C	MY46110673	13-Jan-17 (CTTL, No.J17X00286)	Jan-18

Calibrated by: **Zhao Jing** Function: **SAR Test Engineer** Signature: *[Signature]*

Reviewed by: **Yu Zongying** Function: **SAR Test Engineer** Signature: *[Signature]*

Approved by: **Qi Dianyan** Function: **SAR Project Leader** Signature: *[Signature]*

Issued: September 28, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97133

Page 1 of 16

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
d) KDB85664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:
e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:
• **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• **SAR measured:** SAR measured at the stated antenna input power.
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z17-97133

Page 2 of 16

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

Measurement Conditions
DASY system configuration, as far as not given on page 1.

DASY Version	DASY92	52.10.0.1446
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz
The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.7 ± 6 %	4.62 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5200 MHz

	Condition	
SAR averaged over 1 cm ³ (1 g) of Head TSL		
SAR measured	100 mW input power	7.77 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	77.6 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL		
SAR measured	100 mW input power	2.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.3 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 3 of 16

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@chinaatl.com http://www.chinaatl.cn

Head TSL parameters at 5300 MHz
The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.1 ± 6 %	4.67 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5300 MHz

	Condition	
SAR averaged over 1 cm ³ (1 g) of Head TSL		
SAR measured	100 mW input power	8.13 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	81.3 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL		
SAR measured	100 mW input power	2.32 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.2 mW / g ± 24.2 % (k=2)

Head TSL parameters at 5500 MHz
The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.9 ± 6 %	4.93 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5500 MHz

	Condition	
SAR averaged over 1 cm ³ (1 g) of Head TSL		
SAR measured	100 mW input power	8.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	82.5 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL		
SAR measured	100 mW input power	2.37 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.8 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 4 of 16

D5GHzV2 Sn:1079



Head TSL parameters at 5600 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.7 ± 6 %	4.98 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.16 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	81.6 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.34 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.4 mW / g ± 24.2 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.8 ± 6 %	5.16 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.85 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	78.7 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.25 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.6 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 5 of 16



Body TSL parameters at 5200 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.5 ± 6 %	5.38 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.52 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	75.4 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.12 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.3 mW / g ± 24.2 % (k=2)

Body TSL parameters at 5300 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.42 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.2 ± 6 %	5.50 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL at 5300 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.68 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	76.9 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.18 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.9 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 6 of 16



Body TSL parameters at 5500 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.0 ± 6 %	5.72 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	8.22 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	82.4 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.35 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.6 mW / g ± 24.2 % (k=2)

Body TSL parameters at 5600 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.73 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	8.08 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	80.7 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.30 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.0 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 7 of 16



Body TSL parameters at 5800 MHz

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.0 ± 6 %	5.94 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	----	----

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.73 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	77.5 mW / g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.17 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.8 mW / g ± 24.2 % (k=2)

Certificate No: Z17-97133

Page 8 of 16

D5GHzV2 Sn:1079



Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	47.6Ω - 8.77jΩ
Return Loss	- 20.7dB

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	45.5Ω - 6.82jΩ
Return Loss	- 21.4dB

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	50.7Ω - 7.14jΩ
Return Loss	- 23.0dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	55.2Ω - 4.00jΩ
Return Loss	- 24.1dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	52.2Ω - 8.20jΩ
Return Loss	- 21.8dB

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	50.8Ω - 10.1jΩ
Return Loss	- 20.0dB

Antenna Parameters with Body TSL at 5300 MHz

Impedance, transformed to feed point	48.5Ω - 8.56jΩ
Return Loss	- 21.1dB

Certificate No: Z17-97133

Page 9 of 16



Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	54.9Ω - 6.85jΩ
Return Loss	- 21.9dB

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	58.6Ω - 2.29jΩ
Return Loss	- 23.7dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	56.7Ω - 8.19jΩ
Return Loss	- 20.2dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.313 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z17-97133

Page 10 of 16



DASY5 Validation Report for Head TSL

Date: 09.21.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1079

Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz;
Medium parameters used: f = 5200 MHz; $\sigma = 4.616$ mho/m; $\epsilon_r = 35.72$; $\rho = 1000$ kg/m³; Medium parameters used: f = 5300 MHz; $\sigma = 4.668$ mho/m; $\epsilon_r = 35.72$; $\rho = 1000$ kg/m³; Medium parameters used: f = 5500 MHz; $\sigma = 4.934$ mho/m; $\epsilon_r = 35.92$; $\rho = 1000$ kg/m³; Medium parameters used: f = 5600 MHz; $\sigma = 4.984$ mho/m; $\epsilon_r = 35.73$; $\rho = 1000$ kg/m³; Medium parameters used: f = 5800 MHz; $\sigma = 5.159$ mho/m; $\epsilon_r = 35.83$; $\rho = 1000$ kg/m³;
Phantom section: Left Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3846; ConvF(5.37,5.37,5.37); Calibrated: 1/13/2017, ConvF(5.37,5.37,5.37); Calibrated: 1/13/2017, ConvF(4.72,4.72,4.72); Calibrated: 1/13/2017, ConvF(4.72,4.72,4.72); Calibrated: 1/13/2017, ConvF(4.95,4.95,4.95); Calibrated: 1/13/2017,
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1331; Calibrated: 2017/1/19
- Phantom: Triple Flat Phantom 5-IC; Type: QD 000 P51 CA; Serial: 1161/3
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 58.81 V/m; Power Drift = -0.01 dB
Peak SAR (extrapolated) = 30.8 W/kg
SAR(1 g) = 7.77 W/kg; SAR(10 g) = 2.24 W/kg
Maximum value of SAR (measured) = 18.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 65.19 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 33.7 W/kg
SAR(1 g) = 8.13 W/kg; SAR(10 g) = 2.32 W/kg
Maximum value of SAR (measured) = 19.3 W/kg

Certificate No: Z17-97133


Page 11 of 16



Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 57.80 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 34.3 W/kg
SAR(1 g) = 8.24 W/kg; SAR(10 g) = 2.37 W/kg
Maximum value of SAR (measured) = 19.6 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 57.89 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 35.7 W/kg
SAR(1 g) = 8.16 W/kg; SAR(10 g) = 2.34 W/kg
Maximum value of SAR (measured) = 20.0 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 53.56 V/m; Power Drift = -0.06 dB
Peak SAR (extrapolated) = 35.0 W/kg
SAR(1 g) = 7.85 W/kg; SAR(10 g) = 2.25 W/kg
Maximum value of SAR (measured) = 19.7 W/kg

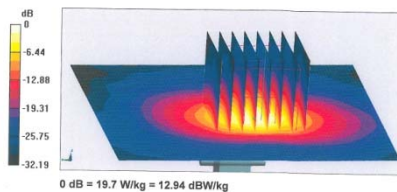


Certificate No: Z17-97133

Page 12 of 16

D5GHzV2 Sn:1079



Impedance Measurement Plot for Head TSL

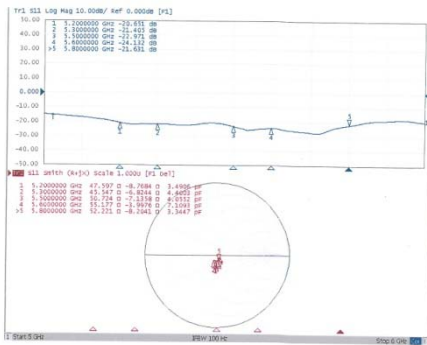

Certificate No: Z17-97133

Page 13 of 16



DASY5 Validation Report for Body TSL

Date: 09/25/2017

Test Laboratory: CTTT, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: 1079

Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Medium parameters used: $f = 5200$ MHz; $\sigma = 5.382$ mho/m; $\epsilon_r = 49.47$; $\rho = 1000$ kg/m³; Medium parameters used: $f = 5300$ MHz; $\sigma = 5.498$ mho/m; $\epsilon_r = 49.21$; $\rho = 1000$ kg/m³; Medium parameters used: $f = 5500$ MHz; $\sigma = 5.722$ mho/m; $\epsilon_r = 49.03$; $\rho = 1000$ kg/m³; Medium parameters used: $f = 5600$ MHz; $\sigma = 5.733$ mho/m; $\epsilon_r = 48.37$; $\rho = 1000$ kg/m³; Medium parameters used: $f = 5800$ MHz; $\sigma = 5.935$ mho/m; $\epsilon_r = 48.99$; $\rho = 1000$ kg/m³.

Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3846; ConvF(4.95, 4.95, 4.95); Calibrated: 1/13/2017; ConvF(4.95, 4.95, 4.95); Calibrated: 1/13/2017; ConvF(4.18, 4.18, 4.18); Calibrated: 1/13/2017; ConvF(4.18, 4.18, 4.18); Calibrated: 1/13/2017; ConvF(4.53, 4.53, 4.53); Calibrated: 1/13/2017.
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 SN1331; Calibrated: 2017/1/19
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/3
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 55.18 V/m; Power Drift = 0.01 dB
Peak SAR (extrapolated) = 30.0 W/kg
SAR(1 g) = 7.52 W/kg; SAR(10 g) = 2.12 W/kg
Maximum value of SAR (measured) = 18.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 53.94 V/m; Power Drift = 0.01 dB
Peak SAR (extrapolated) = 31.9 W/kg
SAR(1 g) = 7.68 W/kg; SAR(10 g) = 2.18 W/kg
Maximum value of SAR (measured) = 18.3 W/kg

Certificate No: Z17-97133


Page 14 of 16



Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 66.70 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 33.7 W/kg
SAR(1 g) = 8.22 W/kg; SAR(10 g) = 2.35 W/kg
Maximum value of SAR (measured) = 19.3 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 67.75 V/m; Power Drift = 0.01 dB
Peak SAR (extrapolated) = 34.2 W/kg
SAR(1 g) = 8.08 W/kg; SAR(10 g) = 2.3 W/kg
Maximum value of SAR (measured) = 19.3 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 68.20 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 33.3 W/kg
SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.17 W/kg
Maximum value of SAR (measured) = 19.3 W/kg

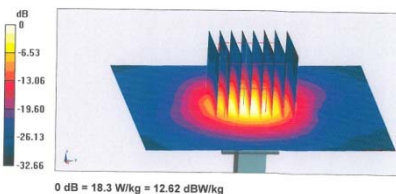


Certificate No: Z17-97133

Page 15 of 16



Impedance Measurement Plot for Body TSL

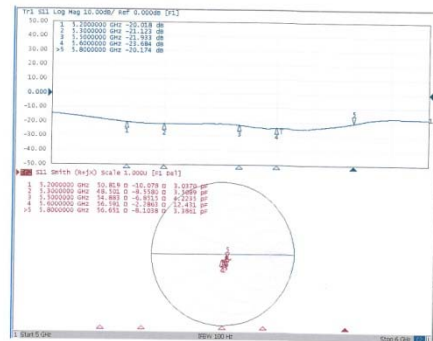

Certificate No: Z17-97133

Page 16 of 16

-----End of the test report-----