

O.P. # DKPX-10050-001-1 Rev. 1.1

Title Description: Device Label Application

APPROVALSManufacturing M. Norris Date 7/27/17 Quality K. Dolan Date 7/26/17Engineering S. Holland Date 7/26/17**EQUIPMENT REQUIRED**

N/A

FIXTURES REQUIRED

N/A


SUPPLIES

N/A

O.P. # DKPX-10050-001-1 Rev. 1.1

Title Description: Device Label Application


Place 2x DKPX-09033-001 tie down labels on the housing.
Place one on each side front under tie down loops.

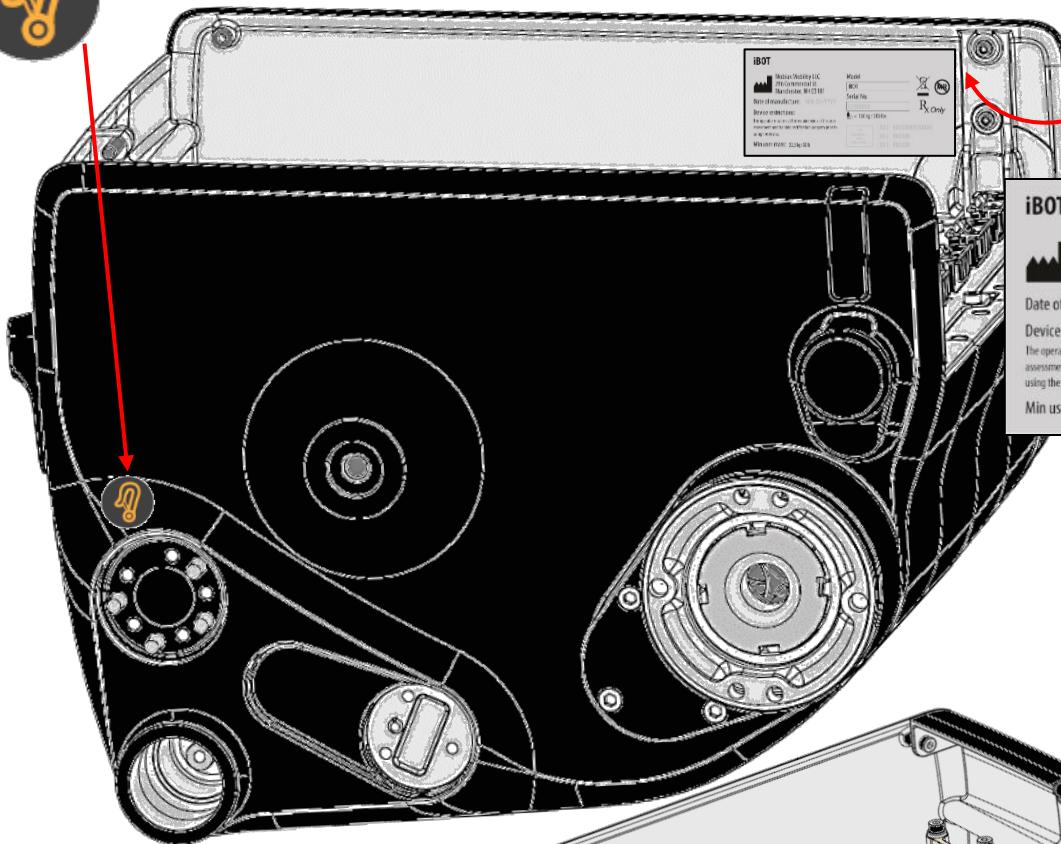

Align DKPX-09035-001
main label here


iBOT	
Mobius Mobility LLC 286 Commercial St. Manchester, NH 03101	Model iBOT
Date of manufacture: MM-DD-YYYY XXXXXX	Serial No. XXXXXXXXXXXX
Device restrictions: The operator must meet the requirements of the user assessment and training certification program prior to using the device.	 R_X Only
Min user mass: 22.5kg/50lb	 < 136 kg / 300 lbs

Place 2x DKPX-09034-001 tie down
labels on the rear of the housing.
Place one on either side under tie down loops.

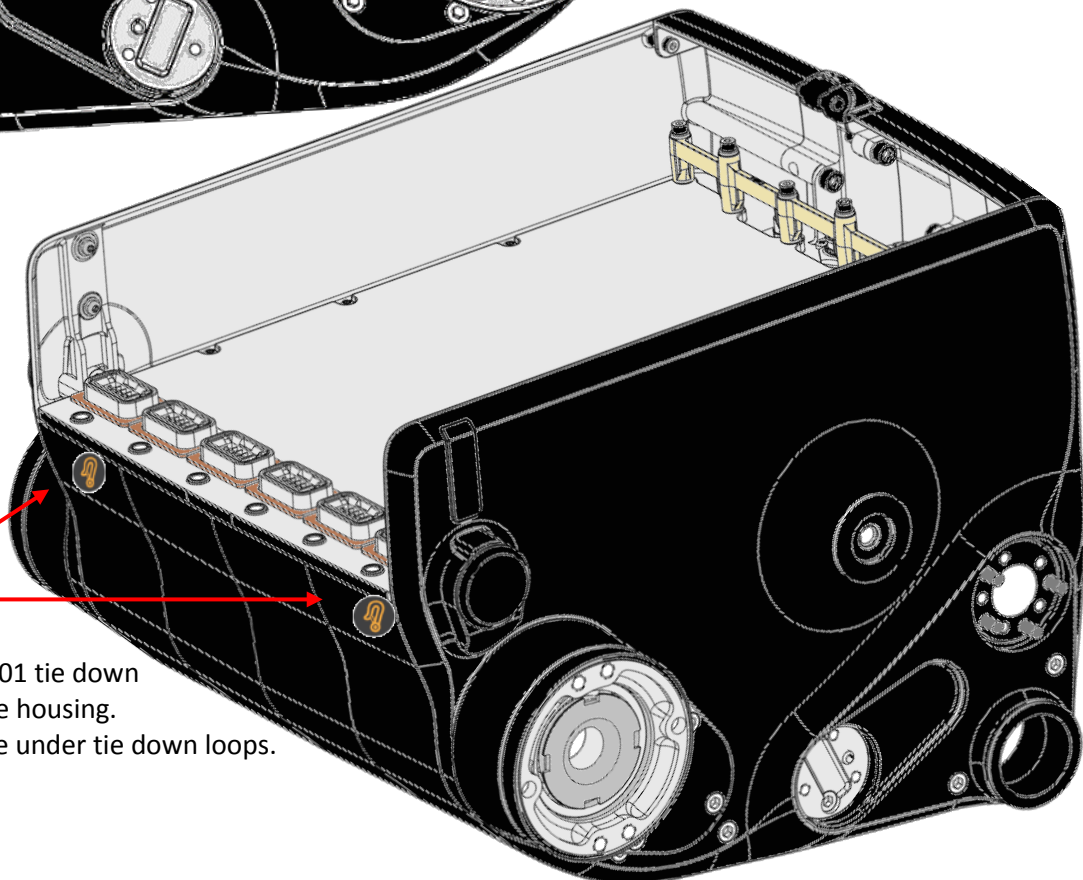

O.P. # DKPX-10050-001-1 Rev. 1.1

Title Description: Device Label Application

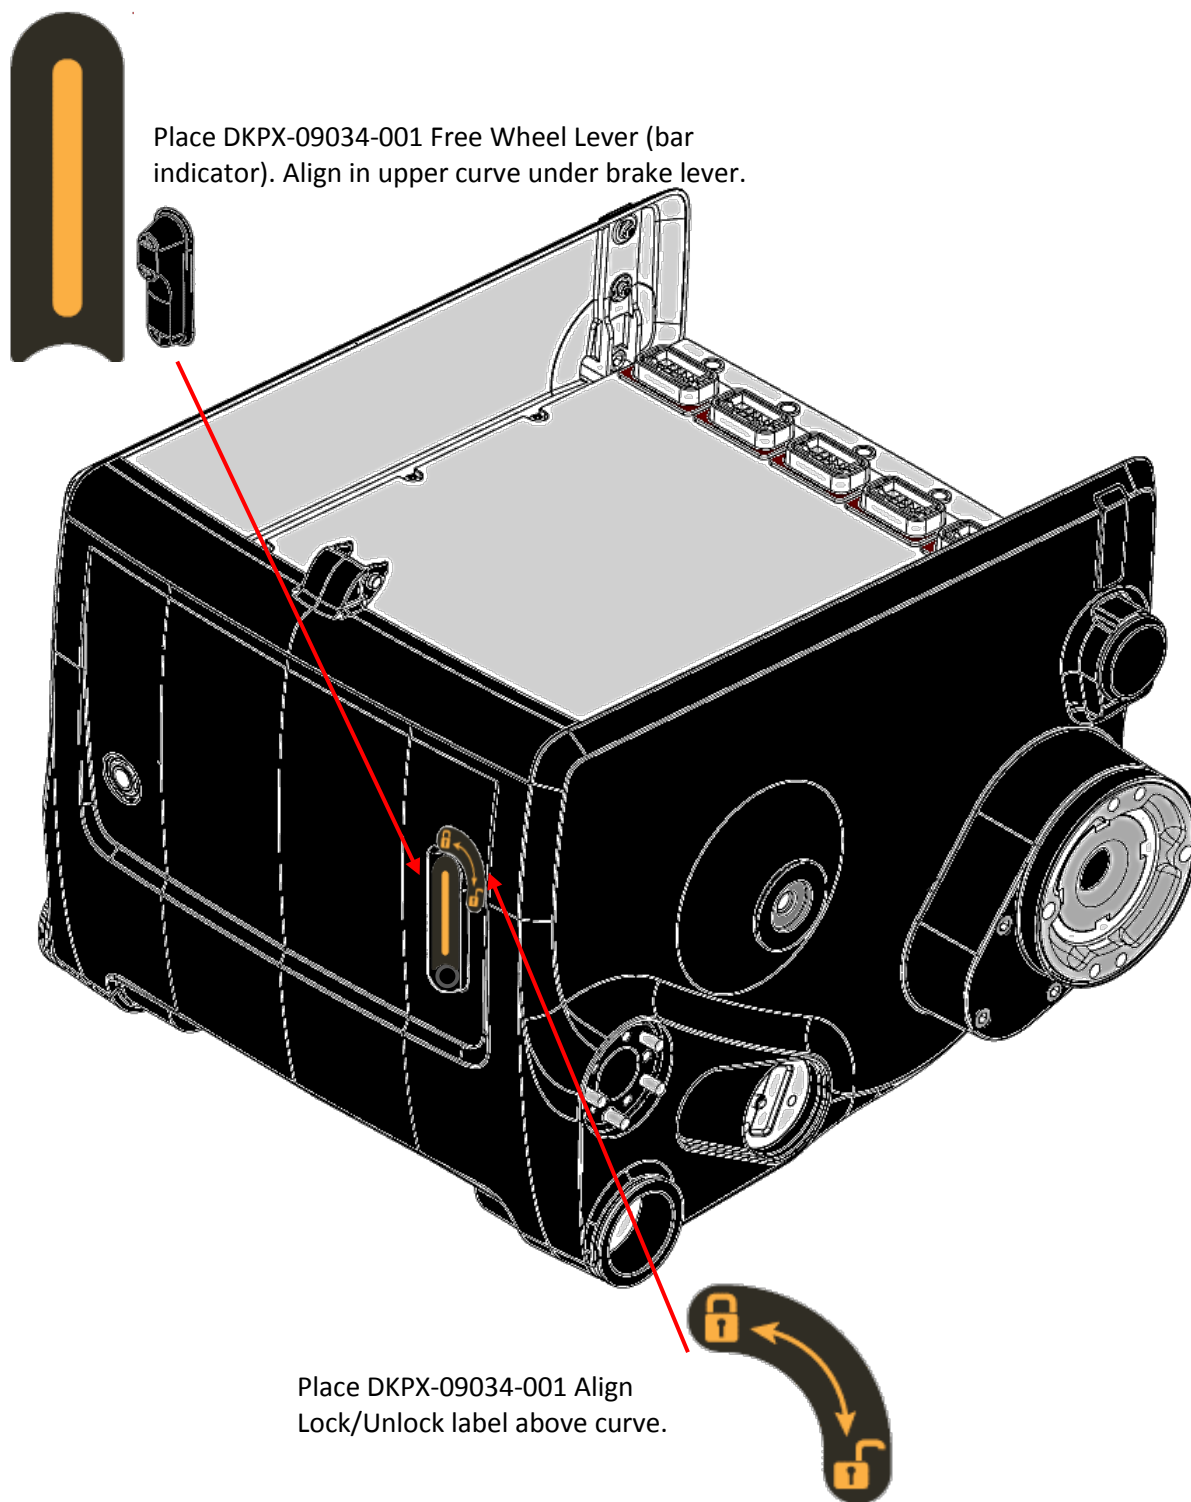


O.P. # DKPX-10050-001-1 Rev. 1.1

Title Description: Device Label Application

Place DKPX-09037-001 FCC label on the back of

n..

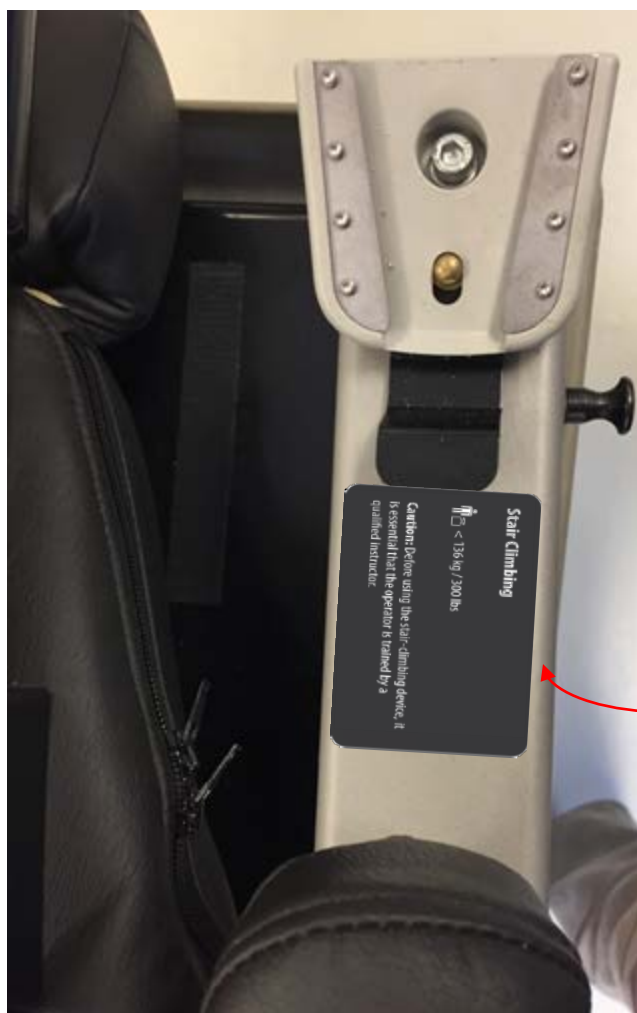

Stair Climbing

 < 136 kg / 300 lbs

Caution: Before using the stair-climbing device, it is essential that the operator is trained by a qualified instructor.

Place DKPX-09036-001 Stair Climbing label on swing away arm under user controller.

O.P. # DKPX-10050-001-1 Rev. 1.1

Title Description: Device Label Application

QUALITY AWARENESS

This Operation Procedure (OP) establishes product/process quality requirements for the defined manufacturing operation. Manufacturing personnel who encounter defects as part of their job functions refer to DKQA-13-003 to address such issues.

REVISION RECORDS

REV.	CHANGE	REASON	APPR/DATE	ECO #
1.0	Release to change order control	Initial Release	7/27/17	13911
1.1	1. Update FCC label and main label images	1. Labels updated.	7/2/18	14863