Impedance Plot for

SN 47/14 DIP 0G750-340; 750Head

Calibrated impedance: 54.2Ω+3.9JΩ; Measurement impedance: 55.1Ω-2.2jΩ(within 5Ω)

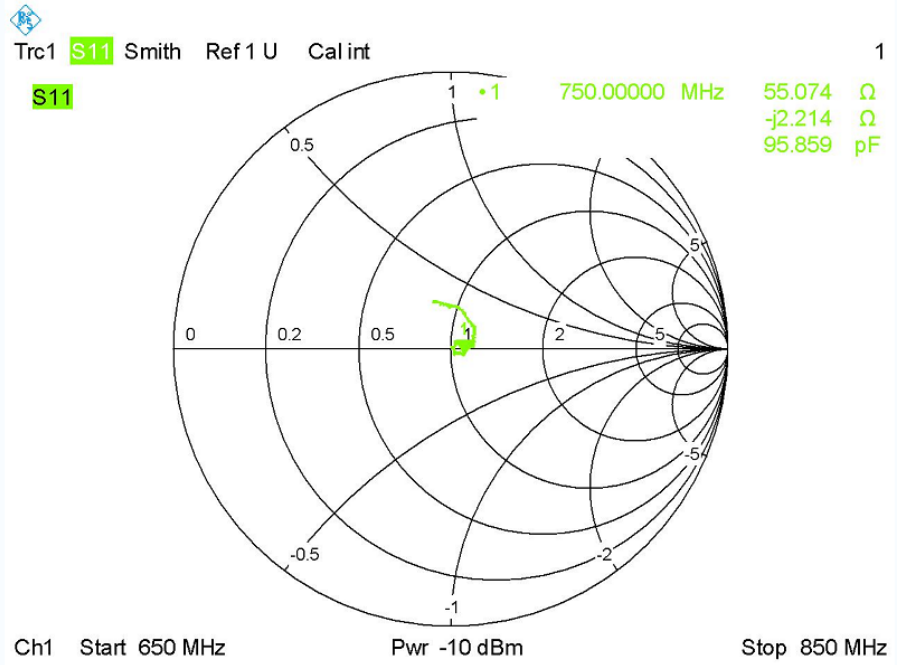

Calibrated return loss: -25.20dB; Measurement return loss: -23.05 dB(within 20%)

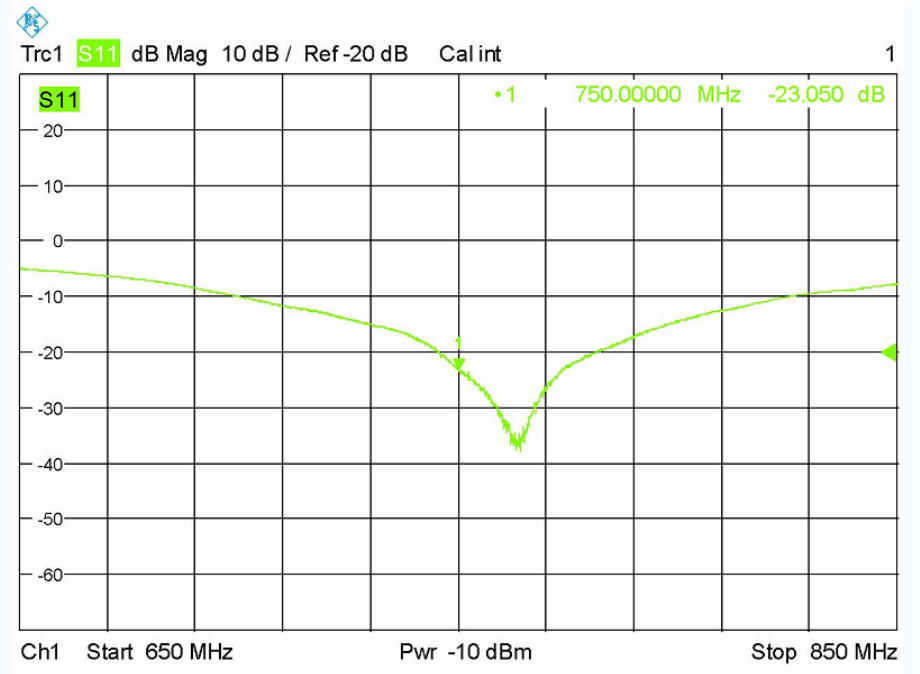

SN 29/15 DIP 0G835-383; 835Head

Calibrated impedance: 56.3Ω+0.8JΩ; Measurement impedance: 57.1Ω-5.0jΩ(within 5Ω)

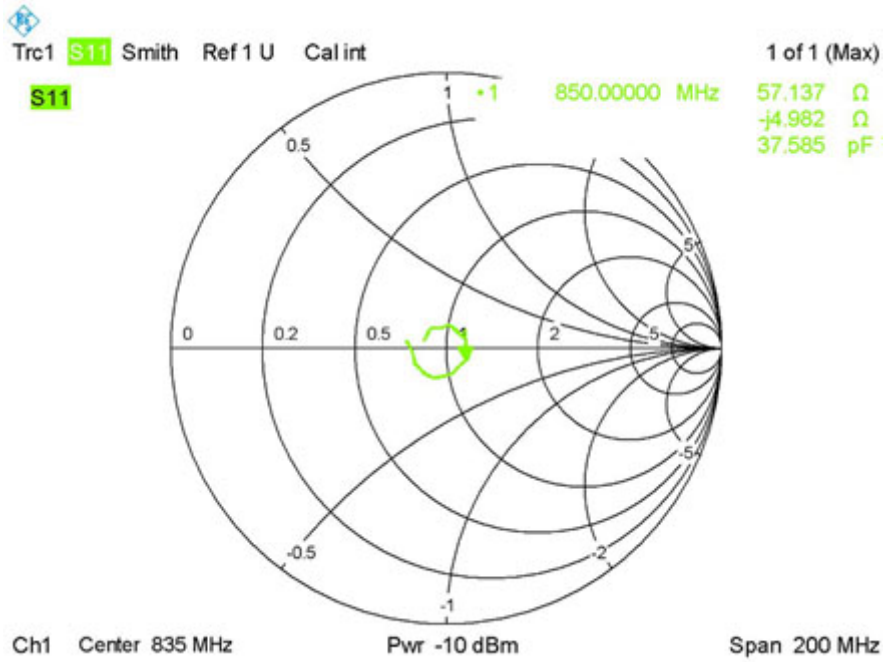

Calibrated return loss: -24.51dB; Measurement return loss: -22.89 dB(within 20%)

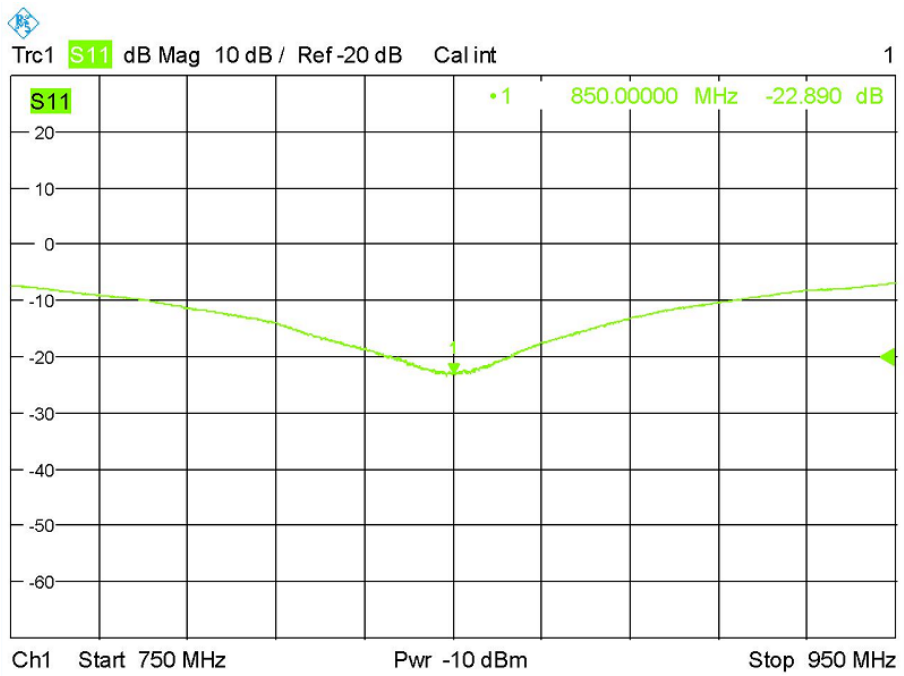

SN 46/11 DIP 1G800-186; 1800Head

Calibrated impedance: 46.7Ω+3.0JΩ; Measurement impedance: 48.5Ω+2.3jΩ(within 5Ω)

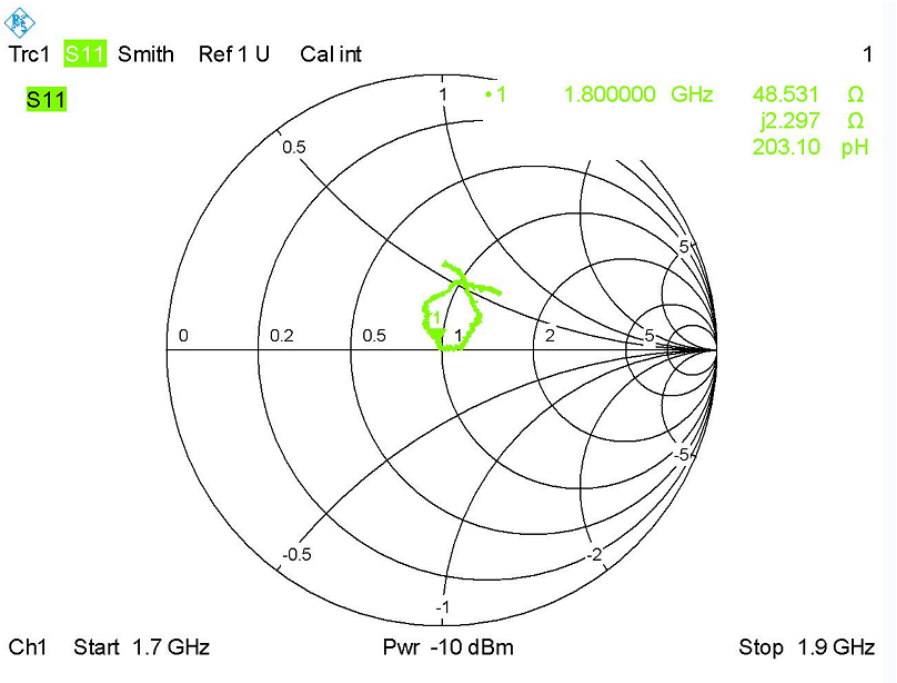

Calibrated return loss: -26.66dB; Measurement return loss: -27.3 dB(within 20%)

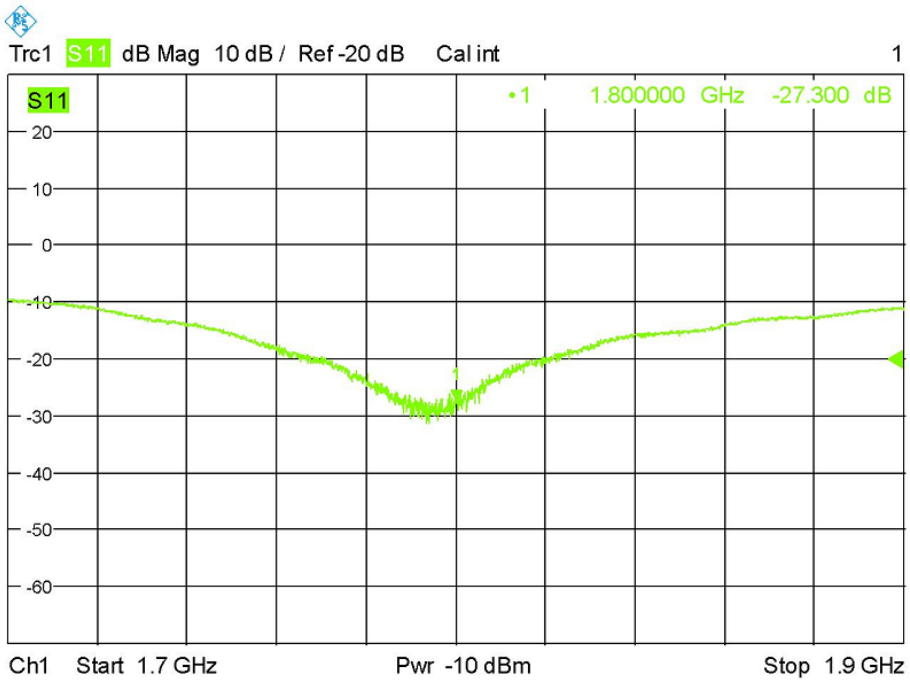

SN 46/11 DIP 1G900-187; 1900Head

Calibrated impedance: 50.7Ω+4.1JΩ; Measurement impedance: 48.6Ω+2.9jΩ(within 5Ω)

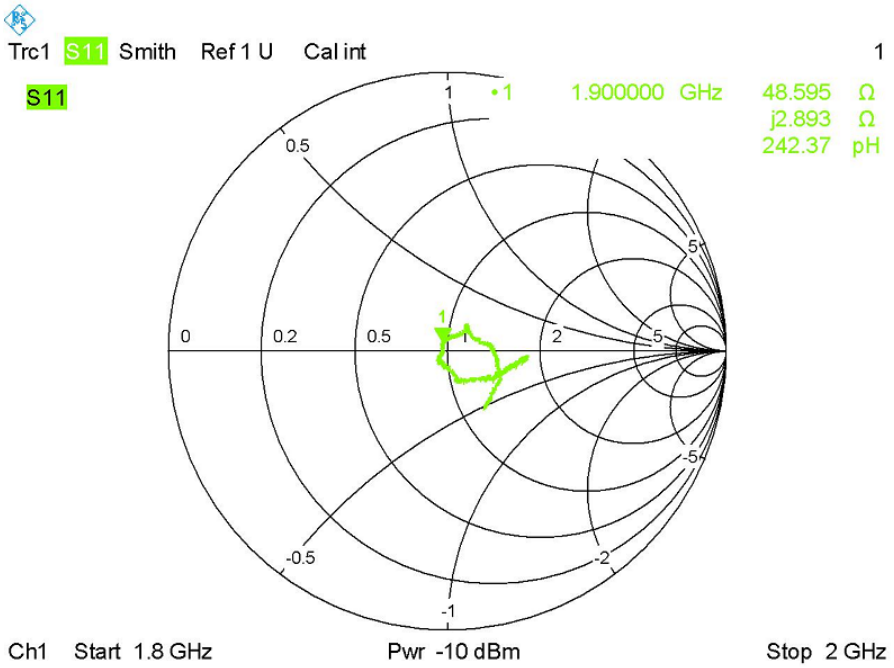

Calibrated return loss: -27.75dB; Measurement return loss: -28.54 dB(within 20%)

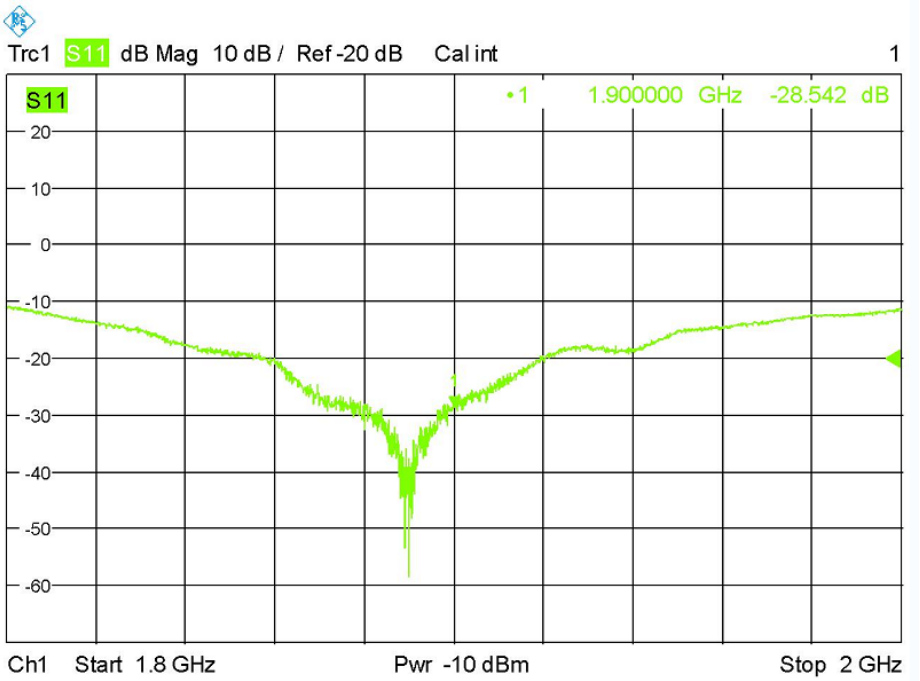

SN 46/11 DIP 2G450-189; 2450Head

Calibrated impedance: 49.8Ω+3.3JΩ; Measurement impedance: 50.9Ω-2.1jΩ(within 5Ω)

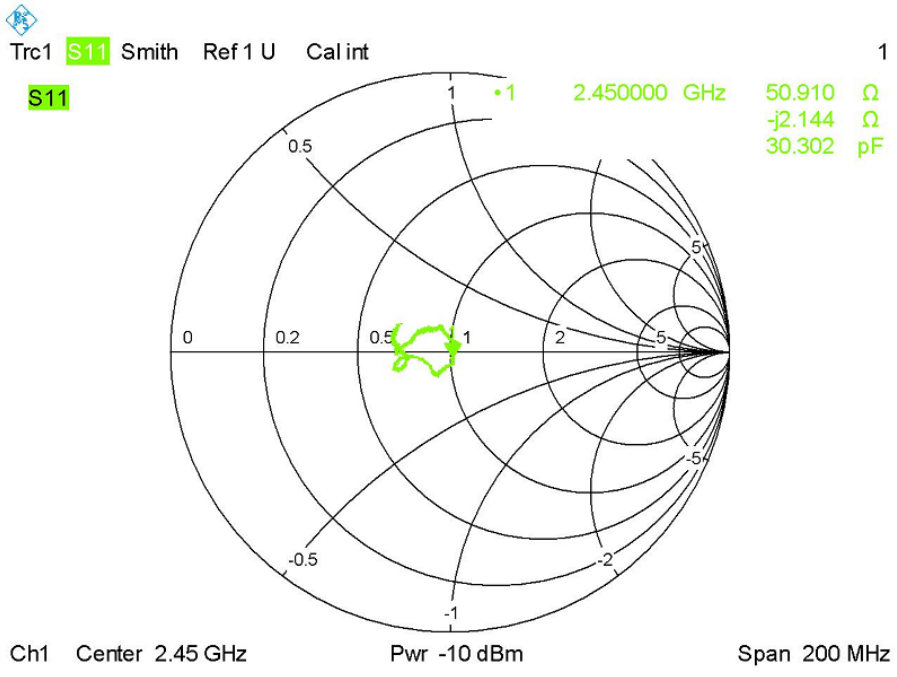

Calibrated return loss: -29.54dB; Measurement return loss: -31.08 dB(within 20%)

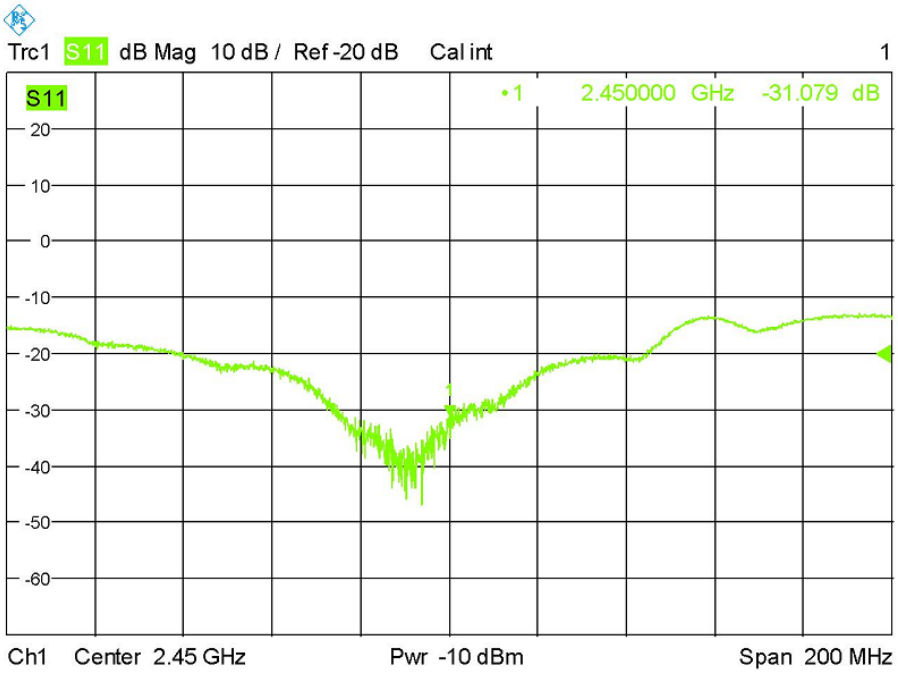

SN 47/14 DIP 2G600-342; 2600Head

Calibrated impedance: 55.5Ω+2.6JΩ; Measurement impedance: 57.2Ω+3.2jΩ(within 5Ω)

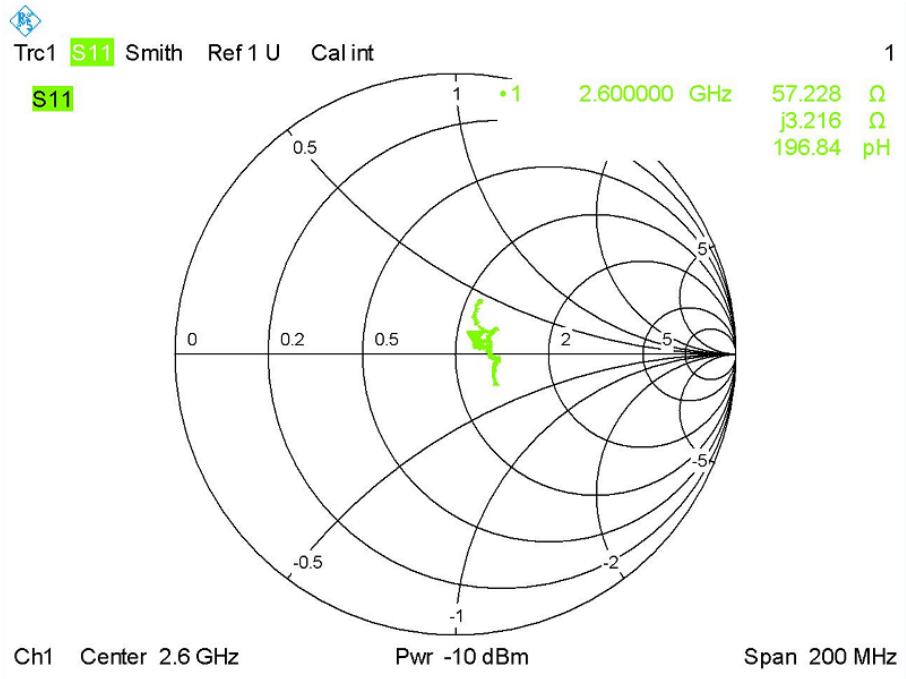
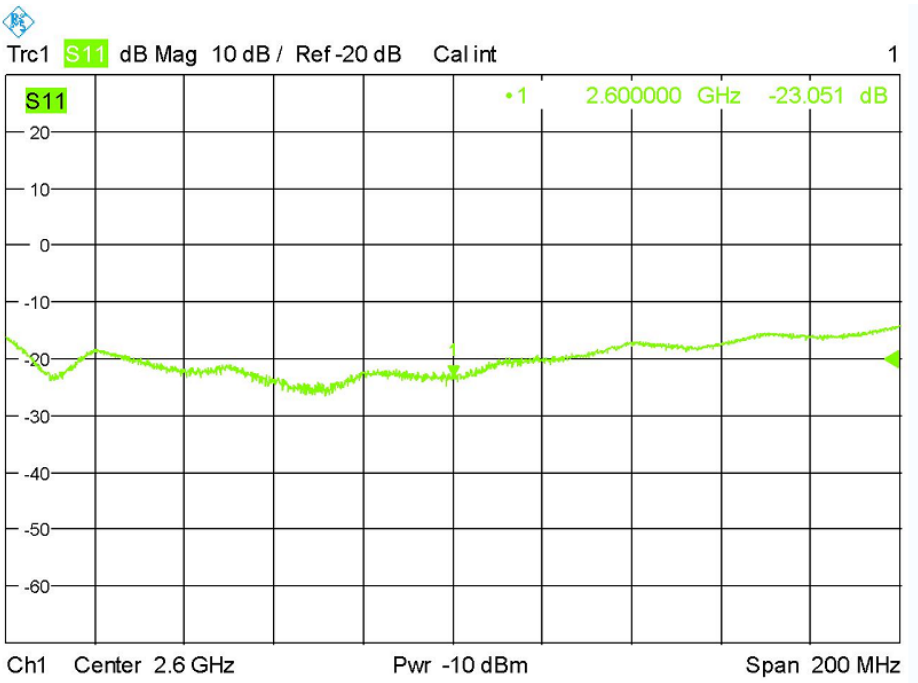
Calibrated return loss: -24.86dB; Measurement return loss: -23.1 dB(within 20%)